




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061022\
 Data File : BN020089.D
 Acq On : 09 Jun 2022 20:19
 Operator : CG/JU
 Sample : N3212-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F5A50

Manual IntegrationsAPPROVED

Quant Time: Jun 10 02:43:19 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN053122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 10 02:40:52 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/10/2022
 Supervised By :mohammad ahmed 06/10/2022

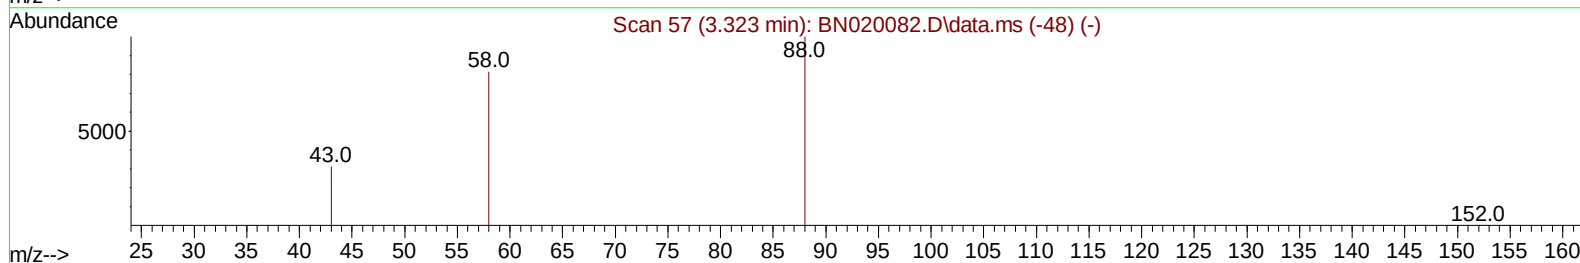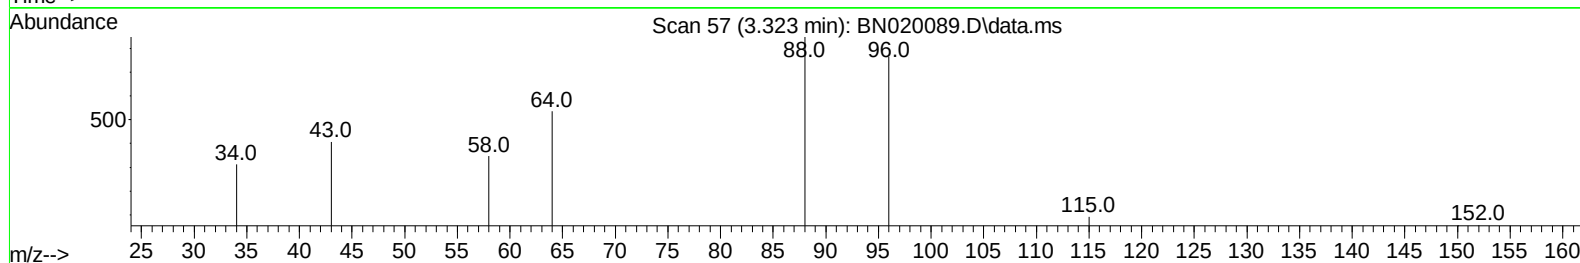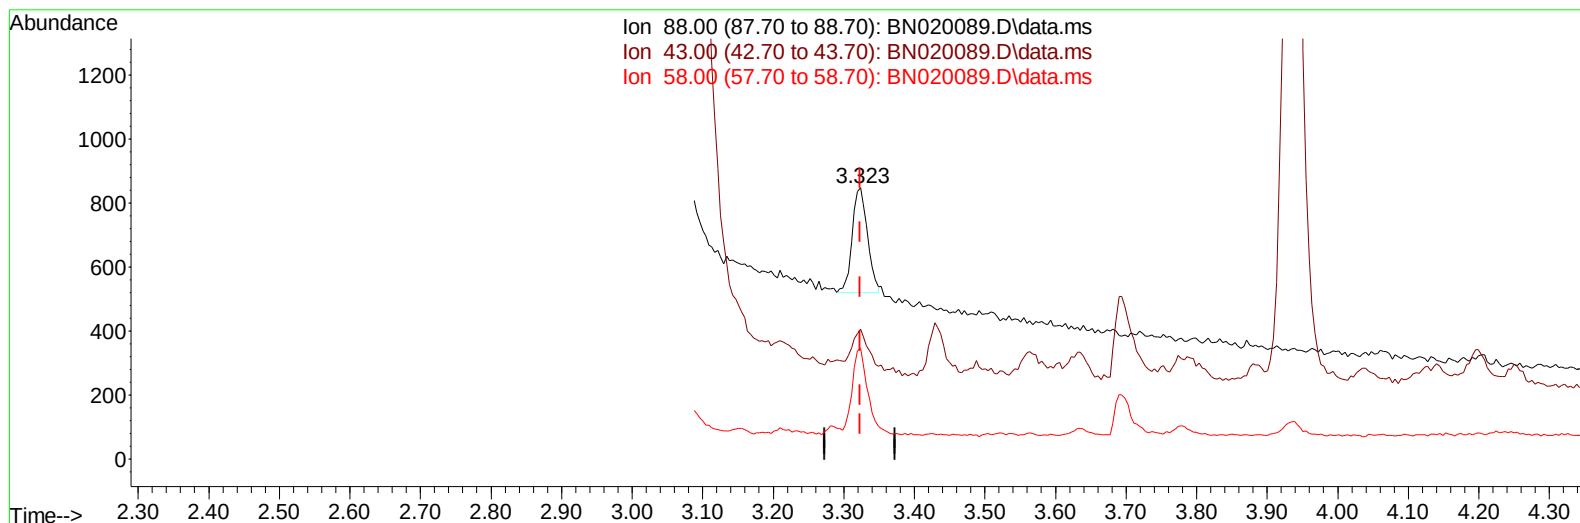

TIC: BN020089.D\data.ms

(2) 1,4-Dioxane

3.323min (+ 0.000) 0.10 ng/u1

response 490

Ion	Exp%	Act%
88.00	100.00	100.00
43.00	48.70	48.05
58.00	49.80	40.97
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061022\
Data File : BN020089.D
Acq On : 09 Jun 2022 20:19
Operator : CG/JU
Sample : N3212-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F5A50

Manual IntegrationsAPPROVED

Quant Time: Jun 10 02:43:19 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN053122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 10 02:40:52 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/10/2022
Supervised By :mohammad ahmed 06/10/2022

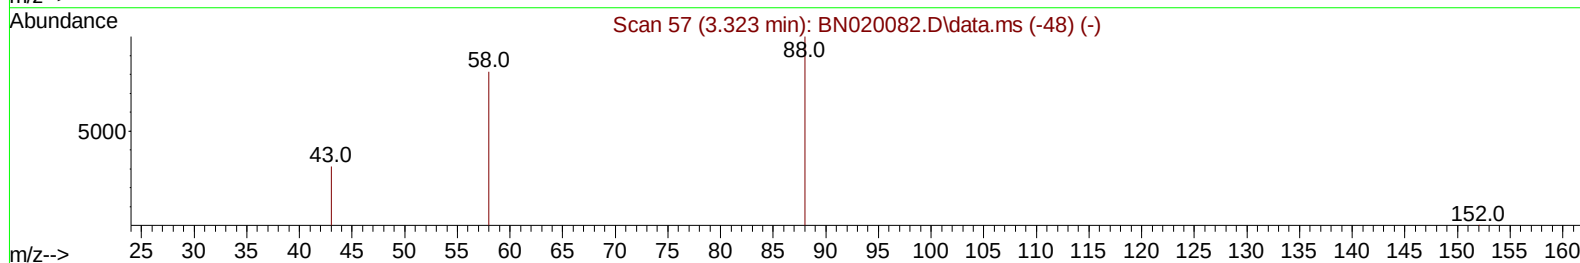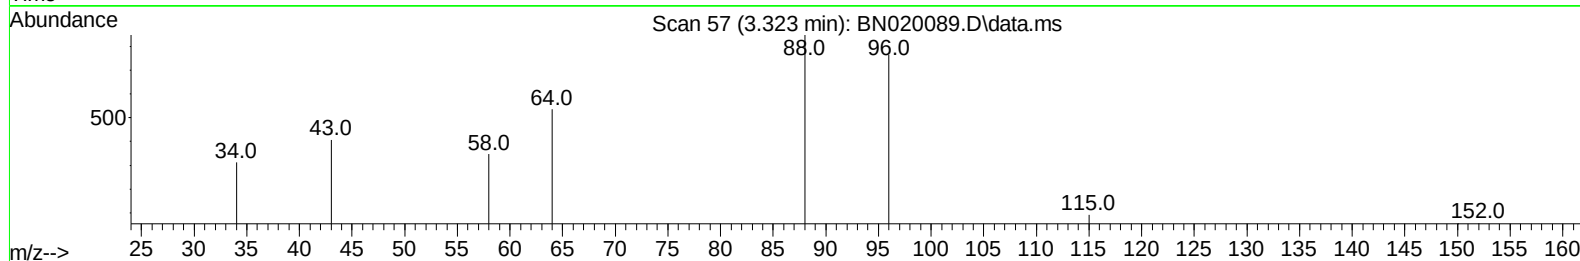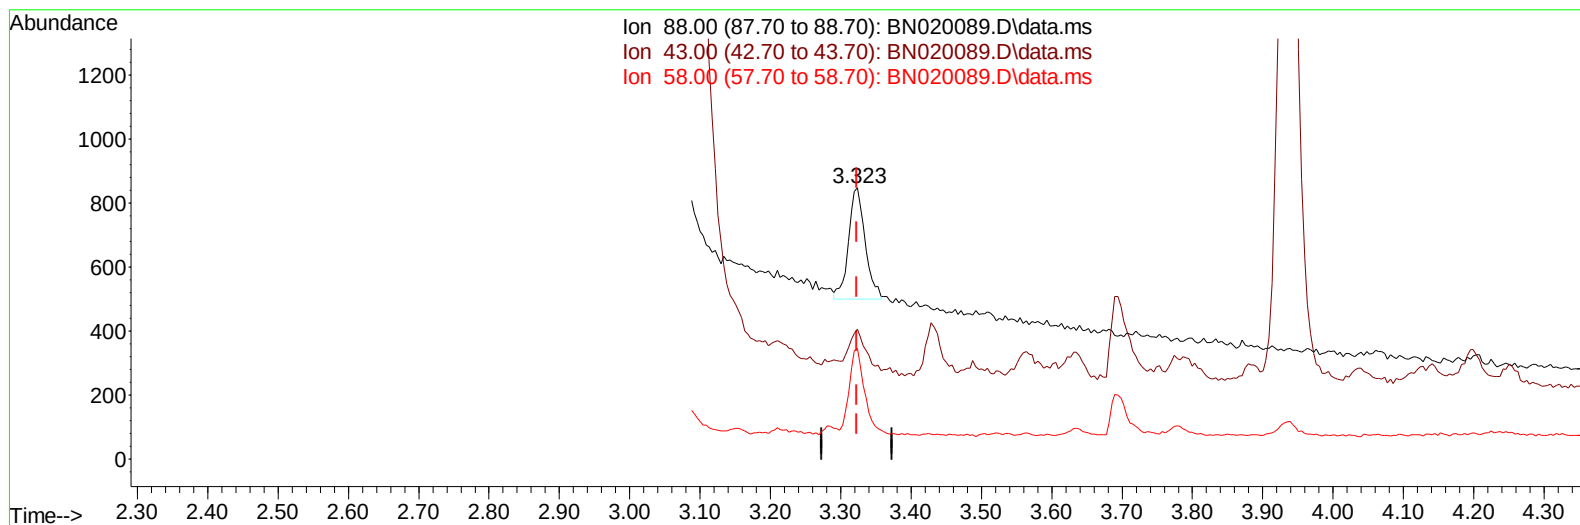

TIC: BN020089.D\data.ms

(2) 1,4-Dioxane

3.323min (+ 0.000) 0.11 ng/ul m

response 573

Ion	Exp%	Act%
88.00	100.00	100.00
43.00	48.70	48.05
58.00	49.80	40.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061022\
 Data File : BN020089.D
 Acq On : 09 Jun 2022 20:19
 Operator : CG/JU
 Sample : N3212-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F5A50

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/10/2022
 Supervised By :mohammad ahmed 06/10/2022

Quant Time: Jun 10 02:43:19 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN053122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 10 02:40:52 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.825	152		4283	0.400	ng/ul	0.00
4) Naphthalene-d8	10.611	136		14684	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.450	164		9140	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.190	188		19763	0.400	ng/ul	0.00
17) Chrysene-d12	21.376	240		17452	0.400	ng/ul	0.00
23) Perylene-d12	23.703	264		14534	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.286	96		22500	4.610	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.205	152		6475	0.276	ng/ul	0.00
18) Fluoranthene-d10	19.219	212		18149	0.344	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.323	88		573m	0.112	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061022\
Data File : BN020089.D
Acq On : 09 Jun 2022 20:19
Operator : CG/JU
Sample : N3212-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F5A50

Manual IntegrationsAPPROVED

Quant Time: Jun 10 02:43:19 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN053122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 10 02:40:52 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/10/2022
Supervised By :mohammad ahmed 06/10/2022

