

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061022\
 Data File : BN020087.D
 Acq On : 09 Jun 2022 19:06
 Operator : CG/JU
 Sample : N3212-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F5A51

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 06/10/2022
 Supervised By :mohammad ahmed 06/10/2022

Quant Time: Jun 10 02:43:12 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN053122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 10 02:40:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.825	152	3907	0.400	ng/ul	0.00
4) Naphthalene-d8	10.612	136	13441	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.451	164	8567	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.187	188	18860	0.400	ng/ul	0.00
17) Chrysene-d12	21.381	240	16107	0.400	ng/ul	0.00
23) Perylene-d12	23.708	264	13343	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.285	96	23365	5.248	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.207	152	7668	0.357	ng/ul	0.00
18) Fluoranthene-d10	19.220	212	21143	0.434	ng/ul	0.00
Target Compounds						
2) 1,4-Dioxane	3.323	88	609m	0.130	ng/ul	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061022\
Data File : BN020087.D
Acq On : 09 Jun 2022 19:06
Operator : CG/JU
Sample : N3212-05
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
F5A51

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 06/10/2022
Supervised By :mohammad ahmed 06/10/2022


Quant Time: Jun 10 02:43:12 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN053122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 10 02:40:52 2022
Response via : Initial Calibration

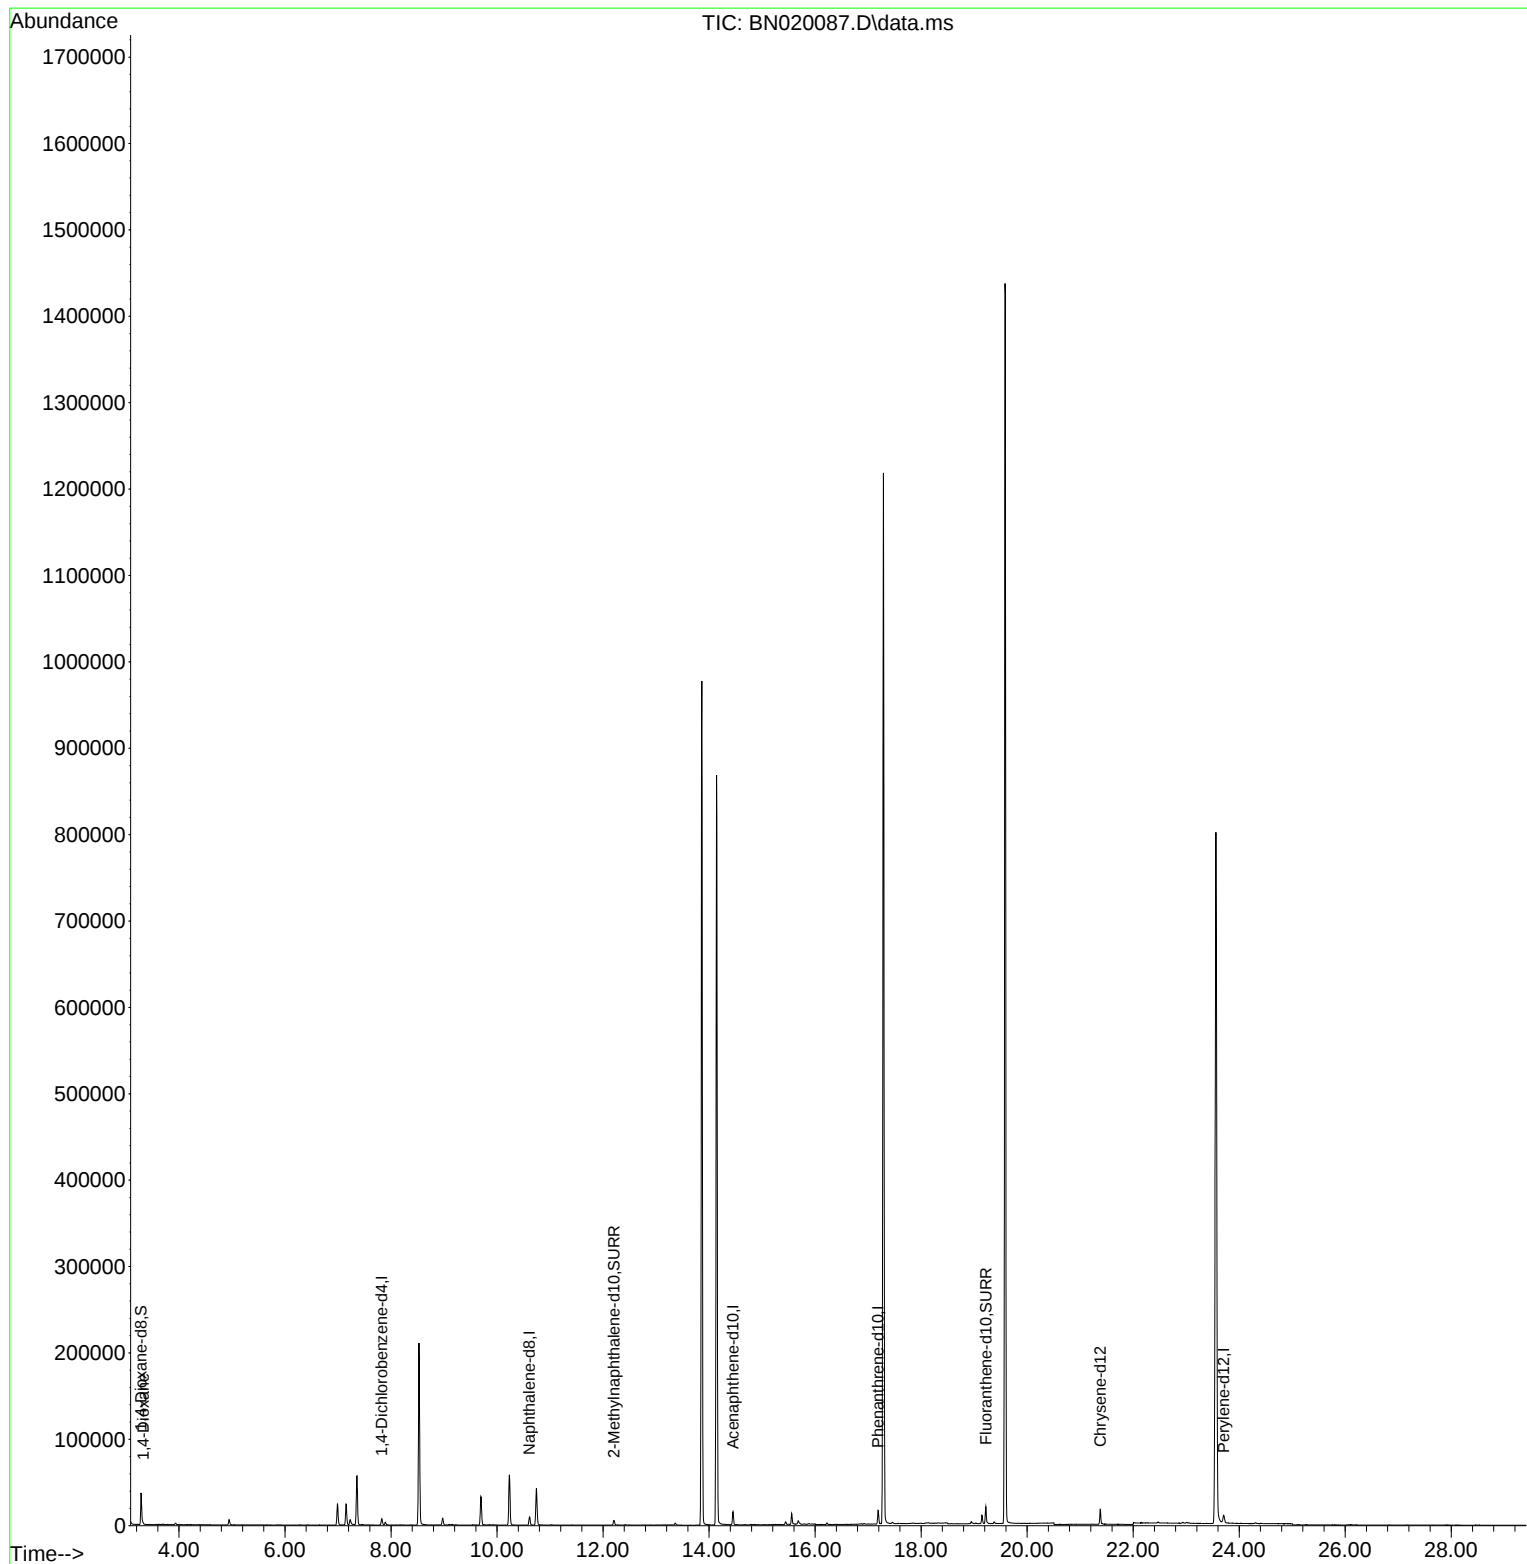

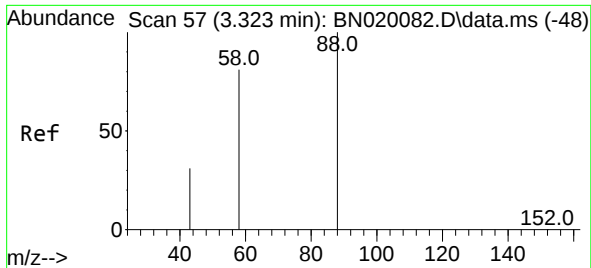

#2
 1,4-Dioxane
 Concen: 0.130 ng/ul m
 RT: 3.323 min Scan# 51
 Delta R.T. 0.000 min
 Lab File: BN020087.D
 Acq: 09 Jun 2022 19:06

Instrument :
 BNA_N
 ClientSampleId :
 F5A51

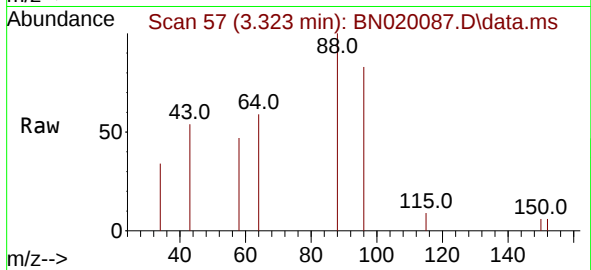

Tgt Ion: 88 Resp: 609

Ion	Ratio	Lower	Upper
88	100		
43	54.2	39.0	58.4
58	46.7	39.8	59.8

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 06/10/2022
 Supervised By :mohammad ahmed 06/10/2022

