

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061119\
 Data File : BN006248.D
 Acq On : 11 Jun 2019 16:19
 Operator : JU/SJ
 Sample : PB120295BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 12 01:11:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jun 09 05:10:30 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	4526	0.40	ng/ul	0.00
2) Naphthalene-d8	10.43	136	18545	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	10815	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.15	188	1875263	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.26
20) Perylene-d12	23.39	264	1260322	0.40	ng/ul	-0.10
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.03	152	11340	0.40	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.30	166	3927	0.080	ng/ul#	Ovalue 14




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061119\
Data File : BN006248.D
Acq On : 11 Jun 2019 16:19
Operator : JU/SJ
Sample : PB120295BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 12 01:11:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

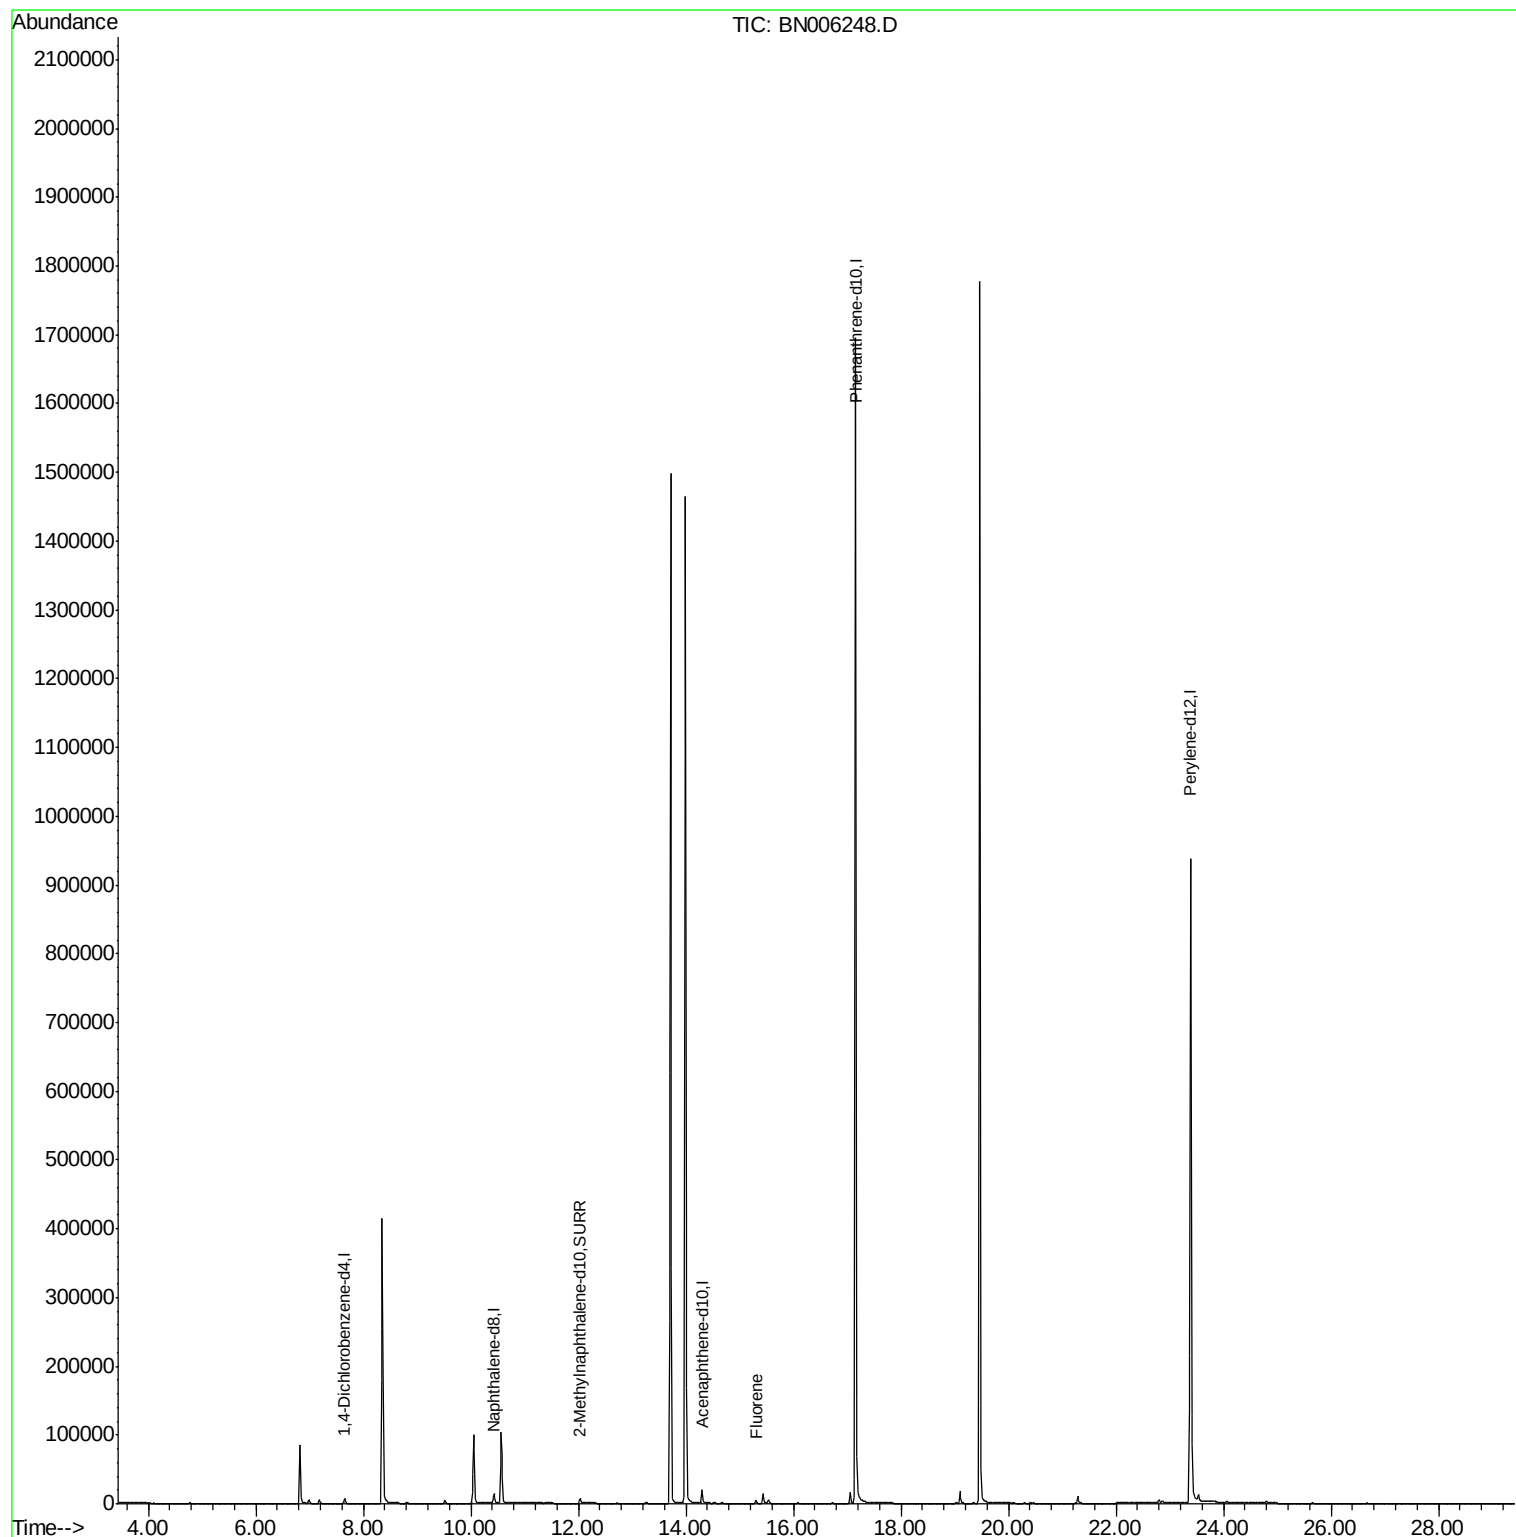

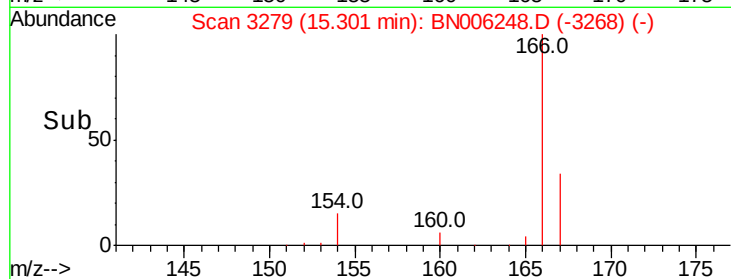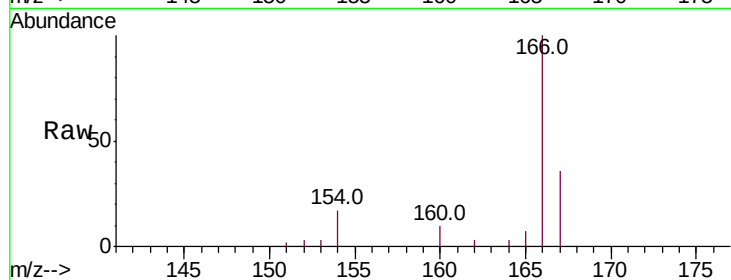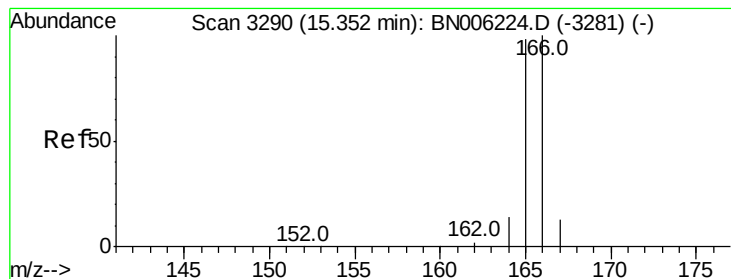

#9

Fluorene

Concen: 0.080 ng/ul

RT: 15.30 min Scan# 3279

Delta R.T. -0.05 min

Lab File: BN006248.D

Acq: 11 Jun 2019 16:19

Instrument :

BNA_N

ClientSampleId :

Tot Ion:166 Resp: 3927

Ion Ratio Lower Upper

166 100

165 7.1 76.4 114.6#

167 35.6 11.0 16.6#

