

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061119\
 Data File : BN006257.D
 Acq On : 11 Jun 2019 21:32
 Operator : JU/SJ
 Sample : PB120444BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 12 01:12:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jun 09 05:10:30 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	6108	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	24527	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	13439	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.15	188	2039742	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.26
20) Perylene-d12	23.35	264	1499024	0.40	ng/ul	-0.14
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	13464	0.36	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.30	166	4376	0.072	ng/ul#	Ovalue 14


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061119\
Data File : BN006257.D
Acq On : 11 Jun 2019 21:32
Operator : JU/SJ
Sample : PB120444BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 12 01:12:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

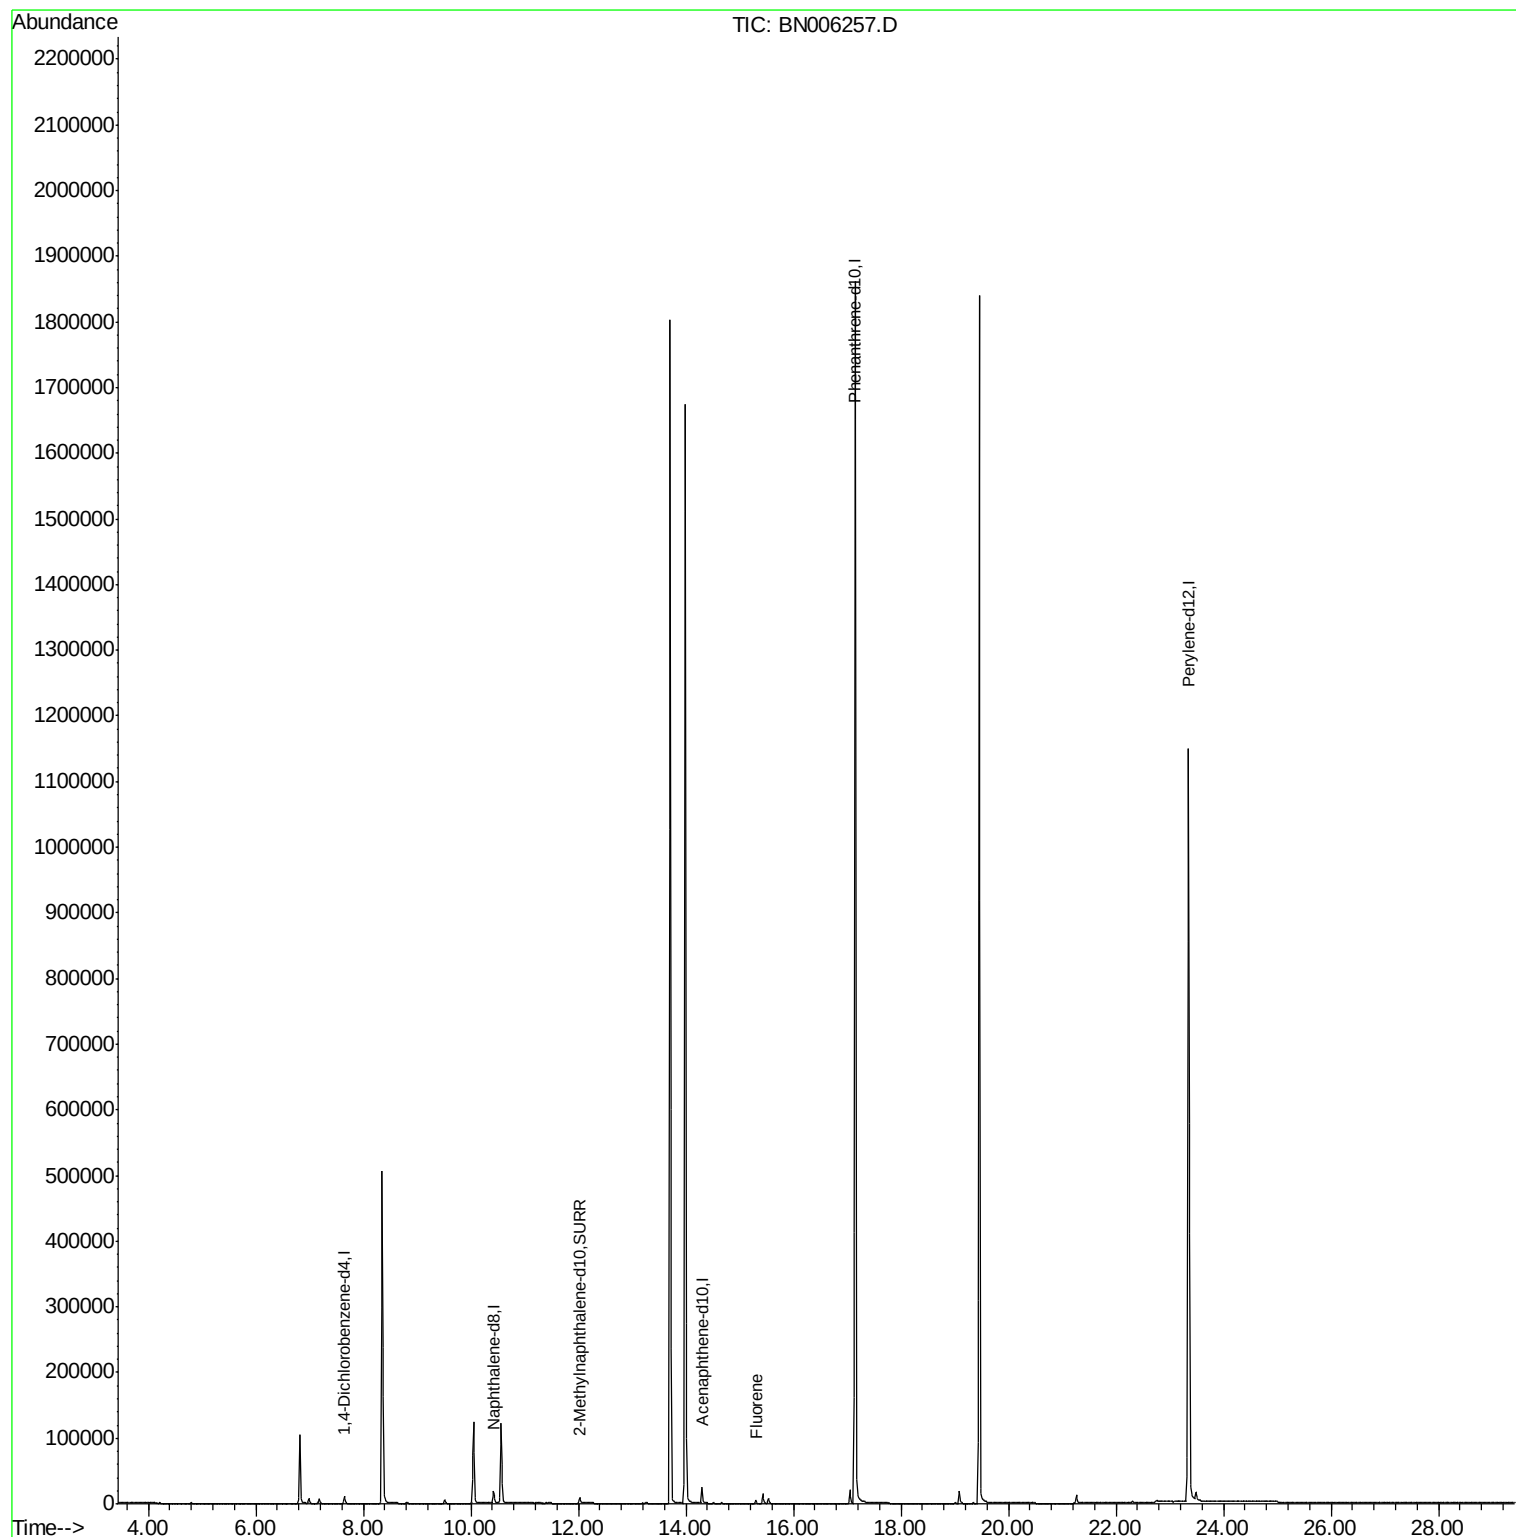

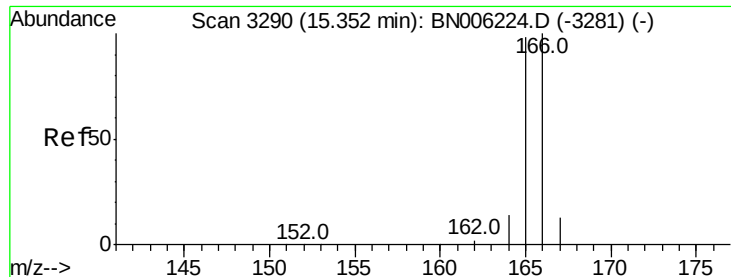

#9

Fluorene

Concen: 0.072 ng/ul

RT: 15.30 min Scan# 3278

Delta R.T. -0.06 min


Lab File: BN006257.D

Acq: 11 Jun 2019 21:32

Instrument :

BNA_N

ClientSampleId :

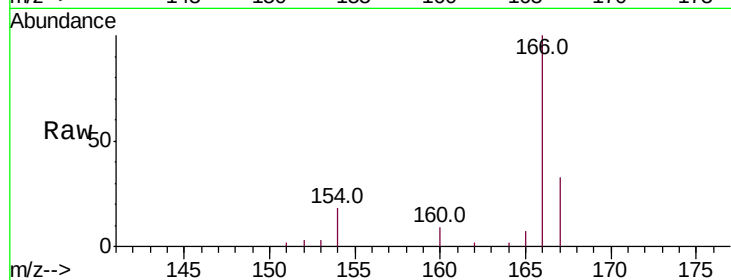


Tot Ion:166 Resp: 4376

Ion Ratio Lower Upper

166 100

165 6.6 76.4 114.6#

167 32.6 11.0 16.6#

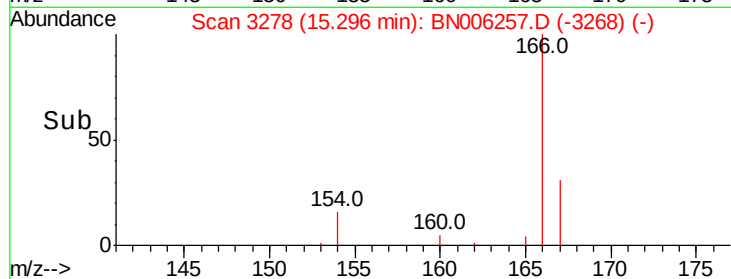

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

