

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061119\
 Data File : BN006263.D
 Acq On : 12 Jun 2019 01:34
 Operator : JU/SJ
 Sample : K3215-07
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 12 02:46:26 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jun 09 05:10:30 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	5876	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	22028	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.29	164	19335	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.15	188	1647306	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.26
20) Perylene-d12	23.35	264	1479848	0.40	ng/ul	-0.14
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	10221	0.30	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
3) Naphthalene	10.47	128	79277	1.304	ng/ul	100
5) 2-Methylnaphthalene	12.09	142	12462	0.294	ng/ul	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061119\
Data File : BN006263.D
Acq On : 12 Jun 2019 01:34
Operator : JU/SJ
Sample : K3215-07
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 12 02:46:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

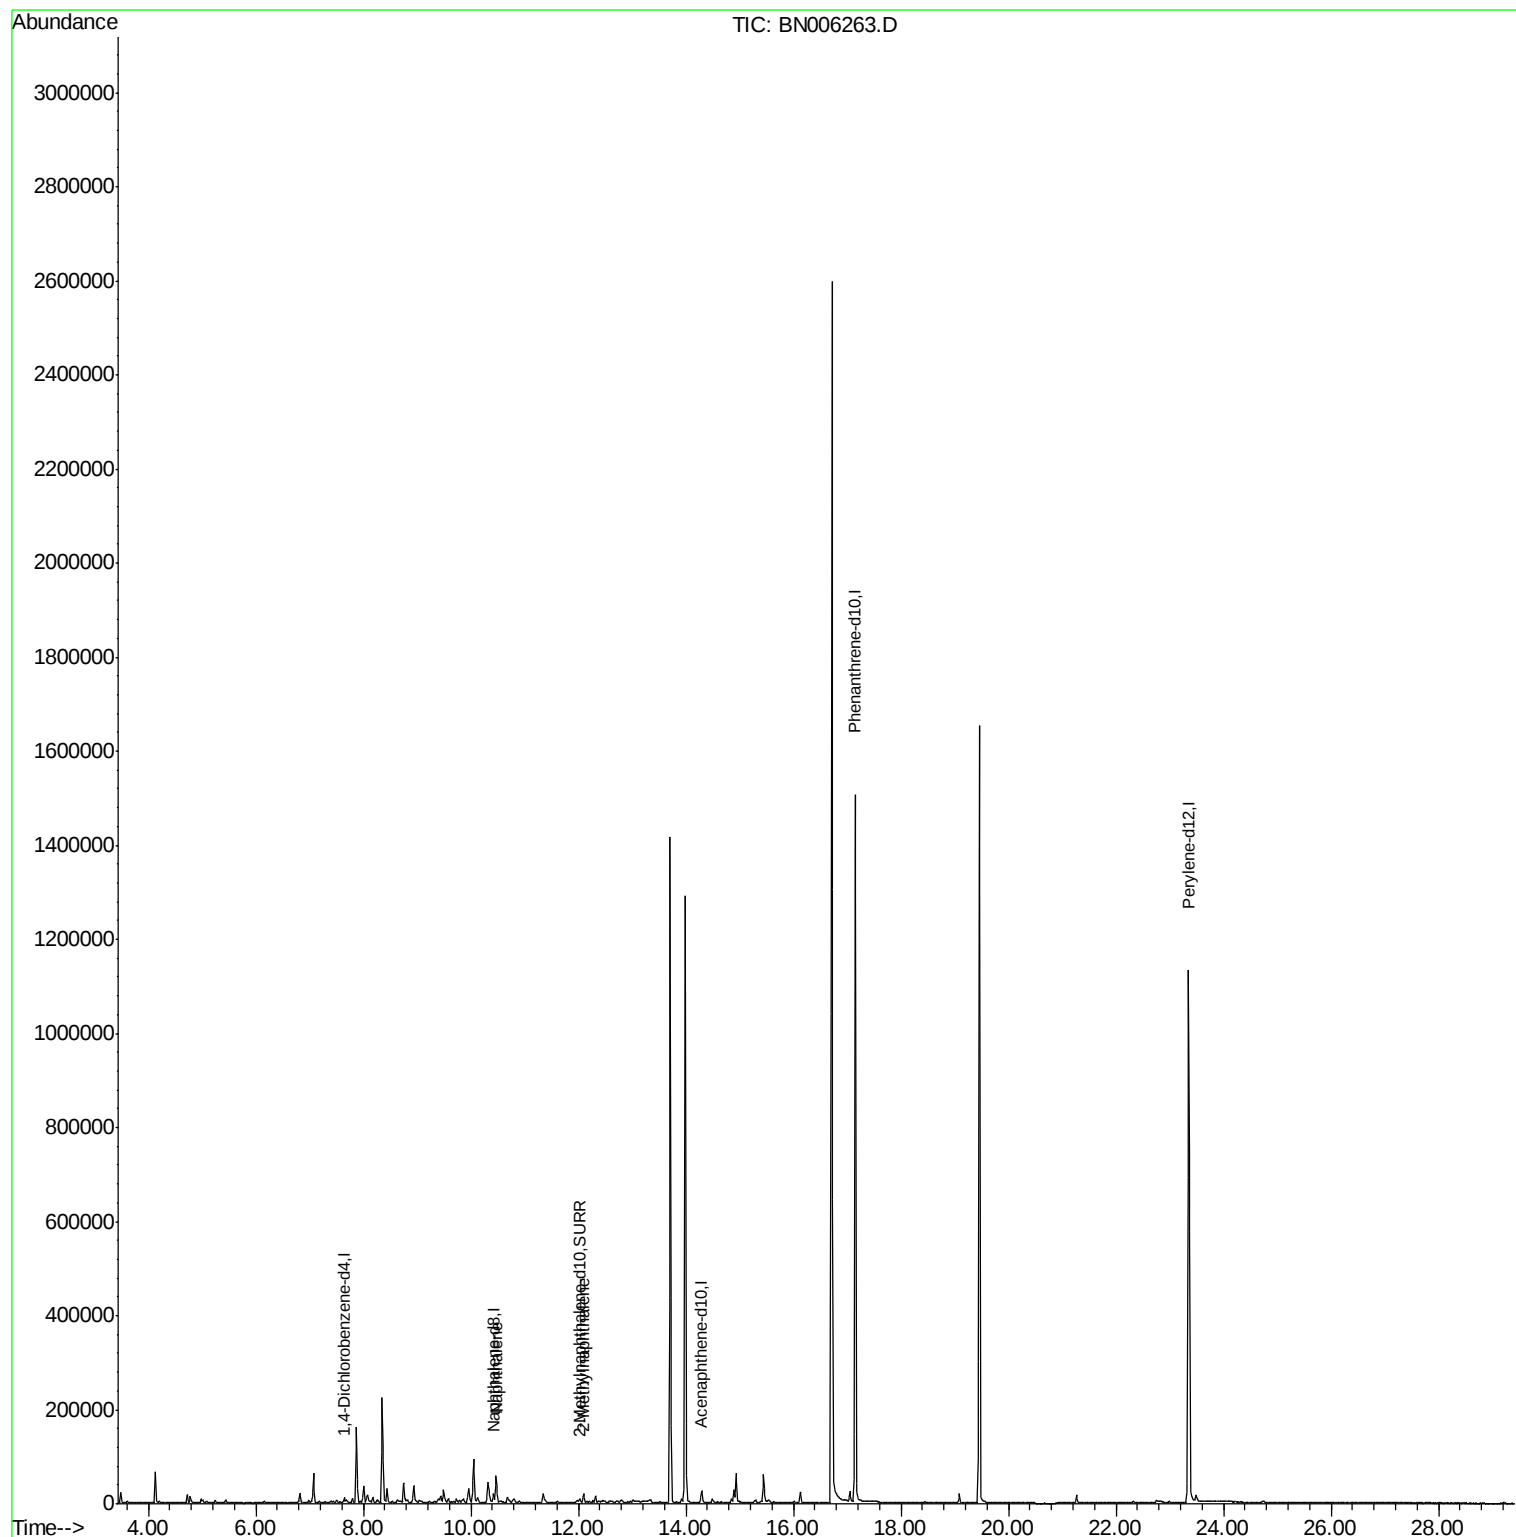

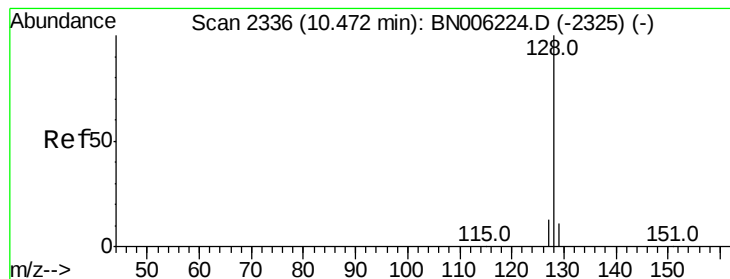

#3

Naphthalene

Concen: 1.304 ng/ul

RT: 10.47 min Scan# 2336

Delta R.T. -0.00 min

Lab File: BN006263.D

Acq: 12 Jun 2019 01:34

Instrument :

BNA_N

ClientSampleId :


Tot Ion:128 Resp: 79277

Ion Ratio Lower Upper

128 100

129 11.6 9.3 13.9




127 13.4 10.7 16.1

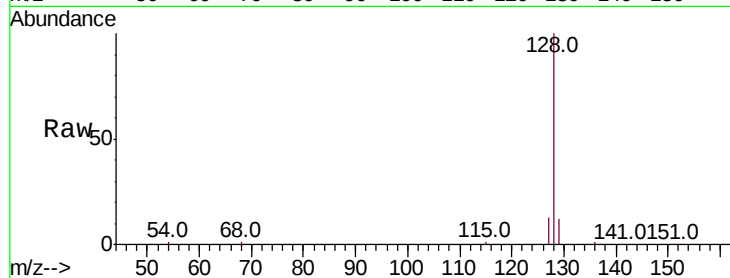

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

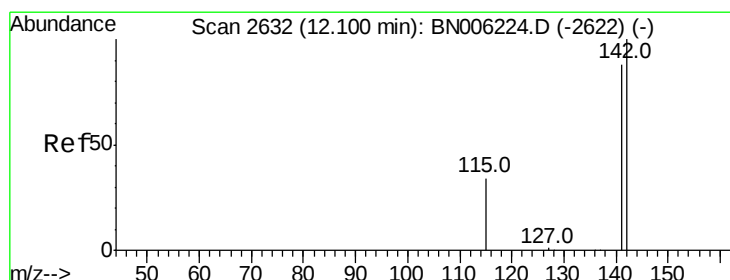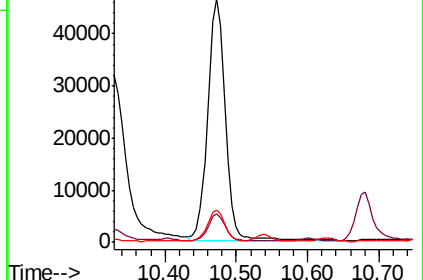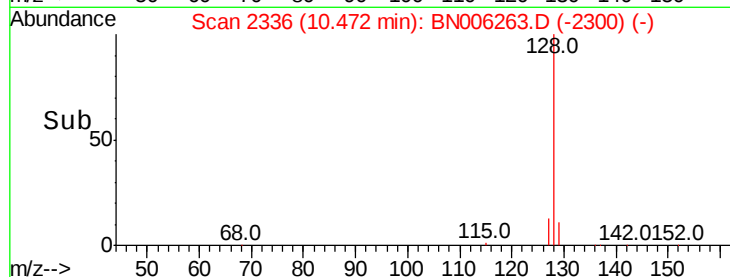

#5

2-Methylnaphthalene

Concen: 0.294 ng/ul

RT: 12.09 min Scan# 2631

Delta R.T. -0.01 min

Lab File: BN006263.D


Acq: 12 Jun 2019 01:34

Tgt Ion:142 Resp: 12462

Ion Ratio Lower Upper

142 100

141 98.3 70.3 105.5

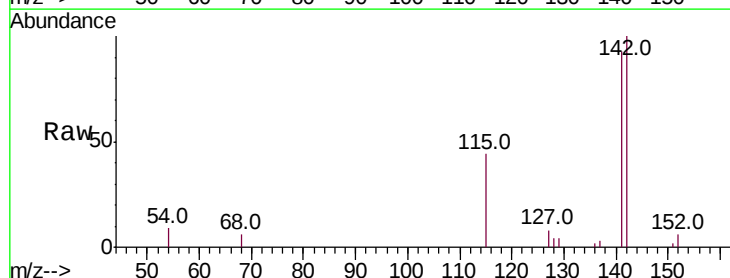

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

