

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061119\
 Data File : BN006270.D
 Acq On : 12 Jun 2019 05:35
 Operator : JU/SJ
 Sample : K3215-14
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 12 06:52:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jun 09 05:10:30 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	5945	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	23042	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.29	164	12735	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.15	188	1679013	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.26
20) Perylene-d12	23.35	264	1430595	0.40	ng/ul	-0.14
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	9820	0.28	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
3) Naphthalene	10.47	128	4185	0.066	ng/ul#	Ovalue 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061119\
Data File : BN006270.D
Acq On : 12 Jun 2019 05:35
Operator : JU/SJ
Sample : K3215-14
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 12 06:52:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

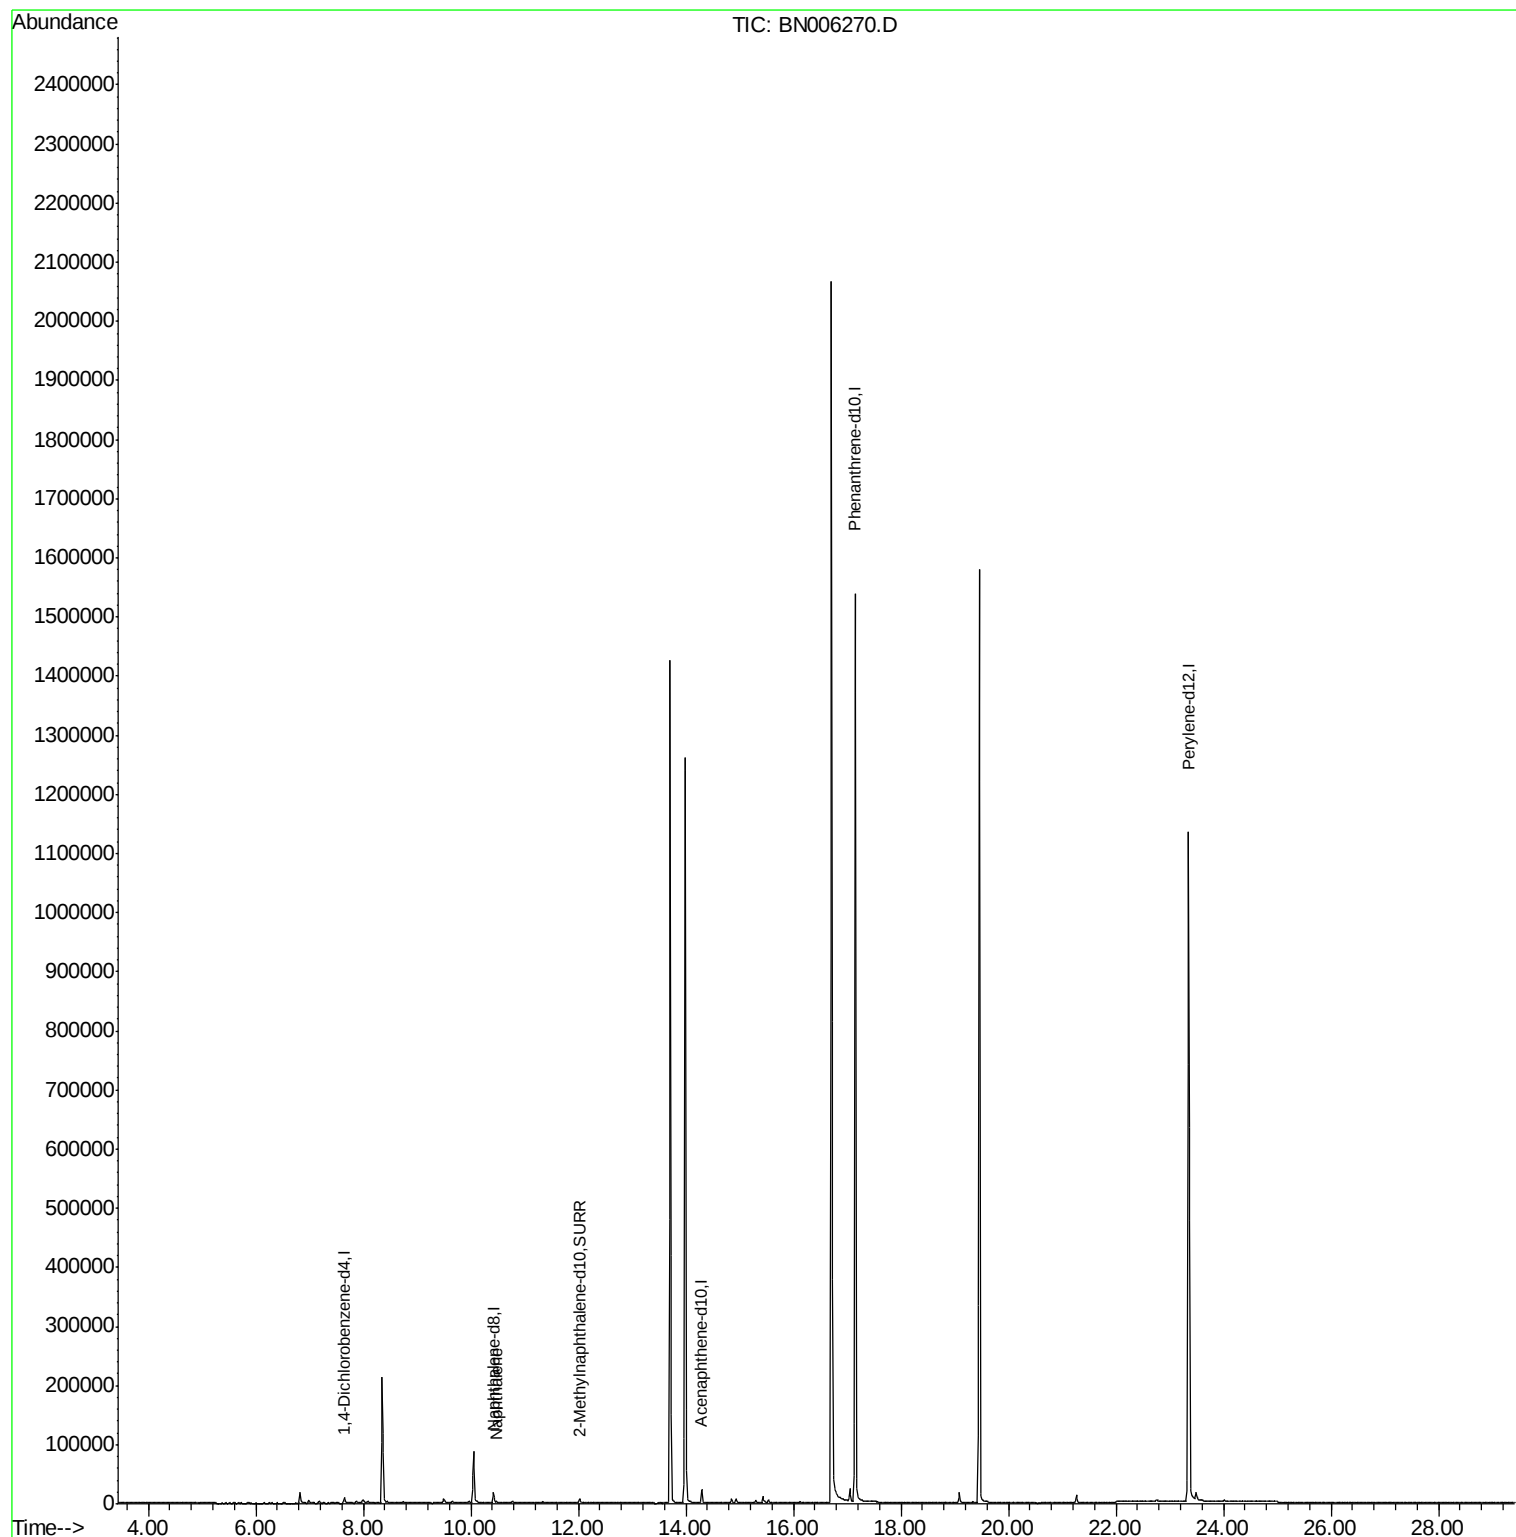

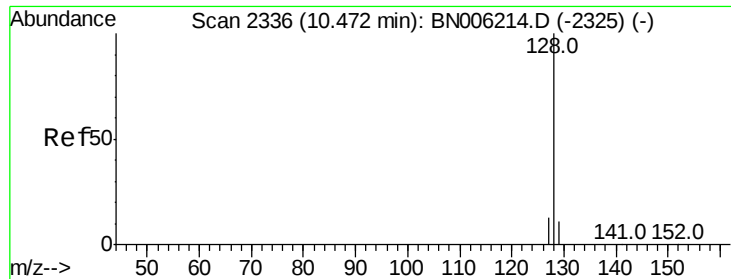

#3

Naphthalene

Concen: 0.066 ng/ul

RT: 10.47 min Scan# 2336

Delta R.T. -0.00 min


Lab File: BN006270.D

Acq: 12 Jun 2019 05:35

Instrument :

BNA_N

ClientSampleId :

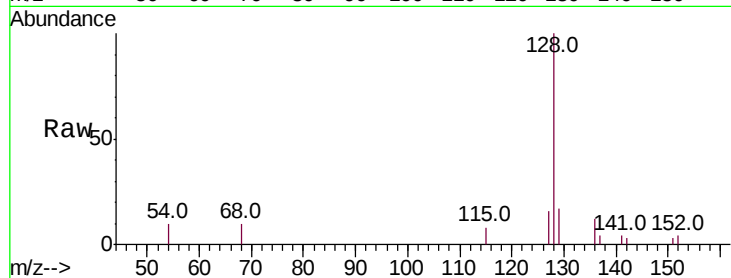


Tot Ion:128 Resp: 4185

Ion Ratio Lower Upper

128 100

129 16.8 9.3 13.9#

127 16.3 10.7 16.1#

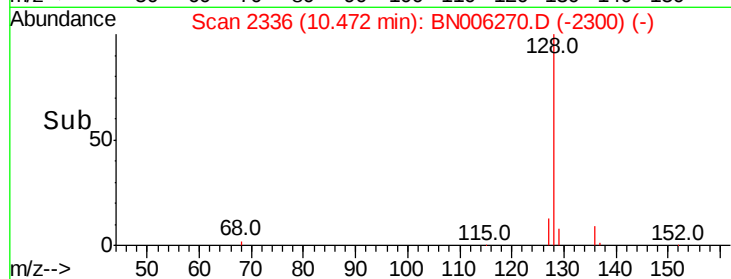

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

