

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061119\
 Data File : BN006267.D
 Acq On : 12 Jun 2019 03:52
 Operator : JU/SJ
 Sample : K3215-11
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB8J5

Manual Integrations
 APPROVED

mohammad
 6/12/2019 8:19:37 AM

Quant Time: Jun 12 07:24:08 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jun 09 05:10:30 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	6471	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	26706	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	14197	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	27035m	0.40	ng/ul	0.00
16) Chrysene-d12	21.26	240	16307m	0.40	ng/ul	0.00
20) Perylene-d12	23.49	264	28180	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	9827	0.24	ng/ul	0.00
14) Fluoranthene-d10	19.08	212	19791m	0.27	ng/ul	0.00
Target Compounds						
9) Fluorene	15.35	166	3488	0.054	ng/ul#	90
11) Pentachlorophenol	16.71	266	1554m	0.226	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061119\
Data File : BN006267.D
Acq On : 12 Jun 2019 03:52
Operator : JU/SJ
Sample : K3215-11
Misc :
ALS Vial : 26 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
DB8J5

Manual Integrations
APPROVED

mohammad
6/12/2019 8:19:37 AM

Quant Time: Jun 12 07:24:08 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

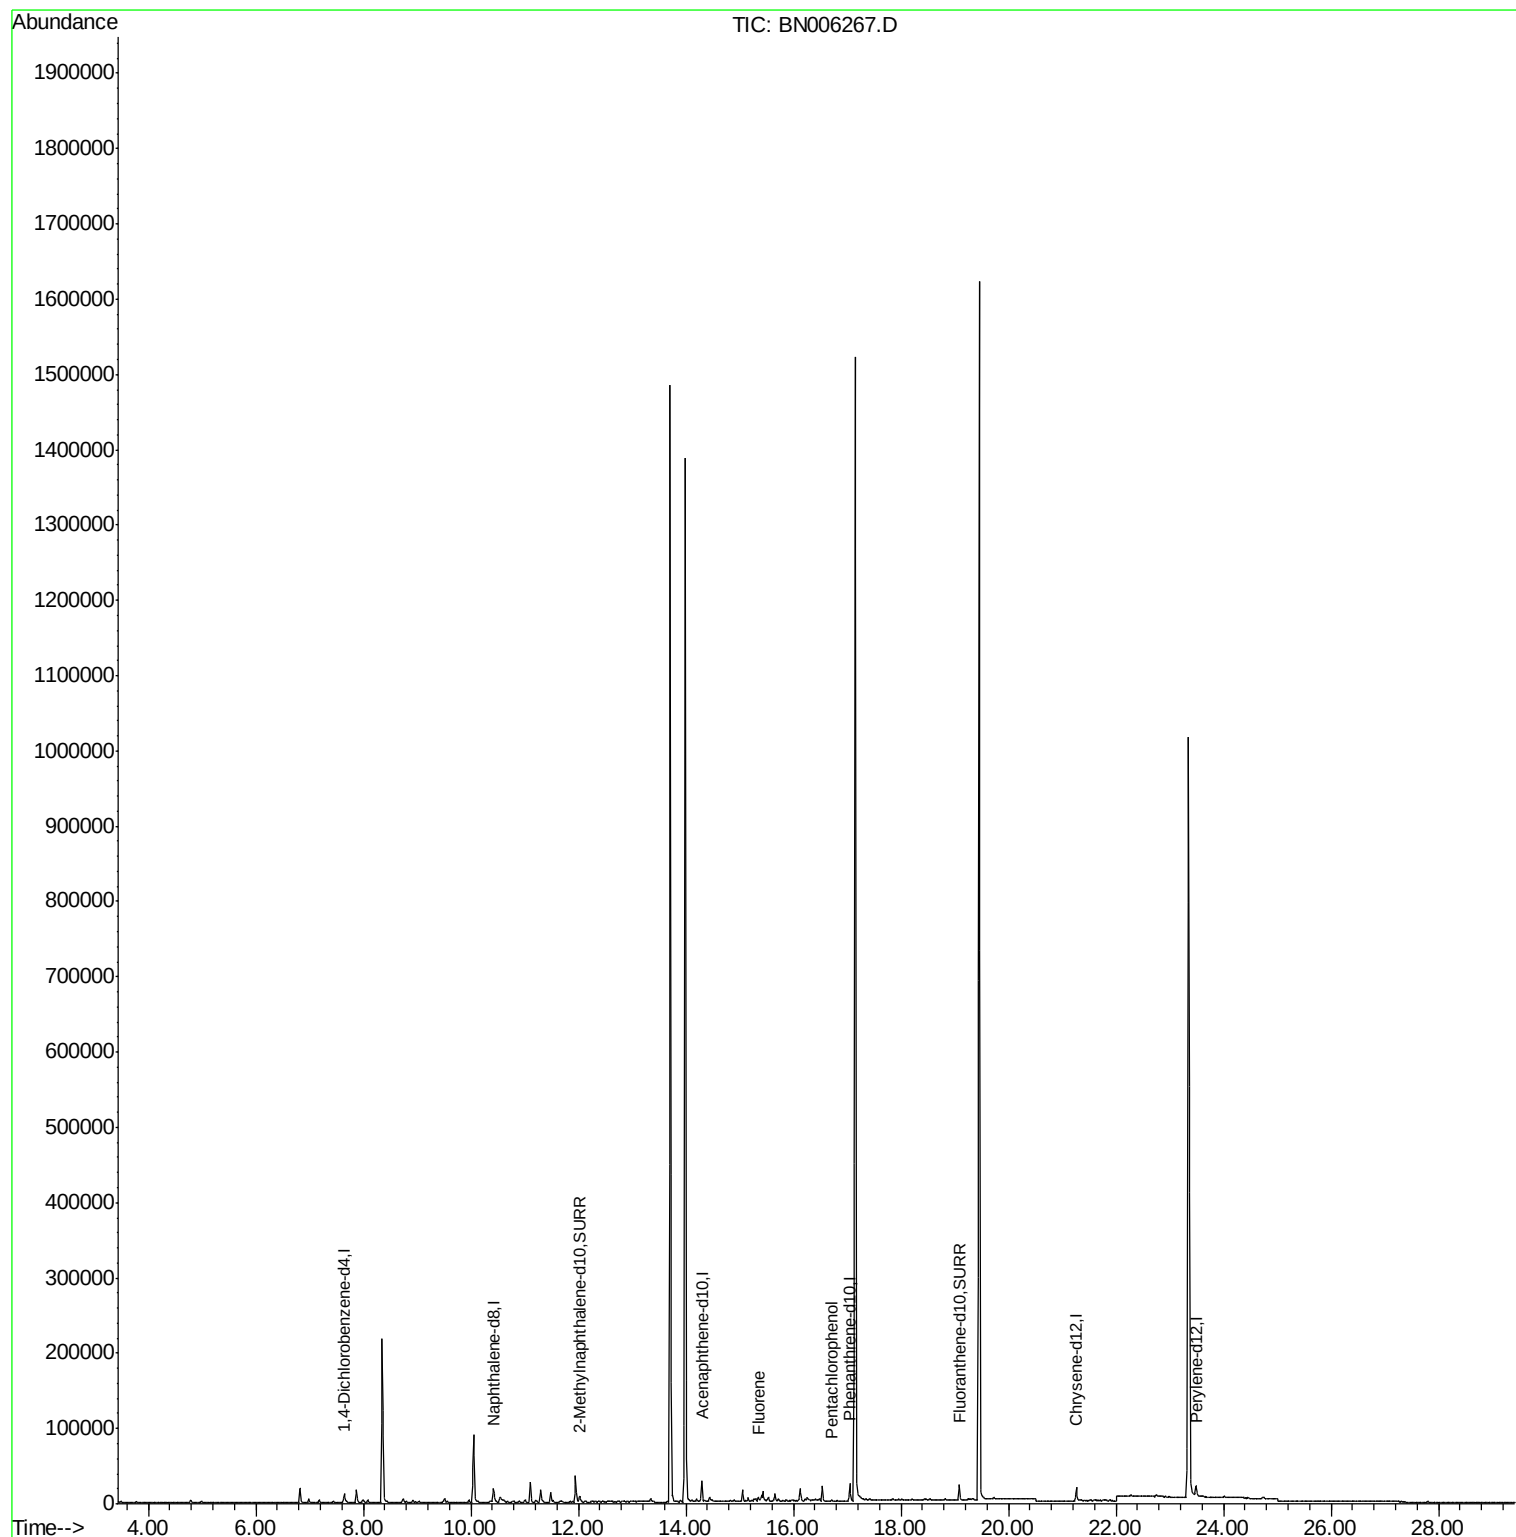

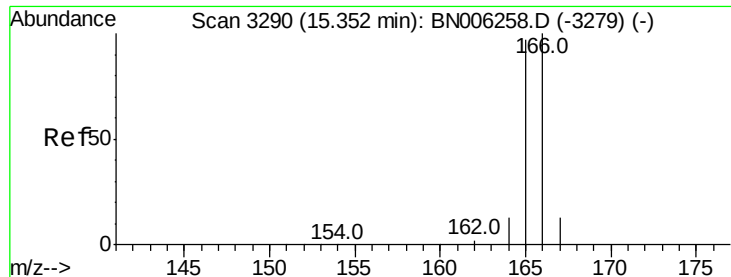

#9

Fluorene

Concen: 0.054 ng/ul

RT: 15.35 min Scan# 3290

Delta R.T. -0.00 min

Lab File: BN006267.D

Acq: 12 Jun 2019 03:52

Instrument :

BNA_N





ClientSampled :

DB8J5

Tot Ion	Ratio	Lower	Upper
166	100		
165	103.0	76.4	114.6
167	24.0	11.0	16.6#

Manual Integrations
APPROVED

mohammad
6/12/2019 8:19:37 AM

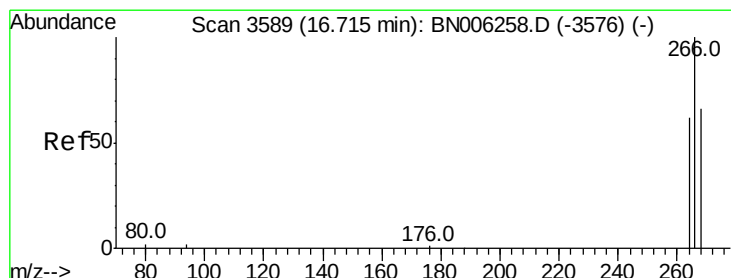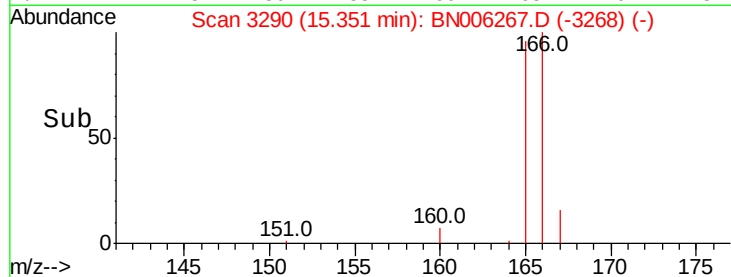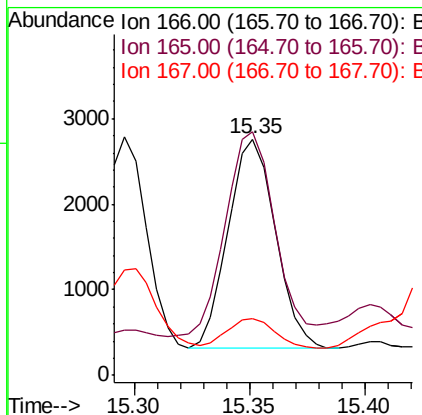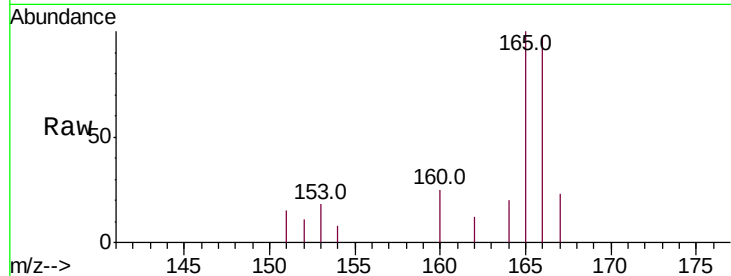

#11

Pentachlorophenol

Concen: 0.226 ng/ul m

RT: 16.71 min Scan# 3588

Delta R.T. -0.00 min

Lab File: BN006267.D

Acq: 12 Jun 2019 03:52

Tgt Ion	Ratio	Lower	Upper
266	100		
264	0.0	50.3	75.5#
268	1.4	51.3	76.9#

