

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061219\
 Data File : BN006295.D
 Acq On : 12 Jun 2019 23:39
 Operator : JU/SJ
 Sample : K3231-16
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 13 01:22:50 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 12 17:24:11 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	5615	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	22678	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	11617	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	21390	0.40	ng/ul	0.00
16) Chrysene-d12	21.27	240	13636	0.40	ng/ul	-0.02
20) Perylene-d12	23.49	264	17643	0.40	ng/ul	-0.05
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	4334	0.12	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	7382	0.13	ng/ul	0.00
Target Compounds				Ovalue		
11) Pentachlorophenol	16.71	266	1286	0.237	ng/ul	97
12) Phenanthrene	17.09	178	1571	0.023	ng/ul#	83
15) Fluoranthene	19.12	202	3480	0.046	ng/ul	62
17) Pyrene	19.48	202	7050	0.098	ng/ul#	85
19) Chrysene	21.30	228	1793	0.032	ng/ul#	79
21) Benzo(b)fluoranthene	22.83	252	3986	0.054	ng/ul#	1
22) Benzo(k)fluoranthene	22.83	252	3986	0.056	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061219\
Data File : BN006295.D
Acq On : 12 Jun 2019 23:39
Operator : JU/SJ
Sample : K3231-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 13 01:22:50 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 12 17:24:11 2019
Response via : Initial Calibration




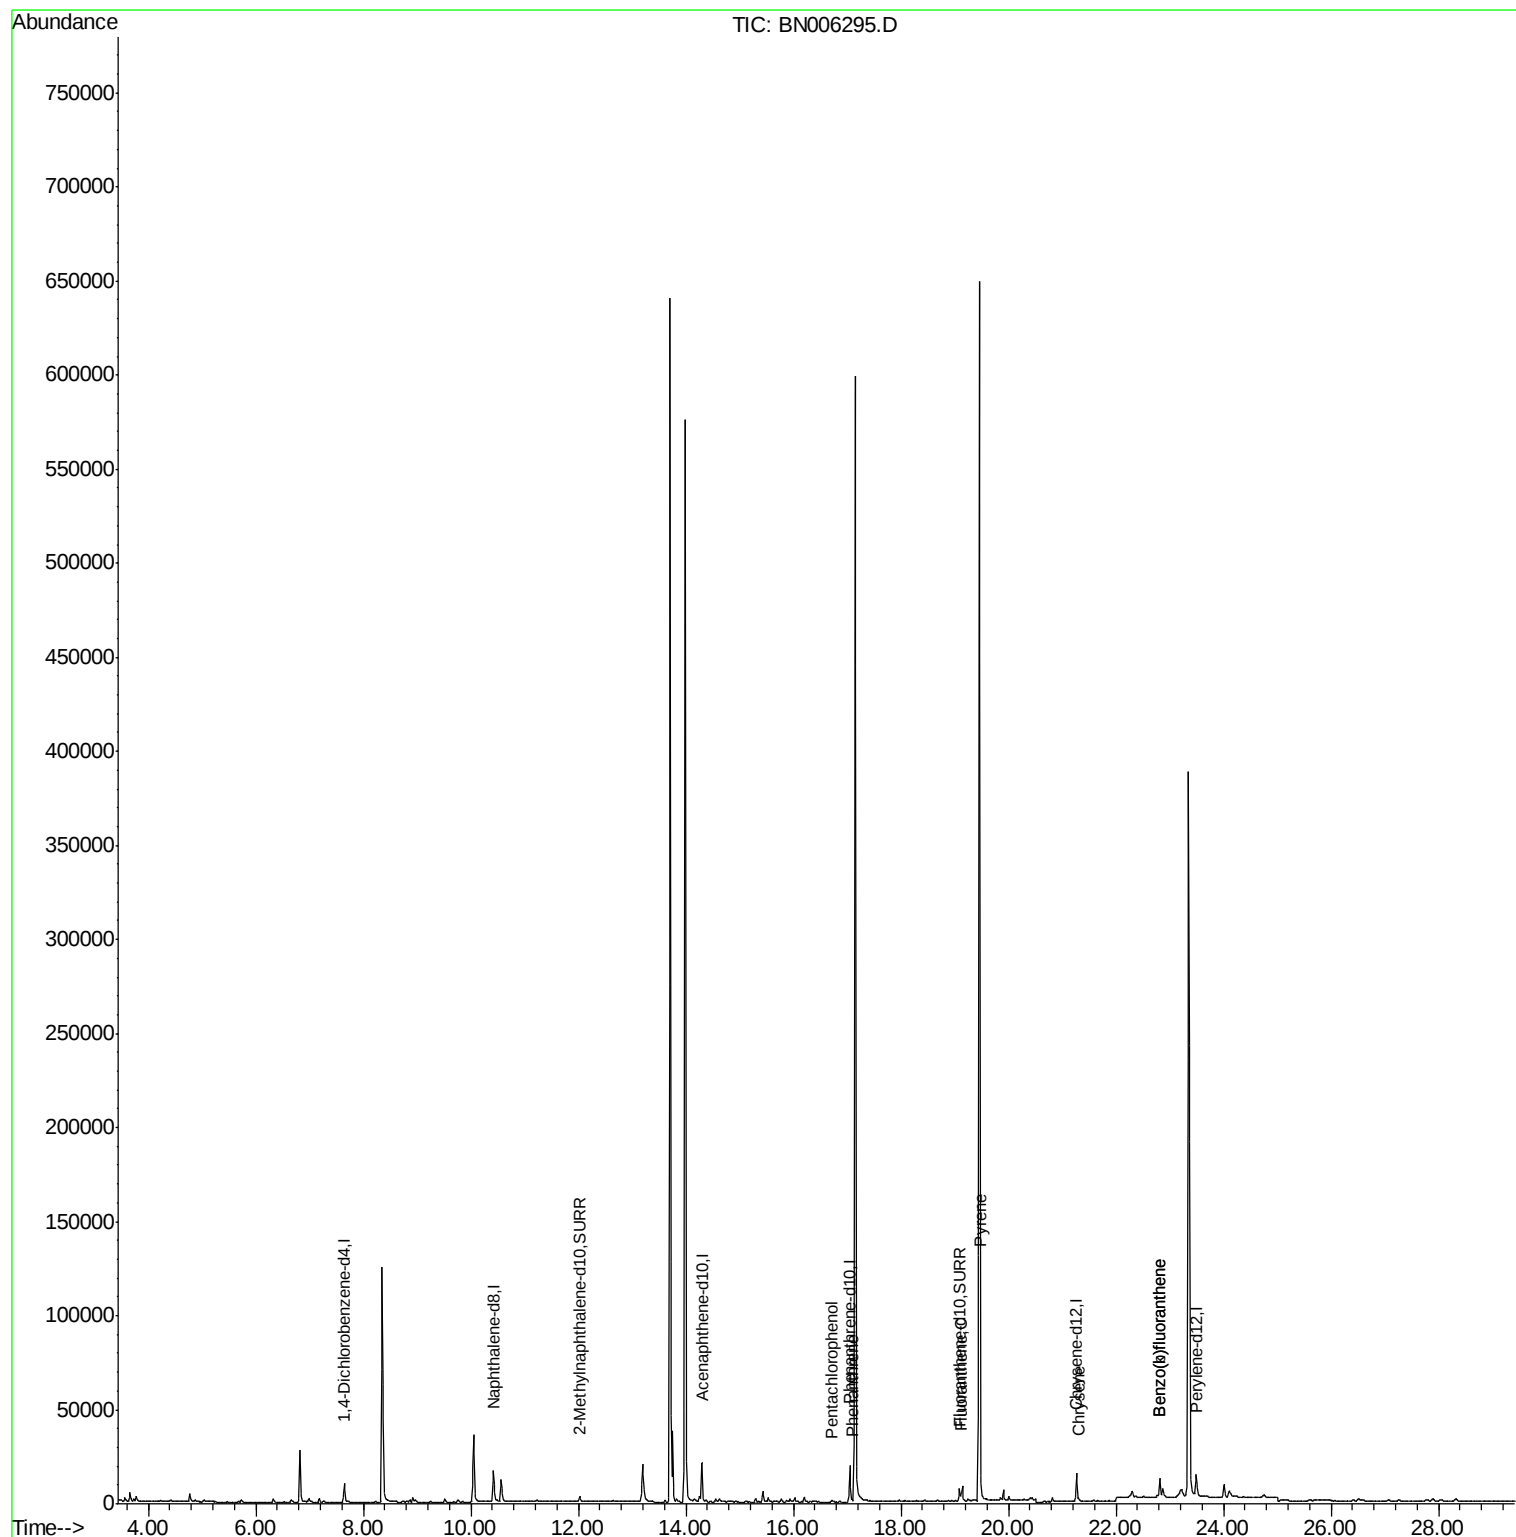


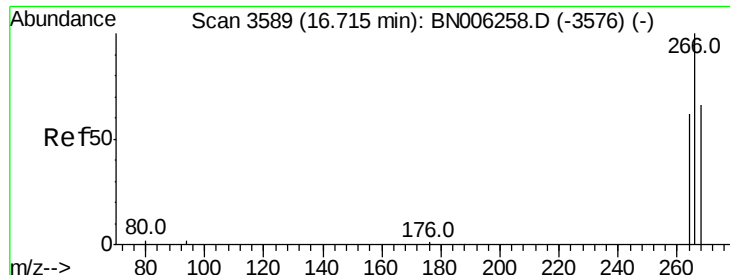

#11
 Pentachlorophenol
 Concen: 0.237 ng/ul
 RT: 16.71 min Scan# 3589
 Delta R.T. -0.00 min
 Lab File: BN006295.D
 Acq: 12 Jun 2019 23:39




Instrument :
 BNA_N
 ClientSampleId :


Tot Ion:	266	Resp:	1286
Ion	Ratio	Lower	Upper
266	100		
264	59.9	50.3	75.5
268	62.1	51.3	76.9

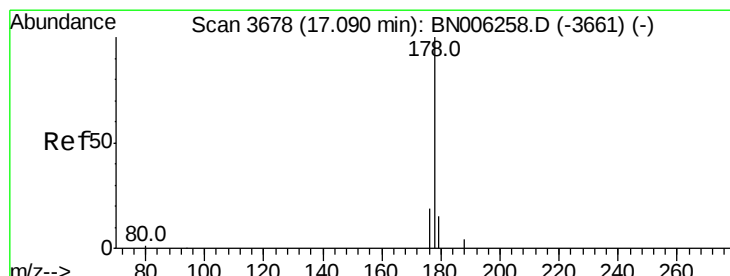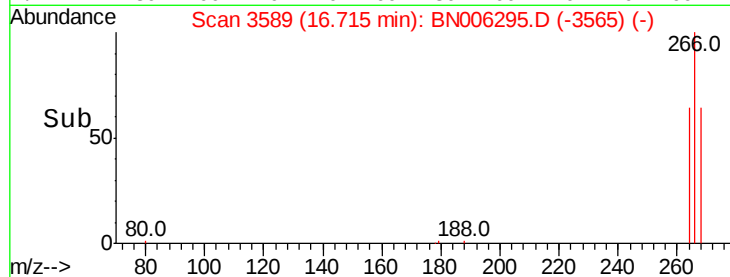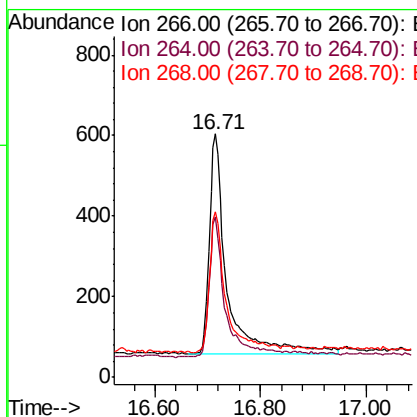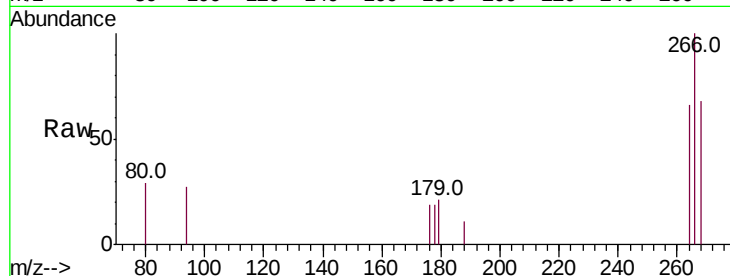

#12
 Phenanthrene
 Concen: 0.023 ng/ul
 RT: 17.09 min Scan# 3678
 Delta R.T. -0.00 min
 Lab File: BN006295.D
 Acq: 12 Jun 2019 23:39

Tgt Ion:	178	Resp:	1571
Ion	Ratio	Lower	Upper
178	100		
179	24.2	12.3	18.5#
176	25.4	15.3	22.9#

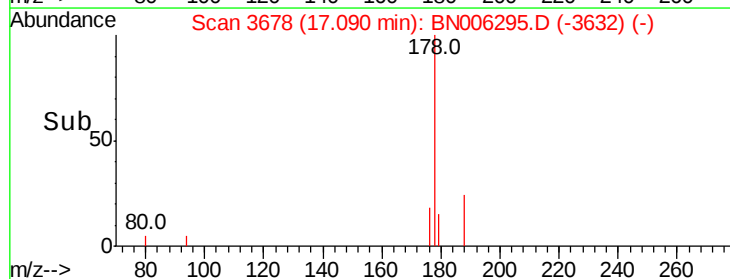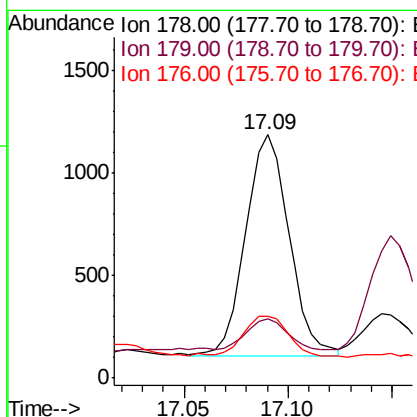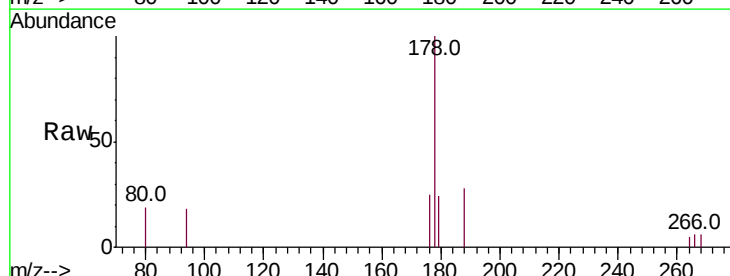


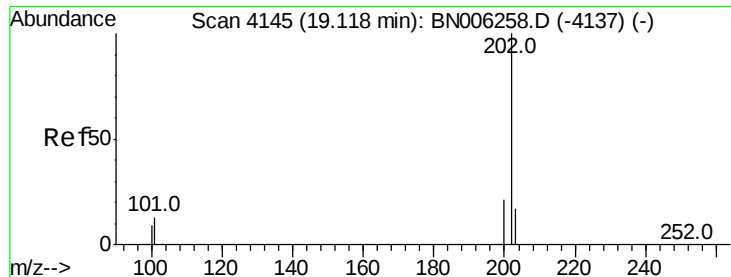




#15
Fluoranthene
Concen: 0.046 ng/ul
RT: 19.12 min Scan# 4145
Delta R.T. -0.01 min
Lab File: BN006295.D
Acq: 12 Jun 2019 23:39

Instrument :
BNA_N
ClientSampleId :

Tot Ion:202 Resp: 3480
Ion Ratio Lower Upper
202 100
101 27.0 0.0 32.1
100 22.0 0.0 28.7

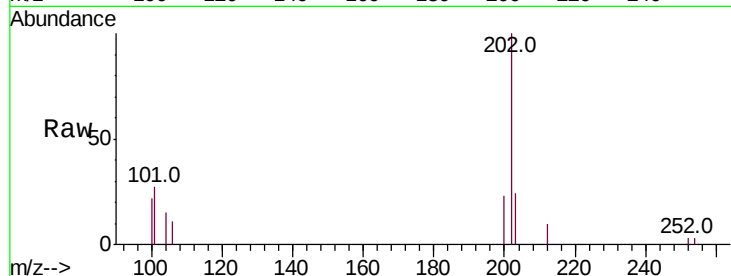


Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

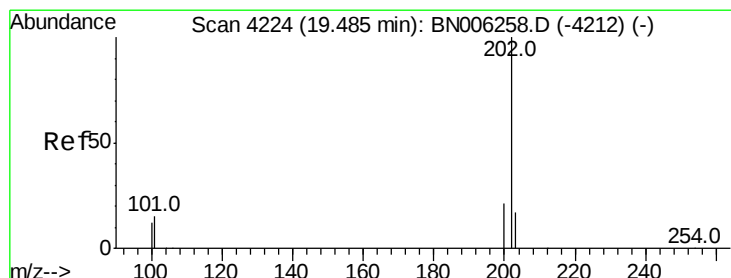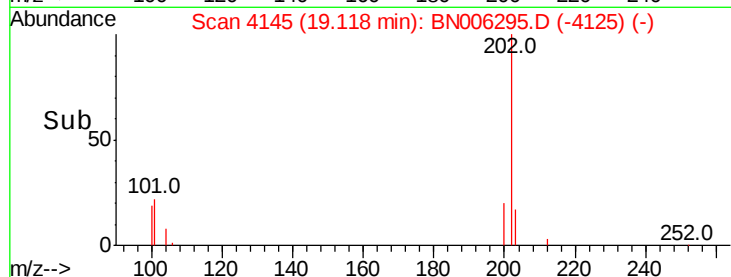
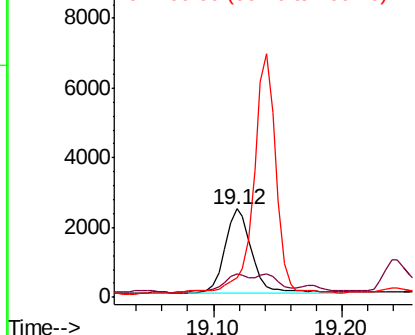



#17
Pyrene
Concen: 0.098 ng/ul
RT: 19.48 min Scan# 4223
Delta R.T. -0.01 min
Lab File: BN006295.D
Acq: 12 Jun 2019 23:39

Tgt Ion:202 Resp: 7050
Ion Ratio Lower Upper
202 100
101 20.4 12.2 18.2#
100 19.0 9.8 14.6#

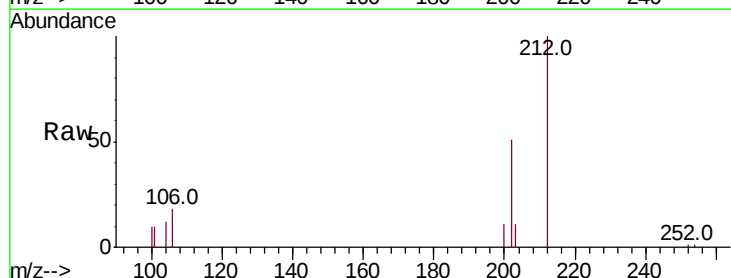

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

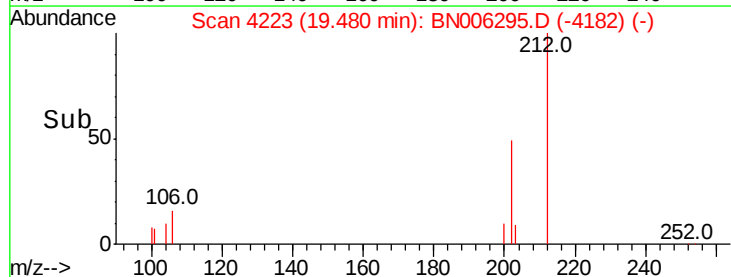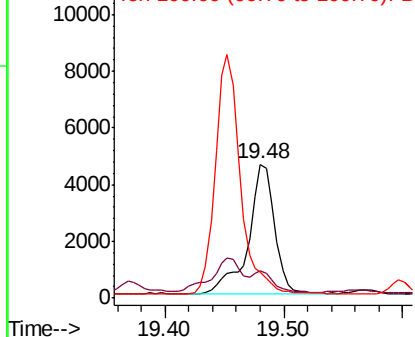

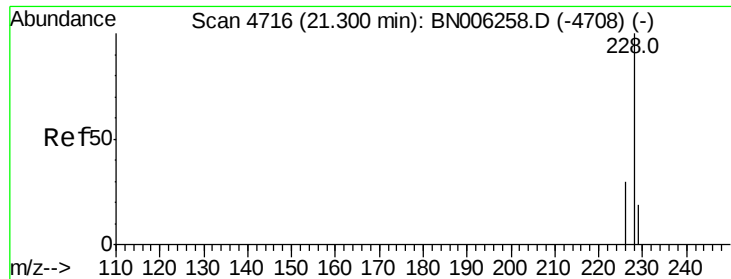

#19

Chrysene

Concen: 0.032 ng/ul

RT: 21.30 min Scan# 4715

Delta R.T. -0.03 min

Lab File: BN006295.D

Acq: 12 Jun 2019 23:39

Instrument :

BNA_N

ClientSampleId :


Tot Ion:228 Resp: 1793

Ion Ratio Lower Upper

228 100

226 39.4 25.0 37.6#




229 34.2 16.3 24.5#

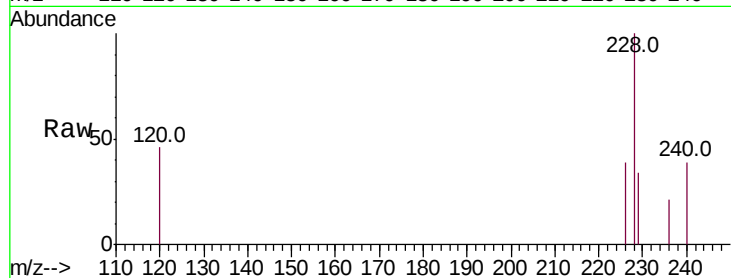

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

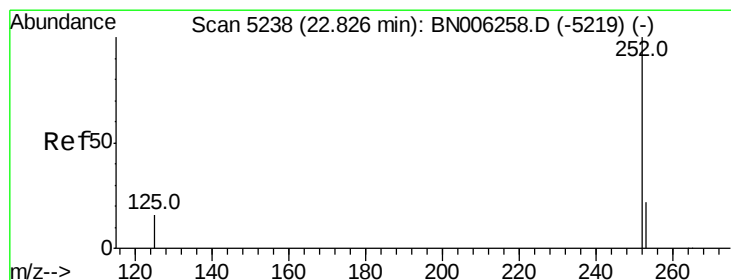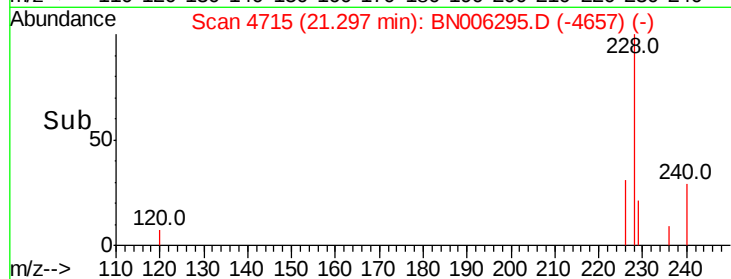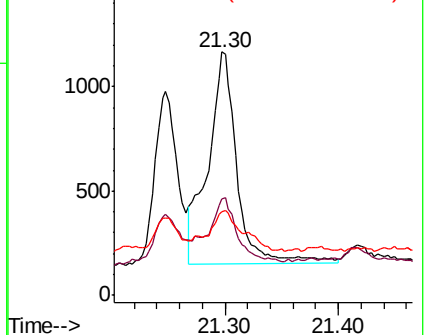

#21

Benzo(b)fluoranthene

Concen: 0.054 ng/ul

RT: 22.83 min Scan# 5238

Delta R.T. -0.05 min

Lab File: BN006295.D

Acq: 12 Jun 2019 23:39


Tgt Ion:252 Resp: 3986

Ion Ratio Lower Upper

252 100

253 66.9 0.0 51.4#



125 296.8 0.0 41.0#

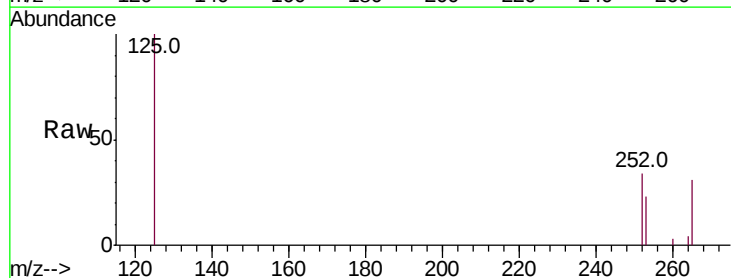


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

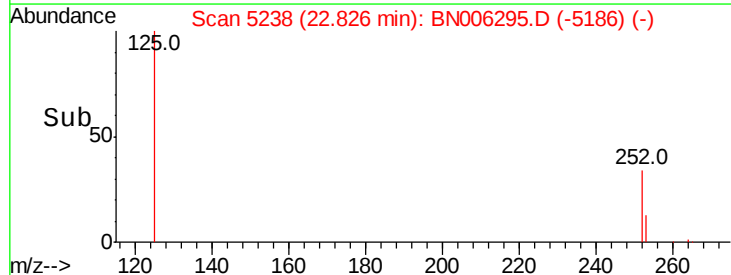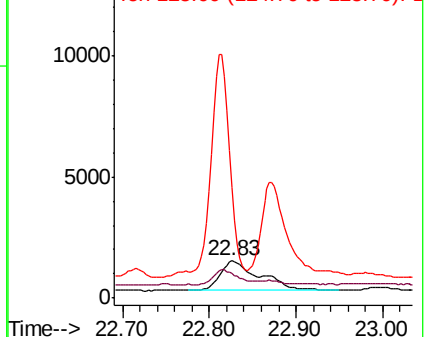

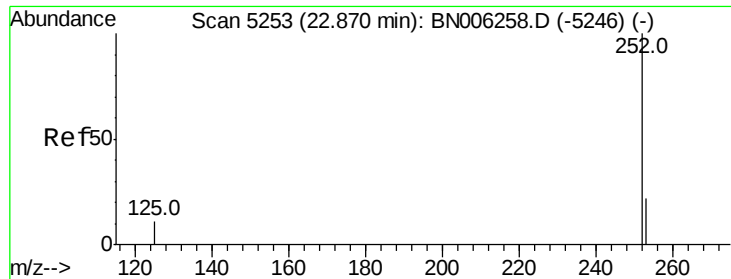

#22

Benzo(k)fluoranthene

Concen: 0.056 ng/ul

RT: 22.83 min Scan# 5238

Delta R.T. -0.09 min

Lab File: BN006295.D

Acq: 12 Jun 2019 23:39

Instrument :

BNA_N

ClientSampleId :


Tot Ion:252 Resp: 3986

Ion Ratio Lower Upper

252 100

253 66.9 20.3 30.5#

125 296.8 14.3 21.5#

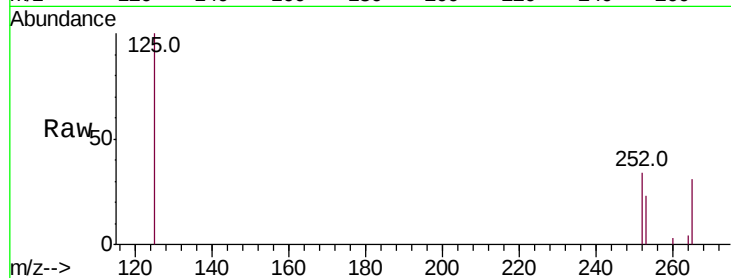

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

