


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN061219\
Data File : BN006287.D
Acq On : 12 Jun 2019 19:02
Operator : JU/SJ
Sample : K3231-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DB8L5

Manual Integrations
APPROVED

mohammad
6/14/2019 8:34:02 AM

Quant Time: Jun 13 02:20:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 12 17:24:11 2019
Response via : Initial Calibration

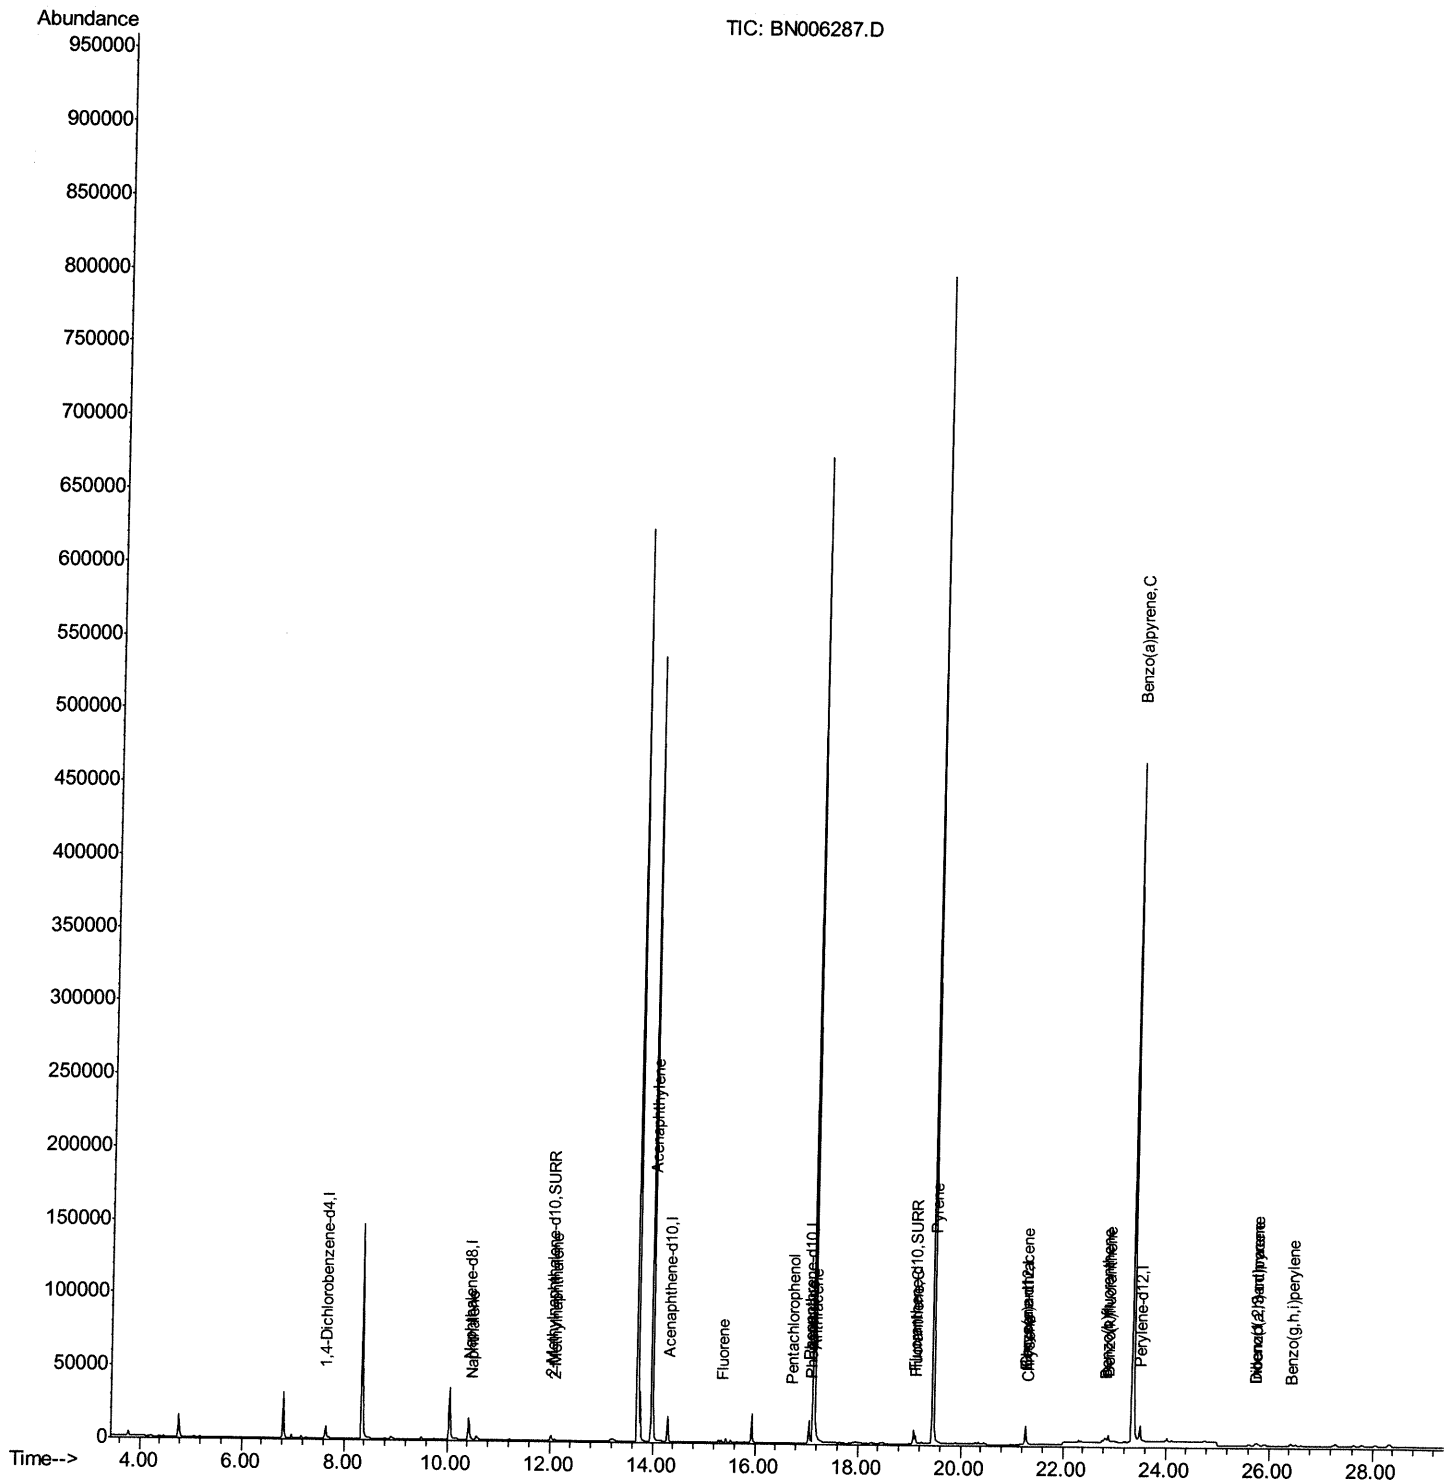

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN061219\
 Data File : BN006287.D
 Acq On : 12 Jun 2019 19:02
 Operator : JU/SJ
 Sample : K3231-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB8L5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:34:02 AM

Quant Time: Jun 13 01:22:15 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 12 17:24:11 2019
 Response via : Initial Calibration

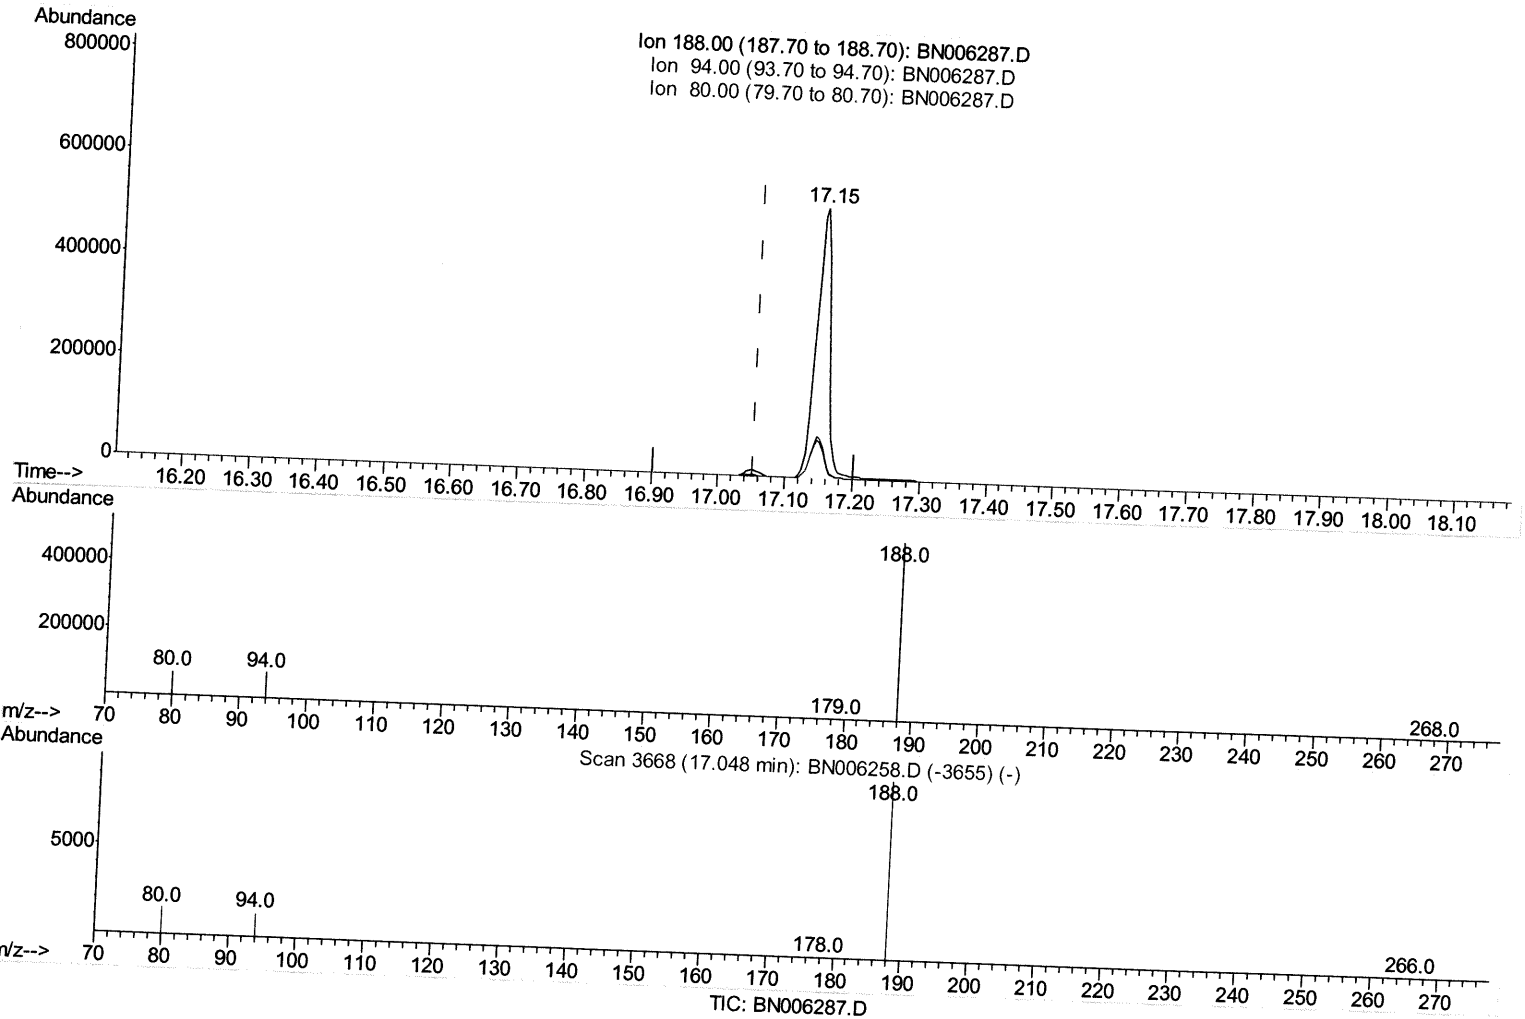

(10) Phenanthrene-d10 (I)

17.149min (+0.097) 0.40ng/ul

response 738839

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	14.34
80.00	13.60	13.10
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN061219\
 Data File : BN006287.D
 Acq On : 12 Jun 2019 19:02
 Operator : JU/SJ
 Sample : K3231-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 DB8L5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:34:02 AM

Quant Time: Jun 13 01:22:15 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 12 17:24:11 2019
 Response via : Initial Calibration

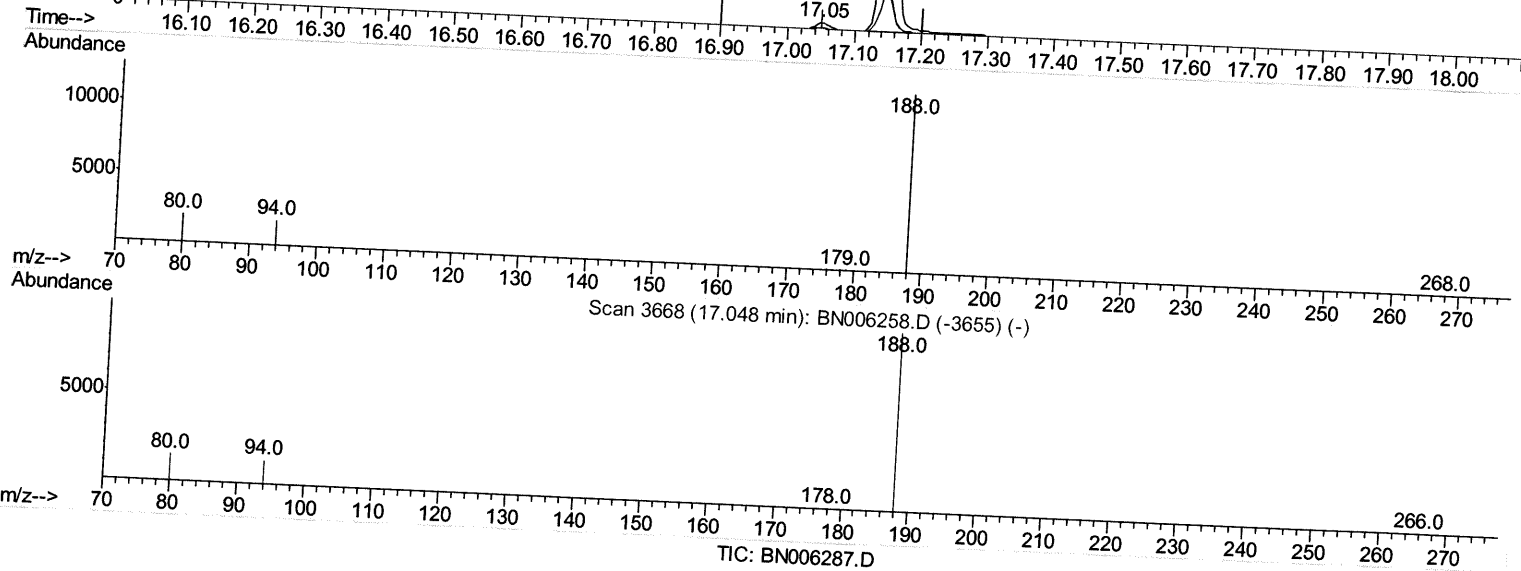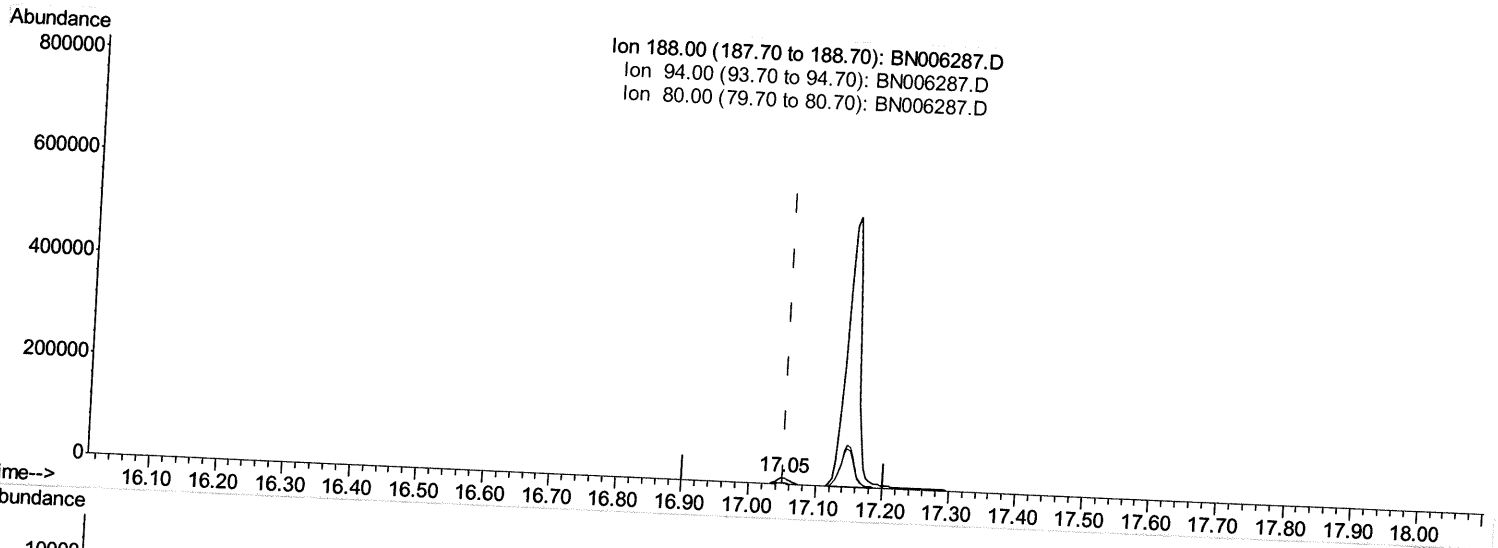

(10) Phenanthrene-d10 (I)

17.048min (-0.005) 0.40ng/ul m

JU 06/13/19

response 18037

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	14.18
80.00	13.60	16.04
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN061219\
 Data File : BN006287.D
 Acq On : 12 Jun 2019 19:02
 Operator : JU/SJ
 Sample : K3231-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 DB8L5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:34:02 AM

Quant Time: Jun 13 02:15:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 12 17:24:11 2019
 Response via : Initial Calibration

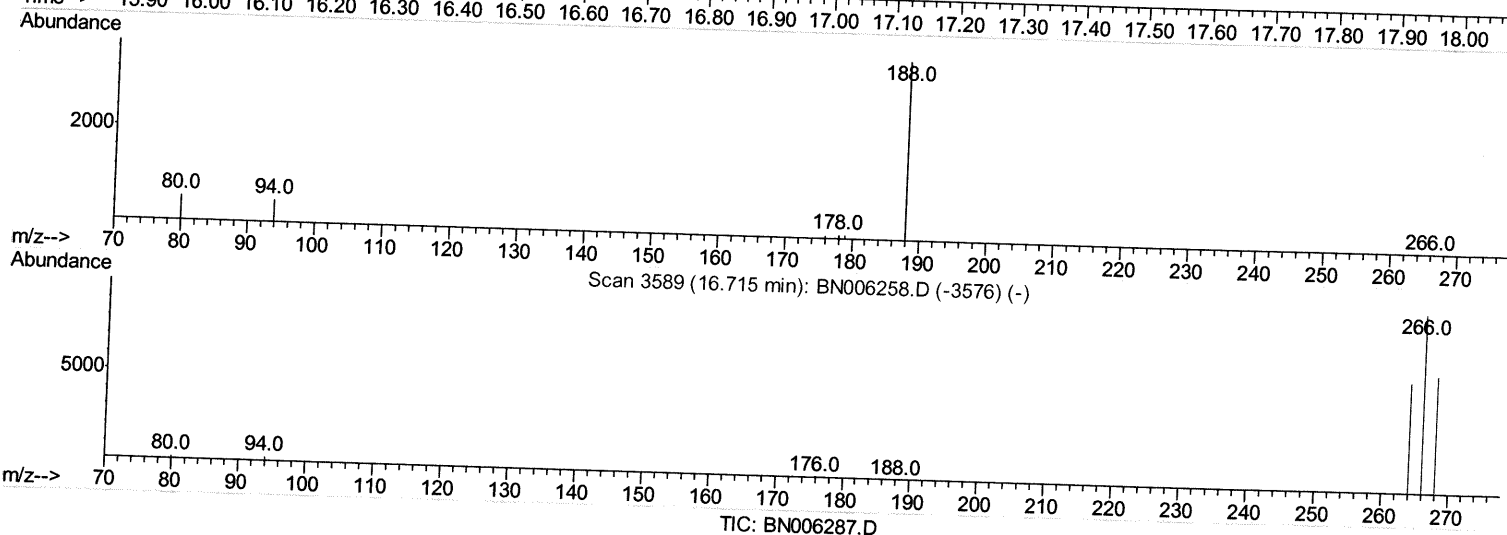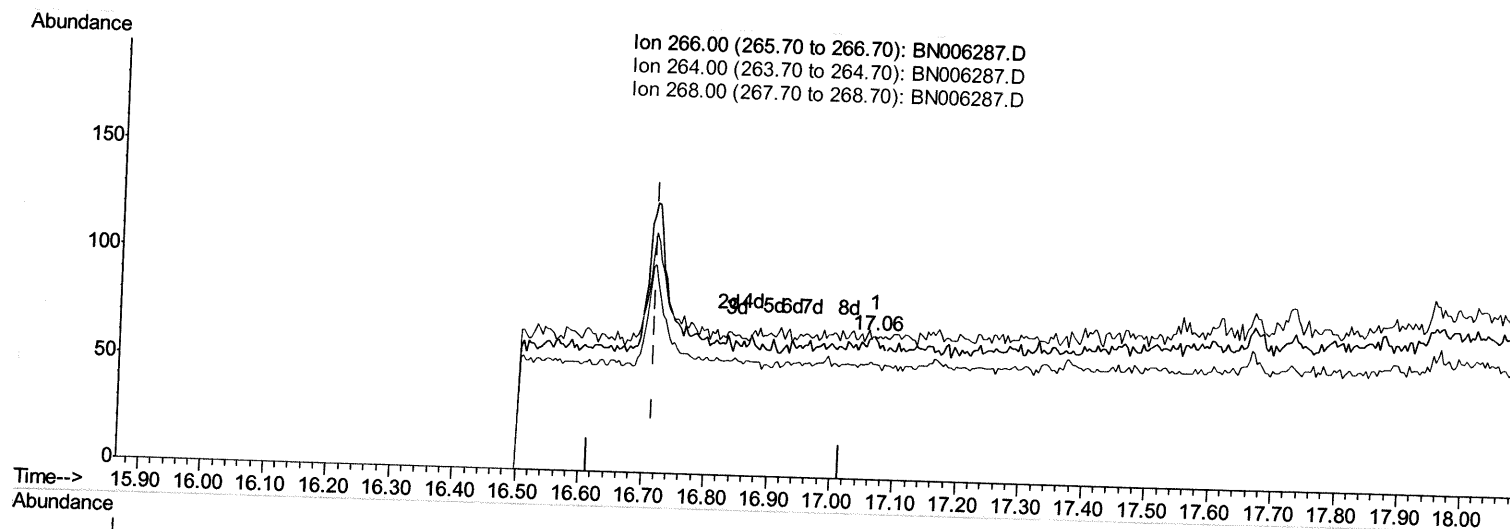

(11) Pentachlorophenol

17.065min (+0.350) 0.00ng/ul

response 9

Ion	Exp%	Act%
266.00	100	100
264.00	62.90	66.67
268.00	64.10	66.67
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN061219\
 Data File : BN006287.D
 Acq On : 12 Jun 2019 19:02
 Operator : JU/SJ
 Sample : K3231-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB8L5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:34:02 AM

Quant Time: Jun 13 02:15:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 12 17:24:11 2019
 Response via : Initial Calibration

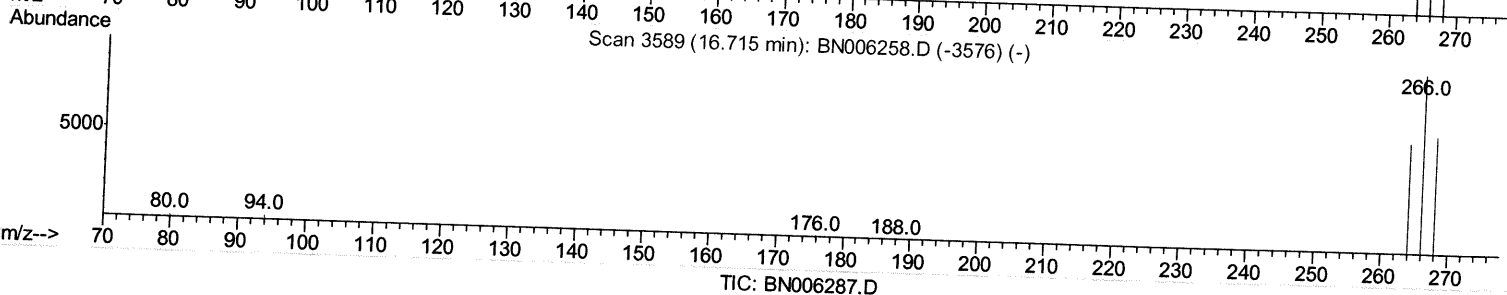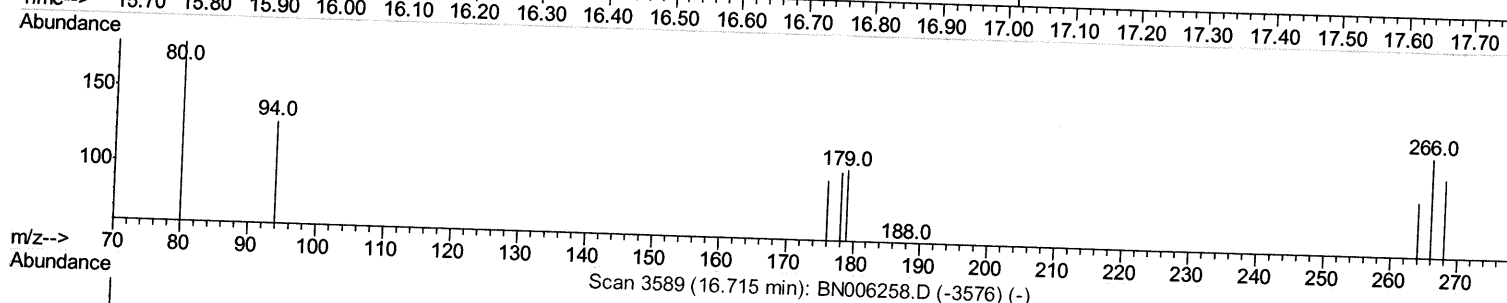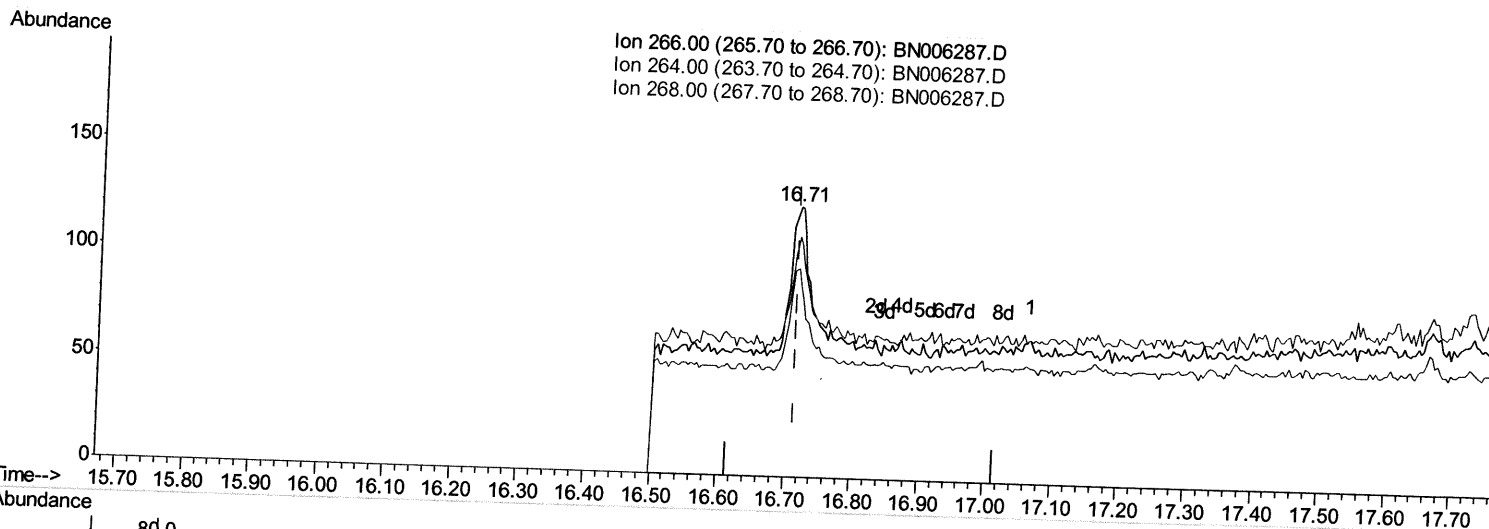

(11) Pentachlorophenol

16.714min (-0.000) 0.03ng/ul m *JU 06/13/19*

response 151

Ion	Exp%	Act%
266.00	100	100
264.00	62.90	3.97#
268.00	64.10	3.97#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN061219\
 Data File : BN006287.D
 Acq On : 12 Jun 2019 19:02
 Operator : JU/SJ
 Sample : K3231-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB8L5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:34:02 AM

Quant Time: Jun 13 02:15:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 12 17:24:11 2019
 Response via : Initial Calibration

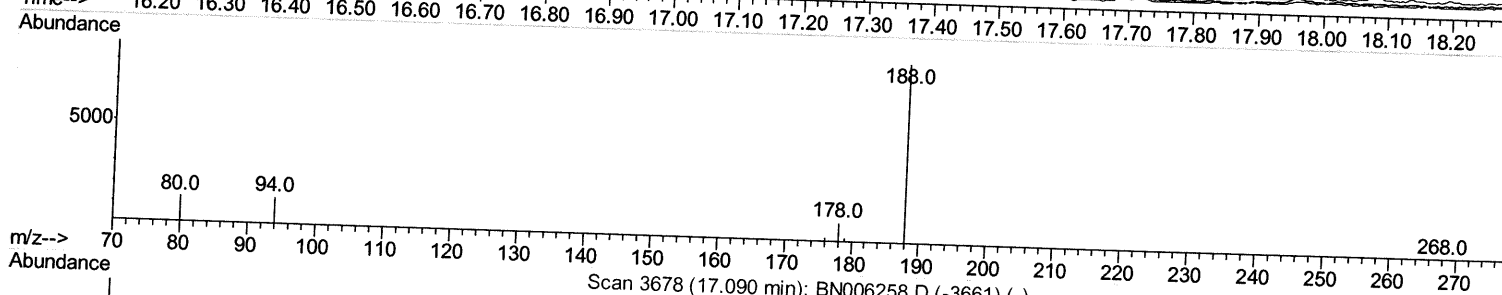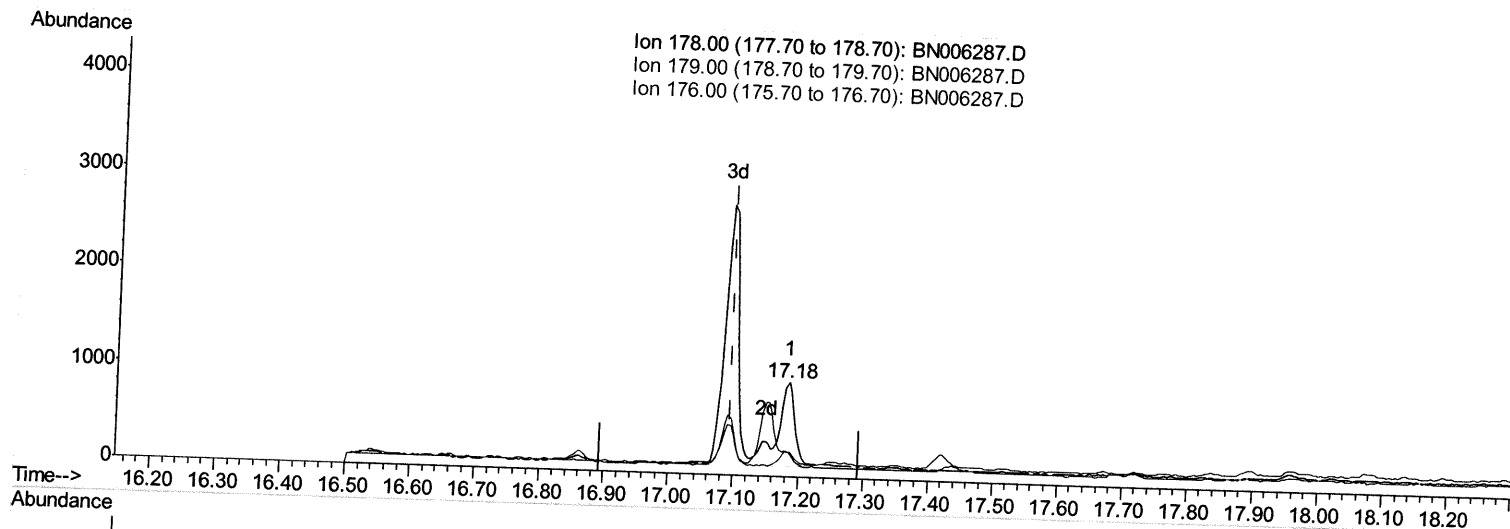

TIC: BN006287.D

(12) Phenanthrene

17.183min (+0.088) 0.02ng/ul

response 1402

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	26.37#
176.00	19.10	26.27#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN061219\
 Data File : BN006287.D
 Acq On : 12 Jun 2019 19:02
 Operator : JU/SJ
 Sample : K3231-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB8L5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:34:02 AM

Quant Time: Jun 13 02:15:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 12 17:24:11 2019
 Response via : Initial Calibration

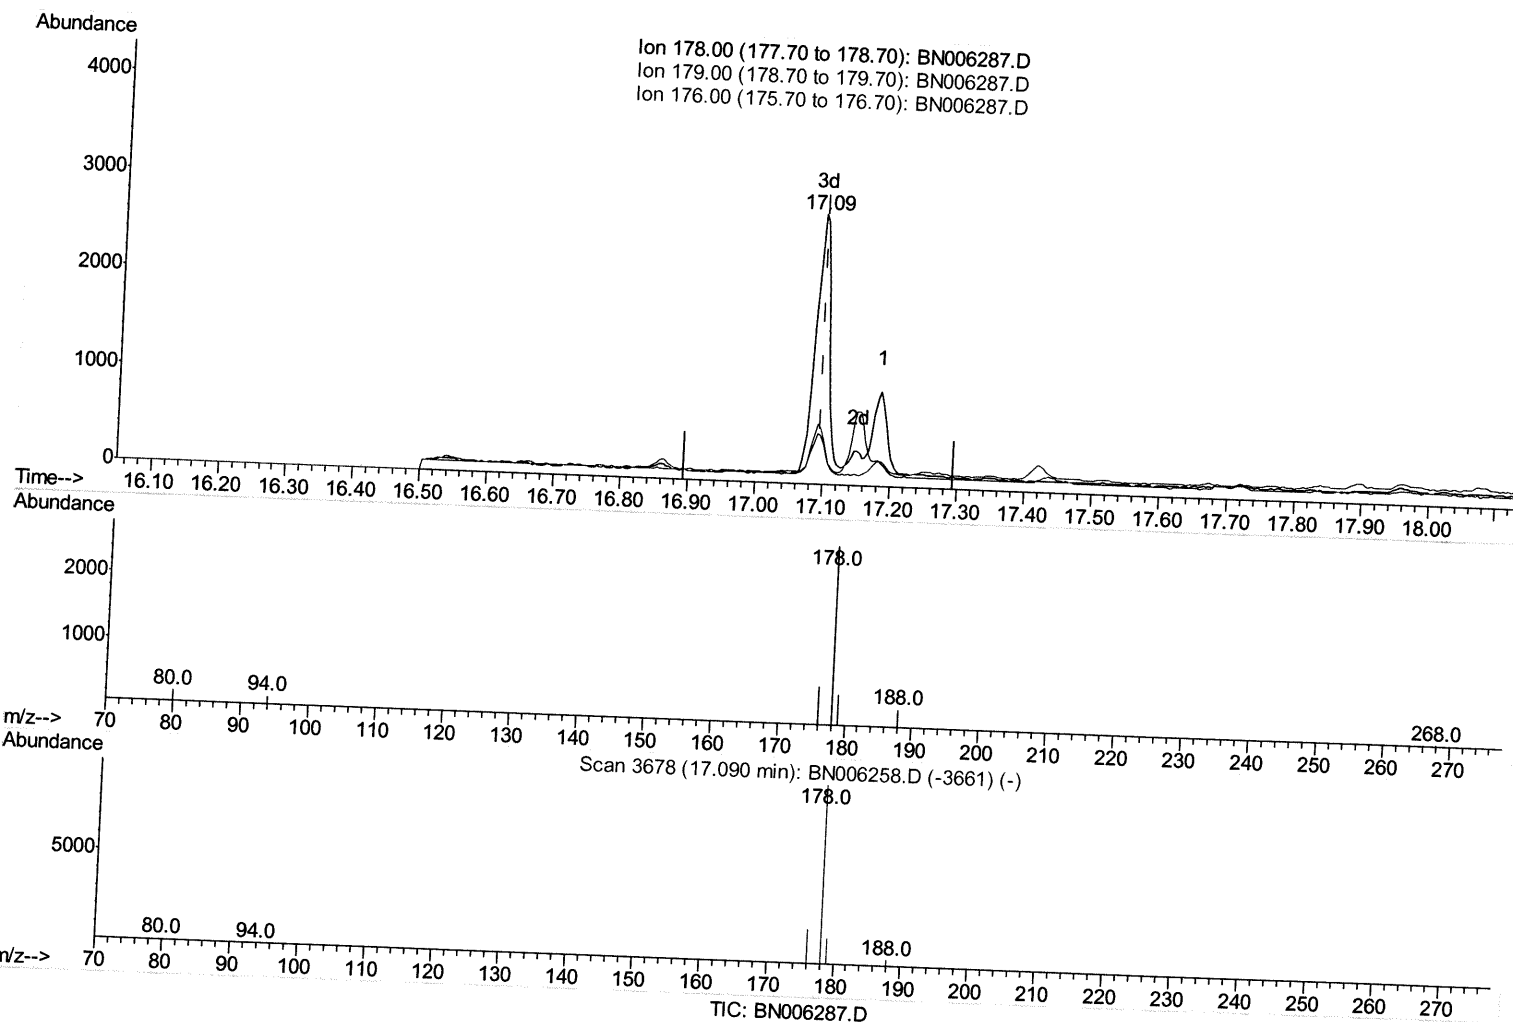

(12) Phenanthrene

17.090min (-0.005) 0.07ng/ul m *JU* *06/13/19*

response 3851

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	18.60#
176.00	19.10	22.43
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN061219\
 Data File : BN006287.D
 Acq On : 12 Jun 2019 19:02
 Operator : JU/SJ
 Sample : K3231-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB8L5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:34:02 AM

Quant Time: Jun 13 02:15:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 12 17:24:11 2019
 Response via : Initial Calibration

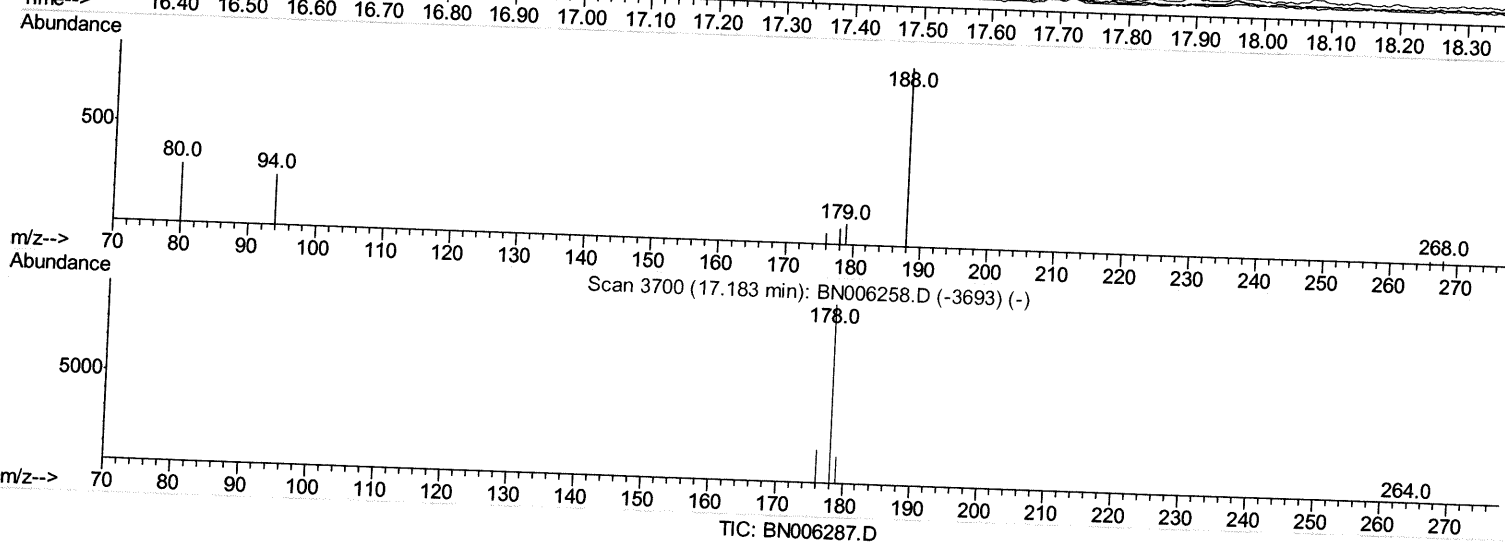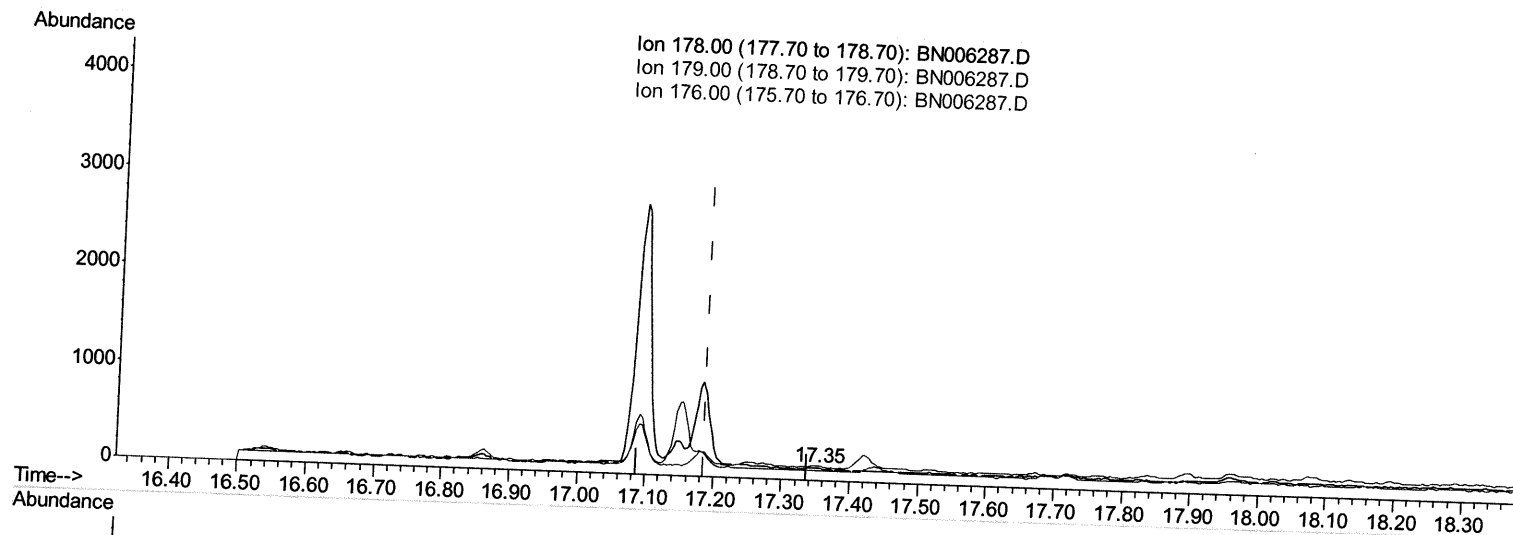

(13) Anthracene

17.352min (+0.164) 0.00ng/ul

response 33

Ion	Exp%	Act%
178.00	100	100
179.00	15.30	115.87#
176.00	18.90	80.16#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN061219\
 Data File : BN006287.D
 Acq On : 12 Jun 2019 19:02
 Operator : JU/SJ
 Sample : K3231-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB8L5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:34:02 AM

Quant Time: Jun 13 02:15:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 12 17:24:11 2019
 Response via : Initial Calibration

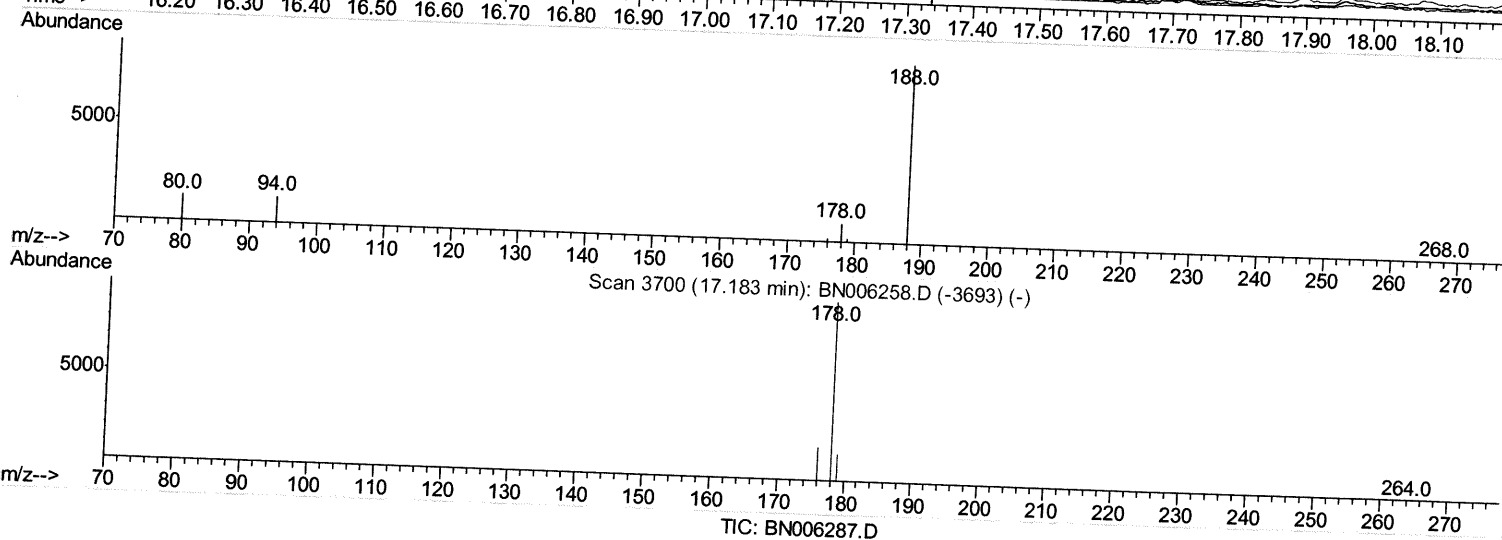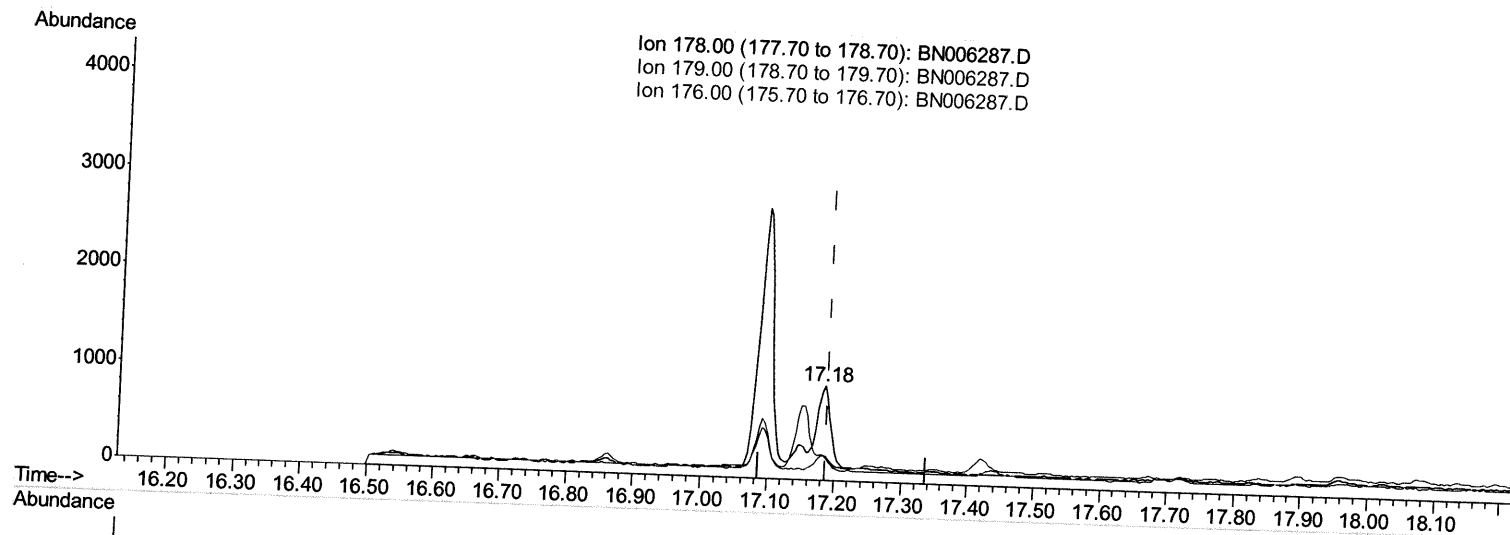

(13) Anthracene

17.183min (-0.005) 0.03ng/ul m *JU 06/13/19*

response 1505

Ion	Exp%	Act%
178.00	100	100
179.00	15.30	26.37#
176.00	18.90	26.27#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN061219\
 Data File : BN006287.D
 Acq On : 12 Jun 2019 19:02
 Operator : JU/SJ
 Sample : K3231-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB8L5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:34:02 AM

Quant Time: Jun 13 02:15:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 12 17:24:11 2019
 Response via : Initial Calibration

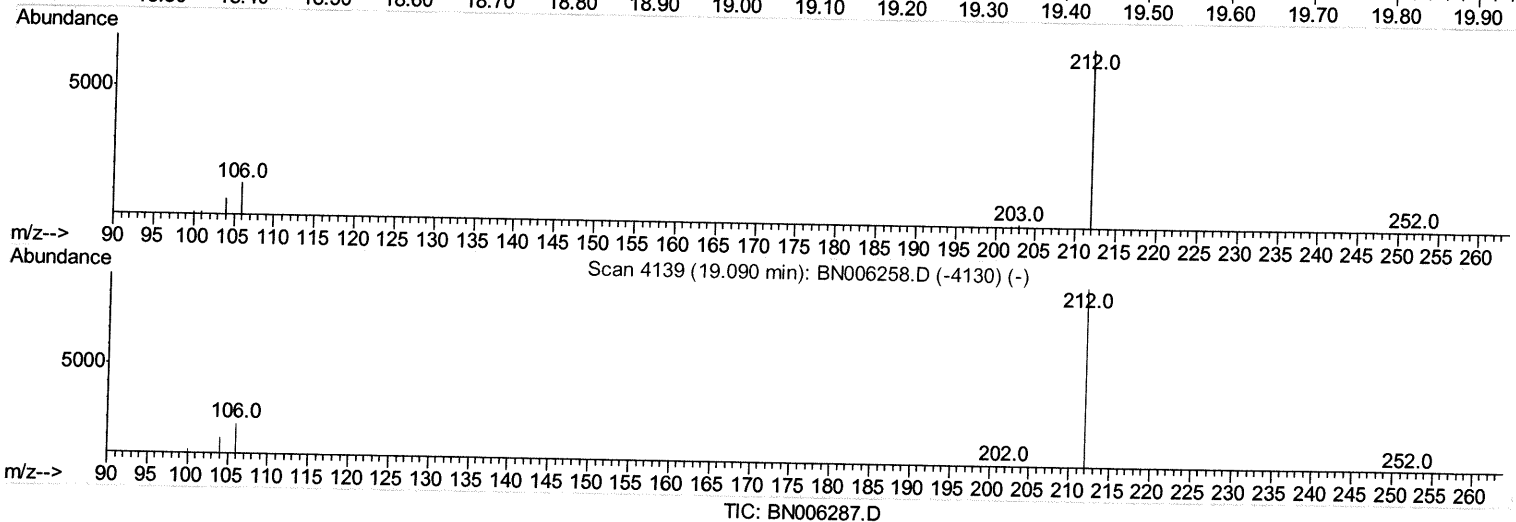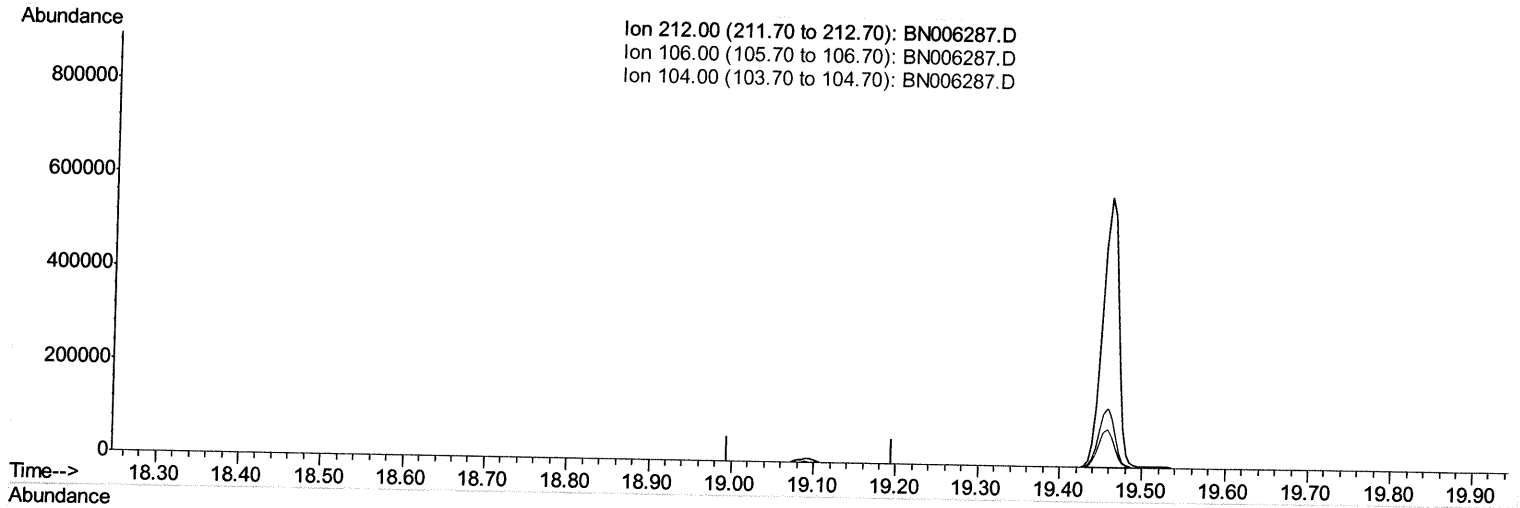

(14) Fluoranthene-d10 (SURR)

19.095min (-19.095) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN061219\
 Data File : BN006287.D
 Acq On : 12 Jun 2019 19:02
 Operator : JU/SJ
 Sample : K3231-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB8L5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:34:02 AM

Quant Time: Jun 13 02:15:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 12 17:24:11 2019
 Response via : Initial Calibration

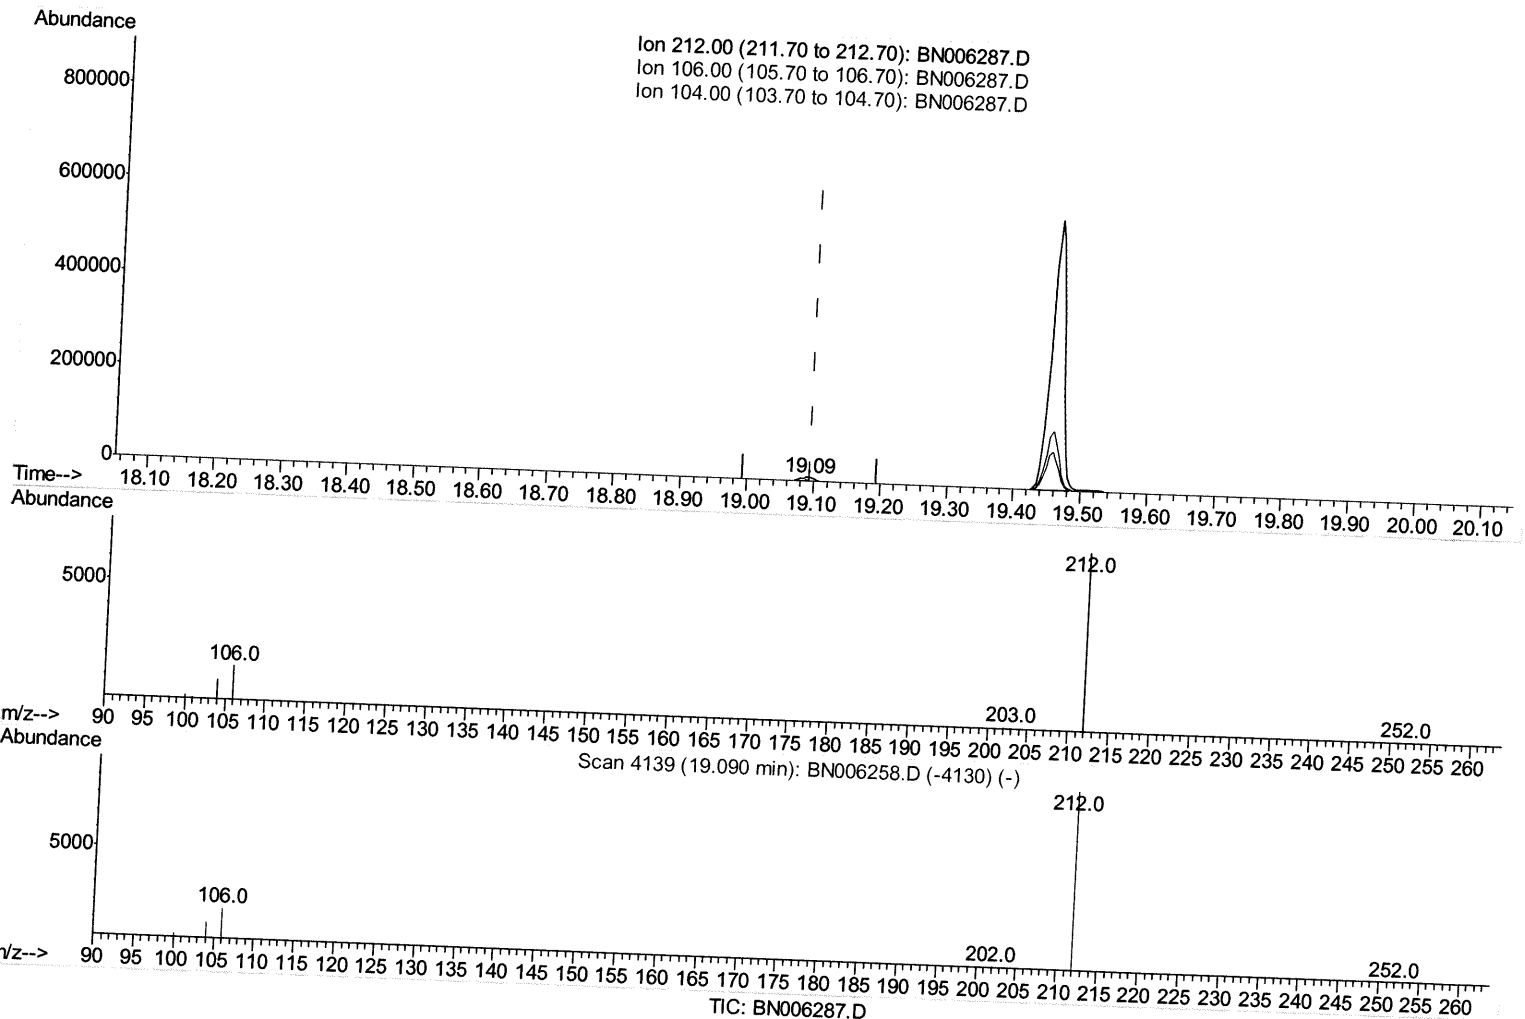

(14) Fluoranthene-d10 (SURR)

19.090min (-0.005) 0.22ng/ul m *JU 06/13/19*

response 10429

Ion	Exp%	Act%
212.00	100	100
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN061219\
 Data File : BN006287.D
 Acq On : 12 Jun 2019 19:02
 Operator : JU/SJ
 Sample : K3231-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB8L5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:34:02 AM

Quant Time: Jun 13 02:15:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 12 17:24:11 2019
 Response via : Initial Calibration

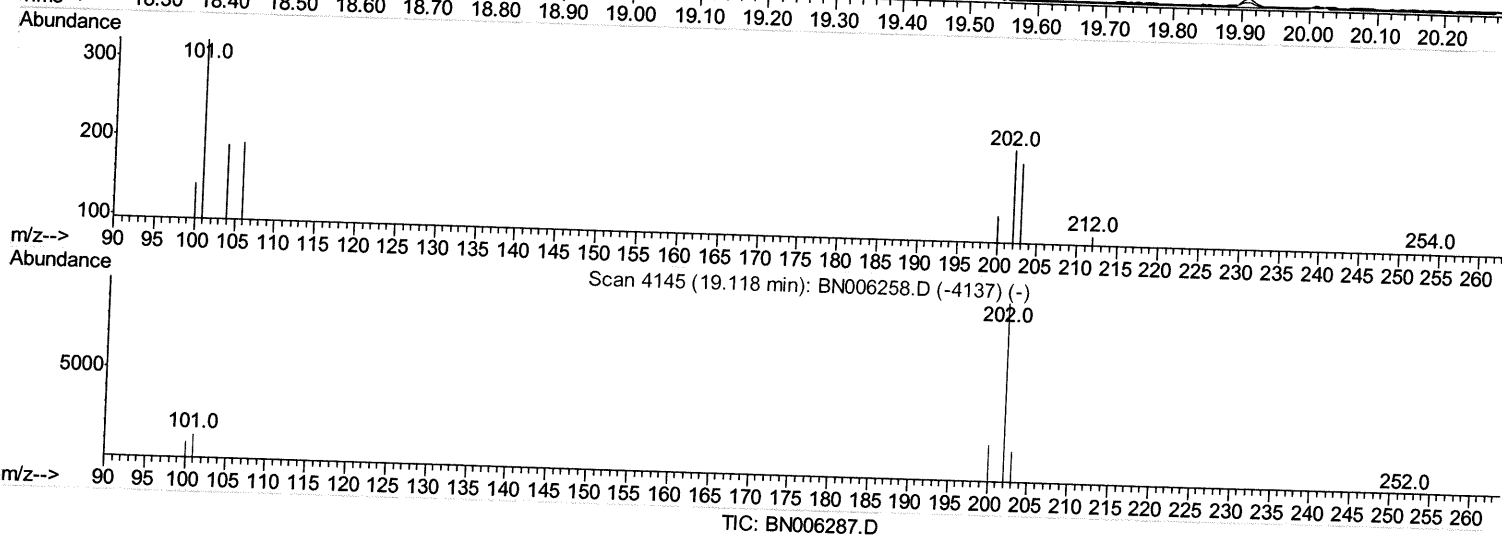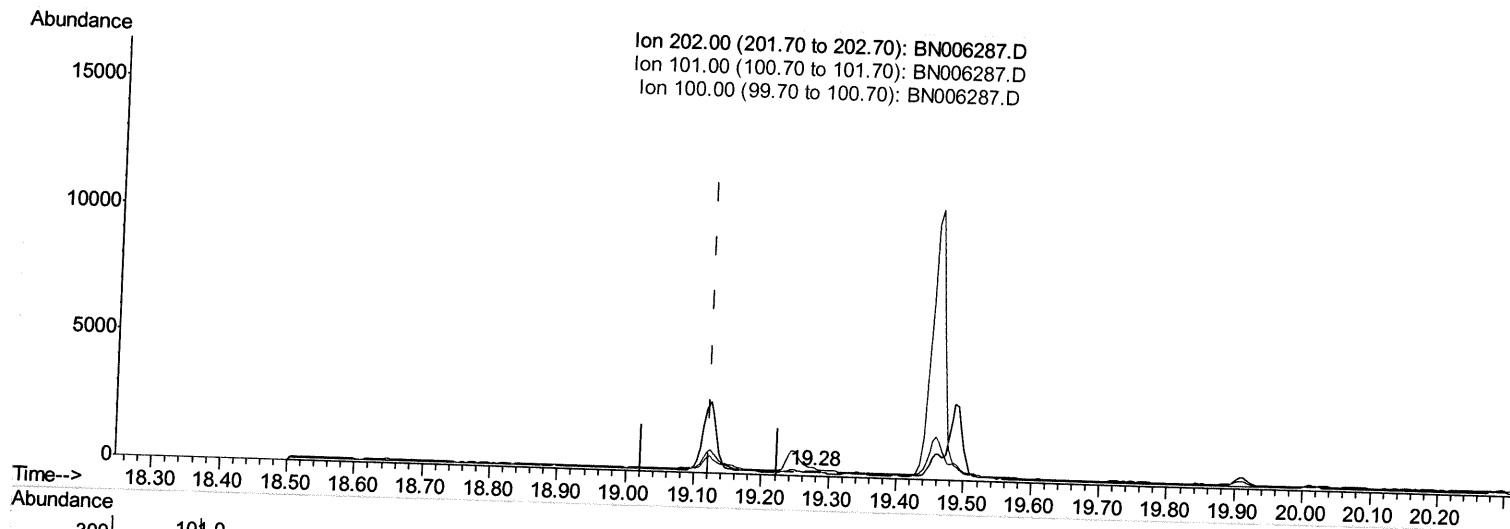

(15) Fluoranthene (C)

19.276min (+0.153) 0.00ng/ul

response 135

Ion	Exp%	Act%
202.00	100	100
101.00	12.10	151.42#
100.00	8.70	66.04#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN061219\
 Data File : BN006287.D
 Acq On : 12 Jun 2019 19:02
 Operator : JU/SJ
 Sample : K3231-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB8L5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:34:02 AM

Quant Time: Jun 13 02:15:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 12 17:24:11 2019
 Response via : Initial Calibration

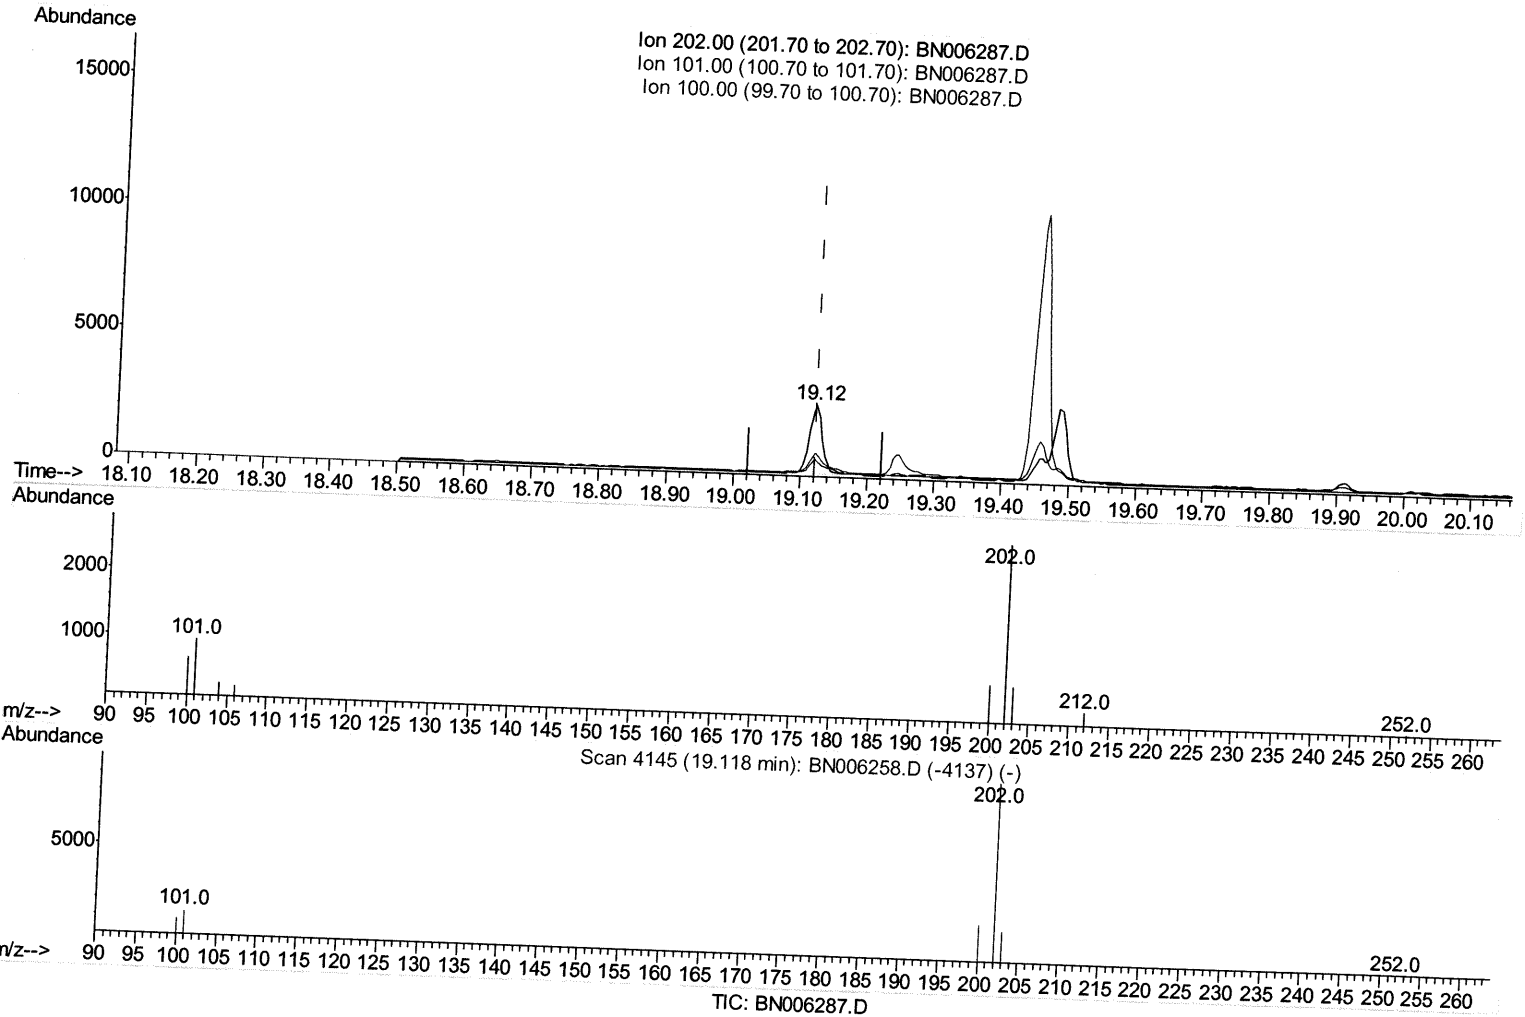

(15) Fluoranthene (C)

19.123min (-0.000) 0.06ng/ul m ^{JU} 06/13/19

response 3644

Ion	Exp%	Act%
202.00	100	100
101.00	12.10	33.35#
100.00	8.70	23.46
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN061219\
 Data File : BN006287.D
 Acq On : 12 Jun 2019 19:02
 Operator : JU/SJ
 Sample : K3231-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 DB8L5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:34:02 AM

Quant Time: Jun 13 02:15:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 12 17:24:11 2019
 Response via : Initial Calibration

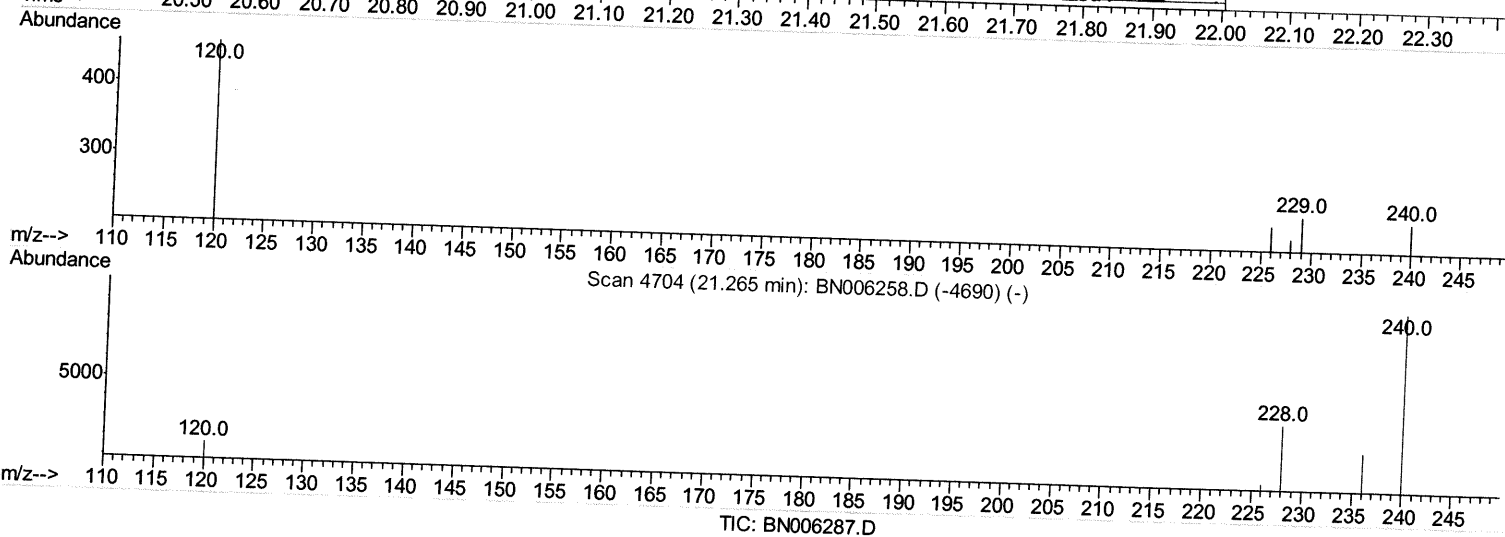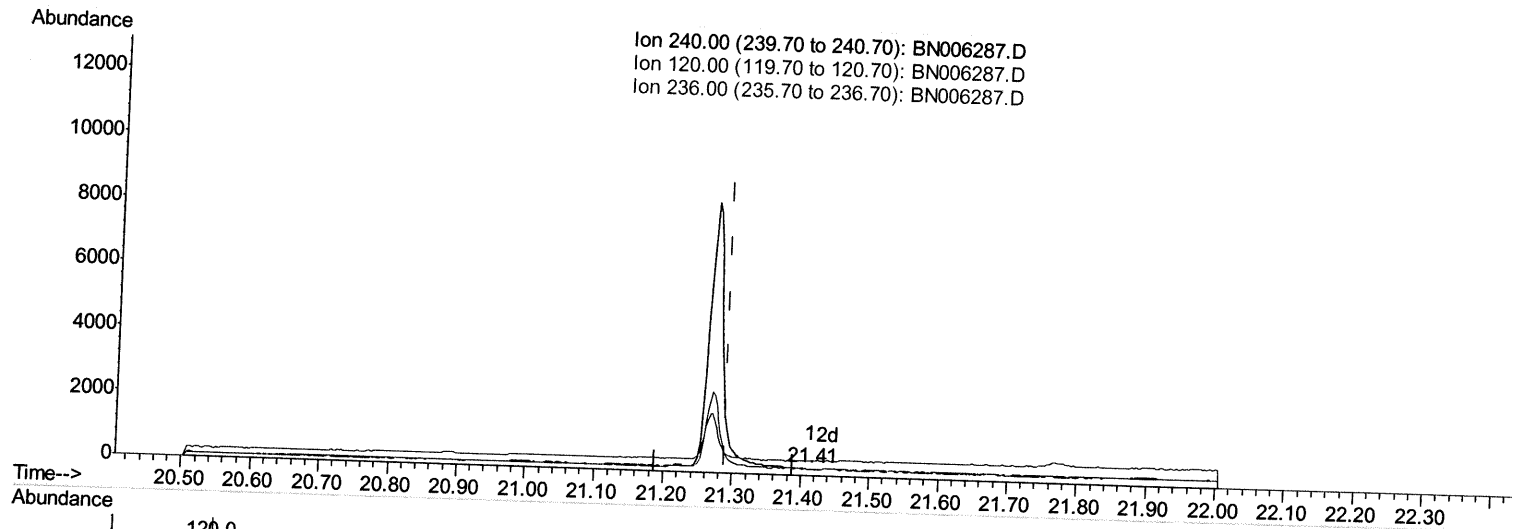

(16) Chrysene-d12 (I)

21.413min (+0.124) 0.40ng/ul

response 20

Ion	Exp%	Act%
240.00	100	100
120.00	20.10	188.16#
236.00	30.10	82.45#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN061219\
 Data File : BN006287.D
 Acq On : 12 Jun 2019 19:02
 Operator : JU/SJ
 Sample : K3231-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB8L5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:34:02 AM

Quant Time: Jun 13 02:15:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 12 17:24:11 2019
 Response via : Initial Calibration

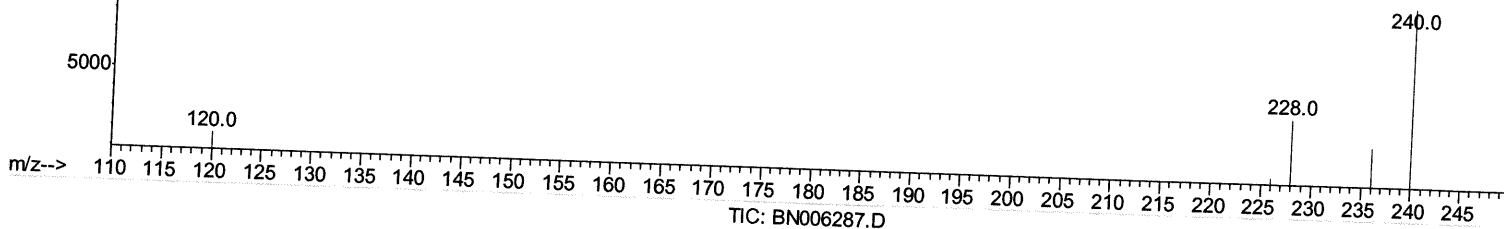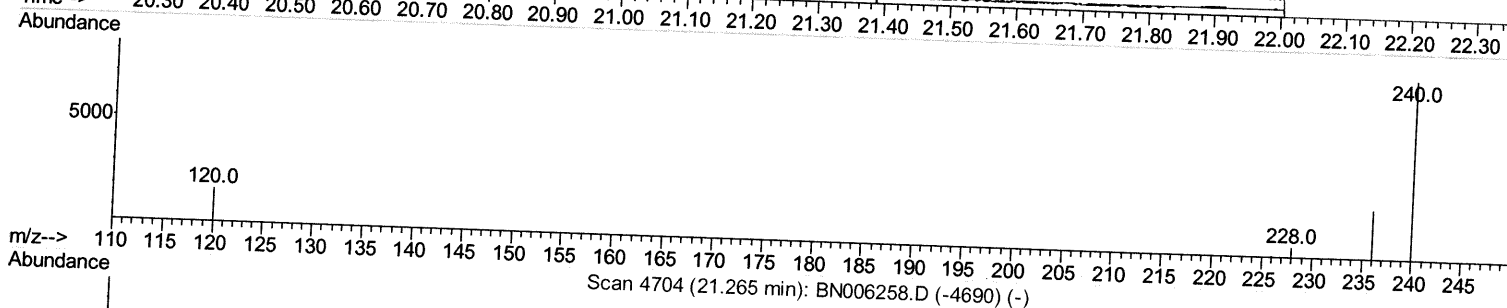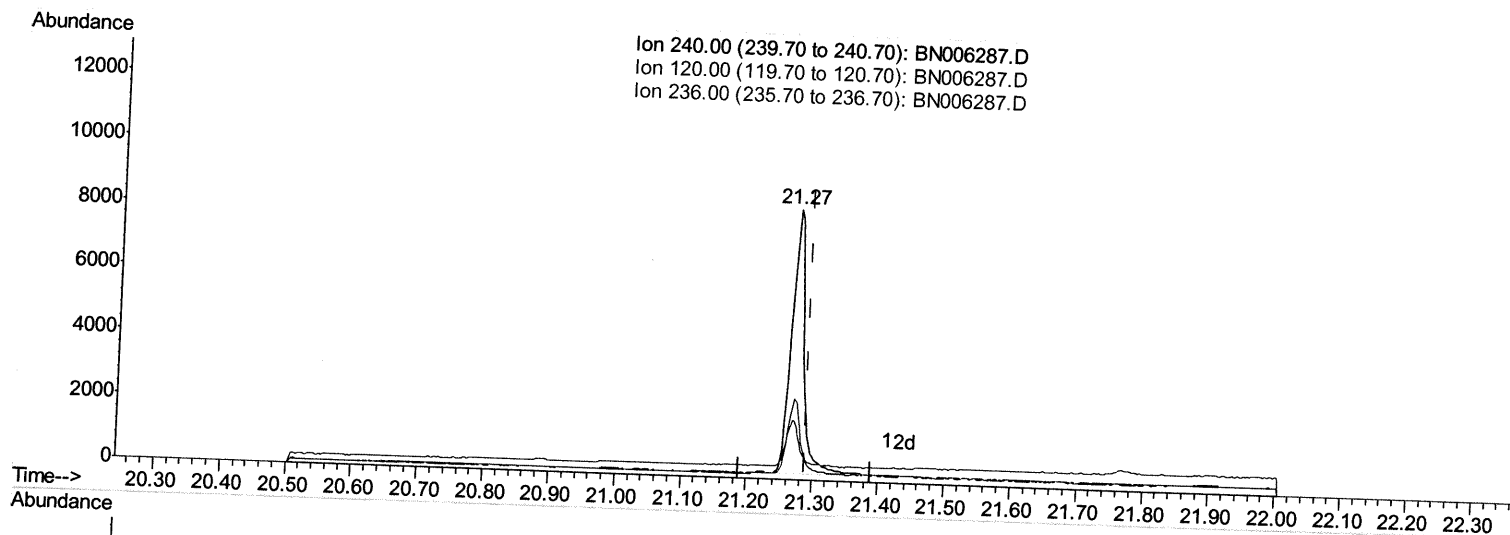

(16) Chrysene-d12 (I)

21.270min (-0.019) 0.40ng/ul m ^{JU} 06/13/19

response 11612

Ion	Exp%	Act%
240.00	100	100
120.00	20.10	21.65
236.00	30.10	30.15
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN061219\
 Data File : BN006287.D
 Acq On : 12 Jun 2019 19:02
 Operator : JU/SJ
 Sample : K3231-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB8L5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:34:02 AM

Quant Time: Jun 13 02:18:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 12 17:24:11 2019
 Response via : Initial Calibration

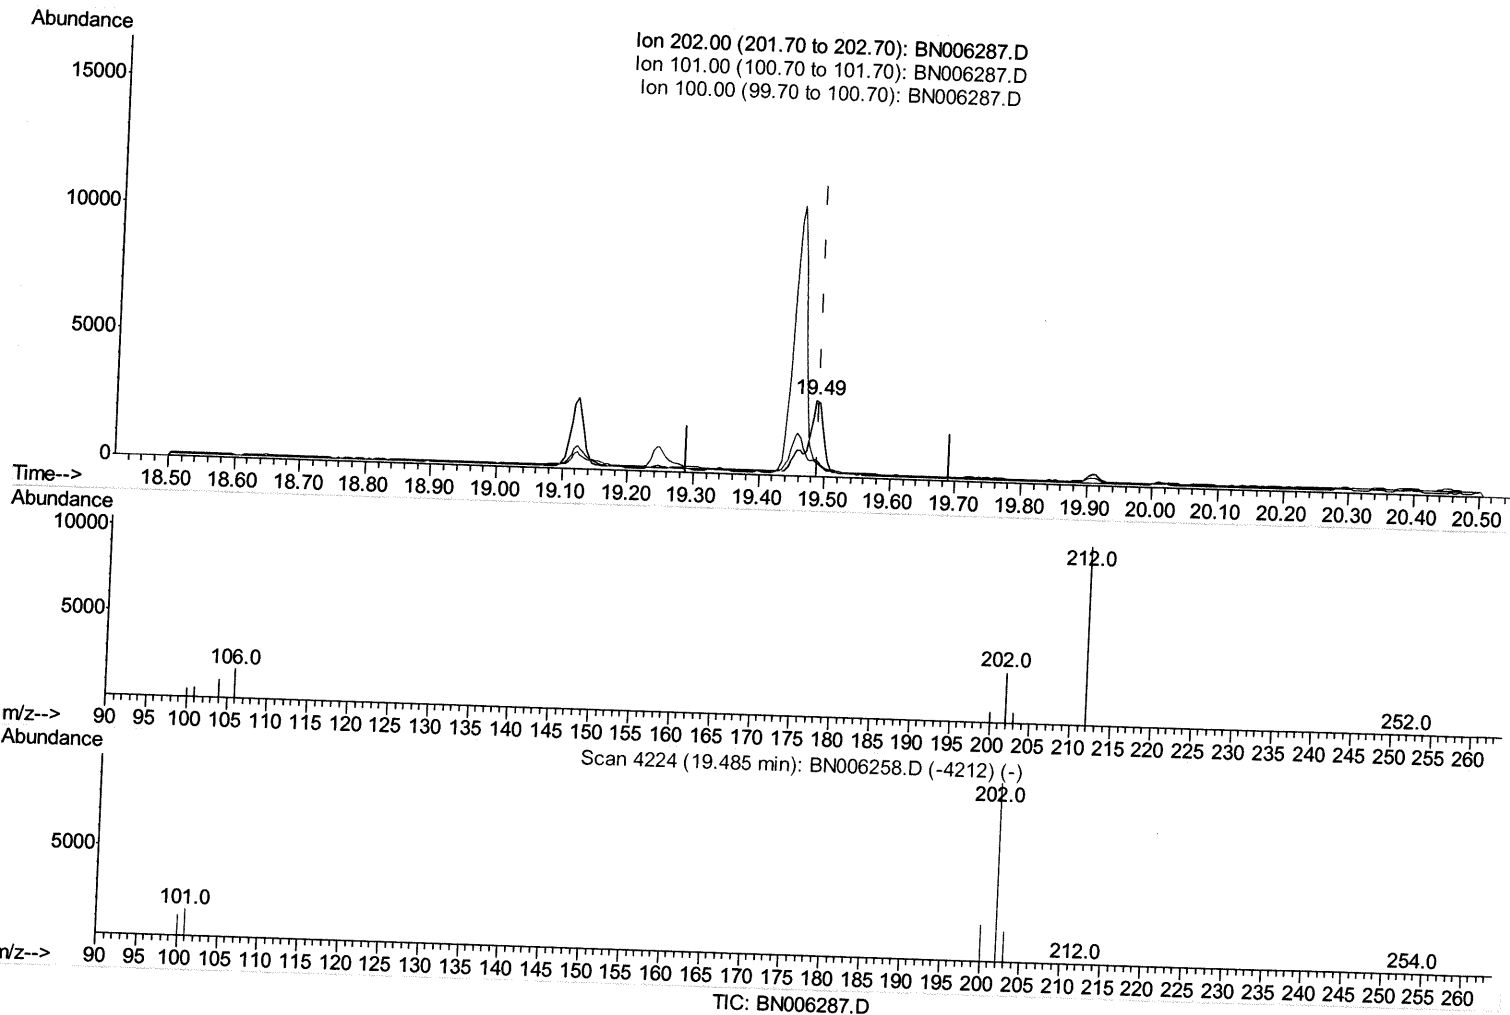

(17) Pyrene

19.485min (-0.005) 0.08ng/ul

response 5031

Ion	Exp%	Act%
202.00	100	100
101.00	15.20	22.33#
100.00	12.20	20.13#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN061219\
 Data File : BN006287.D
 Acq On : 12 Jun 2019 19:02
 Operator : JU/SJ
 Sample : K3231-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB8L5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:34:02 AM

Quant Time: Jun 13 02:18:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 12 17:24:11 2019
 Response via : Initial Calibration

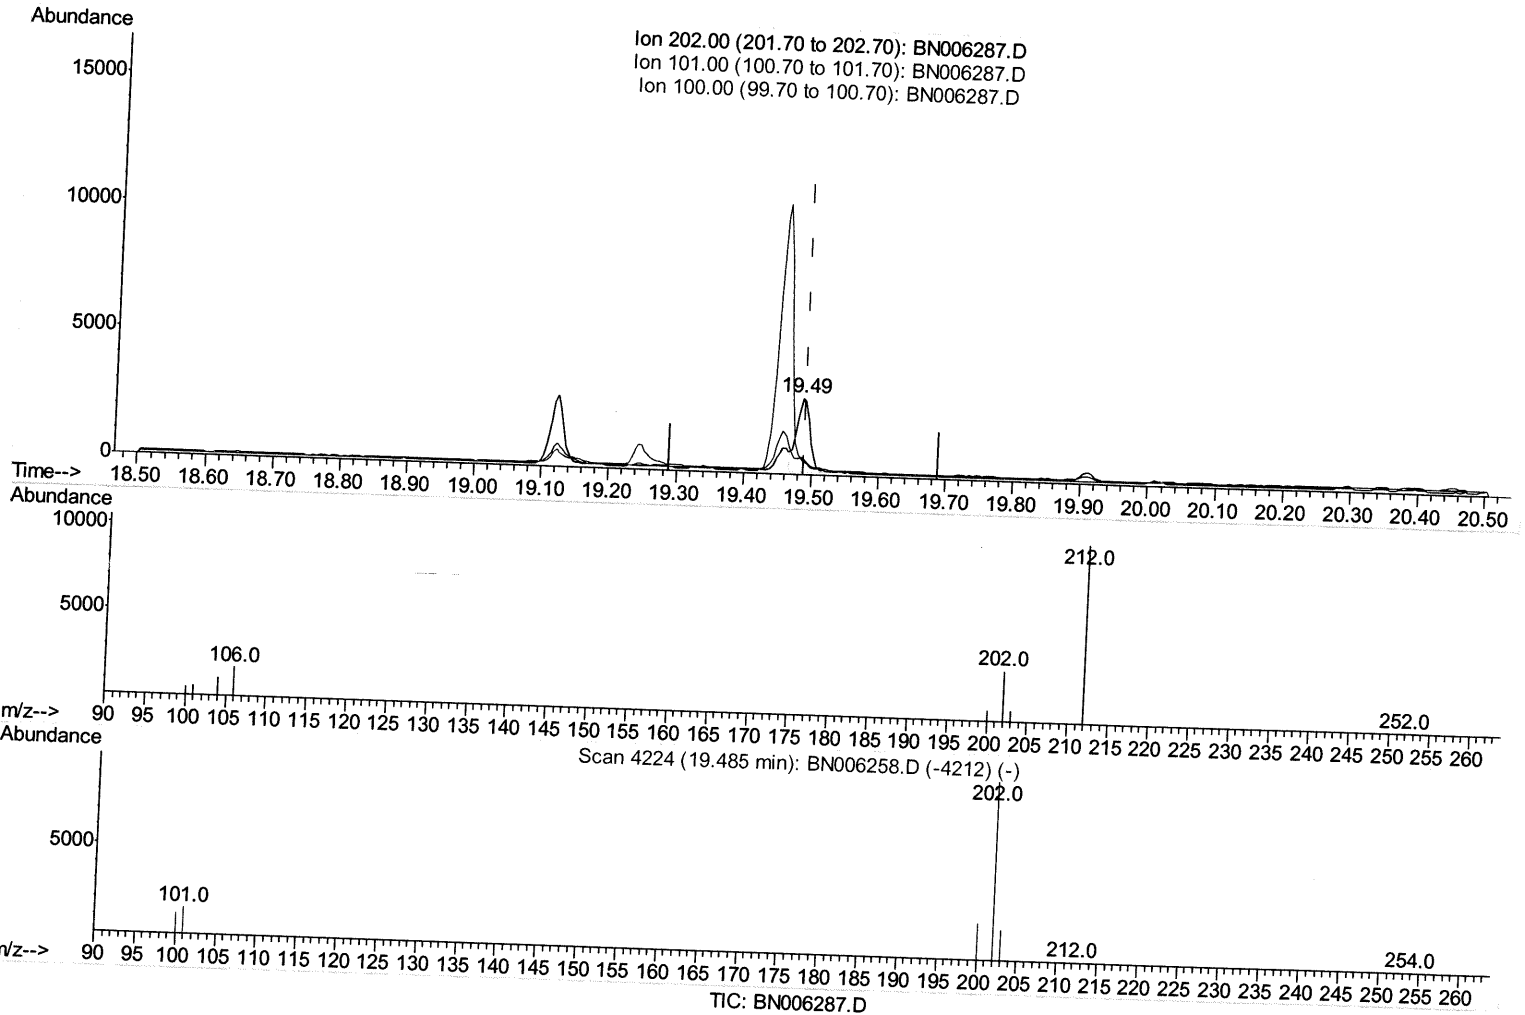

(17) Pyrene

19.485min (-0.005) 0.06ng/ul m *JU* 06/12/19

response 3956

Ion	Exp%	Act%
202.00	100	100
101.00	15.20	22.33#
100.00	12.20	20.13#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN061219\
 Data File : BN006287.D
 Acq On : 12 Jun 2019 19:02
 Operator : JU/SJ
 Sample : K3231-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB8L5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:34:02 AM

Quant Time: Jun 13 02:18:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 12 17:24:11 2019
 Response via : Initial Calibration

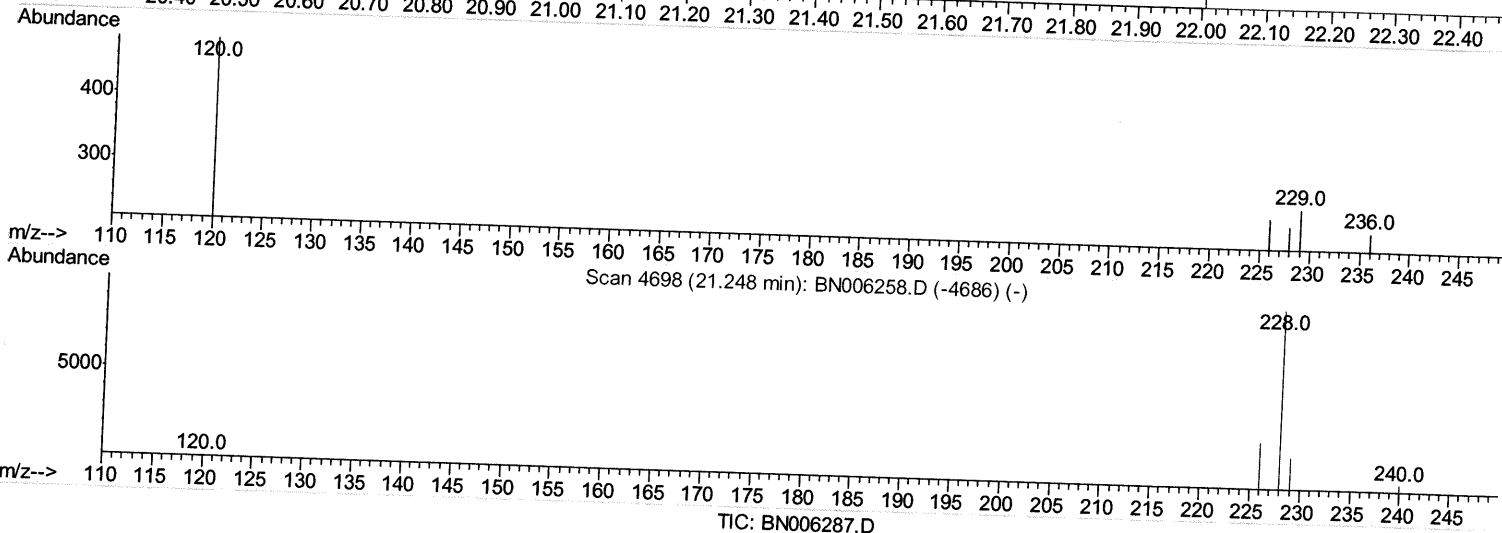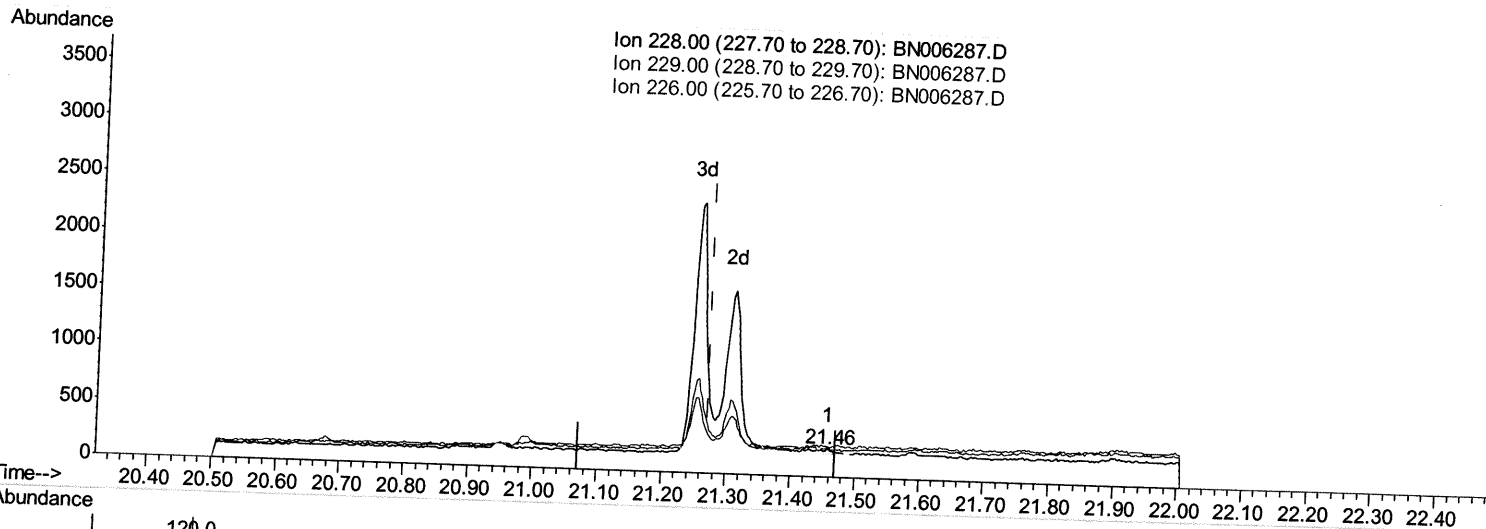

(18) Benzo(a)anthracene

21.457min (+0.185) 0.00ng/ul

response 121

Ion	Exp%	Act%
228.00	100	100
229.00	20.60	111.02#
226.00	28.50	104.90#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN061219\
 Data File : BN006287.D
 Acq On : 12 Jun 2019 19:02
 Operator : JU/SJ
 Sample : K3231-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB8L5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:34:02 AM

Quant Time: Jun 13 02:19:17 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 12 17:24:11 2019
 Response via : Initial Calibration

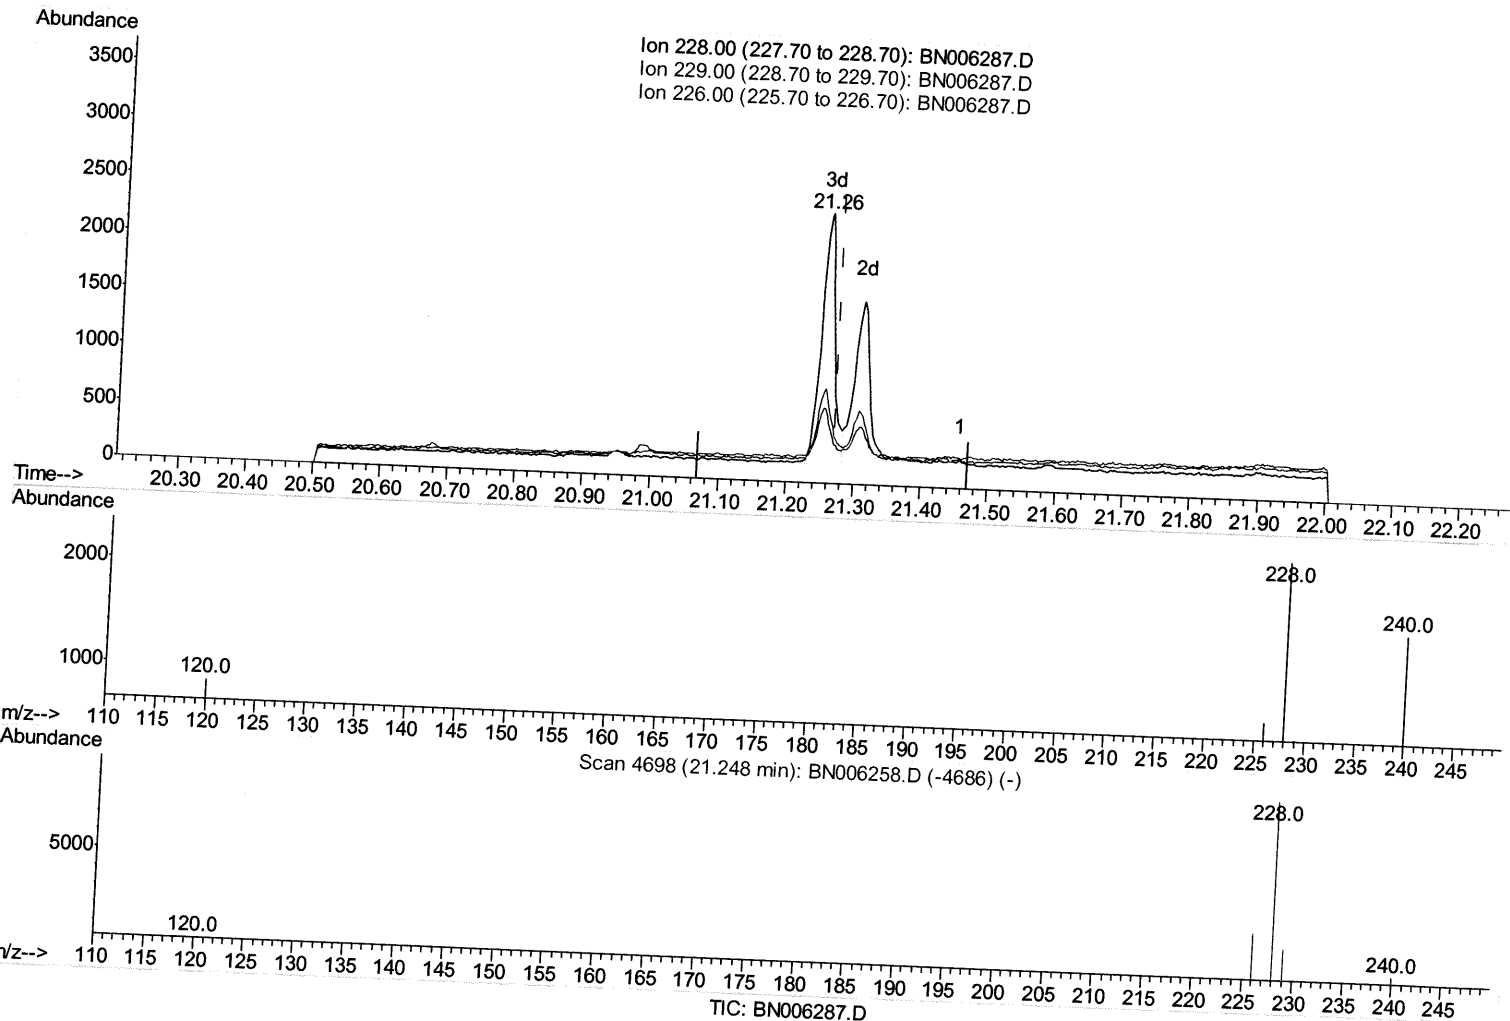

(18) Benzo(a)anthracene

21.255min (-0.016) 0.06ng/ul m *JU* 06/13/19

response 3116

Ion	Exp%	Act%
228.00	100	100
229.00	20.60	27.80#
226.00	28.50	34.79#
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN061219\
 Data File : BN006287.D
 Acq On : 12 Jun 2019 19:02
 Operator : JU/SJ
 Sample : K3231-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleID :
 DB8L5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:34:02 AM

Quant Time: Jun 13 02:20:15 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 12 17:24:11 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	4962	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	19400	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	9788	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	18037m >	0.40	ng/ul	0.00
16) Chrysene-d12	21.27	240	11612m >	0.40	ng/ul	-0.02
20) Perylene-d12	23.51	264	16456	0.40	ng/ul	-0.04
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	4919	0.17	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	10429m >	0.22	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.47	128	1285	0.024	ng/ul#	78
5) 2-Methylnaphthalene	12.10	142	775	0.021	ng/ul	99
7) Acenaphthylene	14.01	152	3293	0.061	ng/ul#	93
9) Fluorene	15.35	166	1247	0.028	ng/ul#	94
11) Pentachlorophenol	16.71	266	151m >	0.033	ng/ul	
12) Phenanthrene	17.09	178	3851m >	0.067	ng/ul	
13) Anthracene	17.18	178	1505m >	0.027	ng/ul	
15) Fluoranthene	19.12	202	3644m >	0.057	ng/ul	
17) Pyrene	19.49	202	3956m >	0.065	ng/ul	
18) Benzo(a)anthracene	21.26	228	3116m >	0.061	ng/ul	
19) Chrysene	21.31	228	2209	0.046	ng/ul#	82
21) Benzo(b)fluoranthene	22.84	252	2365	0.034	ng/ul#	1
22) Benzo(k)fluoranthene	22.88	252	2543	0.038	ng/ul#	1
23) Benzo(a)pyrene	23.36	252	2935	0.046	ng/ul#	15
24) Indeno(1,2,3-cd)pyrene	25.74	276	2426	0.035	ng/ul#	99
25) Dibenzo(a,h)anthracene	25.75	278	1627	0.029	ng/ul#	19
26) Benzo(a,h,i)perylene	26.43	276	2833	0.049	ng/ul#	68

JU 06/13/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed