

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061219\
 Data File : BN006294.D
 Acq On : 12 Jun 2019 23:05
 Operator : JU/SJ
 Sample : K3231-15
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB8M2

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:34:24 AM

Quant Time: Jun 13 03:46:33 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 12 17:24:11 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	5261	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	20096	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	10218	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	18743m	0.40	ng/ul	0.00
16) Chrysene-d12	21.27	240	13195m	0.40	ng/ul	-0.02
20) Perylene-d12	23.50	264	19003	0.40	ng/ul	-0.05
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	4534	0.15	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	7857m	0.16	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	16.71	266	24327m	5.108	ng/ul	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061219\
Data File : BN006294.D
Acq On : 12 Jun 2019 23:05
Operator : JU/SJ
Sample : K3231-15
Misc :
ALS Vial : 22 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
DB8M2

Manual Integrations
APPROVED

mohammad
6/14/2019 8:34:24 AM

Quant Time: Jun 13 03:46:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 12 17:24:11 2019
Response via : Initial Calibration

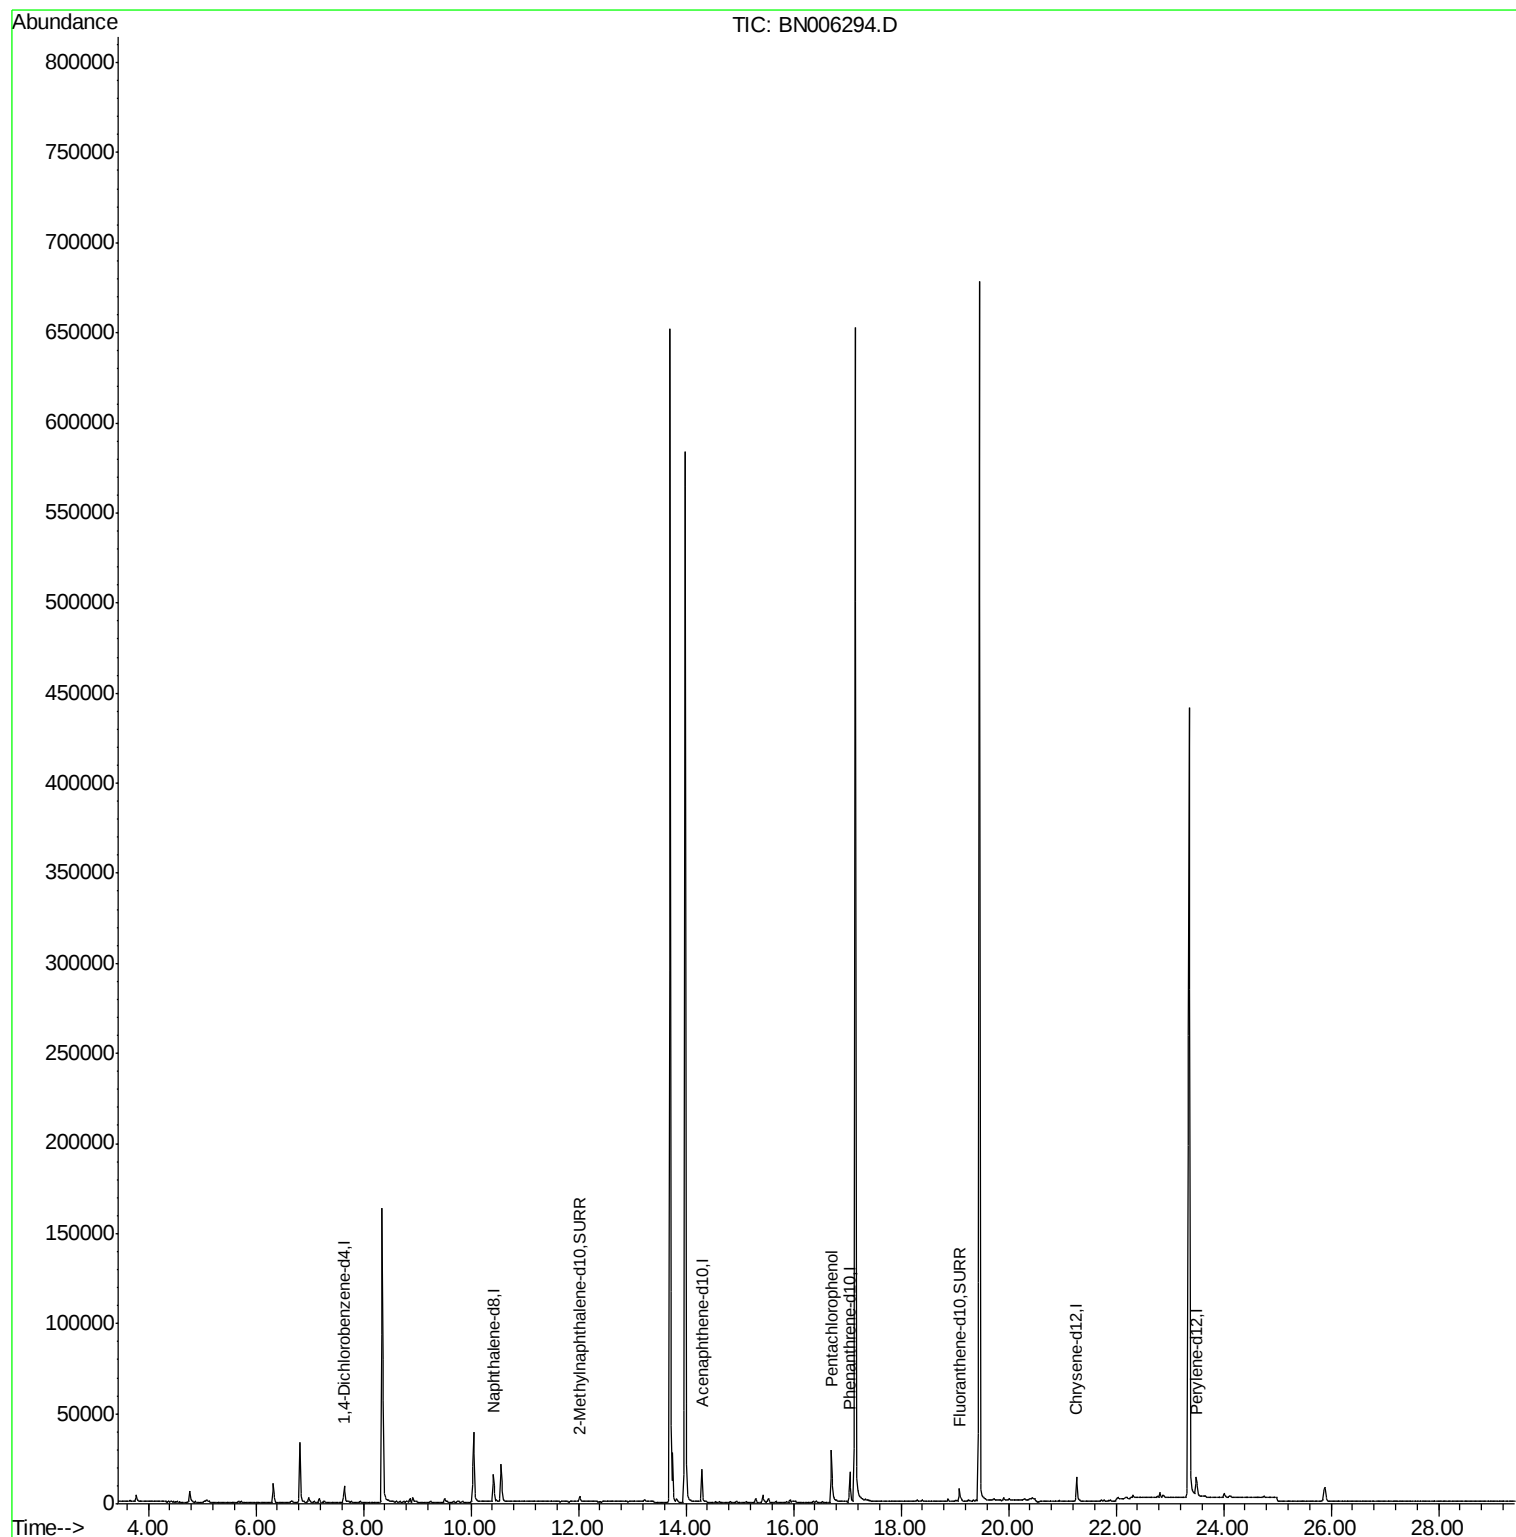

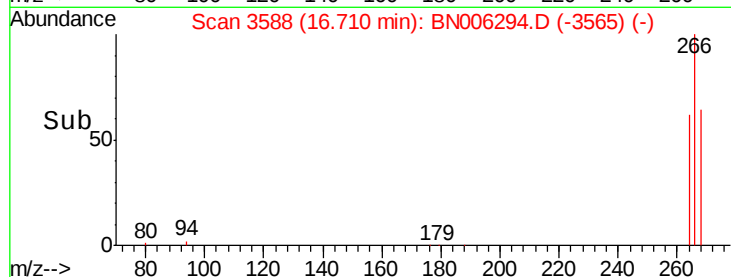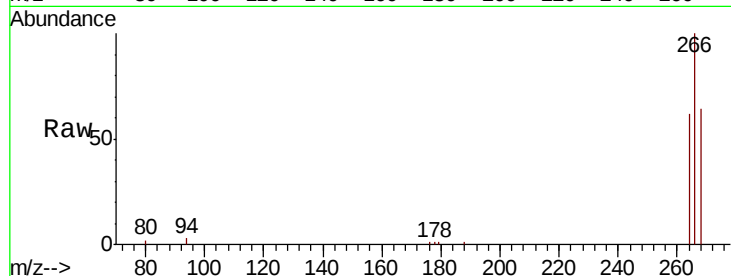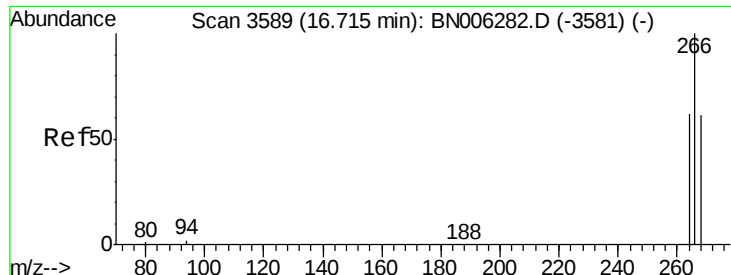

#11

Pentachlorophenol

Concen: 5.108 ng/ul m

RT: 16.71 min Scan# 3588

Delta R.T. -0.00 min

Lab File: BN006294.D

Acq: 12 Jun 2019 23:05

Instrument :

BNA_N

ClientSampleId :

DB8M2

Tot Ion: 266 Resp: 24327

Ion Ratio Lower Upper

266 100

264 0.0 50.3 75.5#

268 0.0 51.3 76.9#

Manual Integrations
APPROVED

mohammad
6/14/2019 8:34:24 AM

