

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061221\
 Data File : BN014894.D
 Acq On : 12 Jun 2021 15:23
 Operator : CG/JU
 Sample : M2620-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN014894.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.617	88	90	93	rBV3	9255	12645	0.52%	0.134%
2	3.728	107	109	112	rBV3	8272	6837	0.28%	0.072%
3	4.064	164	166	167	rBV	6359	5120	0.21%	0.054%
4	4.205	188	190	193	rBV4	5540	8140	0.33%	0.086%
5	4.899	306	308	311	rBV3	5893	6352	0.26%	0.067%
6	5.034	329	331	332	rBV2	4505	3611	0.15%	0.038%
7	5.317	378	379	381	rBV	6173	5494	0.23%	0.058%
8	5.499	408	410	411	rBV2	6671	4501	0.18%	0.048%
9	5.546	417	418	421	rBV3	6138	4213	0.17%	0.045%
10	5.811	461	463	464	rBV2	4001	3718	0.15%	0.039%
11	5.864	469	472	473	rBV2	6785	6338	0.26%	0.067%
12	6.028	498	500	503	rVB2	6705	4845	0.20%	0.051%
13	6.064	503	506	508	rBV2	7416	6136	0.25%	0.065%
14	6.122	513	516	518	rBV4	4119	5289	0.22%	0.056%
15	6.287	543	544	549	rBV3	4223	6244	0.26%	0.066%
16	6.381	558	560	563	rBV3	6256	7139	0.29%	0.076%
17	6.575	591	593	596	rBV2	3434	4523	0.19%	0.048%
18	6.764	621	625	628	rVB6	3858	5004	0.21%	0.053%
19	7.105	680	683	684	rBV2	5983	5499	0.23%	0.058%
20	7.687	776	782	790	rBV	381461	622393	25.56%	6.587%
21	7.740	790	791	795	rVB3	9018	5937	0.24%	0.063%
22	8.164	862	863	866	rVB2	4566	3700	0.15%	0.039%
23	8.446	909	911	914	rBV4	3265	3792	0.16%	0.040%
24	8.534	923	926	929	rBV4	4106	4750	0.20%	0.050%
25	8.564	929	931	934	rVB2	5046	5087	0.21%	0.054%
26	8.593	934	936	937	rBV	4236	3860	0.16%	0.041%
27	8.781	966	968	971	rBV3	3930	5613	0.23%	0.059%
28	8.875	983	984	987	rVB3	4890	3833	0.16%	0.041%
29	8.922	987	992	997	rBV4	4556	7028	0.29%	0.074%
30	9.011	1005	1007	1009	rBV2	4218	4110	0.17%	0.043%
31	9.069	1015	1017	1019	rVB2	5974	3615	0.15%	0.038%
32	9.093	1019	1021	1025	rBV2	4000	6269	0.26%	0.066%
33	9.363	1064	1067	1068	rBV3	5259	4752	0.20%	0.050%
34	9.381	1068	1070	1074	rVB3	5251	3828	0.16%	0.041%
35	9.528	1094	1095	1099	rVV	3236	3692	0.15%	0.039%
36	10.316	1225	1229	1230	rBV2	3154	3706	0.15%	0.039%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061221\
 Data File : BN014894.D
 Acq On : 12 Jun 2021 15:23
 Operator : CG/JU
 Sample : M2620-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
 Title : SVOA CALIBRATION

37	10.475	1249	1256	1266	rBV	458070	803321	32.99%	8.502%
38	10.628	1281	1282	1286	rVB3	5095	4799	0.20%	0.051%
39	10.675	1286	1290	1292	rBV2	3987	6283	0.26%	0.066%
40	11.093	1356	1361	1362	rBV3	3298	4553	0.19%	0.048%

41	11.169	1372	1374	1377	rVB3	4920	6136	0.25%	0.065%
42	11.205	1377	1380	1382	rBV3	4402	5386	0.22%	0.057%
43	11.505	1423	1431	1433	rBV5	2703	5267	0.22%	0.056%
44	11.528	1433	1435	1437	rVV3	3623	3806	0.16%	0.040%
45	11.699	1460	1464	1466	rVB2	3816	5143	0.21%	0.054%

46	11.722	1466	1468	1471	rBV3	3789	3986	0.16%	0.042%
47	12.181	1543	1546	1549	rBV	4343	3800	0.16%	0.040%
48	12.293	1559	1565	1567	rVB4	3452	5498	0.23%	0.058%
49	12.334	1567	1572	1575	rBV3	3948	6086	0.25%	0.064%
50	12.422	1585	1587	1590	rVB4	4349	4096	0.17%	0.043%

51	12.469	1590	1595	1599	rBV4	3259	6793	0.28%	0.072%
52	12.534	1603	1606	1609	rBV3	6293	7240	0.30%	0.077%
53	12.587	1611	1615	1620	rVV4	5349	8286	0.34%	0.088%
54	12.704	1630	1635	1636	rBV4	6123	6645	0.27%	0.070%
55	13.340	1741	1743	1746	rVB	3716	3639	0.15%	0.039%

56	13.381	1746	1750	1751	rBV2	2899	3562	0.15%	0.038%
57	13.440	1758	1760	1765	rVB3	3171	4010	0.16%	0.042%
58	13.675	1799	1800	1803	rVB	5049	3610	0.15%	0.038%
59	13.834	1824	1827	1828	rBV	4981	3721	0.15%	0.039%
60	14.087	1867	1870	1872	rBV3	3551	3778	0.16%	0.040%

61	14.257	1896	1899	1900	rBV2	5242	5971	0.25%	0.063%
62	14.340	1907	1913	1927	rBV	780517	1210449	49.70%	12.811%
63	14.551	1945	1949	1954	rVB2	4493	5701	0.23%	0.060%
64	14.804	1990	1992	1994	rBV	4011	3721	0.15%	0.039%
65	15.175	2053	2055	2058	rVB4	5117	5331	0.22%	0.056%

66	15.540	2115	2117	2119	rBV	4207	4183	0.17%	0.044%
67	15.598	2126	2127	2132	rBV3	3652	5832	0.24%	0.062%
68	15.793	2157	2160	2164	rBV4	5150	7529	0.31%	0.080%
69	15.940	2182	2185	2191	rVB3	3900	5981	0.25%	0.063%
70	16.081	2206	2209	2213	rVB	4399	4802	0.20%	0.051%

71	16.140	2213	2219	2220	rBV2	3754	5472	0.22%	0.058%
72	16.281	2239	2243	2244	rVB3	4295	4390	0.18%	0.046%
73	16.816	2330	2334	2337	rVB	2518	3950	0.16%	0.042%
74	16.840	2337	2338	2340	rBV	5538	4673	0.19%	0.049%
75	16.887	2343	2346	2347	rBV2	6937	5430	0.22%	0.057%

76	16.975	2359	2361	2365	rVB3	4131	5798	0.24%	0.061%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061221\
 Data File : BN014894.D
 Acq On : 12 Jun 2021 15:23
 Operator : CG/JU
 Sample : M2620-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
 Title : SVOA CALIBRATION

77	17.016	2365	2368	2370	rBV2	3073	4059	0.17%	0.043%
78	17.034	2370	2371	2374	rBV2	5958	4272	0.18%	0.045%
79	17.092	2375	2381	2392	rBV	1028064	1595220	65.50%	16.884%
80	17.192	2397	2398	2403	rVB4	8587	10422	0.43%	0.110%
81	17.381	2427	2430	2432	rBV4	4229	6152	0.25%	0.065%
82	17.469	2443	2445	2447	rBV3	4256	3611	0.15%	0.038%
83	17.534	2455	2456	2461	rVB3	7350	7023	0.29%	0.074%
84	17.687	2479	2482	2484	rVB3	4586	3873	0.16%	0.041%
85	17.887	2515	2516	2520	rVB2	5626	4578	0.19%	0.048%
86	18.239	2574	2576	2579	rBV2	7348	7438	0.31%	0.079%
87	18.698	2652	2654	2657	rBV2	7171	6913	0.28%	0.073%
88	18.757	2662	2664	2665	rBV2	7334	6549	0.27%	0.069%
89	18.863	2680	2682	2685	rBV4	4066	3821	0.16%	0.040%
90	19.222	2741	2743	2746	rBV4	4195	4483	0.18%	0.047%
91	19.445	2779	2781	2785	rBV4	5949	8090	0.33%	0.086%
92	19.657	2814	2817	2818	rBV2	6211	5707	0.23%	0.060%
93	19.692	2821	2823	2824	rBV2	9970	5640	0.23%	0.060%
94	19.792	2838	2840	2842	rBV3	6749	6174	0.25%	0.065%
95	19.845	2848	2849	2853	rBV3	6225	5228	0.21%	0.055%
96	20.028	2877	2880	2881	rBV2	7520	7779	0.32%	0.082%
97	20.228	2912	2914	2916	rBV3	9162	5012	0.21%	0.053%
98	20.457	2951	2953	2955	rBV3	15824	12732	0.52%	0.135%
99	21.292	3090	3095	3104	rBV	1629829	2271901	93.29%	24.046%
100	23.551	3472	3479	3488	rVB	1238106	2435375	100.00%	25.776%



Sum of corrected areas: 9448322

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061221\
Data File : BN014894.D
Acq On : 12 Jun 2021 15:23
Operator : CG/JU
Sample : M2620-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

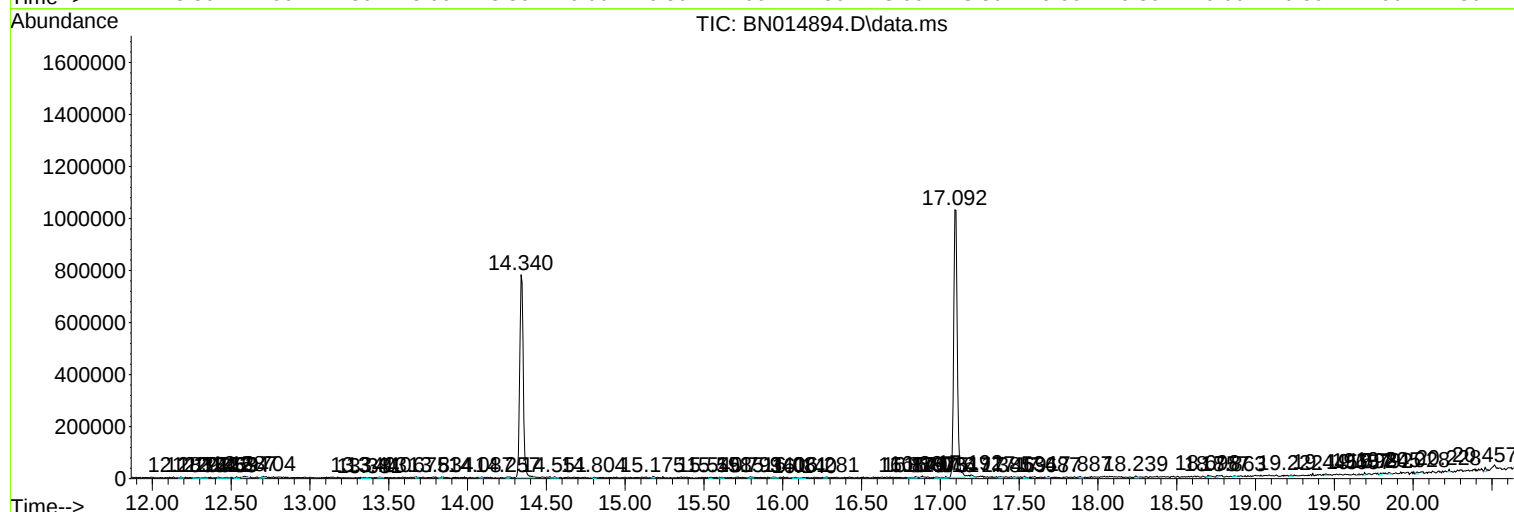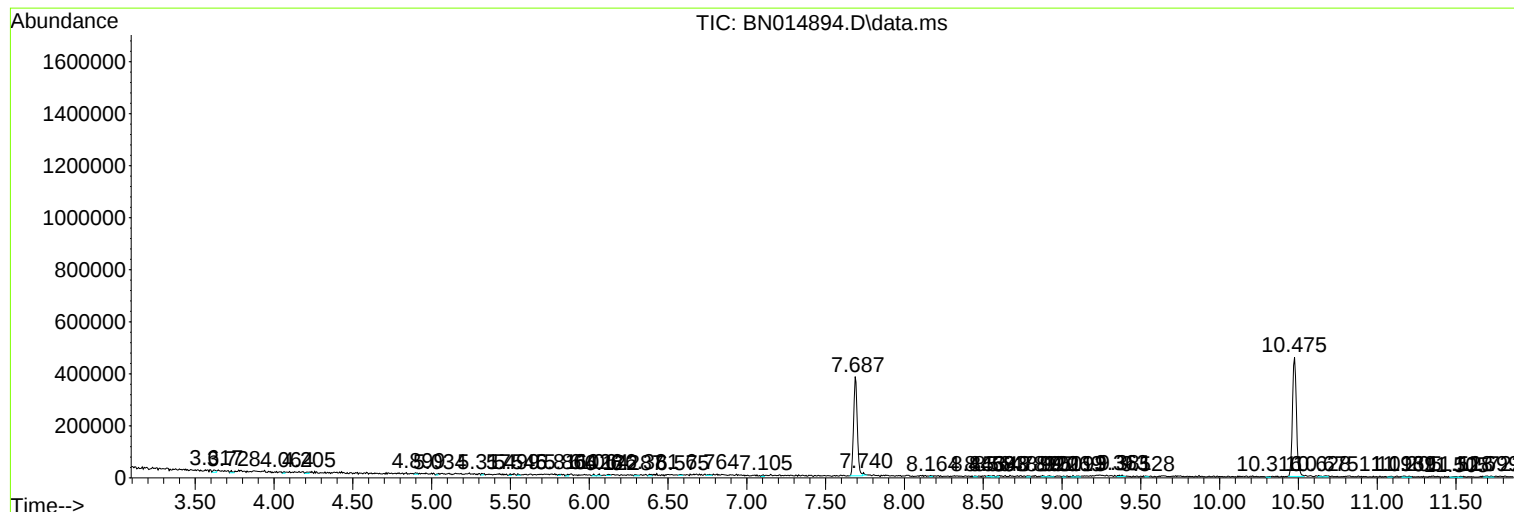

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061221\
Data File : BN014894.D
Acq On : 12 Jun 2021 15:23
Operator : CG/JU
Sample : M2620-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061221\
Data File : BN014894.D
Acq On : 12 Jun 2021 15:23
Operator : CG/JU
Sample : M2620-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061221MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
