

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061223\
 Data File : BN025780.D
 Acq On : 12 Jun 2023 13:54
 Operator : MA/JU
 Sample : PB153180BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK180

Quant Time: Jun 13 00:02:19 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN060923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jun 10 02:01:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.005	152	12267	0.400	ng/ul	0.00
4) Naphthalene-d8	10.820	136	36982	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.641	164	22334	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.386	188	47113	0.400	ng/ul	0.00
17) Chrysene-d12	21.571	240	27563	0.400	ng/ul	0.00
23) Perylene-d12	24.032	264	29641	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	65755	5.452	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.409	152	14380	0.307	ng/ul	0.00
18) Fluoranthene-d10	19.411	212	31030	0.357	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.631	166	5709	0.070	ng/ul#	12
20) Pyrene	19.773	202	5322	0.041	ng/ul#	1
26) Benzo(a)pyrene	23.874	252	8952	0.087	ng/ul#	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061223\
Data File : BN025780.D
Acq On : 12 Jun 2023 13:54
Operator : MA/JU
Sample : PB153180BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK180

Quant Time: Jun 13 00:02:19 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 10 02:01:49 2023
Response via : Initial Calibration




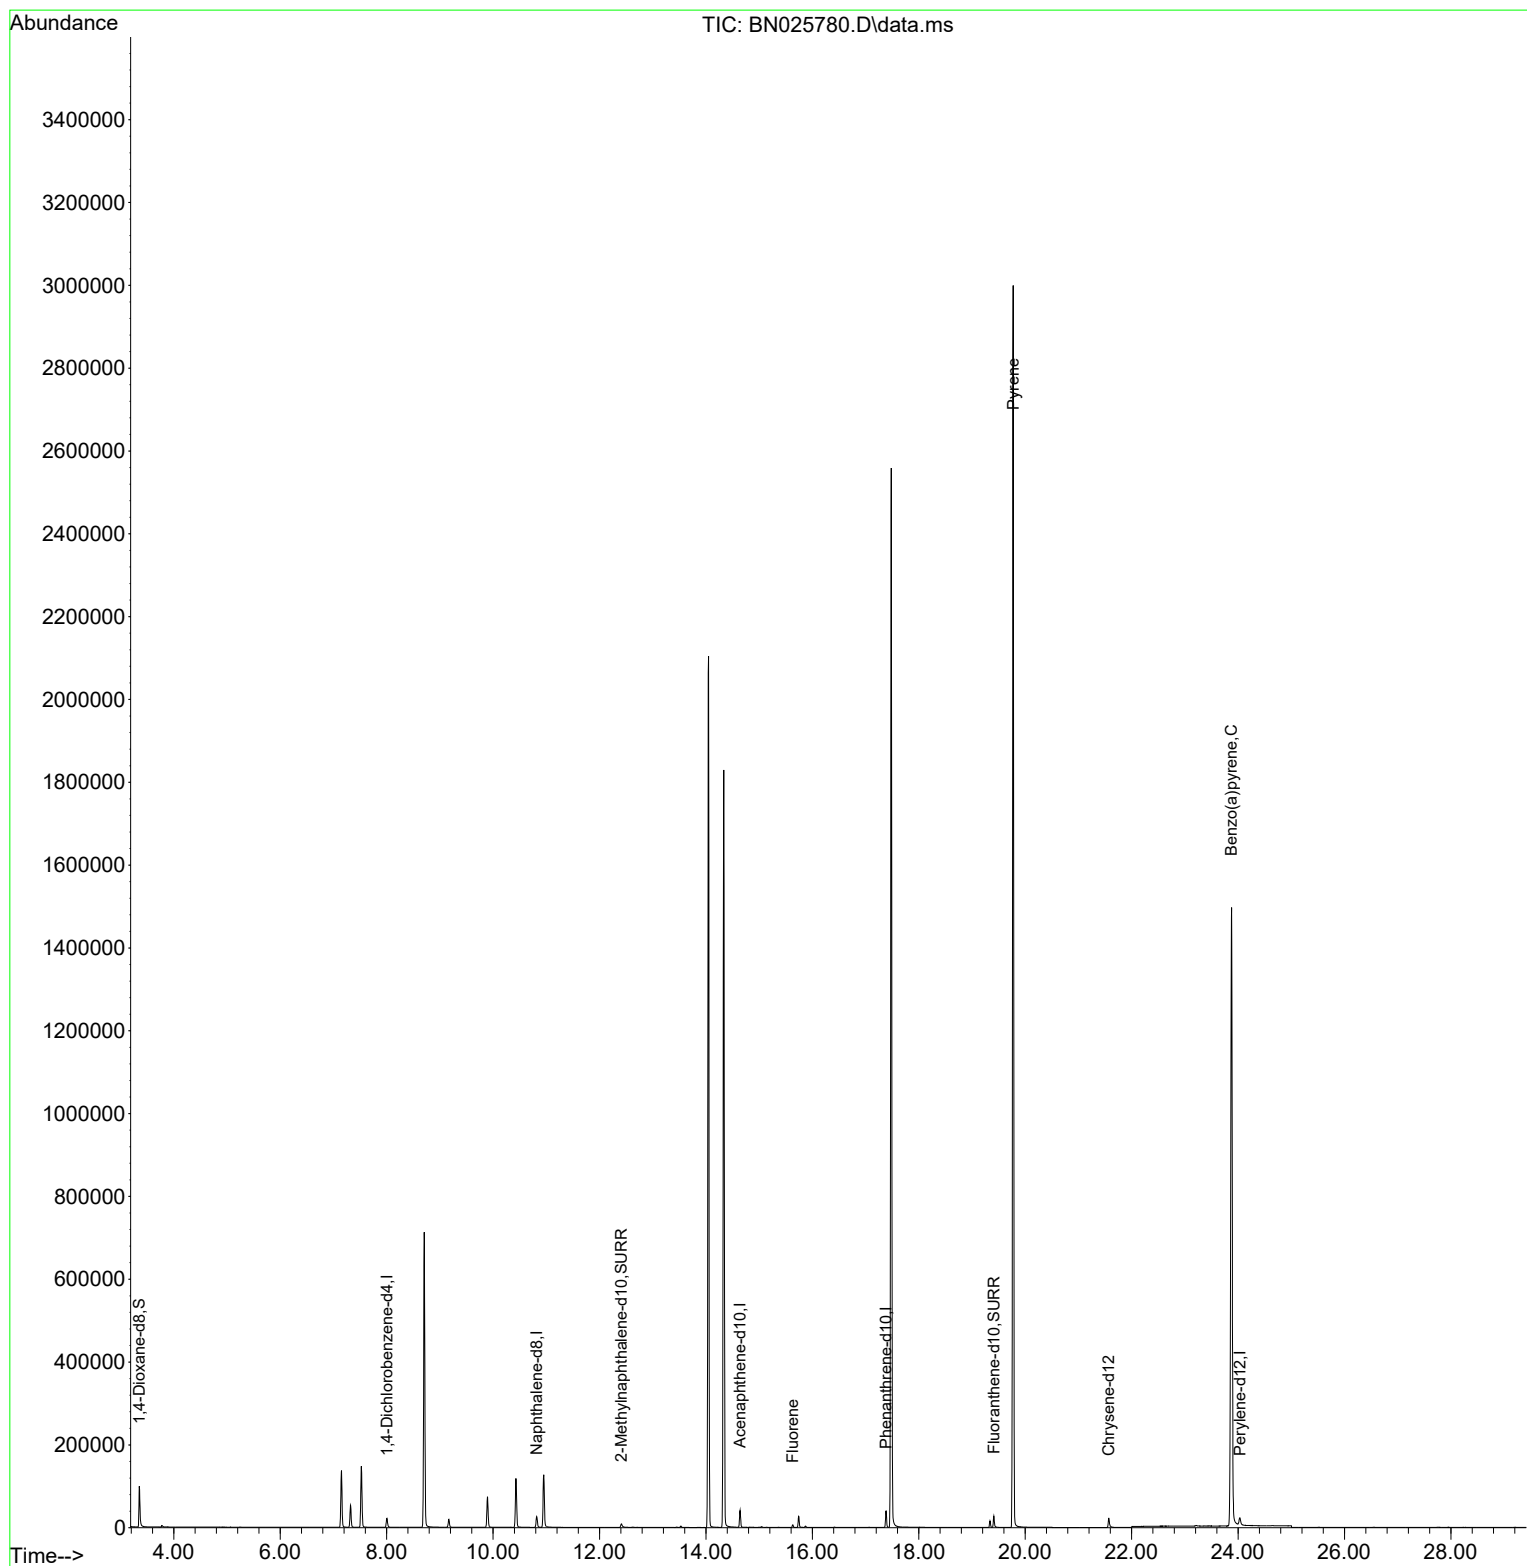


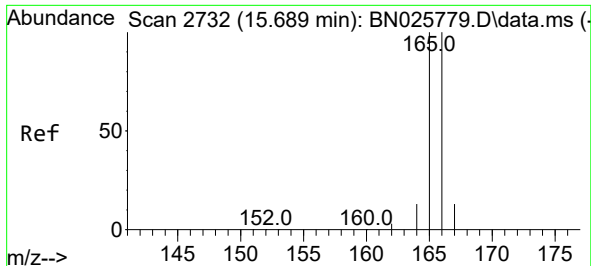

#12
Fluorene
Concen: 0.070 ng/ul
RT: 15.631 min Scan# 21
Delta R.T. -0.059 min
Lab File: BN025780.D
Acq: 12 Jun 2023 13:54




Instrument :
BNA_N
ClientSampleId :
SBLK180


Tgt Ion:166 Resp: 5709
Ion Ratio Lower Upper
166 100
165 5.5 79.2 118.8#
167 31.8 11.0 16.6#

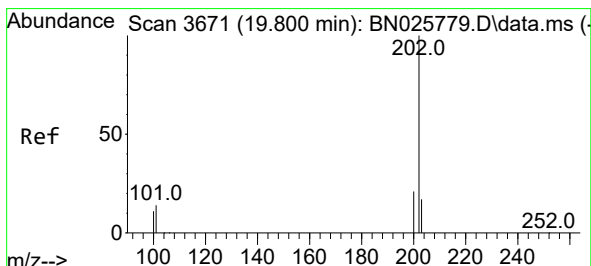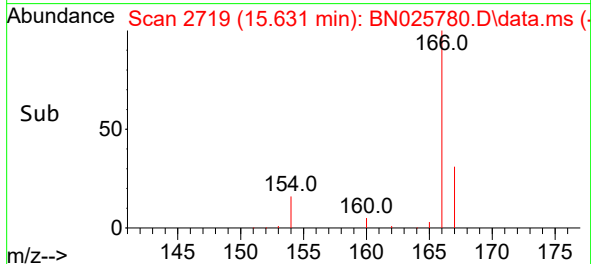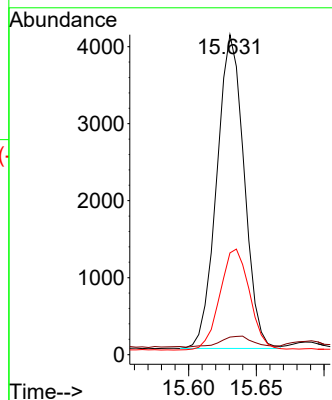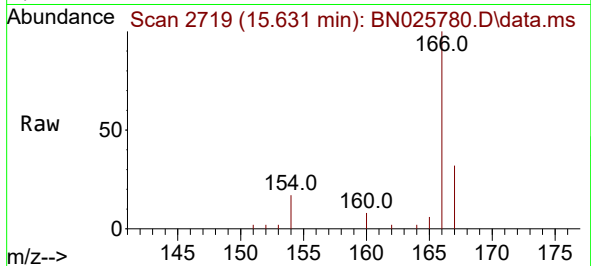

#20
Pyrene
Concen: 0.041 ng/ul
RT: 19.773 min Scan# 3665
Delta R.T. -0.032 min
Lab File: BN025780.D
Acq: 12 Jun 2023 13:54


Tgt Ion:202 Resp: 5322
Ion Ratio Lower Upper
202 100
101 172.5 10.4 15.6#
100 1332.2 8.8 13.2#

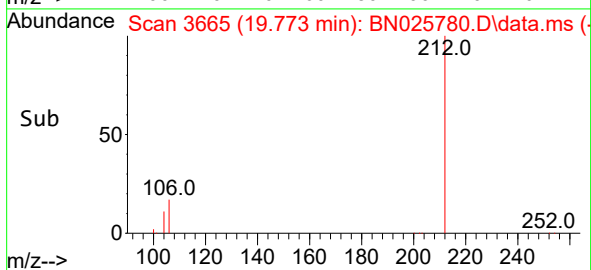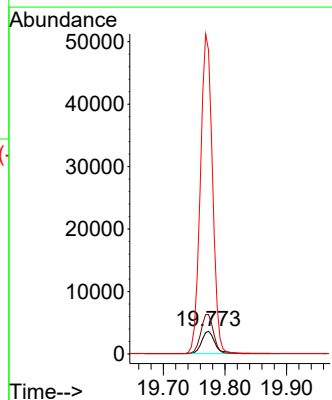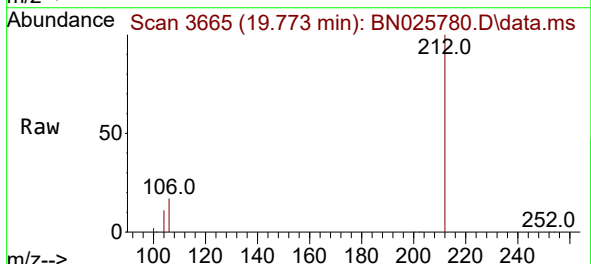

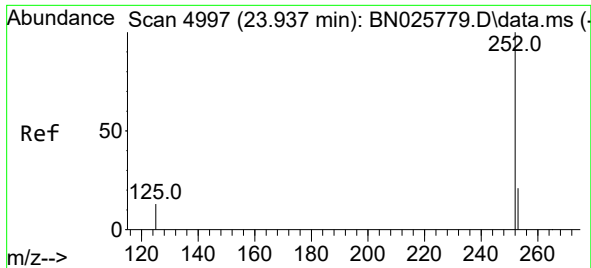

#26
Benzo(a)pyrene
Concen: 0.087 ng/ul
RT: 23.874 min Scan# 4997
Delta R.T. -0.069 min
Lab File: BN025780.D
Acq: 12 Jun 2023 13:54

Instrument :
BNA_N
ClientSampleId :
SBLK180

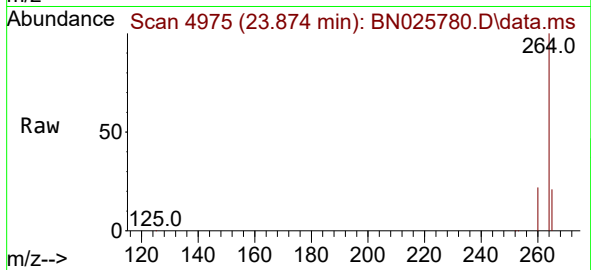

Tgt Ion:252 Resp: 8952
Ion Ratio Lower Upper
252 100
253 51.9 25.8 38.8#
125 31.1 13.5 20.3#

