

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061223\
 Data File : BN025786.D
 Acq On : 12 Jun 2023 17:46
 Operator : MA/JU
 Sample : PB153137BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK137

Quant Time: Jun 13 00:03:16 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN060923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jun 10 02:01:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.009	152	9184	0.400	ng/ul	0.00
4) Naphthalene-d8	10.825	136	27199	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.644	164	15255	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.385	188	28155	0.400	ng/ul	0.00
17) Chrysene-d12	21.576	240	12567	0.400	ng/ul	0.00
23) Perylene-d12	24.051	264	15611	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	55741	6.174	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.414	152	11091	0.322	ng/ul	0.00
18) Fluoranthene-d10	19.414	212	17685	0.446	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.634	166	4075	0.073	ng/ul#	12
20) Pyrene	19.772	202	3057	0.051	ng/ul#	1
26) Benzo(a)pyrene	23.897	252	5130	0.095	ng/ul#	44


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061223\
Data File : BN025786.D
Acq On : 12 Jun 2023 17:46
Operator : MA/JU
Sample : PB153137BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK137

Quant Time: Jun 13 00:03:16 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 10 02:01:49 2023
Response via : Initial Calibration




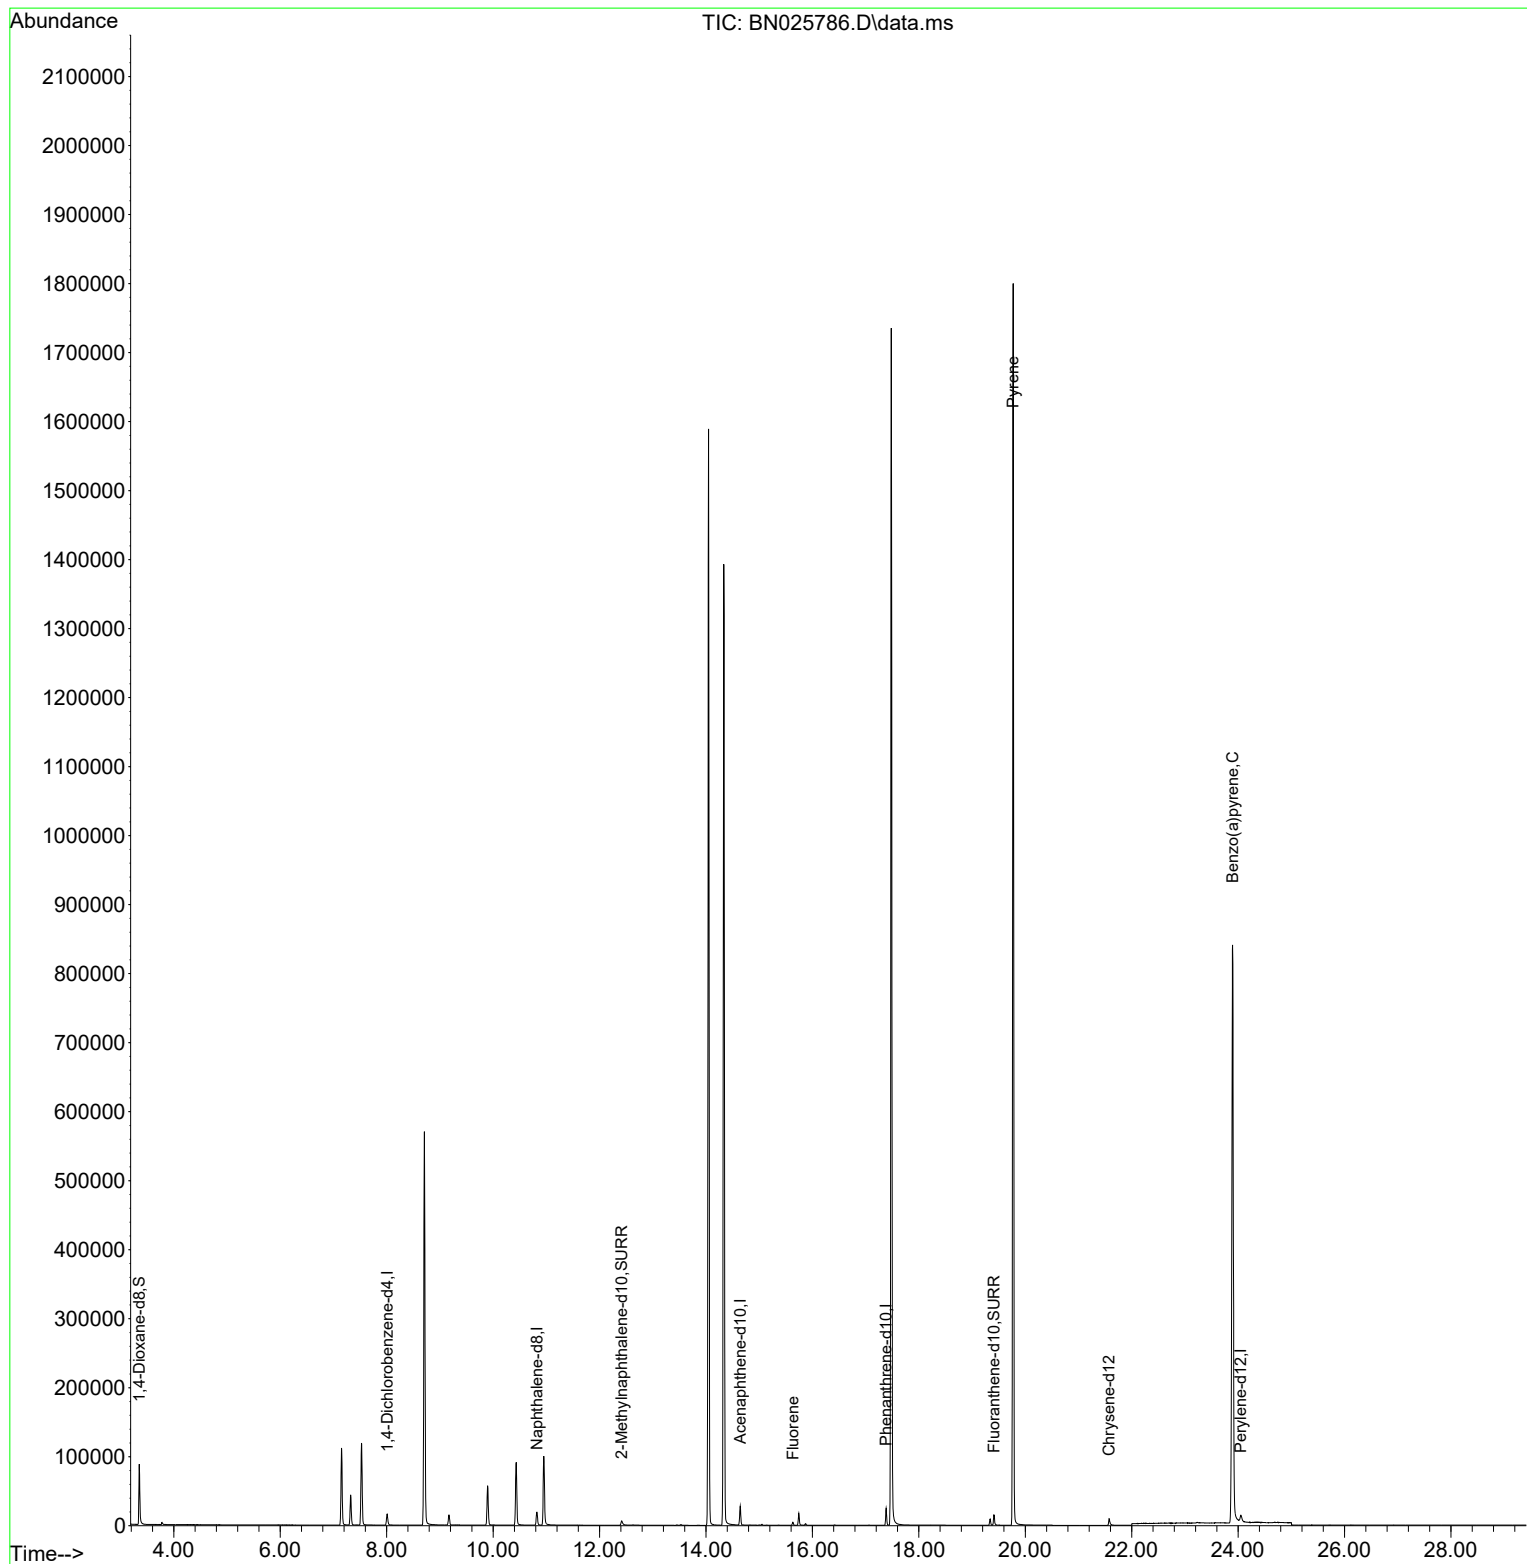


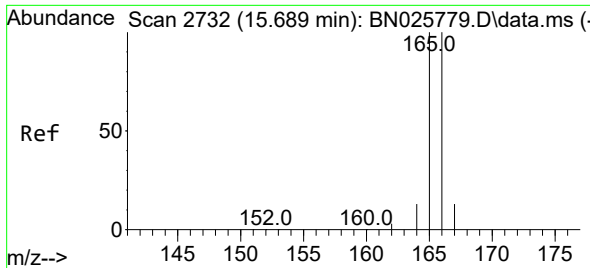

#12
Fluorene
Concen: 0.073 ng/ul
RT: 15.634 min Scan# 21
Delta R.T. -0.056 min
Lab File: BN025786.D
Acq: 12 Jun 2023 17:46




Instrument :
BNA_N
ClientSampleId :
SBLK137


Tgt Ion:166 Resp: 4075
Ion Ratio Lower Upper
166 100
165 6.6 79.2 118.8#
167 34.6 11.0 16.6#

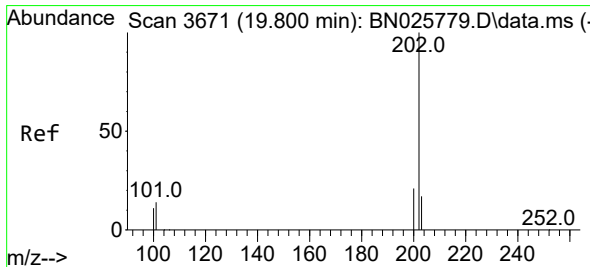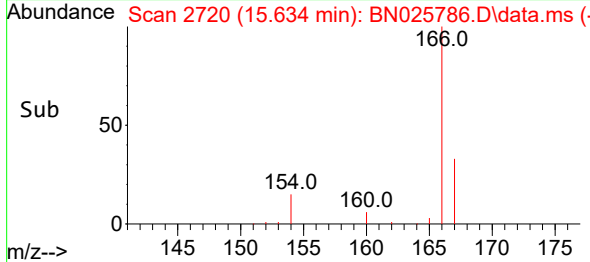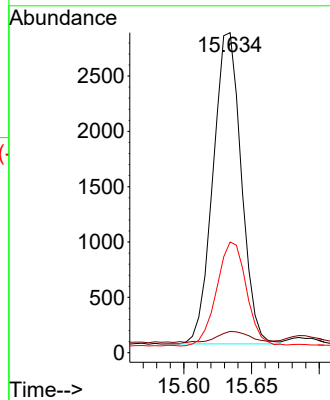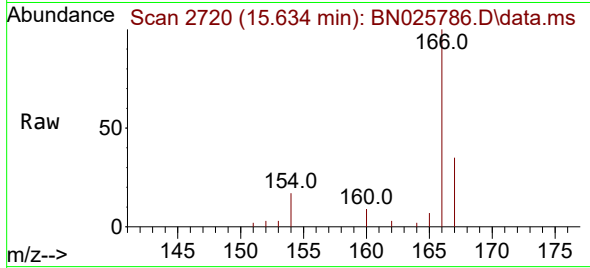

#20
Pyrene
Concen: 0.051 ng/ul
RT: 19.772 min Scan# 3665
Delta R.T. -0.033 min
Lab File: BN025786.D
Acq: 12 Jun 2023 17:46


Tgt Ion:202 Resp: 3057
Ion Ratio Lower Upper
202 100
101 174.7 10.4 15.6#
100 1332.0 8.8 13.2#

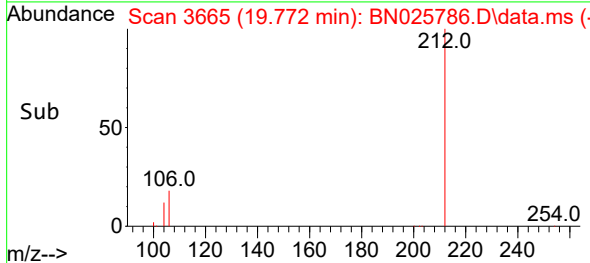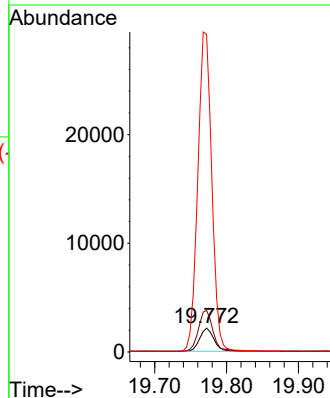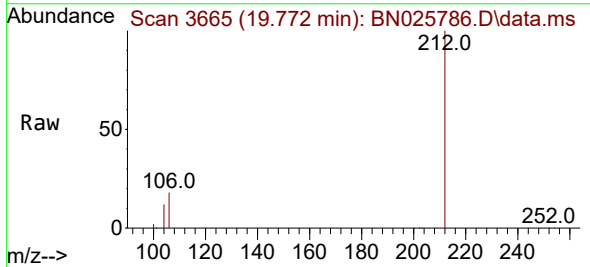

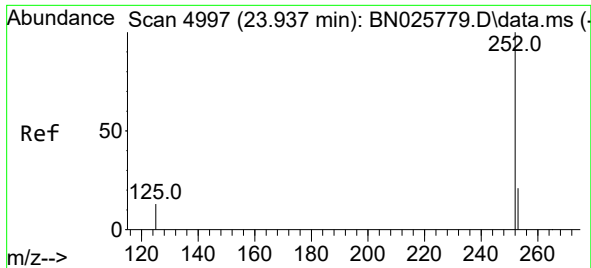

#26
Benzo(a)pyrene
Concen: 0.095 ng/ul
RT: 23.897 min Scan# 4983
Delta R.T. -0.047 min
Lab File: BN025786.D
Acq: 12 Jun 2023 17:46

Instrument :
BNA_N
ClientSampleId :
SBLK137

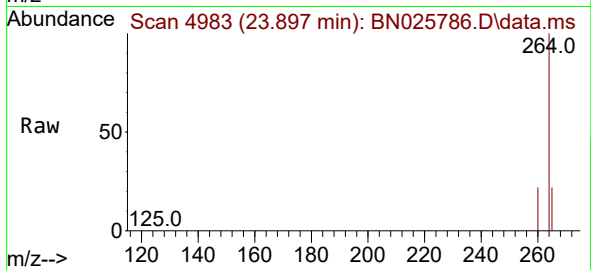

Tgt Ion:252 Resp: 5130
Ion Ratio Lower Upper
252 100
253 67.9 25.8 38.8#
125 35.1 13.5 20.3#

