




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061223\
Data File : BN025793.D
Acq On : 12 Jun 2023 22:01
Operator : MA/JU
Sample : 02960-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
H0FN9

Manual IntegrationsAPPROVED

Quant Time: Jun 13 00:04:19 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 10 02:01:49 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/13/2023
Supervised By :mohammad ahmed 06/13/2023

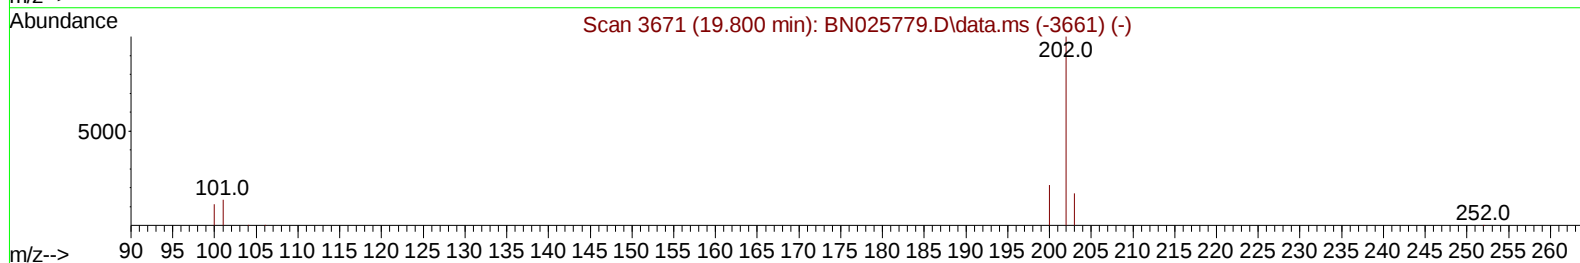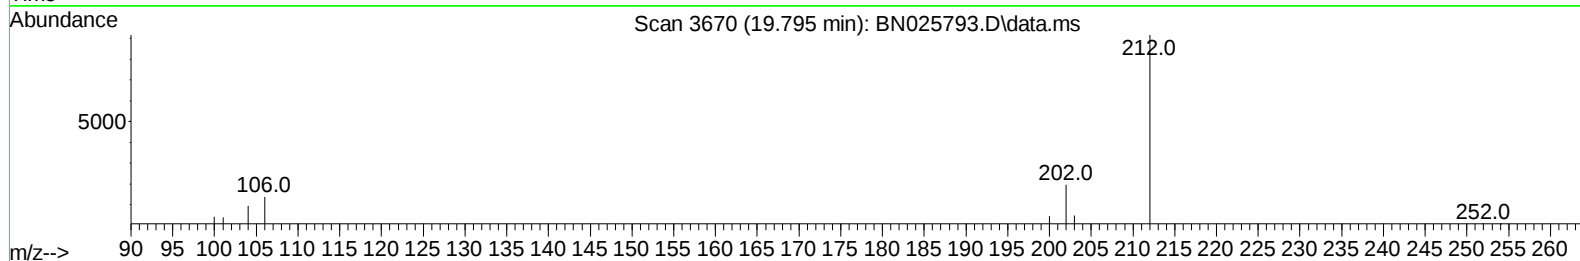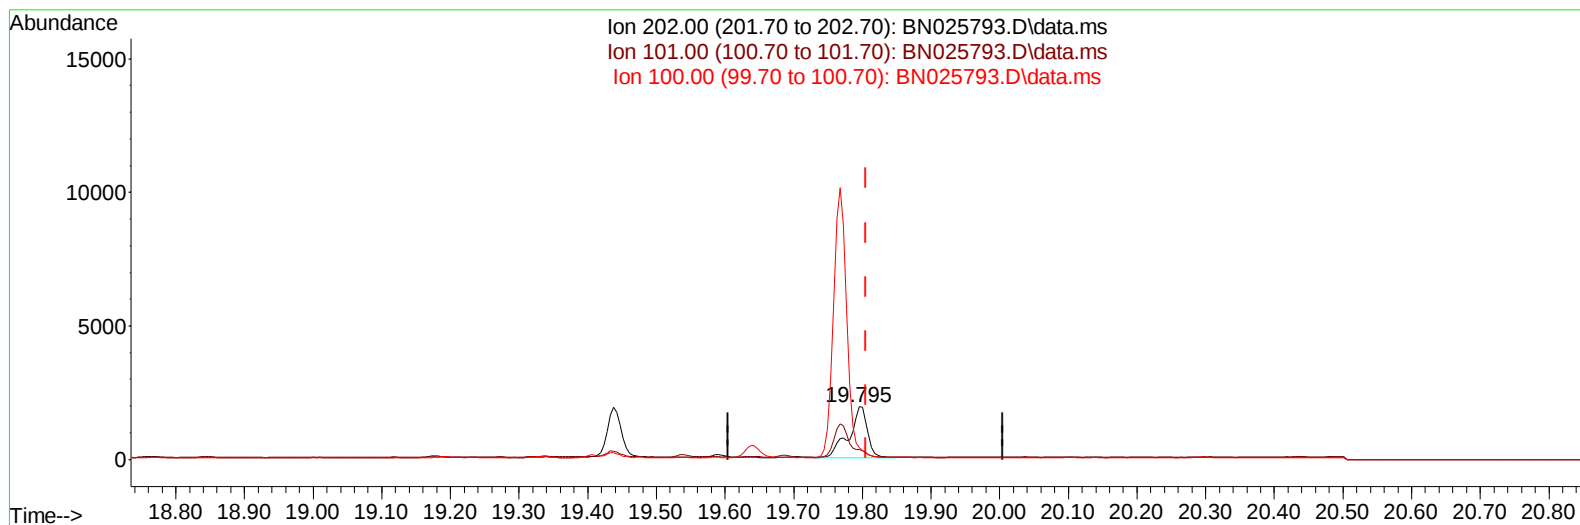

TIC: BN025793.D\data.ms

(20) Pyrene

19.795min (-0.010) 0.05 ng/u1

response 3632

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	13.00	19.55#
100.00	11.00	22.19#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061223\
 Data File : BN025793.D
 Acq On : 12 Jun 2023 22:01
 Operator : MA/JU
 Sample : 02960-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 H0FN9

Manual IntegrationsAPPROVED

Quant Time: Jun 13 00:04:19 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN060923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jun 10 02:01:49 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/13/2023
 Supervised By :mohammad ahmed 06/13/2023

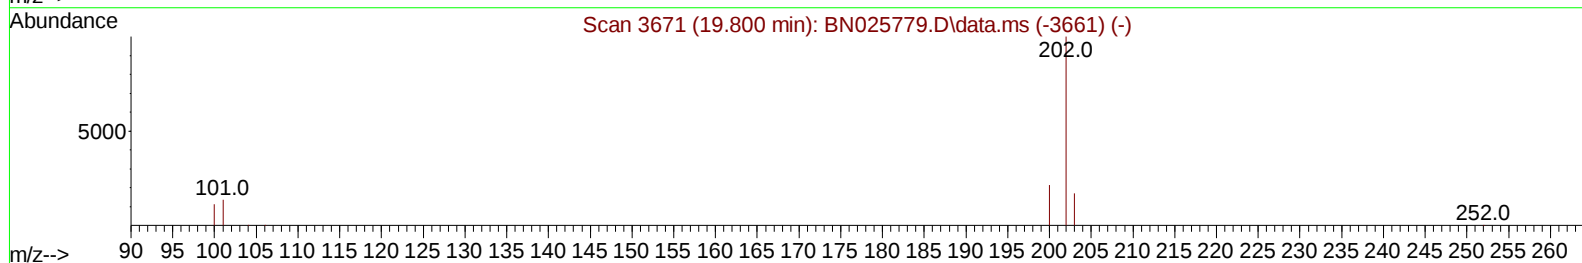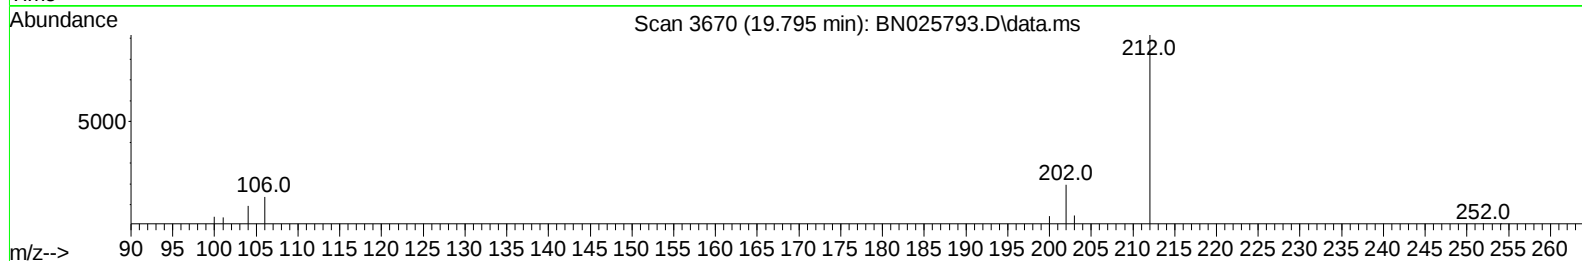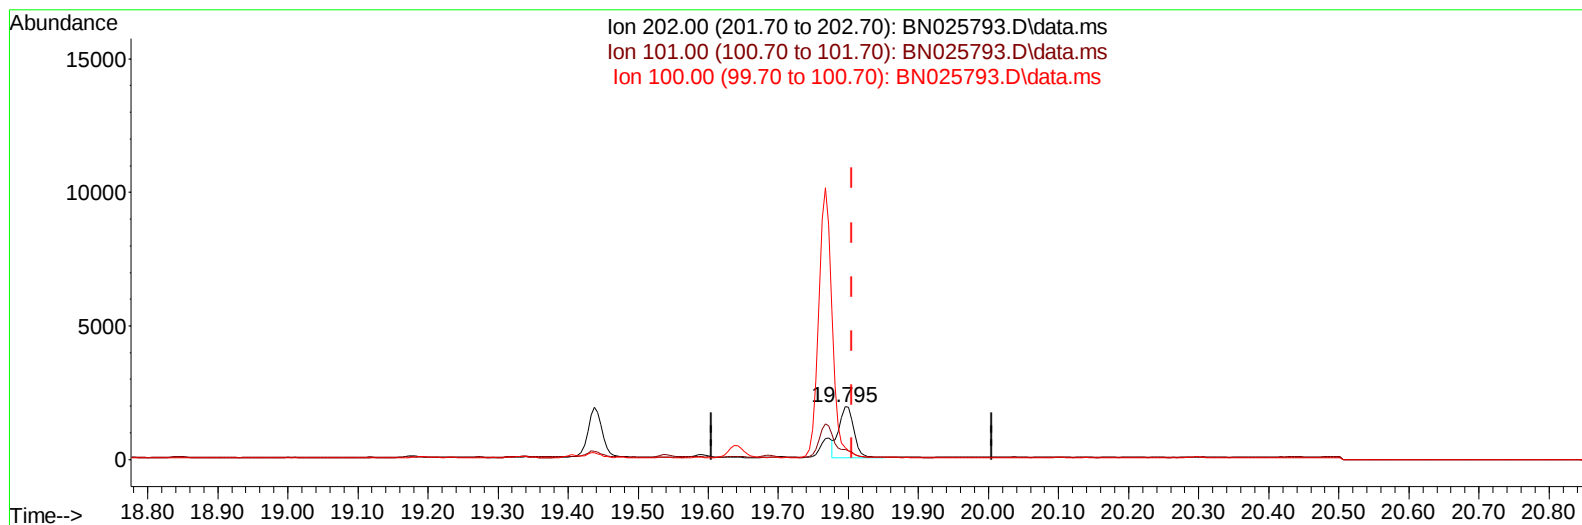

TIC: BN025793.D\data.ms

(20) Pyrene

19.795min (-0.010) 0.04 ng/ul m

response 2765

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	13.00	19.55#
100.00	11.00	22.19#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061223\
 Data File : BN025793.D
 Acq On : 12 Jun 2023 22:01
 Operator : MA/JU
 Sample : 02960-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 H0FN9

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/13/2023
 Supervised By :mohammad ahmed 06/13/2023

Quant Time: Jun 13 00:04:19 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN060923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jun 10 02:01:49 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.005	152		8476	0.400	ng/ul	0.00
4) Naphthalene-d8	10.820	136		25255	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.639	164		14537	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.385	188		28916	0.400	ng/ul	0.00
17) Chrysene-d12	21.566	240		15595	0.400	ng/ul	0.00
23) Perylene-d12	24.033	264		13537	0.400	ng/ul	-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.352	96		10645	1.277	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.409	152		2896	0.090	ng/ul	0.00
18) Fluoranthene-d10	19.409	212		6087	0.124	ng/ul	0.00
Target Compounds							Qvalue
15) Phenanthrene	17.423	178		2390	0.028	ng/ul#	89
19) Fluoranthene	19.437	202		2730	0.038	ng/ul#	89
20) Pyrene	19.795	202		2765m	0.037	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061223\
Data File : BN025793.D
Acq On : 12 Jun 2023 22:01
Operator : MA/JU
Sample : 02960-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
H0FN9

Manual IntegrationsAPPROVED

Quant Time: Jun 13 00:04:19 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 10 02:01:49 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/13/2023
Supervised By :mohammad ahmed 06/13/2023

