

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061318\
 Data File : BN001851.D
 Acq On : 13 Jun 2018 19:54
 Operator : JU/SJ
 Sample : J3375-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 14 05:25:38 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN061318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 13 12:02:12 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	7311	0.40	ng/ul	0.00
2) Naphthalene-d8	10.50	136	29452	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.35	164	18188	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.20	188	3271816	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.30
20) Perylene-d12	23.53	264	31707	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.09	152	18281	0.39	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.40	166	1567	0.021	ng/ul	93
23) Benzo(a)pyrene	23.40	252	11209	0.105	ng/ul#	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061318\
Data File : BN001851.D
Acq On : 13 Jun 2018 19:54
Operator : JU/SJ
Sample : J3375-07
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 14 05:25:38 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN061318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 13 12:02:12 2018
Response via : Initial Calibration




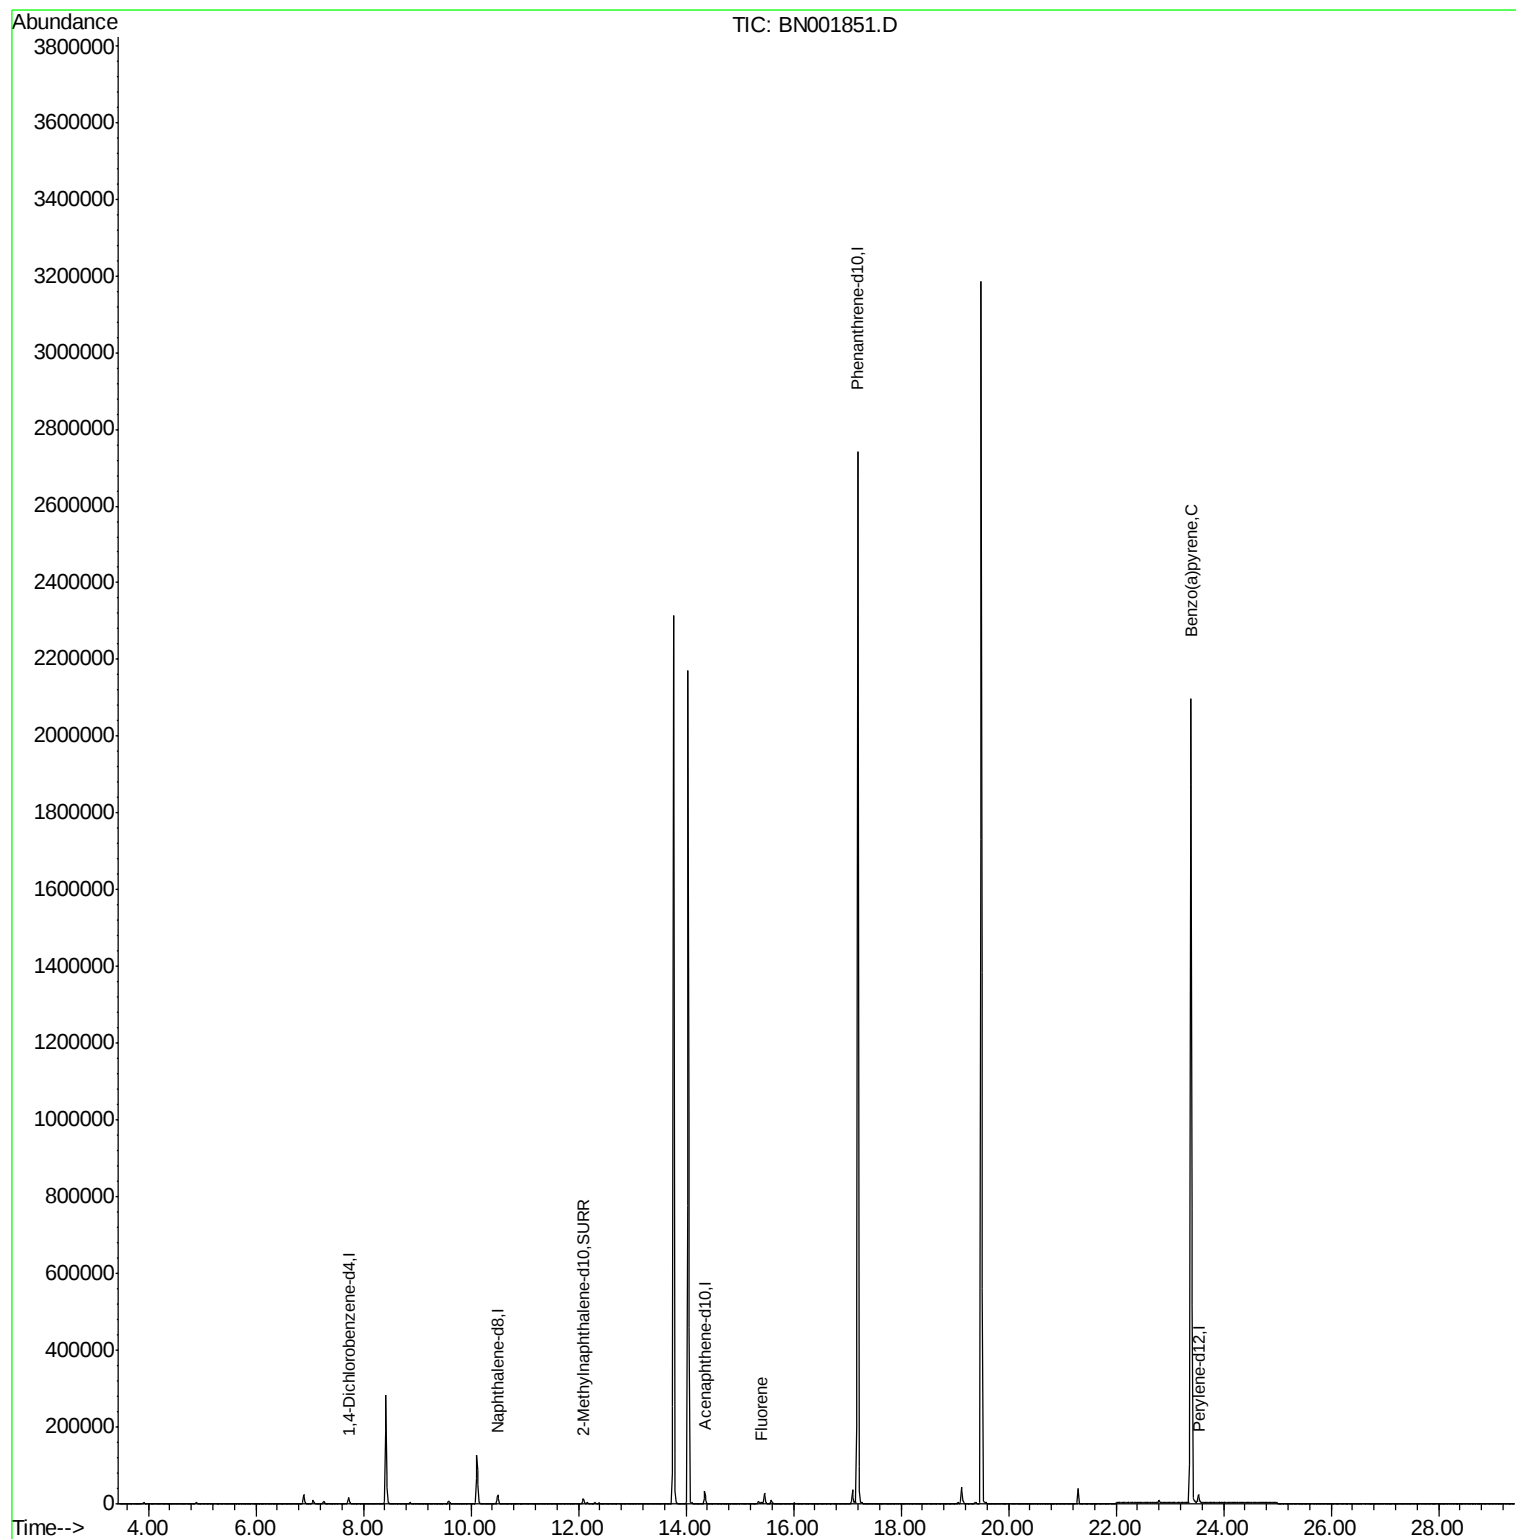


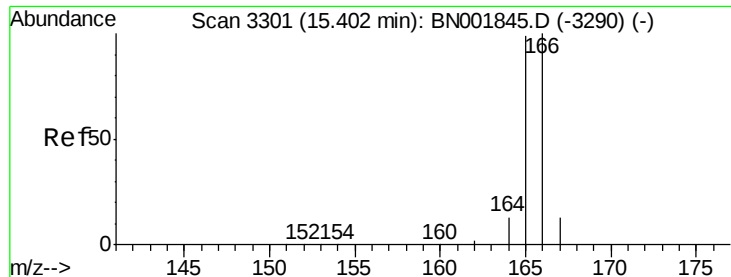

#9
Fluorene
 Concen: 0.021 ng/ul
 RT: 15.40 min Scan# 3301
 Delta R.T. -0.00 min
 Lab File: BN001851.D
 Acq: 13 Jun 2018 19:54

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion:166 Resp: 1567
 Ion Ratio Lower Upper
 166 100
 165 99.7 73.4 110.2
 167 19.4 14.6 22.0

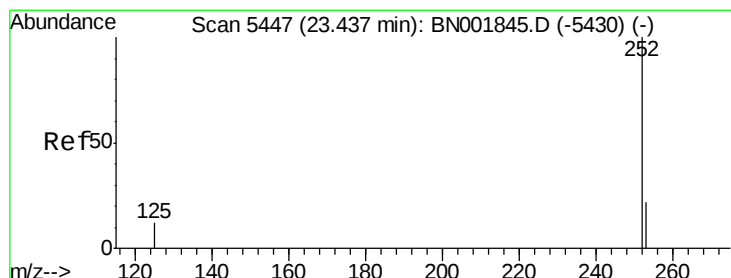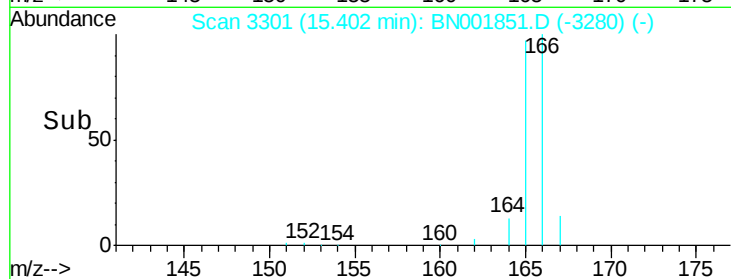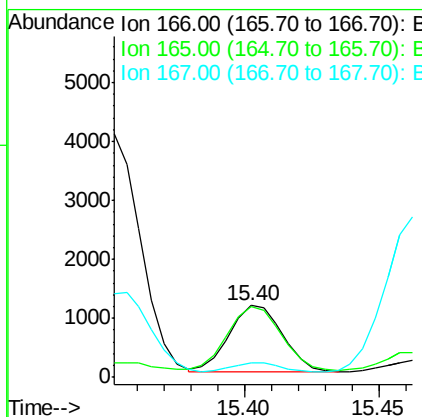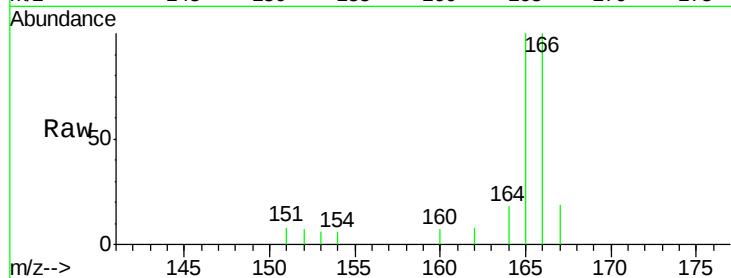

#23
Benzo(a)pyrene
 Concen: 0.105 ng/ul
 RT: 23.40 min Scan# 5433
 Delta R.T. -0.04 min
 Lab File: BN001851.D
 Acq: 13 Jun 2018 19:54

Tgt Ion:252 Resp: 11209
 Ion Ratio Lower Upper
 252 100
 253 29.7 16.0 24.0#
 125 24.4 12.0 18.0#

