

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN061318\
 Data File : BN001847.D
 Acq On : 13 Jun 2018 17:33
 Operator : JU/SJ
 Sample : J3375-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DAWS1

Manual Integrations
 APPROVED

Sohil
 6/14/2018 3:57:31 PM

Quant Time: Jun 13 18:37:50 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN061318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 13 18:19:19 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	7081	0.40	ng/ul	0.00
2) Naphthalene-d8	10.50	136	28170	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.35	164	17094	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.10	188	38642m	0.40	ng/ul	0.00
16) Chrysene-d12	21.29	240	35943m	0.40	ng/ul	0.00
20) Perylene-d12	23.53	264	35873	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.09	152	14861	0.33	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	41097m	0.35	ng/ul	0.00
Target Compounds						
9) Fluorene	15.41	166	2584	0.036	ng/ul	94
12) Phenanthrene	17.14	178	7326m	0.064	ng/ul	
13) Anthracene	17.23	178	6047m	0.055	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN061318\
Data File : BN001847.D
Acq On : 13 Jun 2018 17:33
Operator : JU/SJ
Sample : J3375-06
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
DAWS1

Manual Integrations
APPROVED

Sohil
6/14/2018 3:57:31 PM

Quant Time: Jun 13 18:37:50 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN061318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 13 18:19:19 2018
Response via : Initial Calibration

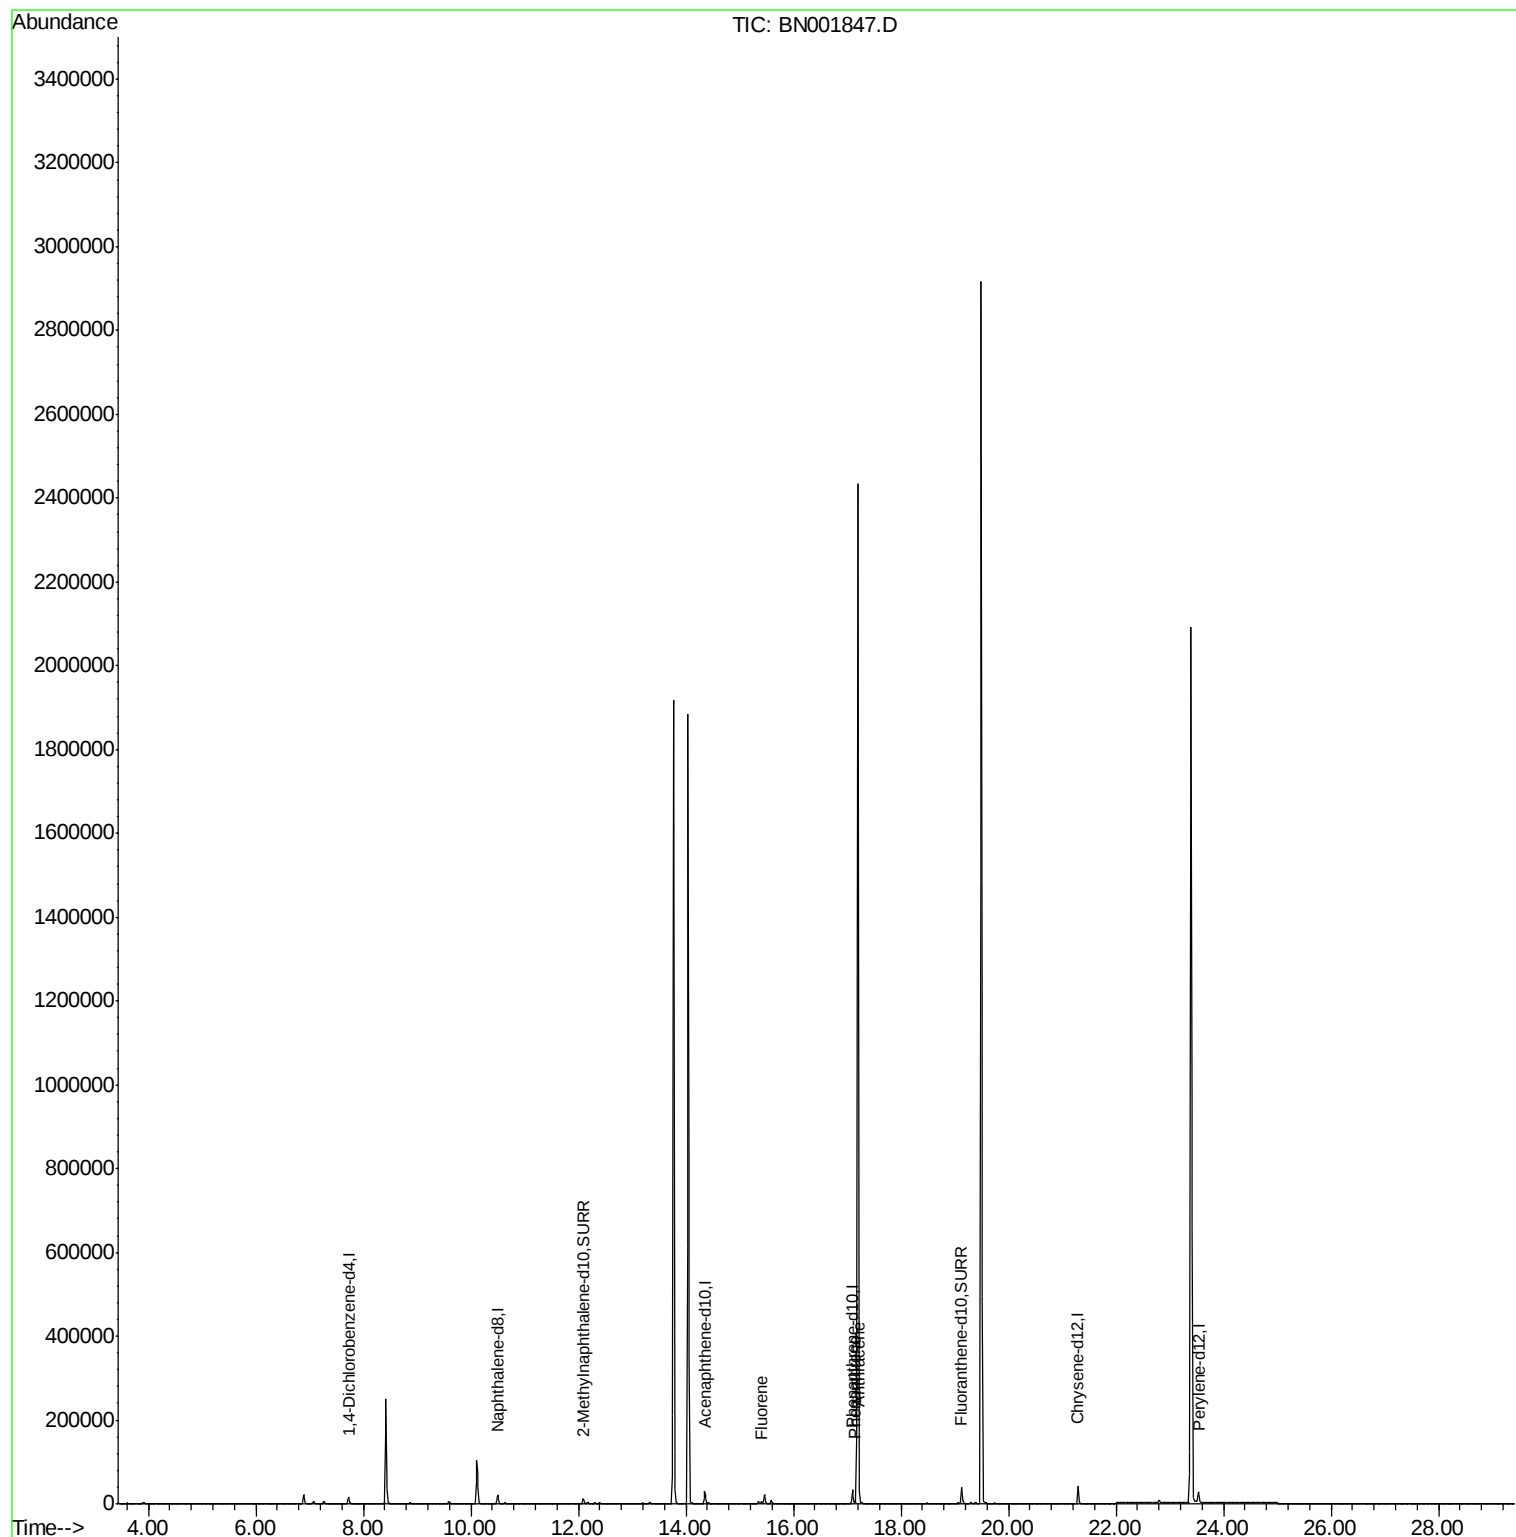

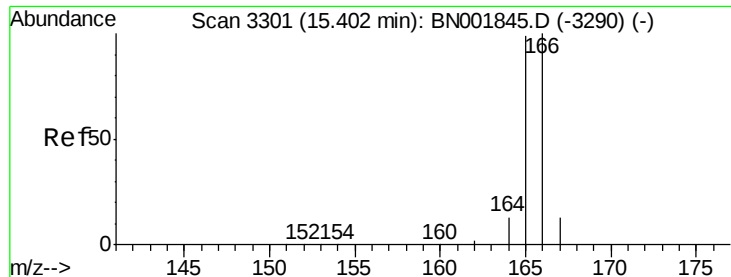

#9

Fluorene

Concen: 0.036 ng/ul

RT: 15.41 min Scan# 3302

Delta R.T. 0.00 min

Lab File: BN001847.D

Acq: 13 Jun 2018 17:33

Instrument :

BNA_N





ClientSampleId :

DAWS1

Tgt Ion:	166	Resp:	2584
Ion Ratio	Lower	Upper	
166	100		
165	98.7	73.4	110.2
167	17.3	14.6	22.0

Manual Integrations
APPROVED

Sohil
6/14/2018 3:57:31 PM

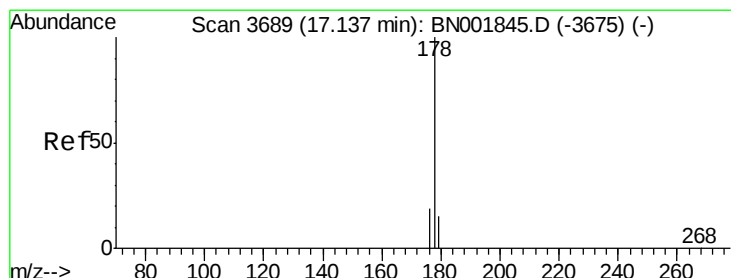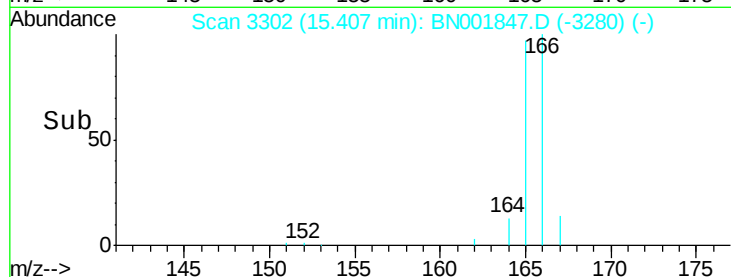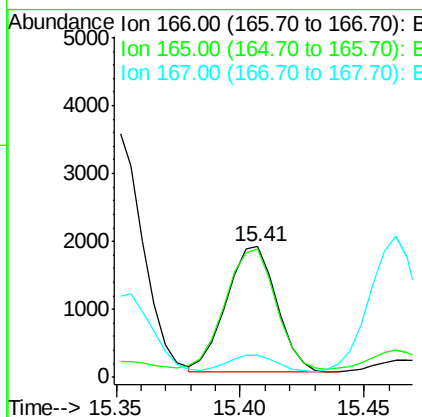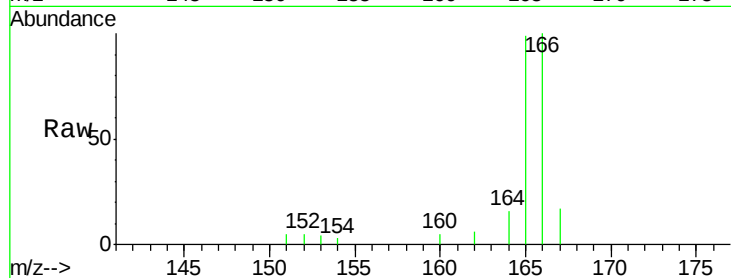

#12

Phenanthrene

Concen: 0.064 ng/ul m




RT: 17.14 min Scan# 3689


Delta R.T. -0.00 min

Lab File: BN001847.D

Acq: 13 Jun 2018 17:33


Tgt Ion:	178	Resp:	7326
Ion Ratio	Lower	Upper	
178	100		
179	16.9	18.4	27.6#
176	20.2	13.6	20.4

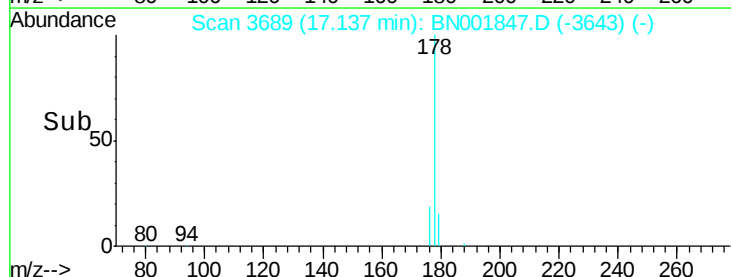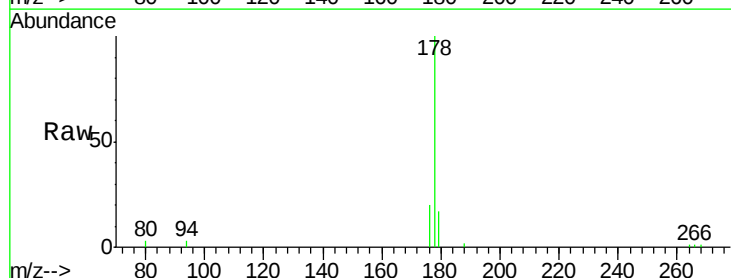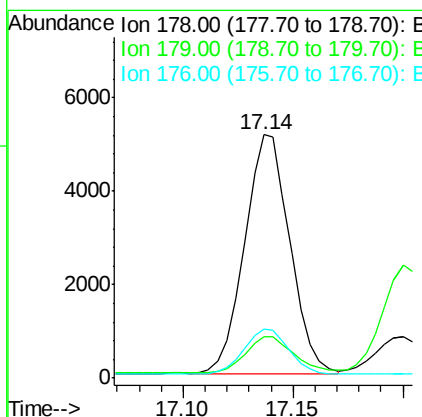

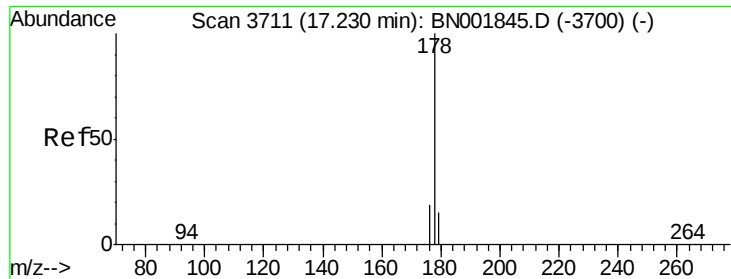

#13
 Anthracene
 Concen: 0.055 ng/ul m
 RT: 17.23 min Scan# 3711
 Delta R.T. 0.00 min
 Lab File: BN001847.D
 Acq: 13 Jun 2018 17:33

Instrument :
 BNA_N
 ClientSampleId :
 DAWS1

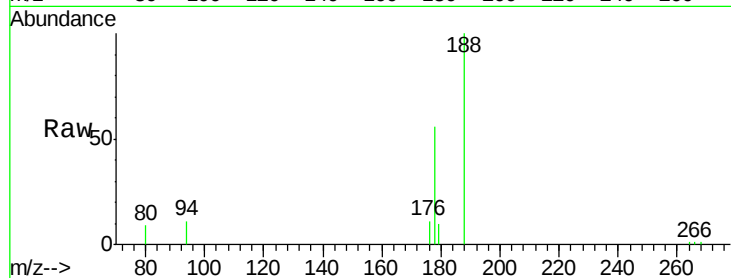

Tgt Ion	Ratio	Lower	Upper
178	100		
179	18.0	18.1	27.1#
176	19.9	14.7	22.1

Manual Integrations
 APPROVED

Sohil
 6/14/2018 3:57:31 PM

