

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN061318\
 Data File : BN001850.D
 Acq On : 13 Jun 2018 19:18
 Operator : JU/SJ
 Sample : J3375-12
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DAWS9

Manual Integrations
 APPROVED

Sohil
 6/14/2018 3:57:35 PM

Quant Time: Jun 14 05:42:36 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN061318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 13 12:02:12 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	7304	0.40	ng/ul	0.00
2) Naphthalene-d8	10.50	136	29833	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.35	164	18457	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.10	188	40928m	0.40	ng/ul	0.00
16) Chrysene-d12	21.29	240	32435m	0.40	ng/ul	0.00
20) Perylene-d12	23.53	264	24277m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.09	152	16668	0.35	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	41903m	0.34	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	16.74	266	38769m	5.003	ng/ul	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN061318\
Data File : BN001850.D
Acq On : 13 Jun 2018 19:18
Operator : JU/SJ
Sample : J3375-12
Misc :
ALS Vial : 18 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
DAWS9

Manual Integrations
APPROVED

Sohil
6/14/2018 3:57:35 PM

Quant Time: Jun 14 05:42:36 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN061318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 13 12:02:12 2018
Response via : Initial Calibration

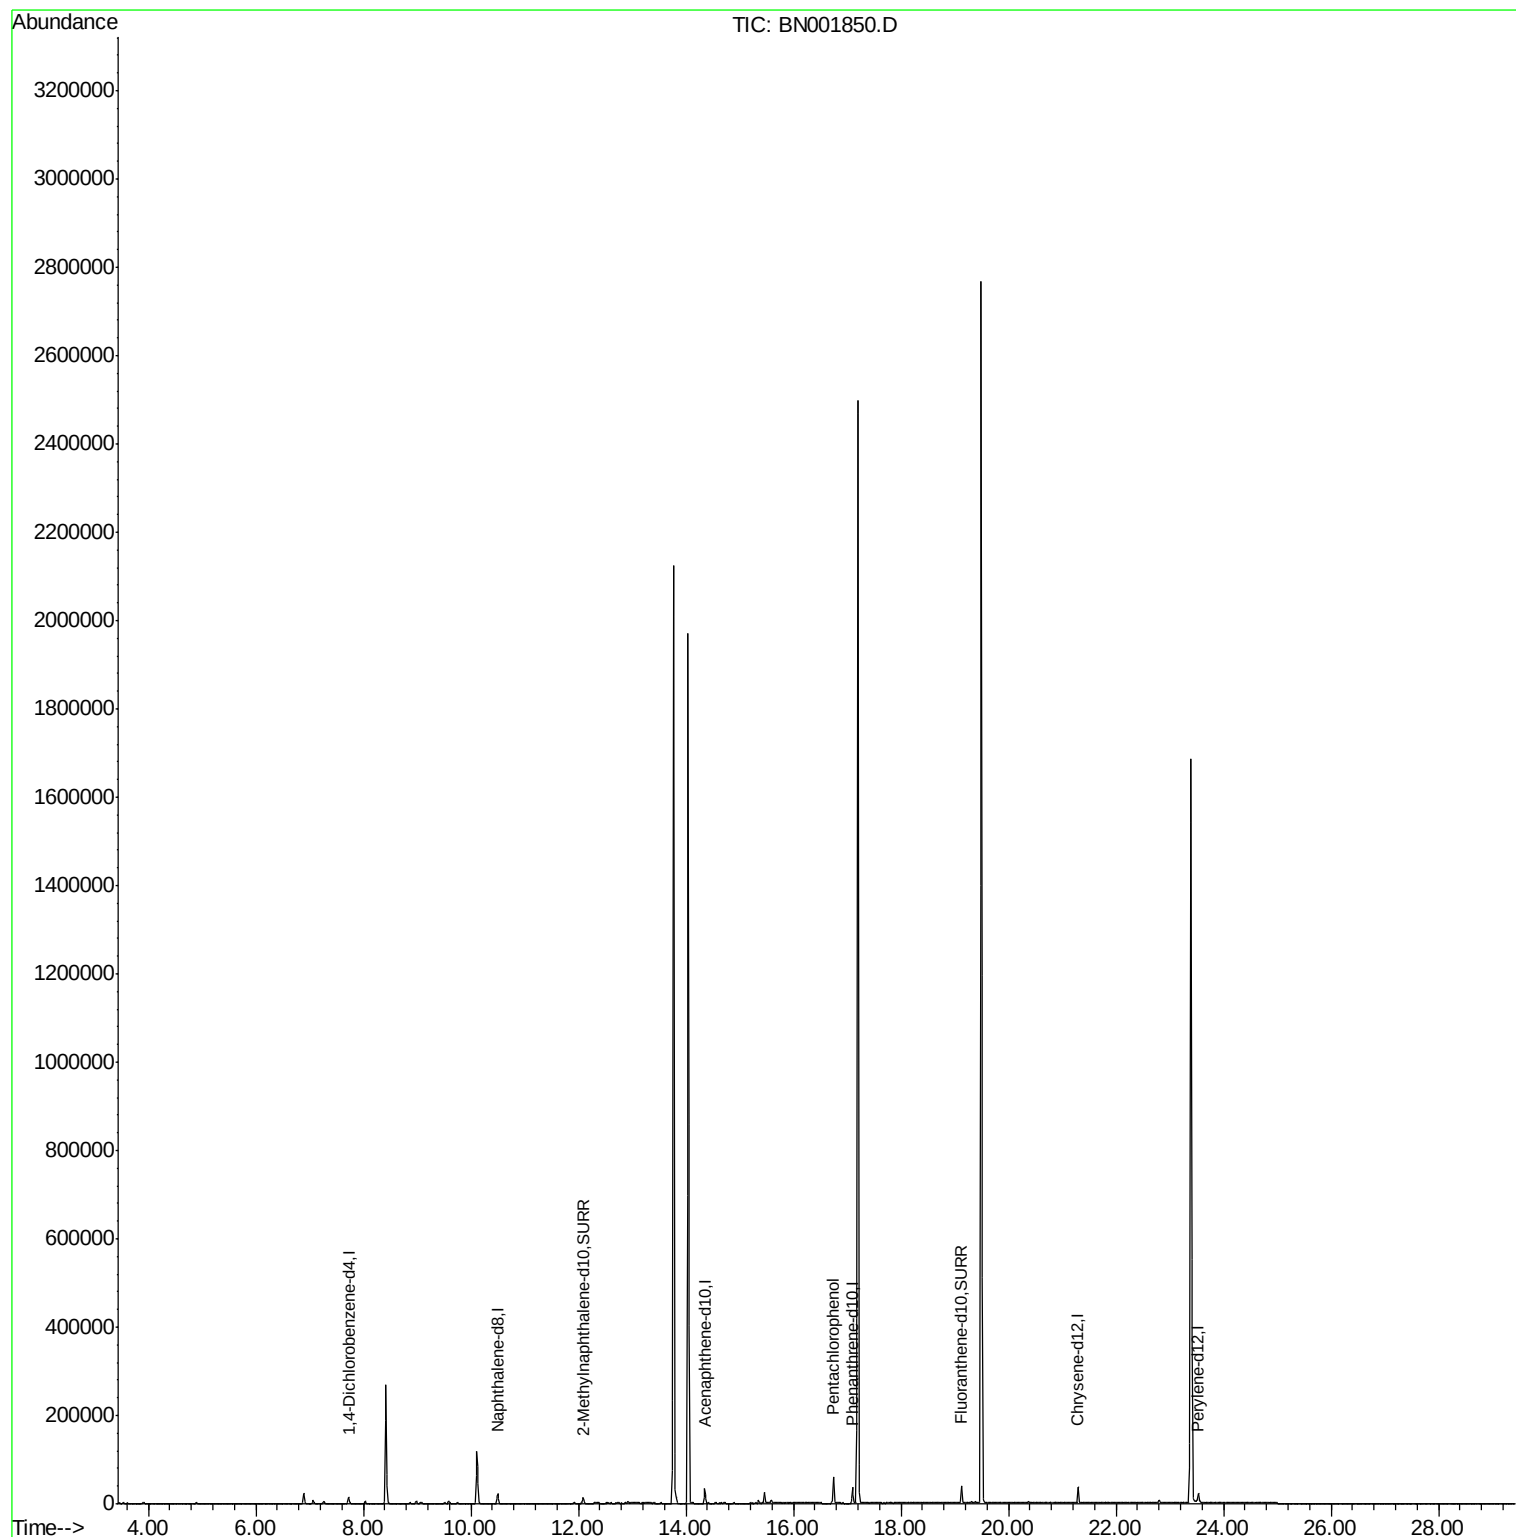

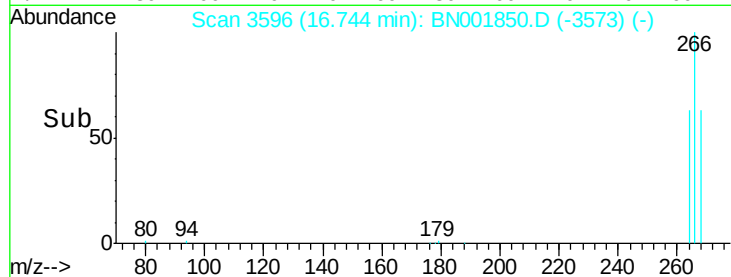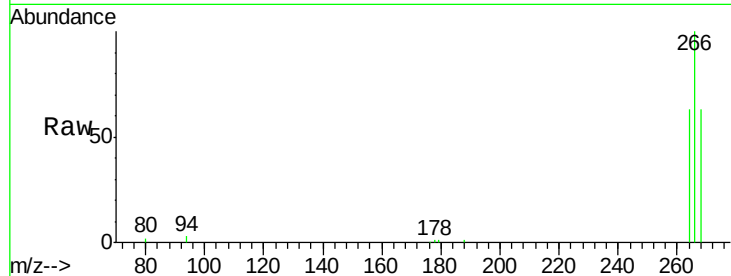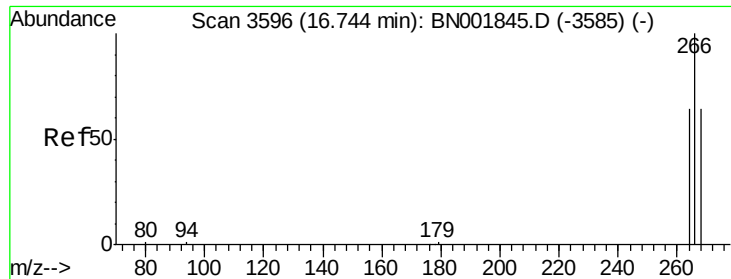

#11
 Pentachlorophenol
 Concen: 5.003 ng/ul m
 RT: 16.74 min Scan# 3596
 Delta R.T. -0.00 min
 Lab File: BN001850.D
 Acq: 13 Jun 2018 19:18

Instrument :
 BNA_N
 ClientSampleId :
 DAWS9

Tgt Ion	Ratio	Resp Lower	Resp Upper
266	100		
264	0.0	47.9	71.9#
268	0.0	49.8	74.8#

Manual Integrations
 APPROVED

Sohil
 6/14/2018 3:57:35 PM

