

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN061318\
 Data File : BN001853.D
 Acq On : 13 Jun 2018 21:04
 Operator : JU/SJ
 Sample : J3375-15
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DAWT2

Manual Integrations
 APPROVED

Sohil
 6/14/2018 3:57:38 PM

Quant Time: Jun 14 05:56:57 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN061318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 13 12:02:12 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	8133	0.40	ng/ul	0.00
2) Naphthalene-d8	10.50	136	35005	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.36	164	28967	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.10	188	40120m	0.40	ng/ul	0.00
16) Chrysene-d12	21.29	240	22774m	0.40	ng/ul	0.00
20) Perylene-d12	23.53	264	18504m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.09	152	25780	0.47	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	33792m	0.28	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.55	128	54083	0.599	ng/ul#	91
9) Fluorene	15.41	166	13848	0.114	ng/ul#	73
12) Phenanthrene	17.12	178	25792m	0.215	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN061318\
Data File : BN001853.D
Acq On : 13 Jun 2018 21:04
Operator : JU/SJ
Sample : J3375-15
Misc :
ALS Vial : 21 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
DAWT2

Manual Integrations
APPROVED

Sohil
6/14/2018 3:57:38 PM

Quant Time: Jun 14 05:56:57 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN061318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 13 12:02:12 2018
Response via : Initial Calibration

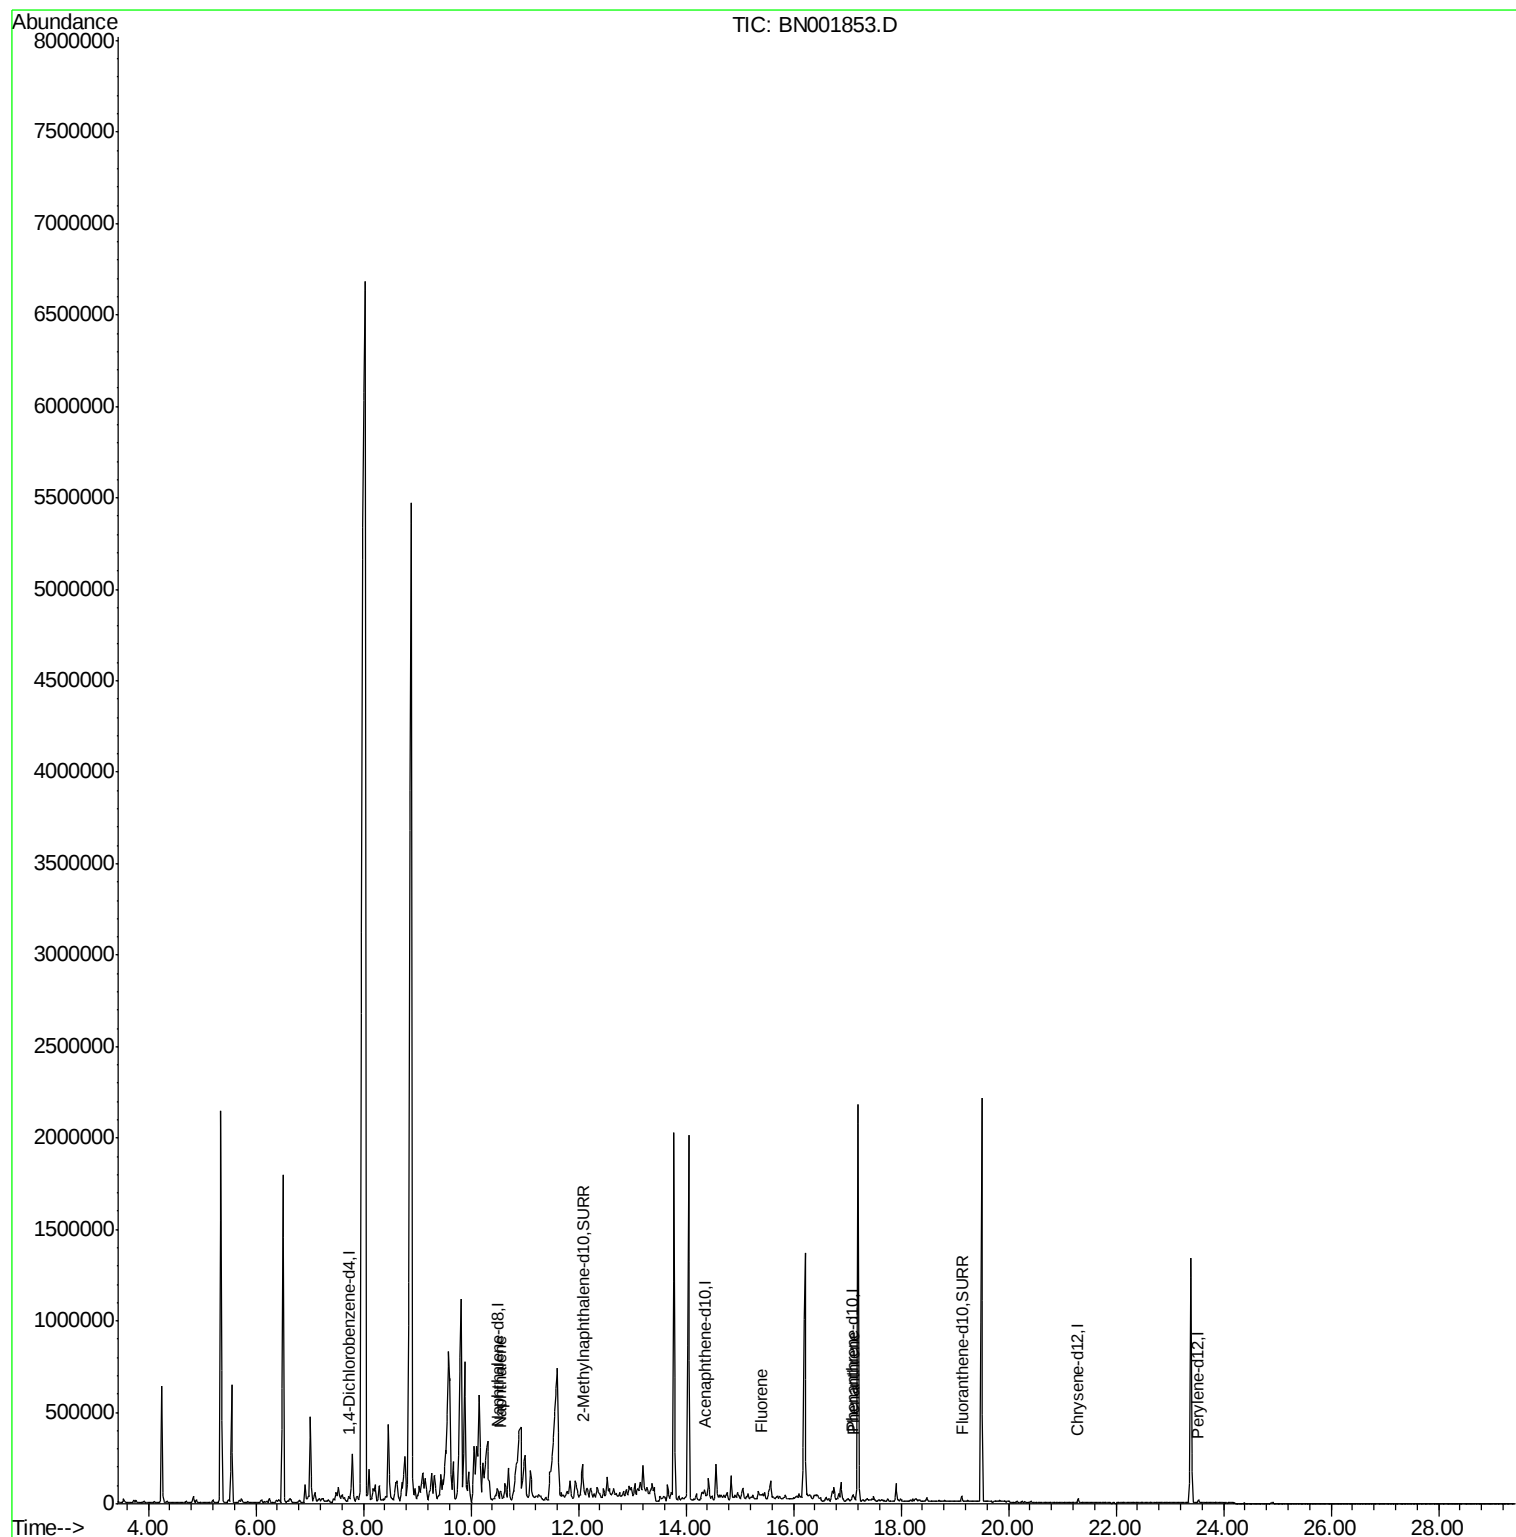

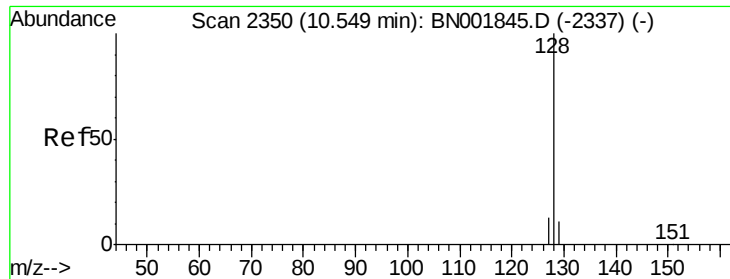

#3

Naphthalene

Concen: 0.599 ng/ul

RT: 10.55 min Scan# 2351

Delta R.T. 0.01 min

Lab File: BN001853.D

Acq: 13 Jun 2018 21:04

Instrument :

BNA_N





ClientSampleId :

DAWT2

Tgt Ion:	128	Resp:	54083
Ion Ratio	Lower	Upper	
128	100		
129	17.3	8.0	12.0#
127	15.9	12.0	18.0

Manual Integrations
APPROVED

Sohil
6/14/2018 3:57:38 PM

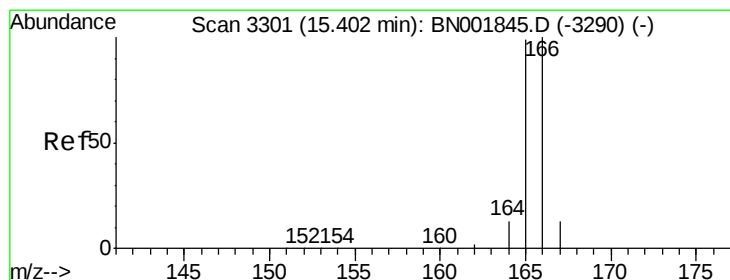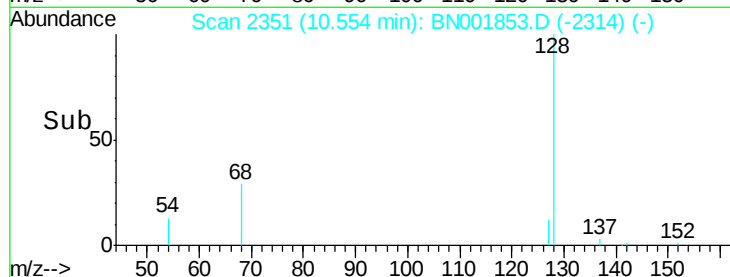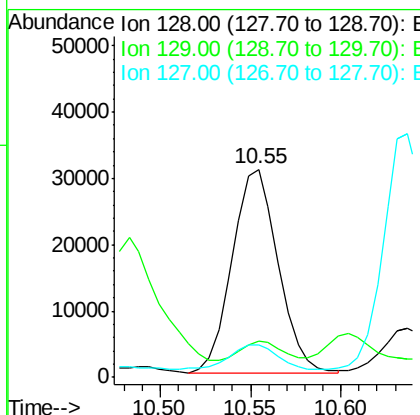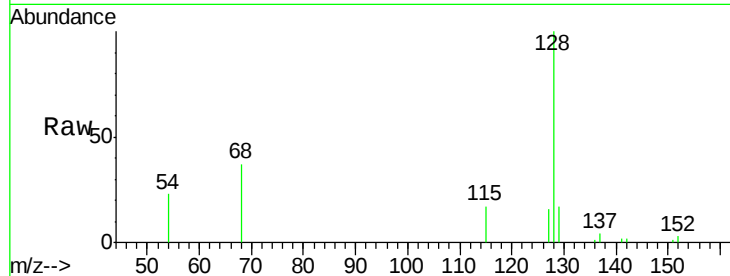

#9

Fluorene

Concen: 0.114 ng/ul




RT: 15.41 min Scan# 3302




Delta R.T. 0.00 min

Lab File: BN001853.D

Acq: 13 Jun 2018 21:04

Tgt Ion:	166	Resp:	13848
Ion Ratio	Lower	Upper	
166	100		
165	107.8	73.4	110.2
167	52.2	14.6	22.0#

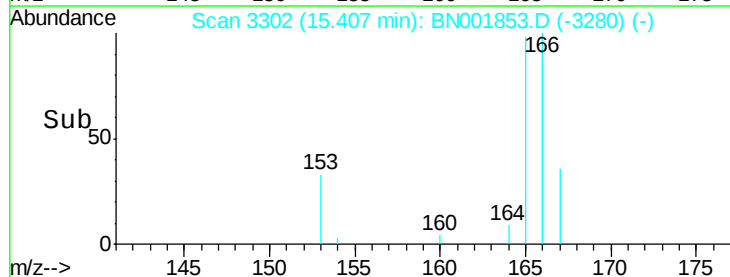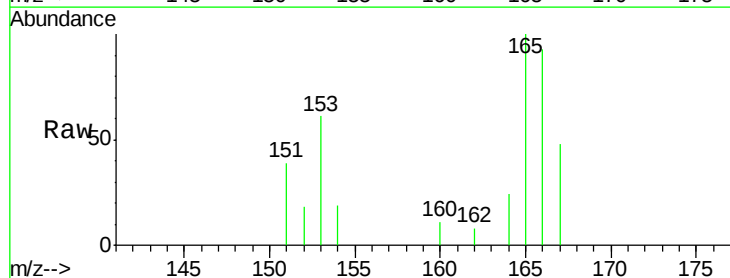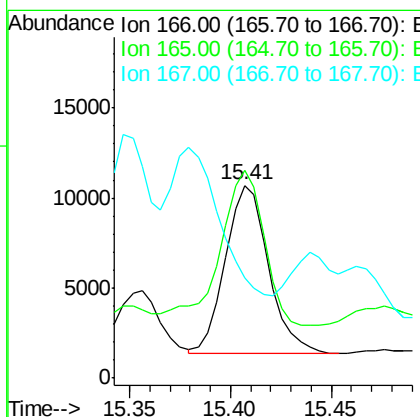

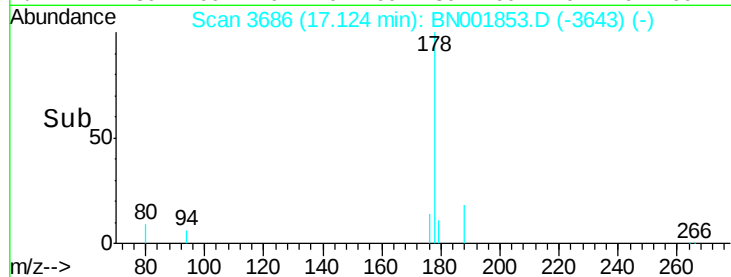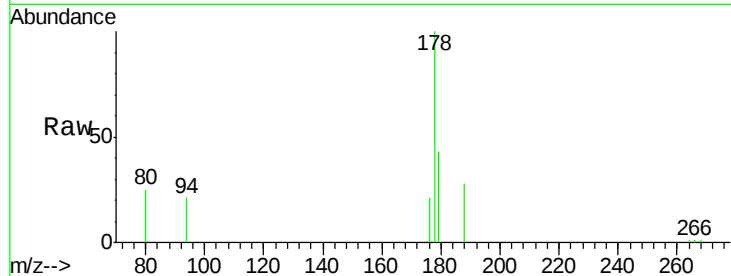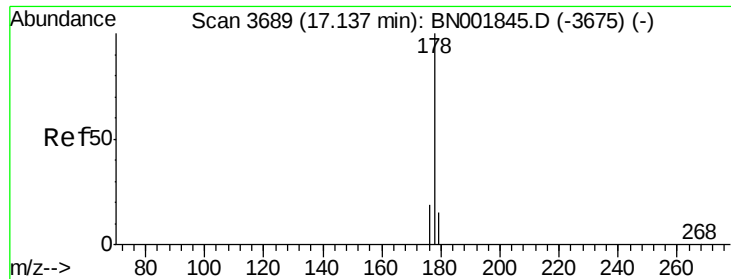

#12

Phenanthrene

Concen: 0.215 ng/ul m

RT: 17.12 min Scan# 3686

Delta R.T. -0.02 min

Lab File: BN001853.D

Acq: 13 Jun 2018 21:04

Instrument :

BNA_N

ClientSampleId :

DAWT2

Tgt Ion:178 Resp: 25792

Ion Ratio Lower Upper

178 100

179 42.7 18.4 27.6#

176 21.4 13.6 20.4#

Manual Integrations
APPROVED

Sohil
6/14/2018 3:57:38 PM

