

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN061318\
 Data File : BN001854.D
 Acq On : 13 Jun 2018 21:40
 Operator : JU/SJ
 Sample : J3375-16
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DAWT3

Manual Integrations
 APPROVED

Sohil
 6/14/2018 3:57:39 PM

Quant Time: Jun 14 05:59:31 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN061318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 13 12:02:12 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	8622	0.40	ng/ul	0.00
2) Naphthalene-d8	10.50	136	35021	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.35	164	22495	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.10	188	41627m	0.40	ng/ul	0.00
16) Chrysene-d12	21.30	240	24400m	0.40	ng/ul	0.00
20) Perylene-d12	23.53	264	20476m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.09	152	24404	0.44	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	36387m	0.29	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.55	128	9938	0.110	ng/ul#	70
9) Fluorene	15.41	166	5520	0.058	ng/ul#	74

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN061318\
Data File : BN001854.D
Acq On : 13 Jun 2018 21:40
Operator : JU/SJ
Sample : J3375-16
Misc :
ALS Vial : 22 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
DAWT3

Quant Time: Jun 14 05:59:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN061318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 13 12:02:12 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
6/14/2018 3:57:39 PM

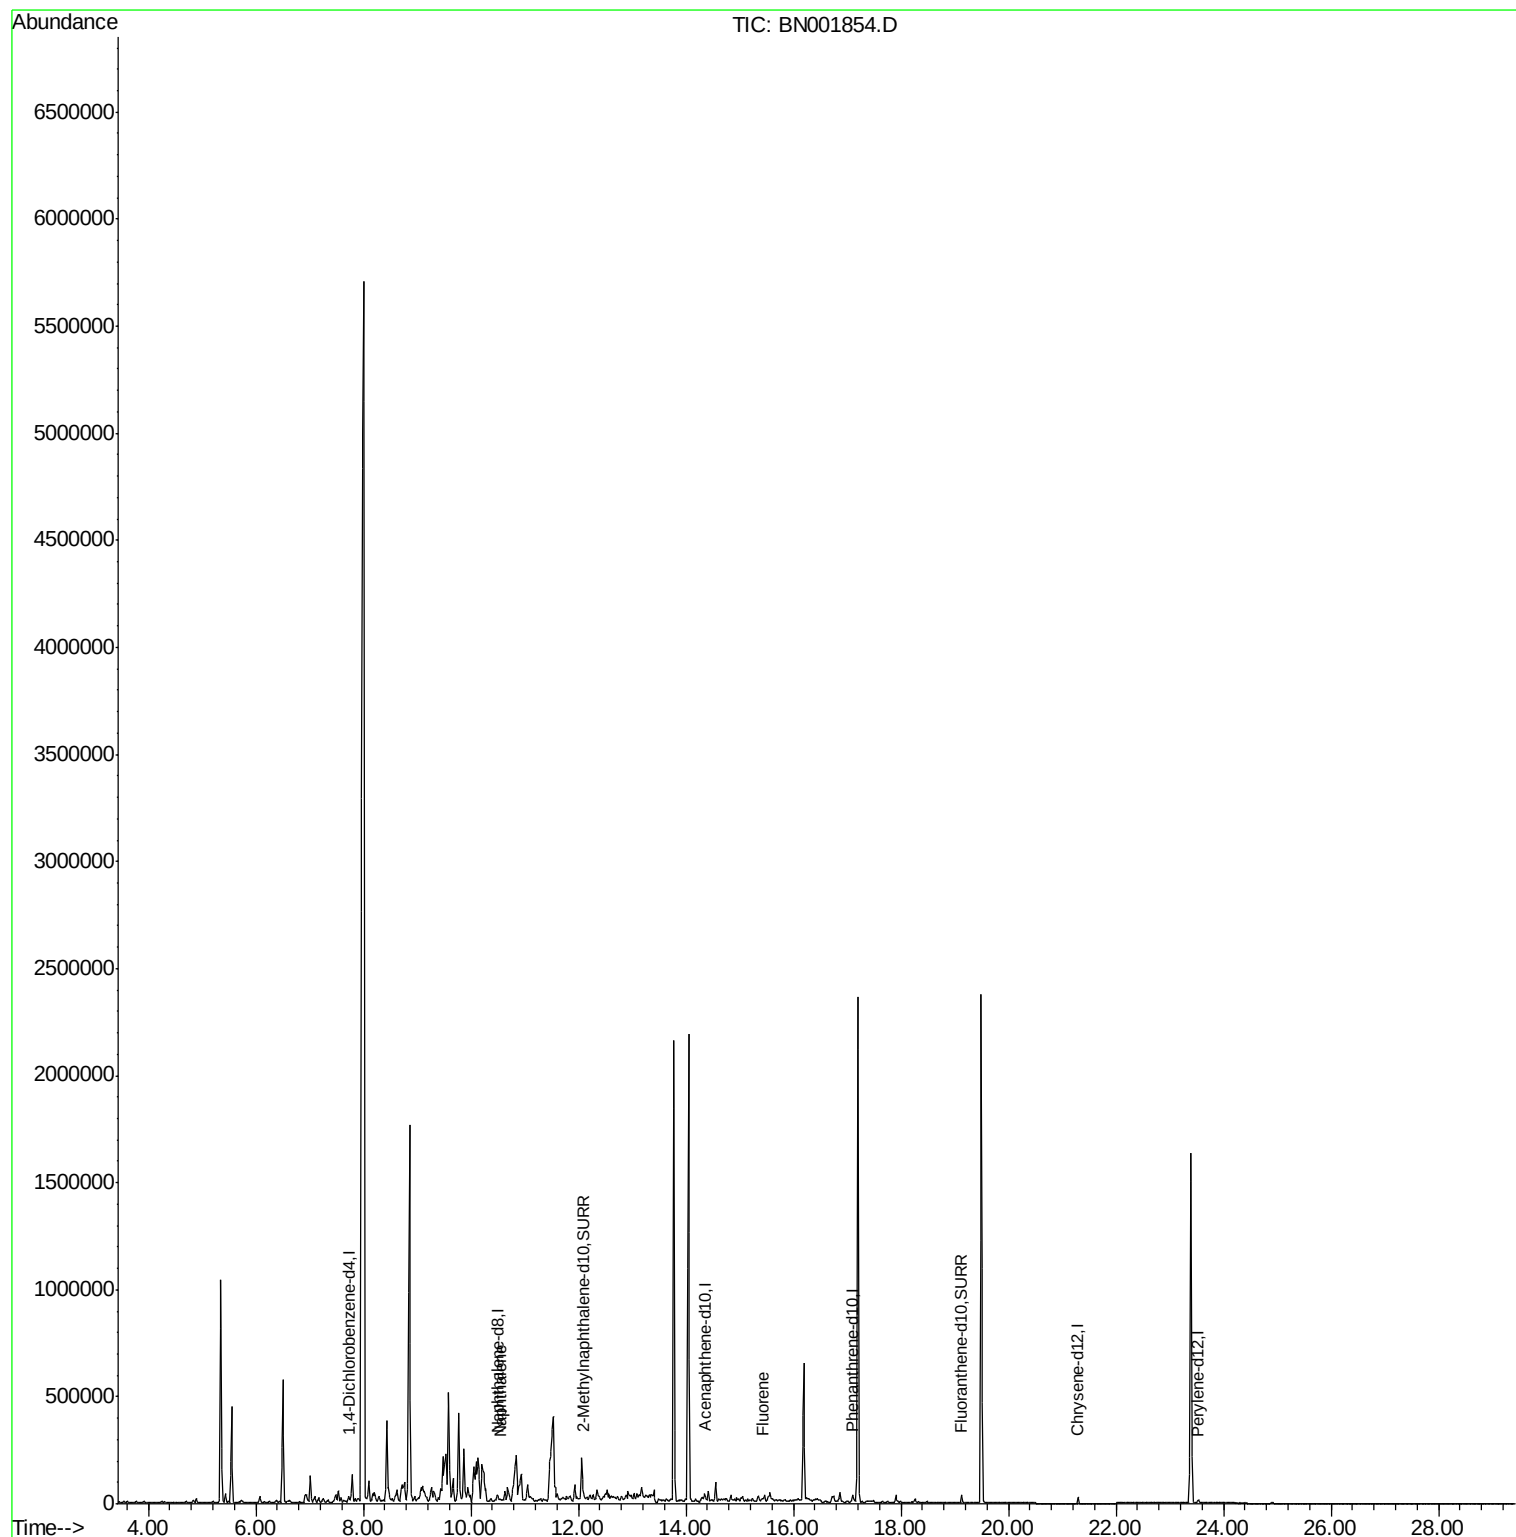

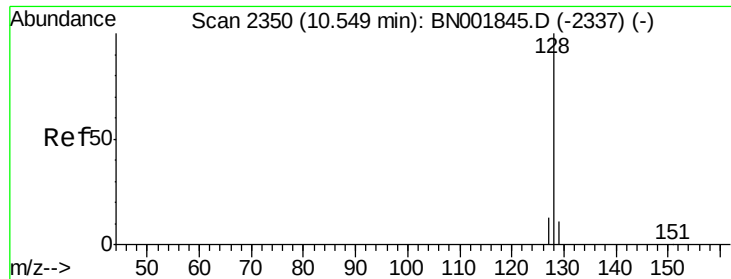

#3

Naphthalene

Concen: 0.110 ng/ul

RT: 10.55 min Scan# 2350

Delta R.T. -0.00 min

Lab File: BN001854.D

Acq: 13 Jun 2018 21:40

Instrument :

BNA_N





ClientSampleId :

DAWT3

Tgt Ion:	128	Resp:	9938
Ion Ratio	Lower	Upper	
128	100		
129	27.7	8.0	12.0#
127	22.4	12.0	18.0#

Manual Integrations
APPROVED

Sohil
6/14/2018 3:57:39 PM

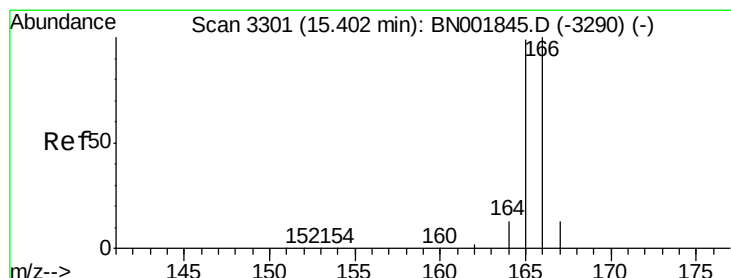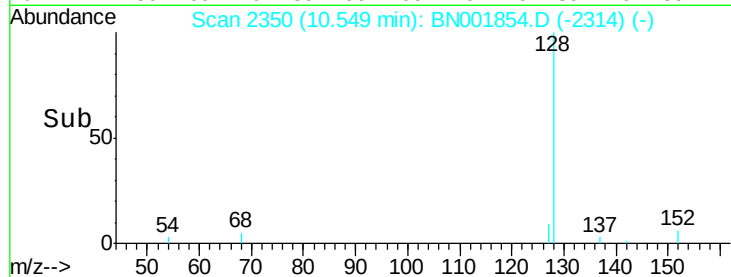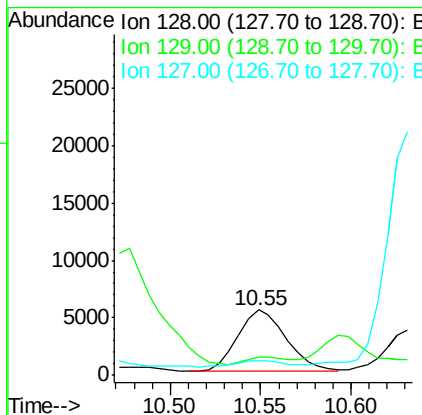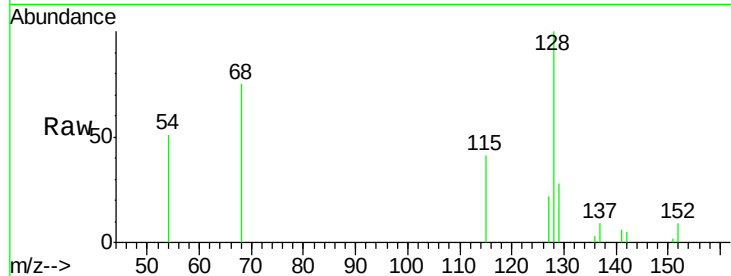

#9

Fluorene

Concen: 0.058 ng/ul

RT: 15.41 min Scan# 3302

Delta R.T. -0.00 min

Lab File: BN001854.D

Acq: 13 Jun 2018 21:40

Tgt Ion:	166	Resp:	5520
Ion Ratio	Lower	Upper	
166	100		
165	106.4	73.4	110.2
167	52.5	14.6	22.0#

