

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN061318\
 Data File : BN001859.D
 Acq On : 14 Jun 2018 00:36
 Operator : JU/SJ
 Sample : J3375-11DL 2X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DAWS8DL

Manual Integrations
 APPROVED

Sohil
 6/14/2018 3:57:44 PM

Quant Time: Jun 14 06:35:13 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN061318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 13 12:02:12 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	6436	0.40	ng/ul	0.00
2) Naphthalene-d8	10.49	136	26419	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.35	164	15625	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.09	188	32583m	0.40	ng/ul	0.00
16) Chrysene-d12	21.29	240	21522m	0.40	ng/ul	0.00
20) Perylene-d12	23.53	264	17838m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.09	152	8177	0.20	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	17135m	0.17	ng/ul	0.00
Target Compounds						
9) Fluorene	15.40	166	1363	0.021	ng/ul#	84
11) Pentachlorophenol	16.74	266	23080m	3.741	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN061318\
Data File : BN001859.D
Acq On : 14 Jun 2018 00:36
Operator : JU/SJ
Sample : J3375-11DL 2X
Misc :
ALS Vial : 27 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
DAWS8DL

Manual Integrations
APPROVED

Sohil
6/14/2018 3:57:44 PM

Quant Time: Jun 14 06:35:13 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN061318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 13 12:02:12 2018
Response via : Initial Calibration

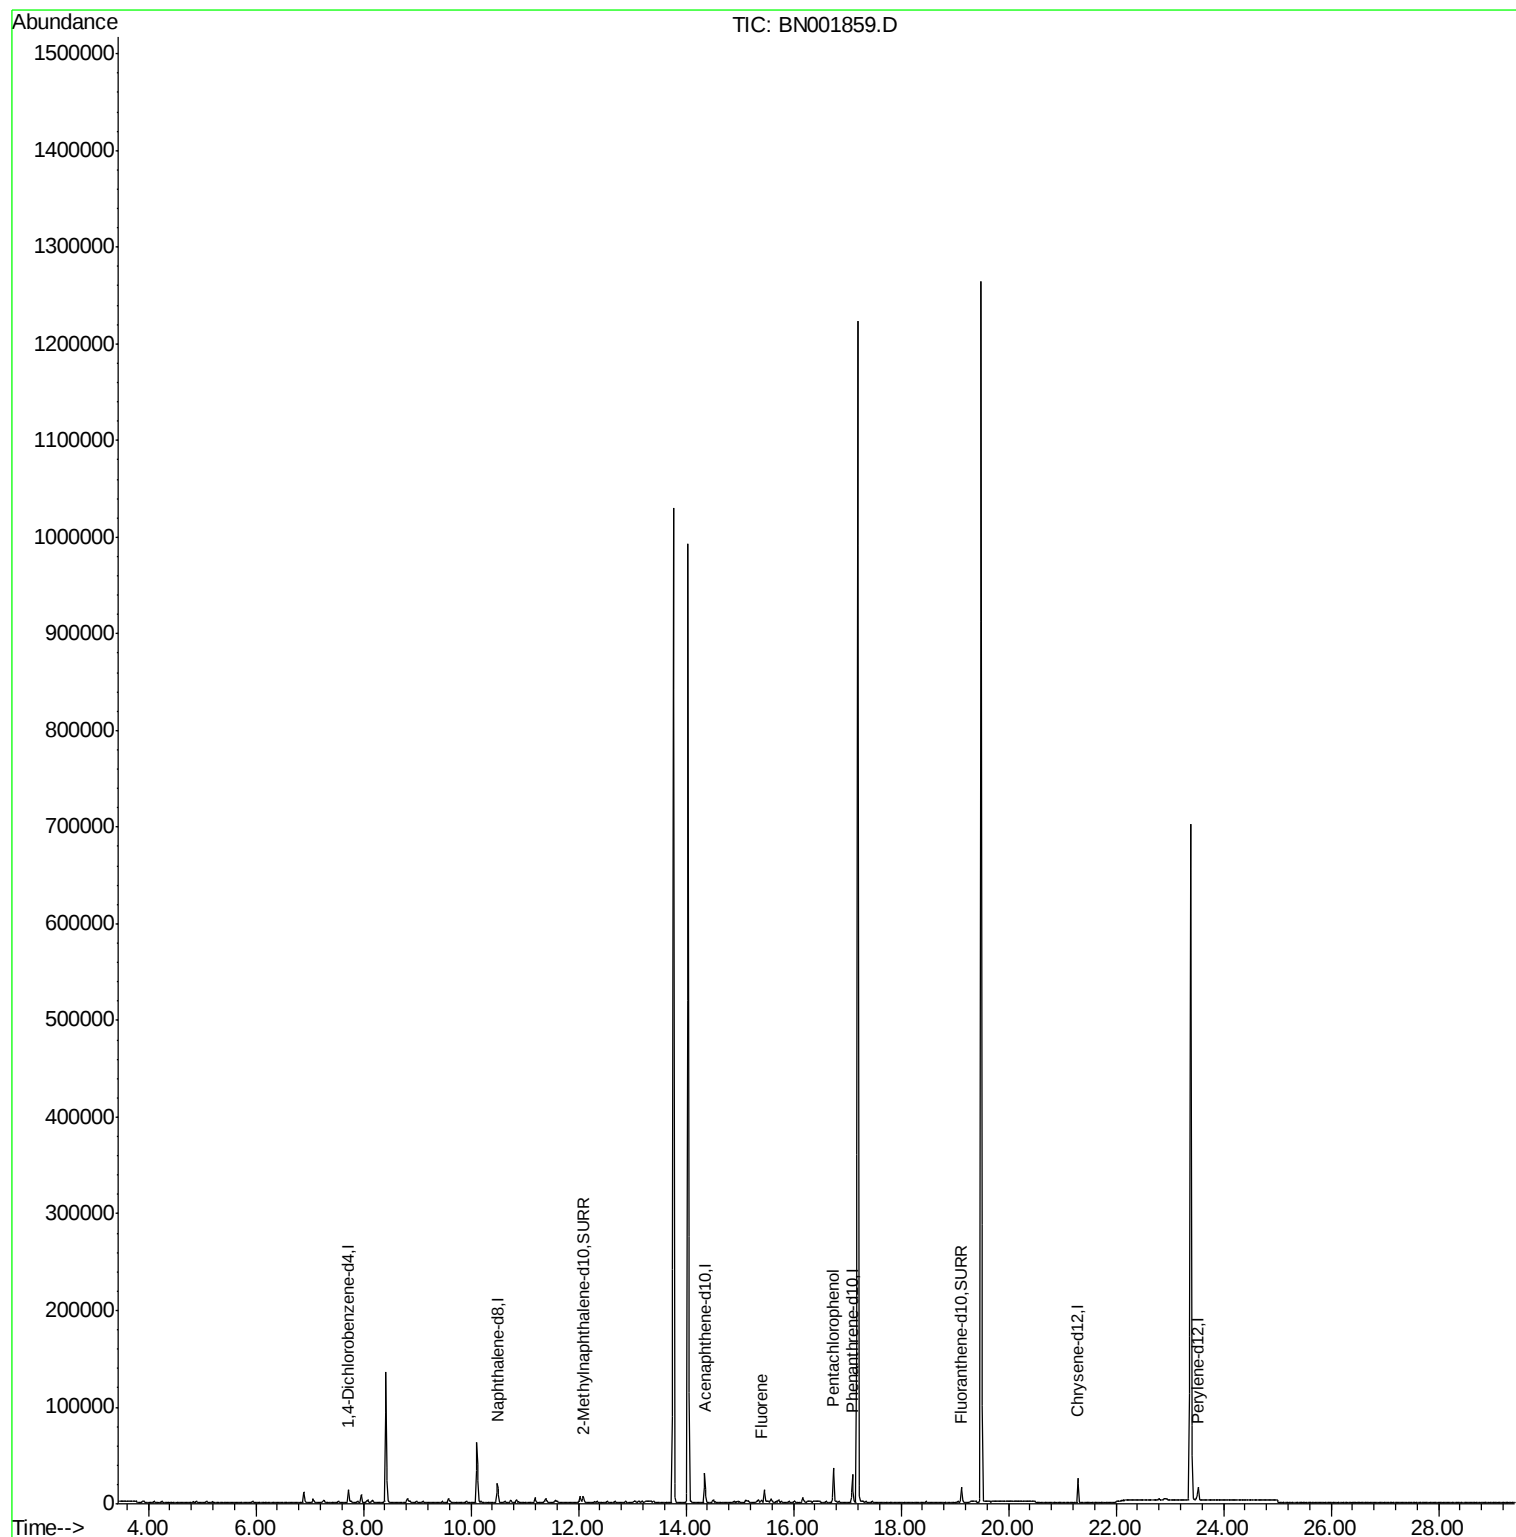

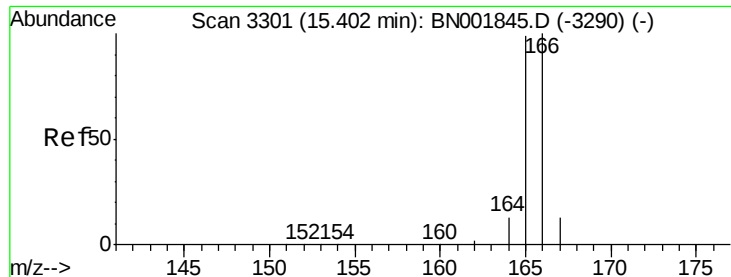





#9
Fluorene
 Concen: 0.021 ng/ul
 RT: 15.40 min Scan# 3301
 Delta R.T. -0.00 min
 Lab File: BN001859.D
 Acq: 14 Jun 2018 00:36

Instrument :
 BNA_N
 ClientSampled :
 DAWS8DL

Tgt Ion	Ratio	Lower	Upper
166	100		
165	105.5	73.4	110.2
167	29.7	14.6	22.0

Manual Integrations
 APPROVED

Sohil
 6/14/2018 3:57:44 PM

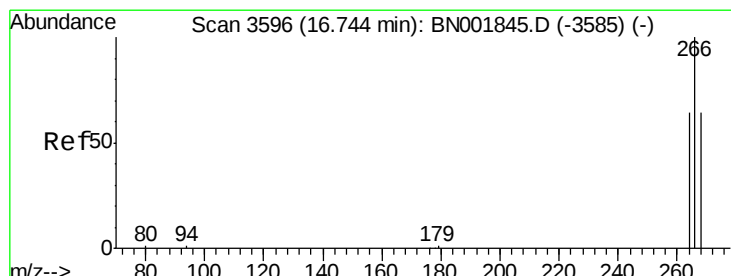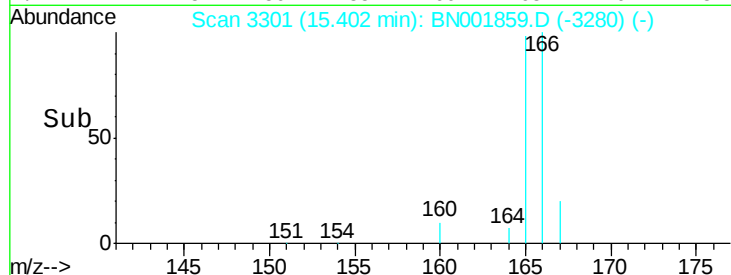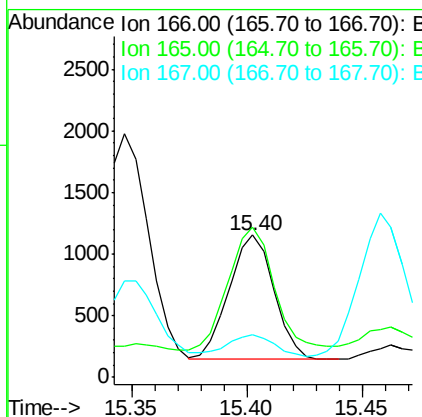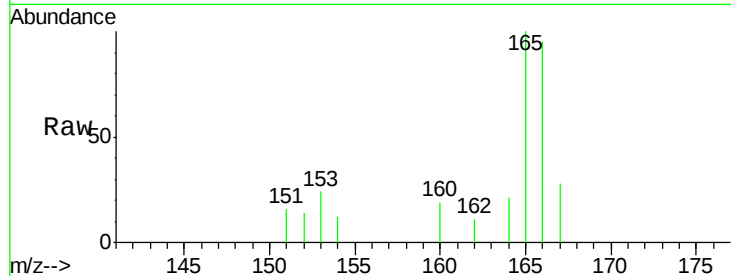

#11
Pentachlorophenol
 Concen: 3.741 ng/ul m
 RT: 16.74 min Scan# 3596
 Delta R.T. -0.00 min
 Lab File: BN001859.D
 Acq: 14 Jun 2018 00:36

Tgt Ion	Ratio	Lower	Upper
266	100		
264	0.0	47.9	71.9
268	0.0	49.8	74.8

