

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061323\
 Data File : BN025813.D
 Acq On : 13 Jun 2023 19:46
 Operator : MA/JU
 Sample : PB153100BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK100

Quant Time: Jun 13 23:49:26 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN060923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jun 10 02:01:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.005	152	7396	0.400	ng/ul	0.00
4) Naphthalene-d8	10.820	136	22726	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.640	164	13350	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.386	188	25274	0.400	ng/ul	0.00
17) Chrysene-d12	21.568	240	11486	0.400	ng/ul	0.00
23) Perylene-d12	24.047	264	13194	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.348	96	44640	6.139	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.409	152	10529	0.365	ng/ul	0.00
18) Fluoranthene-d10	19.406	212	16892	0.466	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.773	202	2866	0.053	ng/ul#	1
26) Benzo(a)pyrene	23.889	252	4580	0.100	ng/ul#	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061323\
Data File : BN025813.D
Acq On : 13 Jun 2023 19:46
Operator : MA/JU
Sample : PB153100BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK100

Quant Time: Jun 13 23:49:26 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 10 02:01:49 2023
Response via : Initial Calibration

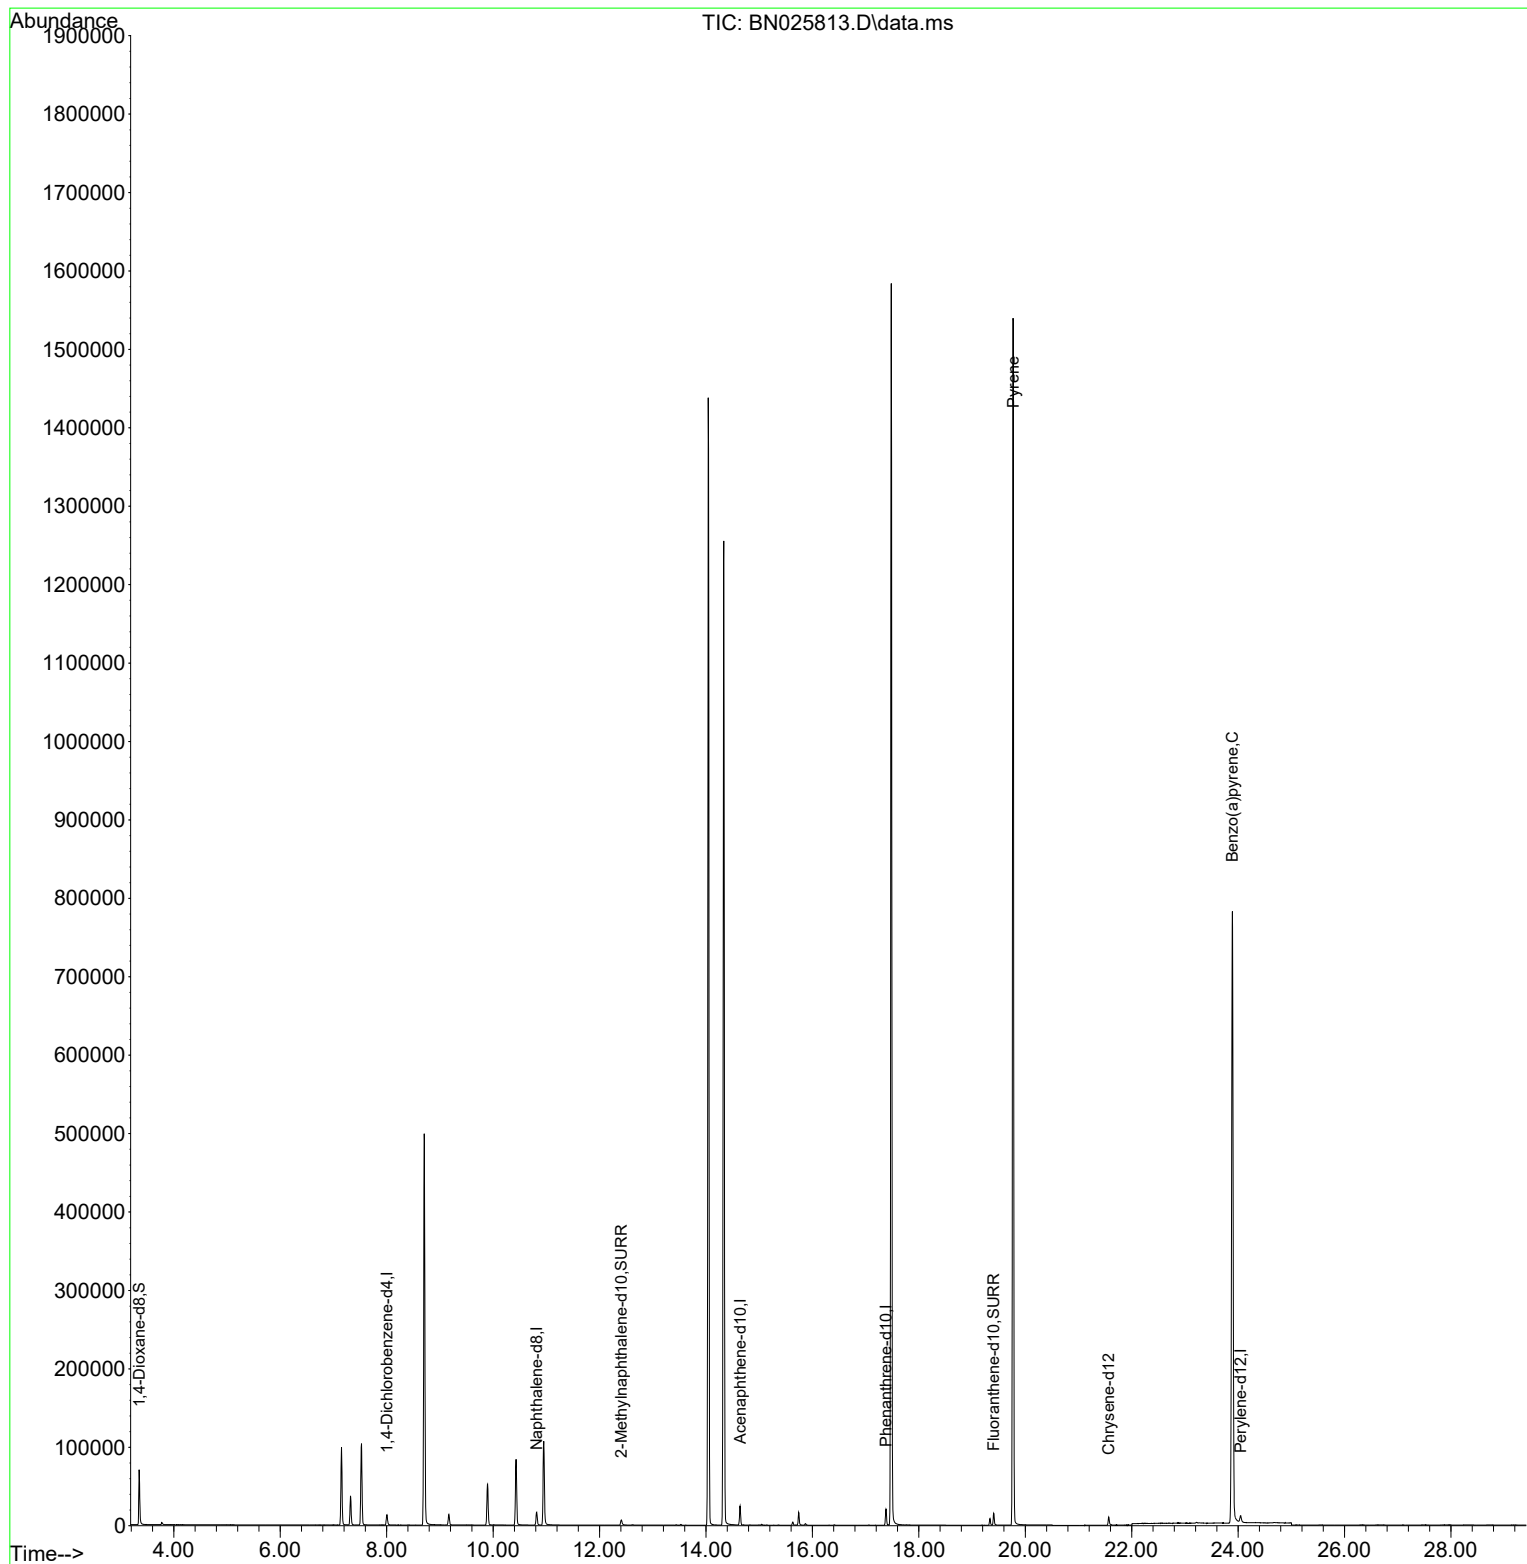

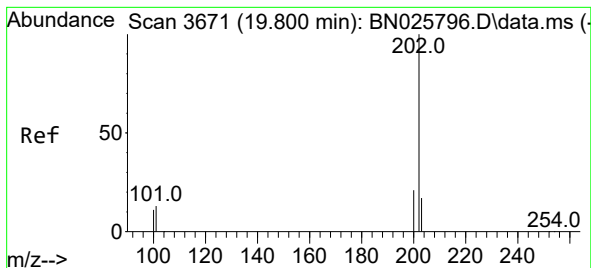

#20

Pyrene

Concen: 0.053 ng/ul

RT: 19.773 min Scan# 3

Delta R.T. -0.032 min

Lab File: BN025813.D

Acq: 13 Jun 2023 19:46

Instrument :

BNA_N

ClientSampleId :

SBLK100





Tgt Ion:202 Resp: 2866

Ion Ratio Lower Upper

202 100

101 168.5 10.4 15.6#

100 1240.5 8.8 13.2#

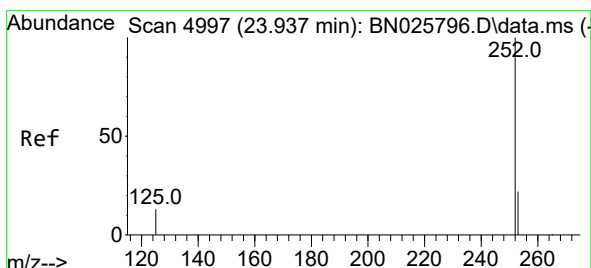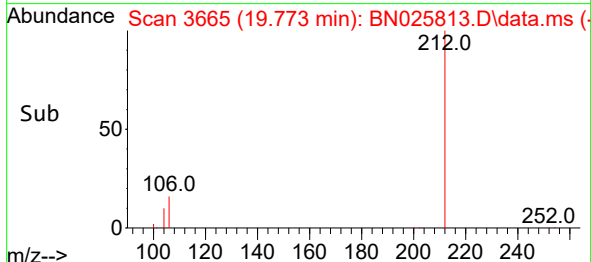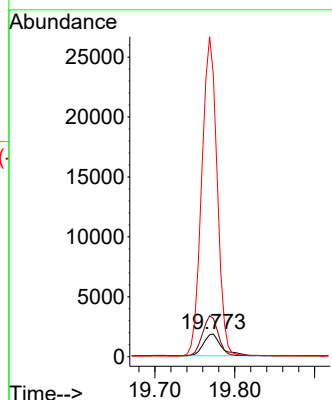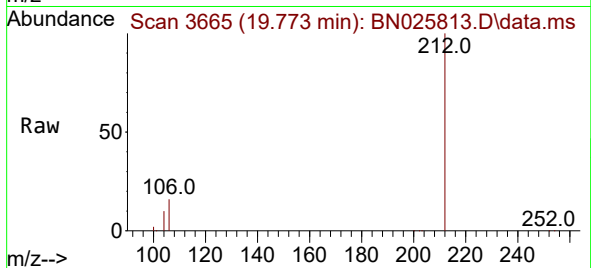

#26

Benzo(a)pyrene

Concen: 0.100 ng/ul

RT: 23.889 min Scan# 4980

Delta R.T. -0.054 min

Lab File: BN025813.D

Acq: 13 Jun 2023 19:46

Tgt Ion:252 Resp: 4580

Ion Ratio Lower Upper

252 100

253 54.6 25.8 38.8#

125 36.9 13.5 20.3#

