

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN061419\
 Data File : BN006328.D
 Acq On : 14 Jun 2019 10:29
 Operator : JU/SJ
 Sample : K3213-17DL 5X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB8K8DL

Manual Integrations
 APPROVED

mohammad
 6/17/2019 8:28:33 AM

Quant Time: Jun 14 16:41:16 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 13 11:20:30 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	5445	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	20740	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.29	164	9930	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	18437	0.40	ng/ul	0.00
16) Chrysene-d12	21.27	240	13793	0.40	ng/ul	0.00
20) Perylene-d12	23.50	264	13923m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	1793	0.06	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	3916	0.08	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	16.71	266	2267	0.484	ng/ul	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN061419\
Data File : BN006328.D
Acq On : 14 Jun 2019 10:29
Operator : JU/SJ
Sample : K3213-17DL 5X
Misc :
ALS Vial : 4 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
DB8K8DL

Manual Integrations
APPROVED

mohammad
6/17/2019 8:28:33 AM

Quant Time: Jun 14 16:41:16 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 11:20:30 2019
Response via : Initial Calibration

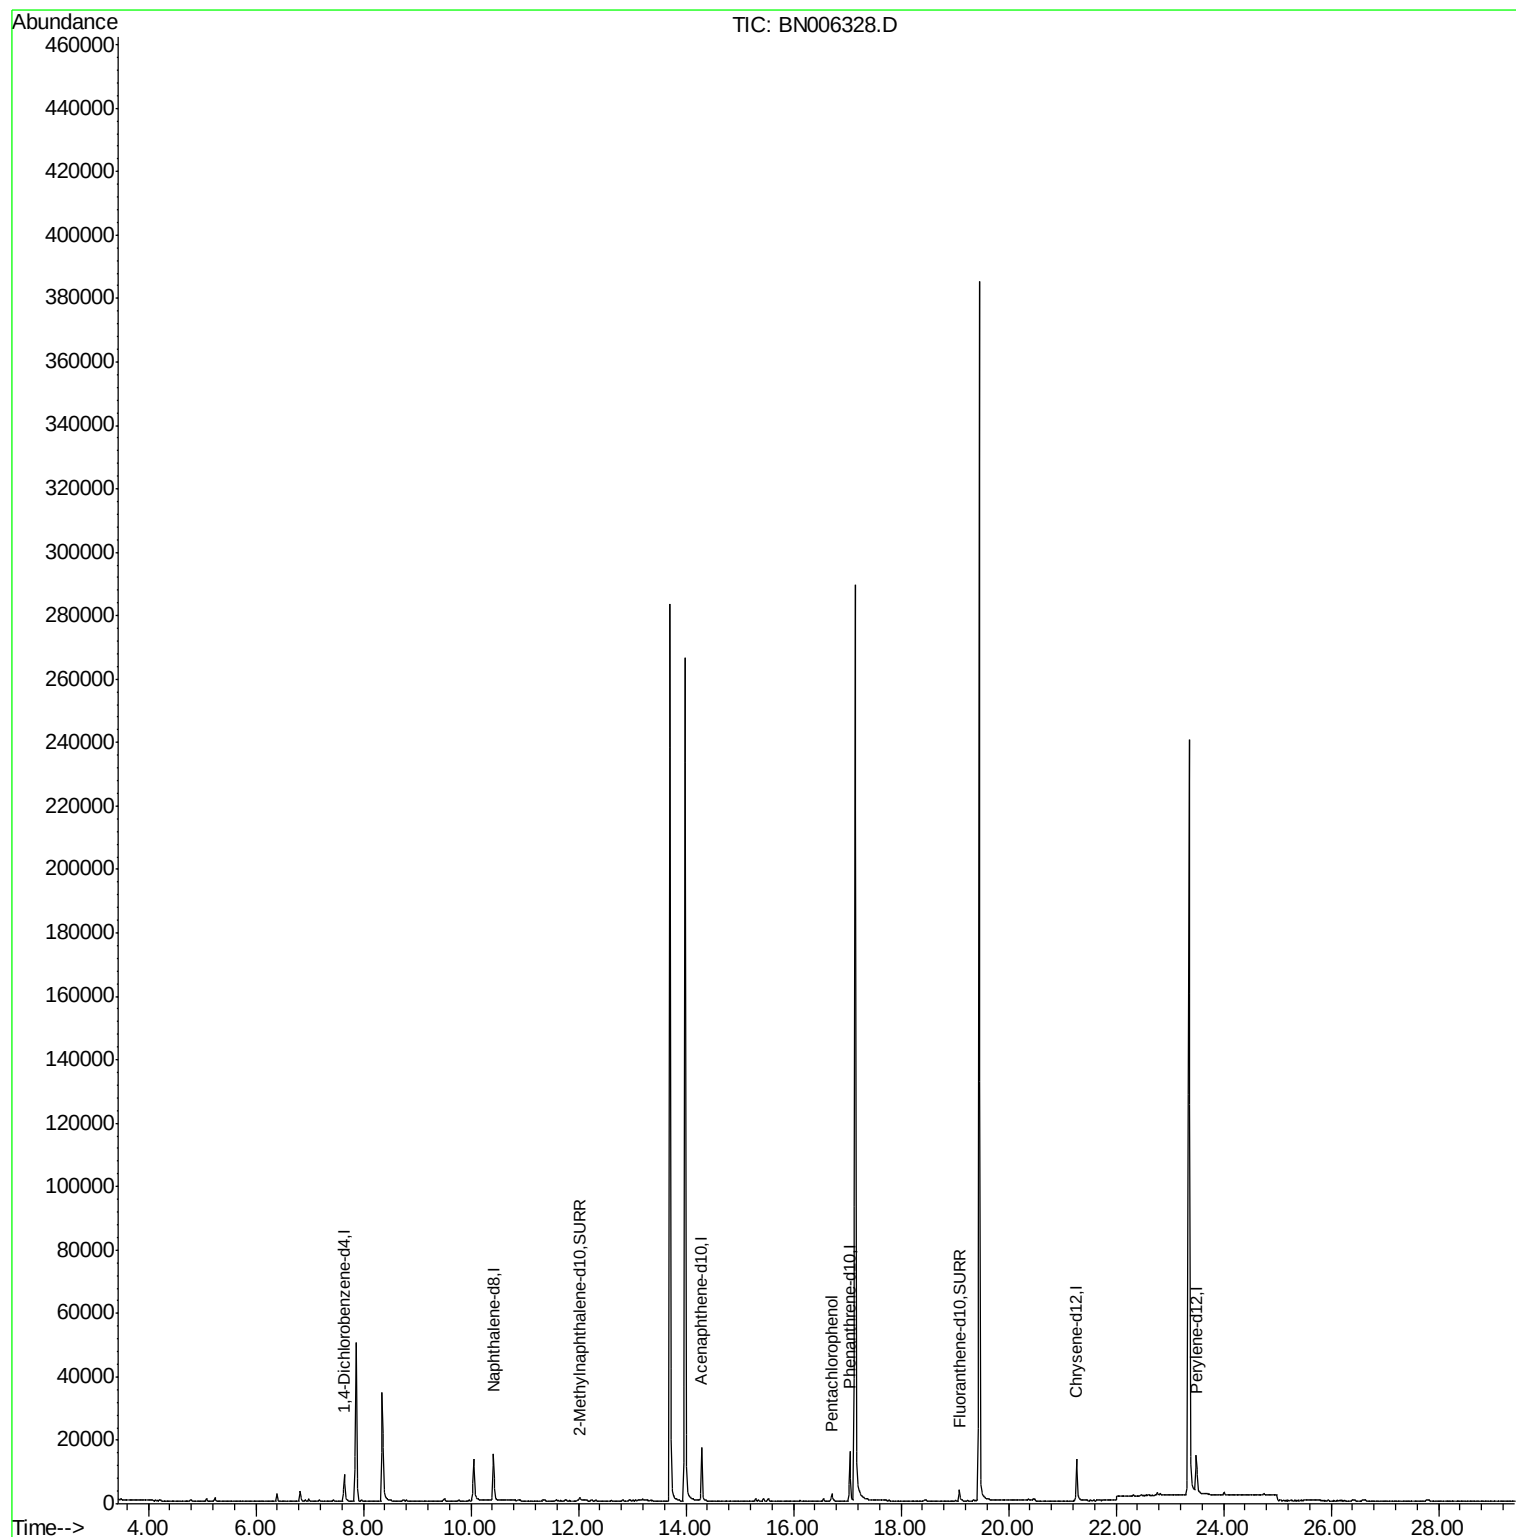

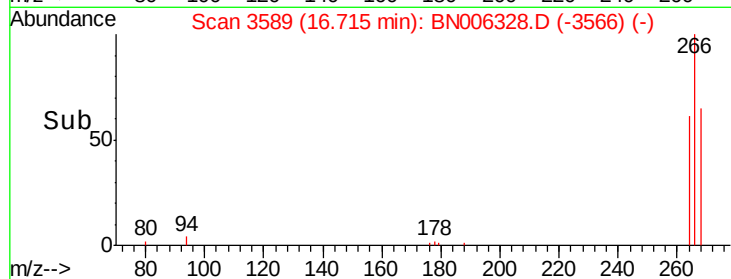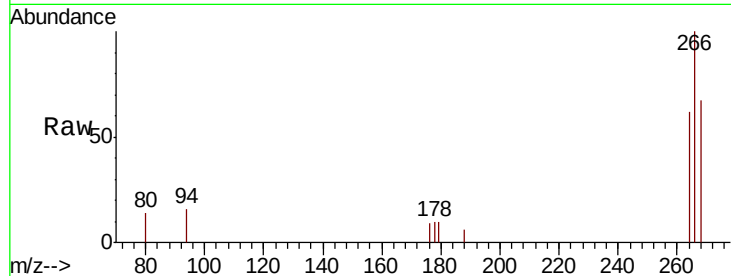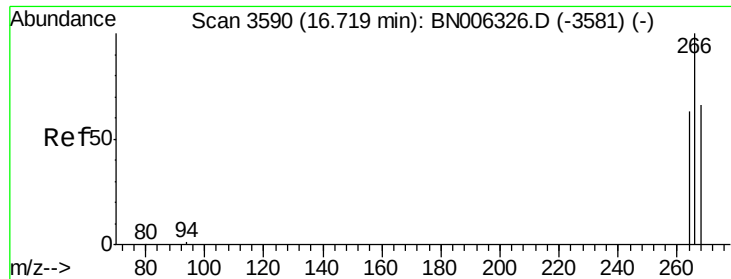

#11

Pentachlorophenol

Concen: 0.484 ng/ul

RT: 16.71 min Scan# 3589

Delta R.T. -0.00 min

Lab File: BN006328.D

Acq: 14 Jun 2019 10:29

Instrument :

BNA_N

ClientSampleId :

DB8K8DL

Tgt Ion	Ratio	Lower	Upper
266	100		
264	61.8	50.3	75.5
268	64.0	51.3	76.9

Manual Integrations
APPROVED

mohammad
6/17/2019 8:28:33 AM

