
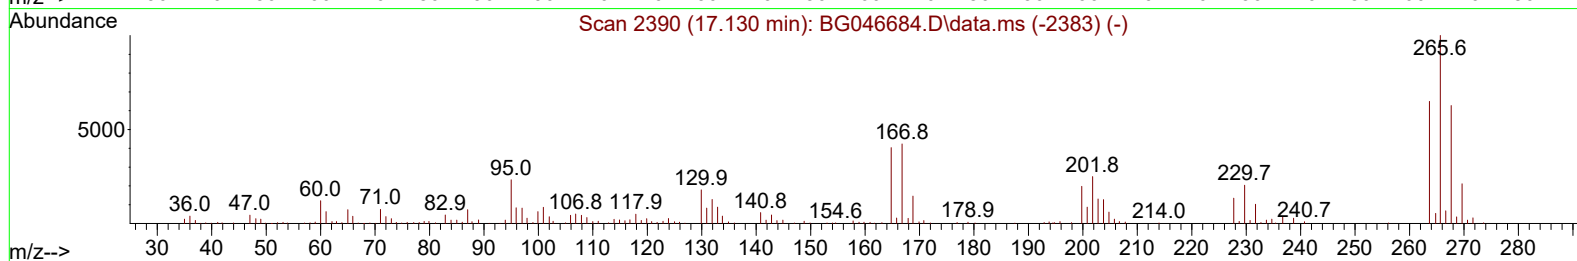
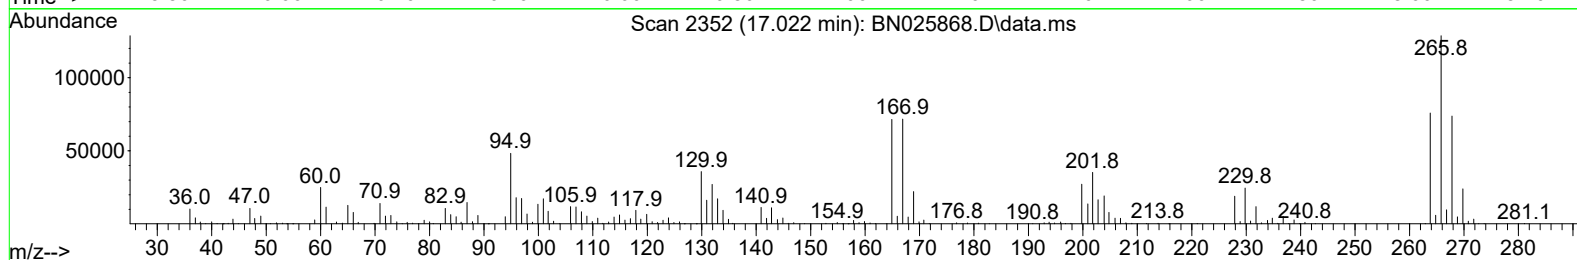


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061523\
 Data File : BN025868.D
 Acq On : 15 Jun 2023 21:45
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 04:37:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 16 04:35:40 2023
 Response via : Initial Calibration

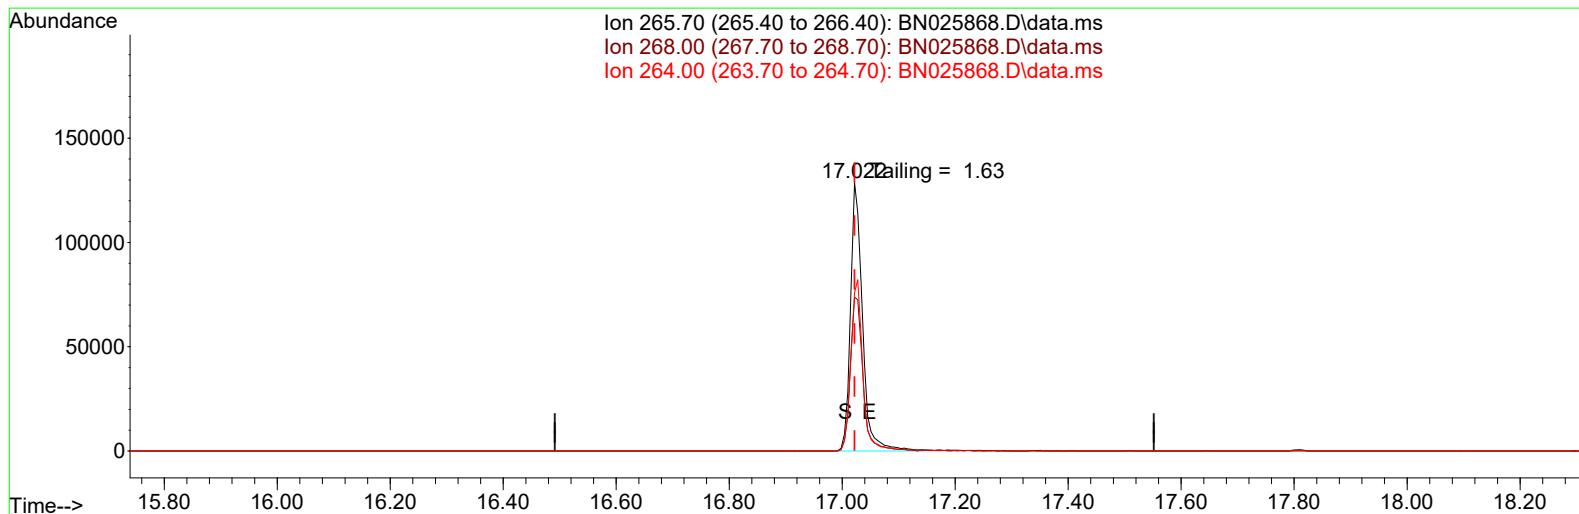

TIC: BN025868.D\data.ms

(70) Pentachlorophenol (C)




17.022min (-0.000) 12874.97 ng

response 191672

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	57.35
264.00	61.60	58.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061523\
Data File : BN025868.D
Acq On : 15 Jun 2023 21:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 04:37:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 16 04:35:40 2023
Response via : Initial Calibration

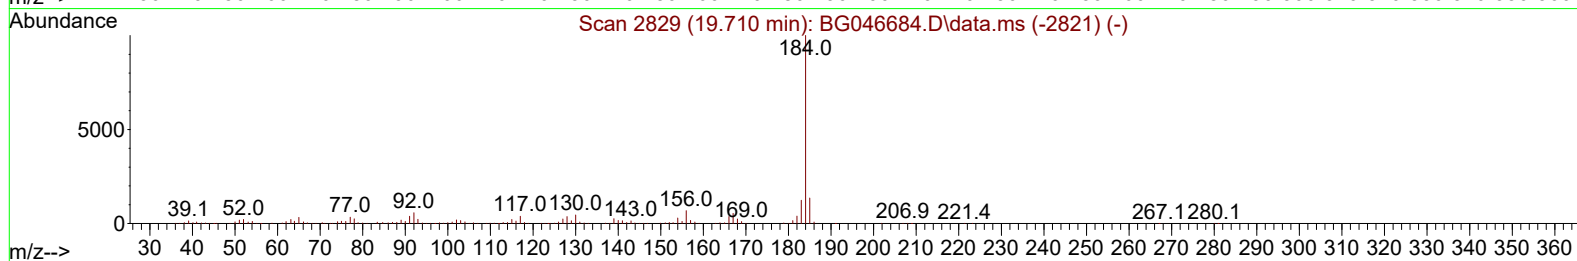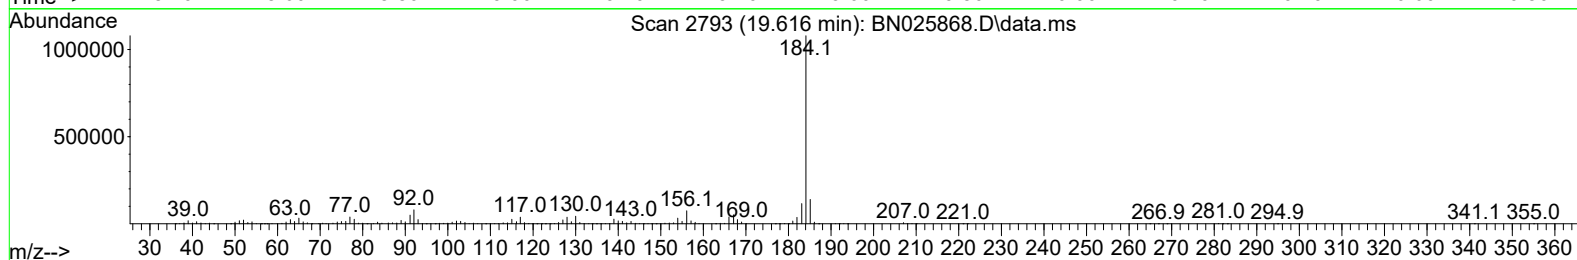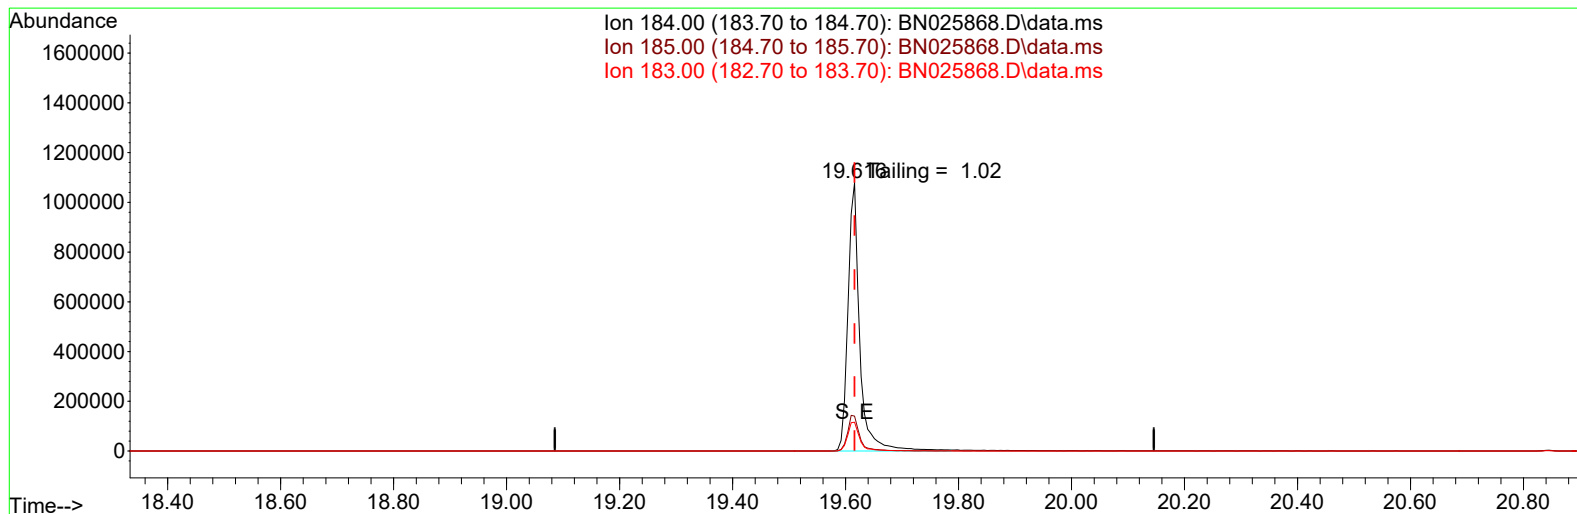

TIC: BN025868.D\data.ms

(77) Benzidine

19.616min (-0.000) 0.00 ng

response 1570155

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	12.99
183.00	13.20	10.75
0.00	0.00	0.00