
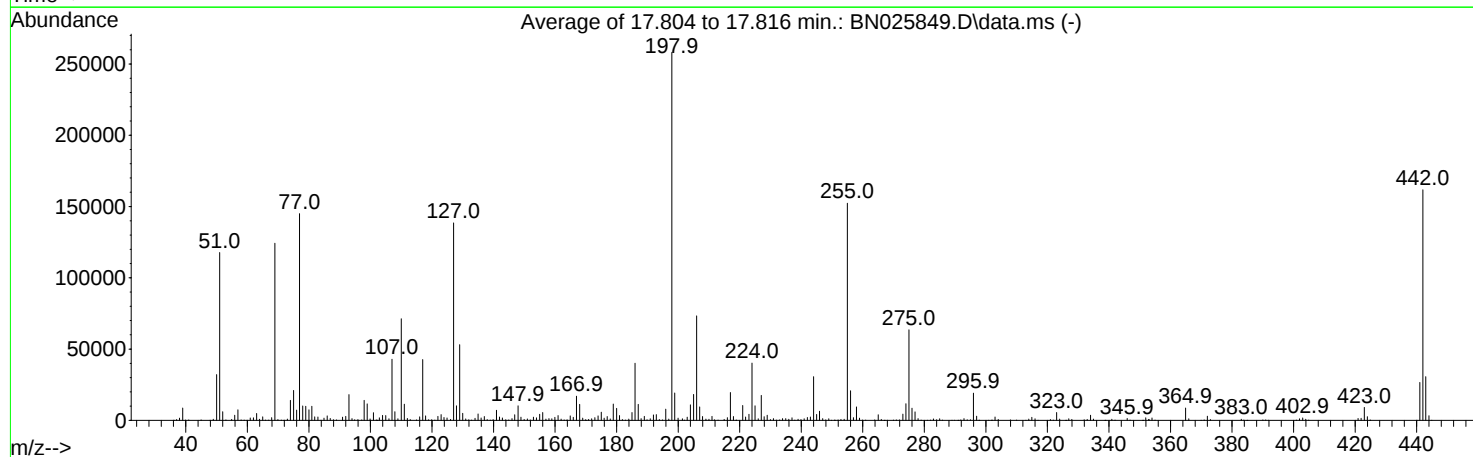


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061523\
 Data File : BN025849.D
 Acq On : 15 Jun 2023 09:29
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN053123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 16 01:41:46 2023

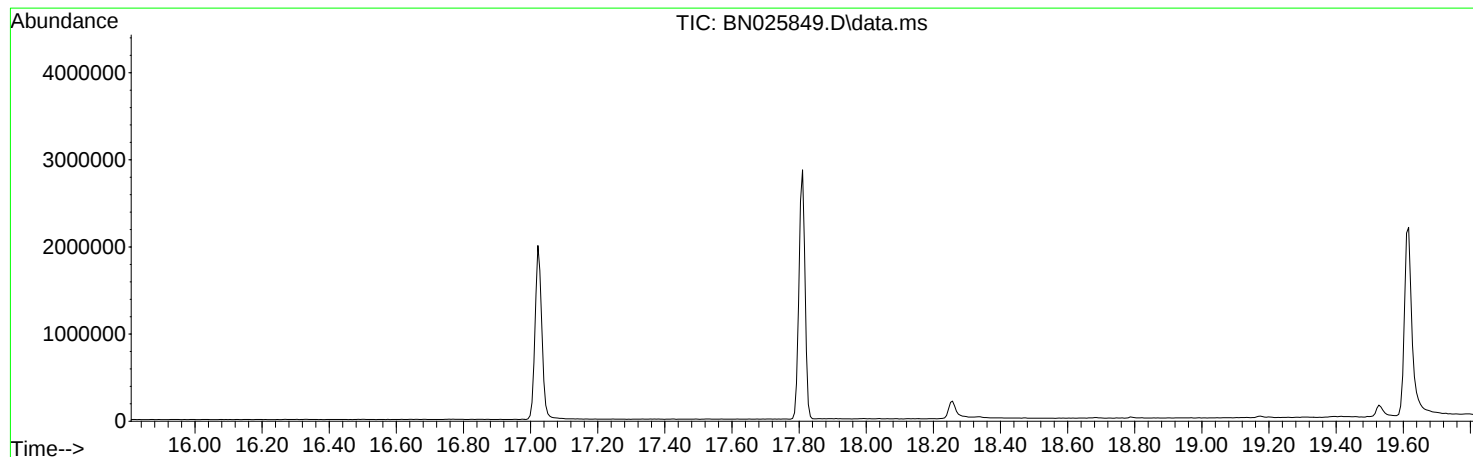

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.6	117700	PASS
68	69	0.00	2	1.6	1945	PASS
69	198	0.00	100	48.2	124259	PASS
70	69	0.00	2	0.4	540	PASS
127	198	10	80	53.7	138541	PASS
197	198	0.00	2	0.3	853	PASS
198	198	100	100	100.0	258048	PASS
199	198	5	9	7.5	19261	PASS
275	198	10	60	24.6	63531	PASS
365	198	1	100	3.4	8666	PASS
441	198	0.01	100	10.3	26592	PASS
442	442	50	100	100.0	161728	PASS
443	442	15	24	18.9	30592	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/15/2023	BNA_N	<u>BN025849.D</u>
Compound Name	Response	Retention Time
DDT	865049	20.845
DDD	18414	20.404
DDE	1109	19.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19523	884572	2.21

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061523\
Data File : BN025849.D
Acq On : 15 Jun 2023 09:29
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 16 04:35:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 16 04:35:40 2023
Response via : Initial Calibration

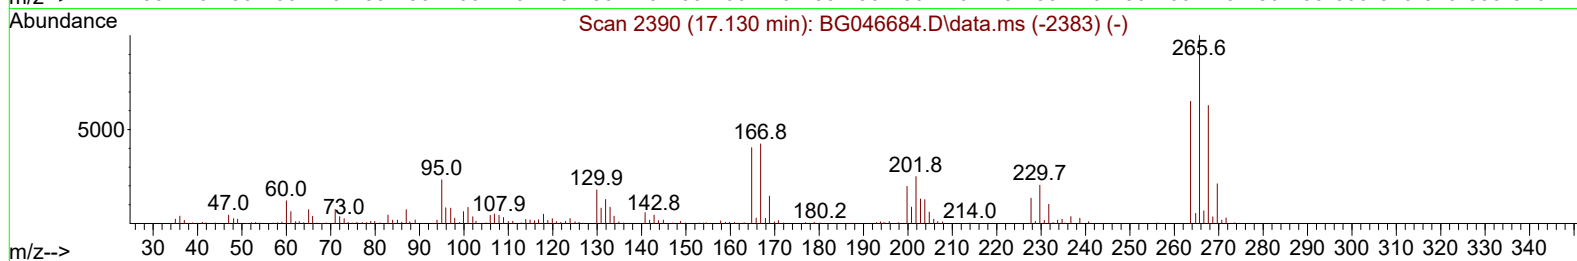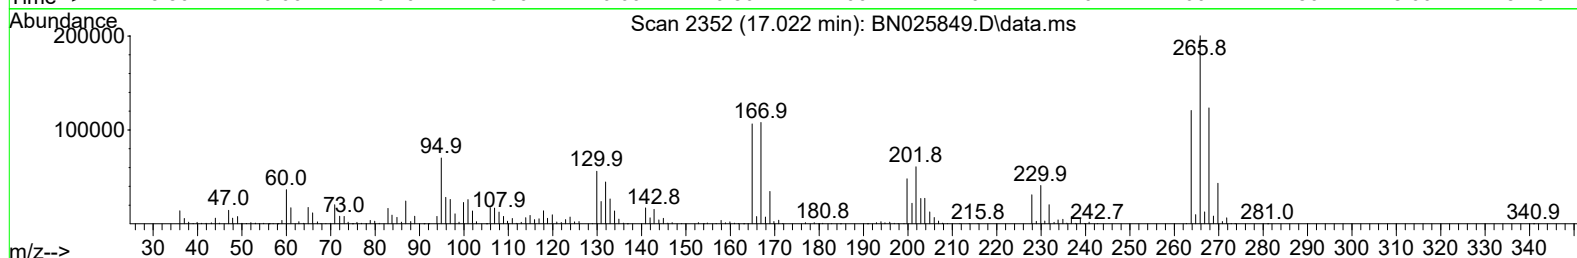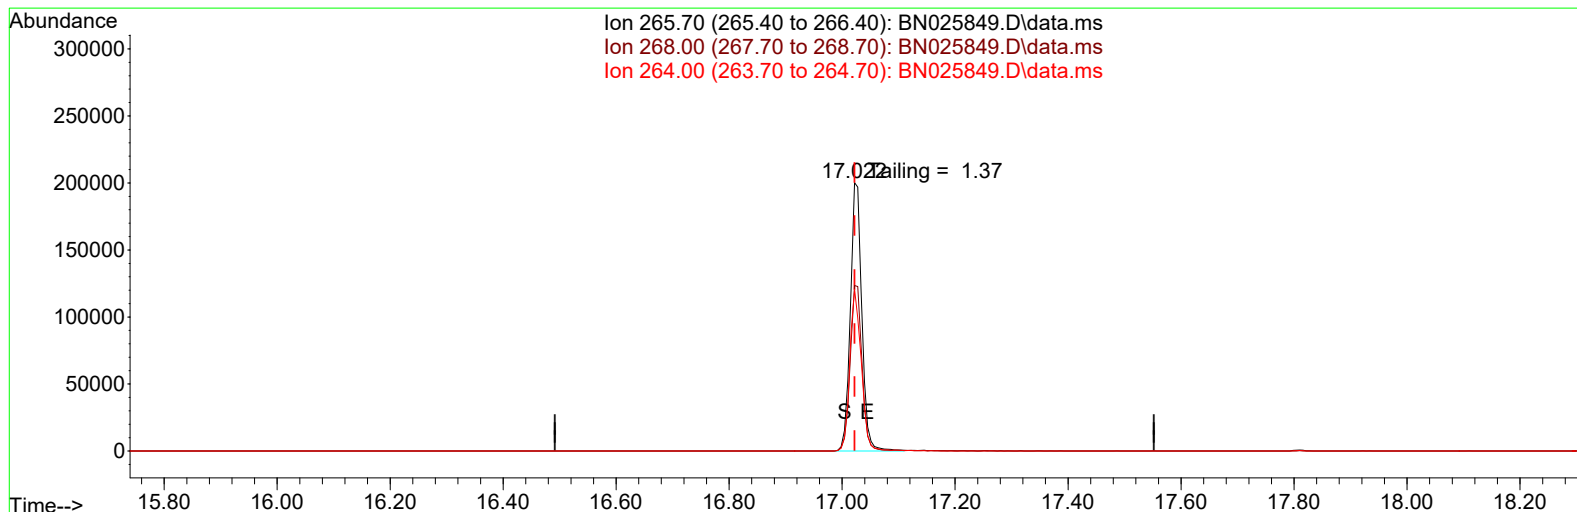

TIC: BN025849.D\data.ms

(70) Pentachlorophenol (C)

17.022min (0.000) 18603.67 ng




response 283380

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.65
264.00	61.60	60.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061523\
 Data File : BN025849.D
 Acq On : 15 Jun 2023 09:29
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jun 16 04:35:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 16 04:35:40 2023
 Response via : Initial Calibration

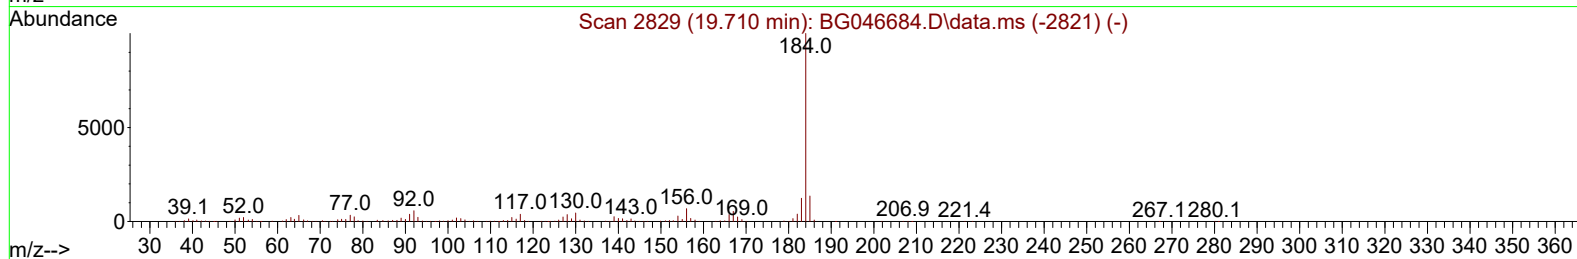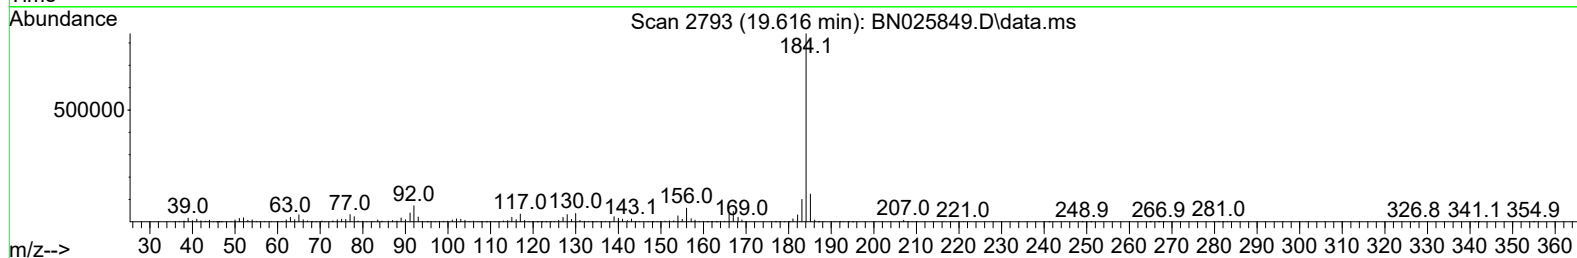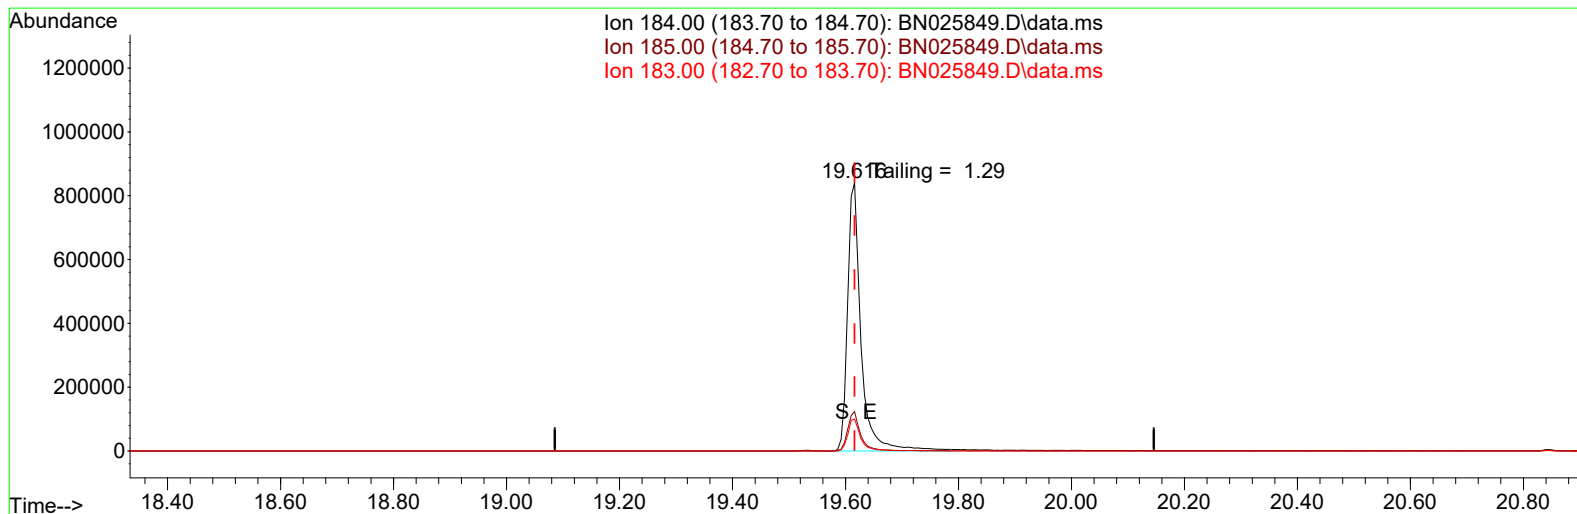

TIC: BN025849.D\data.ms

(77) Benzidine

19.616min (0.000) 745098.91 ng

response 1401045

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.75
183.00	13.20	11.96
0.00	0.00	0.00