


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061523\
Data File : BN025868.D
Acq On : 15 Jun 2023 21:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN053123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 16 01:41:46 2023

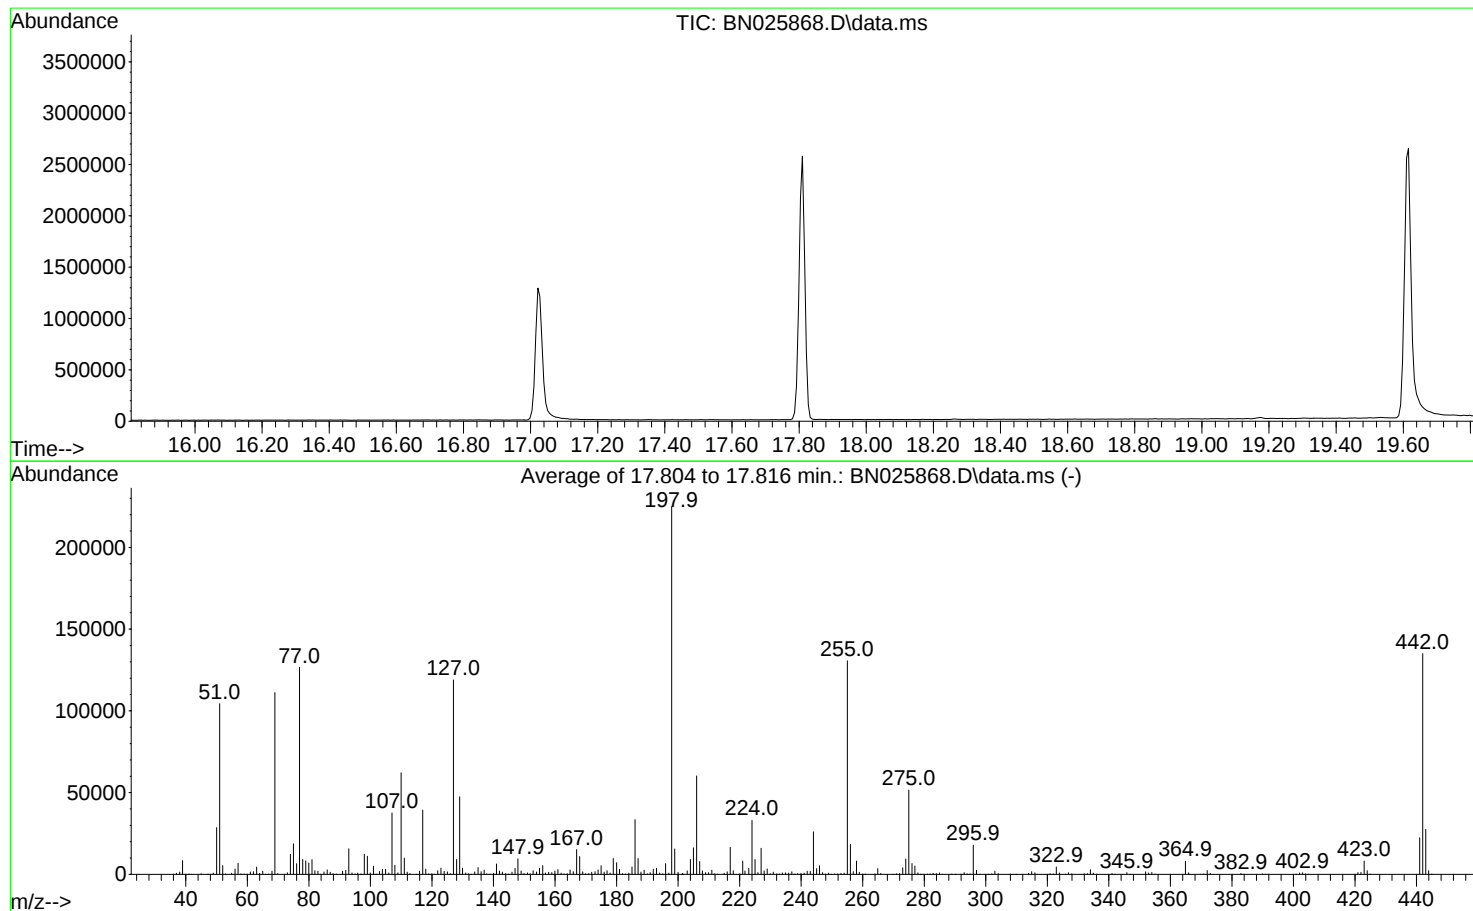

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.4	104443	PASS
68	69	0.00	2	1.7	1944	PASS
69	198	0.00	100	49.4	111213	PASS
70	69	0.00	2	0.5	541	PASS
127	198	10	80	52.9	118941	PASS
197	198	0.00	2	0.4	837	PASS
198	198	100	100	100.0	225024	PASS
199	198	5	9	6.9	15582	PASS
275	198	10	60	22.9	51597	PASS
365	198	1	100	3.6	8011	PASS
441	198	0.01	100	9.9	22388	PASS
442	442	50	100	100.0	135069	PASS
443	442	15	24	20.4	27515	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/15/2023	BNA_N	<u>BN025868.D</u>
Compound Name	Response	Retention Time
DDT	747982	20.845
DDD	16354	20.404
DDE	843	19.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17197	765179	2.25

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061523\
 Data File : BN025868.D
 Acq On : 15 Jun 2023 21:45
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jun 16 04:37:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 16 04:35:40 2023
 Response via : Initial Calibration

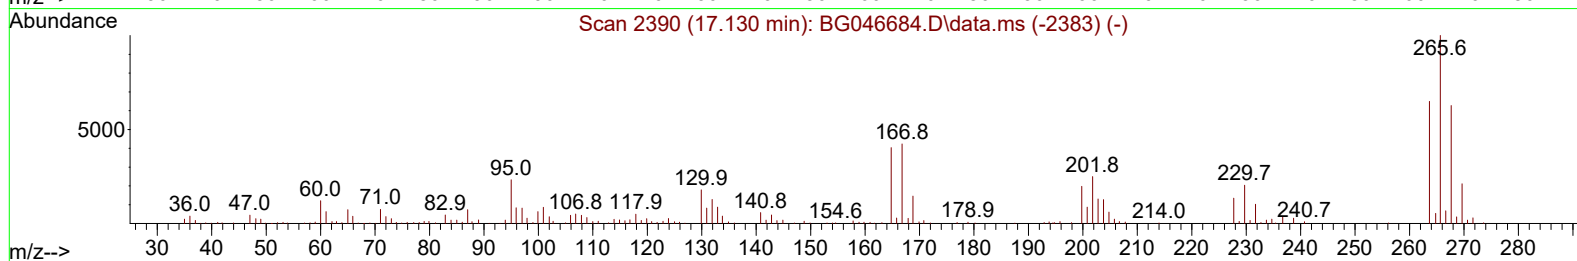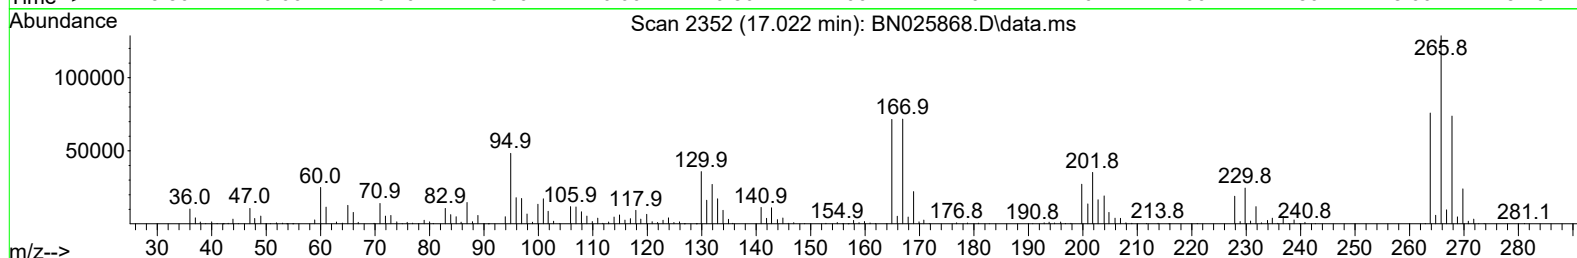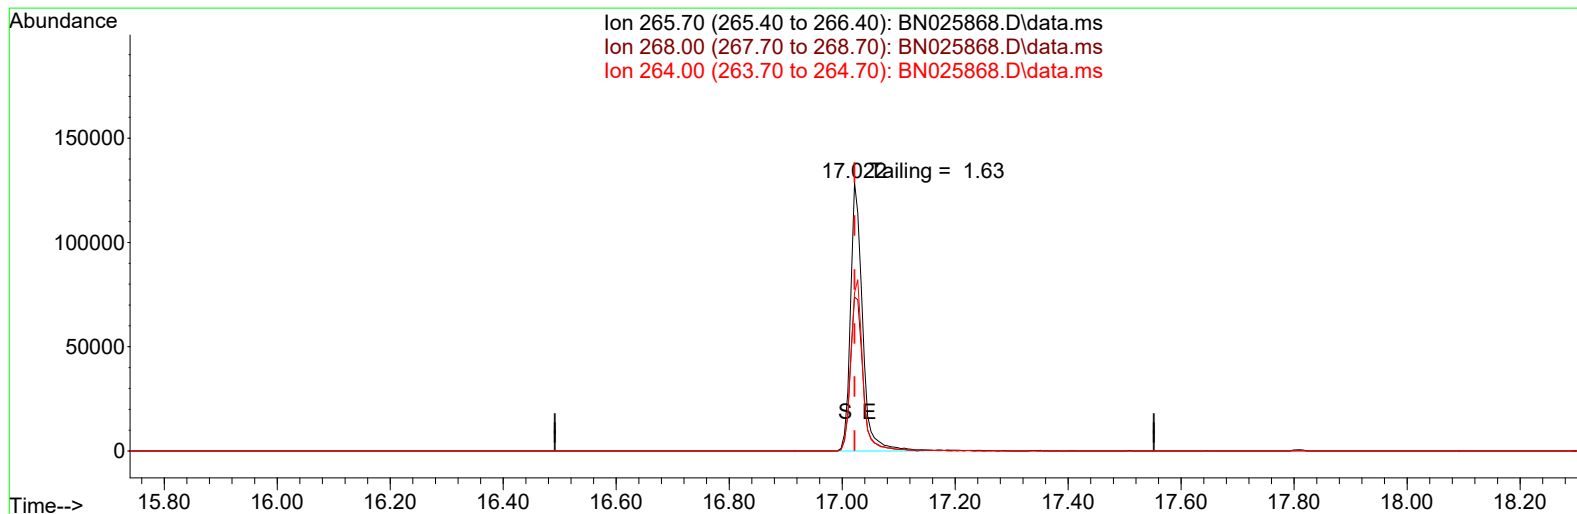

TIC: BN025868.D\data.ms

(70) Pentachlorophenol (C)

17.022min (-0.000) 12874.97 ng




response 191672

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	57.35
264.00	61.60	58.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061523\
Data File : BN025868.D
Acq On : 15 Jun 2023 21:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 16 04:37:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 16 04:35:40 2023
Response via : Initial Calibration

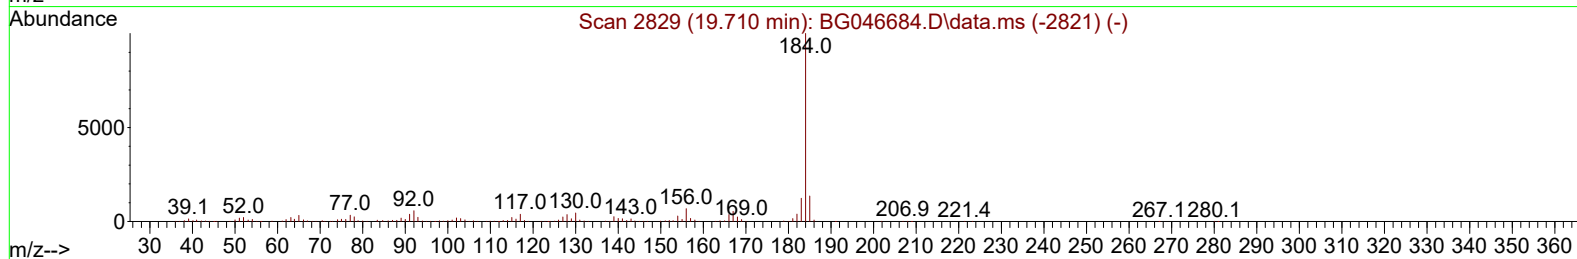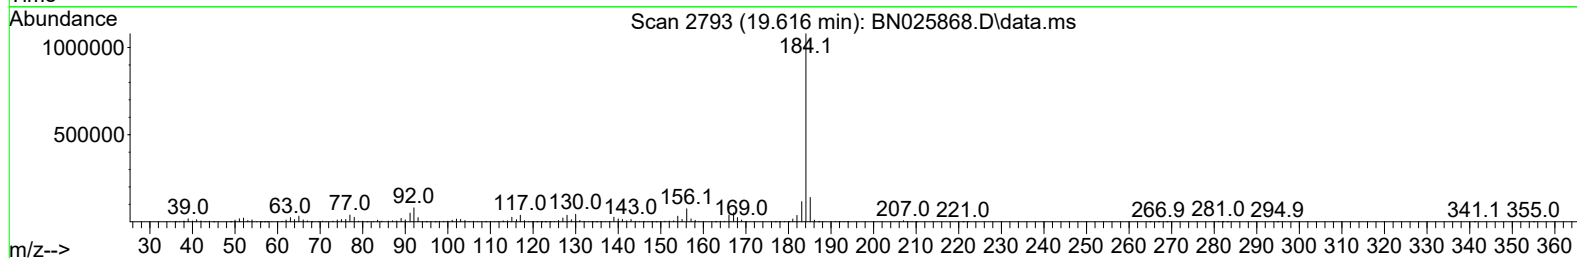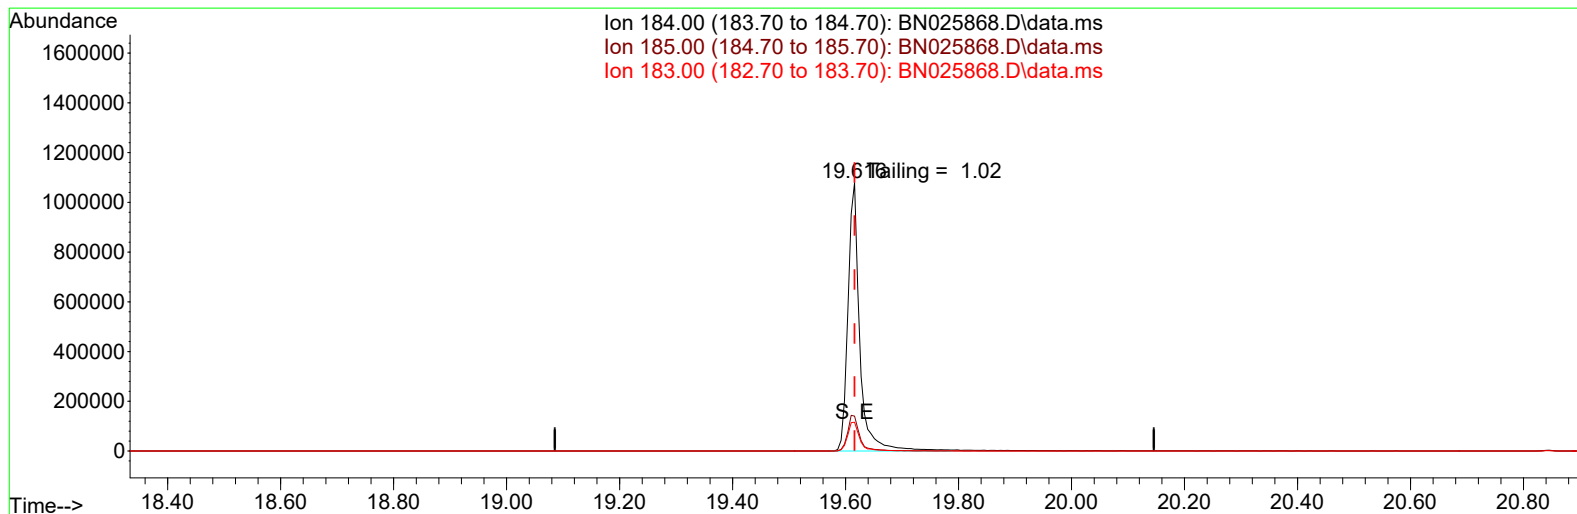

TIC: BN025868.D\data.ms

(77) Benzidine

19.616min (-0.000) 0.00 ng

response 1570155

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	12.99
183.00	13.20	10.75
0.00	0.00	0.00