
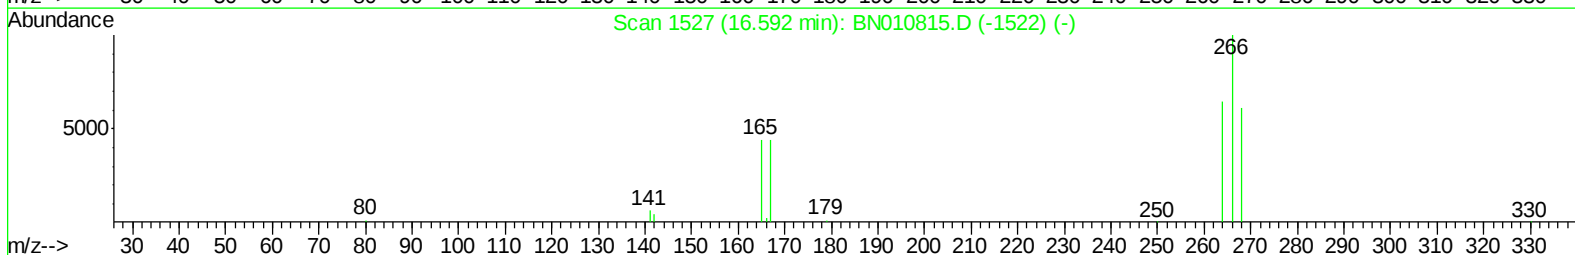
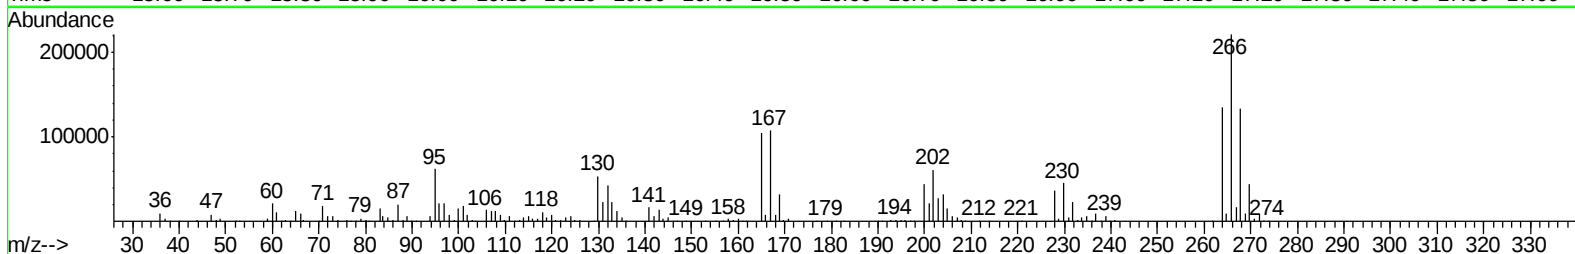


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061620\
 Data File : BN010902.D
 Acq On : 16 Jun 2020 11:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 04:43:06 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN061020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 16 08:49:35 2020
 Response via : Initial Calibration

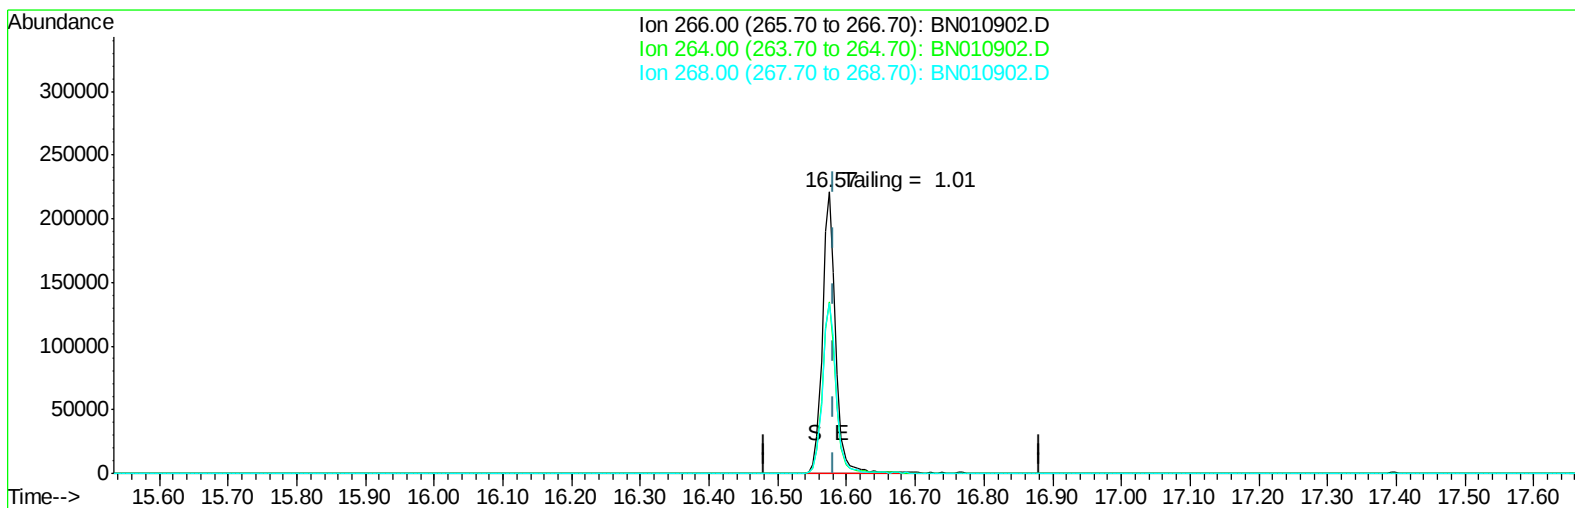

TIC: BN010902.D

(22) Pentachlorophenol

16.575min (-0.007) 12777.55ng

response 295774

Ion	Exp%	Act%
266.00	100	100
264.00	68.50	61.01
268.00	69.90	60.52
0.00	0.00	0.00