
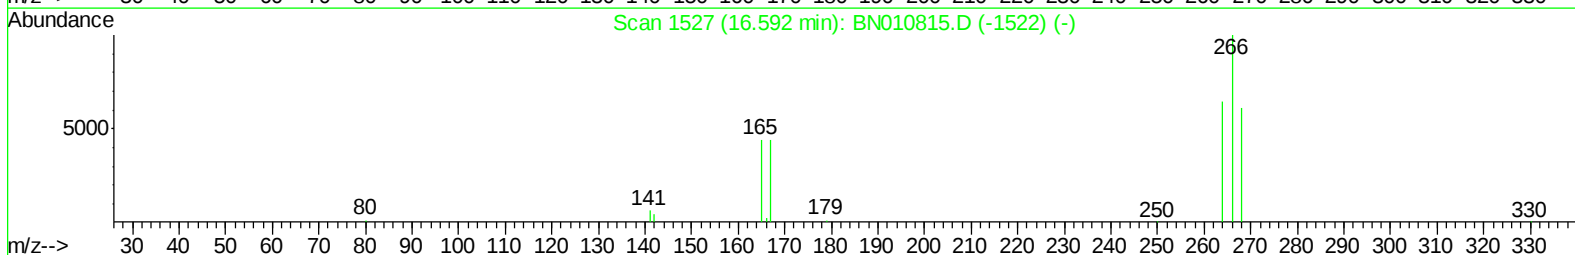
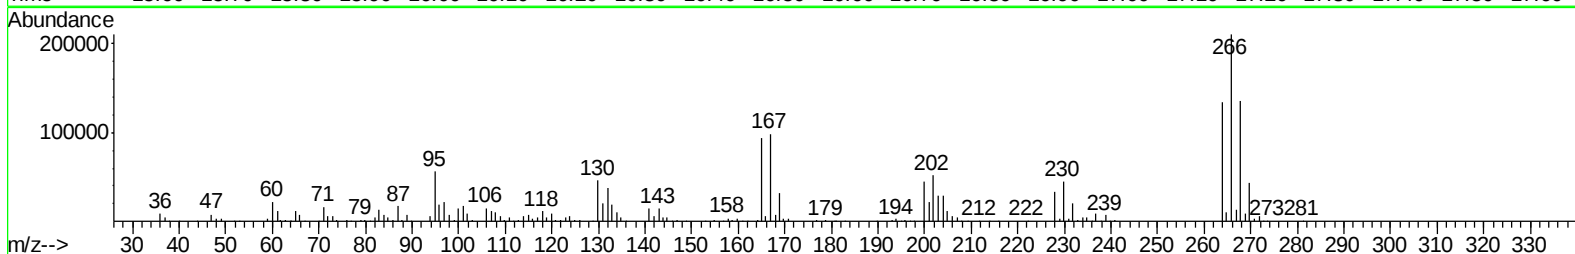


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061620\
Data File : BN010920.D
Acq On : 17 Jun 2020 00:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 00:51:00 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN061020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 16 08:49:35 2020
Response via : Initial Calibration

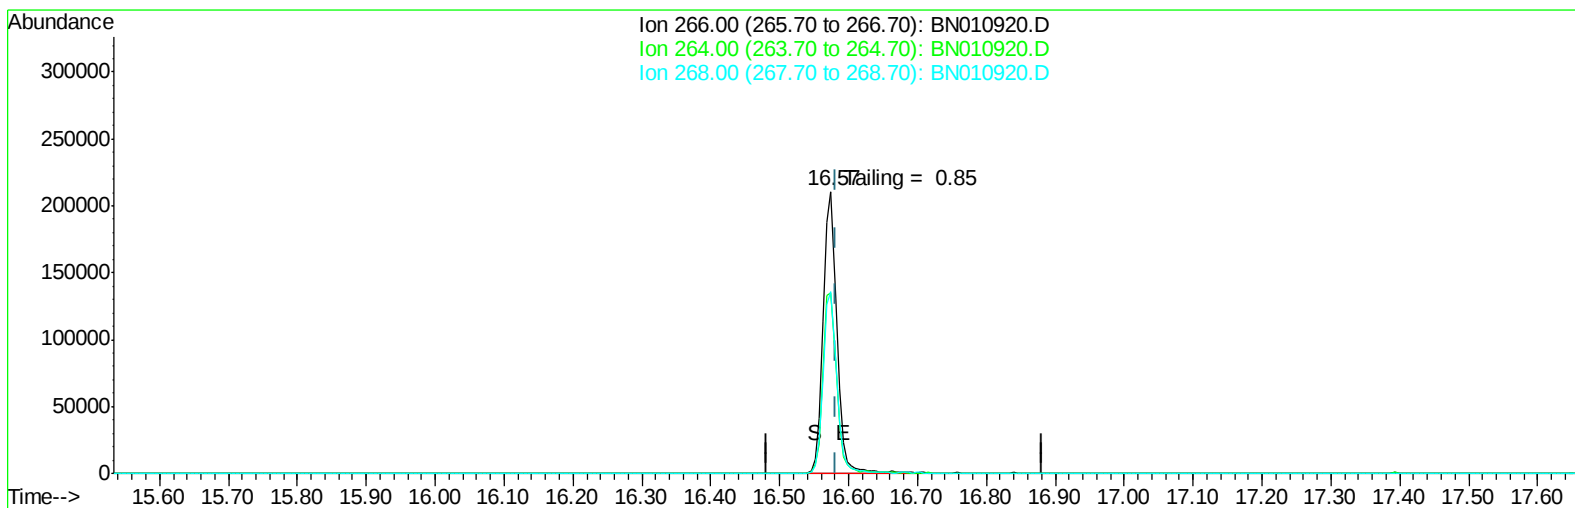

TIC: BN010920.D

(22) Pentachlorophenol

16.575min (-0.007) 0.00ng

response 288792

Ion	Exp%	Act%
266.00	100	100
264.00	68.50	64.06
268.00	69.90	64.34
0.00	0.00	0.00