

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061620\
 Data File : BN010909.D
 Acq On : 16 Jun 2020 16:30
 Operator : CG/JU
 Sample : L2993-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SS043MW014-200610

Quant Time: Jun 16 17:02:38 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN061020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 16 08:49:35 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.54	152	2347	0.40	ng	0.00
7) Naphthalene-d8	10.29	136	8328	0.40	ng	-0.01
13) Acenaphthene-d10	14.17	164	4916	0.40	ng	0.00
19) Phenanthrene-d10	16.91	188	9919	0.40	ng	-0.01
27) Chrysene-d12	21.12	240	9634	0.40	ng	-0.01
34) Perylene-d12	23.27	264	10191	0.40	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Fluorophenol	5.20	112	757	0.17	ng	0.00
5) Phenol-d6	6.74	99	513	0.10	ng	0.00
8) Nitrobenzene-d5	8.68	82	2052	0.33	ng	0.00
11) 2-Methylnaphthalene-d10	11.89	152	3688	0.29	ng	0.00
14) 2,4,6-Tribromophenol	15.67	330	589	0.33	ng	0.00
15) 2-Fluorobiphenyl	12.79	172	6147	0.32	ng	0.00
25) Fluoranthene-d10	18.95	212	10015	0.37	ng	0.00
29) Terphenyl-d14	19.57	244	9211	0.41	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
9) Naphthalene	10.34	128	4991	0.238	ng	97
12) 2-Methylnaphthalene	11.96	142	14117	1.008	ng	98
17) Acenaphthene	14.22	154	431	0.031	ng	# 71
18) Fluorene	15.22	166	1862	0.105	ng	# 81
23) Phenanthrene	16.95	178	8038	0.297	ng	98
28) Pyrene	19.35	202	1072	0.034	ng	# 92
32) Bis(2-ethylhexyl)phthalate	21.07	149	887	0.094	ng	# 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061620\
Data File : BN010909.D
Acq On : 16 Jun 2020 16:30
Operator : CG/JU
Sample : L2993-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SS043MW014-200610

Quant Time: Jun 16 17:02:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN061020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 16 08:49:35 2020
Response via : Initial Calibration

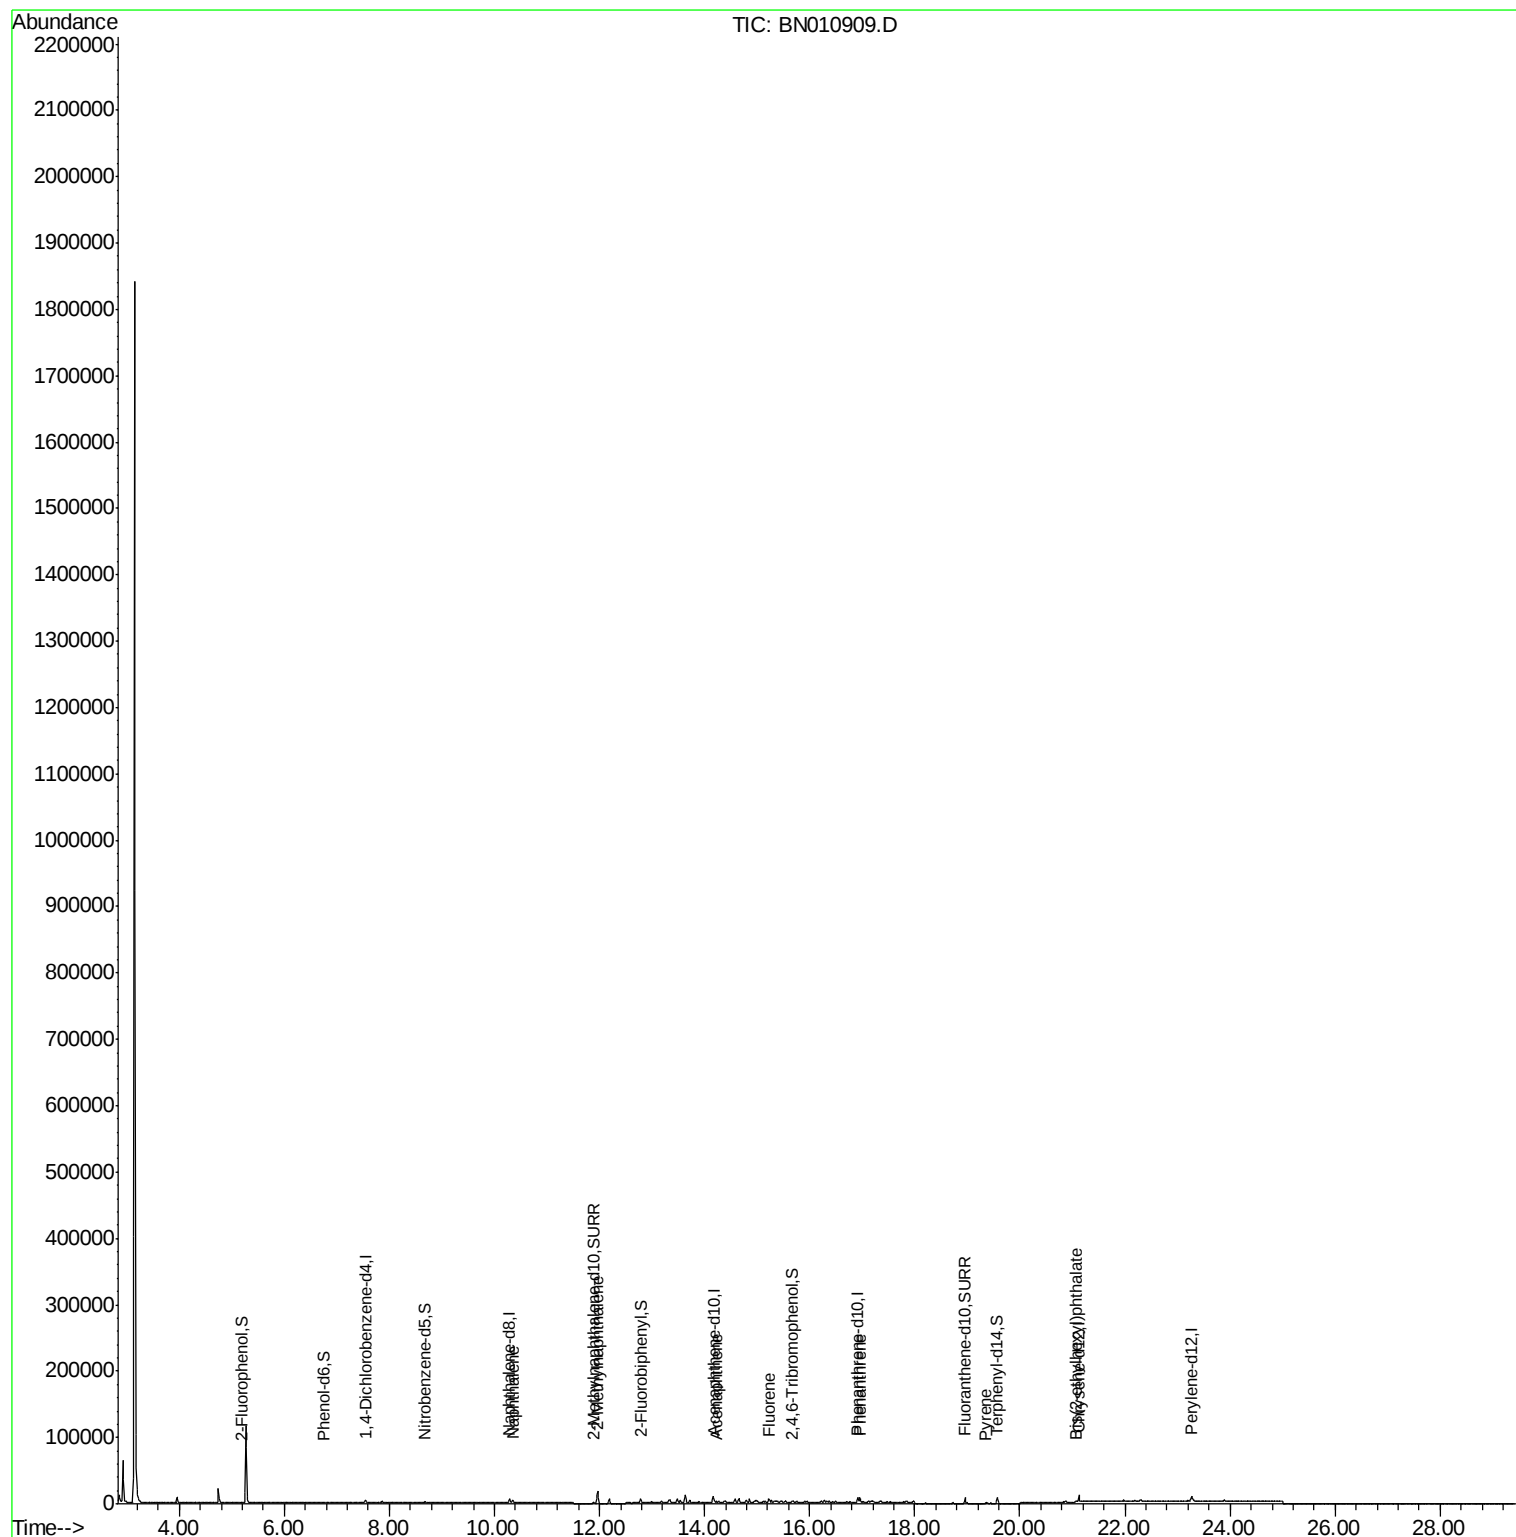




#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.54 min Scan# 585
Delta R.T. -0.01 min
Lab File: BN010909.D
Acq: 16 Jun 2020 16:30

Instrument :
BNA_N
ClientSampleId :
SS043MW014-200610

Tot Ion:152 Resp: 2347
Ion Ratio Lower Upper
152 100
150 156.4 123.8 185.6
115 64.2 49.2 73.8

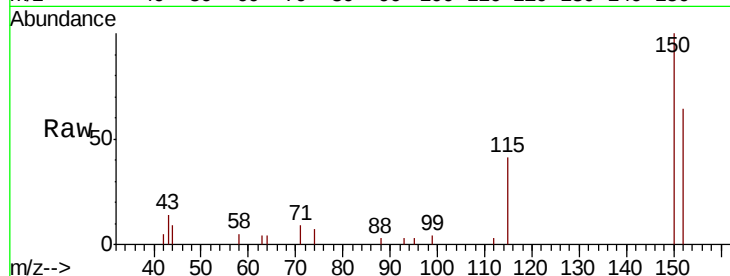


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

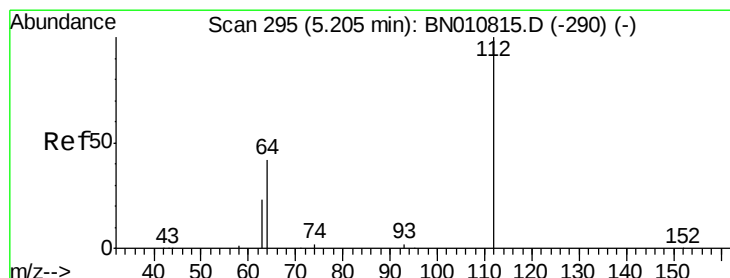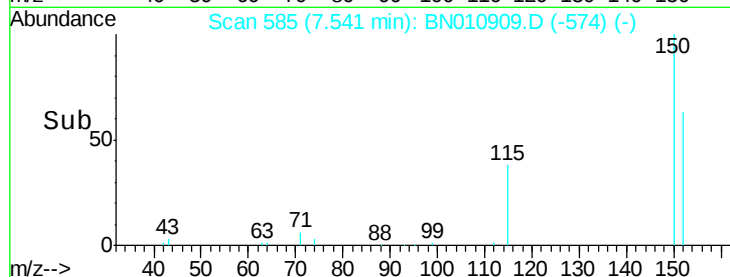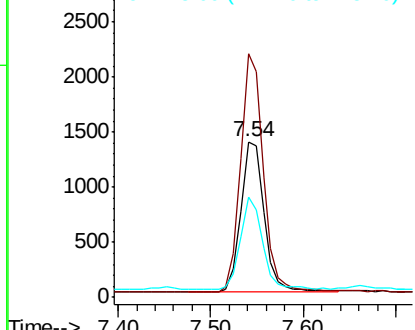



#4


2-Fluorophenol
Concen: 0.167 ng
RT: 5.20 min Scan# 294
Delta R.T. -0.00 min
Lab File: BN010909.D
Acq: 16 Jun 2020 16:30

Tgt Ion:112 Resp: 757
Ion Ratio Lower Upper
112 100
64 43.7 37.4 56.0
63 26.4 22.2 33.4

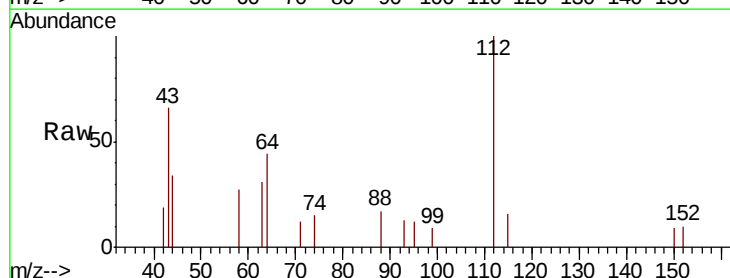

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BNC
Ion 63.00 (62.70 to 63.70): BNC

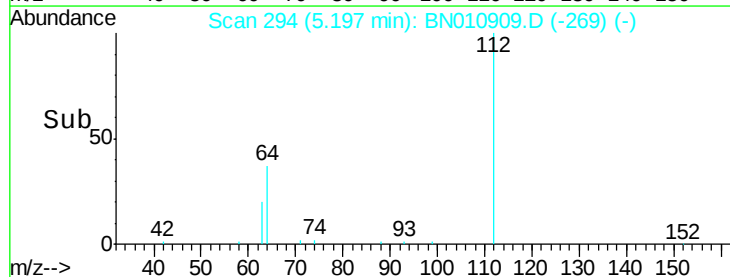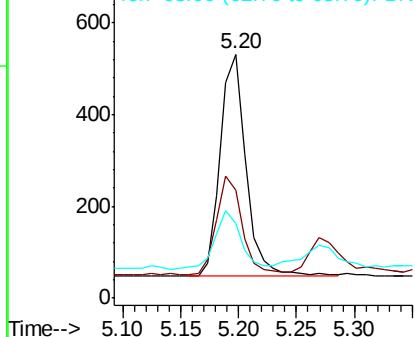

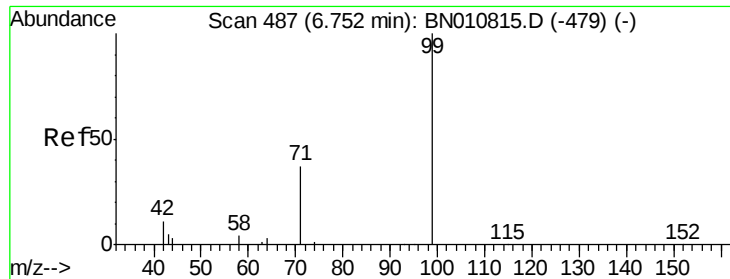

#5

Phenol-d6

Concen: 0.096 ng

RT: 6.74 min Scan# 486

Delta R.T. -0.00 min

Lab File: BN010909.D

Acq: 16 Jun 2020 16:30

Instrument :

BNA_N

ClientSampleId :

SS043MW014-200610


Tot Ion: 99 Resp: 513

Ion Ratio Lower Upper




99 100

42 17.0 11.1 16.7#

71 54.6 31.4 47.2#

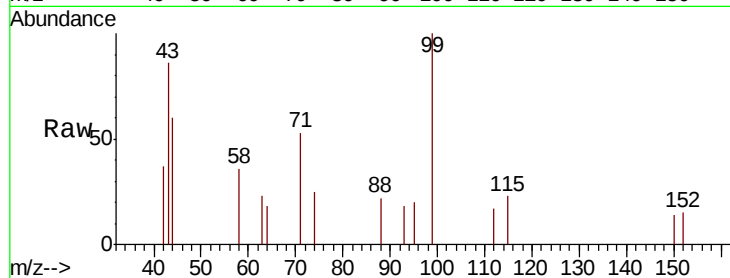

Abundance Ion 99.00 (98.70 to 99.70): BN010815.D (-479) (-)

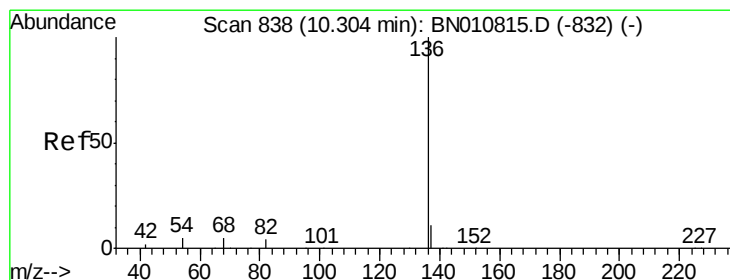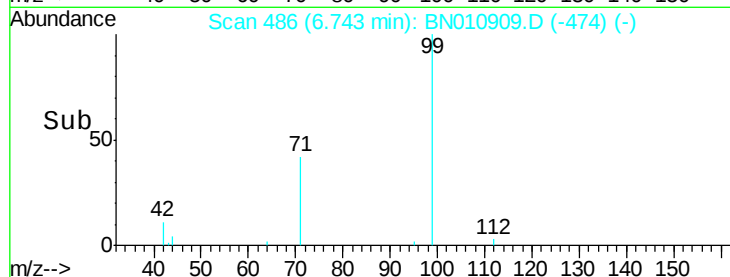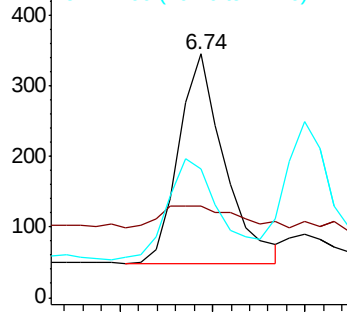

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.29 min Scan# 837

Delta R.T. -0.01 min

Lab File: BN010909.D

Acq: 16 Jun 2020 16:30

Tgt Ion: 136 Resp: 8328


Ion Ratio Lower Upper

136 100



137 11.7 9.7 14.5


54 6.9 4.9 7.3

68 7.3 4.7 7.1#

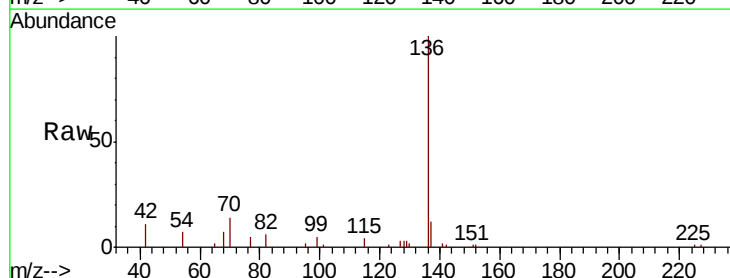

Abundance Ion 136.00 (135.70 to 136.70): BN010815.D (-832) (-)

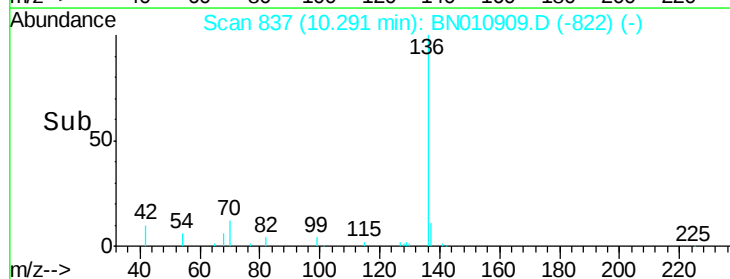

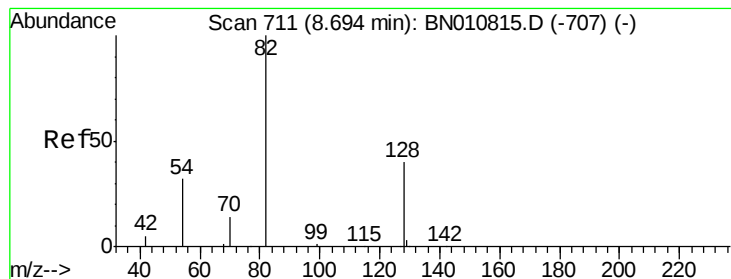

#8

Nitrobenzene-d5

Concen: 0.333 ng

RT: 8.68 min Scan# 710

Delta R.T. -0.00 min

Lab File: BN010909.D

Acq: 16 Jun 2020 16:30

Instrument :

BNA_N

ClientSampleId :

SS043MW014-200610


Tot Ion: 82 Resp: 2052

Ion Ratio Lower Upper

82 100

128 45.0 35.4 53.0




54 35.0 28.2 42.4



Abundance Ion 82.00 (81.70 to 82.70): BN010815.D (-707) (-)

Ion 128.00 (127.70 to 128.70): BN010815.D (-707) (-)

Ion 54.00 (53.70 to 54.70): BN010815.D (-707) (-)

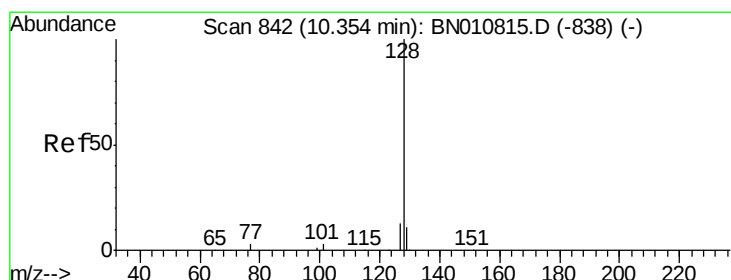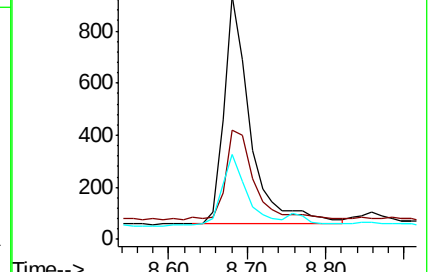

#9

Naphthalene

Concen: 0.238 ng

RT: 10.34 min Scan# 841

Delta R.T. -0.00 min

Lab File: BN010909.D

Acq: 16 Jun 2020 16:30


Tgt Ion:128 Resp: 4991

Ion Ratio Lower Upper

128 100

129 13.1 9.6 14.4



127 15.4 11.4 17.2




Abundance Ion 128.00 (127.70 to 128.70): BN010815.D (-838) (-)

Ion 129.00 (128.70 to 129.70): BN010815.D (-838) (-)

Ion 127.00 (126.70 to 127.70): BN010815.D (-838) (-)




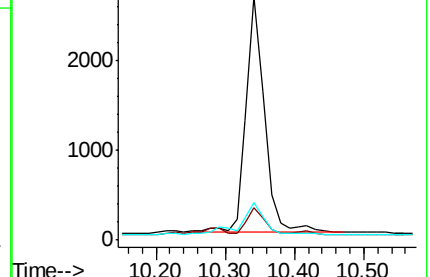


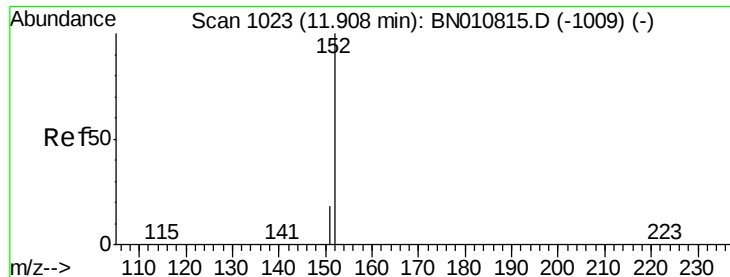

#11
2-Methylnaphthalene-d10
Concen: 0.285 ng
RT: 11.89 min Scan# 1018
Delta R.T. -0.01 min
Lab File: BN010909.D
Acq: 16 Jun 2020 16:30




Instrument :
BNA_N
ClientSampleId :
SS043MW014-200610


Tot Ion:152 Resp: 3688
Ion Ratio Lower Upper
152 100
151 20.1 15.3 22.9

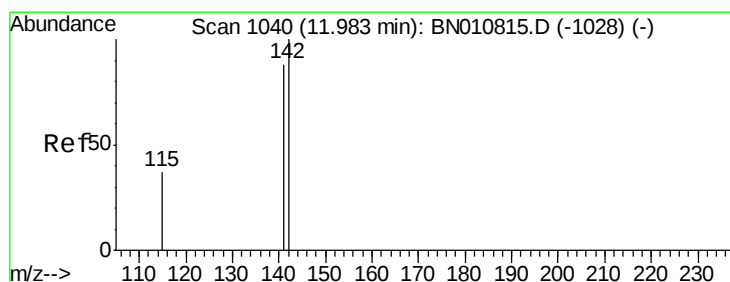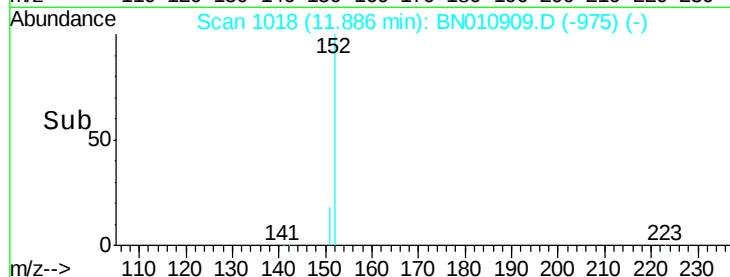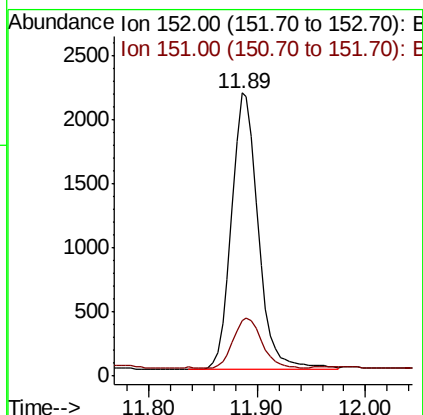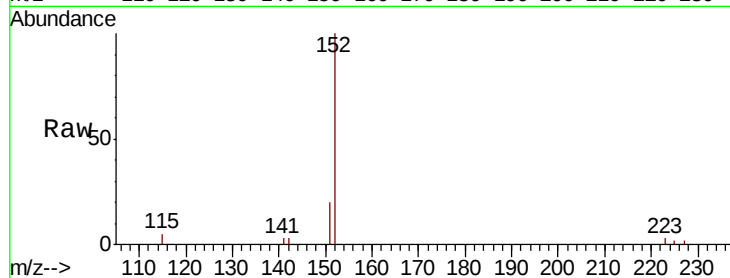

#12
2-Methylnaphthalene
Concen: 1.008 ng
RT: 11.96 min Scan# 1035
Delta R.T. -0.01 min
Lab File: BN010909.D
Acq: 16 Jun 2020 16:30

Tgt Ion:142 Resp: 14117
Ion Ratio Lower Upper
142 100
141 89.3 70.8 106.2
115 36.7 31.5 47.3

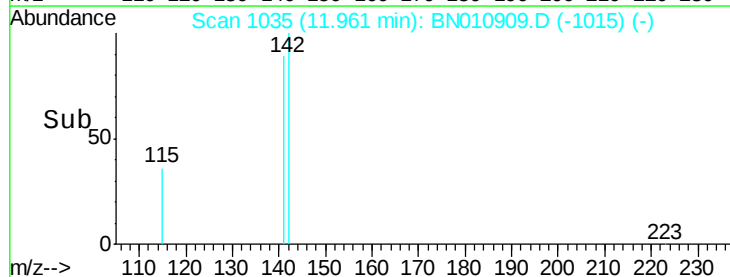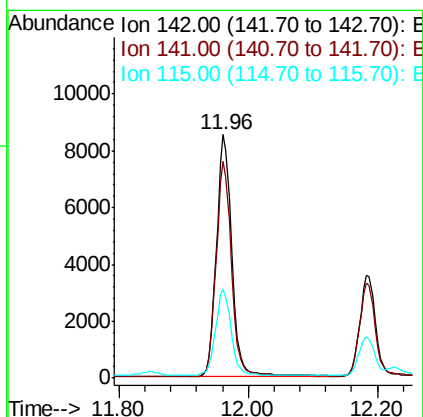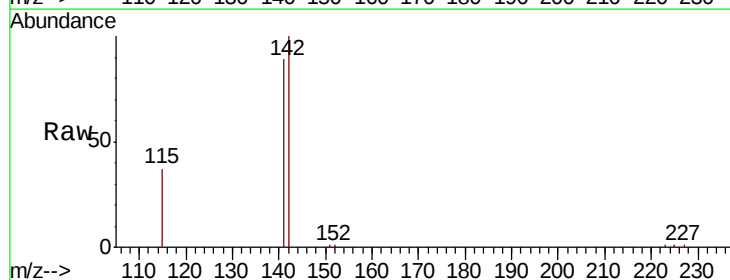



#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.17 min Scan# 1307

Delta R.T. -0.00 min

Lab File: BN010909.D

Acq: 16 Jun 2020 16:30

Instrument :

BNA_N

ClientSampleId :

SS043MW014-200610


Tot Ion:164 Resp: 4916

Ion Ratio Lower Upper

164 100

162 99.4 81.0 121.6




160 46.8 38.9 58.3

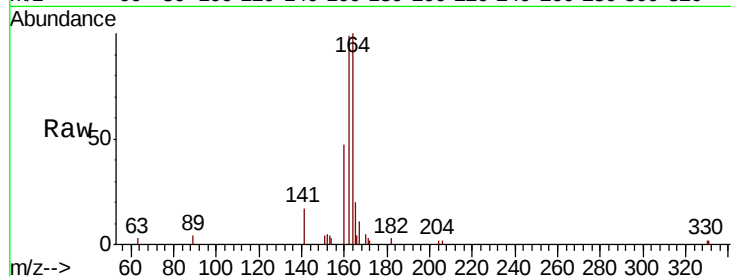

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

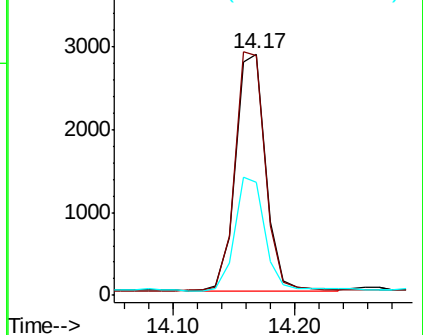

#14

2,4,6-Tribromophenol

Concen: 0.335 ng

RT: 15.67 min Scan# 1442

Delta R.T. -0.00 min

Lab File: BN010909.D

Acq: 16 Jun 2020 16:30


Tgt Ion:330 Resp: 589

Ion Ratio Lower Upper

330 100

332 0.0 0.0 0.0



141 78.3 33.2 49.8#




Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E




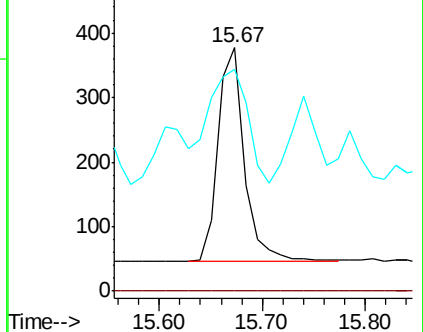


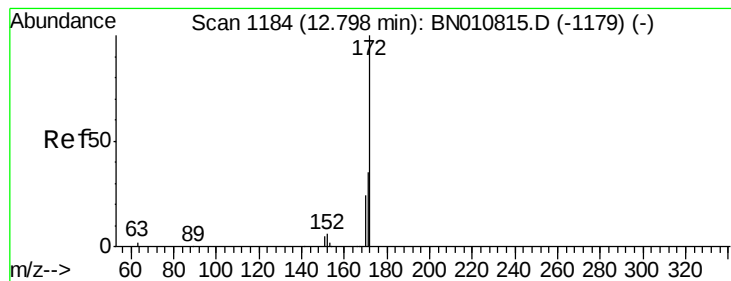

#15
2-Fluorobiphenyl
Concen: 0.317 ng
RT: 12.79 min Scan# 1183
Delta R.T. -0.00 min
Lab File: BN010909.D
Acq: 16 Jun 2020 16:30




Instrument :
BNA_N
ClientSampleId :
SS043MW014-200610


Tot Ion:172 Resp: 6147
Ion Ratio Lower Upper
172 100
171 34.5 28.5 42.7
170 23.0 19.7 29.5

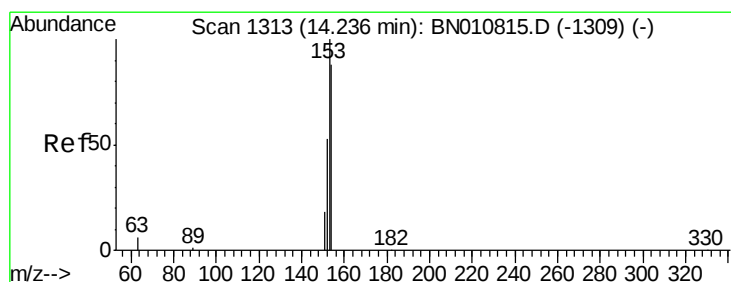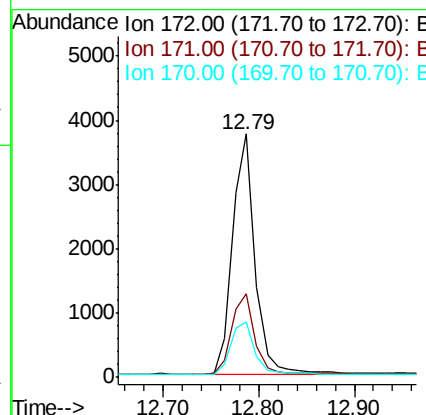

#17
Acenaphthene
Concen: 0.031 ng
RT: 14.22 min Scan# 1312
Delta R.T. -0.01 min
Lab File: BN010909.D
Acq: 16 Jun 2020 16:30

Tgt Ion:154 Resp: 431
Ion Ratio Lower Upper
154 100
153 110.9 91.8 137.6
152 0.0 47.6 71.4#

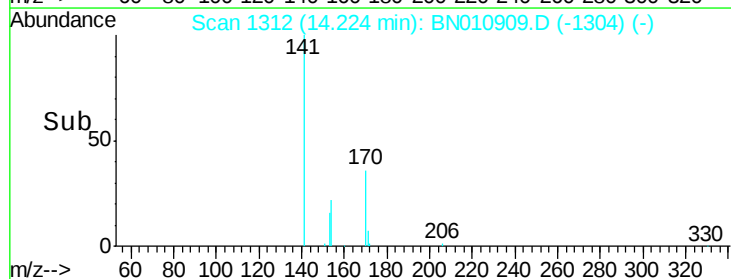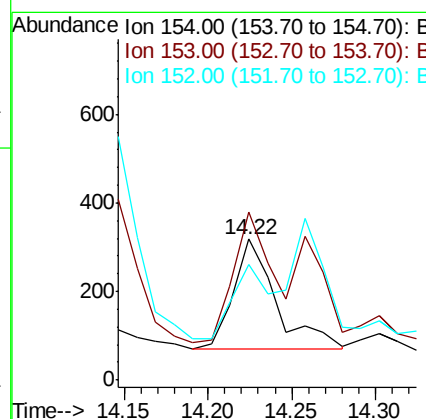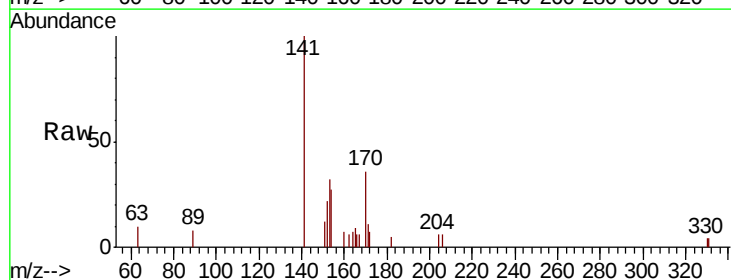

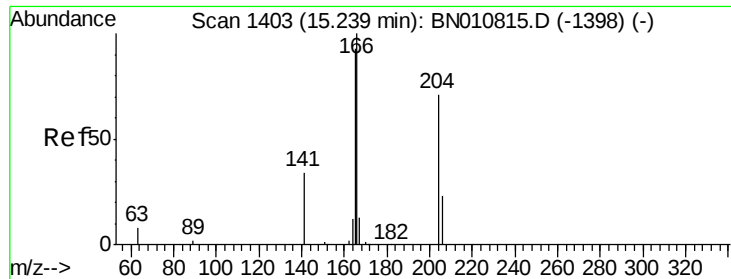

#18

Fluorene

Concen: 0.105 ng

RT: 15.22 min Scan# 1401

Delta R.T. -0.01 min

Lab File: BN010909.D

Acq: 16 Jun 2020 16:30

Instrument :

BNA_N

ClientSampleId :

SS043MW014-200610


Tot Ion:166 Resp: 1862

Ion Ratio Lower Upper

166 100

165 109.0 77.2 115.8




167 38.3 10.7 16.1#

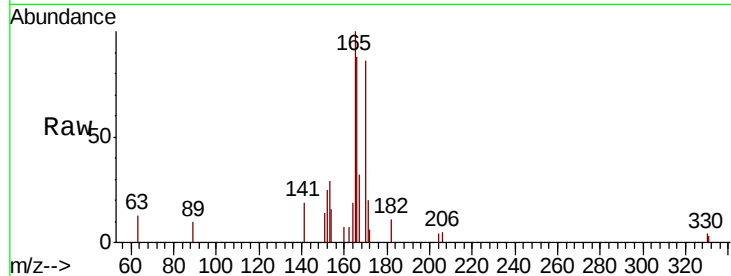

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

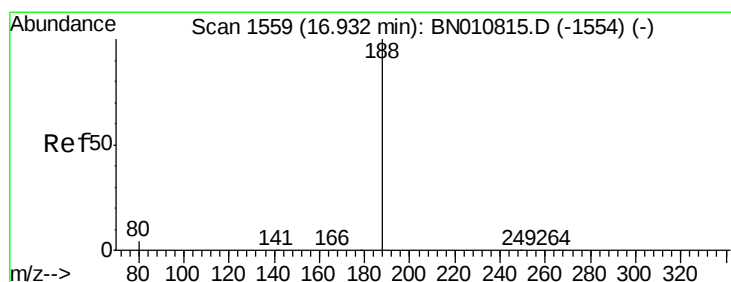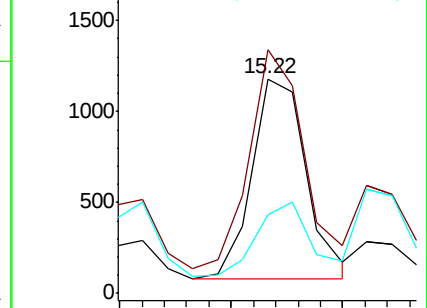

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.91 min Scan# 1557

Delta R.T. -0.01 min

Lab File: BN010909.D

Acq: 16 Jun 2020 16:30


Tgt Ion:188 Resp: 9919

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0



80 10.7 4.5 6.7#

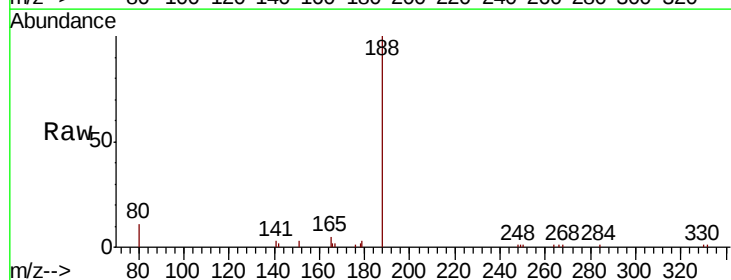


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BNC

Ion 80.00 (79.70 to 80.70): BNC

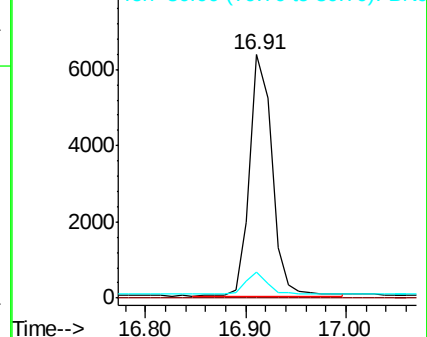



#23

Phenanthrene

Concen: 0.297 ng

RT: 16.95 min Scan# 1561

Delta R.T. -0.01 min

Lab File: BN010909.D

Acq: 16 Jun 2020 16:30

Instrument :

BNA_N

ClientSampleId :

SS043MW014-200610


Tot Ion:178 Resp: 8038

Ion Ratio Lower Upper

178 100

176 18.9 15.3 22.9




179 17.1 12.6 19.0

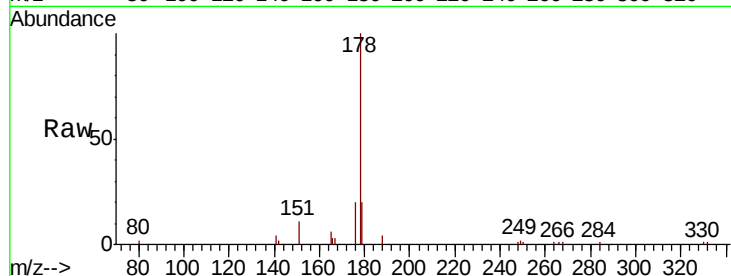

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

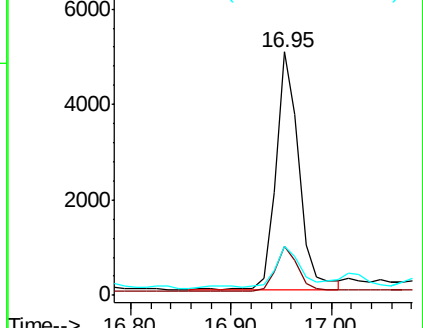

#25

Fluoranthene-d10

Concen: 0.366 ng

RT: 18.95 min Scan# 1851

Delta R.T. -0.01 min

Lab File: BN010909.D

Acq: 16 Jun 2020 16:30


Tgt Ion:212 Resp: 10015

Ion Ratio Lower Upper

212 100

106 10.3 6.6 10.0#



104 6.0 4.0 6.0




Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

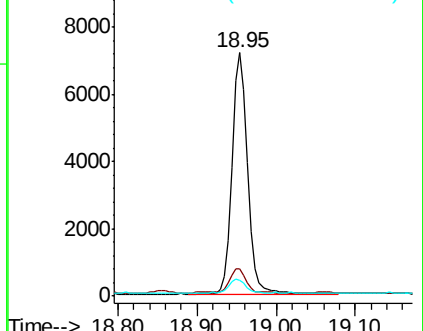



#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.12 min Scan# 2168

Delta R.T. -0.01 min

Lab File: BN010909.D

Acq: 16 Jun 2020 16:30

Instrument :

BNA_N

ClientSampleId :

SS043MW014-200610


Tot Ion:240 Resp: 9634

Ion Ratio Lower Upper

240 100

120 11.2 7.5 11.3




236 27.6 22.3 33.5



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

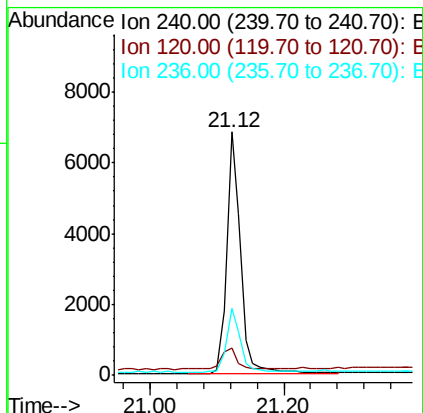

#28

Pyrene

Concen: 0.034 ng

RT: 19.35 min Scan# 1930

Delta R.T. -0.01 min

Lab File: BN010909.D

Acq: 16 Jun 2020 16:30


Tgt Ion:202 Resp: 1072

Ion Ratio Lower Upper

202 100

200 20.9 16.4 24.6



203 25.2 14.2 21.4#




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

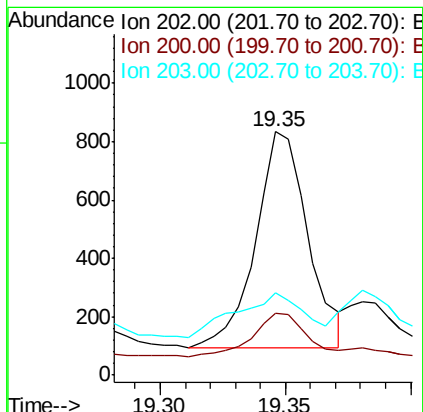

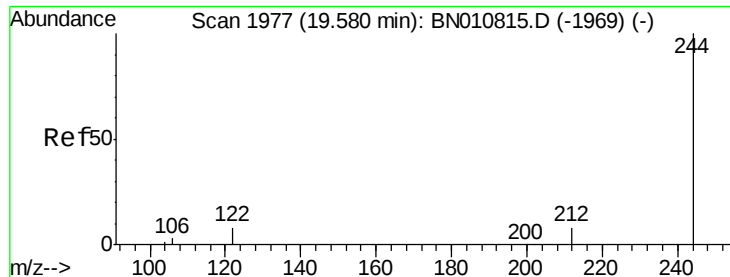

#29

Terphenyl-d14

Concen: 0.408 ng

RT: 19.57 min Scan# 1975

Delta R.T. -0.01 min

Lab File: BN010909.D

Acq: 16 Jun 2020 16:30

Instrument :

BNA_N

ClientSampleId :

SS043MW014-200610


Tot Ion:244 Resp: 9211

Ion Ratio Lower Upper

244 100

212 8.5 7.4 11.2




122 9.9 7.5 11.3

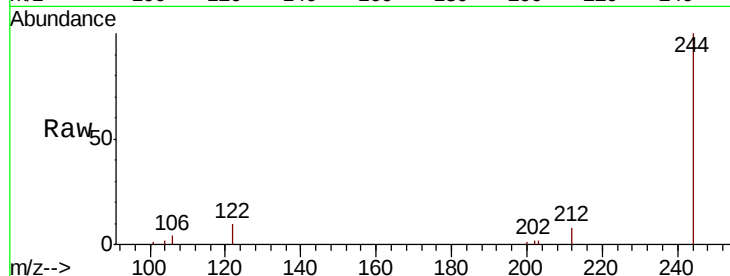

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

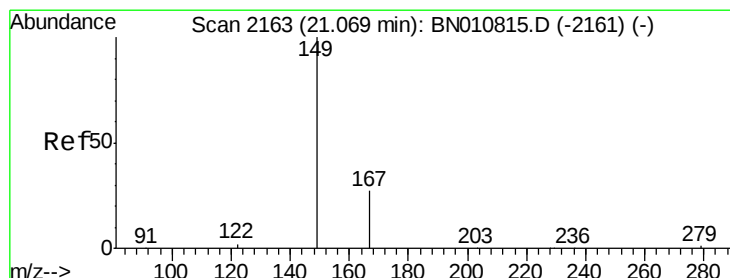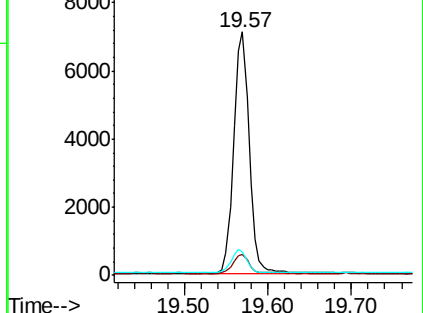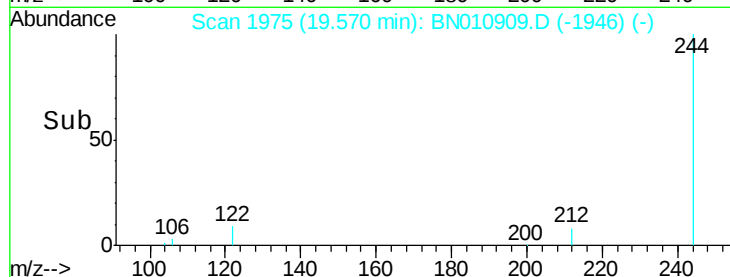

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.094 ng

RT: 21.07 min Scan# 2163

Delta R.T. -0.00 min

Lab File: BN010909.D

Acq: 16 Jun 2020 16:30


Tgt Ion:149 Resp: 887

Ion Ratio Lower Upper

149 100

167 28.7 24.1 36.1



279 9.8 4.6 7.0#



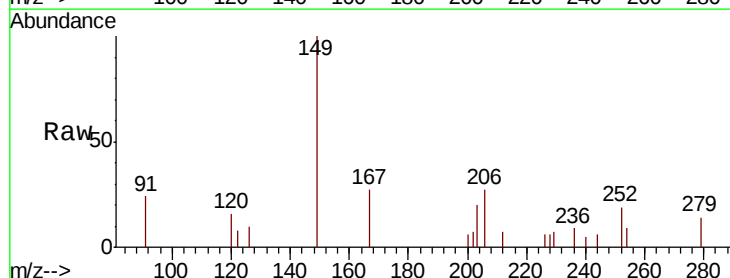


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

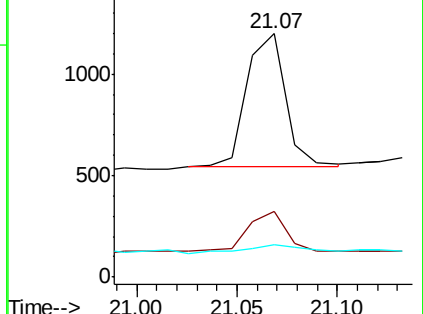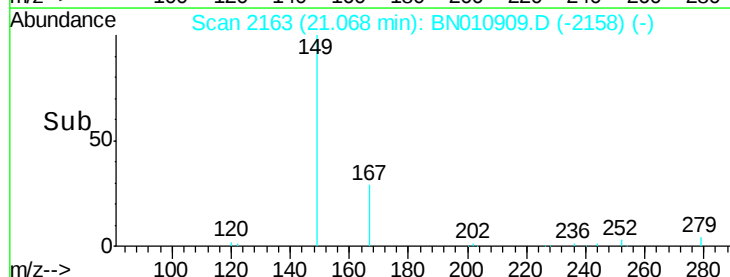

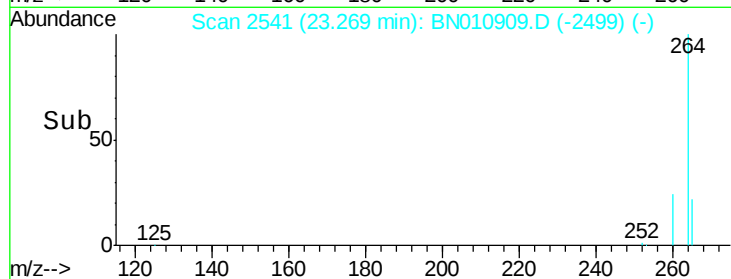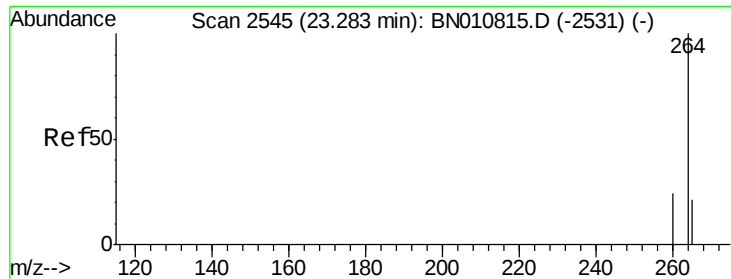

#34

Pervlene-d12

Concen: 0.400 ng

RT: 23.27 min Scan# 2541

Delta R.T. -0.01 min

Lab File: BN010909.D

Acq: 16 Jun 2020 16:30

Instrument :

BNA_N

ClientSampleId :

SS043MW014-200610

Tot Ion: 264 Resp: 10191

Ion Ratio Lower Upper

264 100

260 24.9 20.4 30.6

265 78.2 75.0 112.4

