

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061620\
 Data File : BN010929.D
 Acq On : 17 Jun 2020 05:41
 Operator : CG/JU
 Sample : L3011-14
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RE123D2-20200612

Quant Time: Jun 17 07:03:57 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN061020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 16 08:49:35 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.54	152	2331	0.40	ng	0.00
7) Naphthalene-d8	10.29	136	7999	0.40	ng	-0.01
13) Acenaphthene-d10	14.16	164	4706	0.40	ng	0.00
19) Phenanthrene-d10	16.92	188	9062	0.40	ng	0.00
27) Chrysene-d12	21.12	240	8440	0.40	ng	0.00
34) Perylene-d12	23.27	264	8662	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.20	112	711	0.16	ng	0.00
5) Phenol-d6	6.74	99	462	0.09	ng	0.00
8) Nitrobenzene-d5	8.68	82	2351	0.40	ng	0.00
11) 2-Methylnaphthalene-d10	11.89	152	5630	0.45	ng	0.00
14) 2,4,6-Tribromophenol	15.67	330	538	0.32	ng	0.00
15) 2-Fluorobiphenyl	12.78	172	7195	0.39	ng	0.00
25) Fluoranthene-d10	18.95	212	13717	0.55	ng	0.00
29) Terphenyl-d14	19.57	244	9949	0.50	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.22	88	1160	0.508	ng	# 89
32) Bis(2-ethylhexyl)phthalate	21.06	149	758	0.092	ng	# 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061620\
Data File : BN010929.D
Acq On : 17 Jun 2020 05:41
Operator : CG/JU
Sample : L3011-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RE123D2-20200612

Quant Time: Jun 17 07:03:57 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN061020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 16 08:49:35 2020
Response via : Initial Calibration

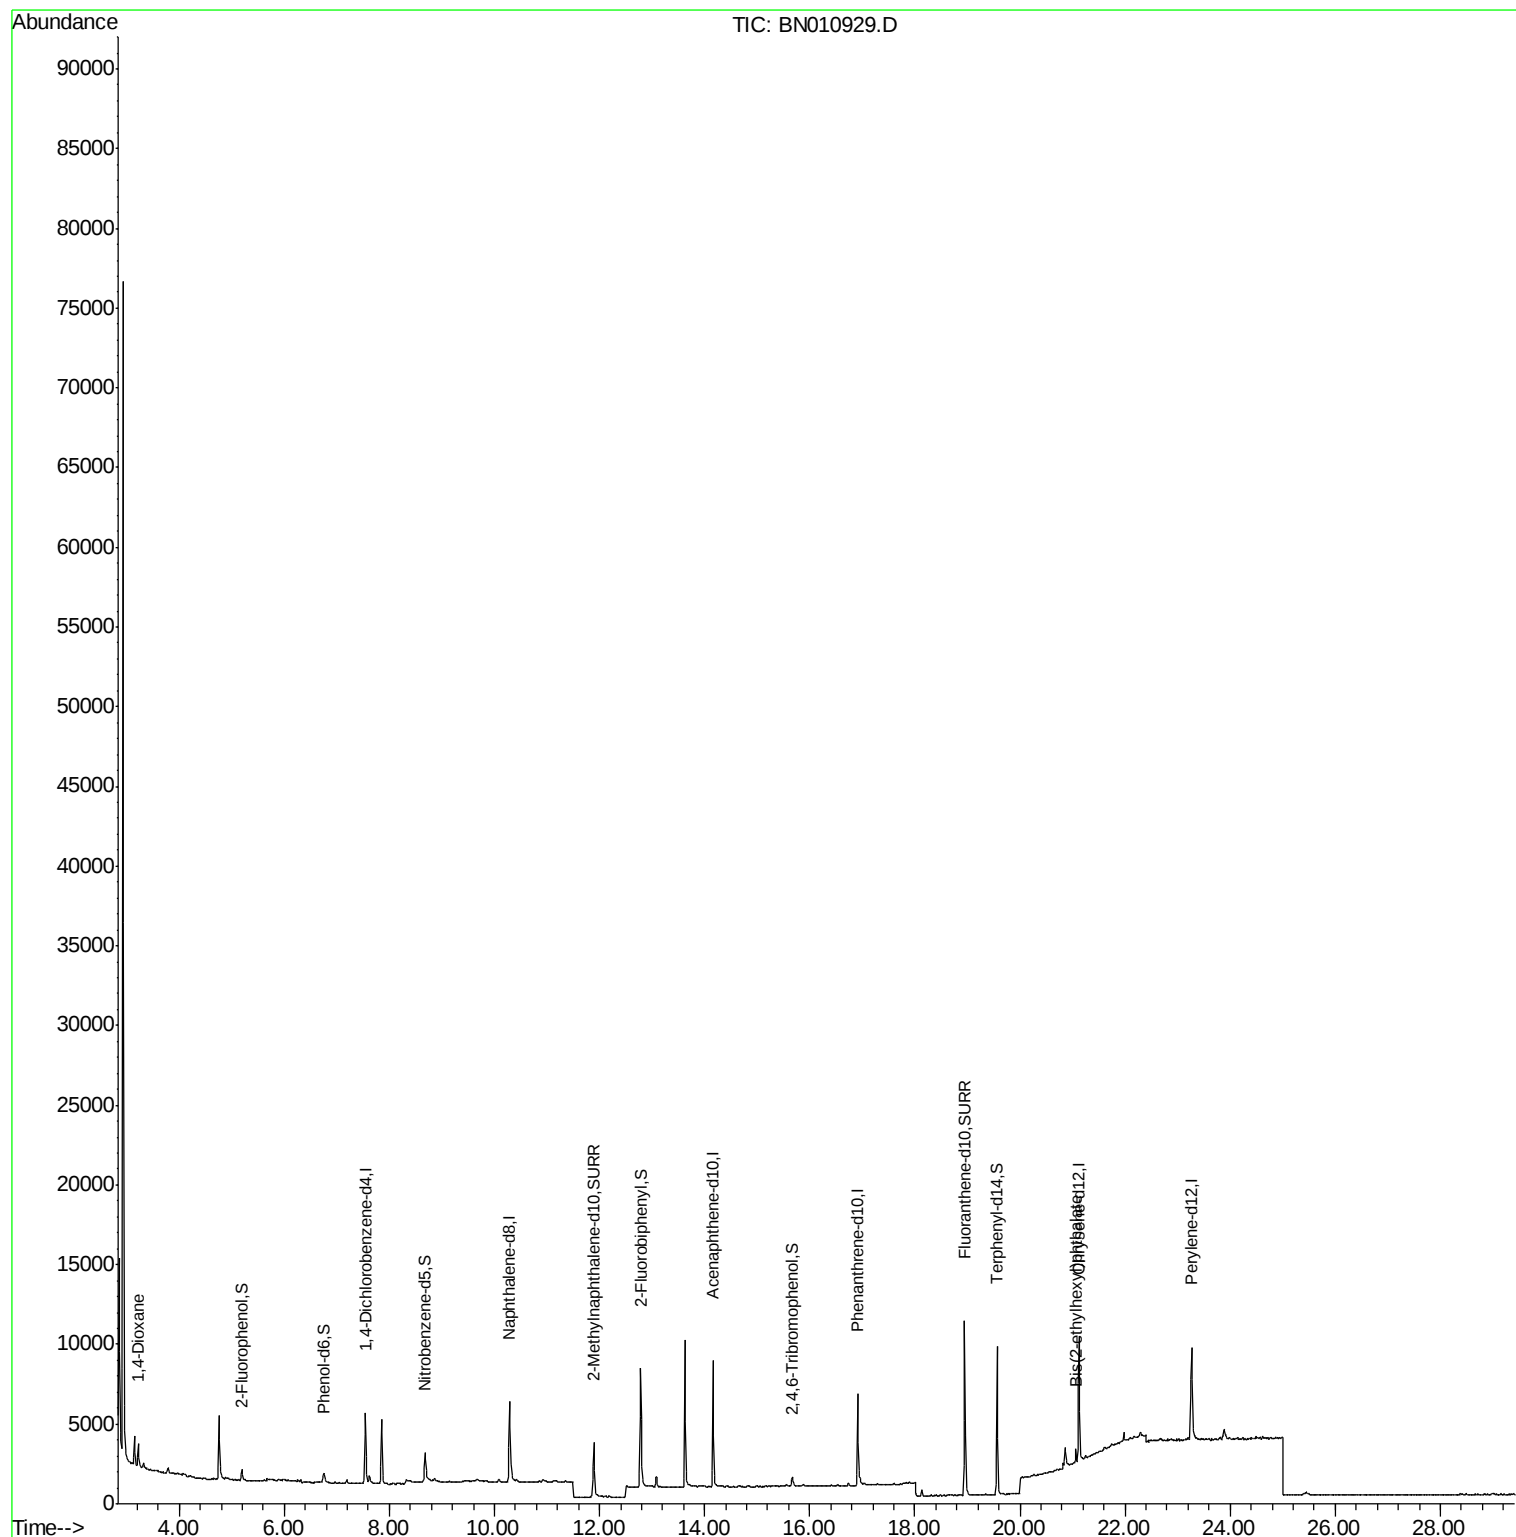




#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.54 min Scan# 585
Delta R.T. -0.01 min
Lab File: BN010929.D
Acq: 17 Jun 2020 05:41

Instrument :
BNA_N
ClientSampleId :
RE123D2-20200612

Tot Ion:152 Resp: 2331
Ion Ratio Lower Upper
152 100
150 157.6 123.8 185.6
115 62.8 49.2 73.8

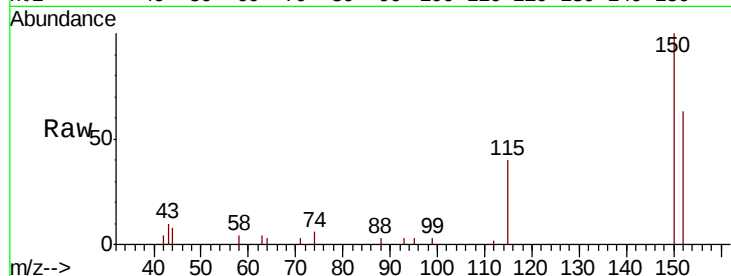


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

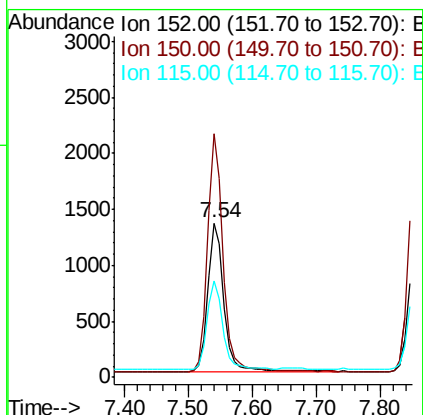



#2


1,4-Dioxane
Concen: 0.508 ng
RT: 3.22 min Scan# 48
Delta R.T. -0.01 min
Lab File: BN010929.D
Acq: 17 Jun 2020 05:41

Tgt Ion: 88 Resp: 1160
Ion Ratio Lower Upper
88 100
58 52.1 38.2 57.4
43 28.7 15.1 22.7#



Abundance Ion 88.00 (87.70 to 88.70): BN0
Ion 58.00 (57.70 to 58.70): BN0
Ion 43.00 (42.70 to 43.70): BN0

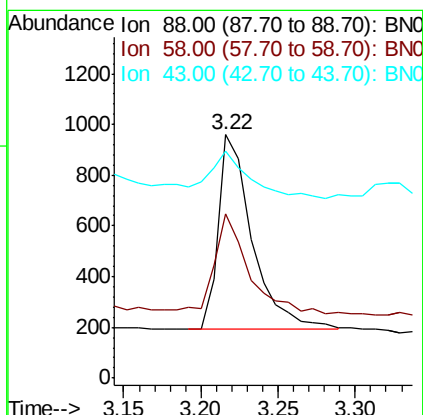

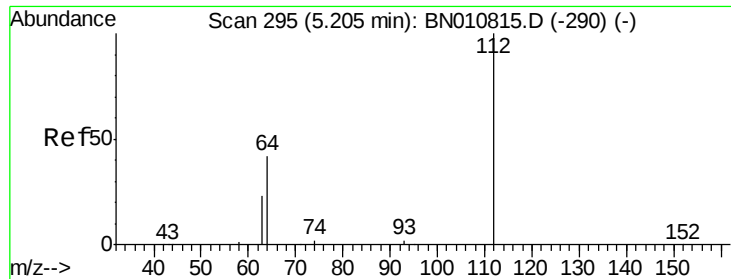

#4

2-Fluorophenol

Concen: 0.158 ng

RT: 5.20 min Scan# 294

Delta R.T. 0.00 min

Lab File: BN010929.D

Acq: 17 Jun 2020 05:41

Instrument :

BNA_N

ClientSampleId :

RE123D2-20200612


Tot Ion: 112 Resp: 711

Ion Ratio Lower Upper

112 100

64 46.1 37.4 56.0




63 26.0 22.2 33.4

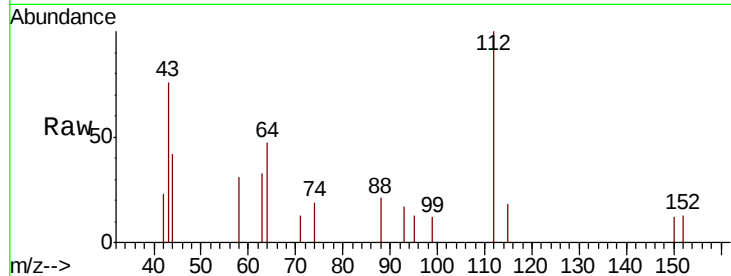

Abundance Ion 112.00 (111.70 to 112.70): B

Ion 64.00 (63.70 to 64.70): BNO

Ion 63.00 (62.70 to 63.70): BNO

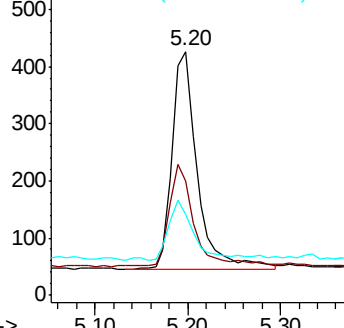

#5

Phenol-d6

Concen: 0.087 ng

RT: 6.74 min Scan# 485

Delta R.T. -0.01 min

Lab File: BN010929.D

Acq: 17 Jun 2020 05:41


Tgt Ion: 99 Resp: 462

Ion Ratio Lower Upper

99 100

42 25.8 11.1 16.7#



71 45.7 31.4 47.2




Abundance Ion 99.00 (98.70 to 99.70): BNO

Ion 42.00 (41.70 to 42.70): BNO

Ion 71.00 (70.70 to 71.70): BNO

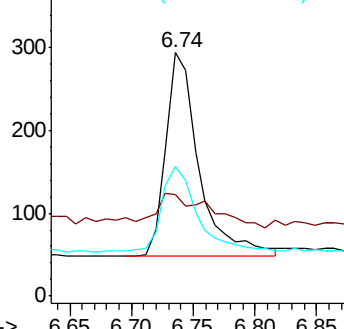



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.29 min Scan# 837

Delta R.T. -0.01 min

Lab File: BN010929.D

Acq: 17 Jun 2020 05:41

Instrument :

BNA_N

ClientSampleId :

RE123D2-20200612

Tot Ion:136 Resp: 7999


Ion Ratio Lower Upper

136 100

137 11.9 9.7 14.5

54 5.2 4.9 7.3

68 6.1 4.7 7.1



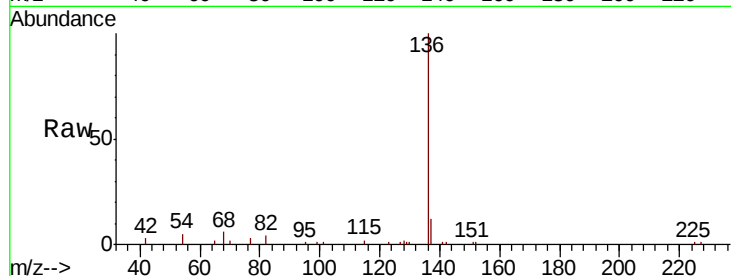


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BNC

Ion 68.00 (67.70 to 68.70): BNC

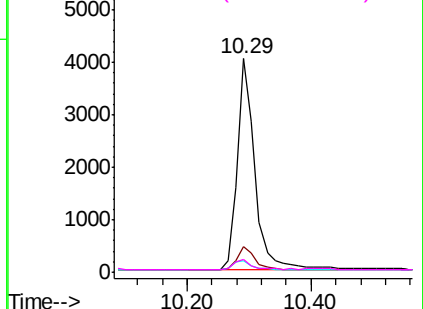

#8

Nitrobenzene-d5

Concen: 0.397 ng

RT: 8.68 min Scan# 710

Delta R.T. 0.00 min

Lab File: BN010929.D

Acq: 17 Jun 2020 05:41


Tgt Ion: 82 Resp: 2351

Ion Ratio Lower Upper

82 100

128 44.3 35.4 53.0



54 34.5 28.2 42.4




Abundance Ion 82.00 (81.70 to 82.70): BNC

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BNC



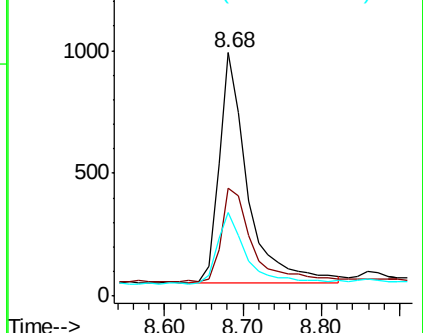



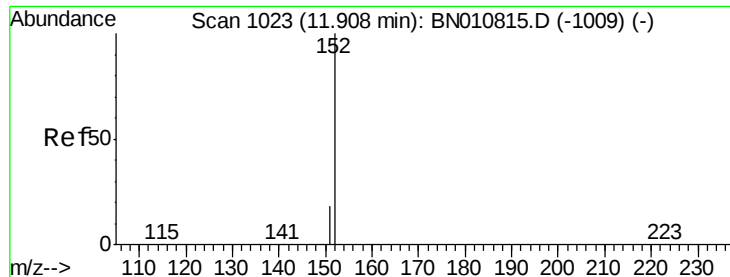

#11
2-Methylnaphthalene-d10
Concen: 0.454 ng
RT: 11.89 min Scan# 1019
Delta R.T. -0.00 min
Lab File: BN010929.D
Acq: 17 Jun 2020 05:41




Instrument :
BNA_N
ClientSampleId :
RE123D2-20200612


Tot Ion:152 Resp: 5630
Ion Ratio Lower Upper
152 100
151 19.2 15.3 22.9

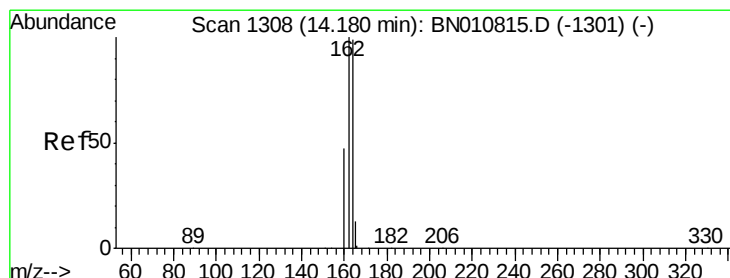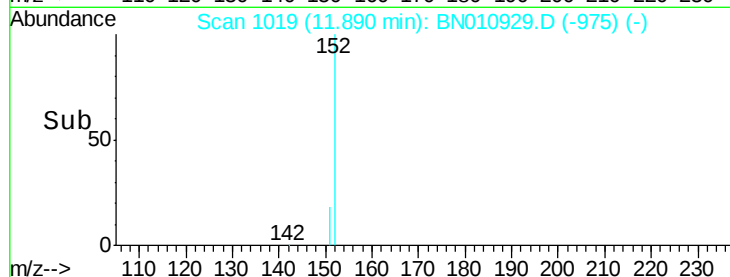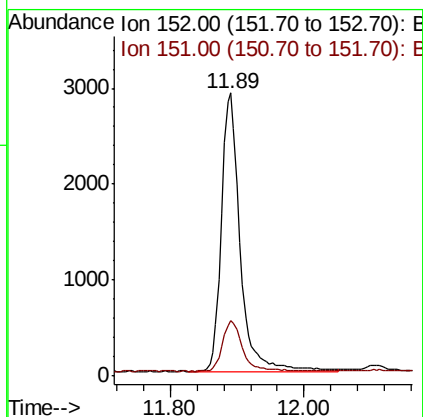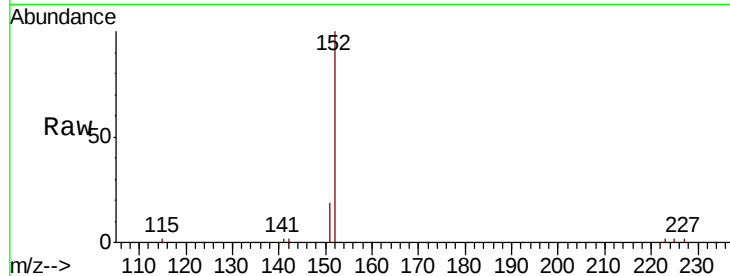

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.16 min Scan# 1306
Delta R.T. -0.00 min
Lab File: BN010929.D
Acq: 17 Jun 2020 05:41

Tgt Ion:164 Resp: 4706
Ion Ratio Lower Upper
164 100
162 101.4 81.0 121.6
160 47.4 38.9 58.3


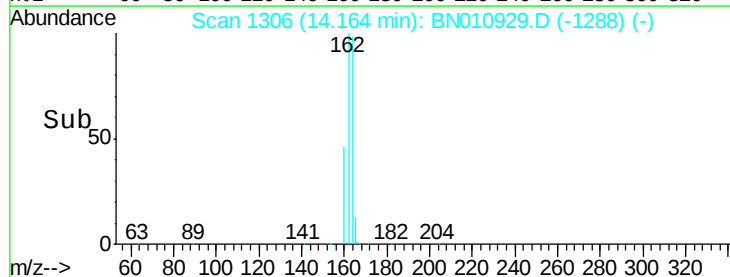
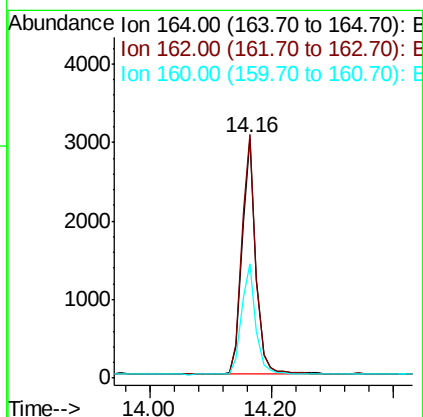
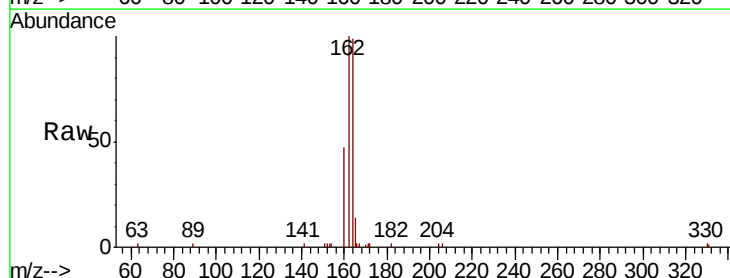


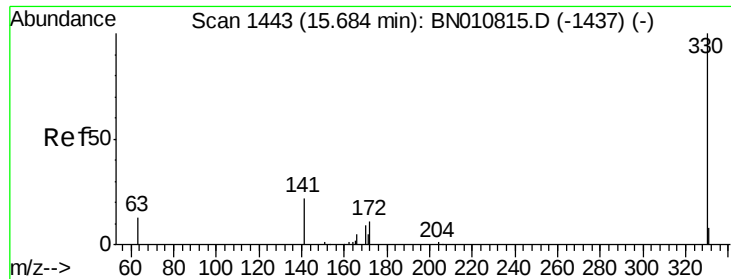

#14
 2,4,6-Tribromophenol
 Concen: 0.320 ng
 RT: 15.67 min Scan# 1441
 Delta R.T. -0.00 min
 Lab File: BN010929.D
 Acq: 17 Jun 2020 05:41




Instrument :
 BNA_N
 ClientSampleId :
 RE123D2-20200612


Tot Ion:330 Resp: 538
 Ion Ratio Lower Upper
 330 100
 332 0.0 0.0 0.0
 141 38.8 33.2 49.8

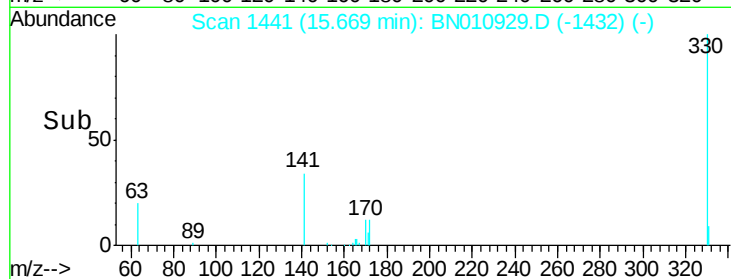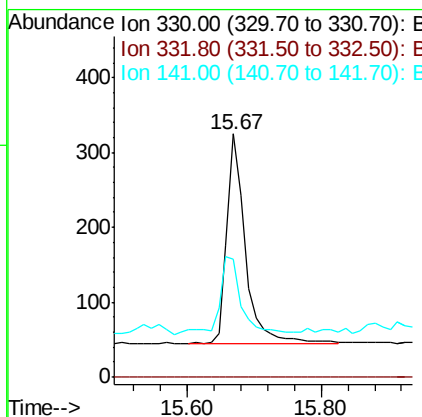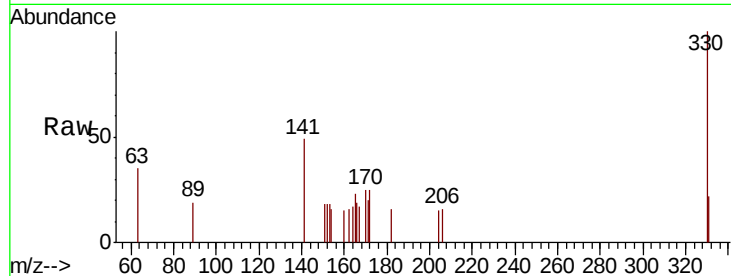

#15
 2-Fluorobiphenyl
 Concen: 0.387 ng
 RT: 12.78 min Scan# 1182
 Delta R.T. -0.00 min
 Lab File: BN010929.D
 Acq: 17 Jun 2020 05:41

Tgt Ion:172 Resp: 7195
 Ion Ratio Lower Upper
 172 100
 171 35.8 28.5 42.7
 170 23.9 19.7 29.5

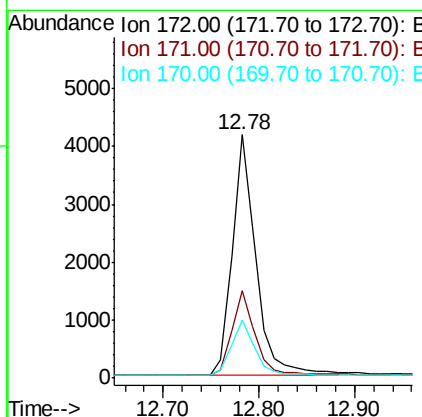

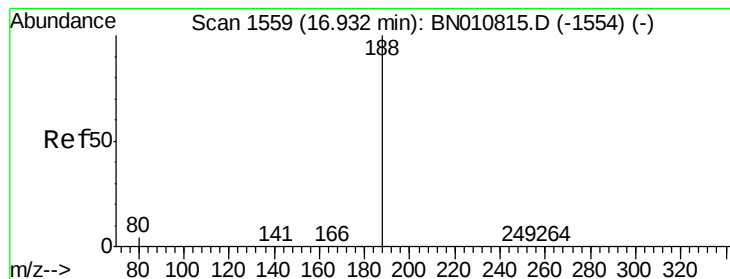

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.92 min Scan# 1557

Delta R.T. -0.00 min

Lab File: BN010929.D

Acq: 17 Jun 2020 05:41

Instrument :

BNA_N

ClientSampleId :

RE123D2-20200612


Tot Ion:188 Resp: 9062

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 7.4 4.5 6.7#

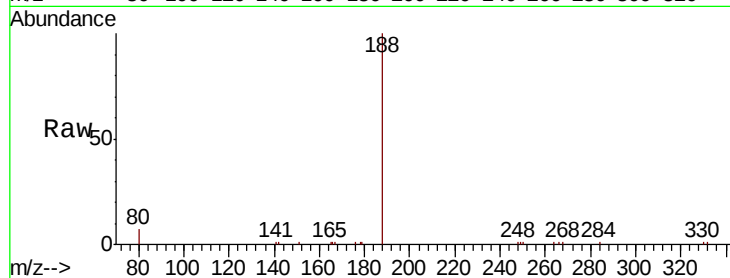

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BNO

Ion 80.00 (79.70 to 80.70): BNO

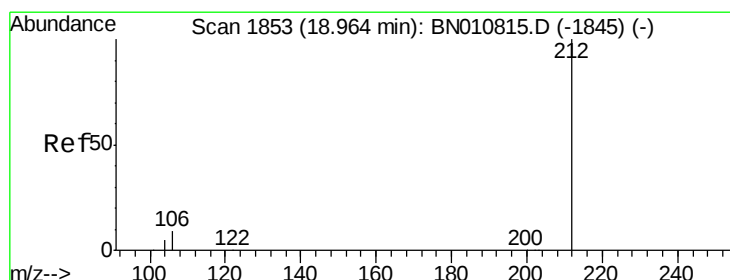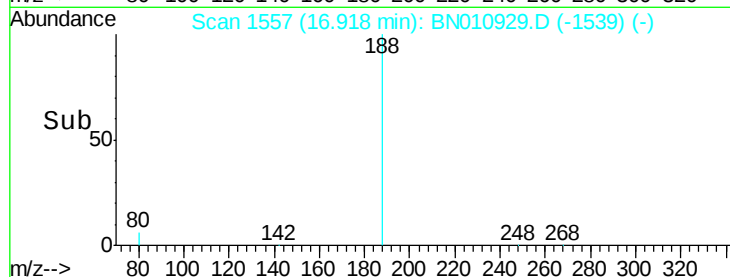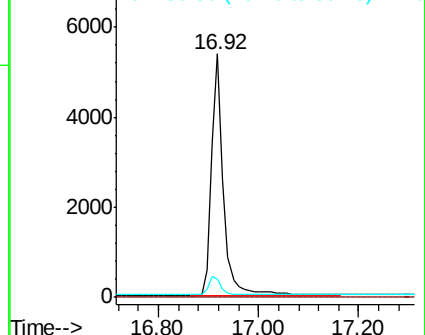

#25

Fluoranthene-d10

Concen: 0.548 ng

RT: 18.95 min Scan# 1849

Delta R.T. -0.01 min

Lab File: BN010929.D

Acq: 17 Jun 2020 05:41


Tgt Ion:212 Resp: 13717

Ion Ratio Lower Upper

212 100

106 9.6 6.6 10.0



104 5.4 4.0 6.0

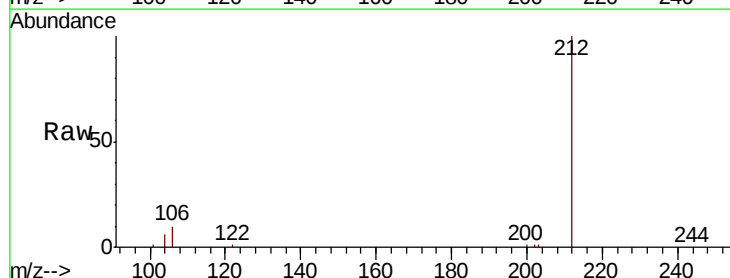


Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E



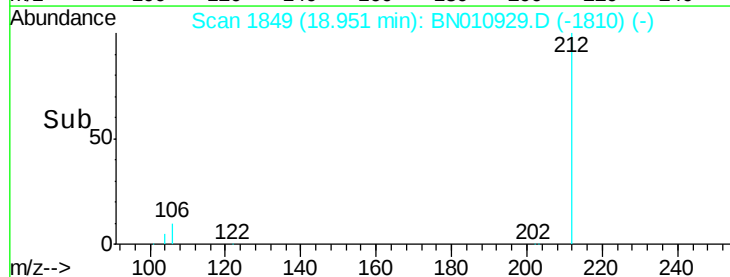
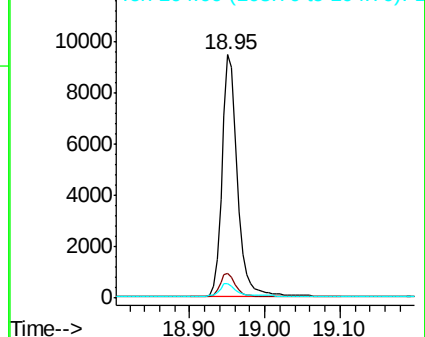




#27
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.12 min Scan# 2167
 Delta R.T. -0.01 min
 Lab File: BN010929.D
 Acq: 17 Jun 2020 05:41




Instrument :
 BNA_N
 ClientSampleId :
 RE123D2-20200612


Tot Ion:240 Resp: 8440
 Ion Ratio Lower Upper
 240 100
 120 8.3 7.5 11.3
 236 27.1 22.3 33.5

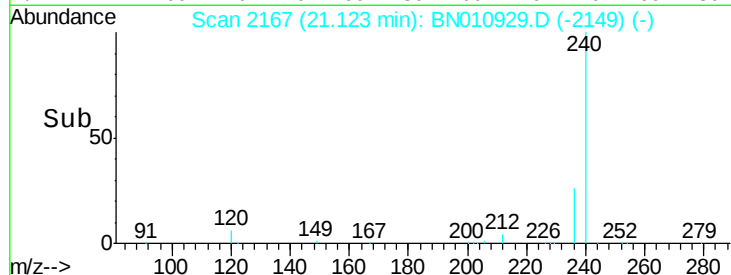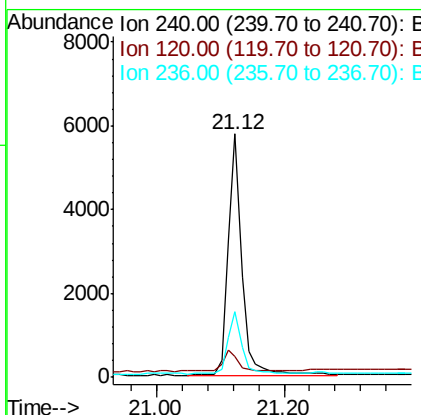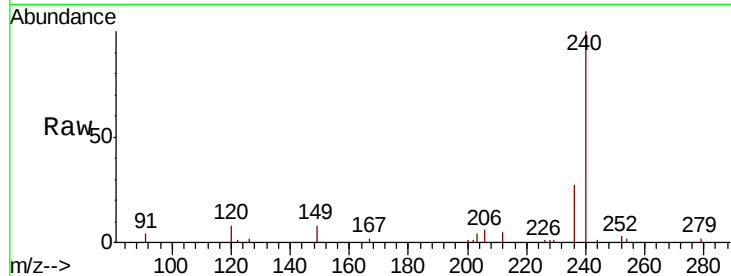

#29
 Terphenyl-d14
 Concen: 0.504 ng
 RT: 19.57 min Scan# 1973
 Delta R.T. -0.01 min
 Lab File: BN010929.D
 Acq: 17 Jun 2020 05:41

Tgt Ion:244 Resp: 9949
 Ion Ratio Lower Upper
 244 100
 212 8.2 7.4 11.2
 122 9.1 7.5 11.3

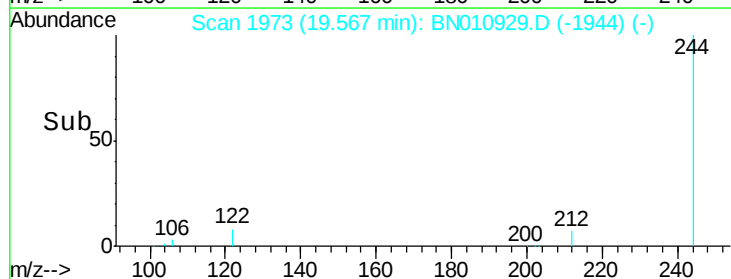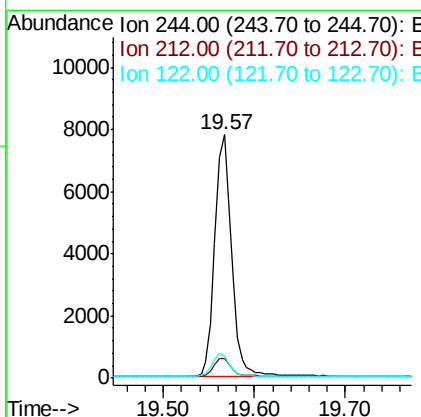

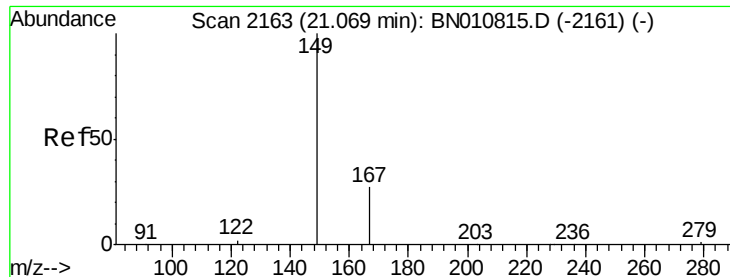

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.092 ng

RT: 21.06 min Scan# 2161

Delta R.T. -0.01 min

Lab File: BN010929.D

Acq: 17 Jun 2020 05:41

Instrument :

BNA_N

ClientSampleId :

RE123D2-20200612


Tot Ion:149 Resp: 758

Ion Ratio Lower Upper

149 100

167 26.9 24.1 36.1




279 7.7 4.6 7.0#

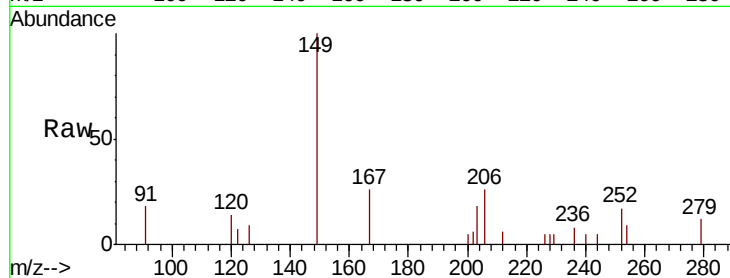

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

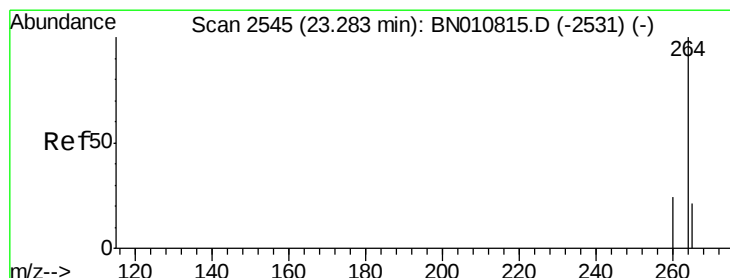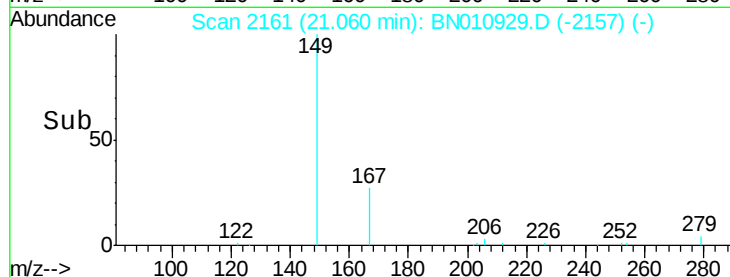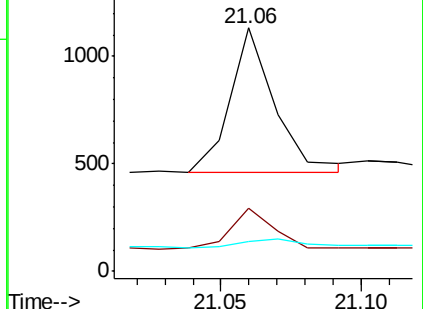

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.27 min Scan# 2539

Delta R.T. -0.01 min

Lab File: BN010929.D

Acq: 17 Jun 2020 05:41


Tgt Ion:264 Resp: 8662

Ion Ratio Lower Upper

264 100

260 24.8 20.4 30.6

265 83.6 75.0 112.4

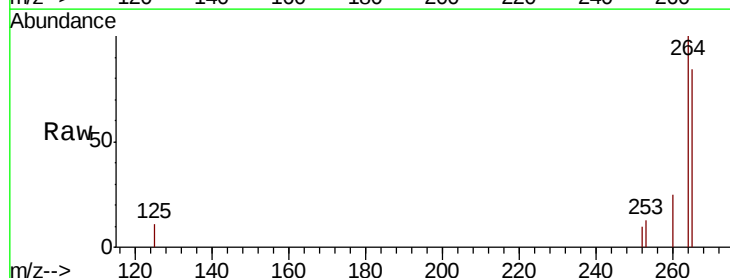

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

