


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061620\
 Data File : BN010902.D
 Acq On : 16 Jun 2020 11:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN061020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 16 08:49:35 2020

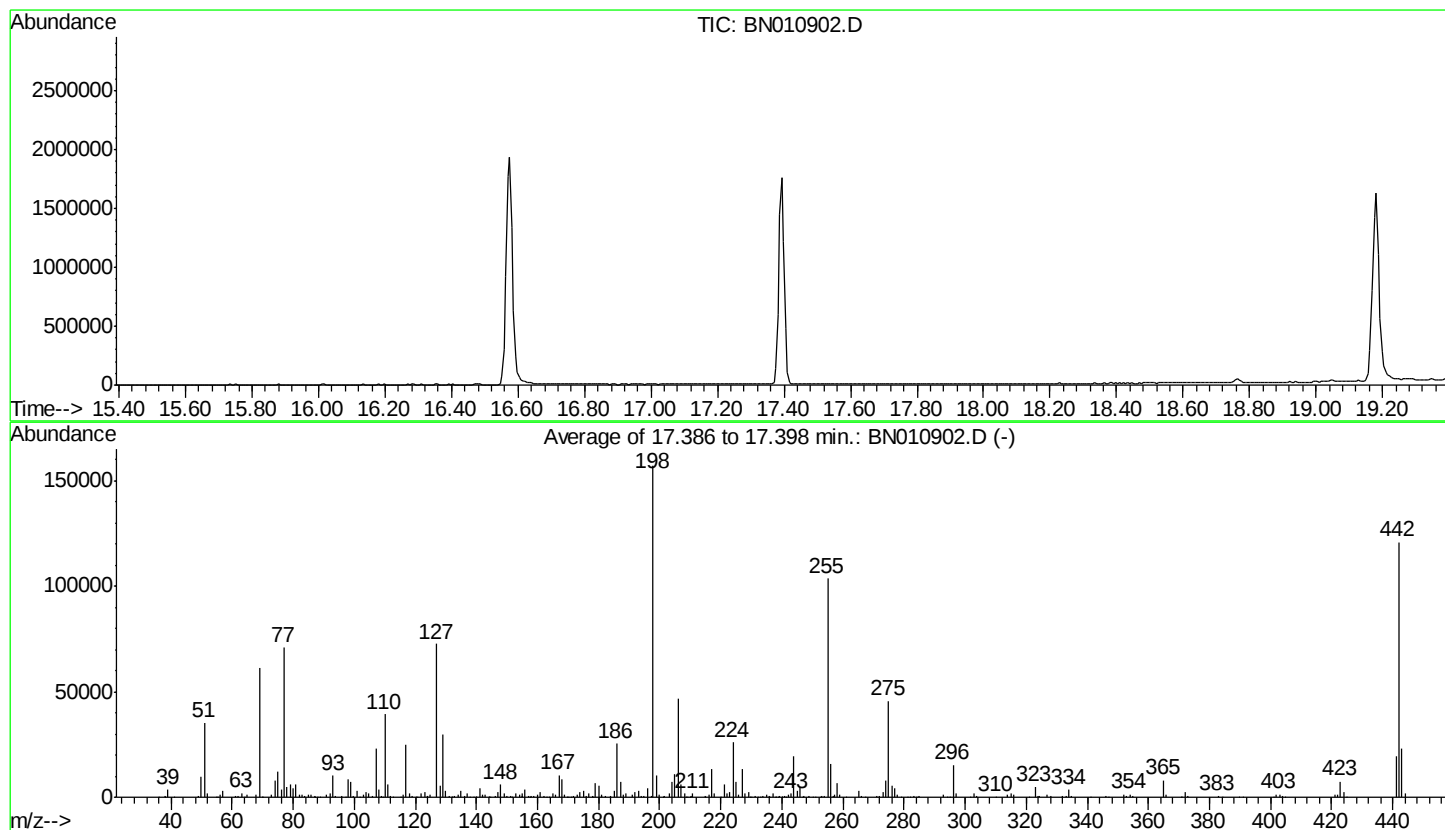

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.6	35464	PASS
68	69	0.00	2	2.0	1221	PASS
69	198	0.00	100	38.9	61106	PASS
70	69	0.00	2	0.3	165	PASS
127	198	10	80	46.2	72552	PASS
197	198	0.00	2	0.3	505	PASS
198	198	100	100	100.0	157184	PASS
199	198	5	9	6.5	10276	PASS
275	198	10	60	29.1	45810	PASS
365	198	1	100	5.1	7993	PASS
441	198	0.01	100	12.4	19539	PASS
442	198	50	100	76.9	120877	PASS
443	442	15	24	19.1	23034	PASS