


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN061620\
 Data File : BN010920.D
 Acq On : 17 Jun 2020 00:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN061020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 16 08:49:35 2020

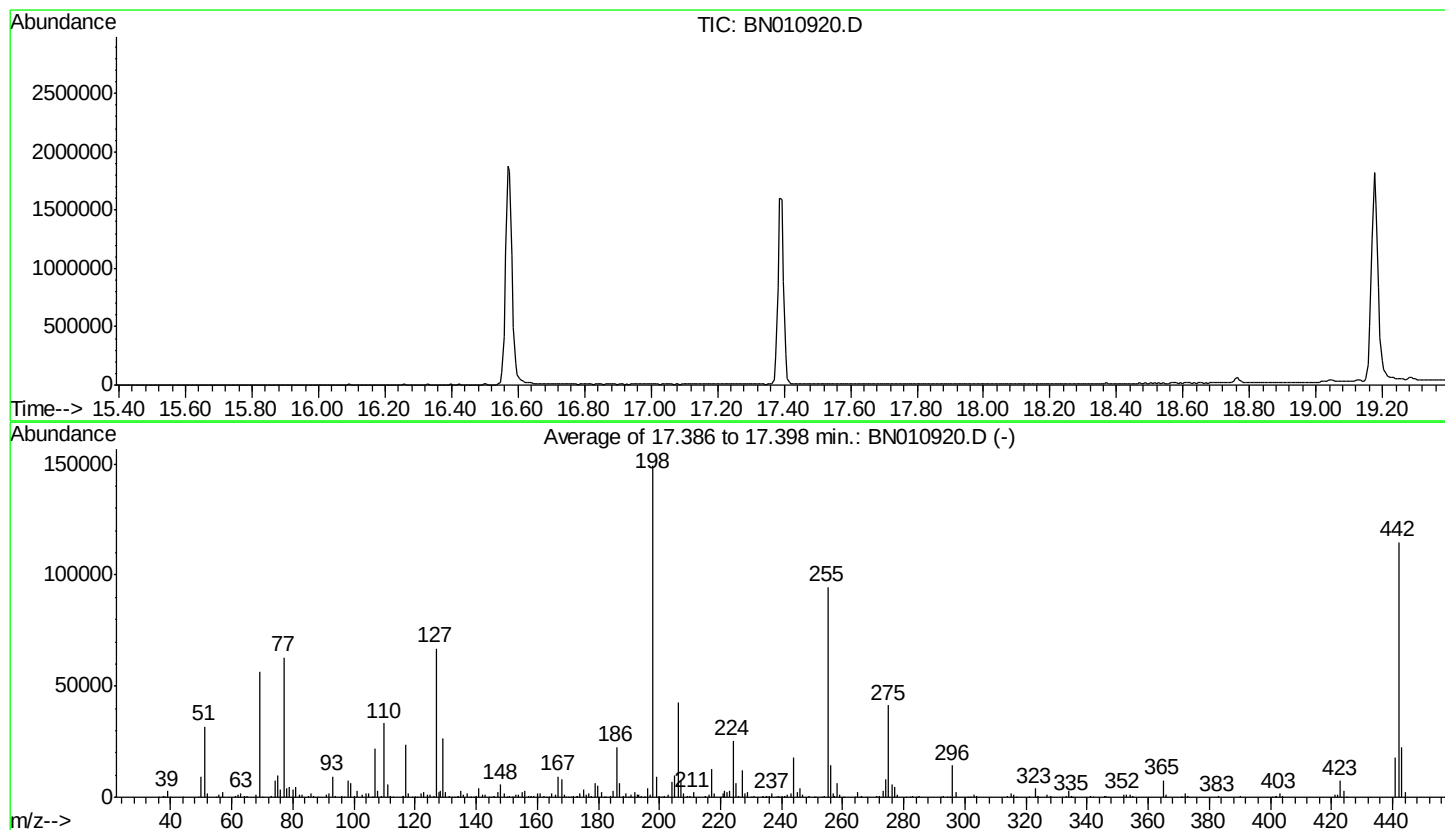

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.4	32000	PASS
68	69	0.00	2	2.0	1113	PASS
69	198	0.00	100	37.8	56384	PASS
70	69	0.00	2	0.4	245	PASS
127	198	10	80	44.9	67050	PASS
197	198	0.00	2	0.9	1362	PASS
198	198	100	100	100.0	149282	PASS
199	198	5	9	6.3	9439	PASS
275	198	10	60	27.6	41229	PASS
365	198	1	100	5.2	7769	PASS
441	198	0.01	100	11.9	17753	PASS
442	198	50	100	77.0	114957	PASS
443	442	15	24	19.3	22229	PASS