
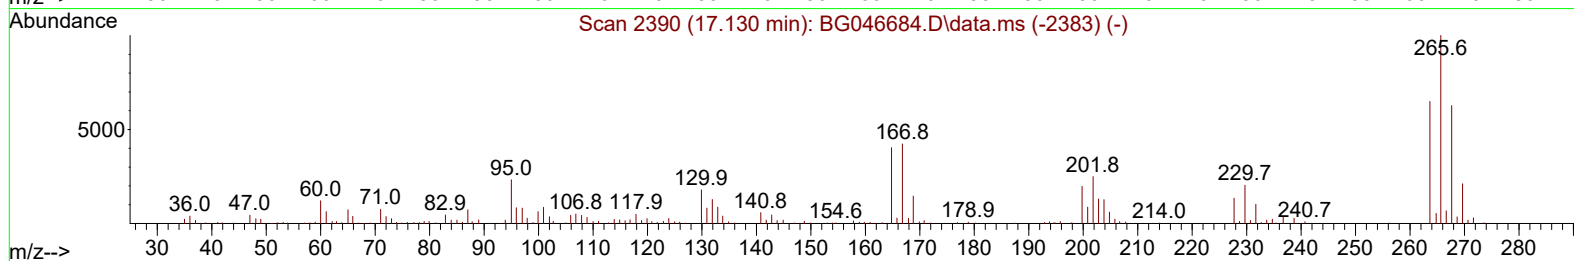
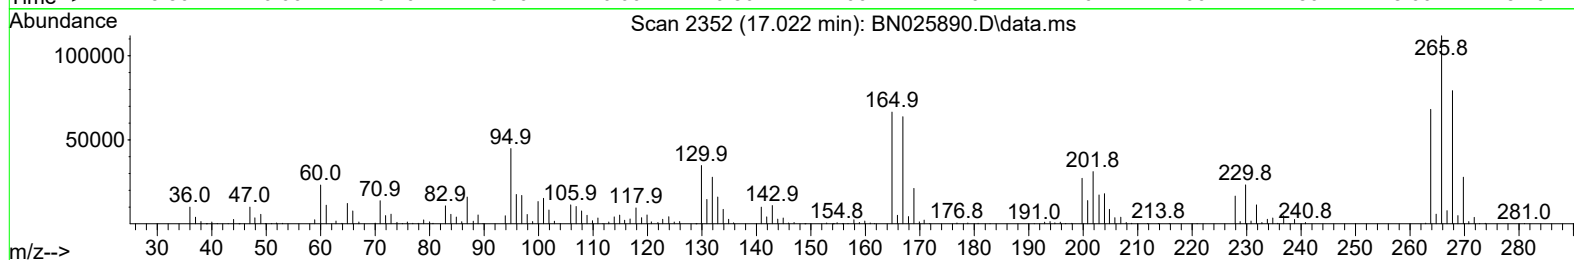


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061623\
Data File : BN025890.D
Acq On : 16 Jun 2023 22:08
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 05:05:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 17 05:04:09 2023
Response via : Initial Calibration

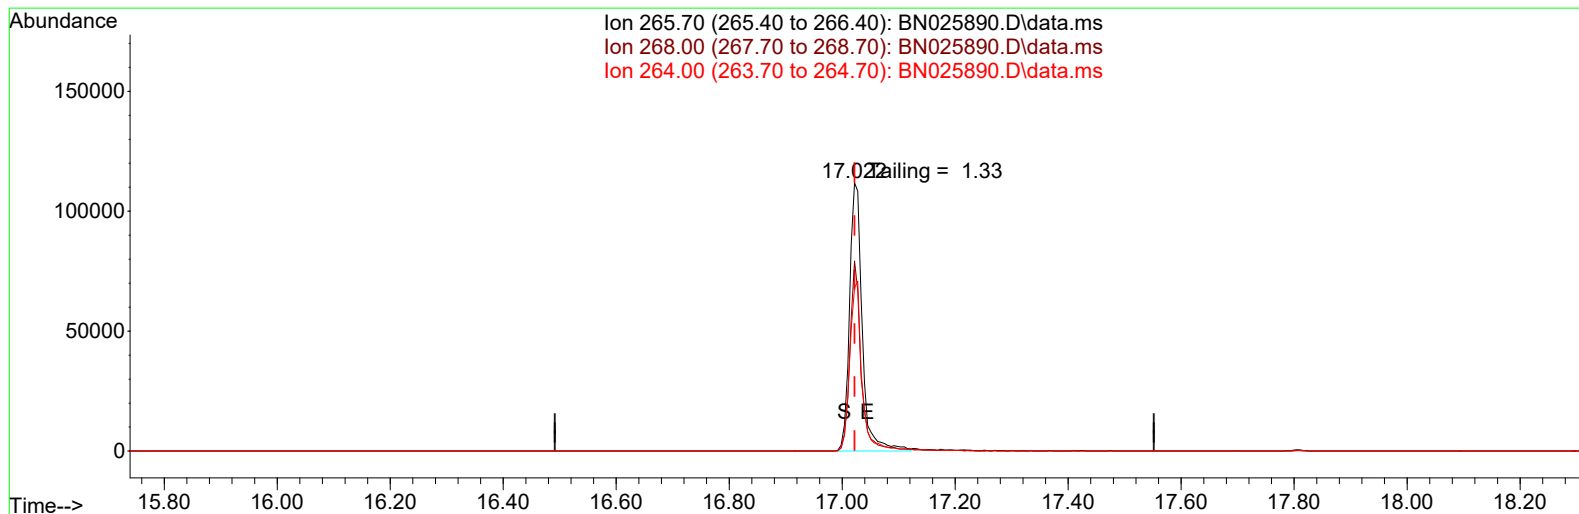

TIC: BN025890.D\data.ms

(70) Pentachlorophenol (C)




17.022min (-0.000) 12114.53 ng

response 176073

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	70.83
264.00	61.60	60.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061623\
Data File : BN025890.D
Acq On : 16 Jun 2023 22:08
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 05:05:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 17 05:04:09 2023
Response via : Initial Calibration

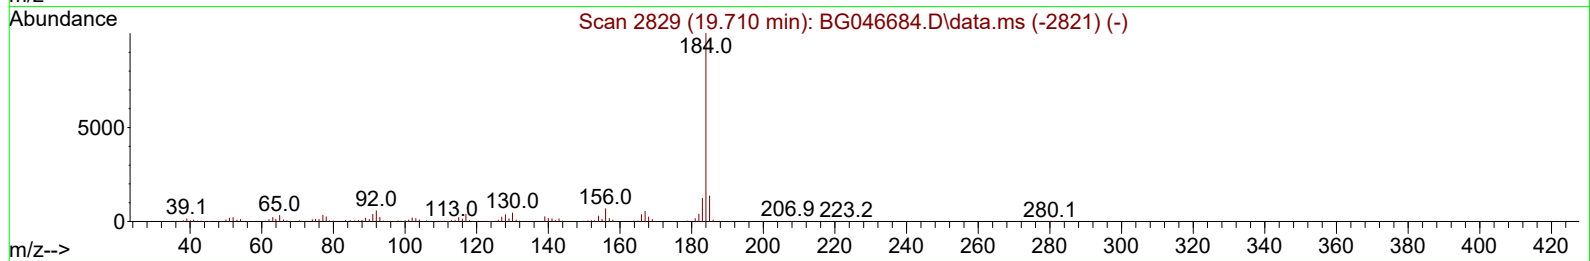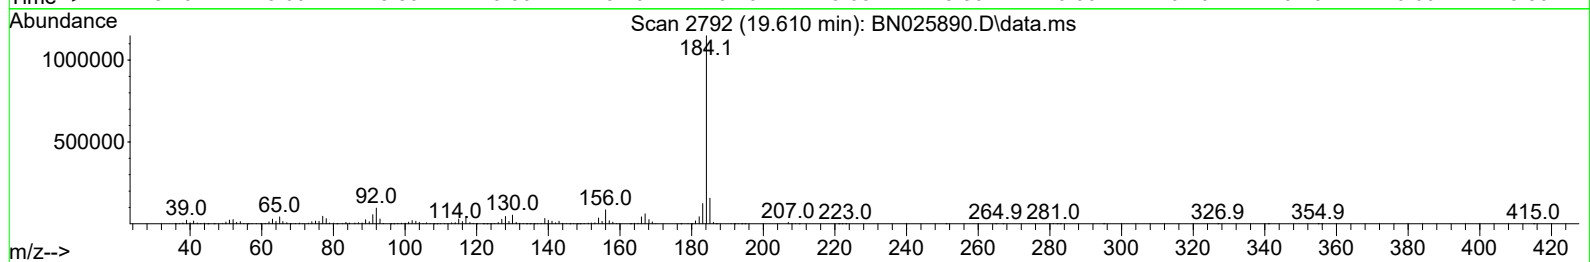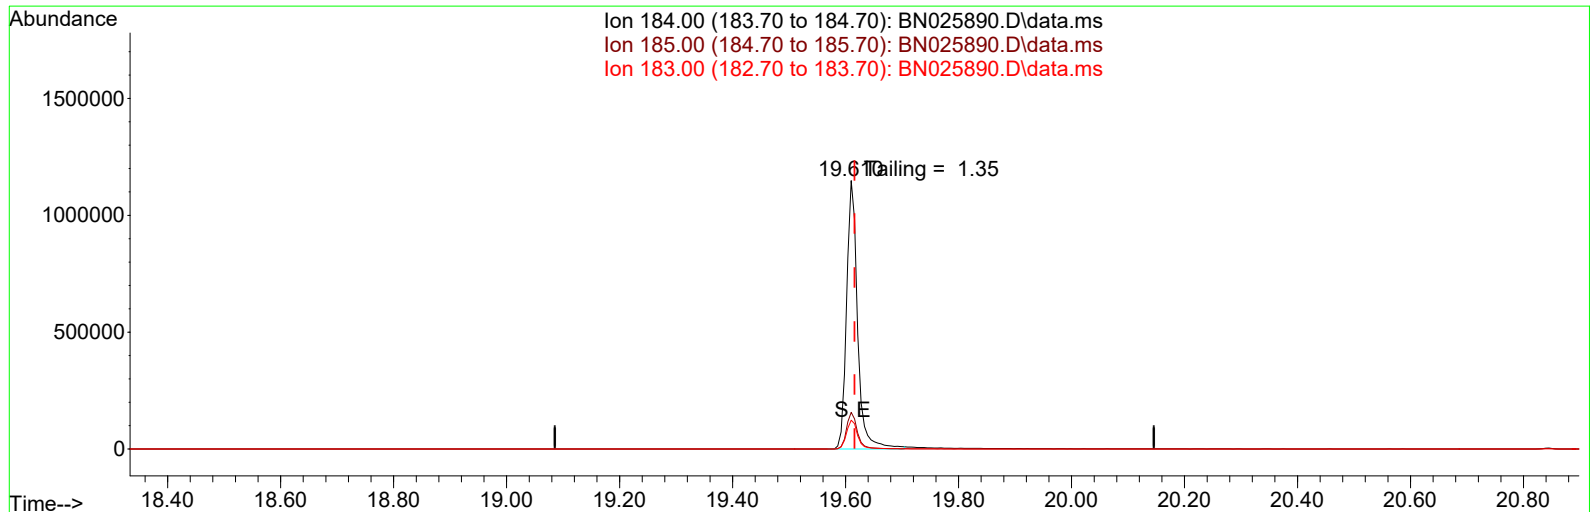

TIC: BN025890.D\data.ms

(77) Benzidine**19.610min (-0.006) 792603.12 ng****response 1539234**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.66
183.00	13.20	10.75
0.00	0.00	0.00