
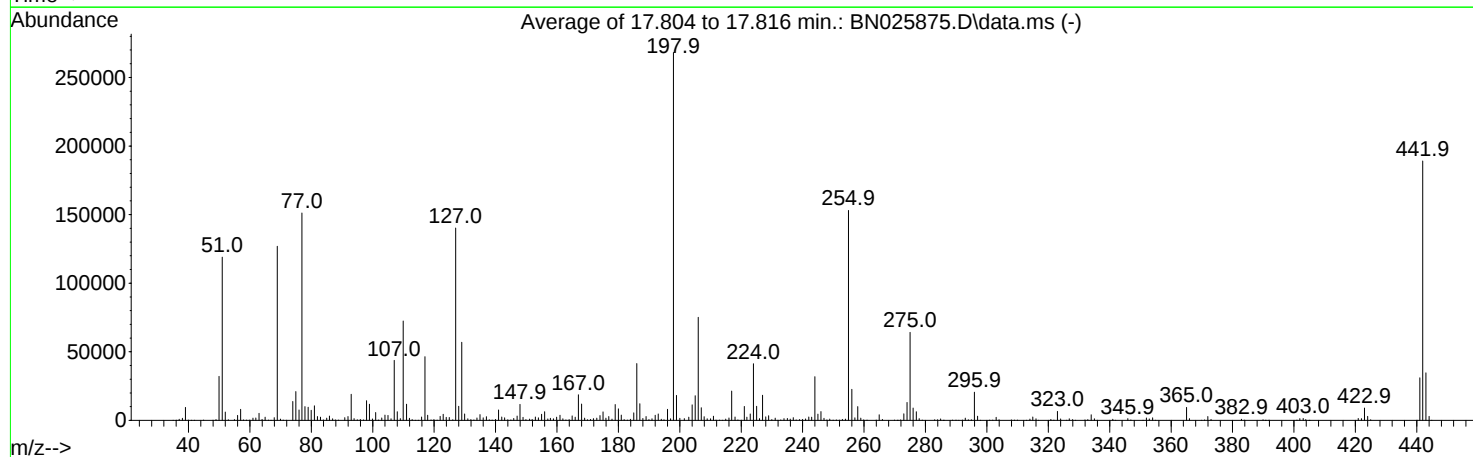


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061623\
 Data File : BN025875.D
 Acq On : 16 Jun 2023 10:11
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN053123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 16 14:10:48 2023

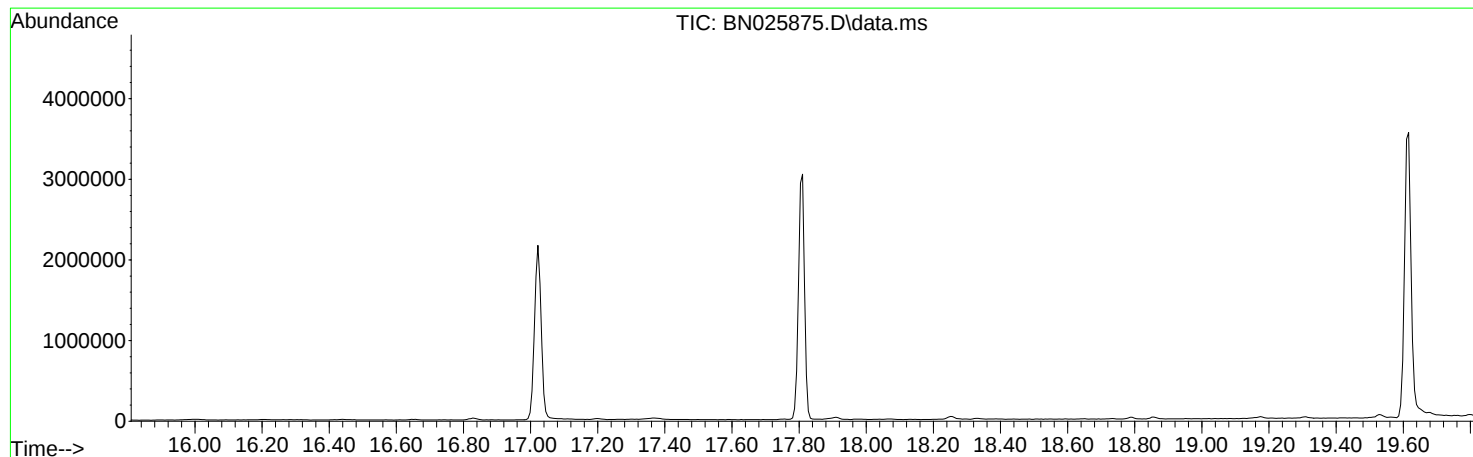

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.4	119053	PASS
68	69	0.00	2	1.6	2041	PASS
69	198	0.00	100	47.3	126914	PASS
70	69	0.00	2	0.7	889	PASS
127	198	10	80	52.3	140245	PASS
197	198	0.00	2	0.4	1204	PASS
198	198	100	100	100.0	268203	PASS
199	198	5	9	6.8	18219	PASS
275	198	10	60	23.9	64187	PASS
365	198	1	100	3.5	9461	PASS
441	198	0.01	100	11.6	31011	PASS
442	442	50	100	100.0	189120	PASS
443	442	15	24	18.3	34619	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/16/2023	BNA_N	<u>BN025875.D</u>
Compound Name	Response	Retention Time
DDT	925971	20.851
DDD	20865	20.41
DDE	1134	19.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21999	947970	2.32

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061623\
Data File : BN025875.D
Acq On : 16 Jun 2023 10:11
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 17 05:04:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 17 05:04:09 2023
Response via : Initial Calibration

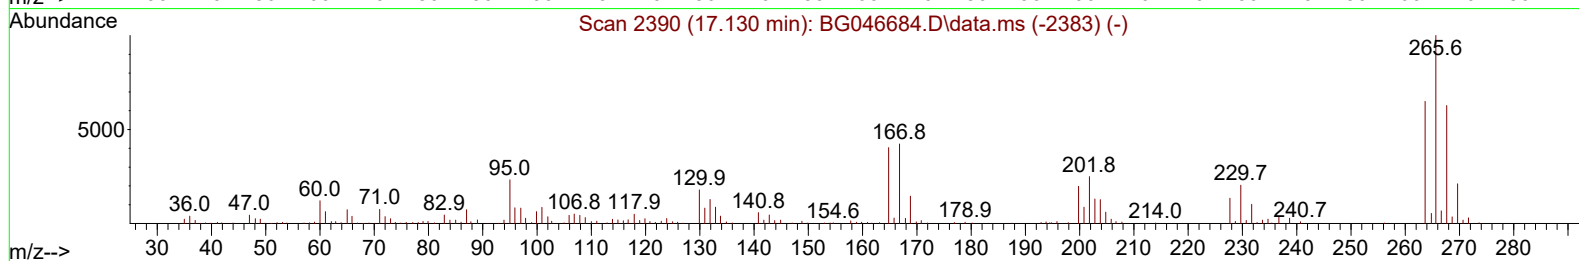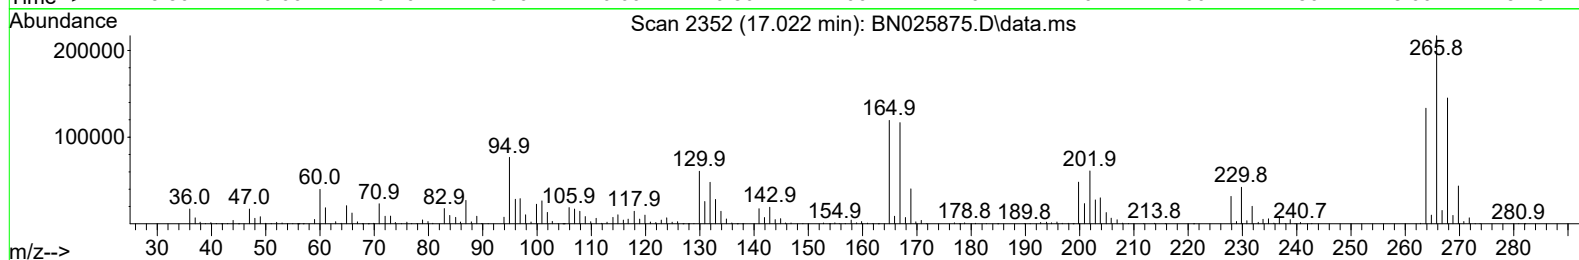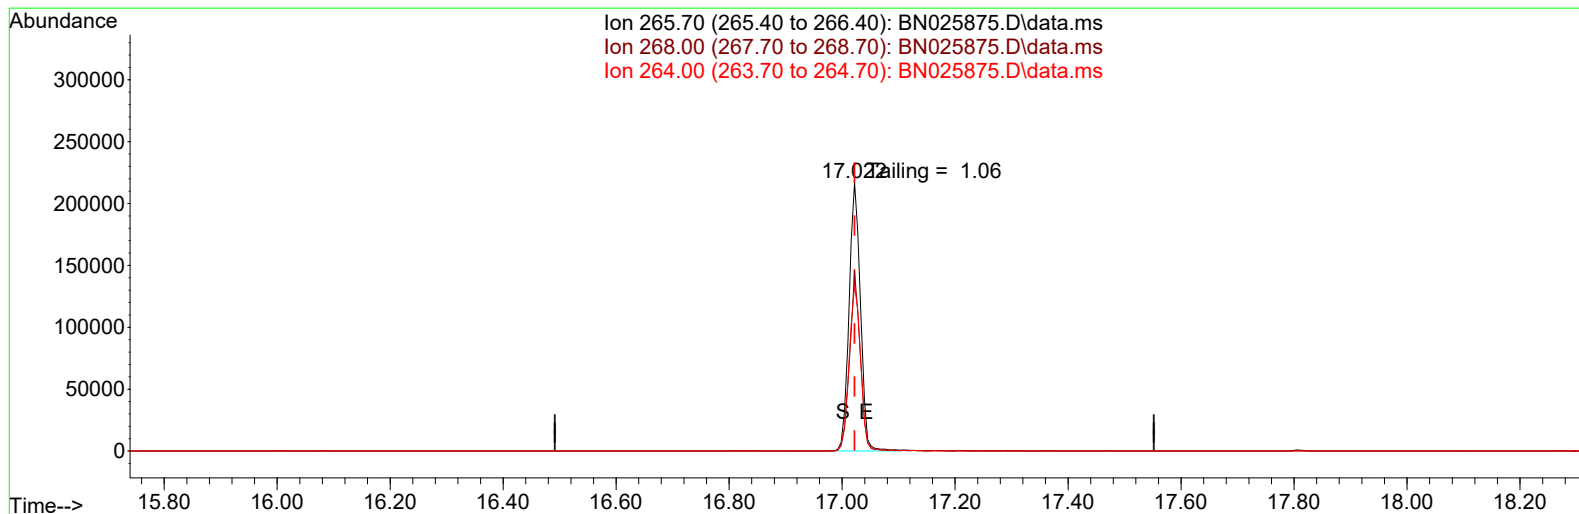

TIC: BN025875.D\data.ms

(70) Pentachlorophenol (C)

17.022min (0.000) 17602.60 ng




response 304186

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.89
264.00	61.60	61.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061623\
Data File : BN025875.D
Acq On : 16 Jun 2023 10:11
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 17 05:04:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 17 05:04:09 2023
Response via : Initial Calibration

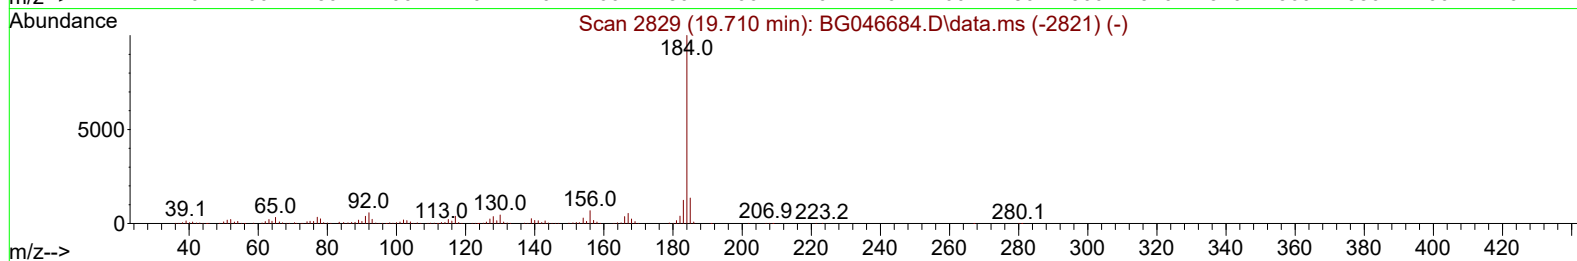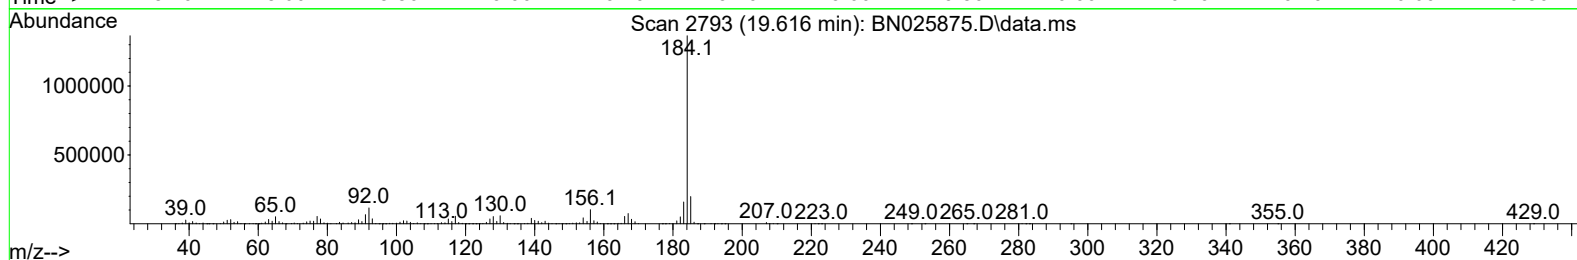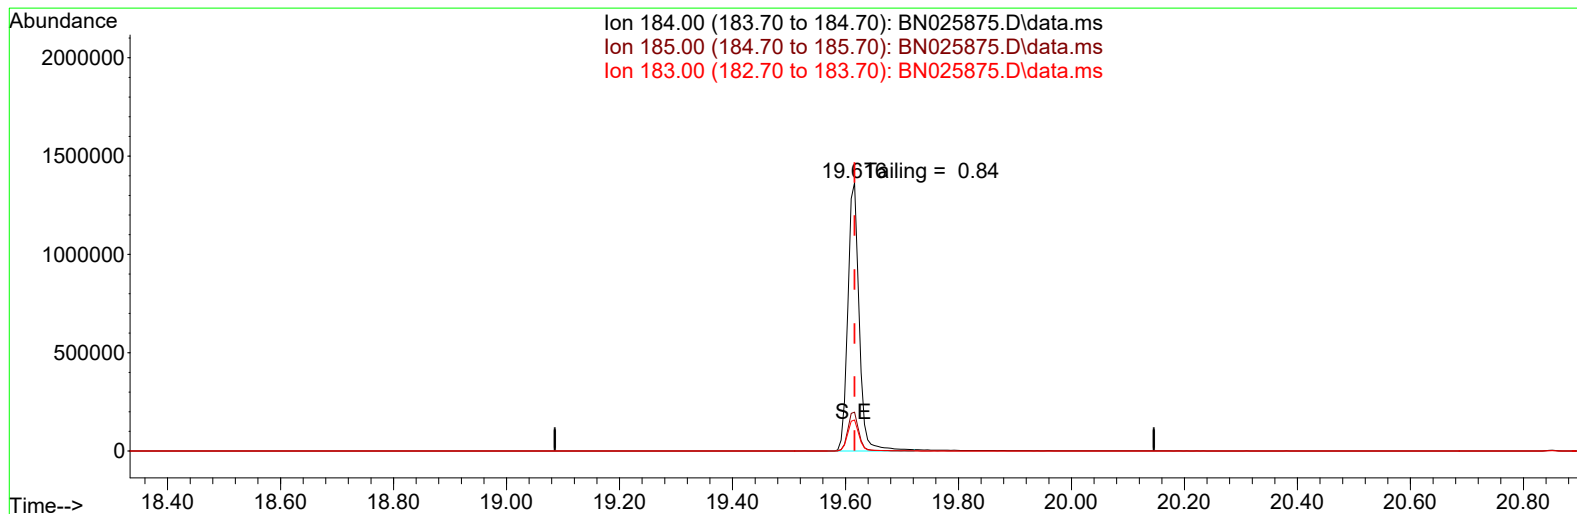

TIC: BN025875.D\data.ms

(77) Benzidine

19.616min (0.000) 19624.07 ng

response 1867991

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.52
183.00	13.20	11.58
0.00	0.00	0.00