


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061623\
Data File : BN025890.D
Acq On : 16 Jun 2023 22:08
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN053123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 16 14:10:48 2023

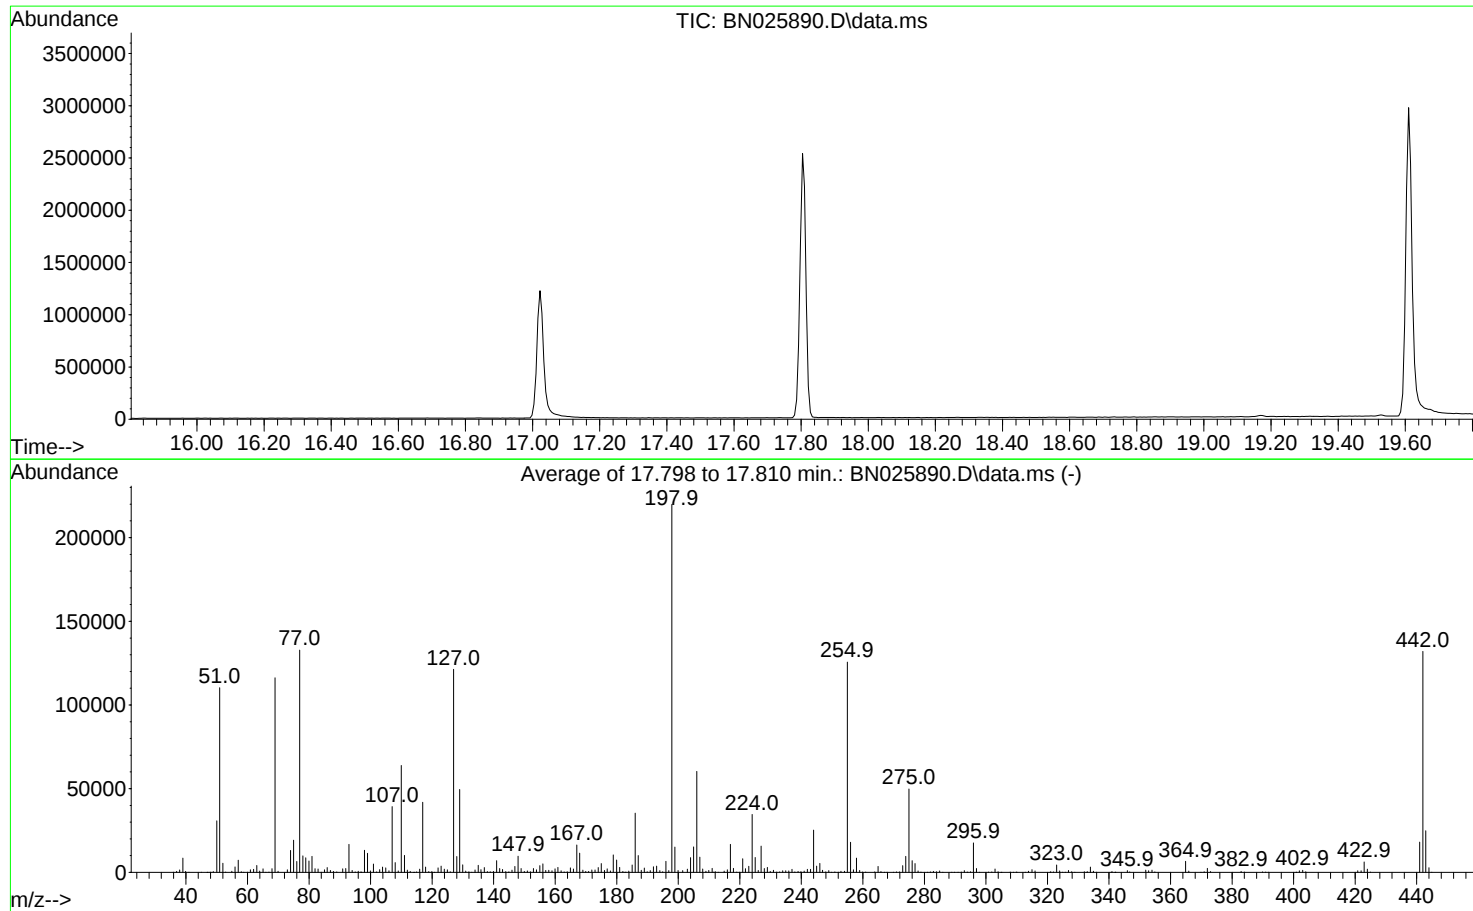

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.2	110304	PASS
68	69	0.00	2	1.9	2185	PASS
69	198	0.00	100	52.9	116237	PASS
70	69	0.00	2	0.6	680	PASS
127	198	10	80	55.2	121283	PASS
197	198	0.00	2	0.5	1033	PASS
198	198	100	100	100.0	219797	PASS
199	198	5	9	6.9	15159	PASS
275	198	10	60	22.7	49797	PASS
365	198	1	100	3.0	6586	PASS
441	198	0.01	100	8.2	18047	PASS
442	442	50	100	100.0	132005	PASS
443	442	15	24	18.9	24896	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/16/2023	BNA_N	<u>BN025890.D</u>
Compound Name	Response	Retention Time
DDT	708933	20.839
DDD	14358	20.404
DDE	827	19.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15185	724118	2.10

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061623\
Data File : BN025890.D
Acq On : 16 Jun 2023 22:08
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 17 05:05:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 17 05:04:09 2023
Response via : Initial Calibration

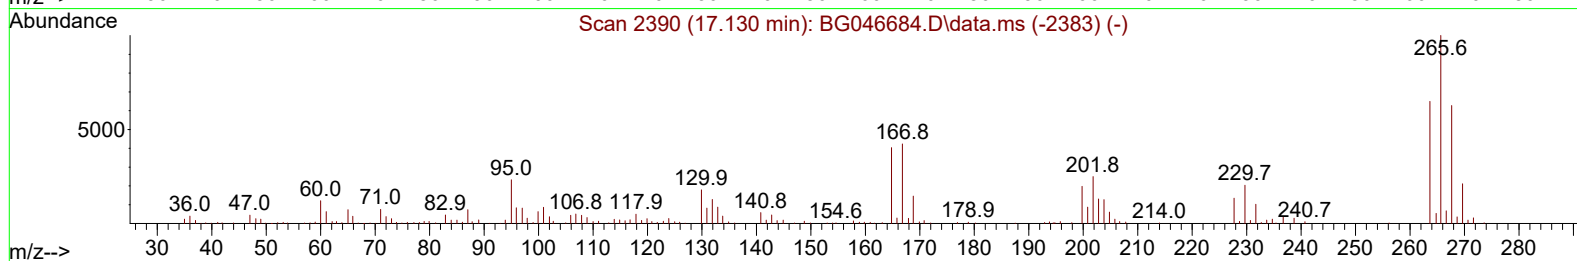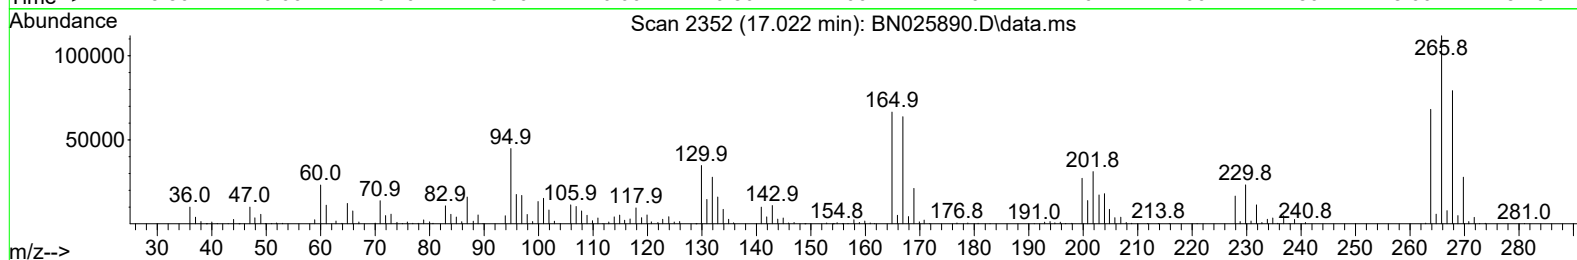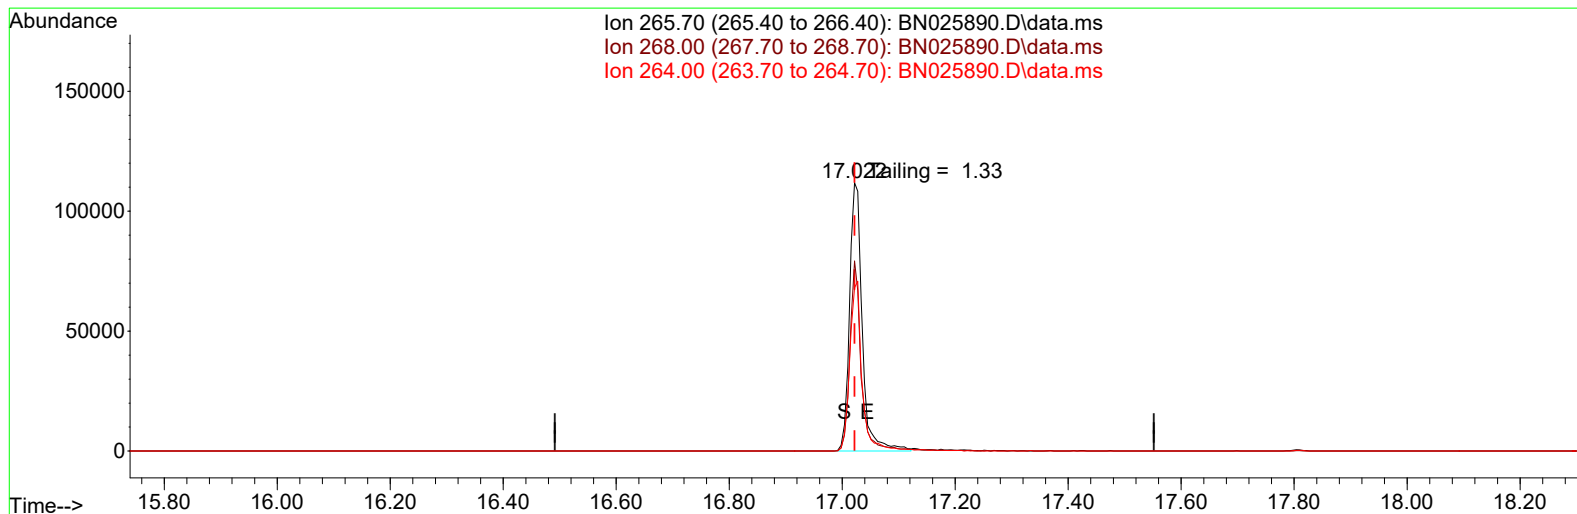

TIC: BN025890.D\data.ms

(70) Pentachlorophenol (C)

17.022min (-0.000) 12114.53 ng




response 176073

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	70.83
264.00	61.60	60.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061623\
Data File : BN025890.D
Acq On : 16 Jun 2023 22:08
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 17 05:05:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 17 05:04:09 2023
Response via : Initial Calibration

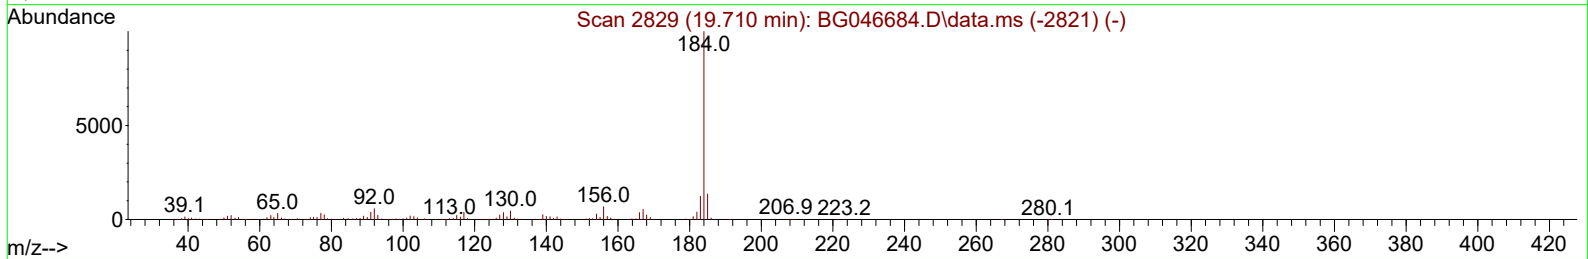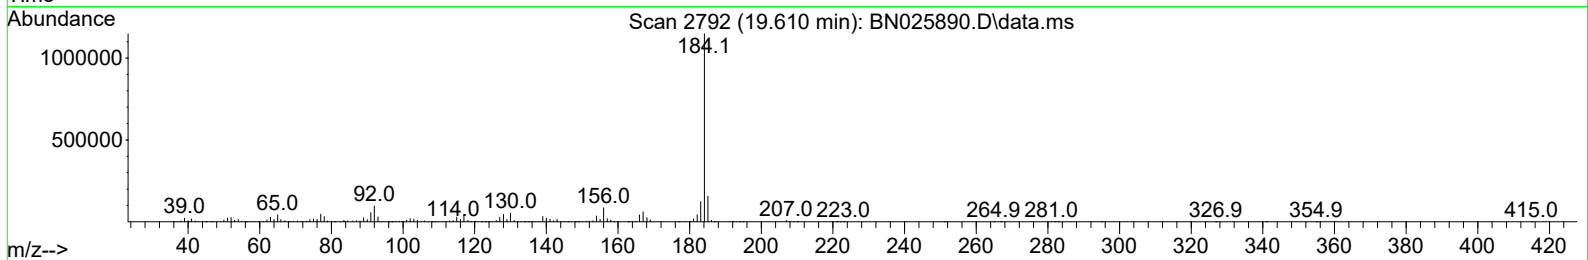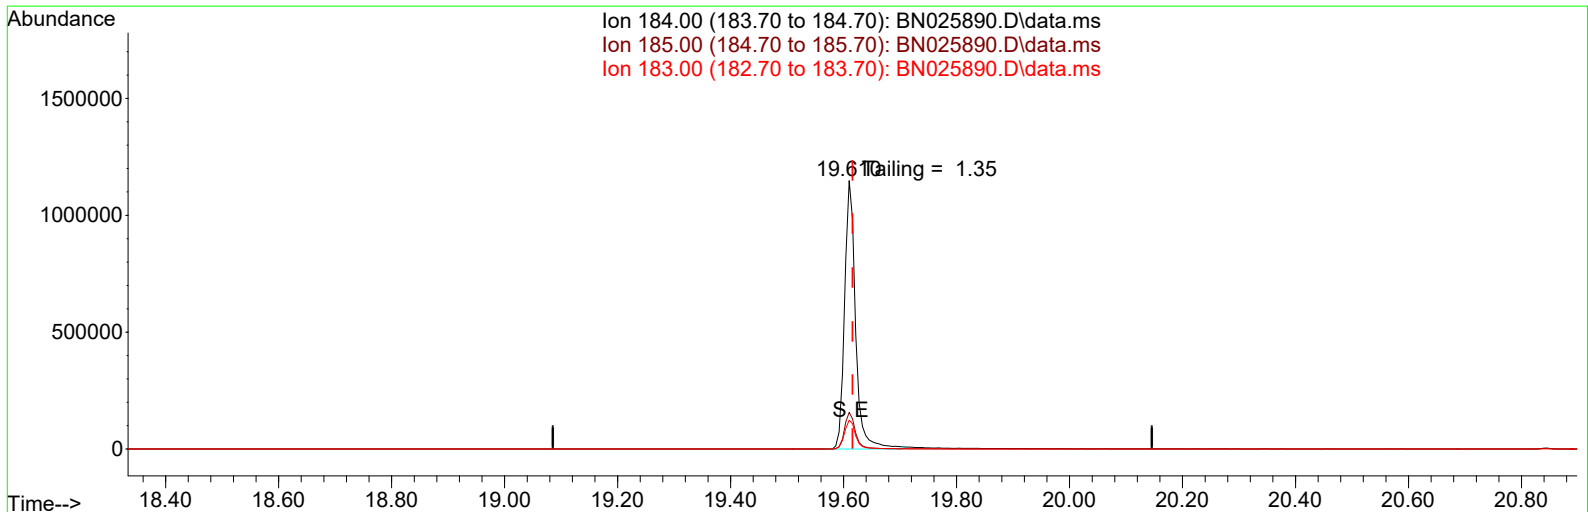

TIC: BN025890.D\data.ms

(77) Benzidine

19.610min (-0.006) 792603.12 ng

response 1539234

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.66
183.00	13.20	10.75
0.00	0.00	0.00