

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006347.D
 Acq On : 17 Jun 2019 14:41
 Operator : JU/SJ
 Sample : K3332-10
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 18 01:51:23 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	4596	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	18450	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.29	164	10086	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.15	188	1182858	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.27
20) Perylene-d12	23.36	264	904202	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	6054	0.21	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
3) Naphthalene	10.47	128	1486	0.029	ng/ul#	83
7) Acenaphthylene	14.01	152	7297	0.130	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
Data File : BN006347.D
Acq On : 17 Jun 2019 14:41
Operator : JU/SJ
Sample : K3332-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 18 01:51:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

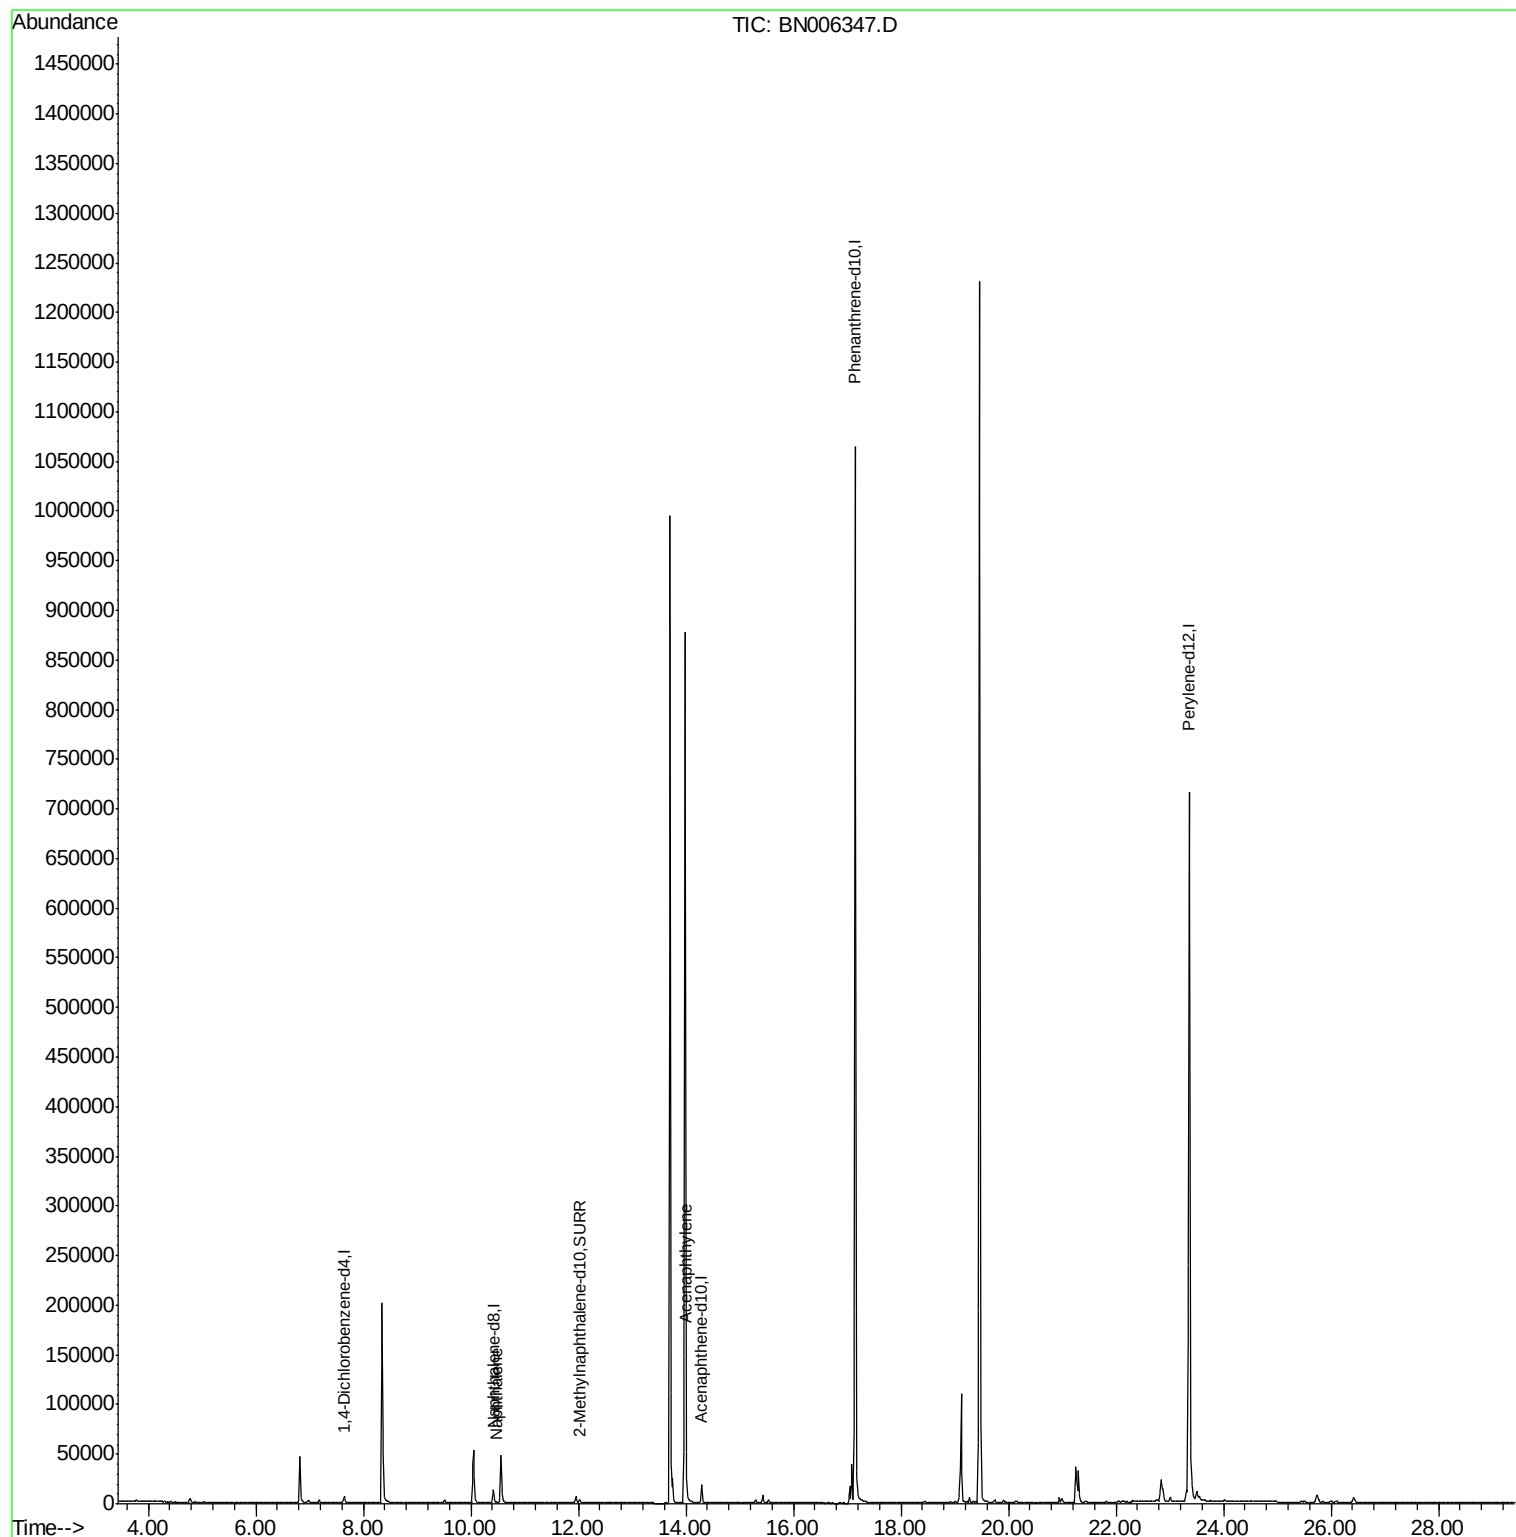

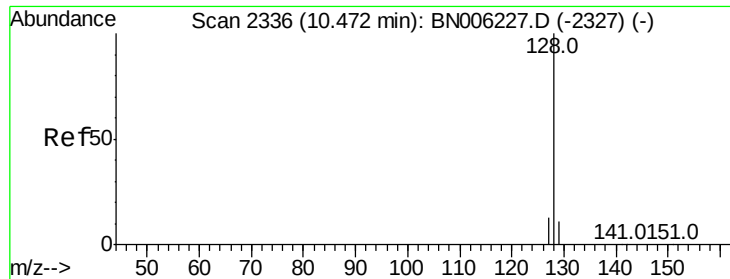

#3

Naphthalene

Concen: 0.029 ng/ul

RT: 10.47 min Scan# 2335

Delta R.T. -0.01 min

Lab File: BN006347.D

Acq: 17 Jun 2019 14:41

Instrument :

BNA_N

ClientSampleId :


Tot Ion:128 Resp: 1486

Ion Ratio Lower Upper

128 100

129 19.7 9.3 13.9#




127 18.5 10.7 16.1#

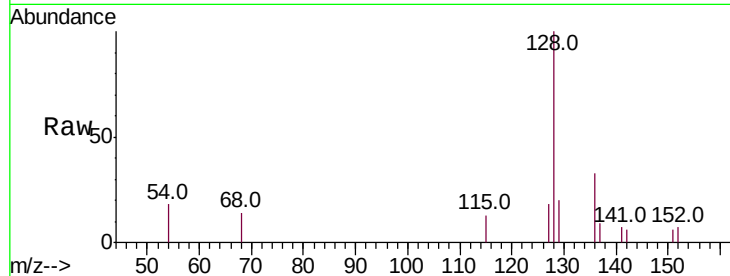

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

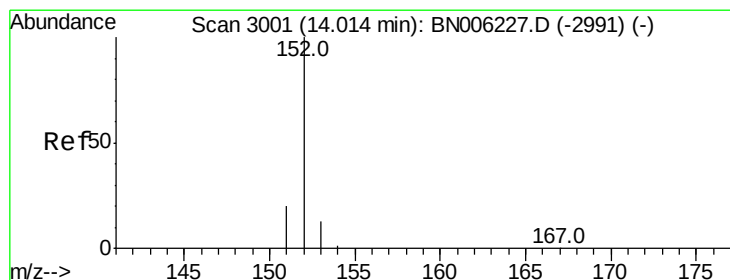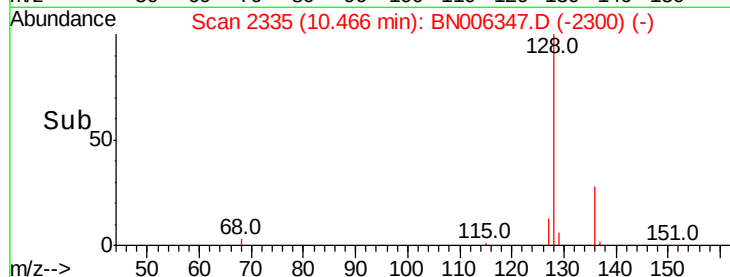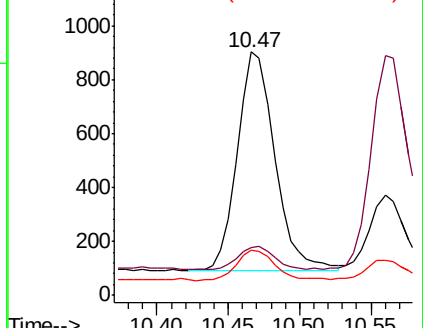

#7

Acenaphthylene

Concen: 0.130 ng/ul

RT: 14.01 min Scan# 3000

Delta R.T. 0.00 min

Lab File: BN006347.D

Acq: 17 Jun 2019 14:41


Tgt Ion:152 Resp: 7297

Ion Ratio Lower Upper

152 100

151 20.4 15.8 23.8

153 14.4 10.8 16.2

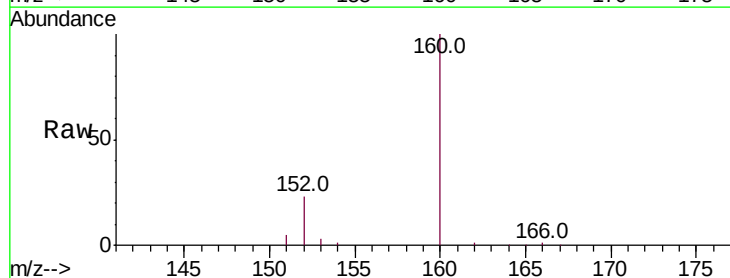

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

