


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
Data File : BN006357.D
Acq On : 17 Jun 2019 20:26
Operator : JU/SJ
Sample : K3332-24
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41W6

Manual Integrations
APPROVED

mohammad
6/21/2019 8:22:38 AM

Quant Time: Jun 18 03:59:12 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

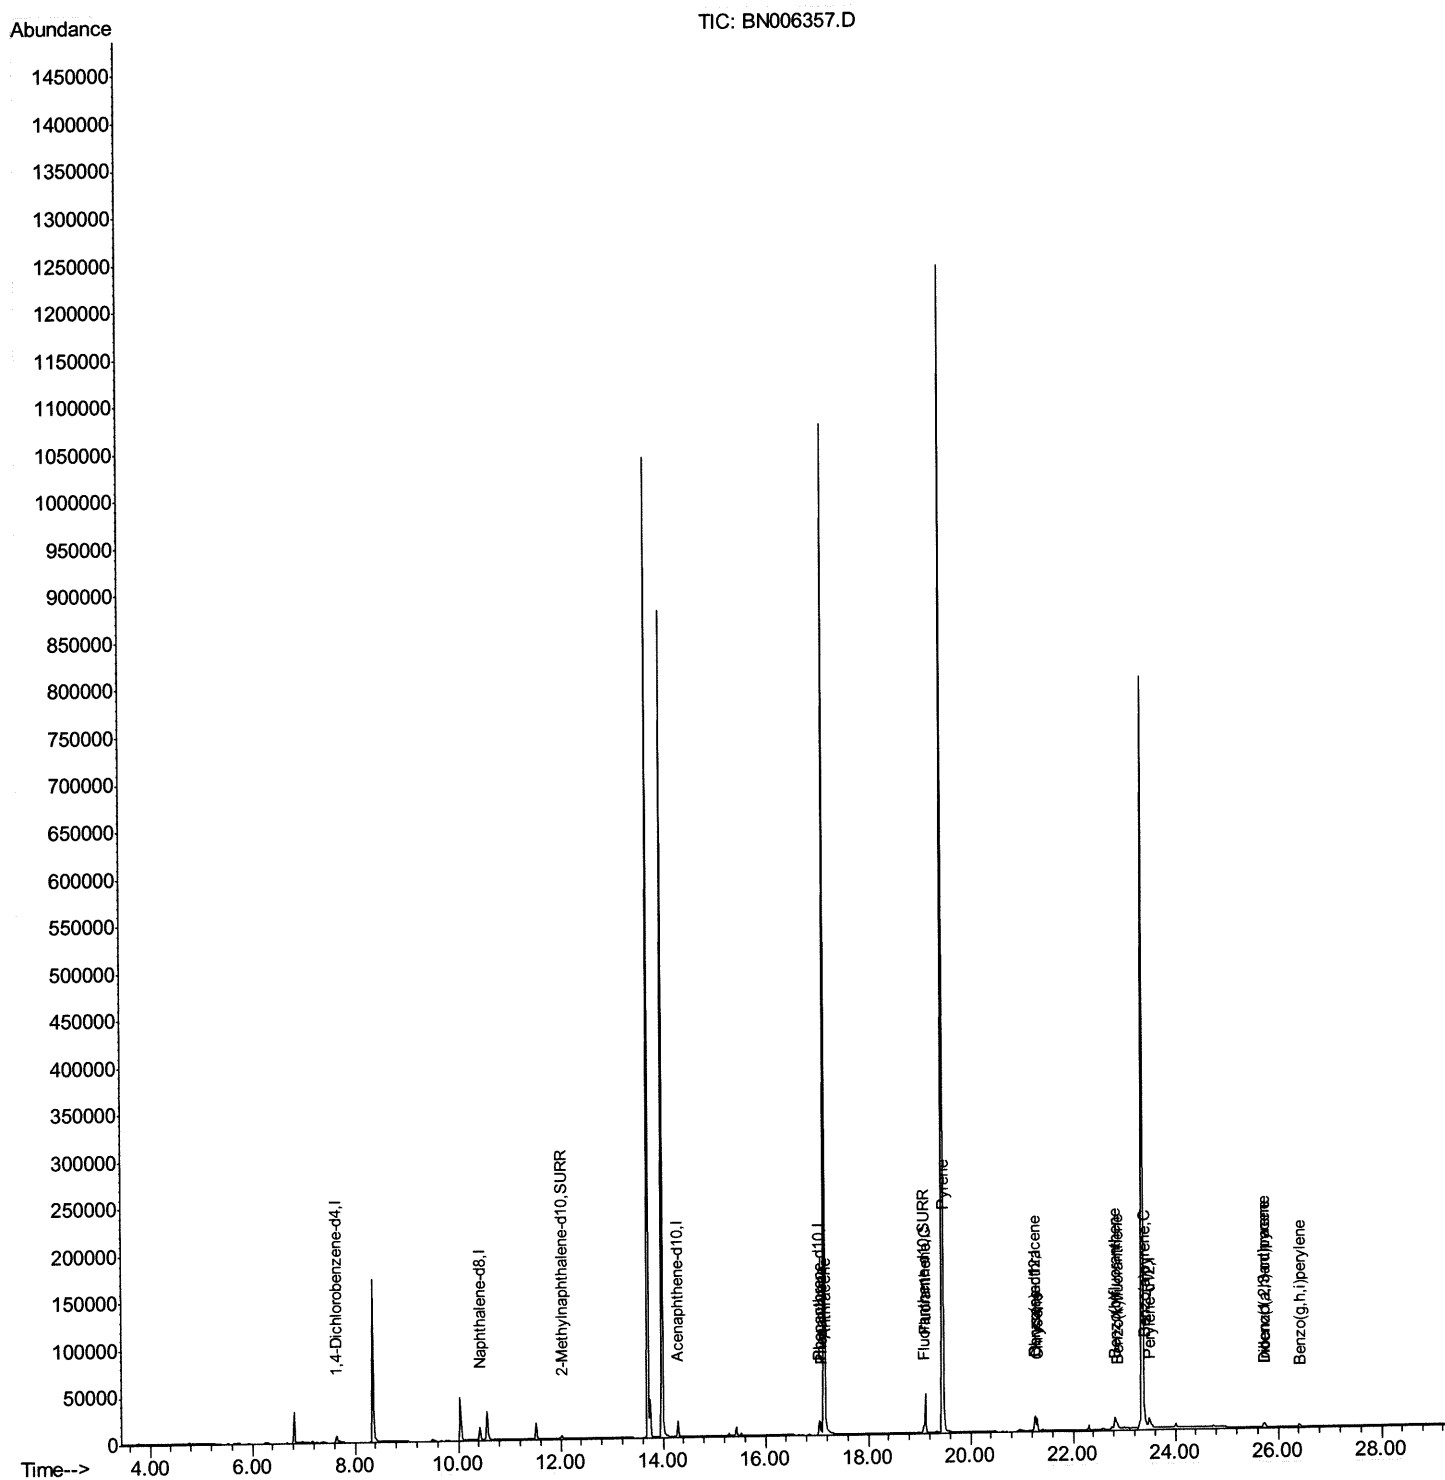

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006357.D
 Acq On : 17 Jun 2019 20:26
 Operator : JU/SJ
 Sample : K3332-24
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 A41W6

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:22:38 AM

Quant Time: Jun 18 01:52:00 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

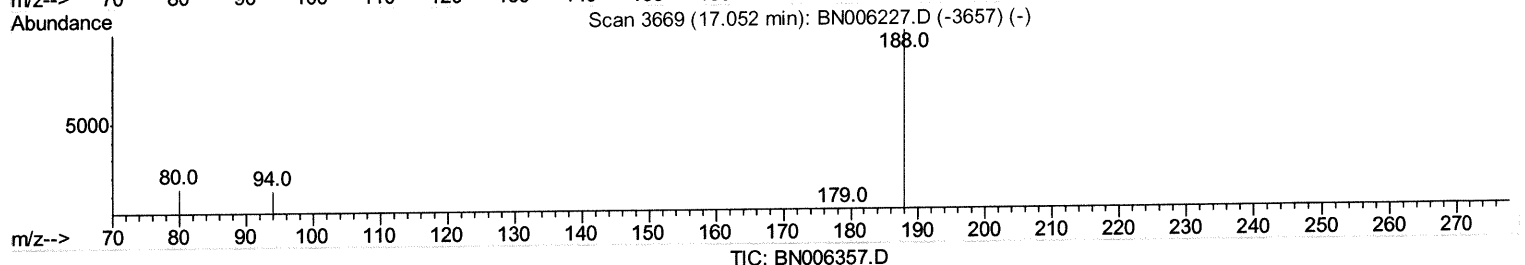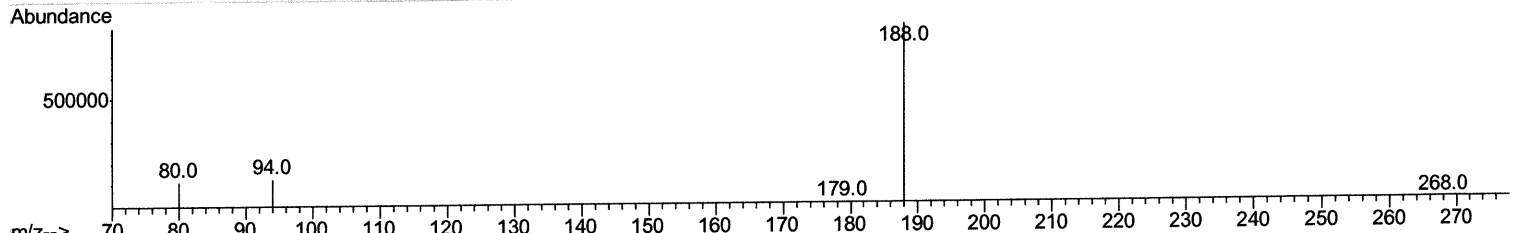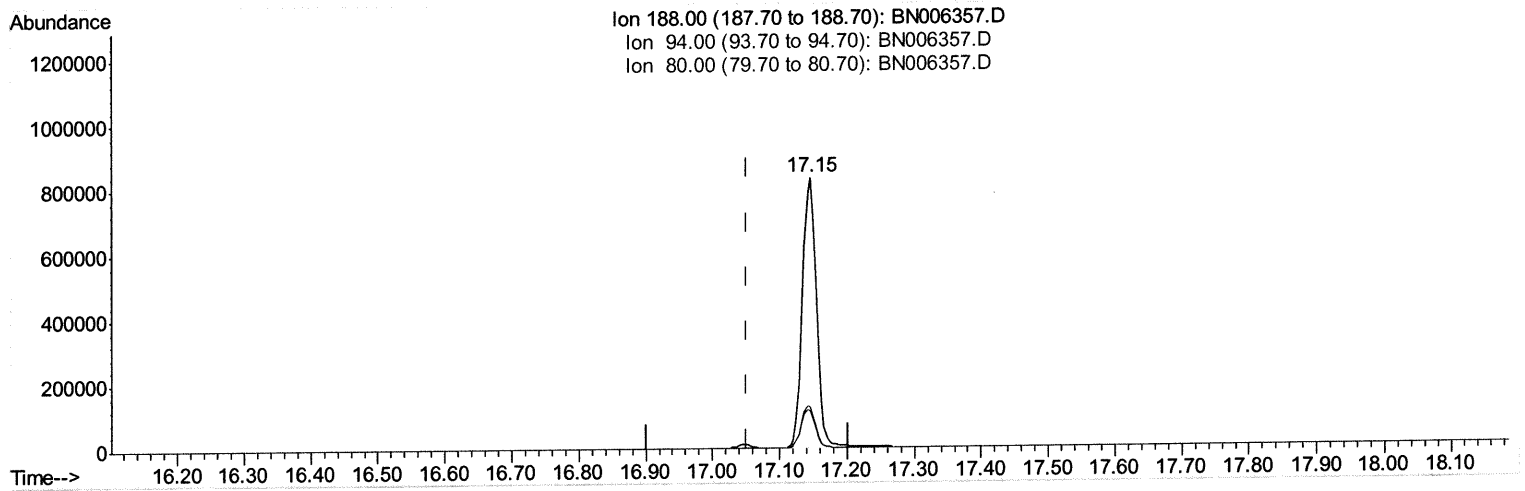

(10) Phenanthrene-d10 (I)
 17.145min (+0.093) 0.40ng/ul
 response 1198708

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	15.15
80.00	13.60	13.82
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006357.D
 Acq On : 17 Jun 2019 20:26
 Operator : JU/SJ
 Sample : K3332-24
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A41W6

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:22:38 AM

Quant Time: Jun 18 01:52:00 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

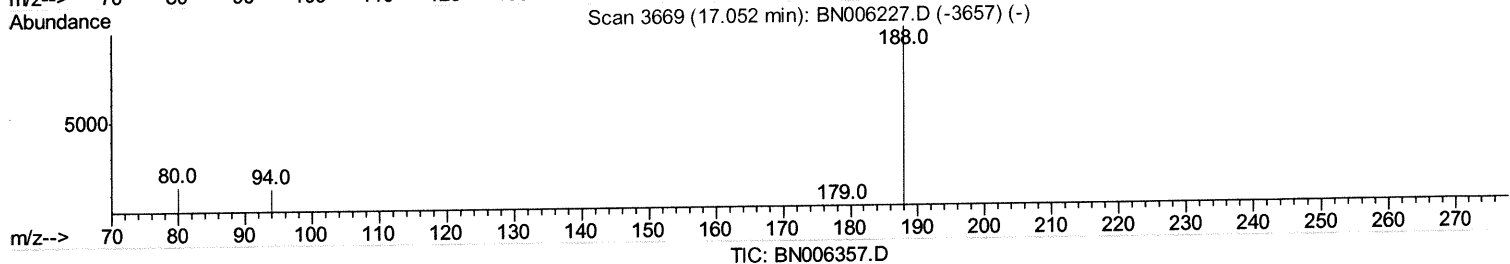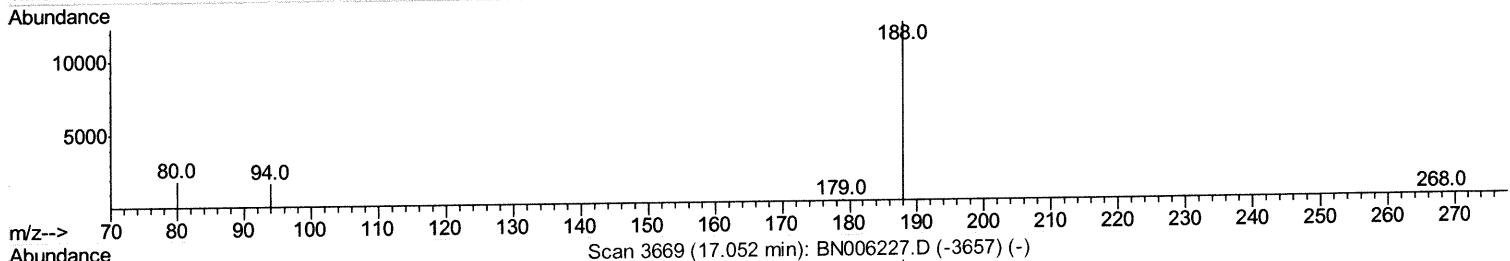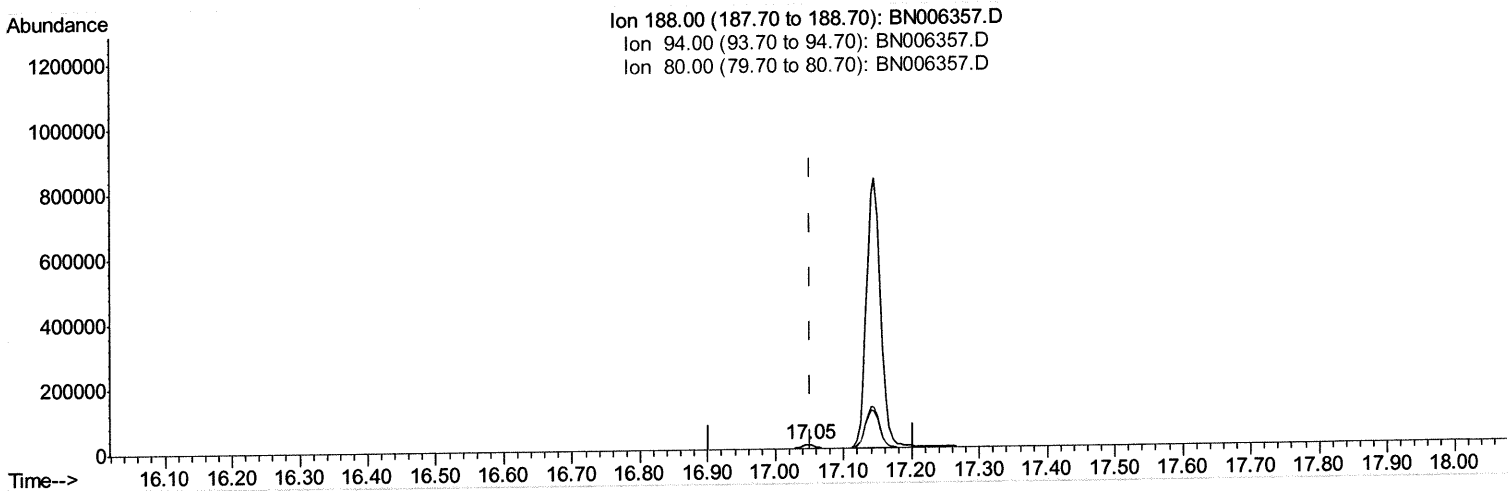

(10) Phenanthrene-d10 (l)

17.048min (-0.004) 0.40ng/ul m *JU* 06/18/19

response 16888

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	13.05
80.00	13.60	14.65
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006357.D
 Acq On : 17 Jun 2019 20:26
 Operator : JU/SJ
 Sample : K3332-24
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A41W6

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:22:38 AM

Quant Time: Jun 18 03:55:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

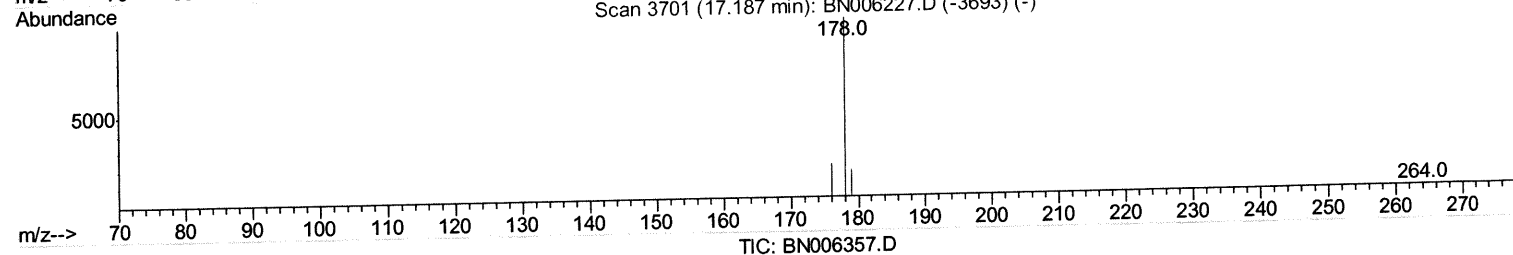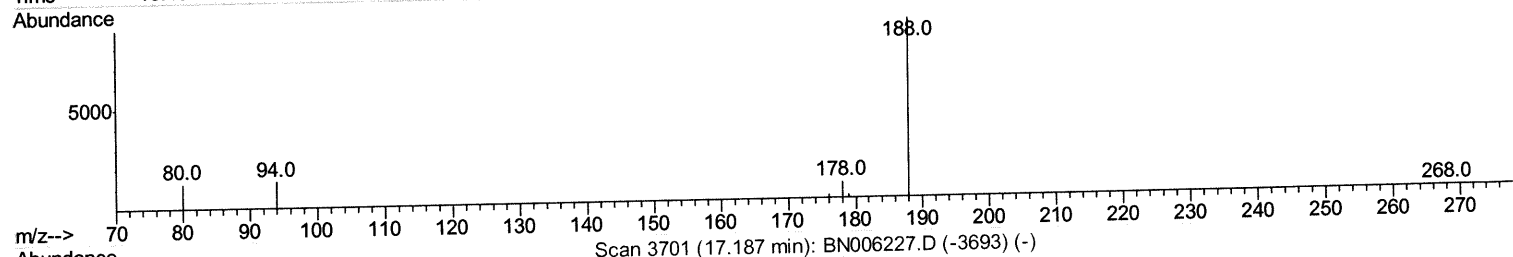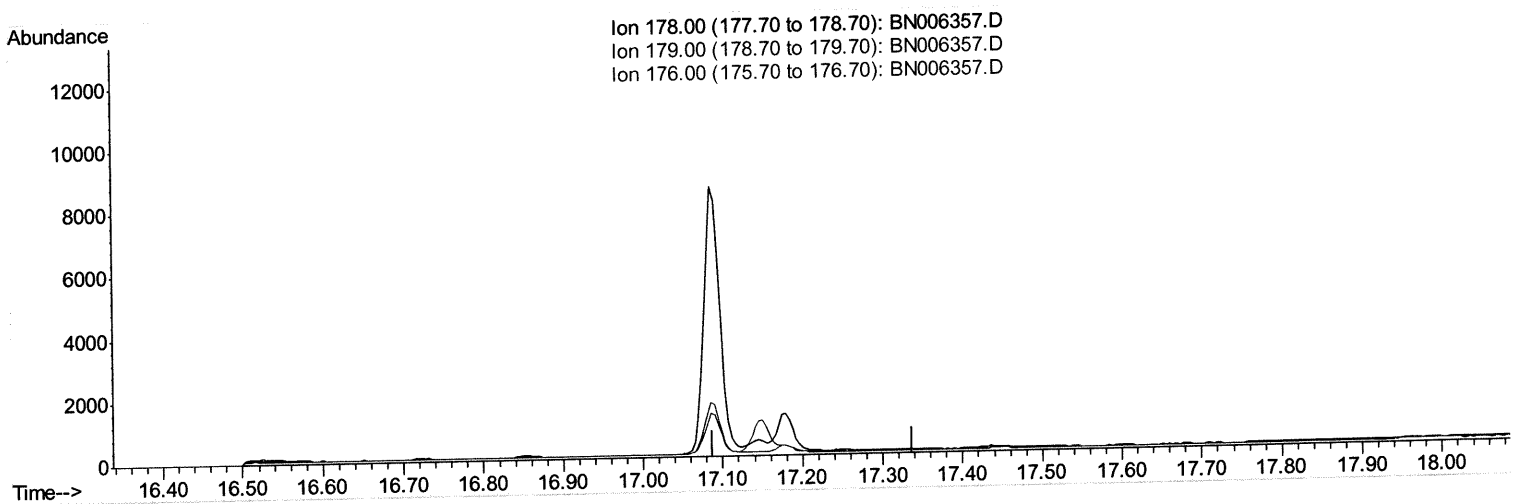

(13) Anthracene

17.187min (-17.187) 0.00ng/ul

response 0

Ion	Exp%	Act%
178.00	100	0.00
179.00	15.30	0.00#
176.00	18.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006357.D
 Acq On : 17 Jun 2019 20:26
 Operator : JU/SJ
 Sample : K3332-24
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A41W6

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:22:38 AM

Quant Time: Jun 18 03:55:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

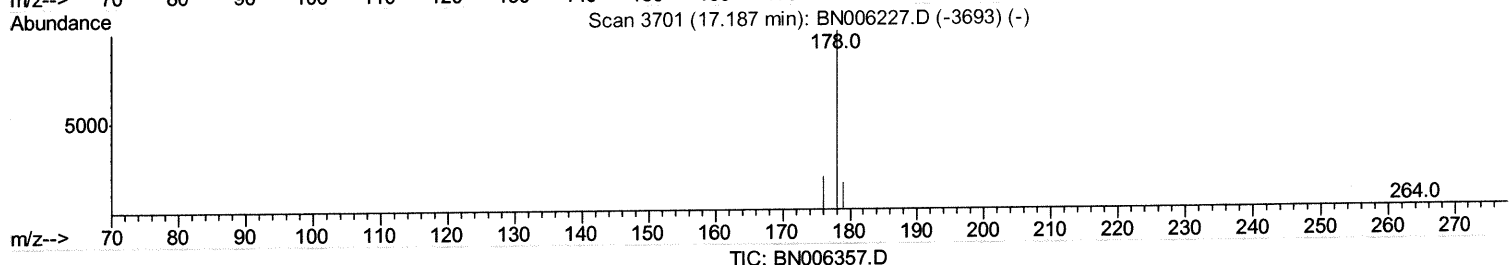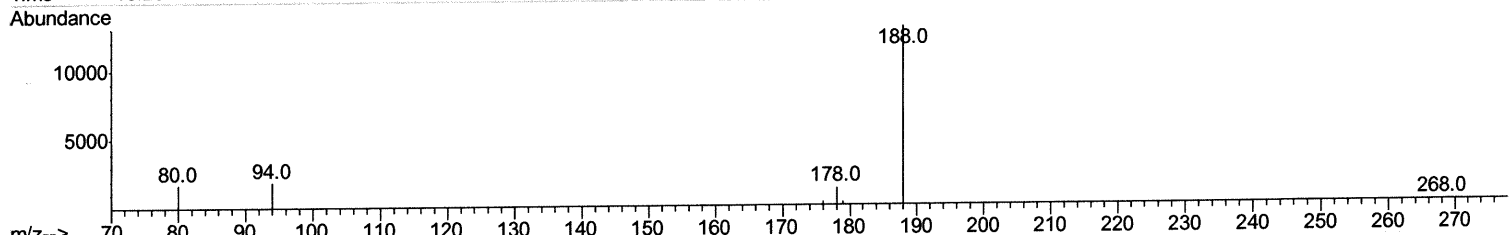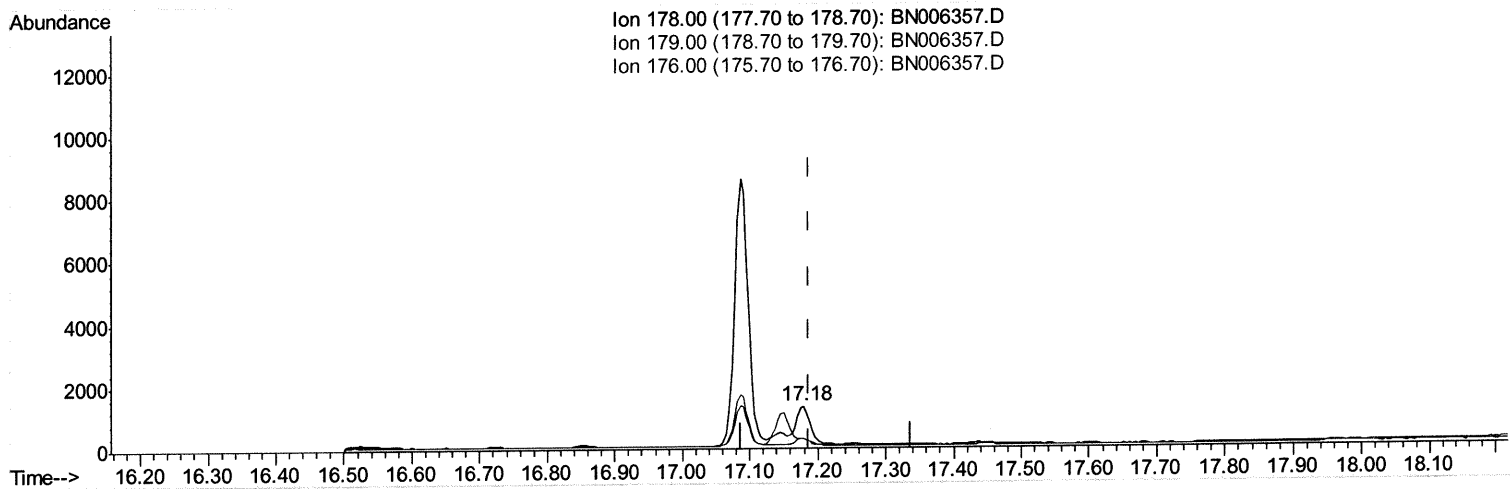

(13) Anthracene

17.179min (-0.008) 0.03ng/ul m *Jv* 06/18/19

response 1702

Ion	Exp%	Act%
178.00	100	100
179.00	15.30	23.02#
176.00	18.90	23.93#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006357.D
 Acq On : 17 Jun 2019 20:26
 Operator : JU/SJ
 Sample : K3332-24
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A41W6

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:22:38 AM

Quant Time: Jun 18 03:55:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

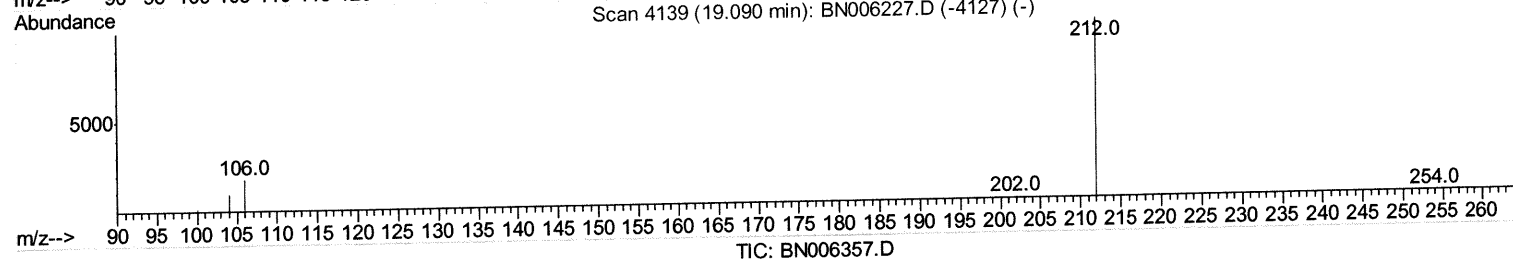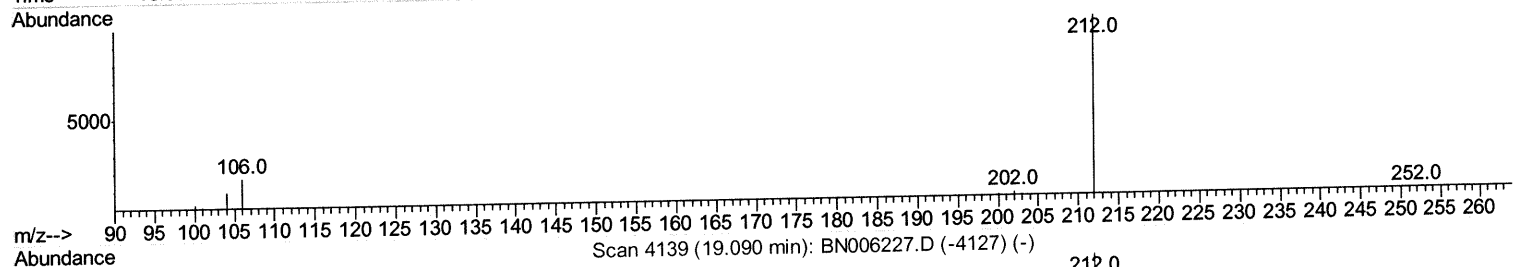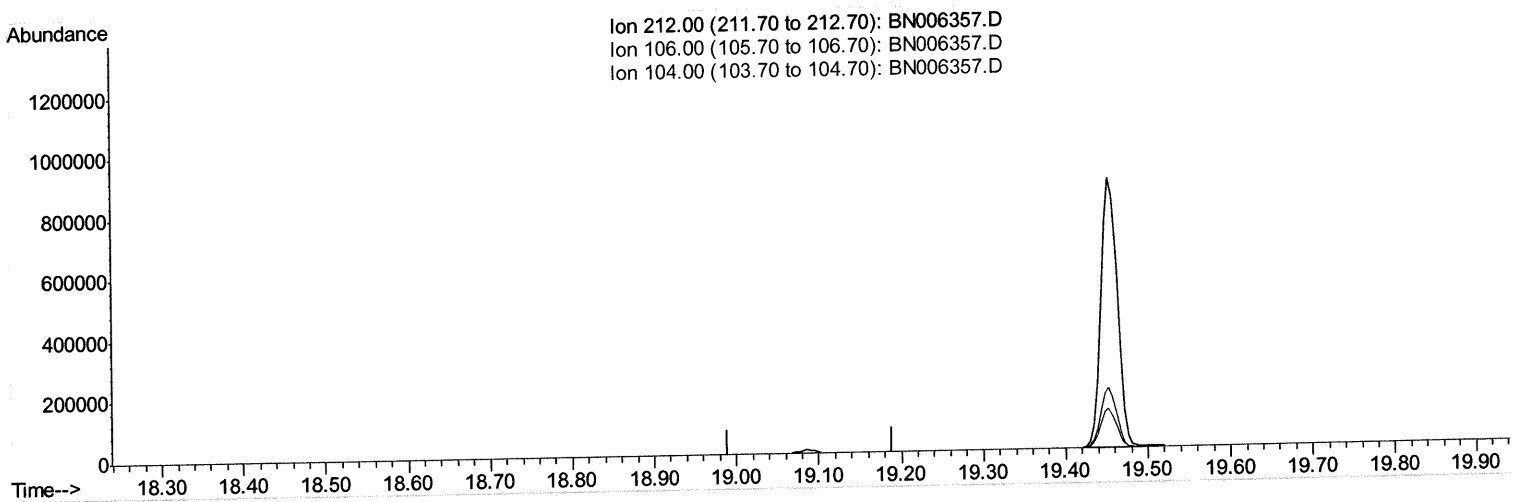

(14) Fluoranthene-d10 (SURR)

19.090min (-19.090) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
Data File : BN006357.D
Acq On : 17 Jun 2019 20:26
Operator : JU/SJ
Sample : K3332-24
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41W6

Manual Integrations
APPROVED

mohammad
6/21/2019 8:22:38 AM

Quant Time: Jun 18 03:55:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

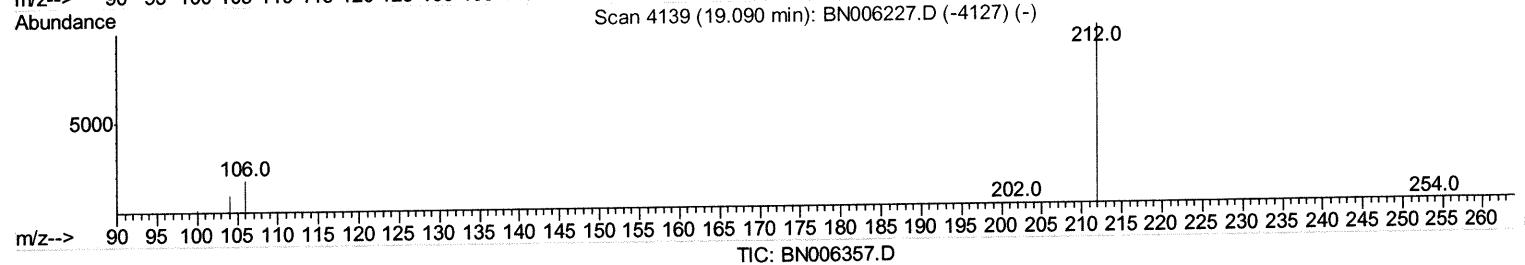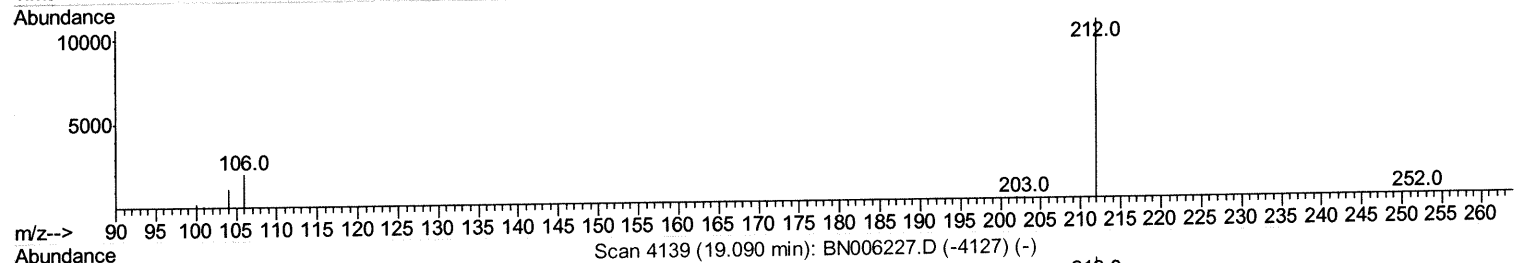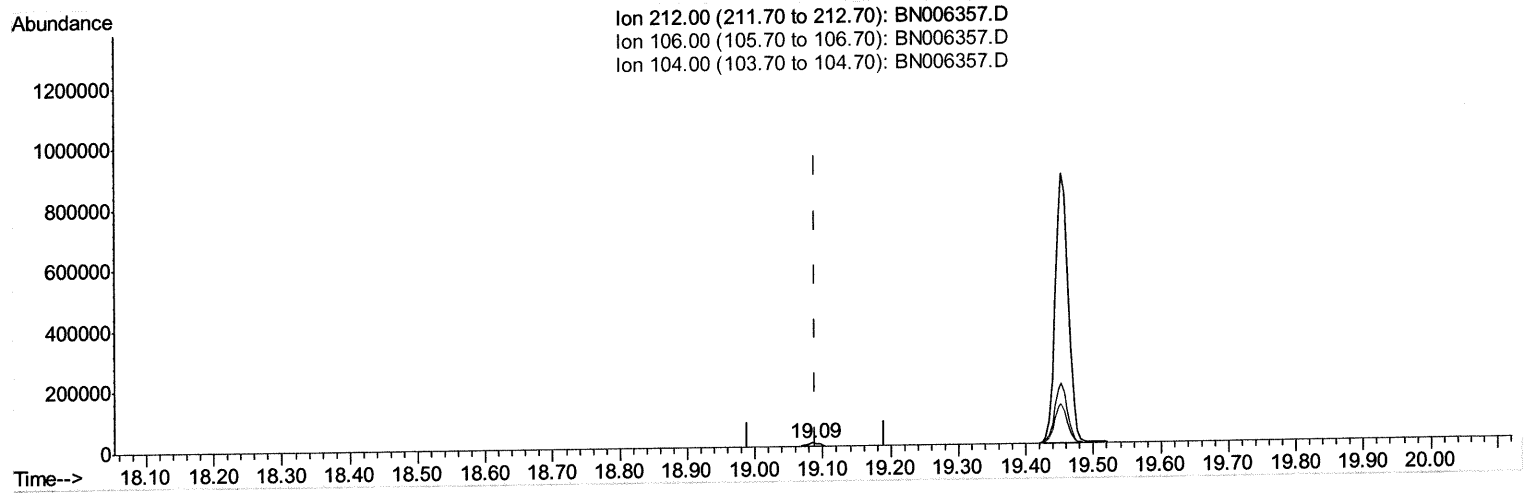

(14) Fluoranthene-d10 (SURR)

19.086min (-0.004) 0.31ng/ul m *JU 06/18/19*

response 14232

Ion	Exp%	Act%
212.00	100	100
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
Data File : BN006357.D
Acq On : 17 Jun 2019 20:26
Operator : JU/SJ
Sample : K3332-24
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41W6

Manual Integrations
APPROVED

mohammad
6/21/2019 8:22:38 AM

Quant Time: Jun 18 03:55:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

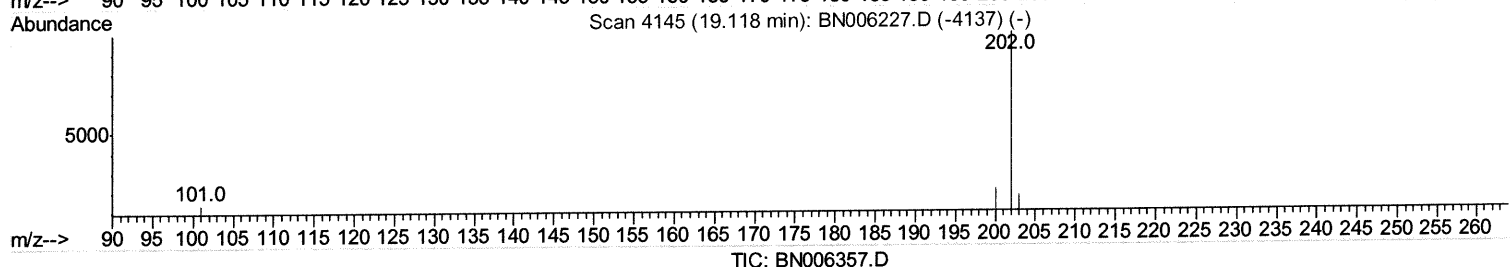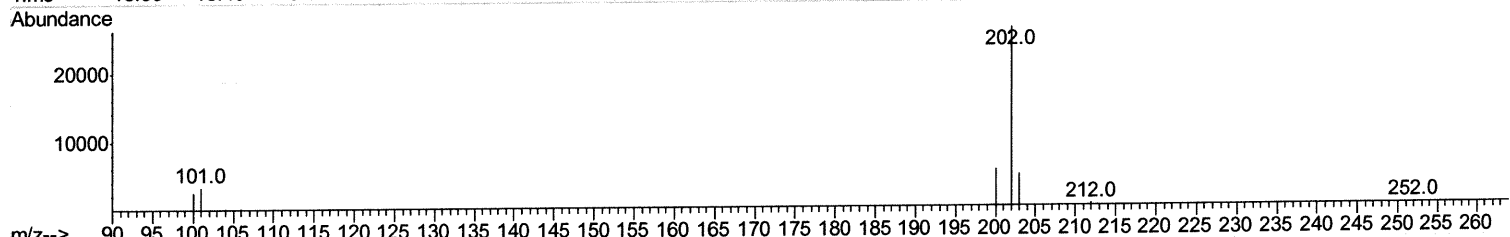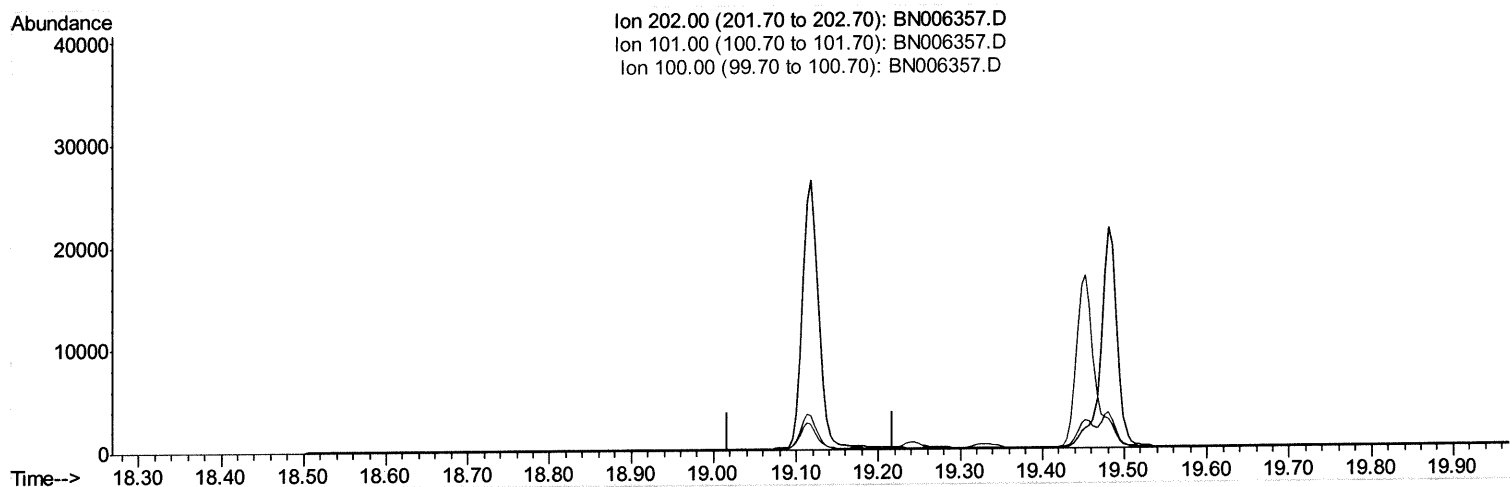

(15) Fluoranthene (C)

19.118min (-19.118) 0.00ng/ul

response 0

Ion	Exp%	Act%
202.00	100	0.00
101.00	12.10	0.00
100.00	8.70	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006357.D
 Acq On : 17 Jun 2019 20:26
 Operator : JU/SJ
 Sample : K3332-24
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A41W6

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:22:38 AM

Quant Time: Jun 18 03:55:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

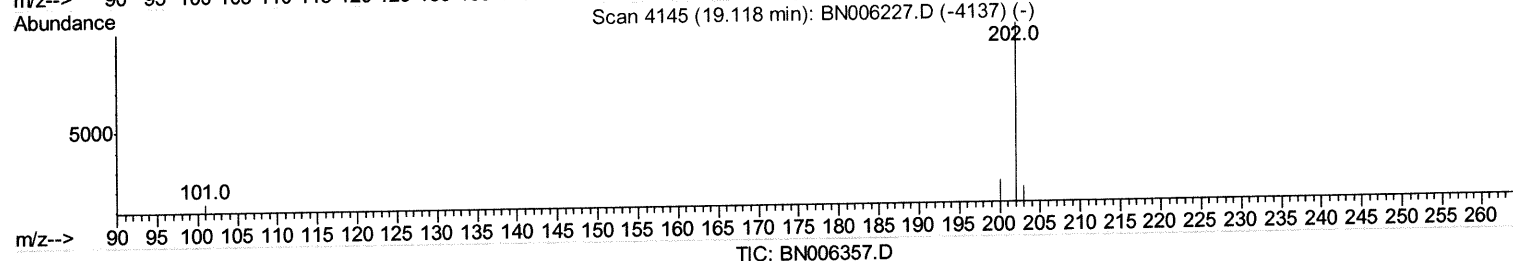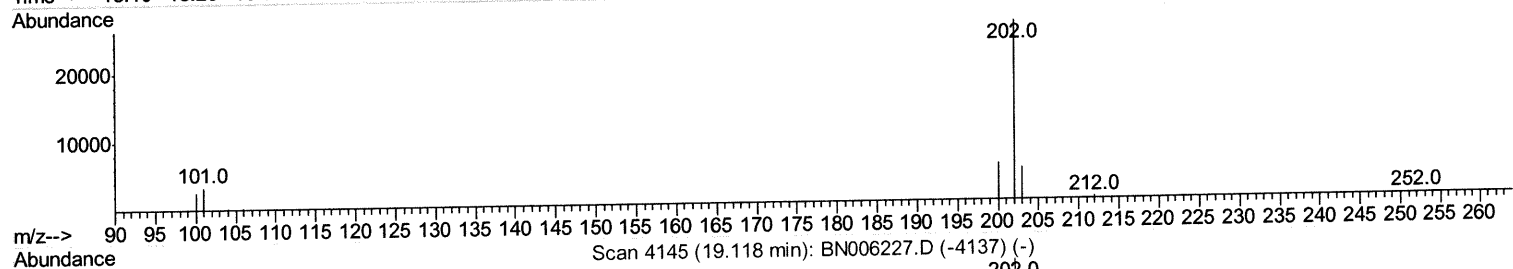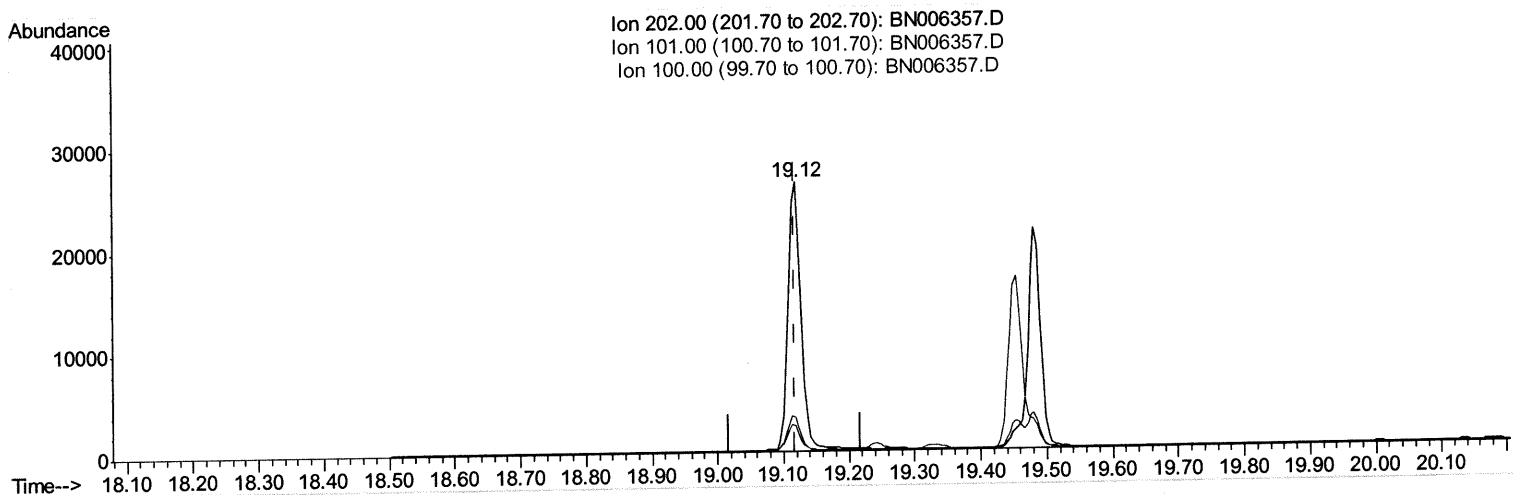

(15) Fluoranthene (C)

19.118min (+0.000) 0.60ng/ul m *JU 06/18/19*

response 36145

Ion	Exp%	Act%
202.00	100	100
101.00	12.10	12.84
100.00	8.70	9.49
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
Data File : BN006357.D
Acq On : 17 Jun 2019 20:26
Operator : JU/SJ
Sample : K3332-24
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A41W6

Manual Integrations
APPROVED

mohammad
6/21/2019 8:22:38 AM

Quant Time: Jun 18 03:55:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

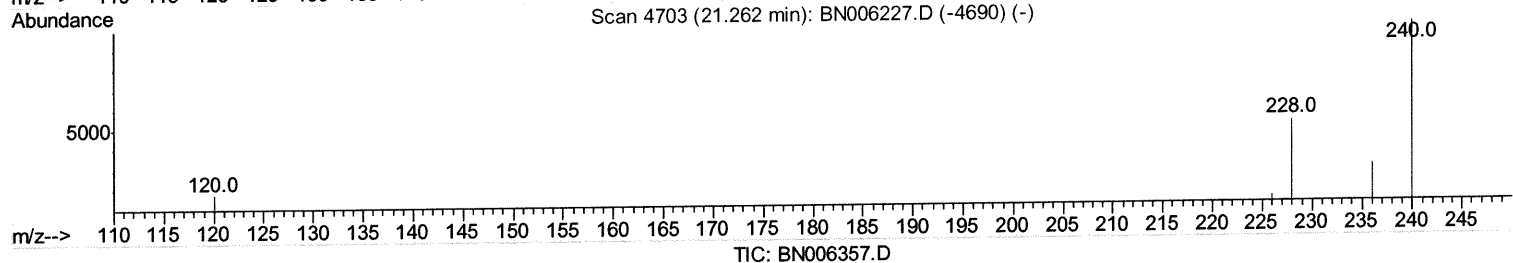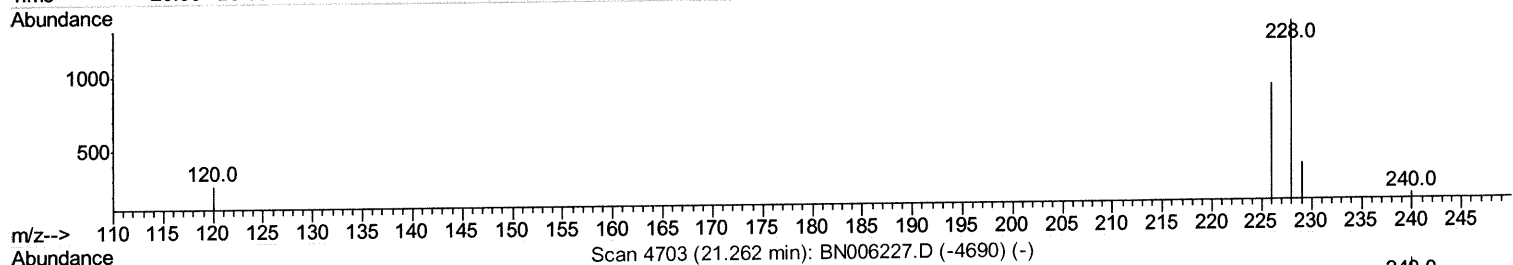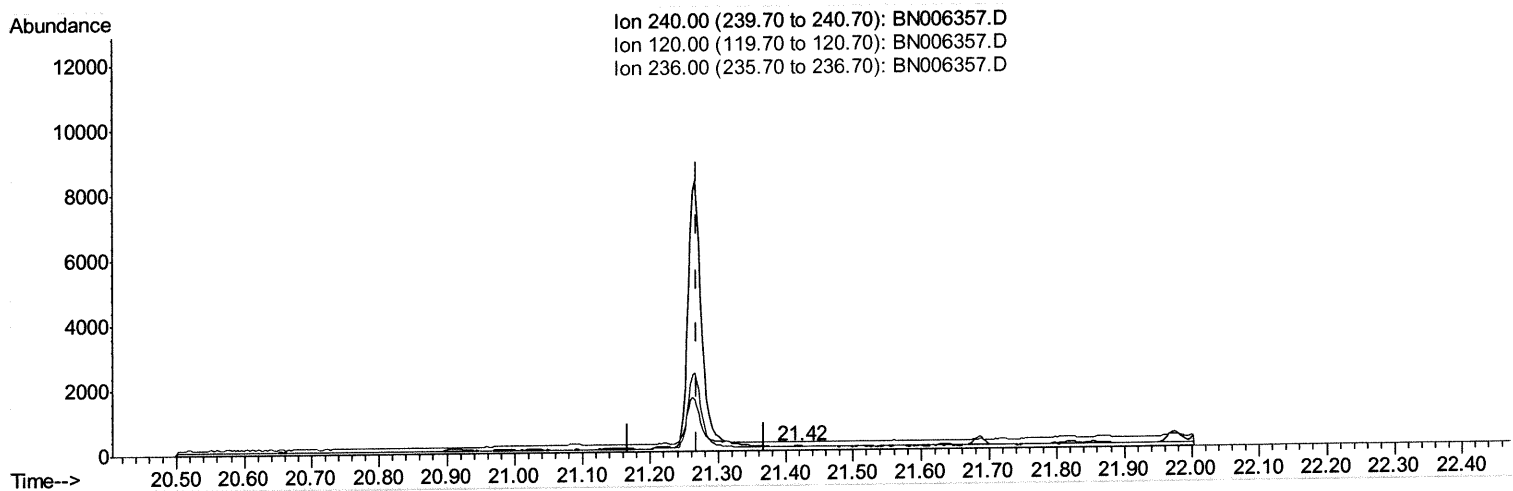

(16) Chrysene-d12 (I)

21.420min (+0.152) 0.40ng/ul

response 68

Ion	Exp%	Act%
240.00	100	100
120.00	20.10	184.72#
236.00	30.10	72.92#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006357.D
 Acq On : 17 Jun 2019 20:26
 Operator : JU/SJ
 Sample : K3332-24
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A41W6

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:22:38 AM

Quant Time: Jun 18 03:55:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

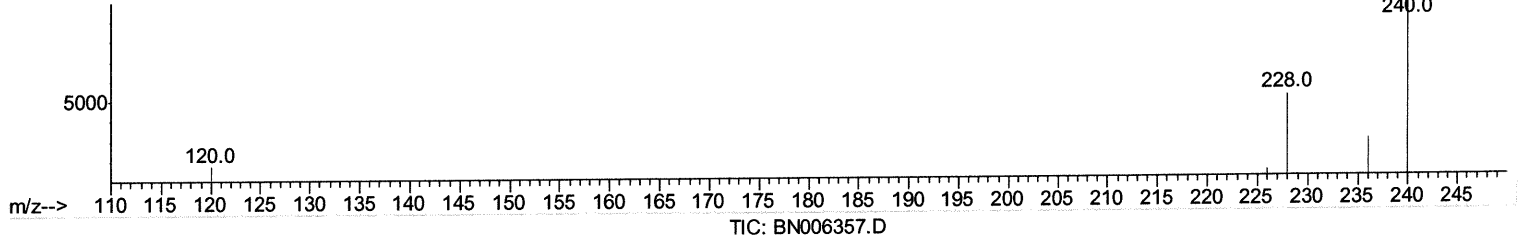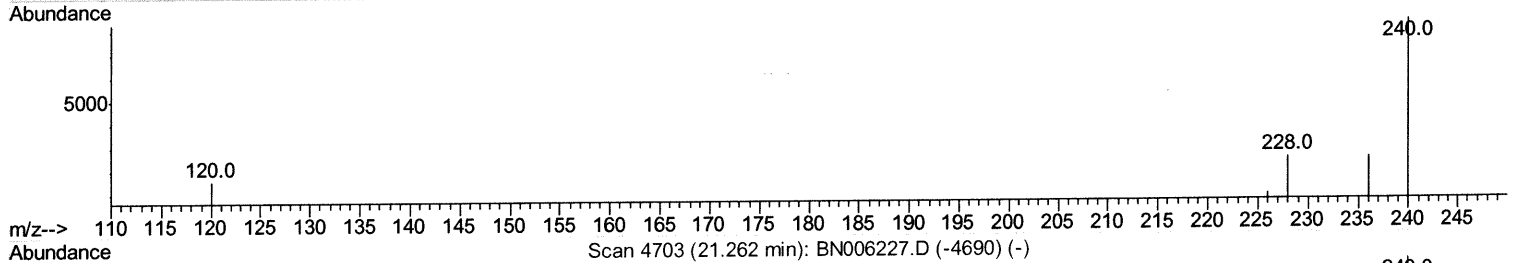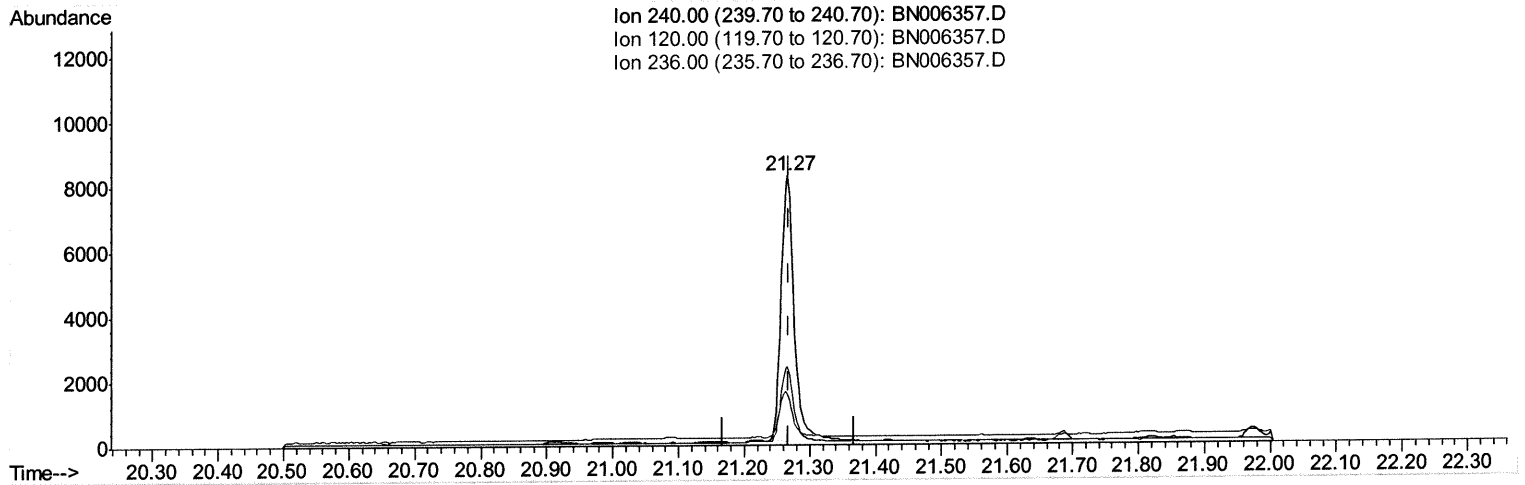

(16) Chrysene-d12 (I)

21.265min (-0.003) 0.40ng/ul m *JU 06/18/19*

response 11557

Ion	Exp%	Act%
240.00	100	100
120.00	20.10	19.32
236.00	30.10	29.15
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
Data File : BN006357.D
Acq On : 17 Jun 2019 20:26
Operator : JU/SJ
Sample : K3332-24
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41W6

Manual Integrations
APPROVED

mohammad
6/21/2019 8:22:38 AM

Quant Time: Jun 18 03:56:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

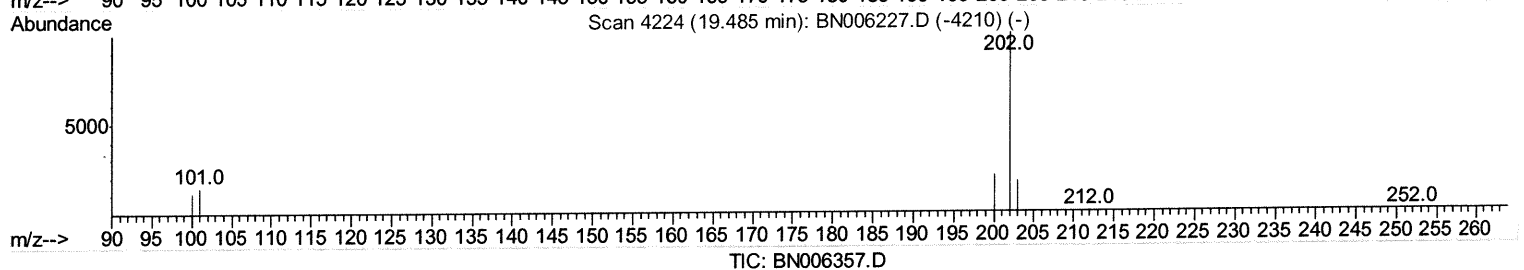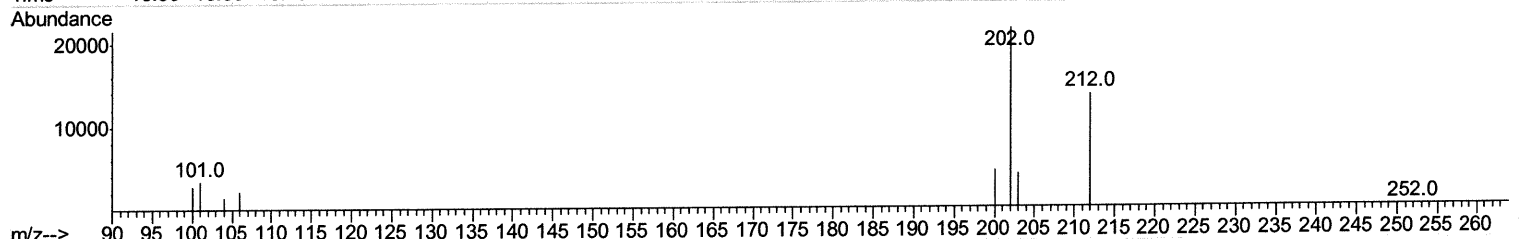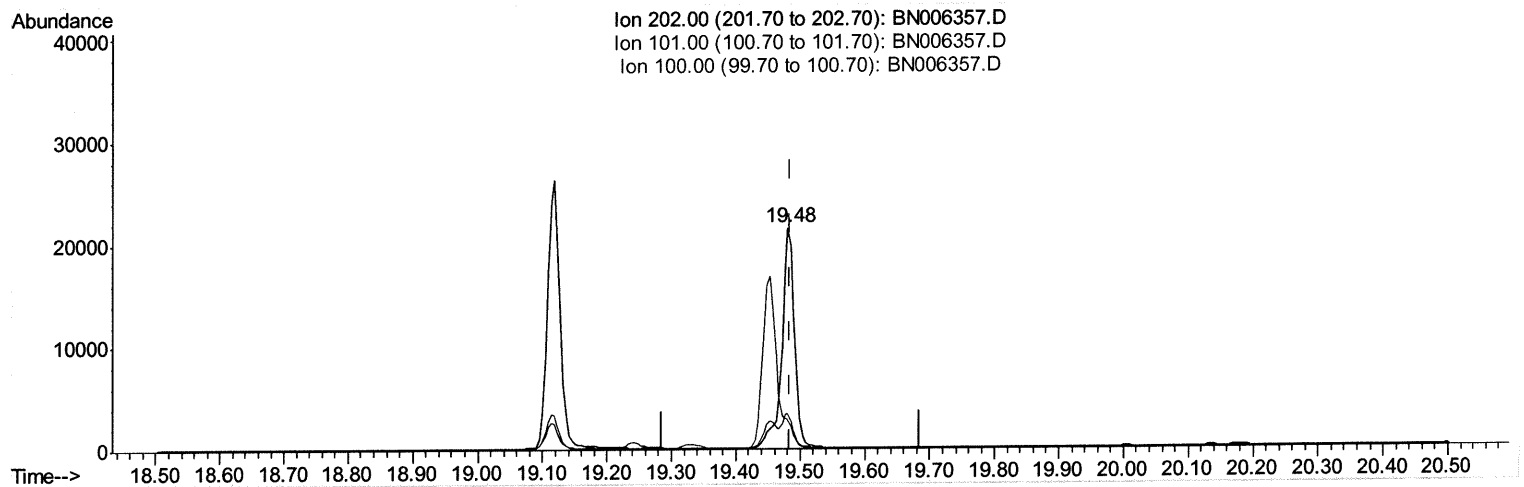

(17) Pyrene

19.481min (-0.004) 0.49ng/ul

response 29779

Ion	Exp%	Act%
202.00	100	100
101.00	15.20	16.17
100.00	12.20	13.48
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006357.D
 Acq On : 17 Jun 2019 20:26
 Operator : JU/SJ
 Sample : K3332-24
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A41W6

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:22:38 AM

Quant Time: Jun 18 03:56:57 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

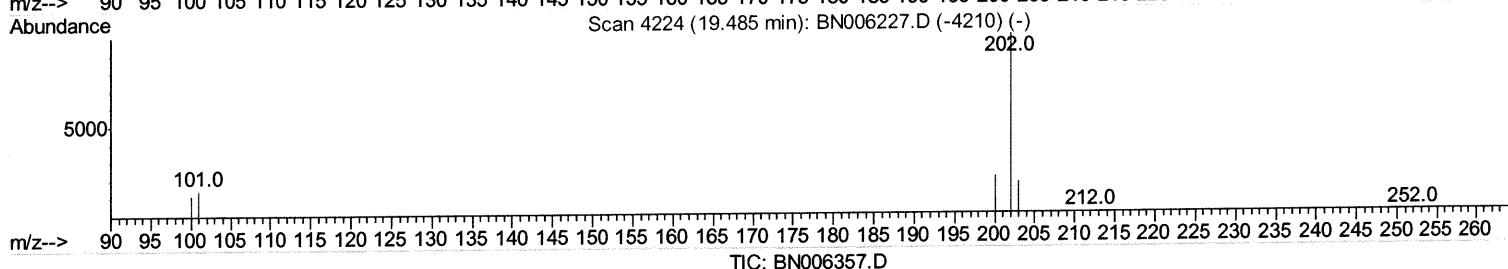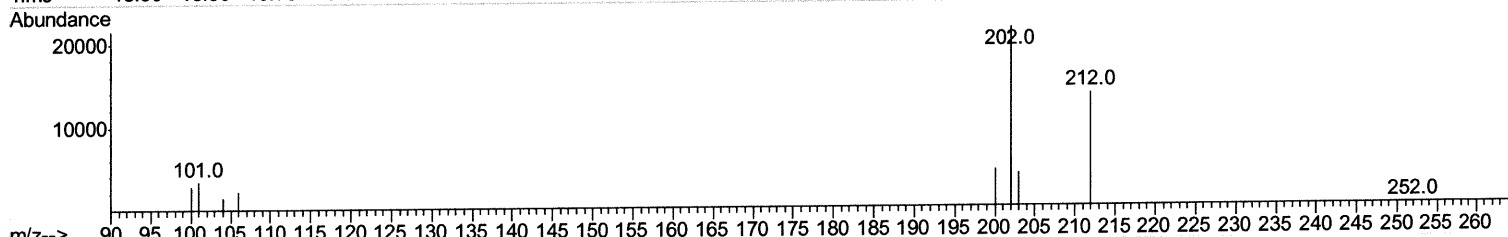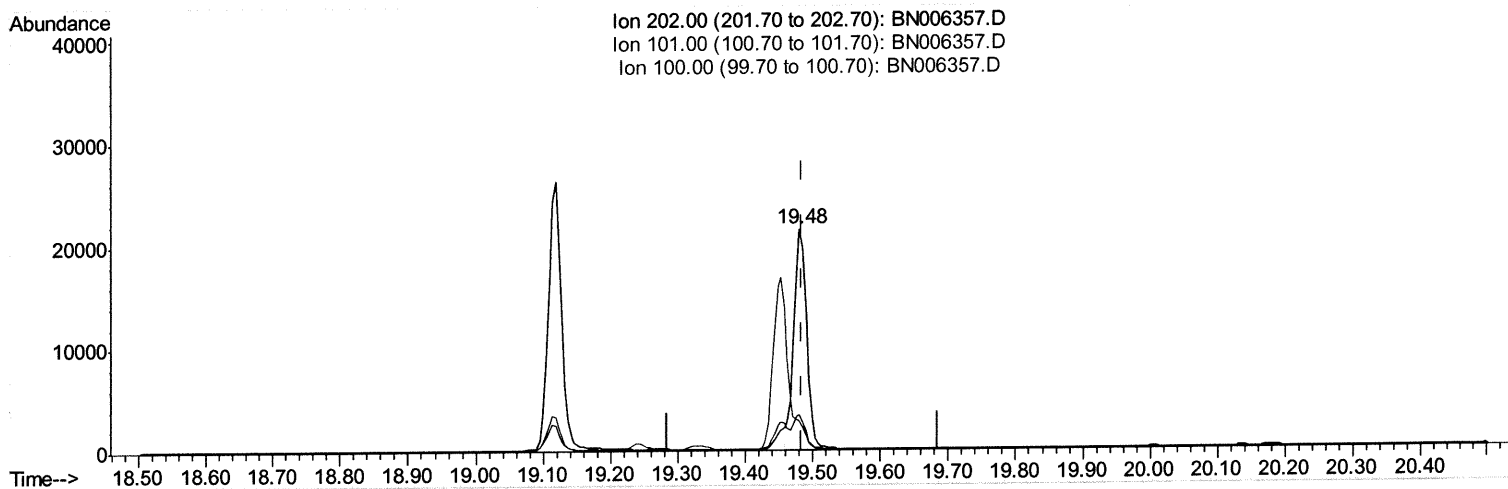

(17) Pyrene

19.481min (-0.004) 0.45ng/ul m *JU 06/18/19*

response 27682

Ion	Exp%	Act%
202.00	100	100
101.00	15.20	16.17
100.00	12.20	13.48
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006357.D
 Acq On : 17 Jun 2019 20:26
 Operator : JU/SJ
 Sample : K3332-24
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A41W6

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:22:38 AM

Quant Time: Jun 18 03:56:57 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

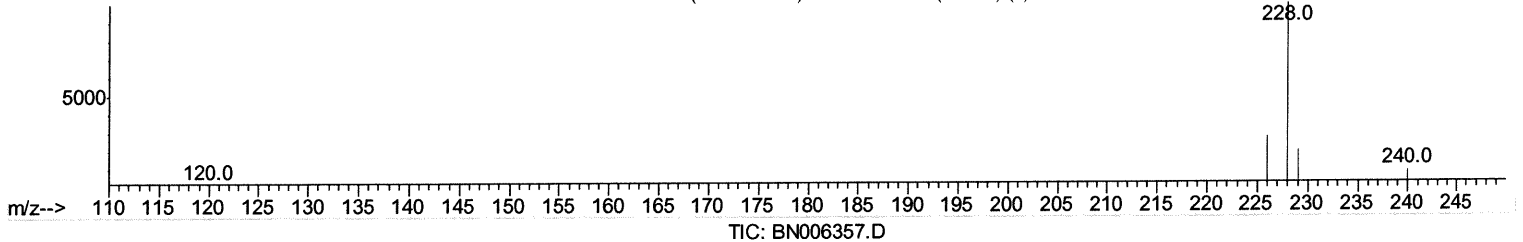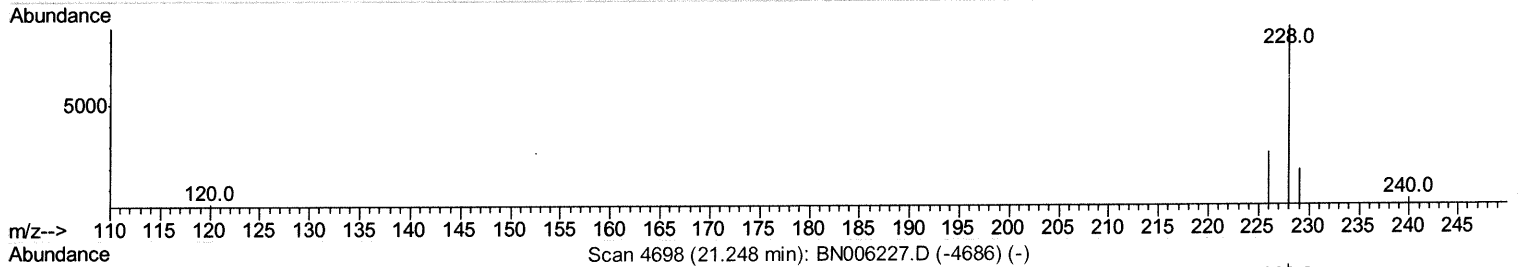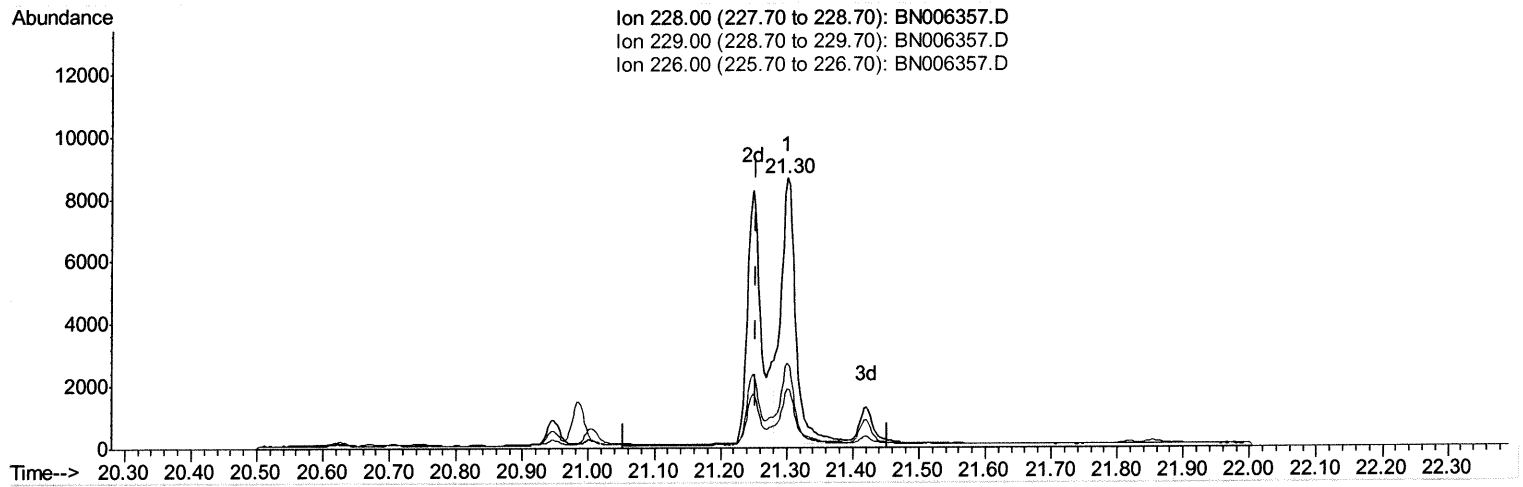

(18) Benzo(a)anthracene

21.300min (+0.047) 0.27ng/ul

response 13783

Ion	Exp%	Act%
228.00	100	100
229.00	20.60	21.63
226.00	28.50	31.18
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
Data File : BN006357.D
Acq On : 17 Jun 2019 20:26
Operator : JU/SJ
Sample : K3332-24
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A41W6

Manual Integrations
APPROVED

mohammad
6/21/2019 8:22:38 AM

Quant Time: Jun 18 03:56:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

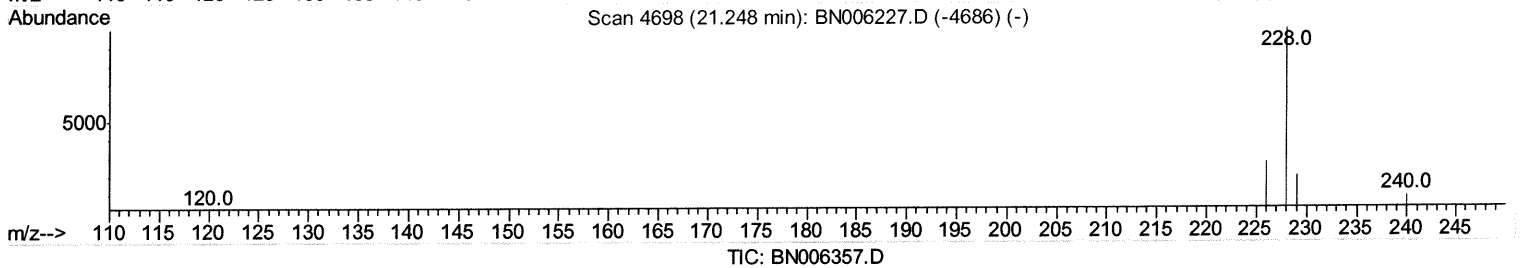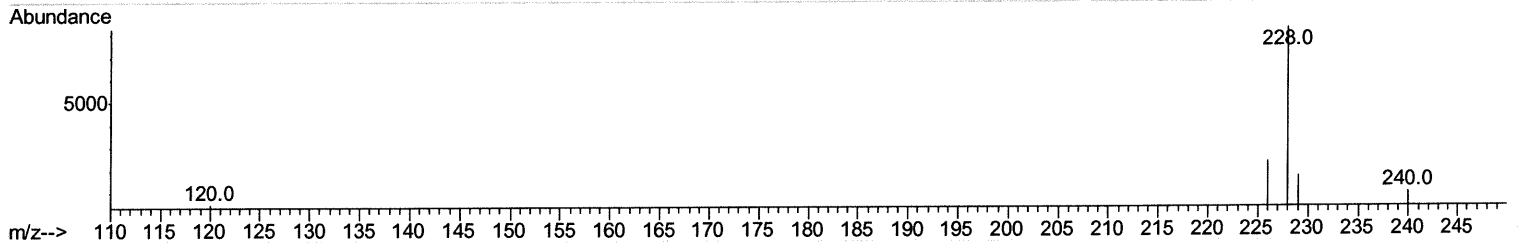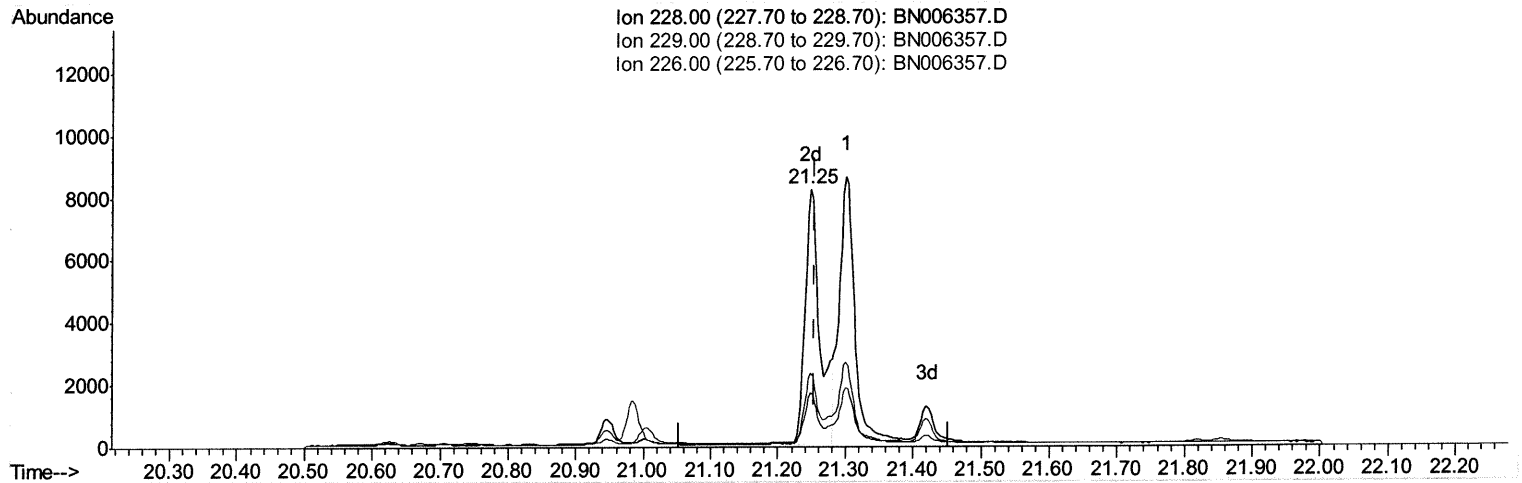

(18) Benzo(a)anthracene

21.248min (-0.006) 0.25ng/ul m *JU 06/18/19*

response 12572

Ion	Exp%	Act%
228.00	100	100
229.00	20.60	20.92
226.00	28.50	28.57
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006357.D
 Acq On : 17 Jun 2019 20:26
 Operator : JU/SJ
 Sample : K3332-24
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A41W6

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:22:38 AM

Quant Time: Jun 18 03:56:57 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

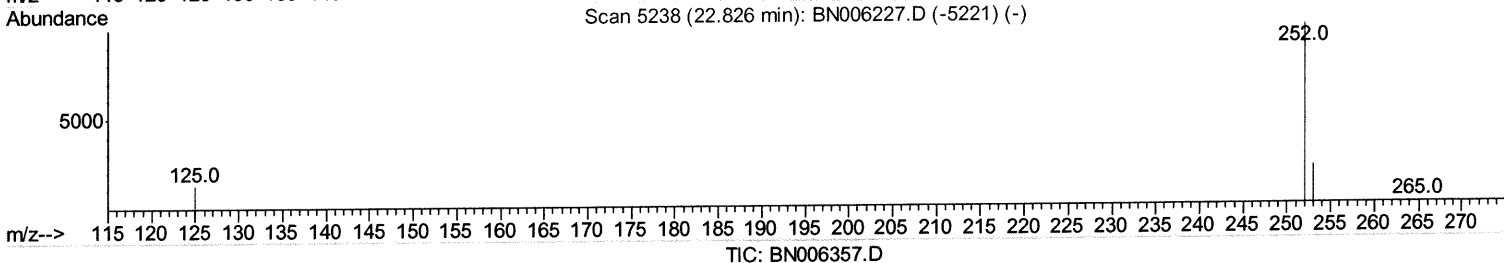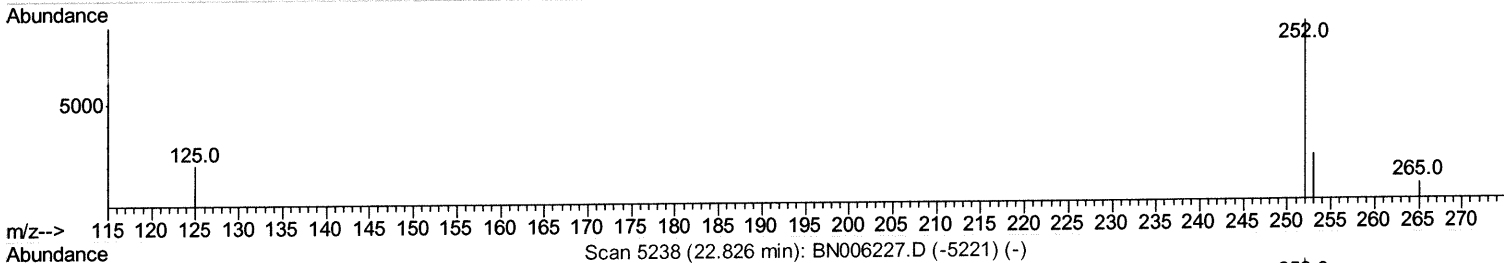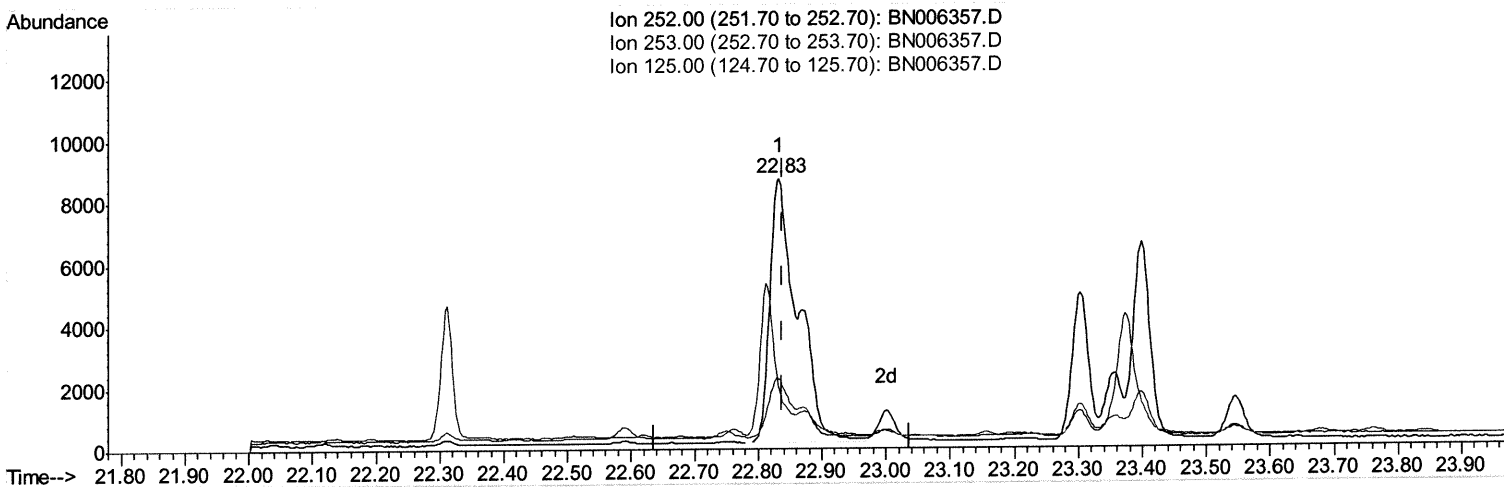

(21) Benzo(b)fluoranthene

22.832min (-0.006) 0.34ng/ul

response 26122

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	25.99
125.00	20.50	23.10
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006357.D
 Acq On : 17 Jun 2019 20:26
 Operator : JU/SJ
 Sample : K3332-24
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A41W6

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:22:38 AM

Quant Time: Jun 18 03:56:57 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

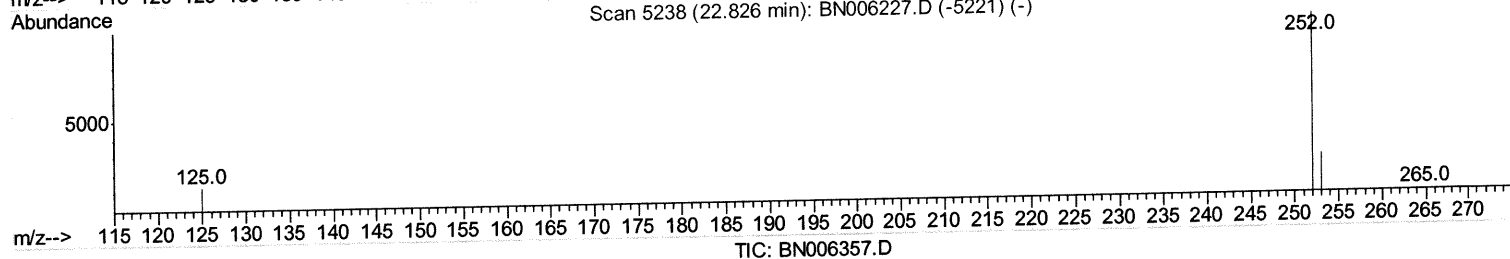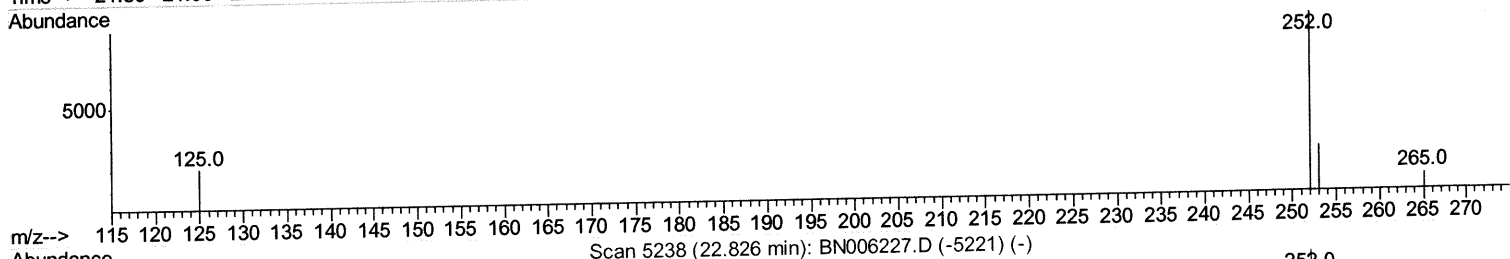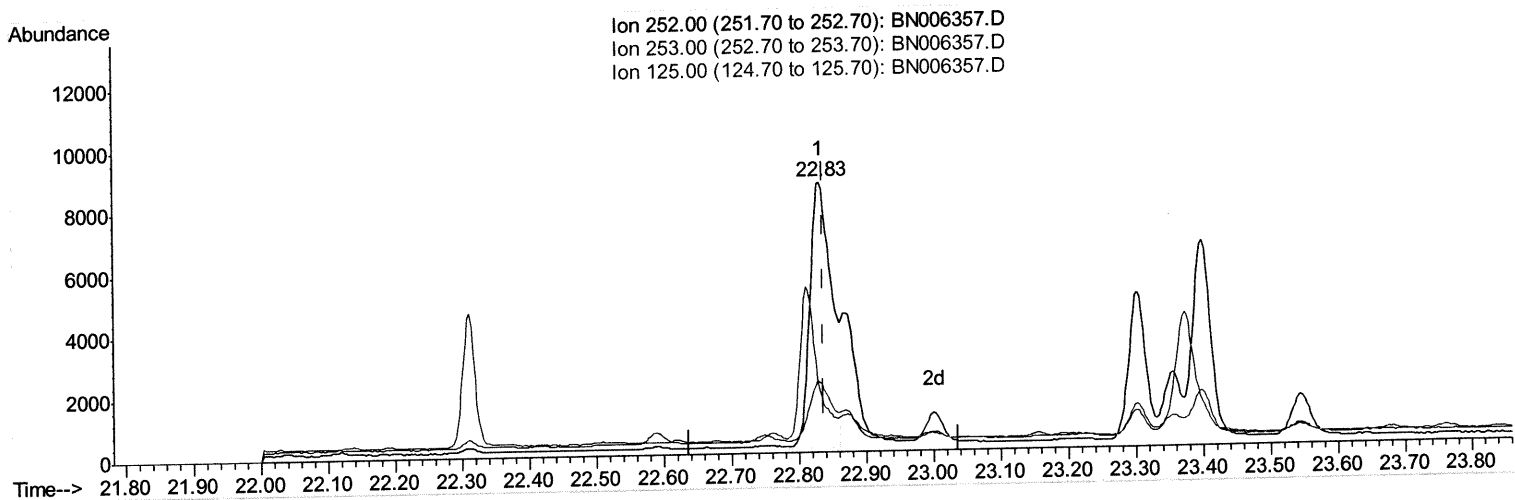

(21) Benzo(b)fluoranthene

22.832min (-0.006) 0.25ng/ul m *JU 06/18/19*

response 19181

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	25.99
125.00	20.50	23.10
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006357.D
 Acq On : 17 Jun 2019 20:26
 Operator : JU/SJ
 Sample : K3332-24
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A41W6

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:22:38 AM

Quant Time: Jun 18 03:56:57 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

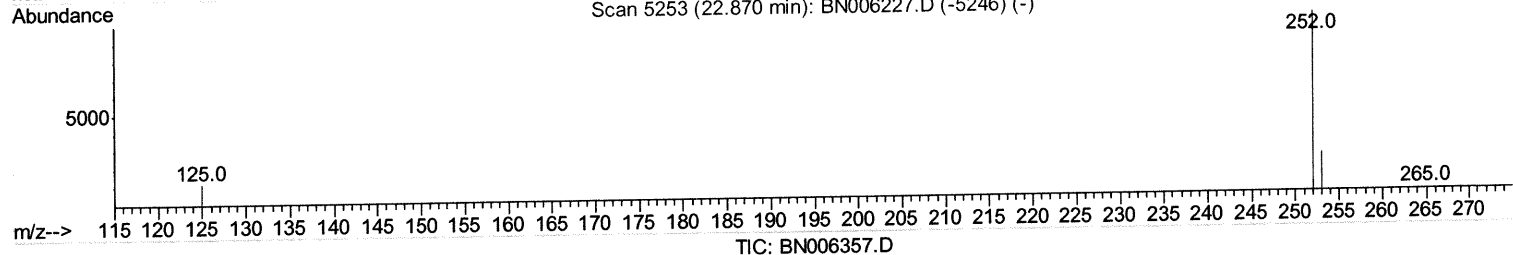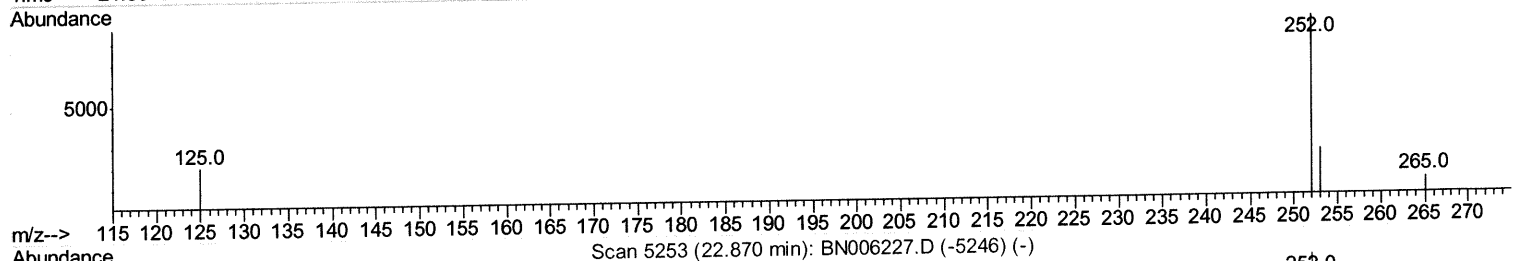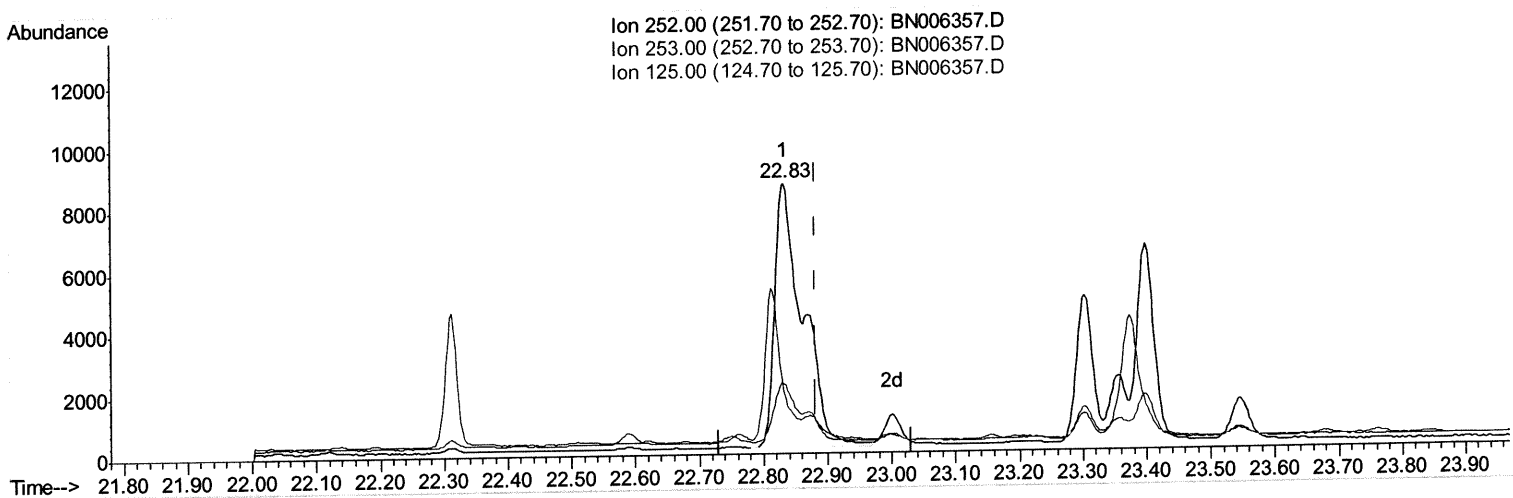

(22) Benzo(k)fluoranthene

22.832min (-0.050) 0.35ng/ul

response 26122

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	25.99
125.00	17.90	23.10#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
Data File : BN006357.D
Acq On : 17 Jun 2019 20:26
Operator : JU/SJ
Sample : K3332-24
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41W6

Manual Integrations
APPROVED

mohammad
6/21/2019 8:22:38 AM

Quant Time: Jun 18 03:56:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

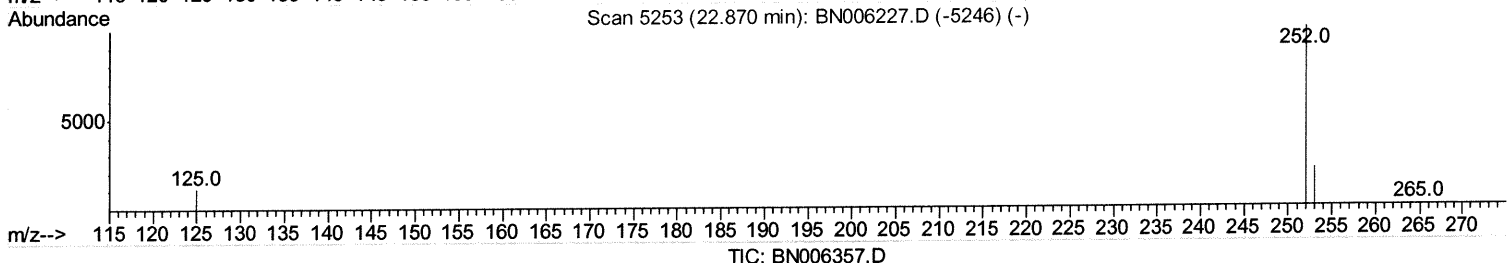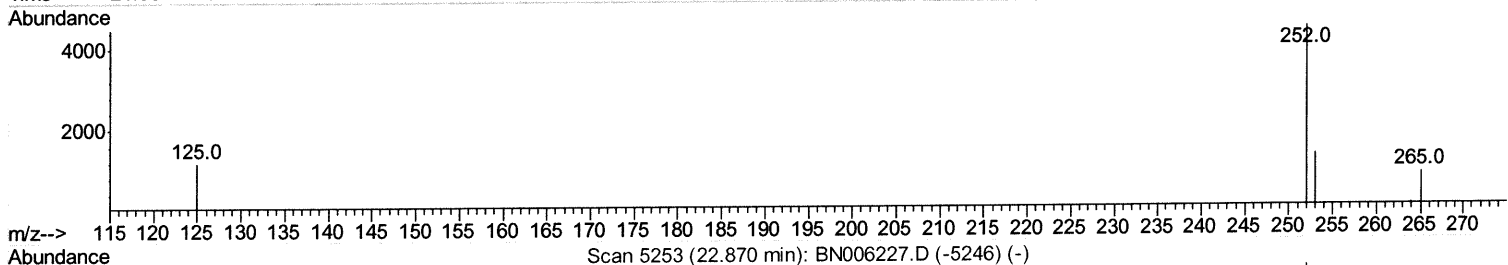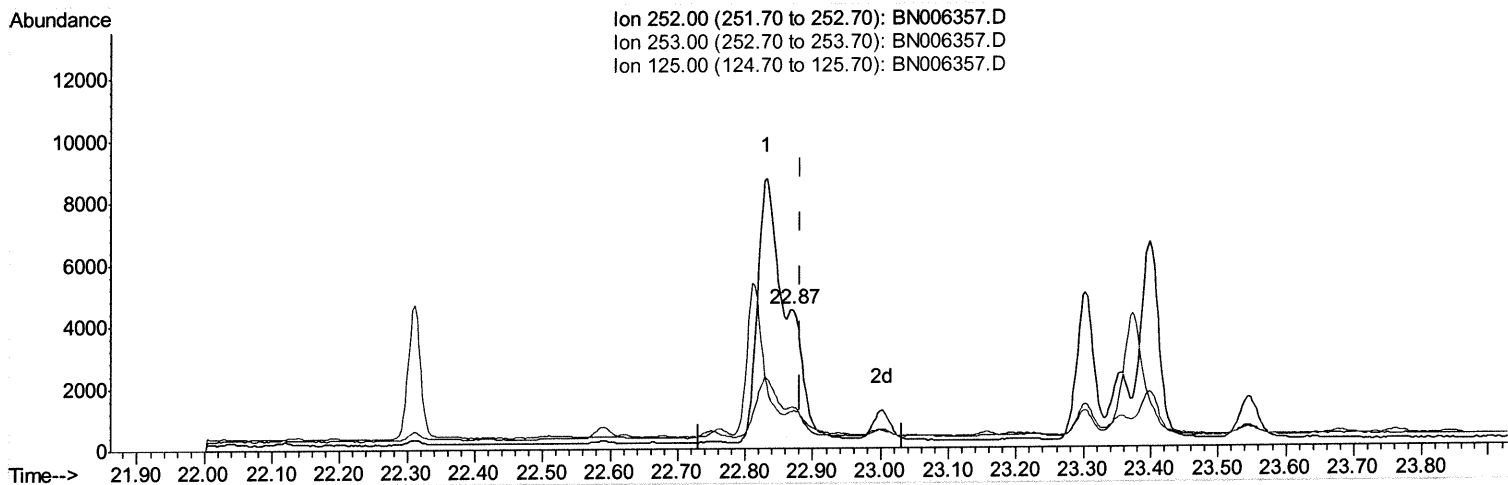

(22) Benzo(k)fluoranthene

22.870min (-0.012) 0.08ng/ul m *JU 06/18/19*

response 6324

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	29.84
125.00	17.90	26.81#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006357.D
 Acq On : 17 Jun 2019 20:26
 Operator : JU/SJ
 Sample : K3332-24
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A41W6

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:22:38 AM

Quant Time: Jun 18 03:59:12 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	4642	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	18516	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.29	164	9528	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	16888m >	0.40	ng/ul	0.00
16) Chrysene-d12	21.27	240	11557m >	0.40	ng/ul	0.00
20) Perylene-d12	23.50	264	18603	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	5541	0.20	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	14232m >	0.31	ng/ul	0.00
Target Compounds						
12) Phenanthrene	17.09	178	11909	0.220	ng/ul	Ovalue 98
13) Anthracene	17.18	178	1702m >	0.033	ng/ul	
15) Fluoranthene	19.12	202	36145m >	0.604	ng/ul	
17) Pyrene	19.48	202	27682m >	0.455	ng/ul	
18) Benzo(a)anthracene	21.25	228	12572m >	0.246	ng/ul	
19) Chrysene	21.30	228	13017	0.271	ng/ul	99
21) Benzo(b)fluoranthene	22.83	252	19181m >	0.247	ng/ul	
22) Benzo(k)fluoranthene	22.87	252	6324m >	0.084	ng/ul	
23) Benzo(a)pyrene	23.40	252	11820	0.164	ng/ul	96
24) Indeno(1,2,3-cd)pyrene	25.74	276	8269	0.106	ng/ul#	88
25) Dibenzo(a,h)anthracene	25.74	278	1883	0.030	ng/ul#	68
26) Benzo(q,h,i)perylene	26.42	276	6737	0.103	ng/ul	100

Jo 06/18/19
 (#) = qualifier out of range (m) = manual integration (+) = signals summed