

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006361.D
 Acq On : 17 Jun 2019 22:44
 Operator : JU/SJ
 Sample : K3335-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4237

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:22:47 AM

Quant Time: Jun 18 04:19:56 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

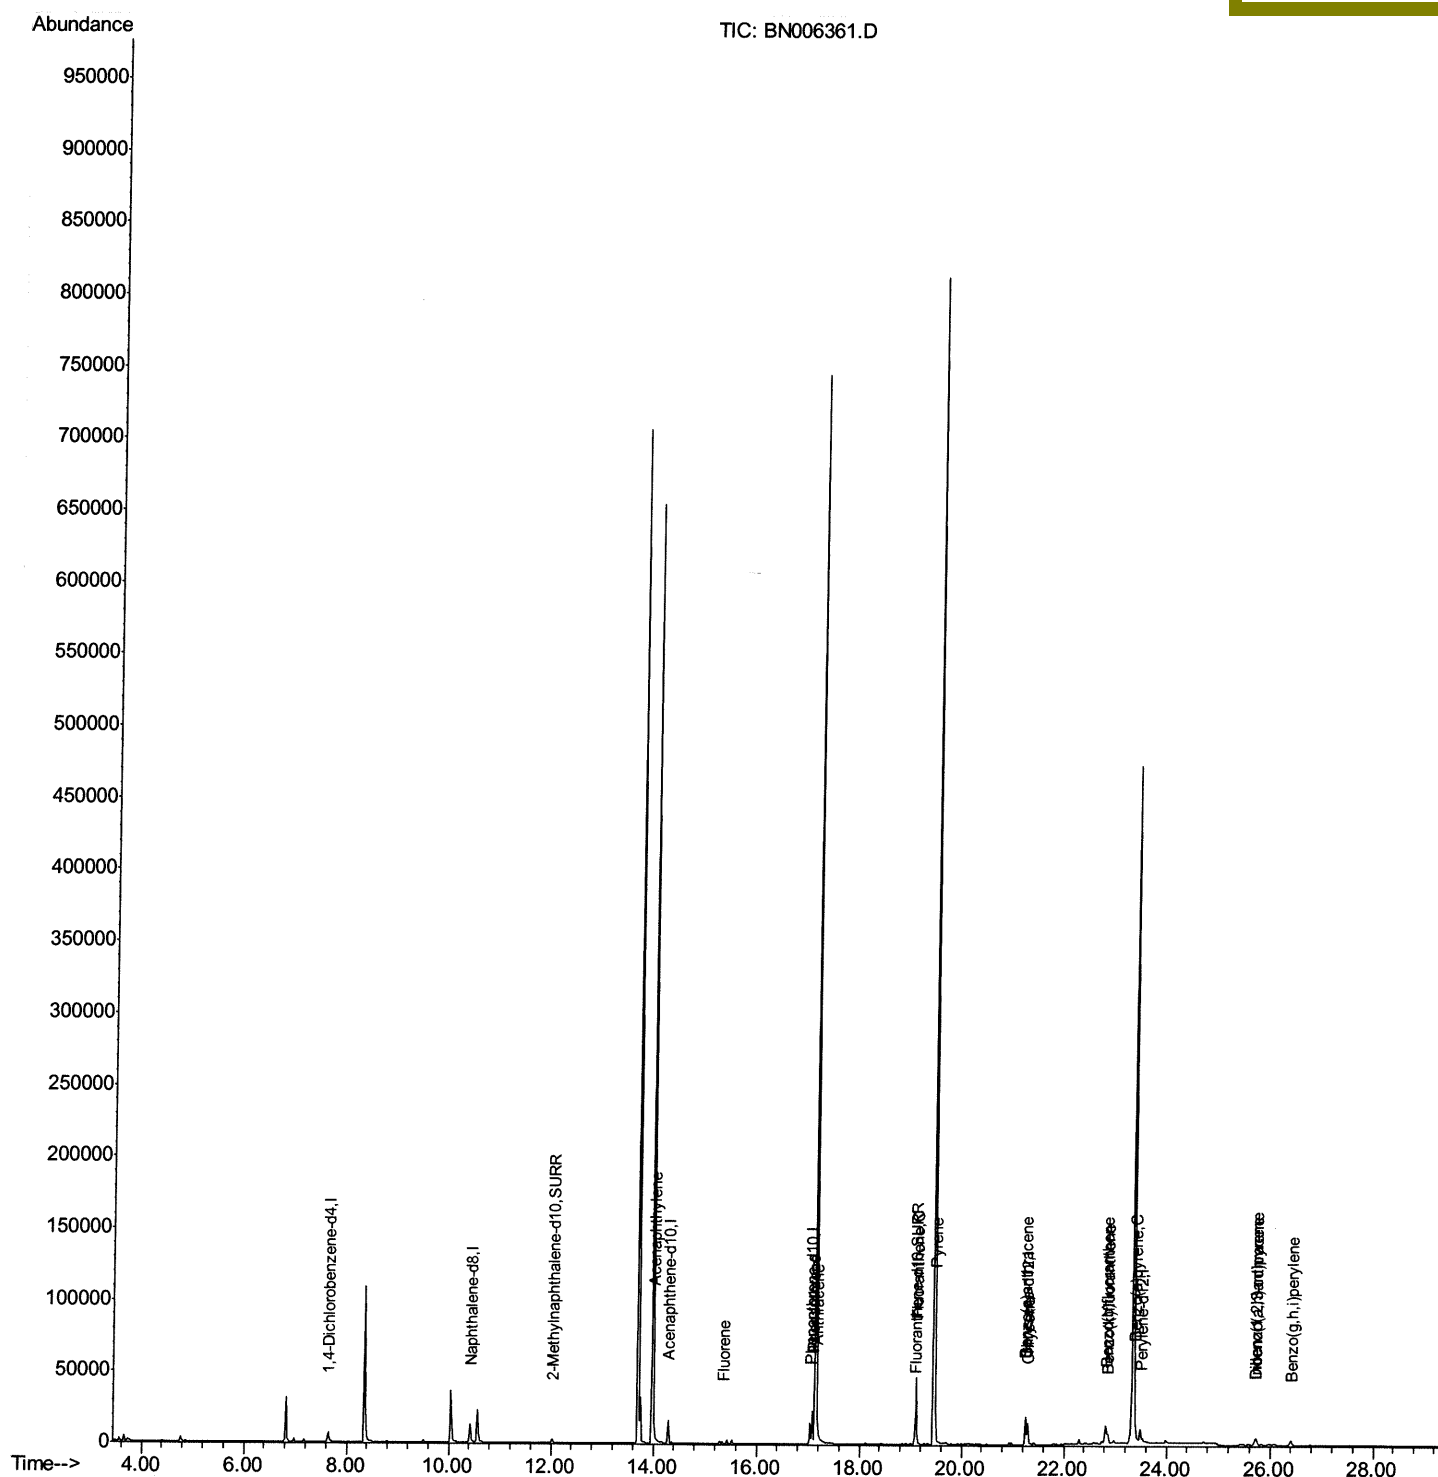

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006361.D
 Acq On : 17 Jun 2019 22:44
 Operator : JU/SJ
 Sample : K3335-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4237

Quant Time: Jun 18 01:52:15 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:22:47 AM

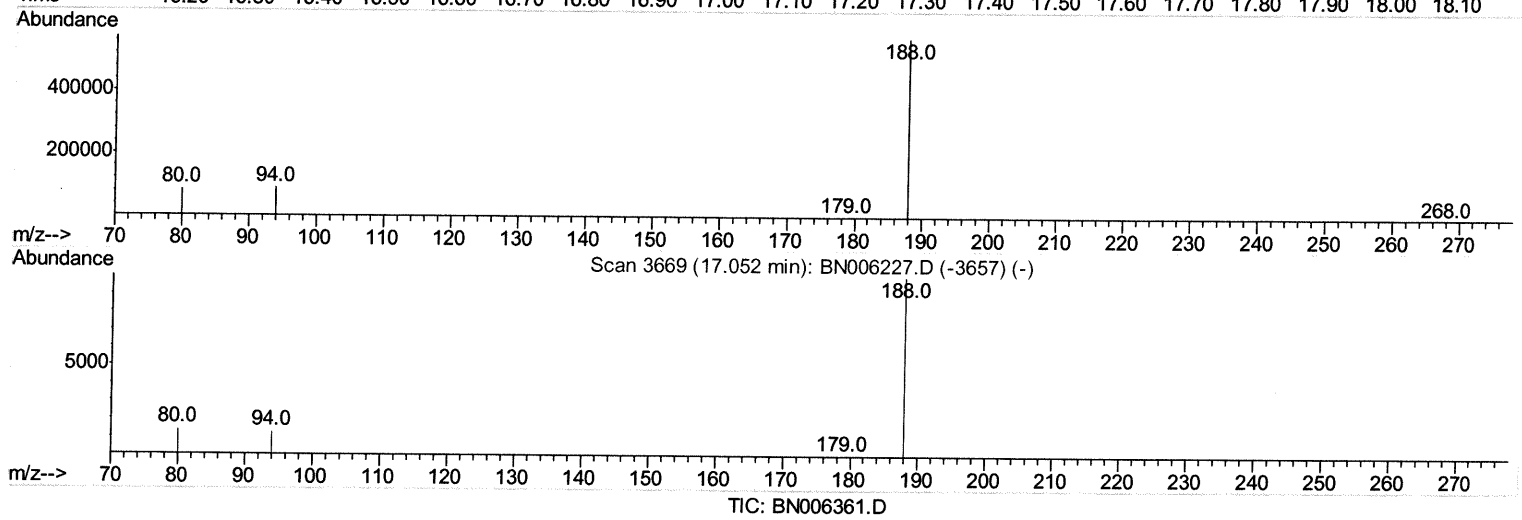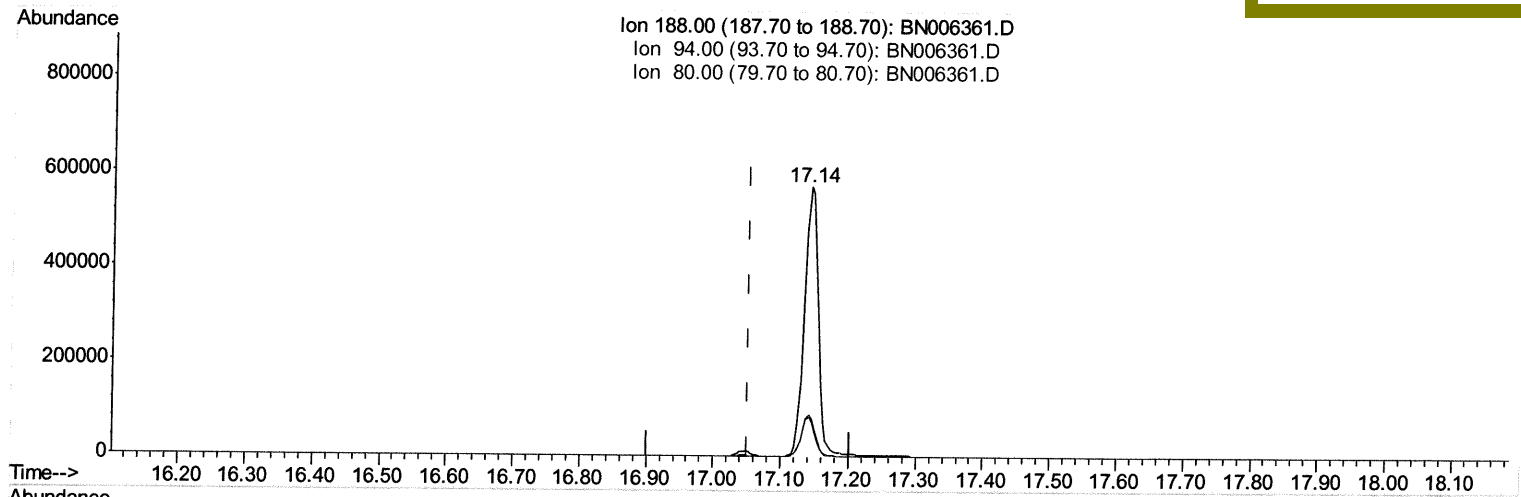

(10) Phenanthrene-d10 (I)

17.141min (+0.089) 0.40ng/ul

response 812889

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	15.58
80.00	13.60	14.46
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006361.D
 Acq On : 17 Jun 2019 22:44
 Operator : JU/SJ
 Sample : K3335-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4237

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:22:47 AM

Quant Time: Jun 18 01:52:15 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

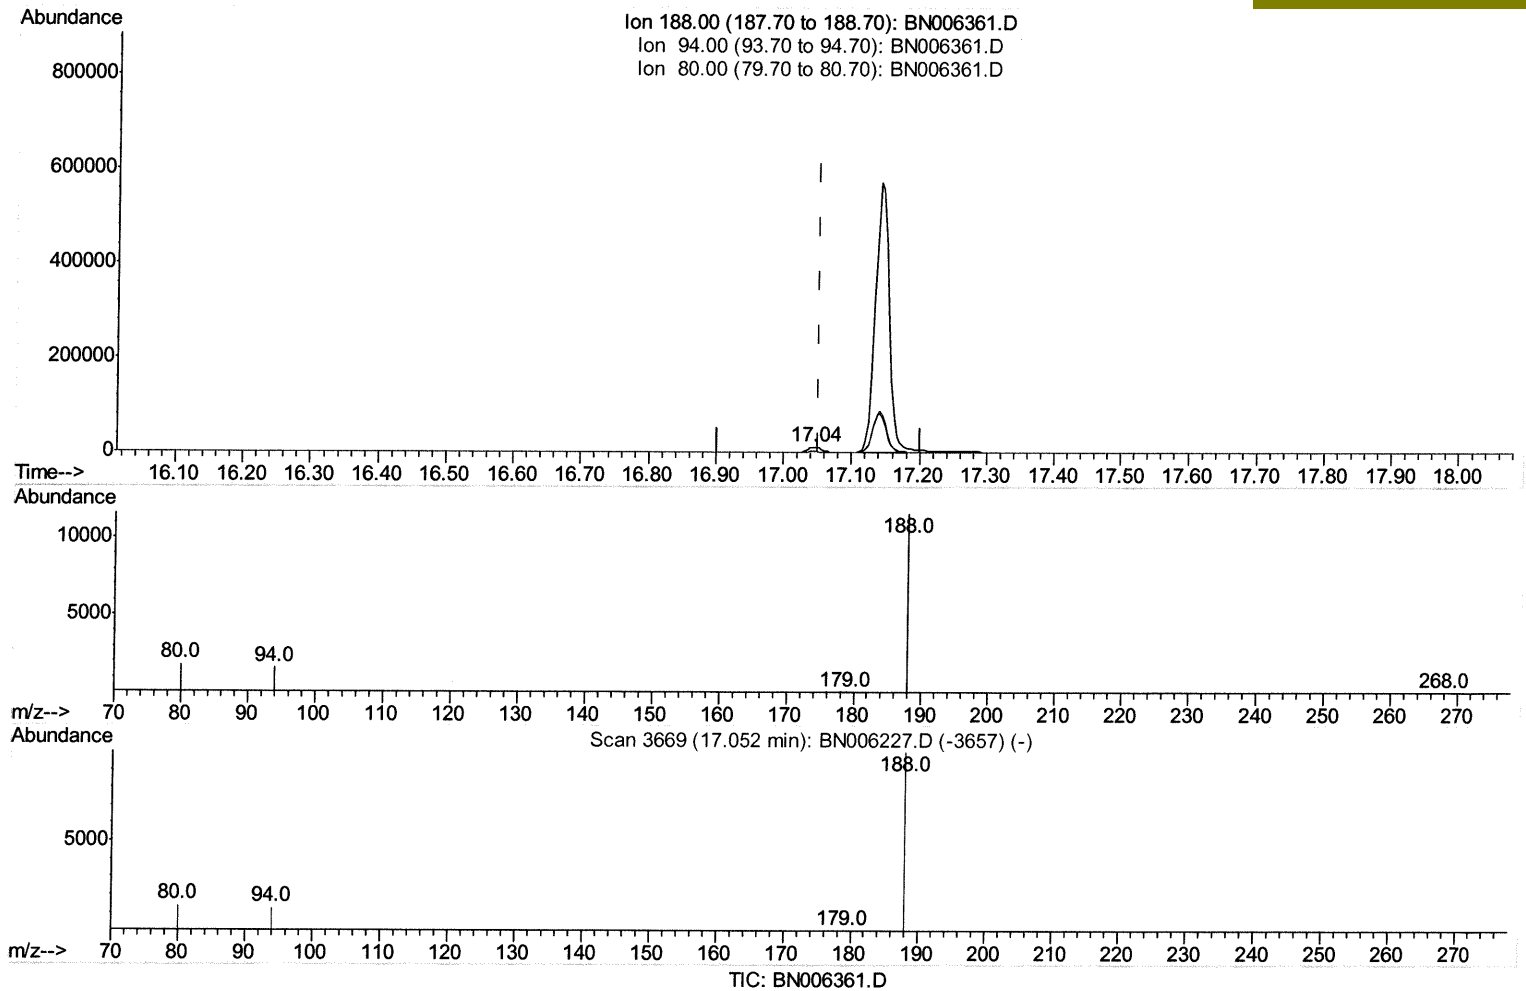

(10) Phenanthrene-d10 (I)

17.044min (-0.008) 0.40ng/ul m *JU 06/18/19*

response 16876

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	14.01
80.00	13.60	15.59
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006361.D
 Acq On : 17 Jun 2019 22:44
 Operator : JU/SJ
 Sample : K3335-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4237

Quant Time: Jun 18 04:16:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:22:47 AM

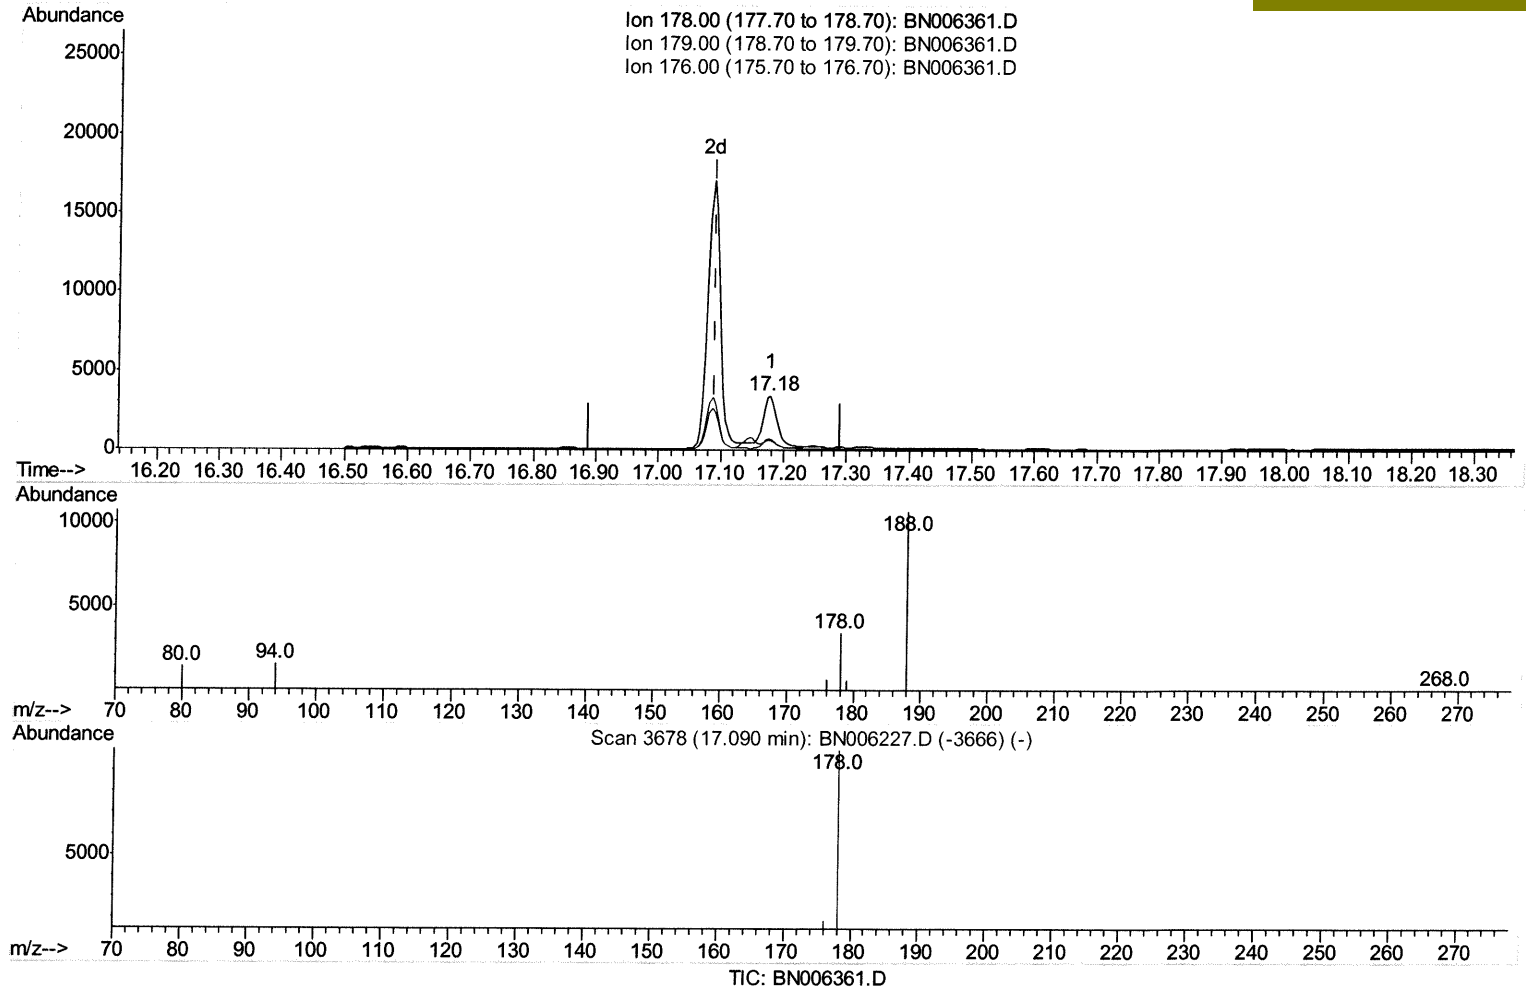

(12) Phenanthrene

17.179min (+0.089) 0.11ng/ul

response 5877

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	18.21
176.00	19.10	20.12
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006361.D
 Acq On : 17 Jun 2019 22:44
 Operator : JU/SJ
 Sample : K3335-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4237

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:22:47 AM

Quant Time: Jun 18 04:16:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

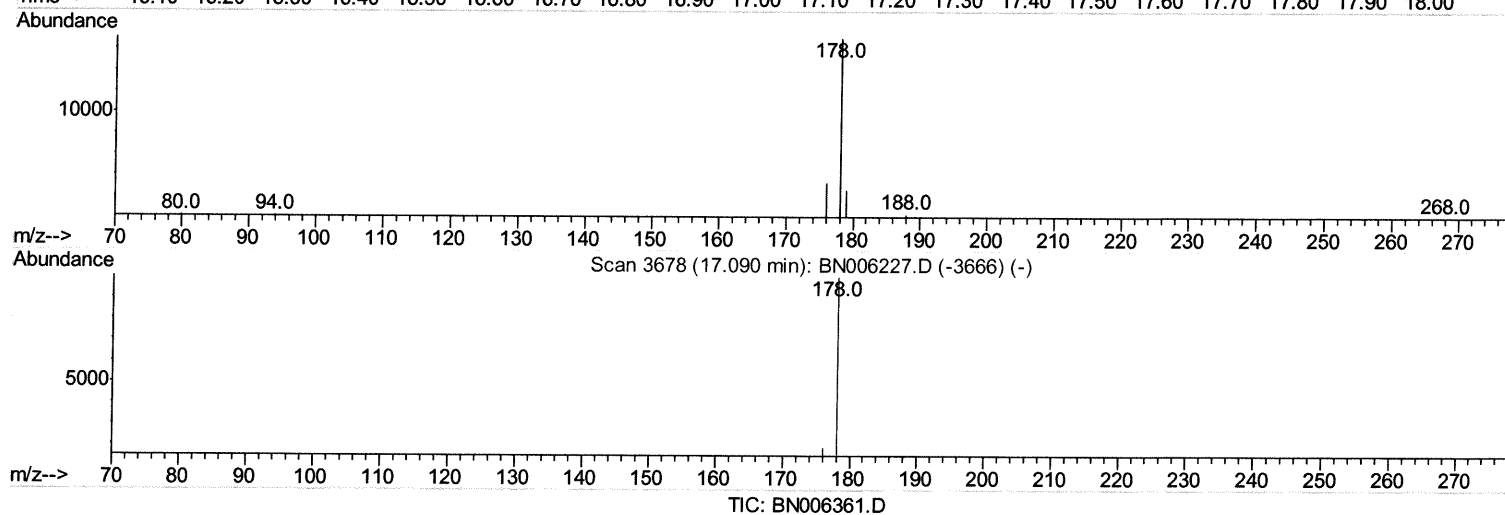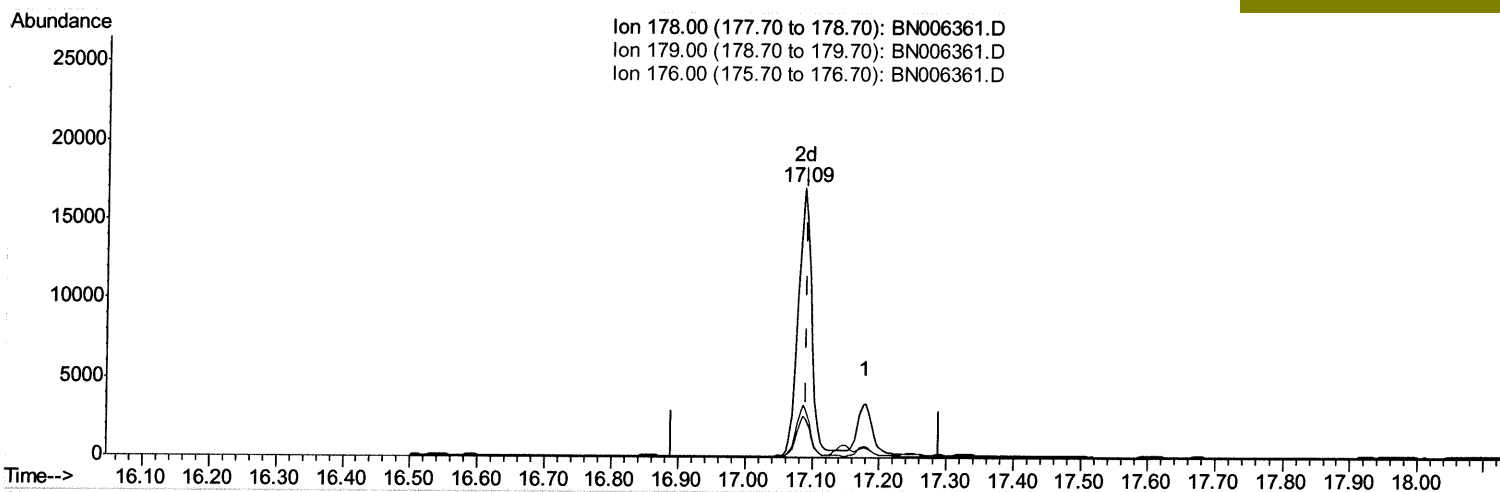

(12) Phenanthrene

17.086min (-0.004) 0.43ng/ul m *JU 06/18/19*

response 23472

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	15.59
176.00	19.10	19.40
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006361.D
 Acq On : 17 Jun 2019 22:44
 Operator : JU/SJ
 Sample : K3335-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4237

Quant Time: Jun 18 04:16:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:22:47 AM

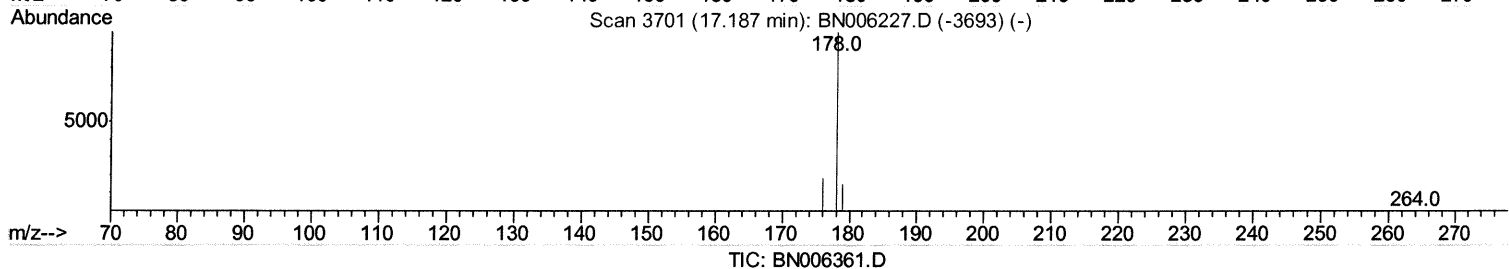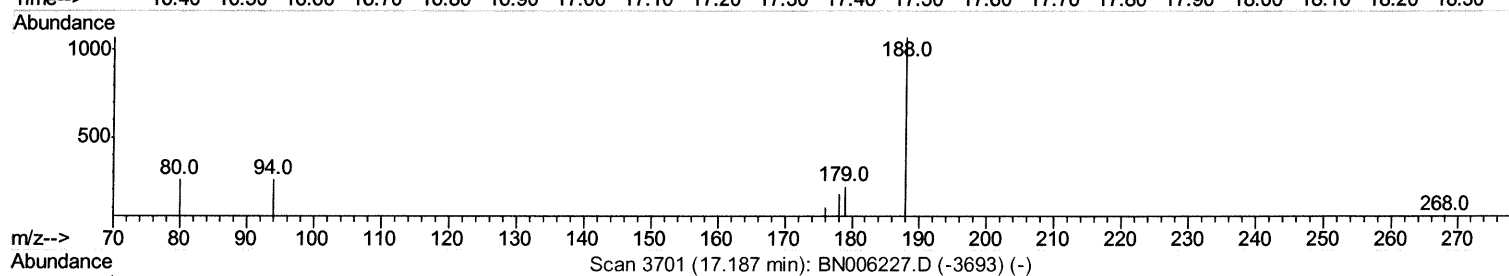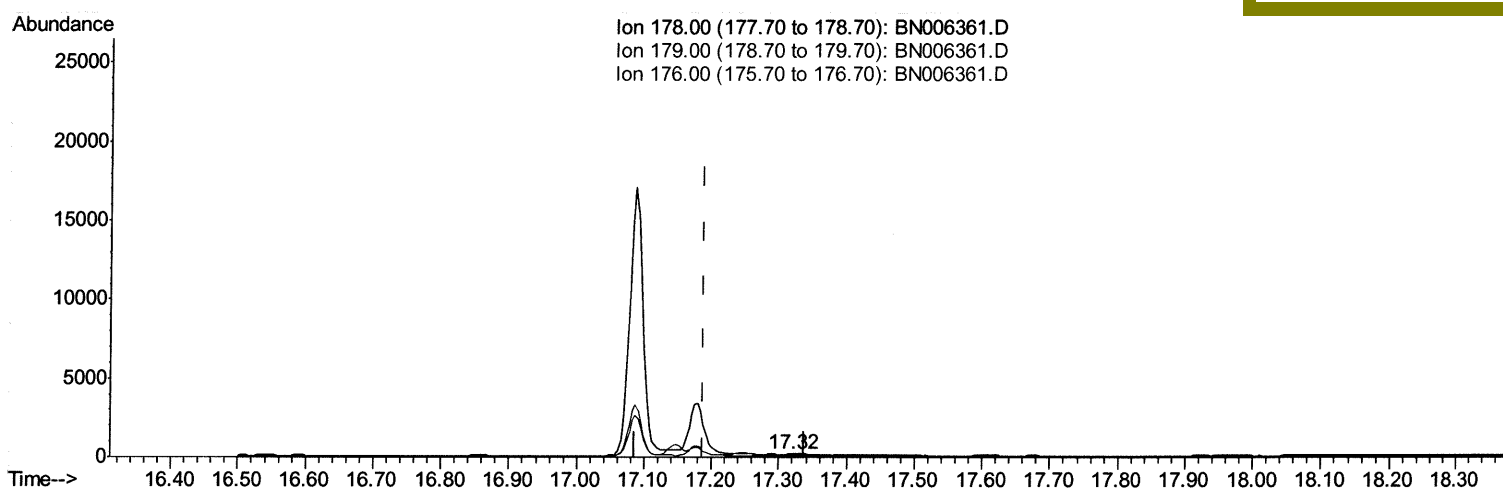

(13) Anthracene

17.318min (+0.131) 0.00ng/ul

response 146

Ion	Exp%	Act%
178.00	100	100
179.00	15.30	126.90#
176.00	18.90	56.73#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006361.D
 Acq On : 17 Jun 2019 22:44
 Operator : JU/SJ
 Sample : K3335-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4237

Quant Time: Jun 18 04:16:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:22:47 AM

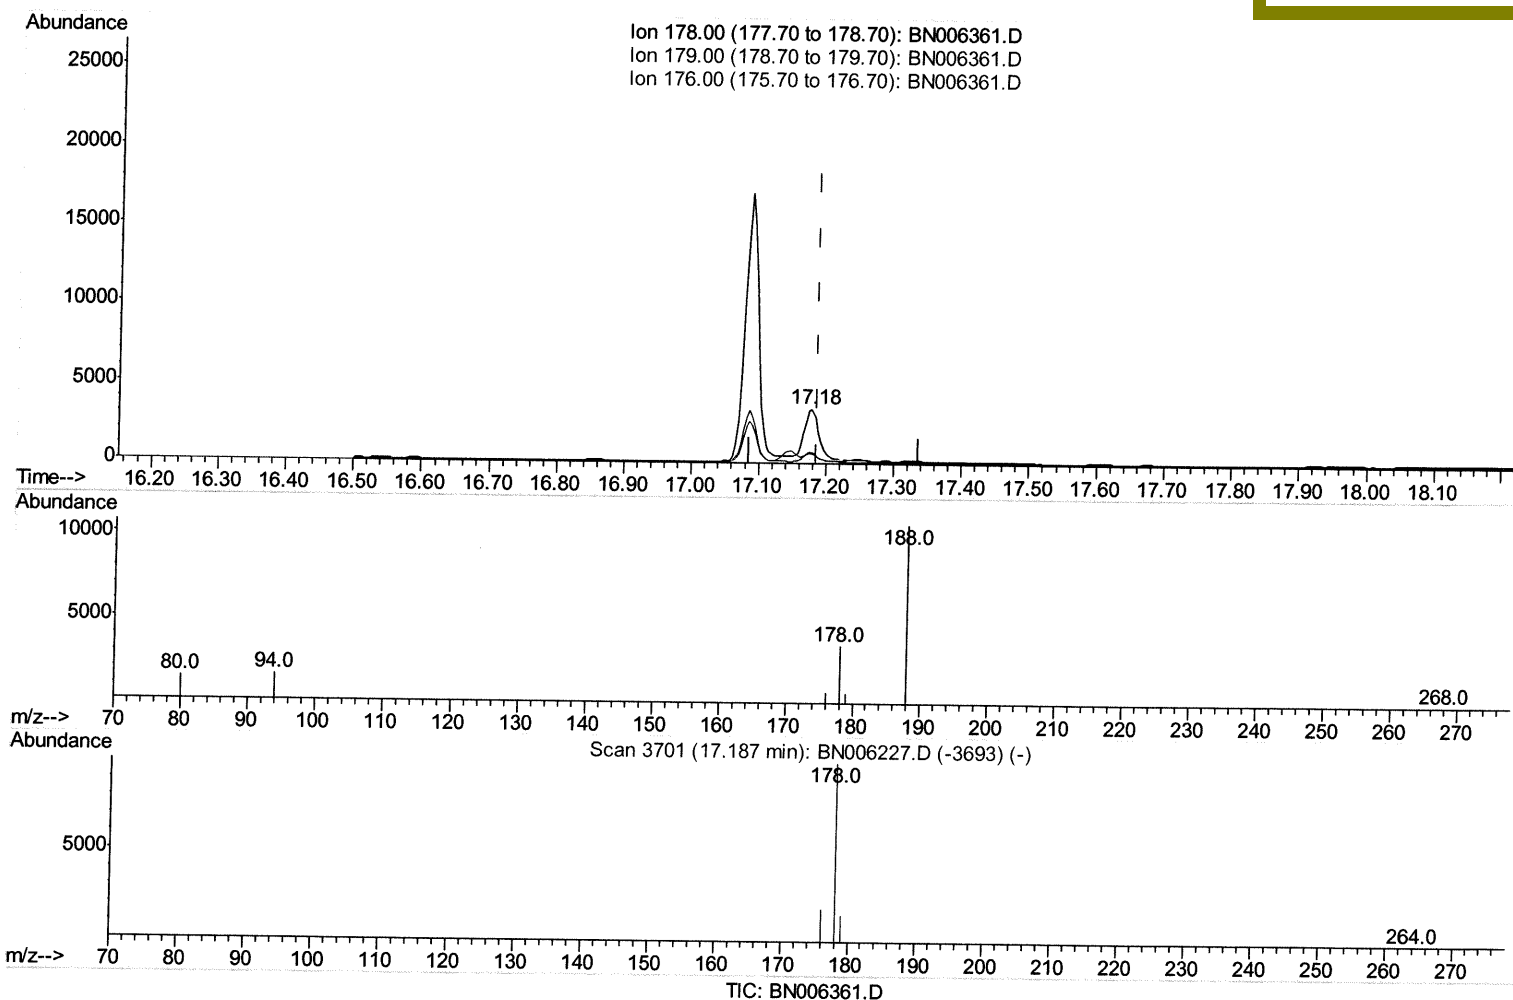

(13) Anthracene

17.179min (-0.008) 0.09ng/ul m *JU* 06/18/19

response 4792

Ion	Exp%	Act%
178.00	100	100
179.00	15.30	18.21
176.00	18.90	20.12
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
Data File : BN006361.D
Acq On : 17 Jun 2019 22:44
Operator : JU/SJ
Sample : K3335-10
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4237

Manual Integrations
APPROVED

mohammad
6/21/2019 8:22:47 AM

Quant Time: Jun 18 04:16:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

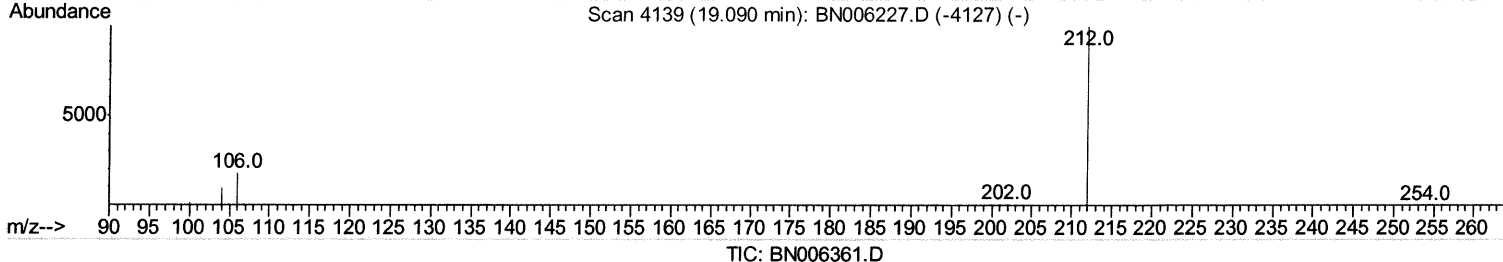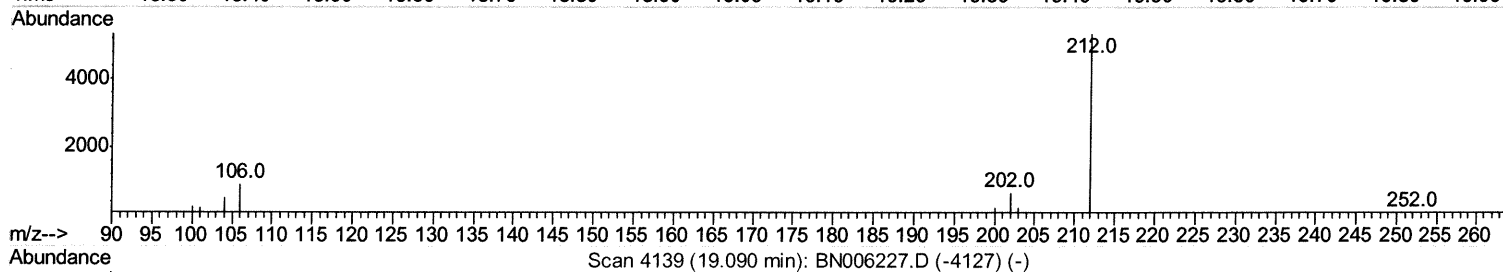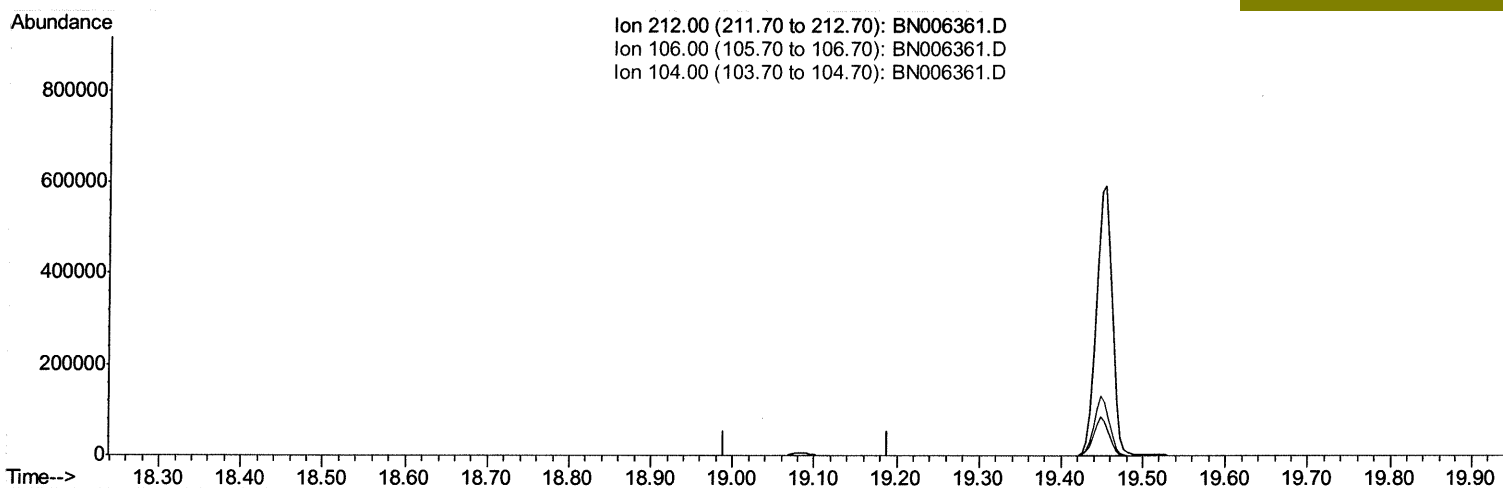

(14) Fluoranthene-d10 (SURR)

19.090min (-19.090) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006361.D
 Acq On : 17 Jun 2019 22:44
 Operator : JU/SJ
 Sample : K3335-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4237

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:22:47 AM

Quant Time: Jun 18 04:16:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

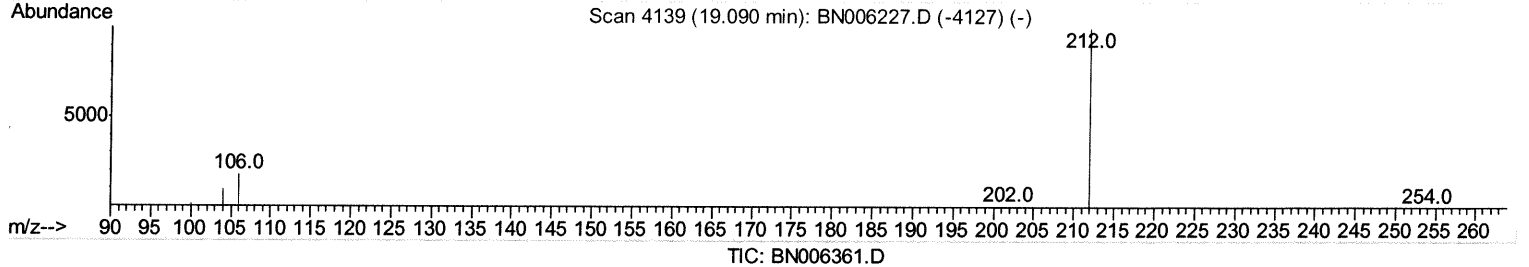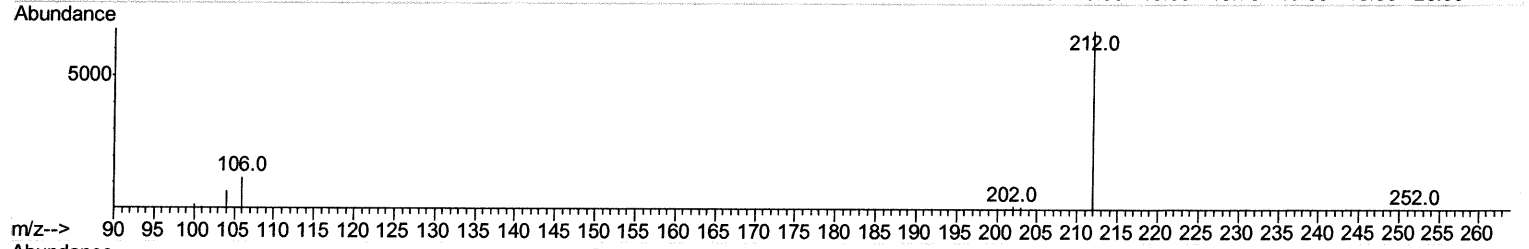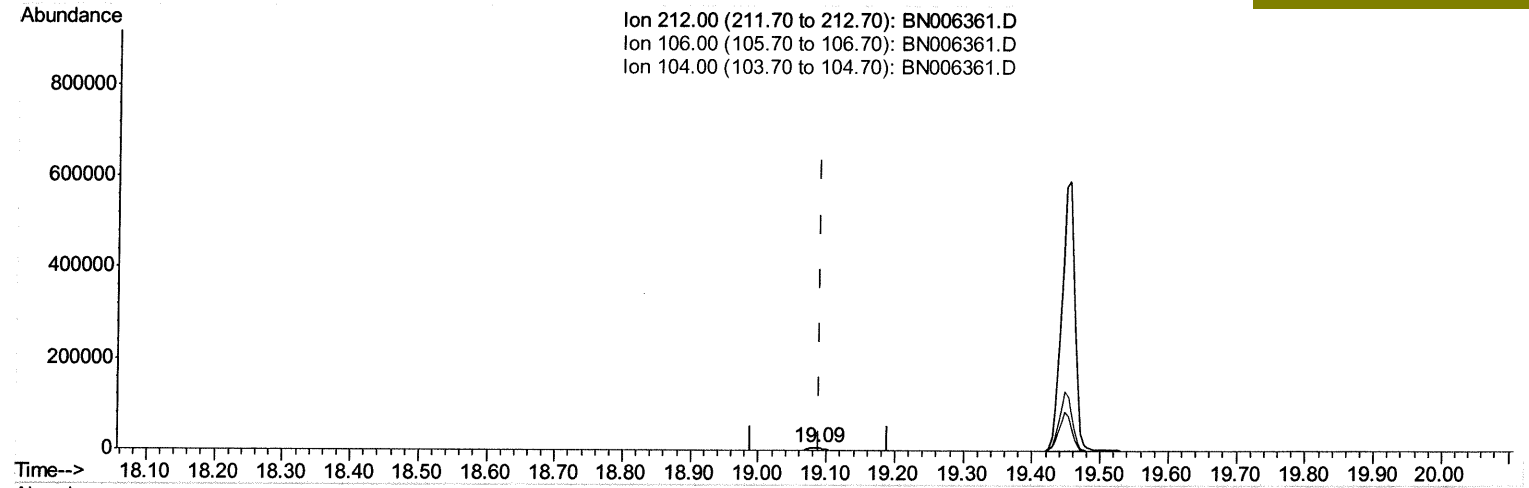

(14) Fluoranthene-d10 (SURR)

19.086min (-0.005) 0.19ng/ul m

response 8661

Ion	Exp%	Act%
212.00	100	100
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00

JU
 06/18/19

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006361.D
 Acq On : 17 Jun 2019 22:44
 Operator : JU/SJ
 Sample : K3335-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4237

Quant Time: Jun 18 04:16:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:22:47 AM

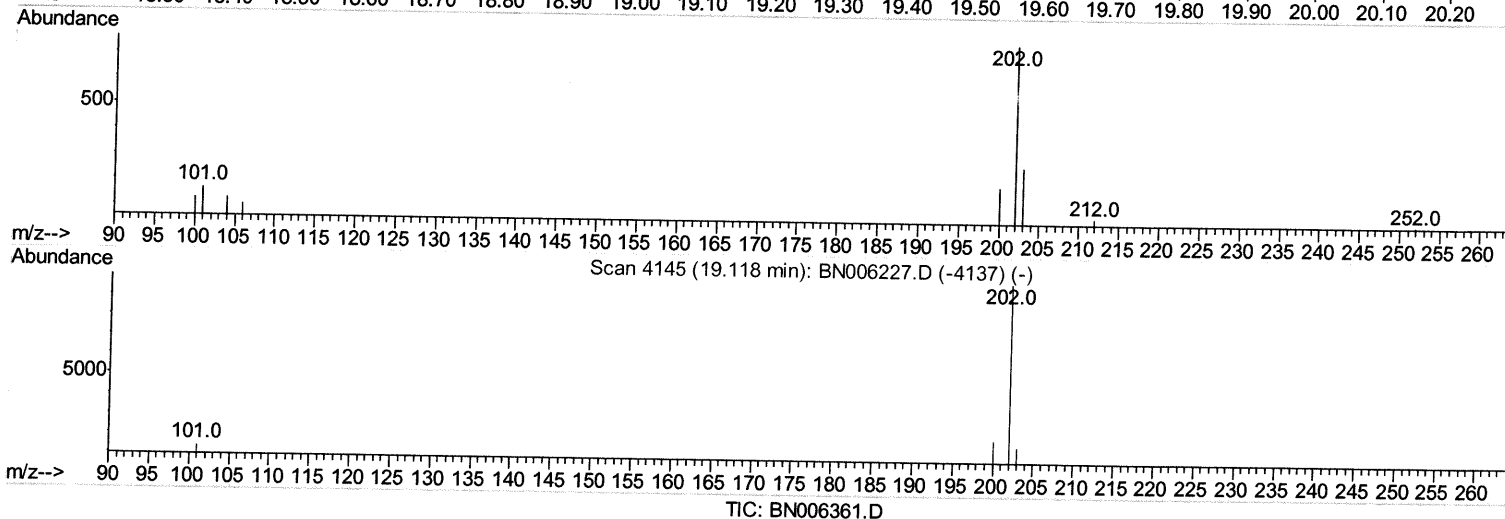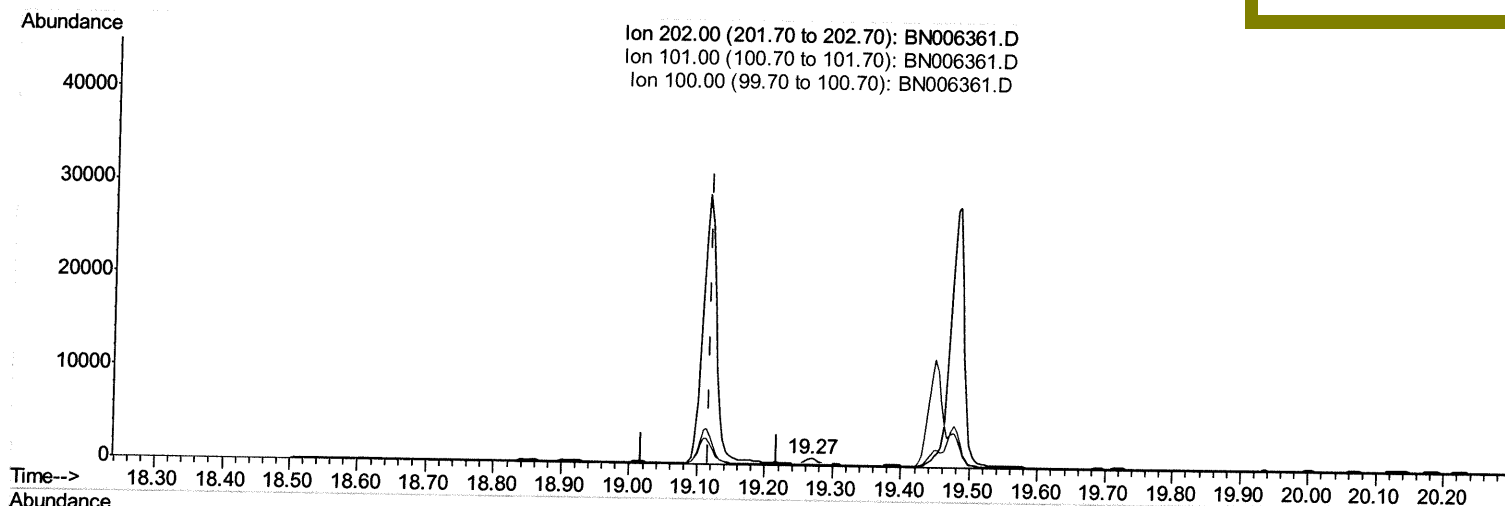

(15) Fluoranthene (C)

19.267min (+0.149) 0.01ng/ul

response 739

Ion	Exp%	Act%
202.00	100	100
101.00	12.10	22.50
100.00	8.70	17.24
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006361.D
 Acq On : 17 Jun 2019 22:44
 Operator : JU/SJ
 Sample : K3335-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4237

Quant Time: Jun 18 04:16:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:22:47 AM

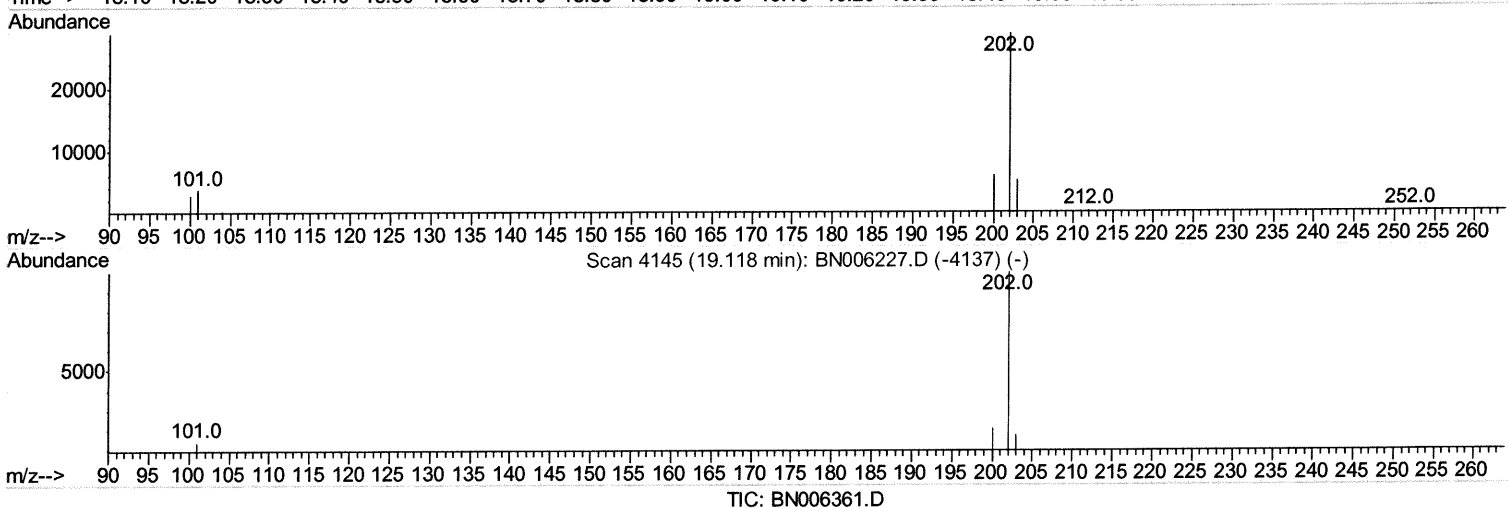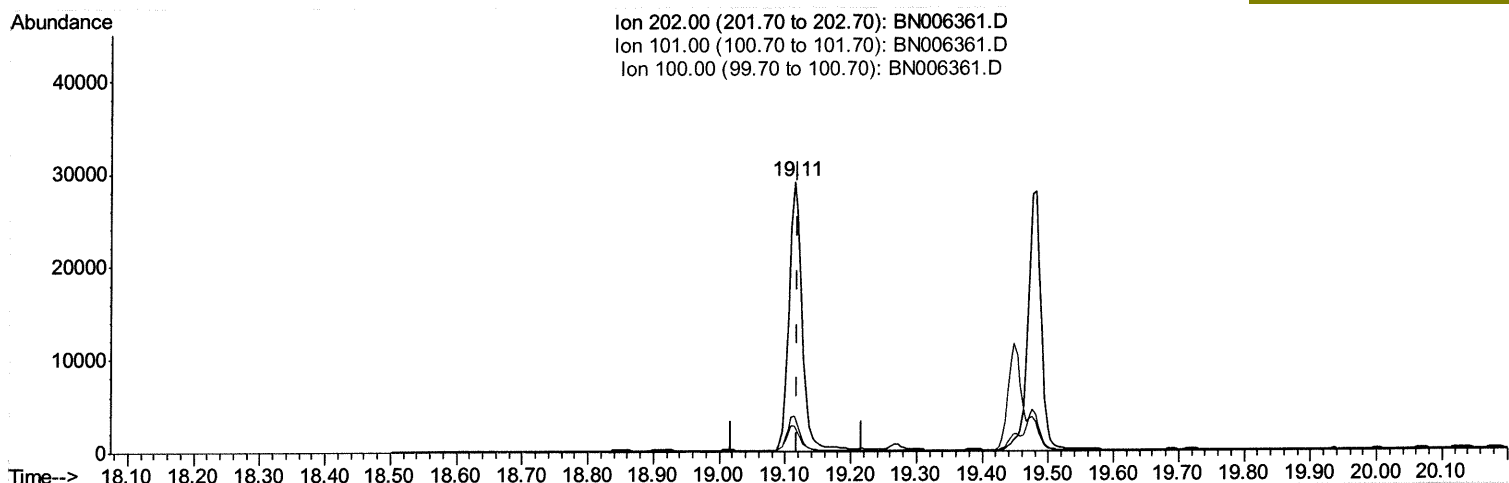

(15) Fluoranthene (C)

19.113min (-0.005) 0.67ng/ul m *JU 06/18/19*

response 40363

Ion	Exp%	Act%
202.00	100	100
101.00	12.10	13.10
100.00	8.70	9.72
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006361.D
 Acq On : 17 Jun 2019 22:44
 Operator : JU/SJ
 Sample : K3335-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4237

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:22:47 AM

Quant Time: Jun 18 04:16:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

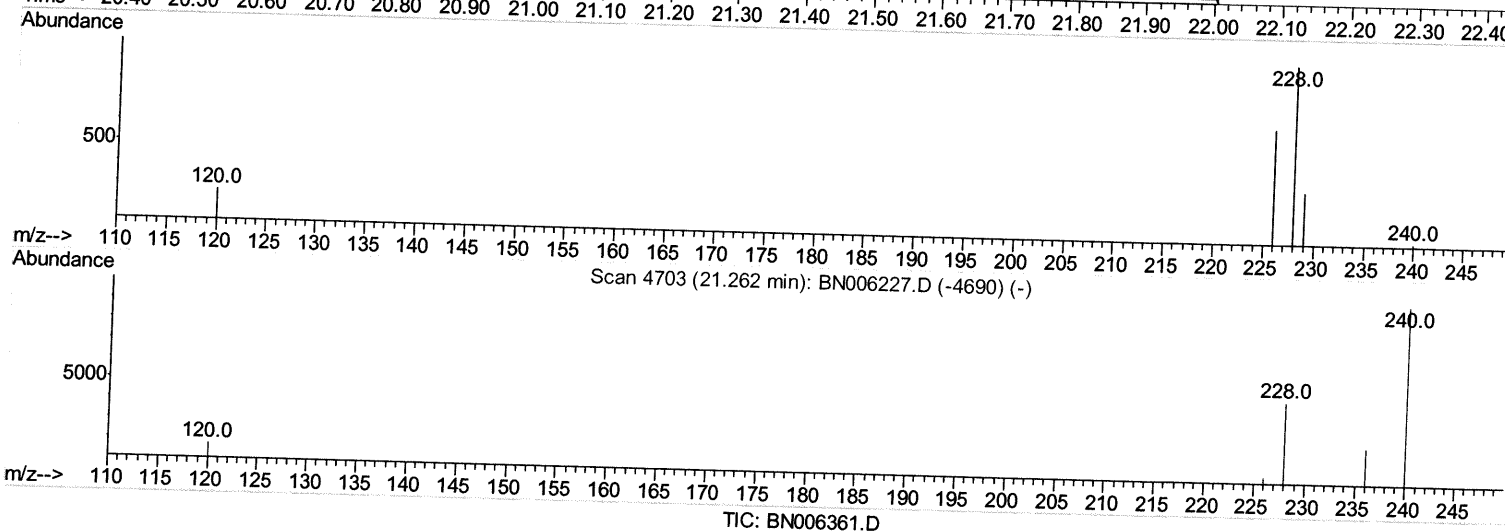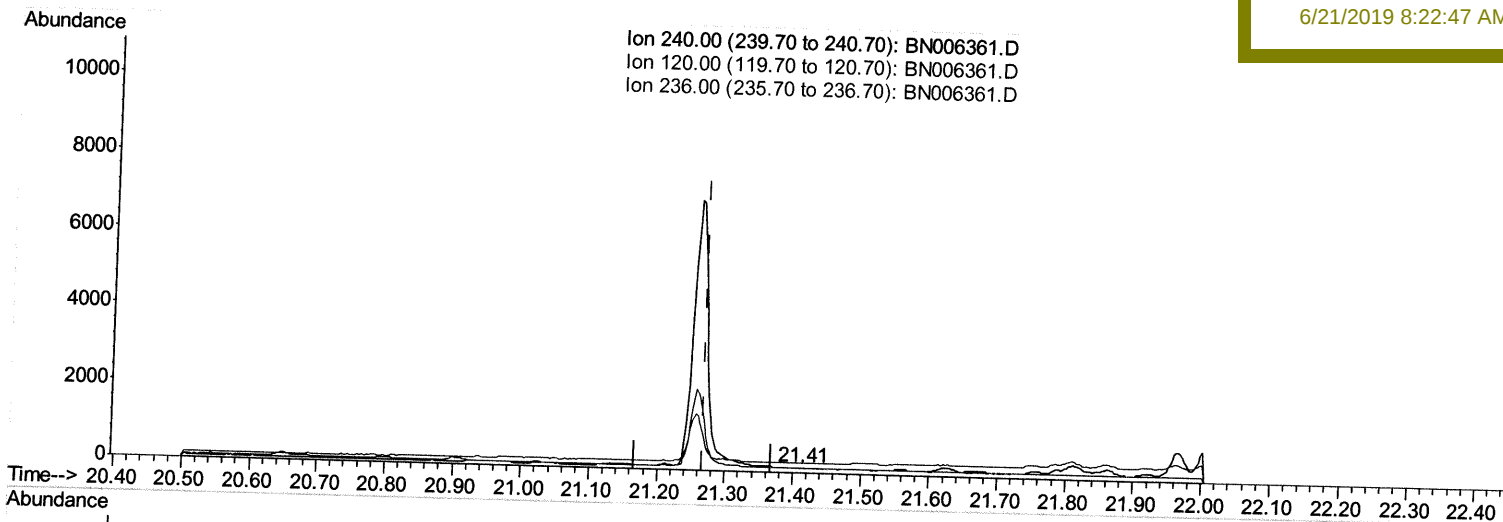

(16) Chrysene-d12 (I)

21.411min (+0.143) 0.40ng/ul

response 51

Ion	Exp%	Act%
240.00	100	100
120.00	20.10	194.96#
236.00	30.10	91.37#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006361.D
 Acq On : 17 Jun 2019 22:44
 Operator : JU/SJ
 Sample : K3335-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4237

Quant Time: Jun 18 04:16:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:22:47 AM

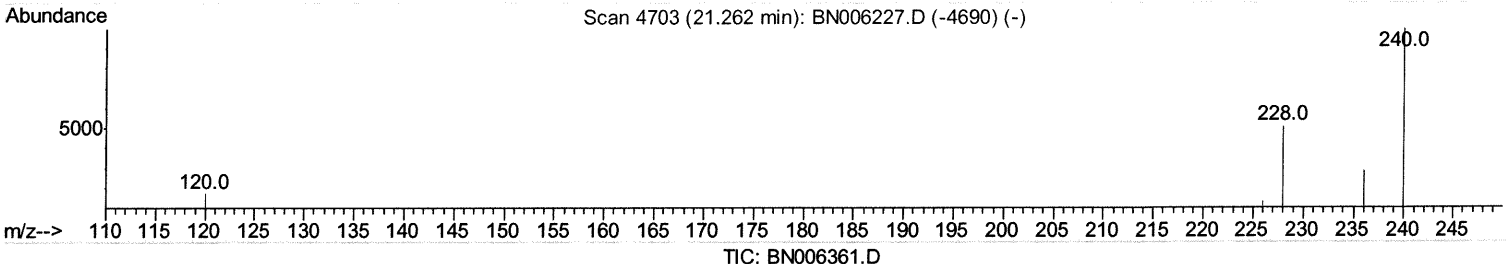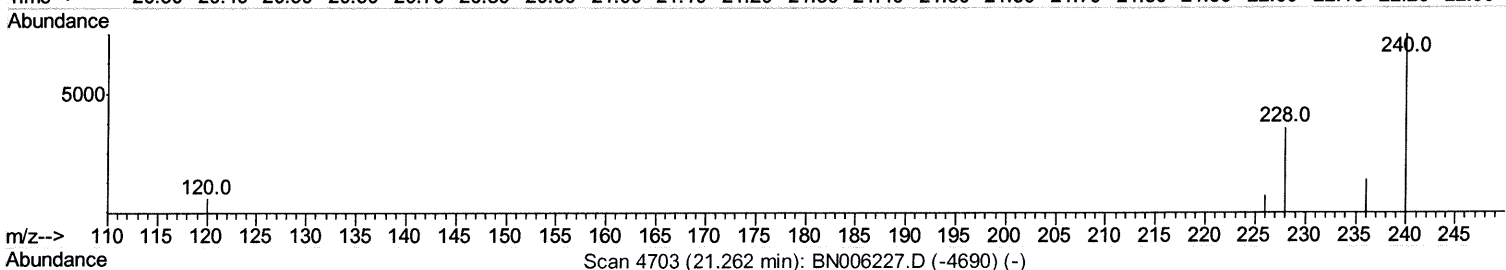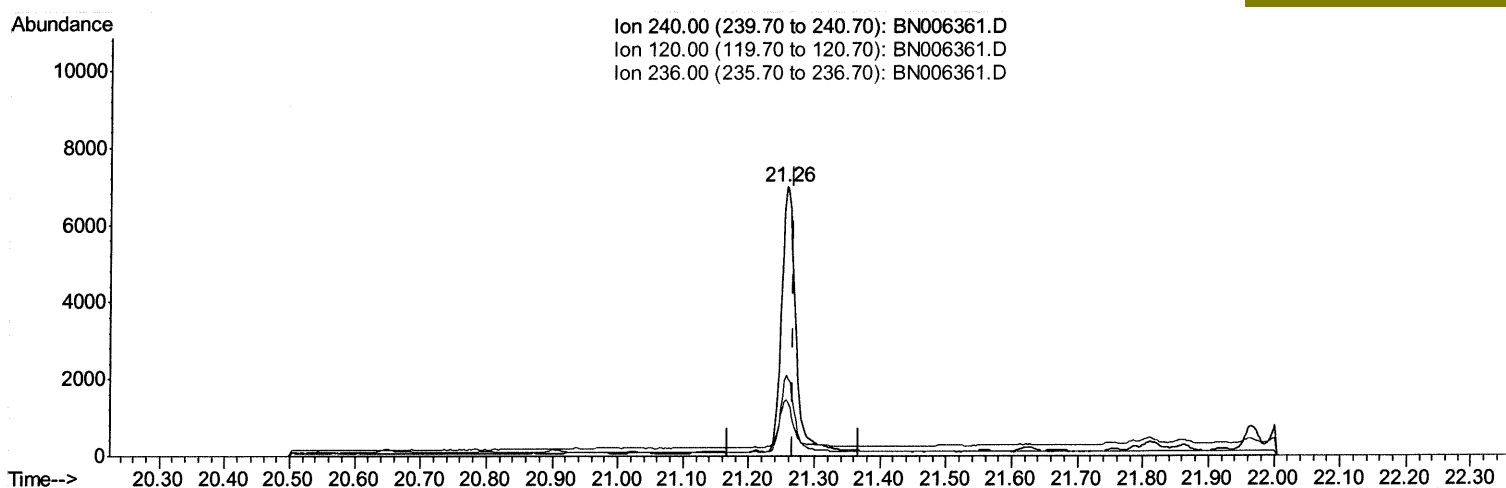

(16) Chrysene-d12 (I)

21.257min (-0.012) 0.40ng/ul m ^{JU} 06/18/19

response 10472

Ion	Exp%	Act%
240.00	100	100
120.00	20.10	20.80
236.00	30.10	29.99
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006361.D
 Acq On : 17 Jun 2019 22:44
 Operator : JU/SJ
 Sample : K3335-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4237

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:22:47 AM

Quant Time: Jun 18 04:18:25 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

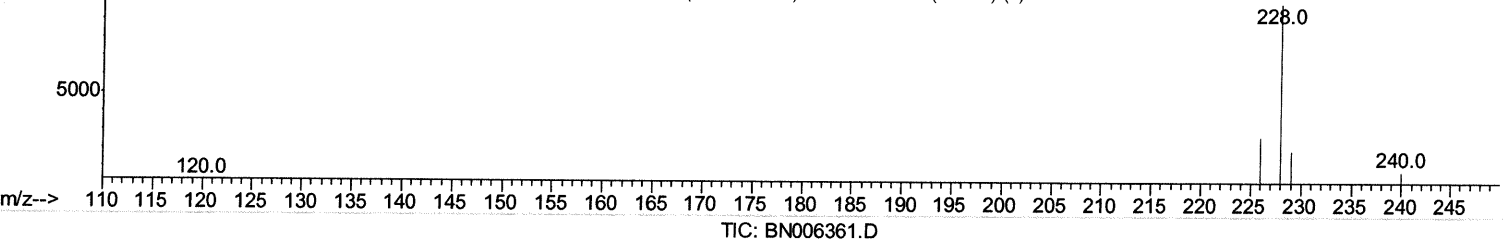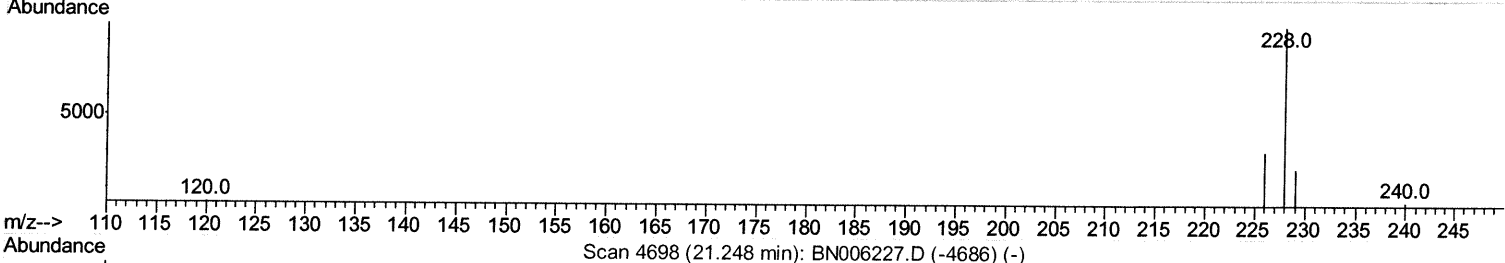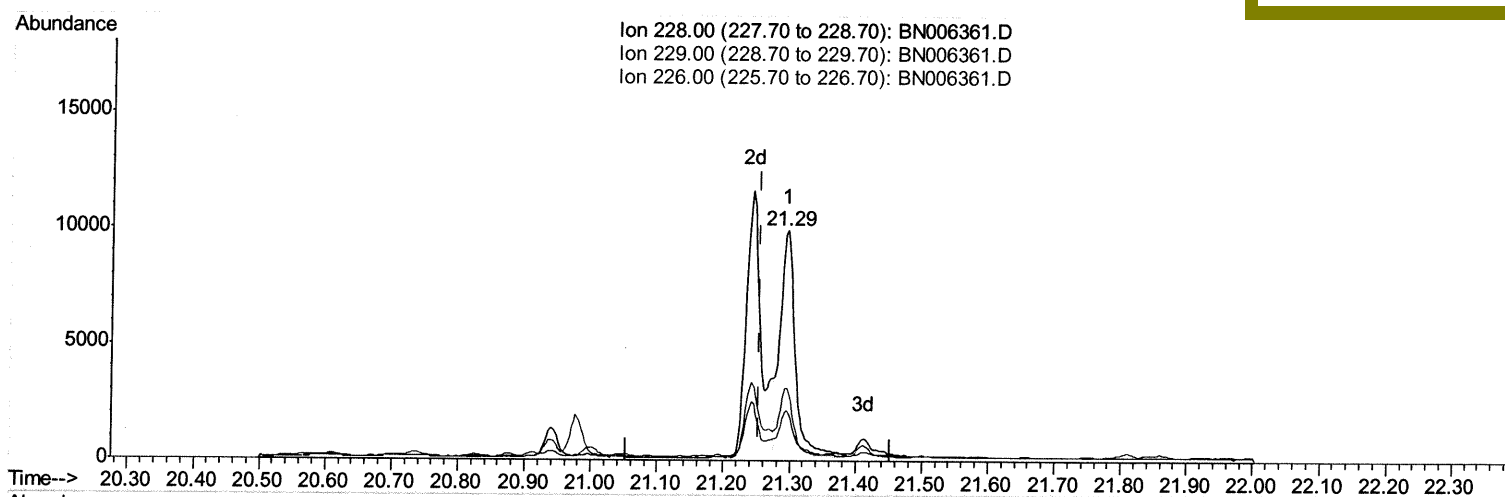

(18) Benzo(a)anthracene
 21.295min (+0.041) 0.35ng/ul
 response 16082

Ion	Exp%	Act%
228.00	100	100
229.00	20.60	21.97
226.00	28.50	31.52
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006361.D
 Acq On : 17 Jun 2019 22:44
 Operator : JU/SJ
 Sample : K3335-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4237

Quant Time: Jun 18 04:18:25 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:22:47 AM

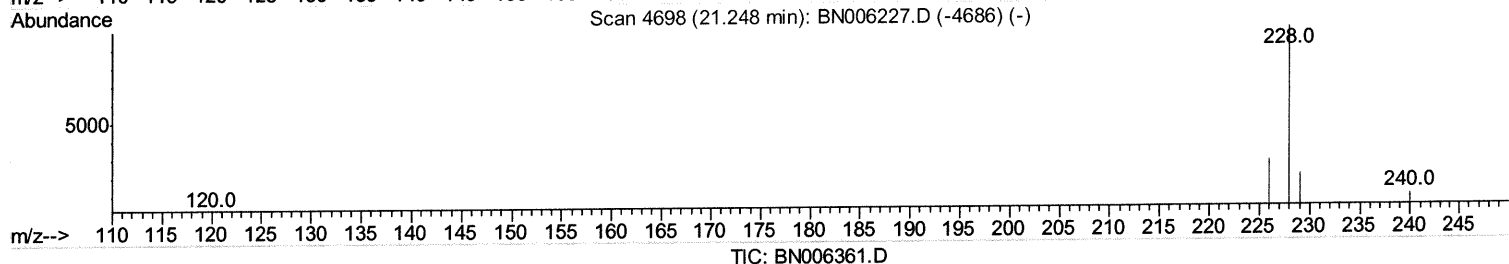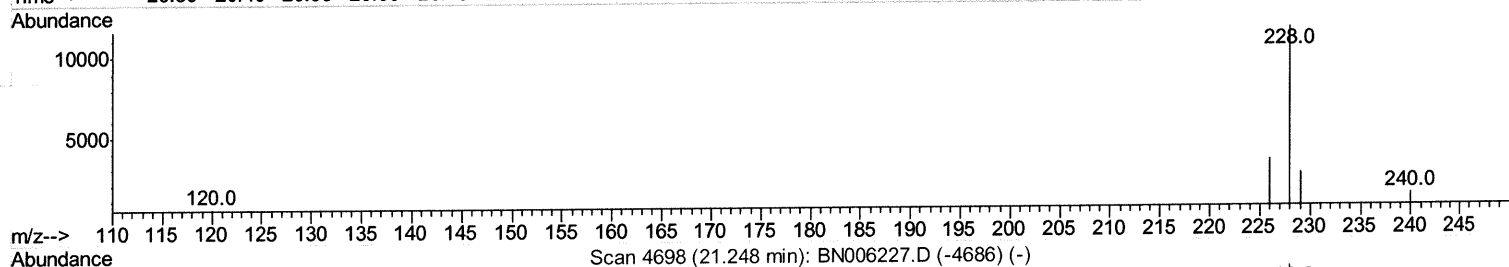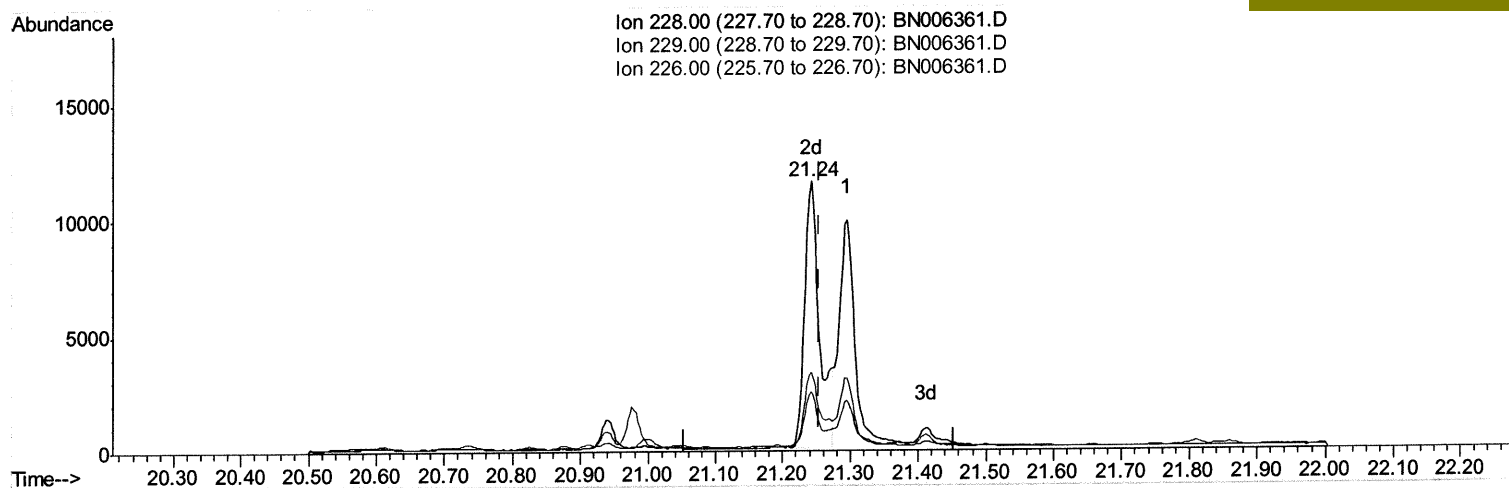

(18) Benzo(a)anthracene

21.242min (-0.012) 0.39ng/ul m *JU 06/18/19*

response 18092

Ion	Exp%	Act%
228.00	100	100
229.00	20.60	21.86
226.00	28.50	28.92
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006361.D
 Acq On : 17 Jun 2019 22:44
 Operator : JU/SJ
 Sample : K3335-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4237

Quant Time: Jun 18 04:18:25 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:22:47 AM

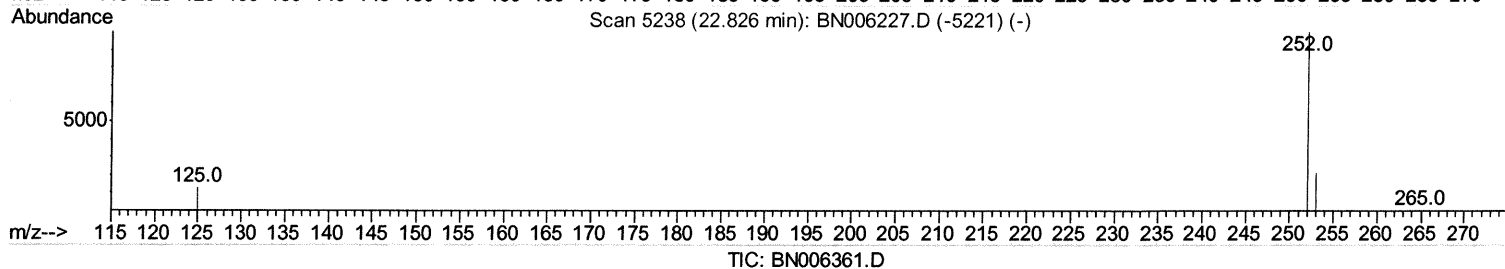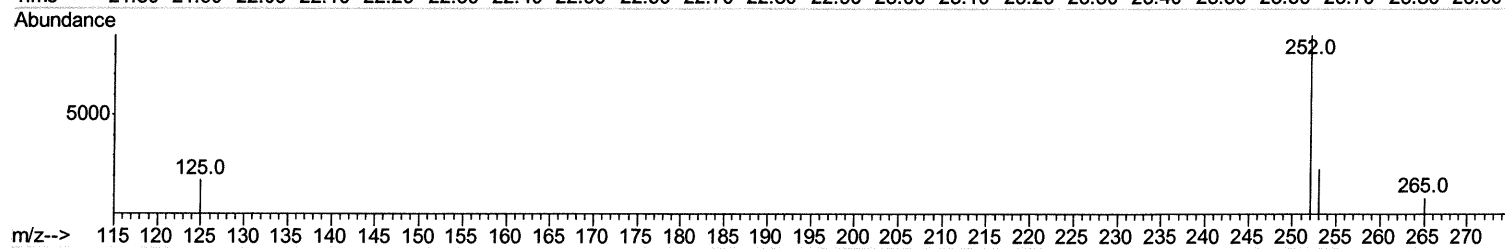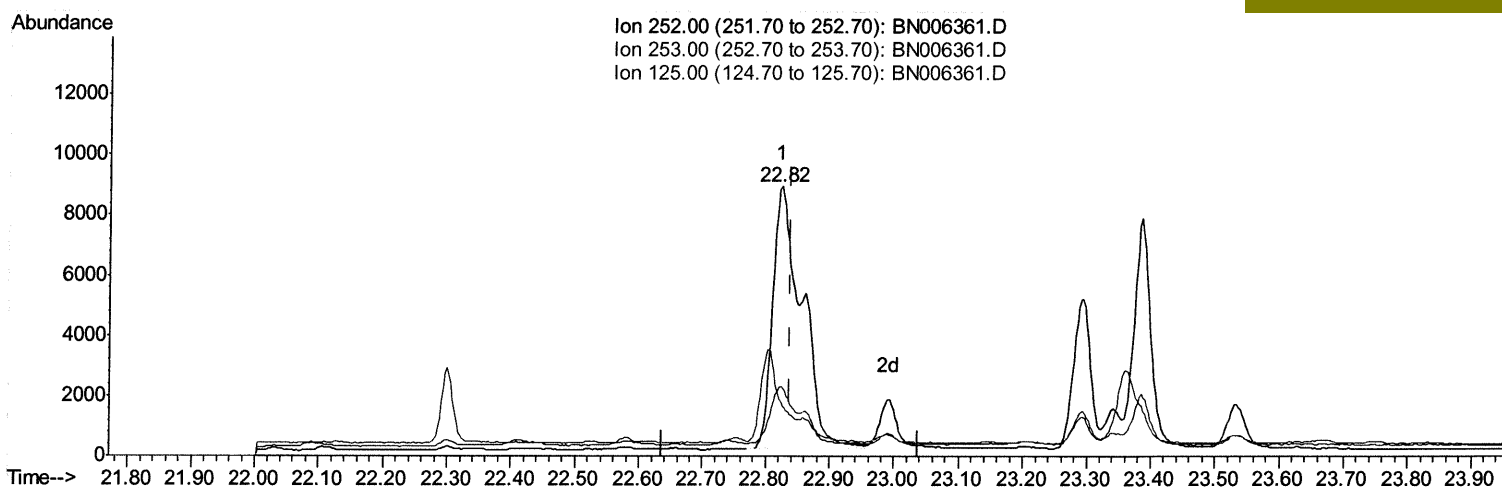

(21) Benzo(b)fluoranthene

22.823min (-0.015) 0.43ng/ul

response 28214

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	26.07
125.00	20.50	19.91
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006361.D
 Acq On : 17 Jun 2019 22:44
 Operator : JU/SJ
 Sample : K3335-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4237

Quant Time: Jun 18 04:18:25 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:22:47 AM

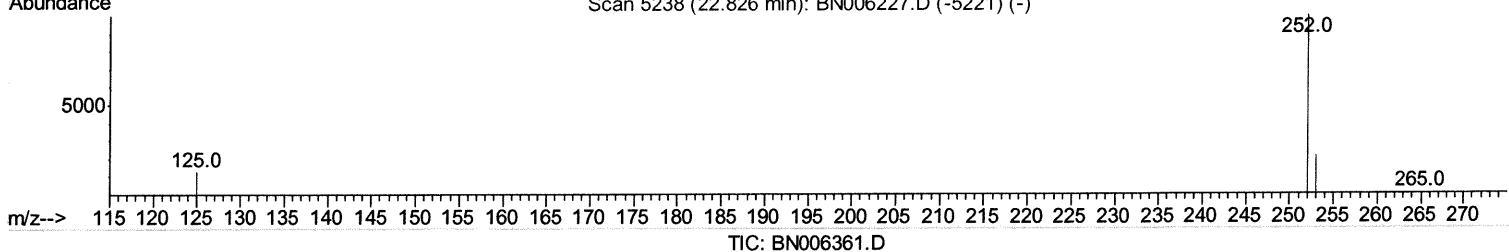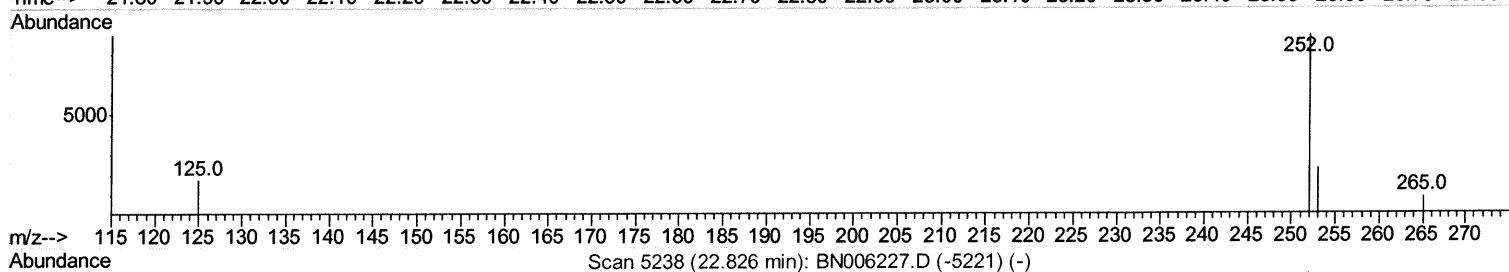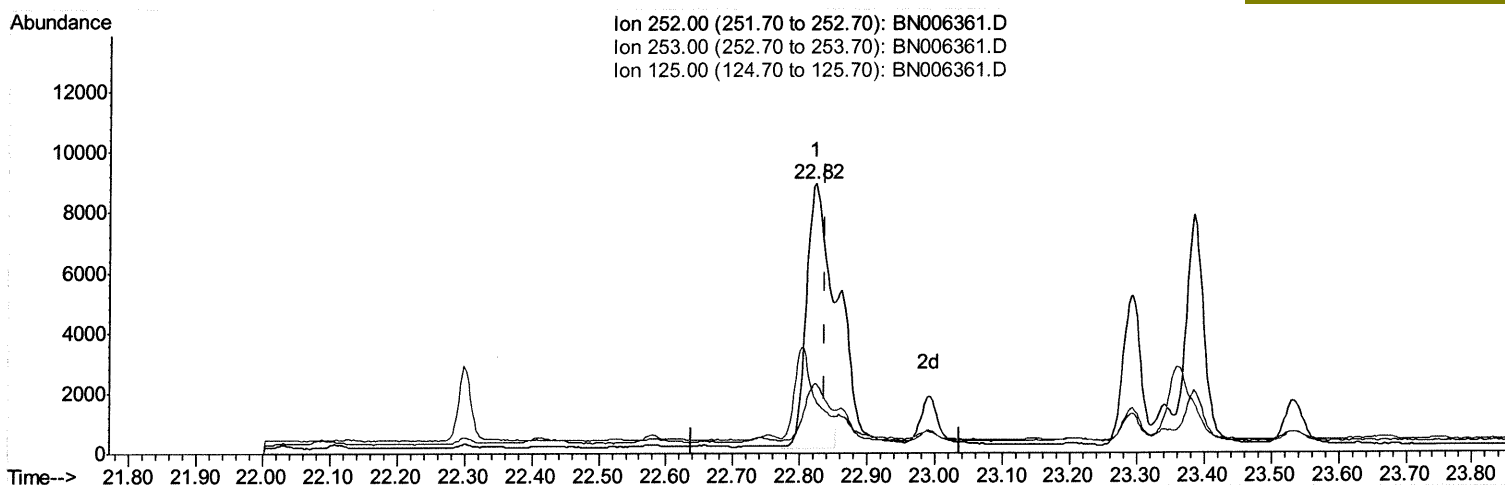

(21) Benzo(b)fluoranthene

22.823min (-0.015) 0.31ng/ul m ^{JU} 06/18/19

response 20484

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	26.07
125.00	20.50	19.91
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006361.D
 Acq On : 17 Jun 2019 22:44
 Operator : JU/SJ
 Sample : K3335-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4237

Quant Time: Jun 18 04:18:25 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:22:47 AM

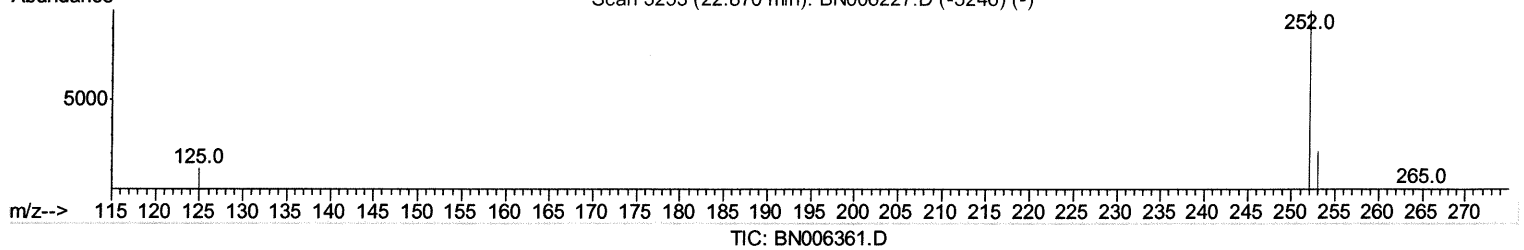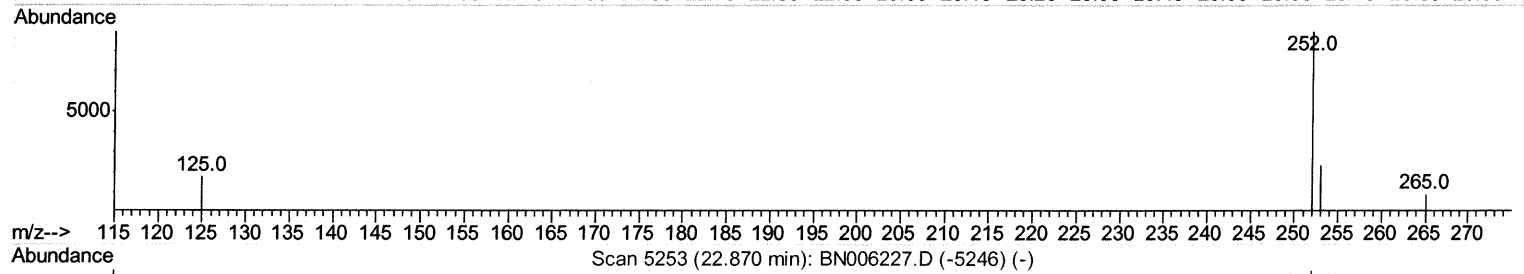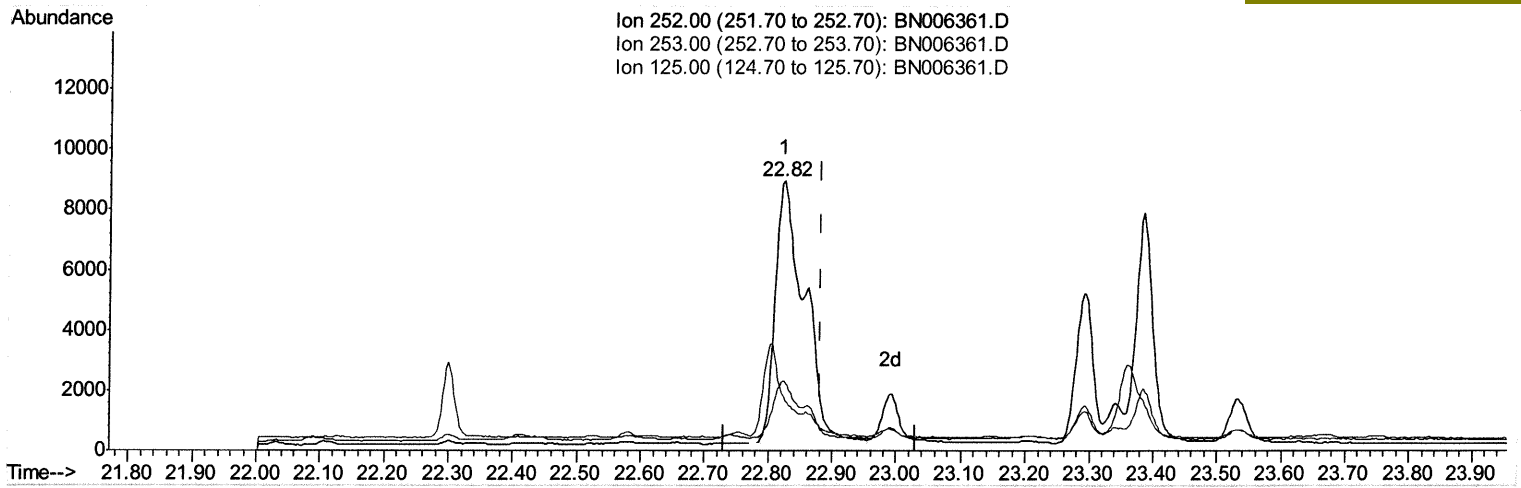

(22) Benzo(k)fluoranthene
 22.823min (-0.058) 0.44ng/ul
 response 28214

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	26.07
125.00	17.90	19.91
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006361.D
 Acq On : 17 Jun 2019 22:44
 Operator : JU/SJ
 Sample : K3335-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4237

Quant Time: Jun 18 04:18:25 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:22:47 AM

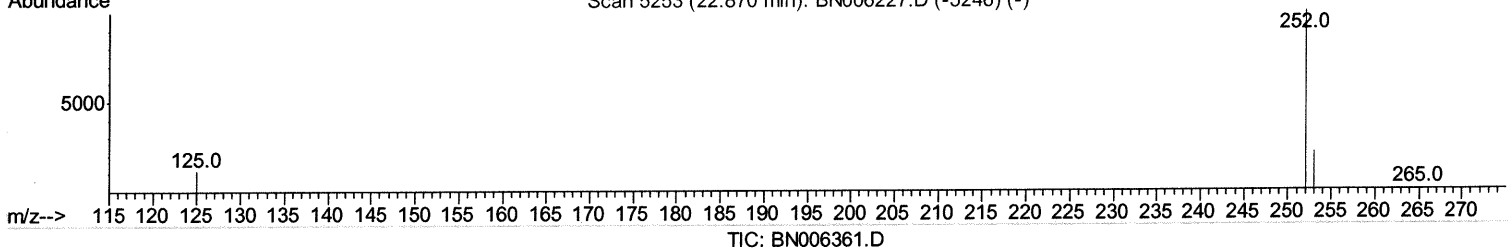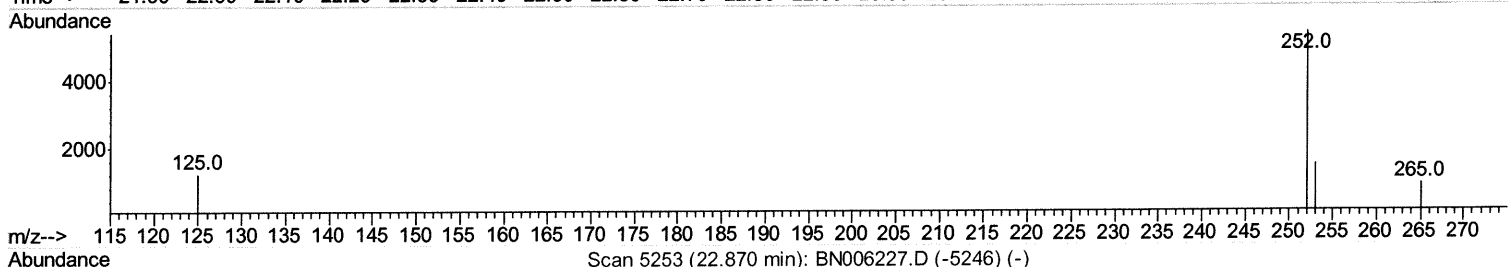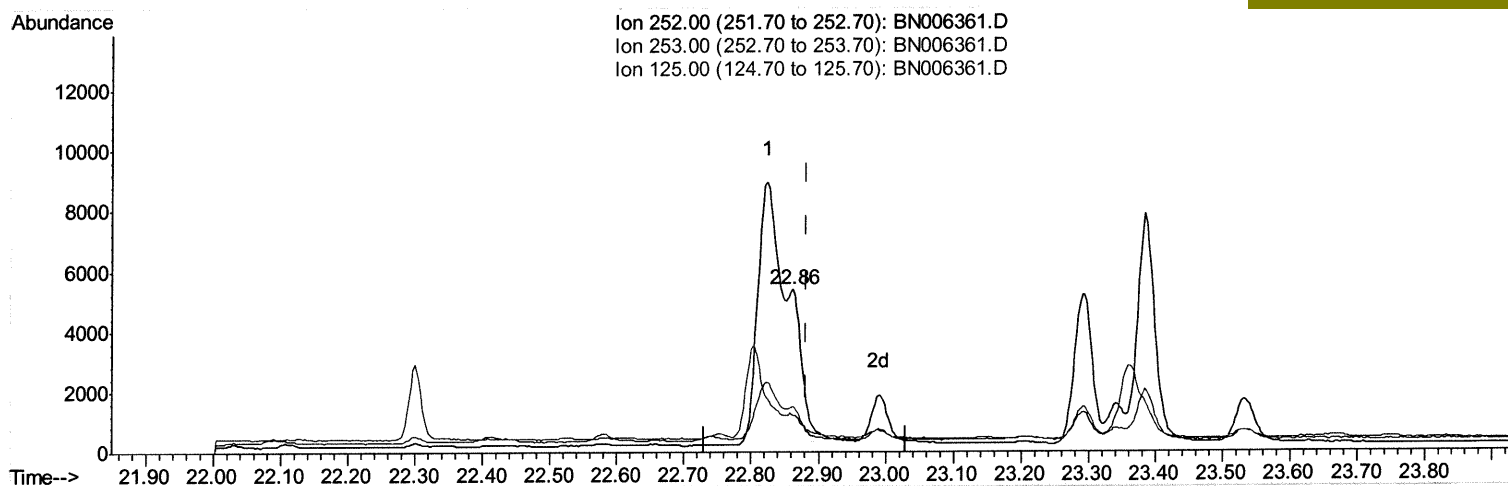

(22) Benzo(k)fluoranthene

22.861min (-0.020) 0.13ng/ul m 06/18/19

response 8108

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	27.61
125.00	17.90	22.90#
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061719\
 Data File : BN006361.D
 Acq On : 17 Jun 2019 22:44
 Operator : JU/SJ
 Sample : K3335-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4237

Quant Time: Jun 18 04:19:56 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:22:47 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	4302	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	17311	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.29	164	9246	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.04	188	16876m>	0.40	ng/ul	0.00
16) Chrysene-d12	21.26	240	10472m>	0.40	ng/ul	-0.01
20) Perylene-d12	23.49	264	15899	0.40	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.02	152	4703	0.18	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	8661m>	0.19	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
7) Acenaphthylene	14.01	152	2698	0.052	ng/ul#	92
9) Fluorene	15.35	166	1432	0.034	ng/ul#	96
12) Phenanthrene	17.09	178	23472m>	0.433	ng/ul	
13) Anthracene	17.18	178	4792m>	0.093	ng/ul	
15) Fluoranthene	19.11	202	40363m>	0.675	ng/ul	
17) Pyrene	19.48	202	38531	0.699	ng/ul	98
18) Benzo(a)anthracene	21.24	228	18092m>	0.391	ng/ul	
19) Chrysene	21.29	228	15050	0.346	ng/ul	98
21) Benzo(b)fluoranthene	22.82	252	20484m>	0.309	ng/ul	
22) Benzo(k)fluoranthene	22.86	252	8108m>	0.126	ng/ul	
23) Benzo(a)pyrene	23.38	252	13907	0.225	ng/ul	95
24) Indeno(1,2,3-cd)pyrene	25.72	276	8838	0.132	ng/ul#	86
25) Dibenzo(a,h)anthracene	25.73	278	2547	0.048	ng/ul#	76
26) Benzo(g,h,i)perylene	26.40	276	7017	0.125	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU 06/18/19