


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061720\
 Data File : BN010938.D
 Acq On : 17 Jun 2020 11:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN061020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 17 13:14:12 2020

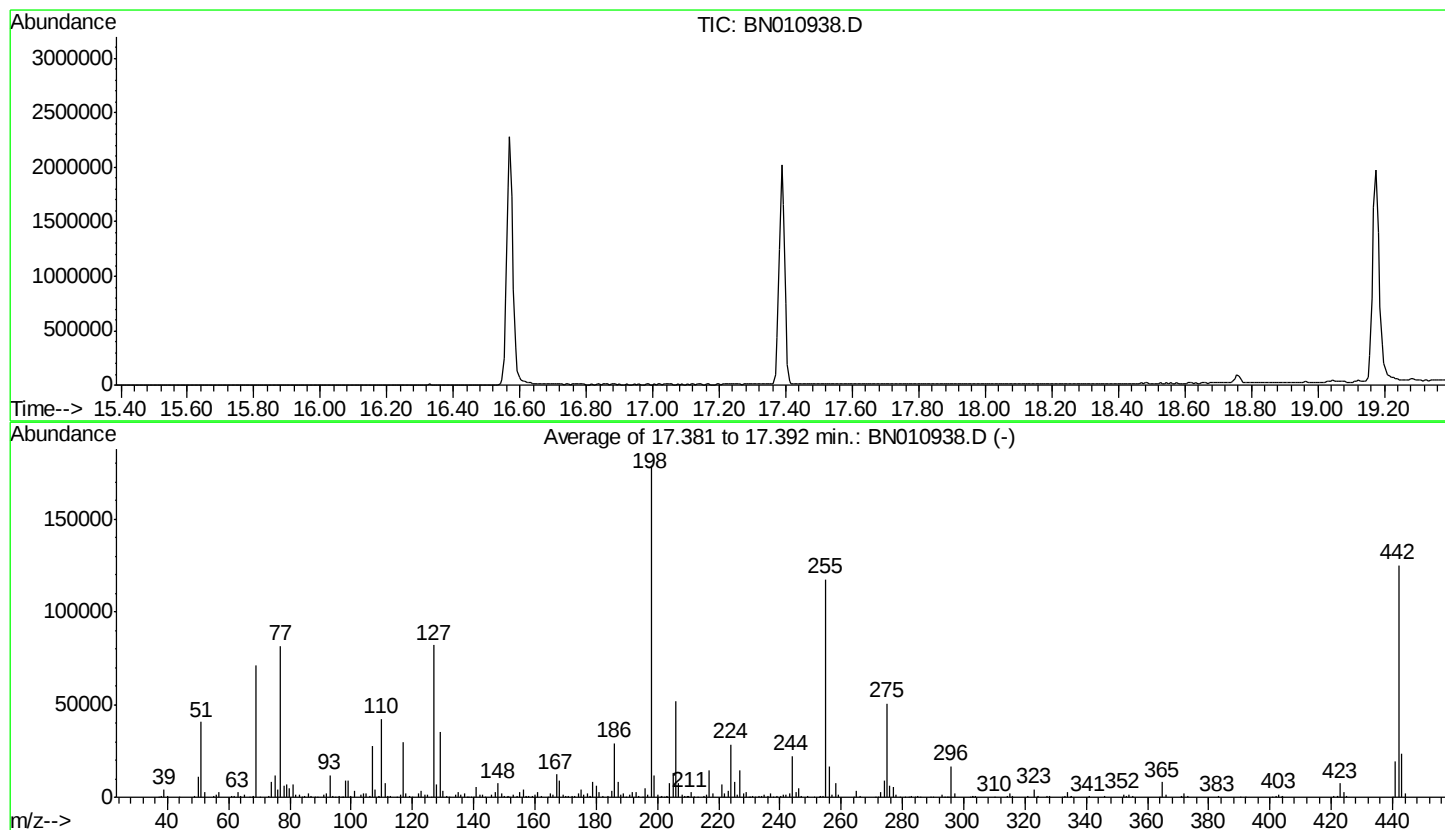

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.7	40600	PASS
68	69	0.00	2	0.7	479	PASS
69	198	0.00	100	39.7	70962	PASS
70	69	0.00	2	0.5	344	PASS
127	198	10	80	45.9	82024	PASS
197	198	0.00	2	0.6	1105	PASS
198	198	100	100	100.0	178730	PASS
199	198	5	9	6.5	11557	PASS
275	198	10	60	28.3	50496	PASS
365	198	1	100	4.6	8161	PASS
441	198	0.01	100	11.0	19619	PASS
442	198	50	100	70.1	125224	PASS
443	442	15	24	18.7	23406	PASS