

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006384.D
 Acq On : 18 Jun 2019 19:34
 Operator : JU/SJ
 Sample : K3335-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 19 01:28:58 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	4024	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	15217	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.29	164	7783	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.14	188	900315	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.27
20) Perylene-d12	23.35	264	853135	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	5521	0.24	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
7) Acenaphthylene	14.01	152	1771	0.041	ng/ul#	89
9) Fluorene	15.35	166	718	0.020	ng/ul#	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
Data File : BN006384.D
Acq On : 18 Jun 2019 19:34
Operator : JU/SJ
Sample : K3335-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 19 01:28:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

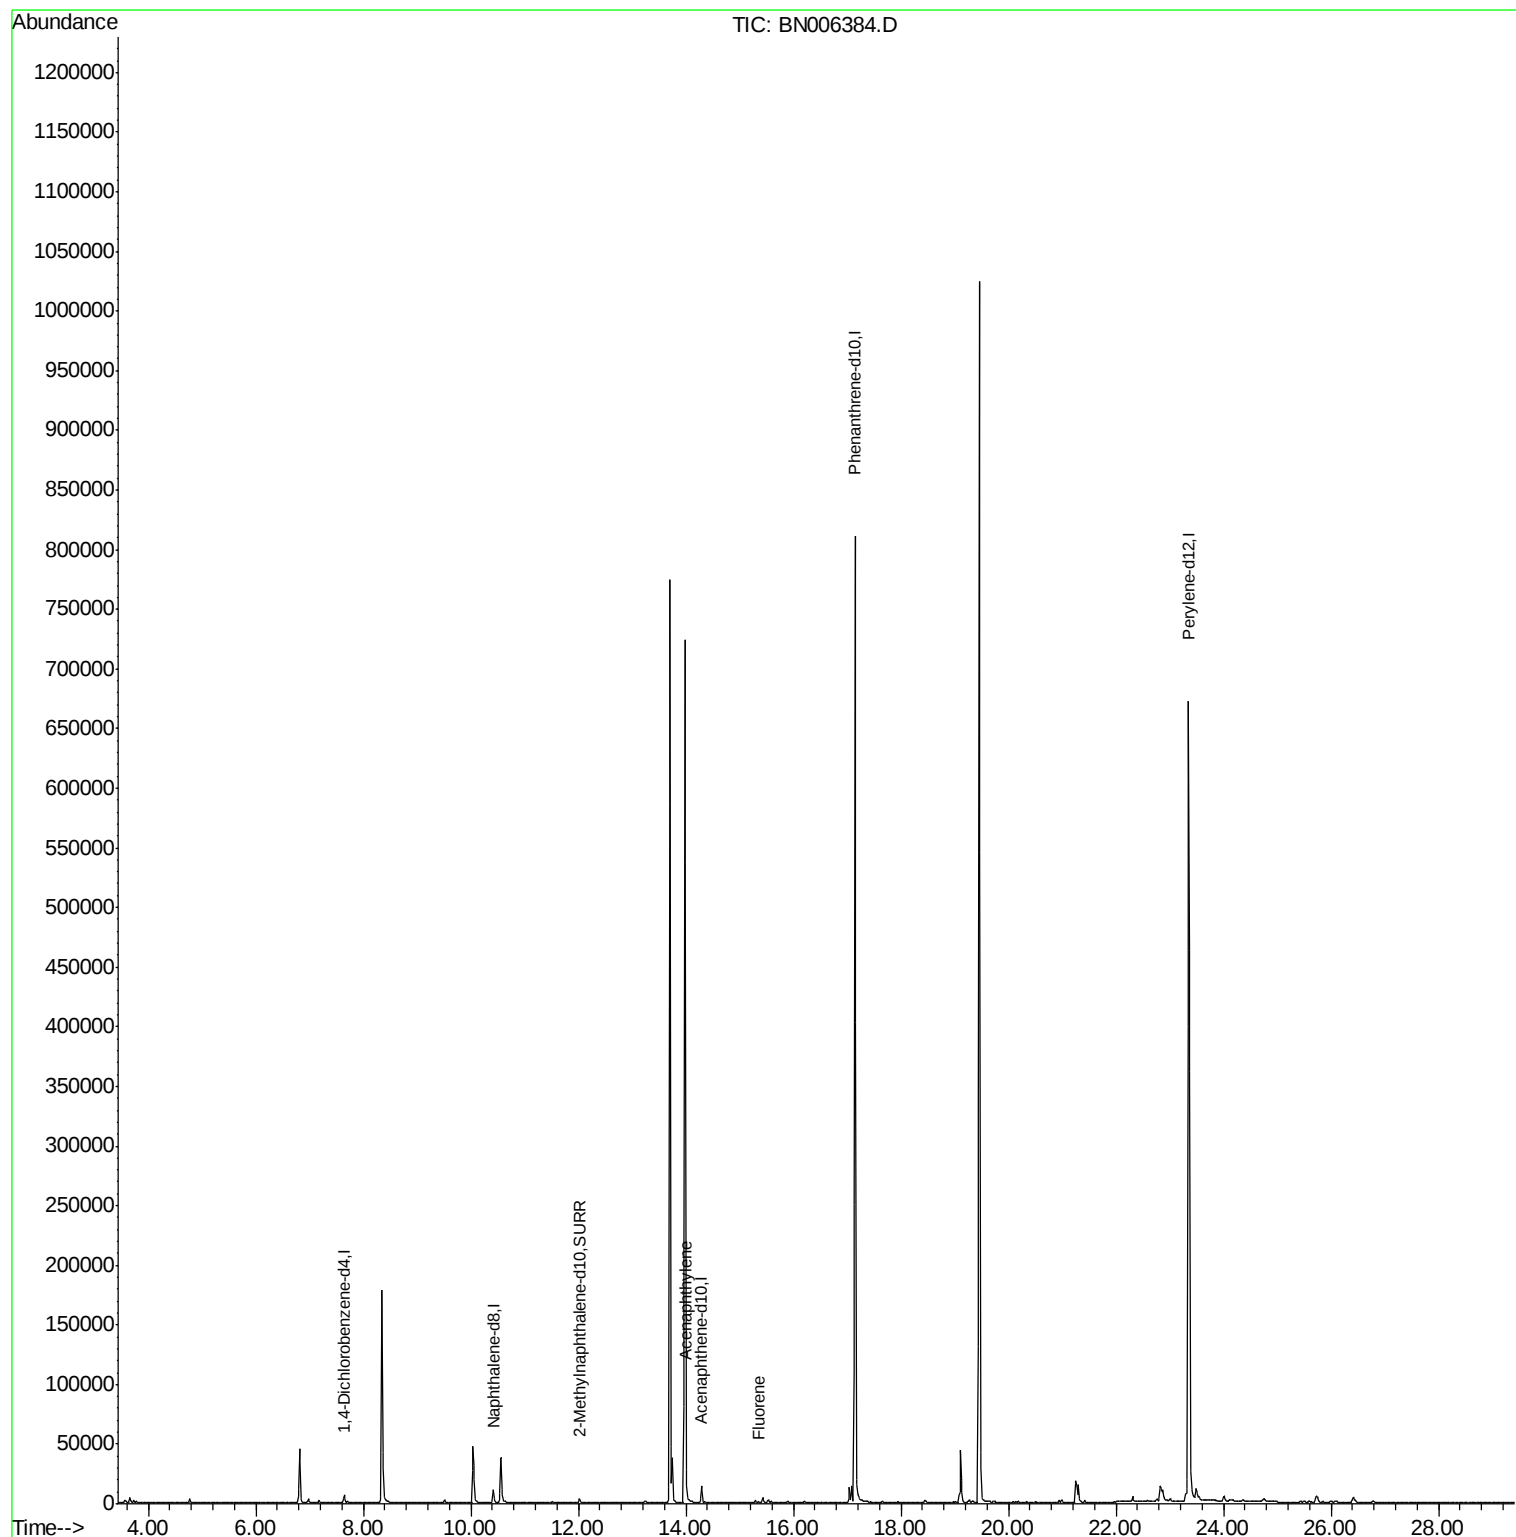

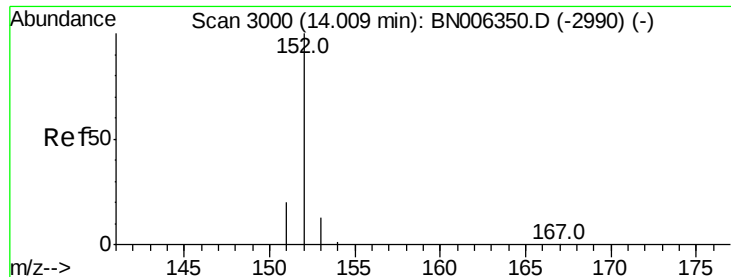

#7

Acenaphthylene

Concen: 0.041 ng/ul

RT: 14.01 min Scan# 3000

Delta R.T. 0.00 min

Lab File: BN006384.D

Acq: 18 Jun 2019 19:34

Instrument :

BNA_N

ClientSampleId :


Tot Ion:152 Resp: 1771

Ion Ratio Lower Upper

152 100

151 23.9 15.8 23.8#




153 18.8 10.8 16.2#

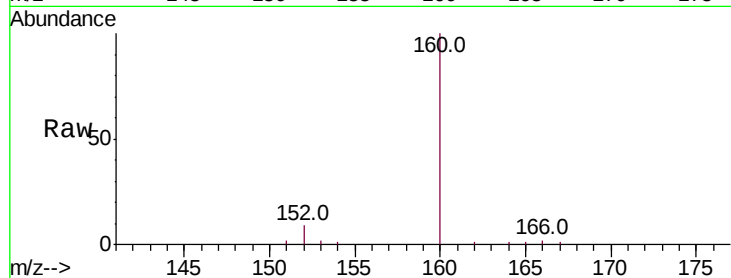

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

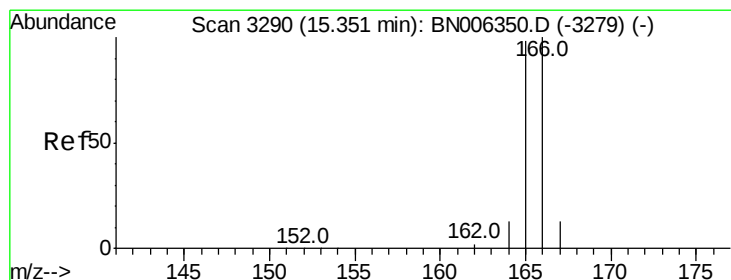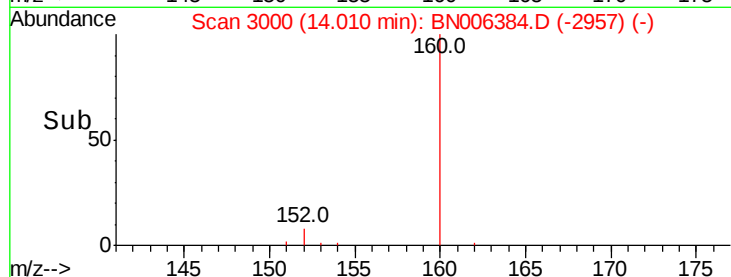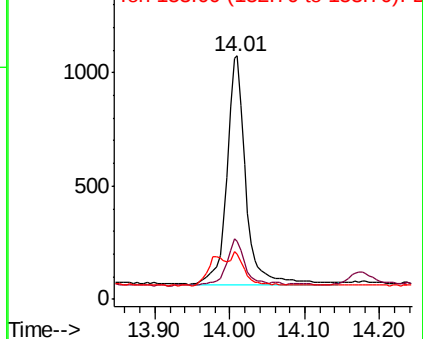

#9

Fluorene

Concen: 0.020 ng/ul

RT: 15.35 min Scan# 3289

Delta R.T. -0.00 min

Lab File: BN006384.D

Acq: 18 Jun 2019 19:34


Tgt Ion:166 Resp: 718

Ion Ratio Lower Upper

166 100

165 96.9 76.4 114.6

167 26.8 11.0 16.6#

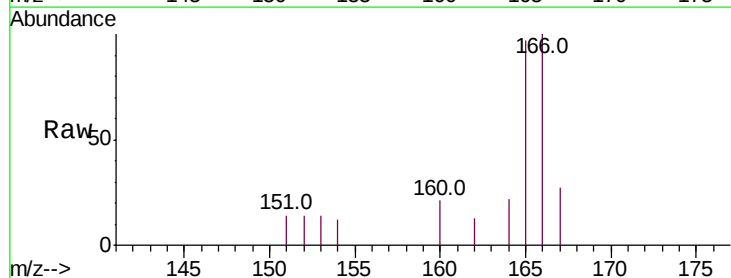

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

