

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006389.D
 Acq On : 18 Jun 2019 22:26
 Operator : JU/SJ
 Sample : K3335-24
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 19 01:29:17 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	4114	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	15179	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.29	164	8252	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.14	188	1223778	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.27
20) Perylene-d12	23.34	264	1077008	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	7326	0.32	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
8) Acenaphthene	14.37	153	2340	0.074	ng/ul#	Ovalue 26


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
Data File : BN006389.D
Acq On : 18 Jun 2019 22:26
Operator : JU/SJ
Sample : K3335-24
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 19 01:29:17 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

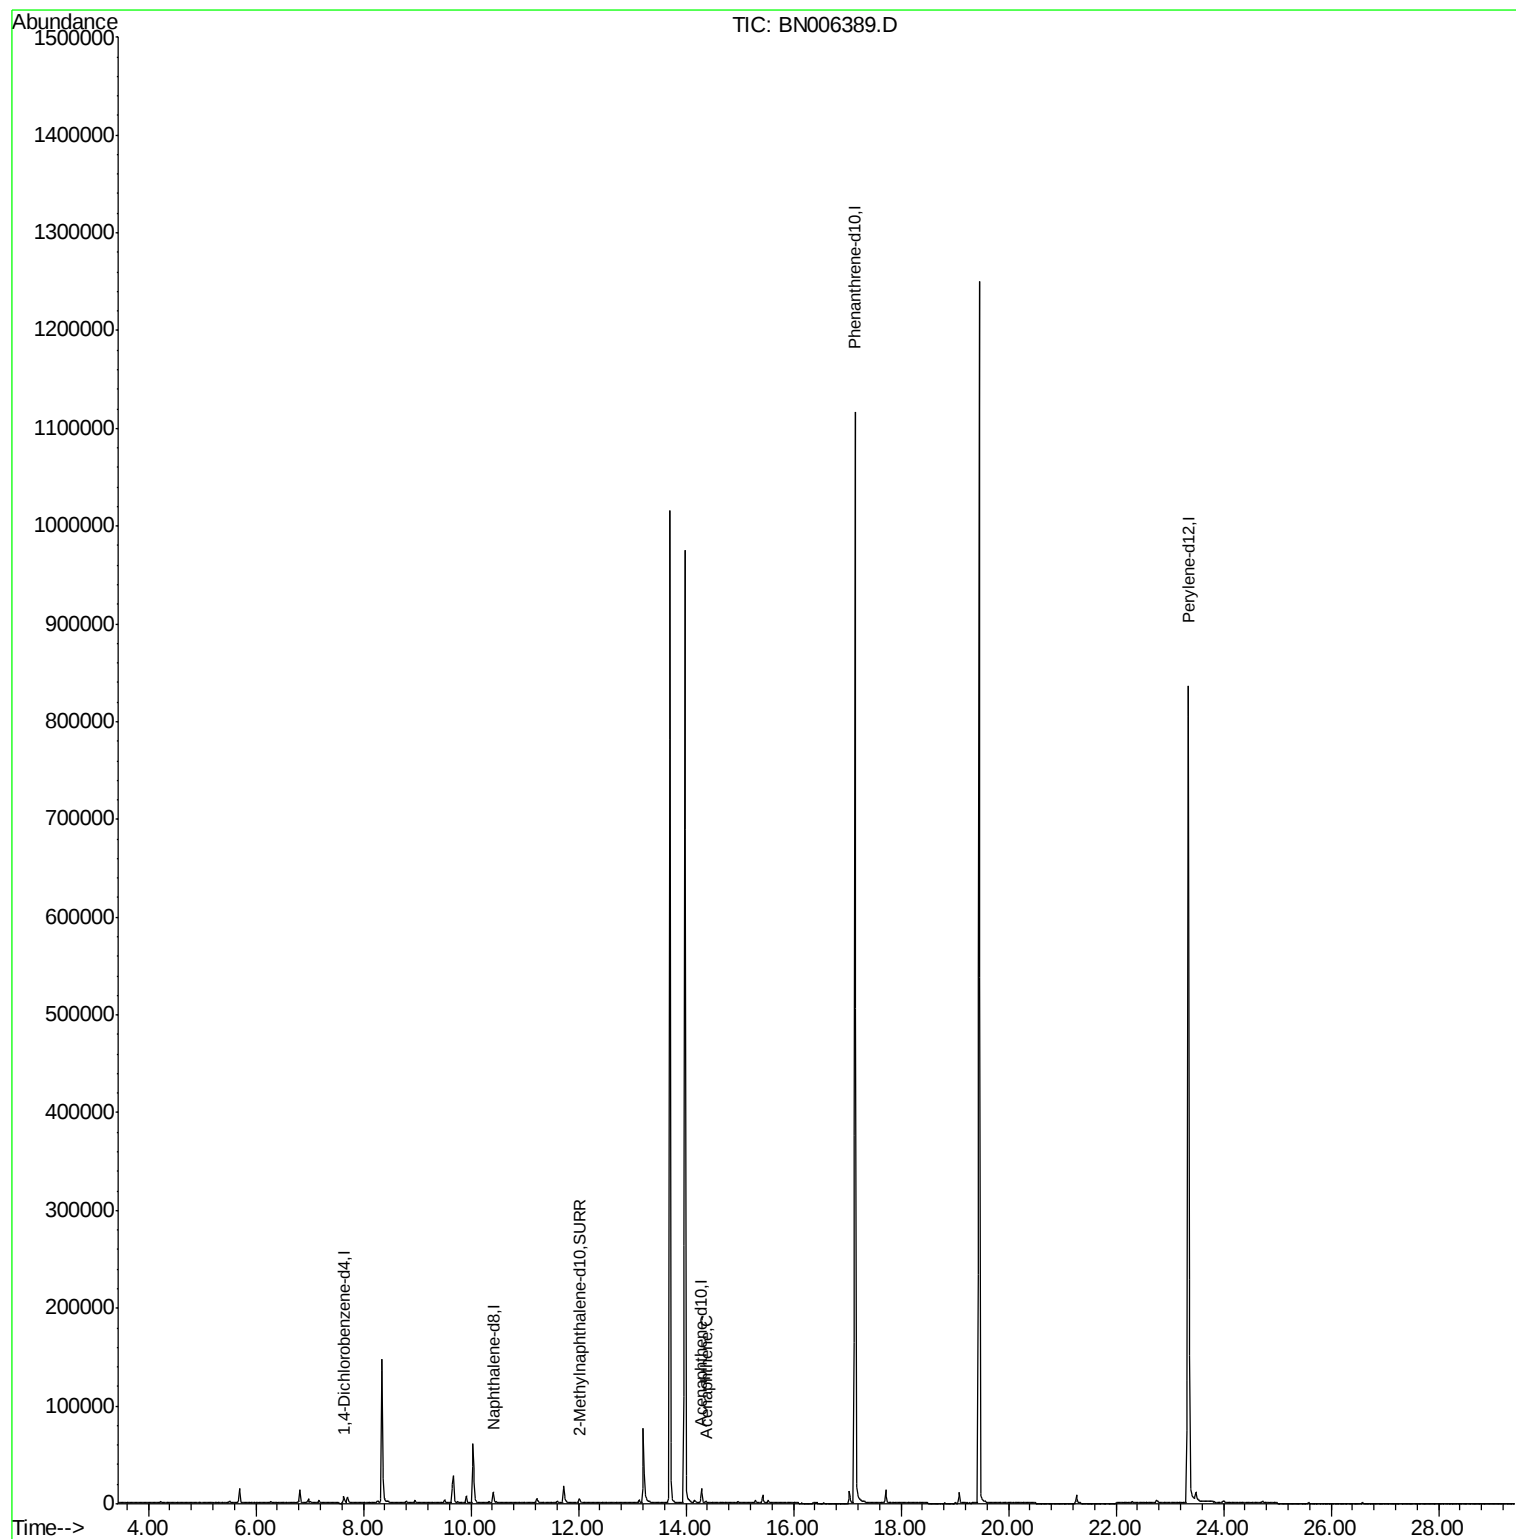

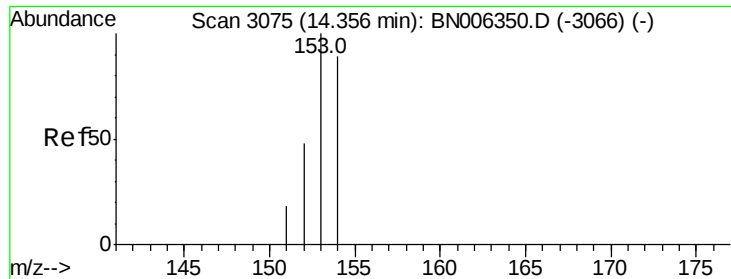

#8

Acenaphthene

Concen: 0.074 ng/ul

RT: 14.37 min Scan# 3078

Delta R.T. 0.01 min

Lab File: BN006389.D

Acq: 18 Jun 2019 22:26

Instrument :

BNA_N

ClientSampleId :


Tot Ion:153 Resp: 2340

Ion Ratio Lower Upper

153 100

152 6.6 39.1 58.7#

154 12.9 71.1 106.7#

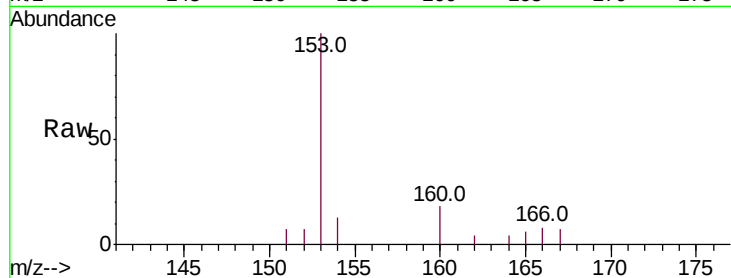

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

