

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006390.D
 Acq On : 18 Jun 2019 23:01
 Operator : JU/SJ
 Sample : K3335-25
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 19 01:29:20 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	3742	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	14590	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.29	164	7620	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.14	188	1053562	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.27
20) Perylene-d12	23.35	264	952187	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	5206	0.23	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
8) Acenaphthene	14.37	153	3369	0.115	ng/ul#	Ovalue 23




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
Data File : BN006390.D
Acq On : 18 Jun 2019 23:01
Operator : JU/SJ
Sample : K3335-25
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 19 01:29:20 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

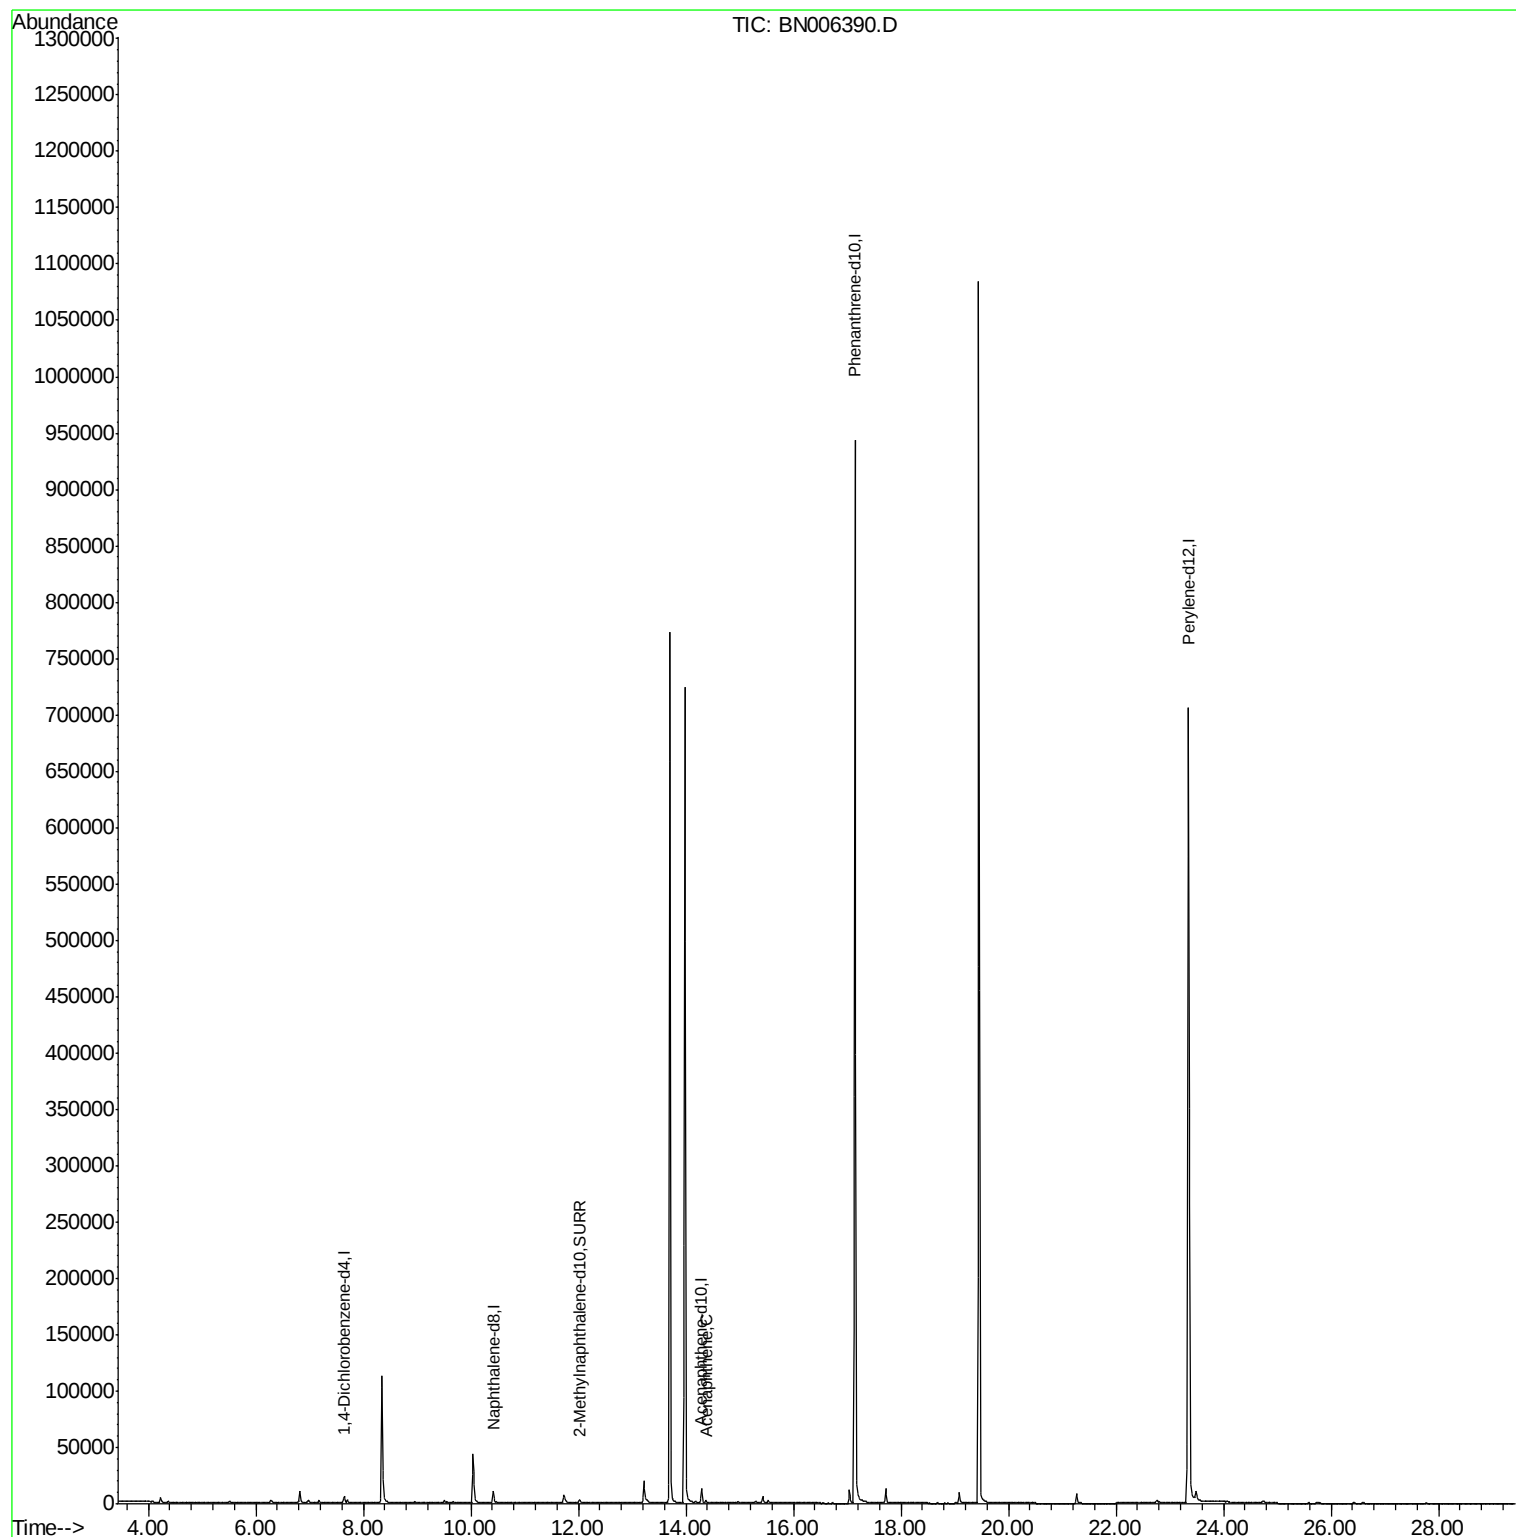

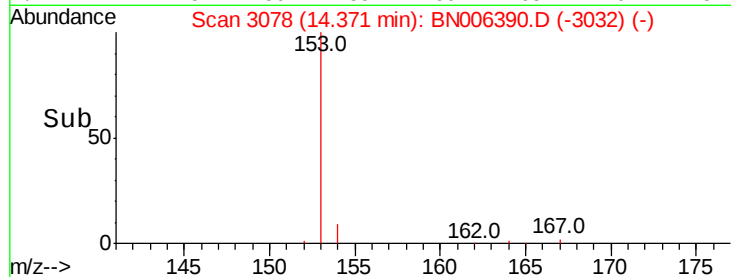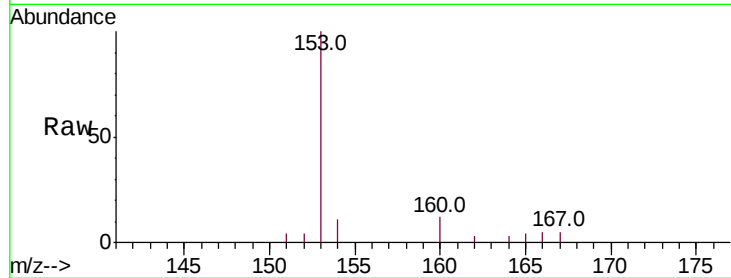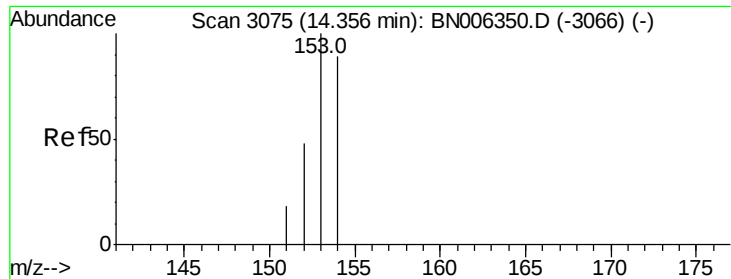

#8

Acenaphthene

Concen: 0.115 ng/ul

RT: 14.37 min Scan# 3078

Delta R.T. 0.01 min

Lab File: BN006390.D

Acq: 18 Jun 2019 23:01

Instrument :

BNA_N

ClientSampleId :

Tot Ion:153 Resp: 3369

Ion Ratio Lower Upper

153 100

152 4.0 39.1 58.7#

154 11.0 71.1 106.7#

