

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061819\

Data File : BN006375.D

Acq On : 18 Jun 2019 13:30

Operator : JU/SJ

Sample : K3335-06

Misc :

ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jun 18 16:41:23 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Jun 18 15:57:40 2019

Response via : Initial Calibration

Instrument :

BNA_N


Client Sampled :

A4220

Manual Integrations
APPROVED

mohammad

6/21/2019 8:38:55 AM

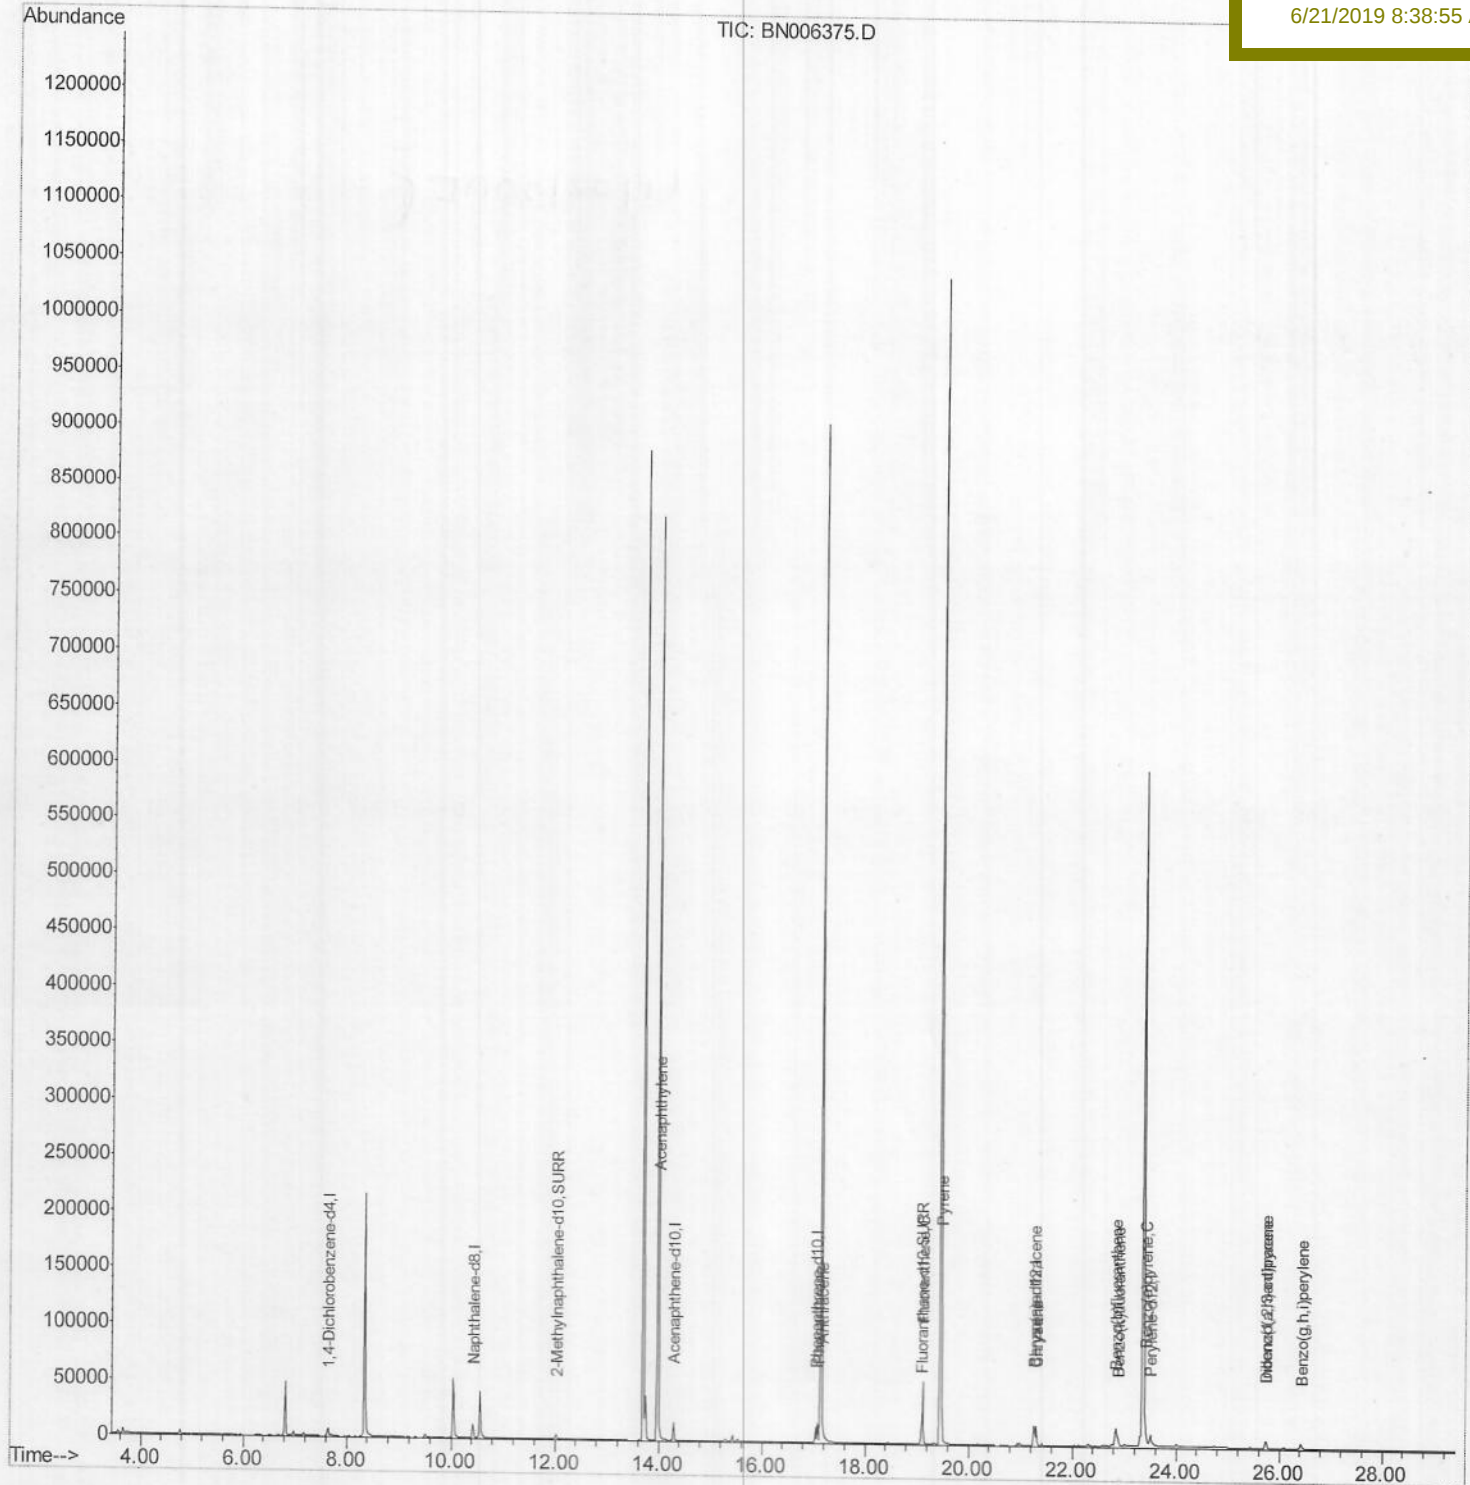

SOM-EPA-SIM-BN053019.M Tue Jun 18 16:34:27 2019

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061819\
 Data File : BN006375.D
 Acq On : 18 Jun 2019 13:30
 Operator : JU/SJ
 Sample : K3335-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jun 18 16:31:52 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 18 15:57:40 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 A4220

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:38:55 AM

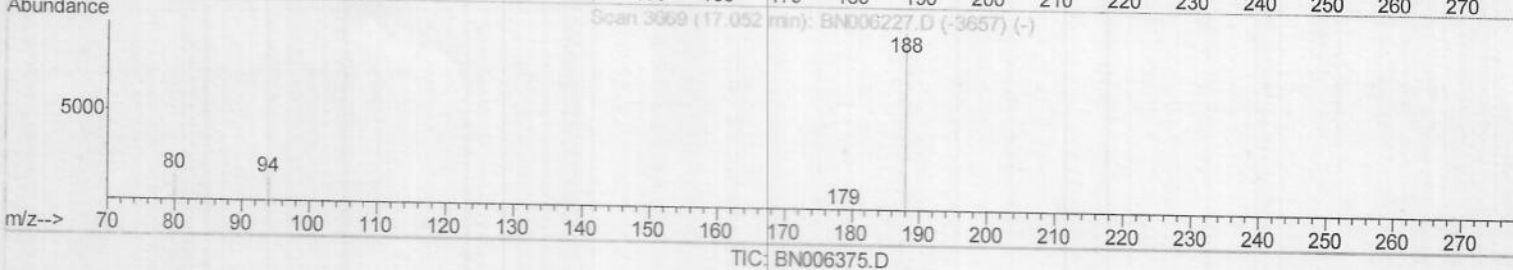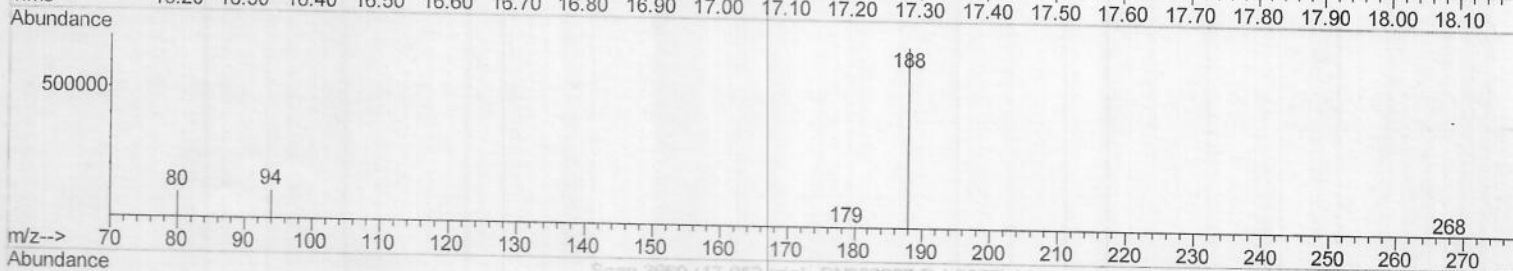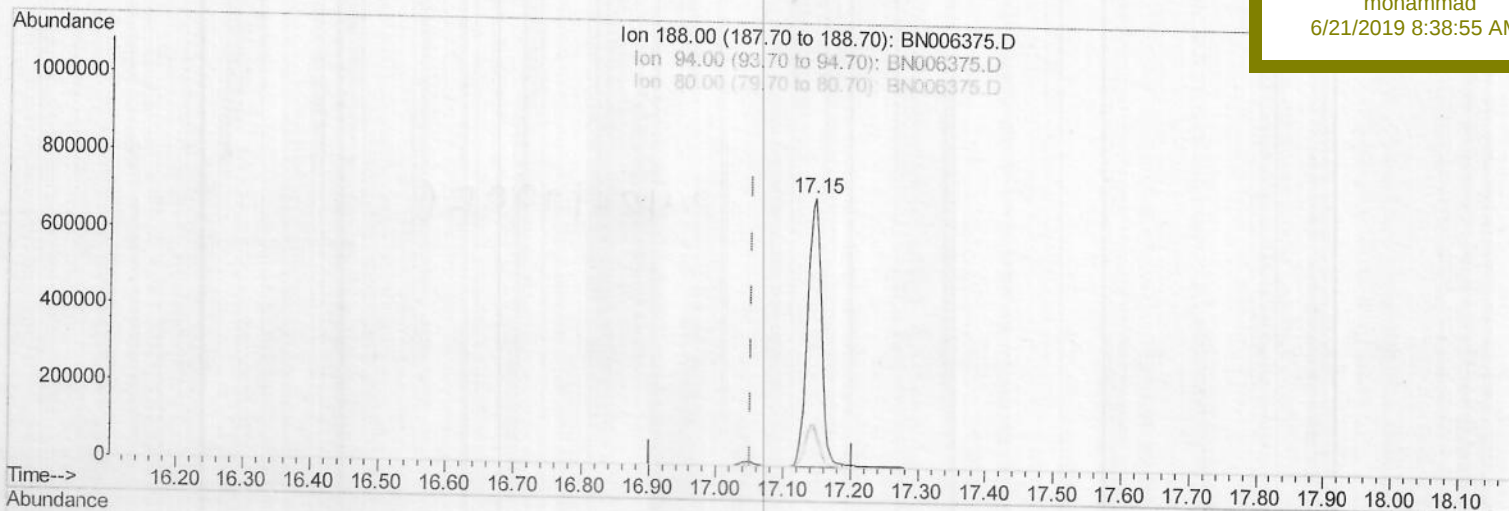

(10) Phenanthrene-d10 (I)
 17.145min (+0.093) 0.40ng/ul
 response 1013321

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	15.31
80.00	13.60	14.05
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061819\
 Data File : BN006375.D
 Acq On : 18 Jun 2019 13:30
 Operator : JU/SJ
 Sample : K3335-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jun 18 16:31:52 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 18 15:57:40 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 A4220

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:38:55 AM

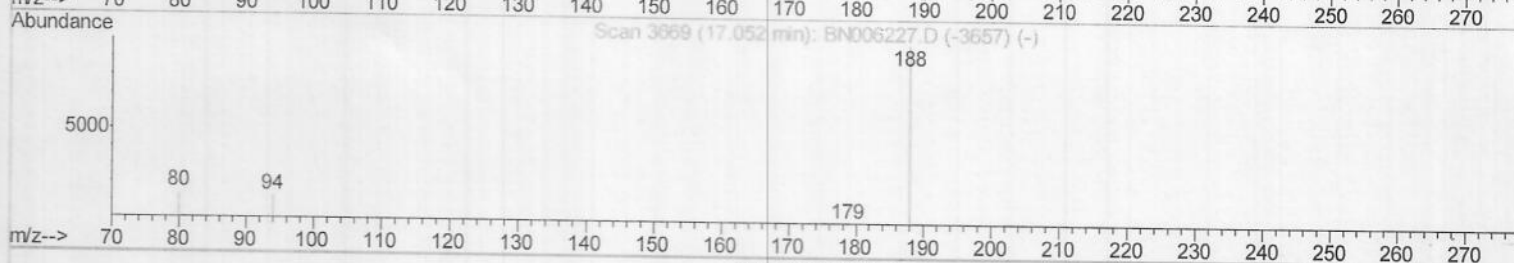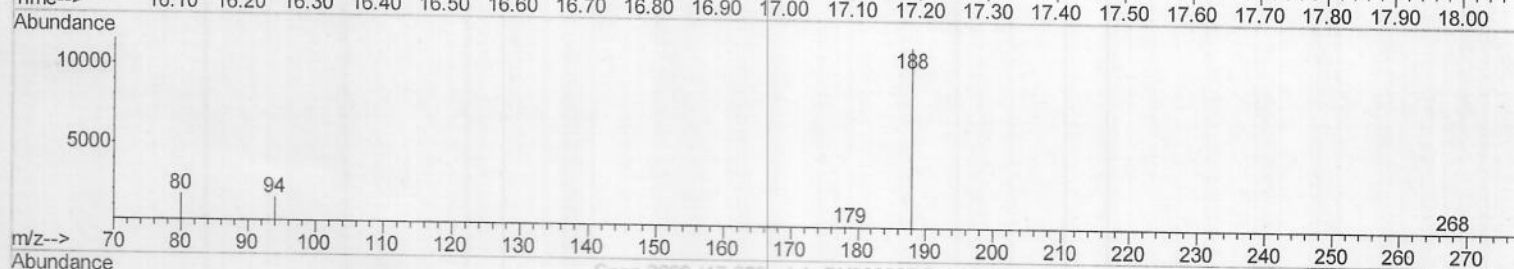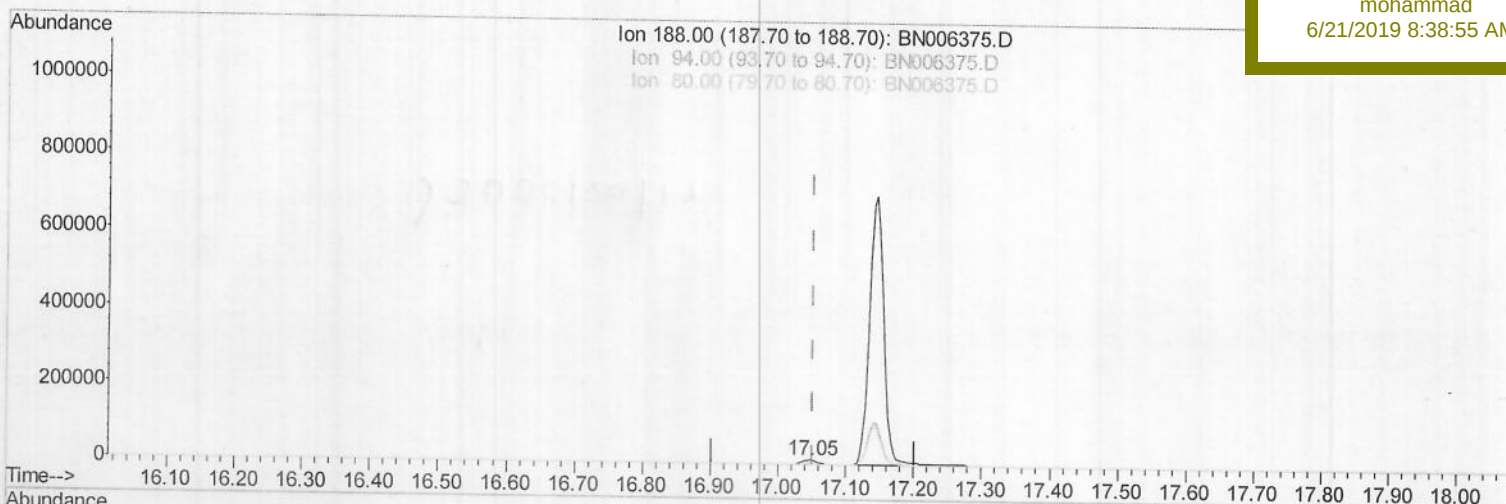

TIC: BN006375.D

(10) Phenanthrene-d10 (I)

17.048min (-0.004) 0.40ng/ul m

> JU 06/25/19

response 16934

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	13.13
80.00	13.60	14.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061819\

Data File : BN006375.D

Acq On : 18 Jun 2019 13:30

Operator : JU/SJ

Sample : K3335-06

Misc :

ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jun 18 16:32:40 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Jun 18 15:57:40 2019




Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A4220

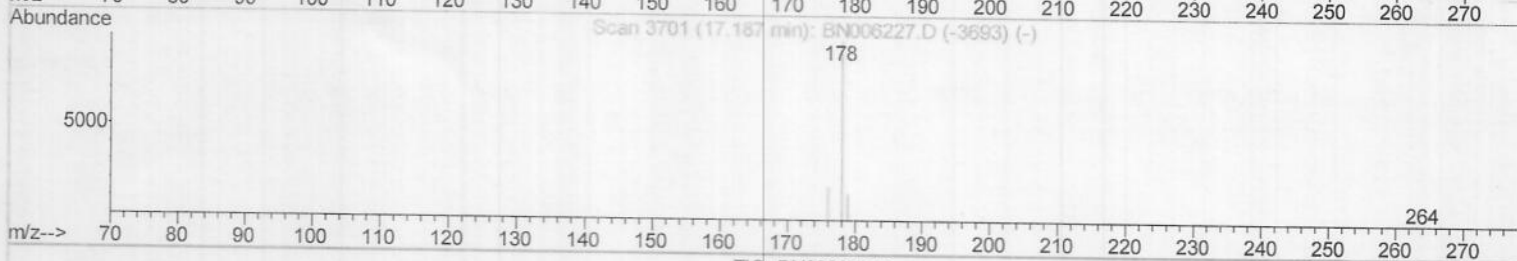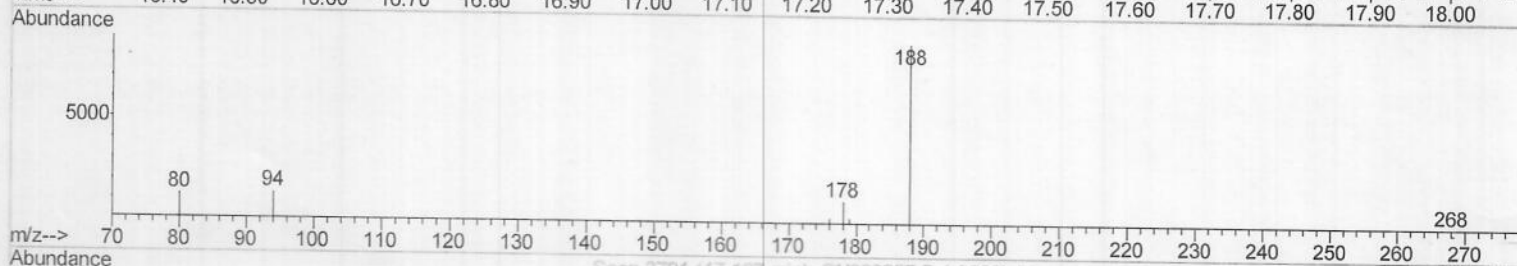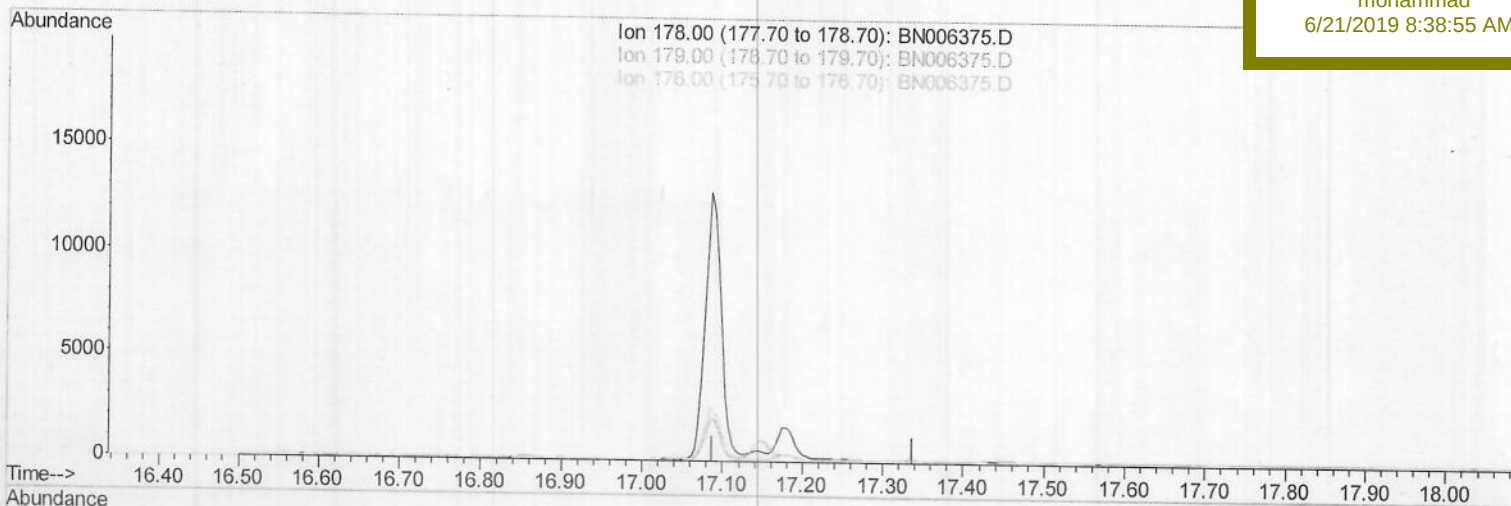Manual Integrations
APPROVEDmohammad
6/21/2019 8:38:55 AM

TIC: BN006375.D

(13) Anthracene

17.187min (-17.187) 0.00ng/ul

response 0

Ion	Exp%	Act%
178.00	100	0.00
179.00	15.30	0.00#
176.00	18.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061819\
 Data File : BN006375.D
 Acq On : 18 Jun 2019 13:30
 Operator : JU/SJ
 Sample : K3335-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jun 18 16:32:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 18 15:57:40 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 A4220

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:38:55 AM

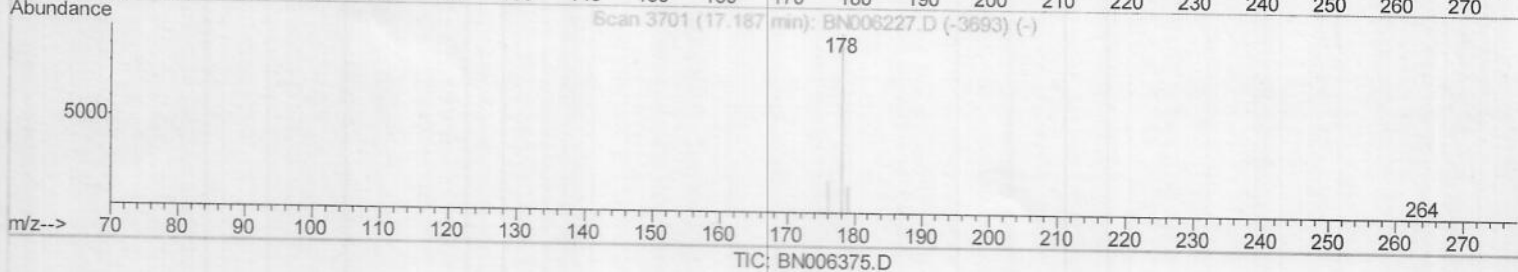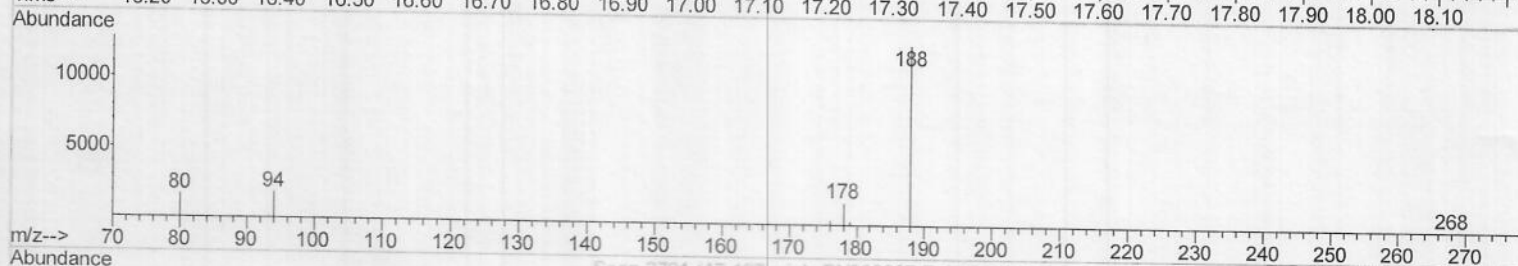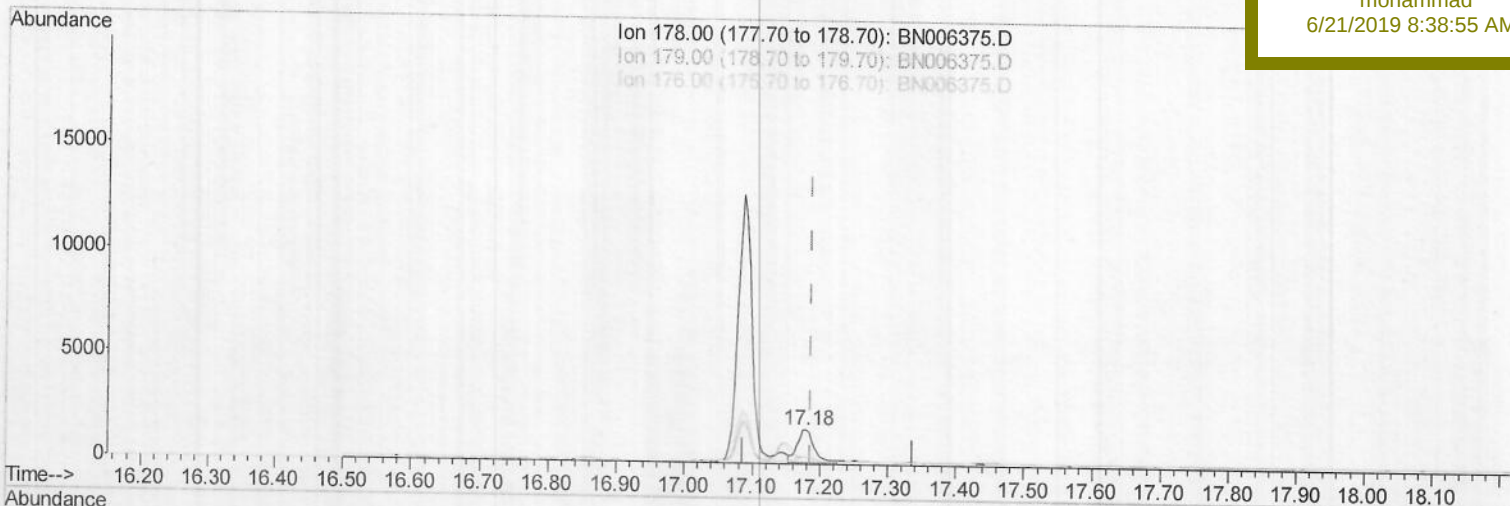

(13) Anthracene

17.179min (-0.008) 0.05ng/ul m

> JU 06/25/19

response 2724

Ion	Exp%	Act%
178.00	100	100
179.00	15.30	21.19#
176.00	18.90	22.88#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061819\
Data File : BN006375.D
Acq On : 18 Jun 2019 13:30
Operator : JU/SJ
Sample : K3335-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jun 18 16:32:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 15:57:40 2019
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
A4220

Manual Integrations
APPROVED

mohammad
6/21/2019 8:38:55 AM

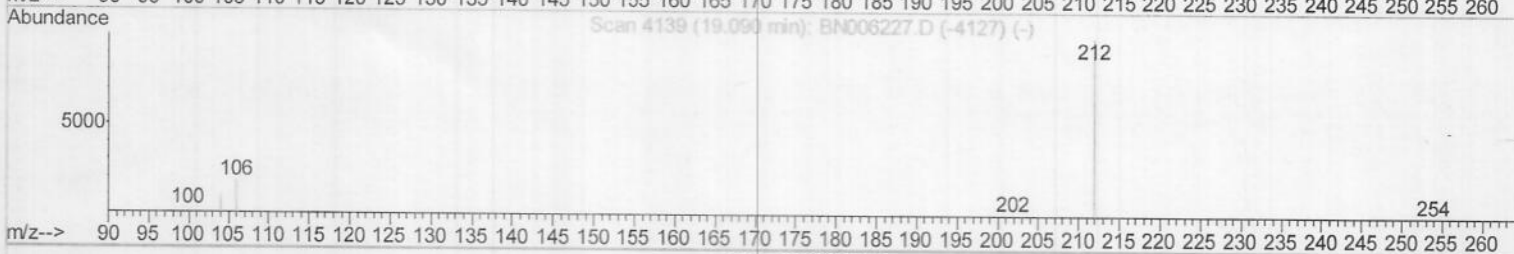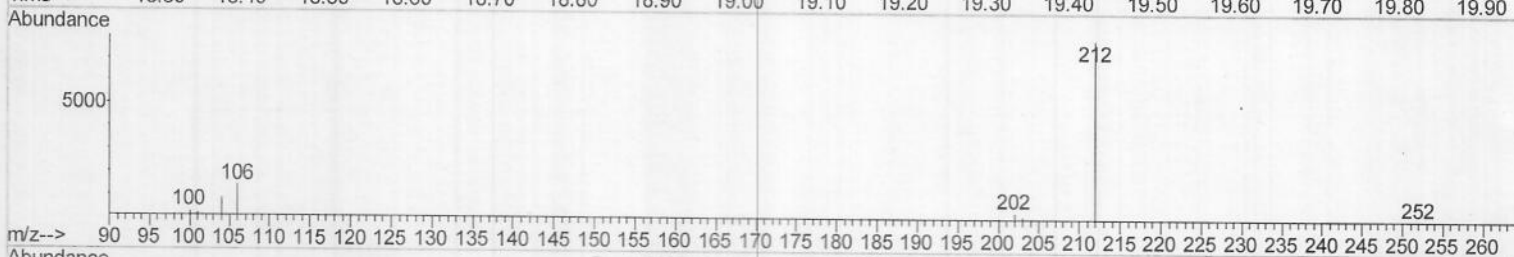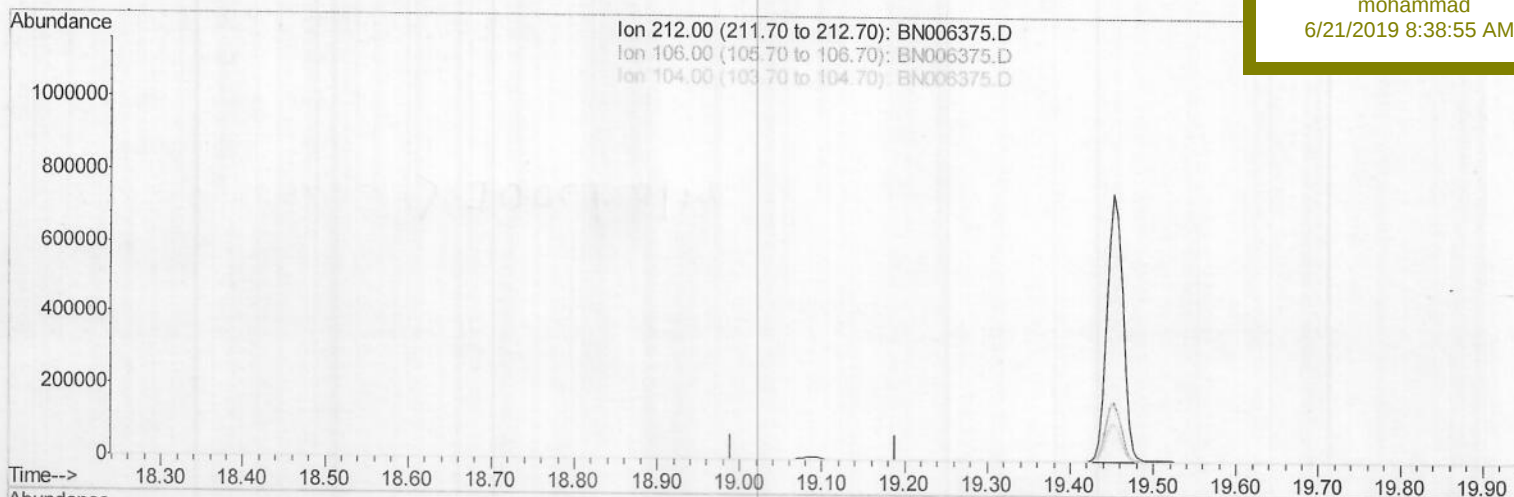

(14) Fluoranthene-d10 (SURR)

19.090min (-19.090) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061819\

Data File : BN006375.D

Acq On : 18 Jun 2019 13:30

Operator : JU/SJ

Sample : K3335-06

Misc :

ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jun 18 16:32:40 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Jun 18 15:57:40 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A4220

Manual Integrations

APPROVED

mohammad

6/21/2019 8:38:55 AM

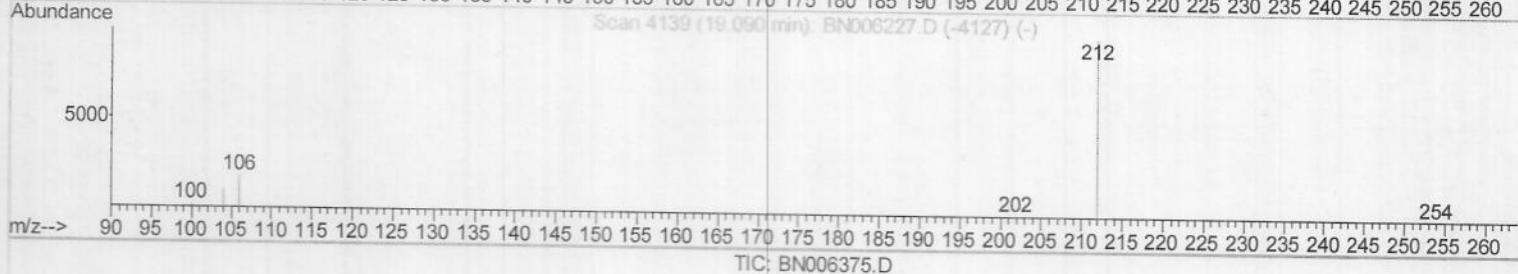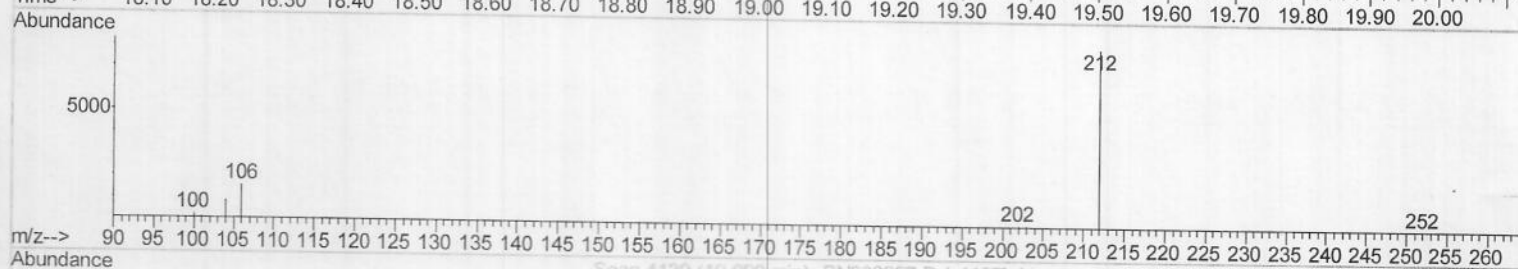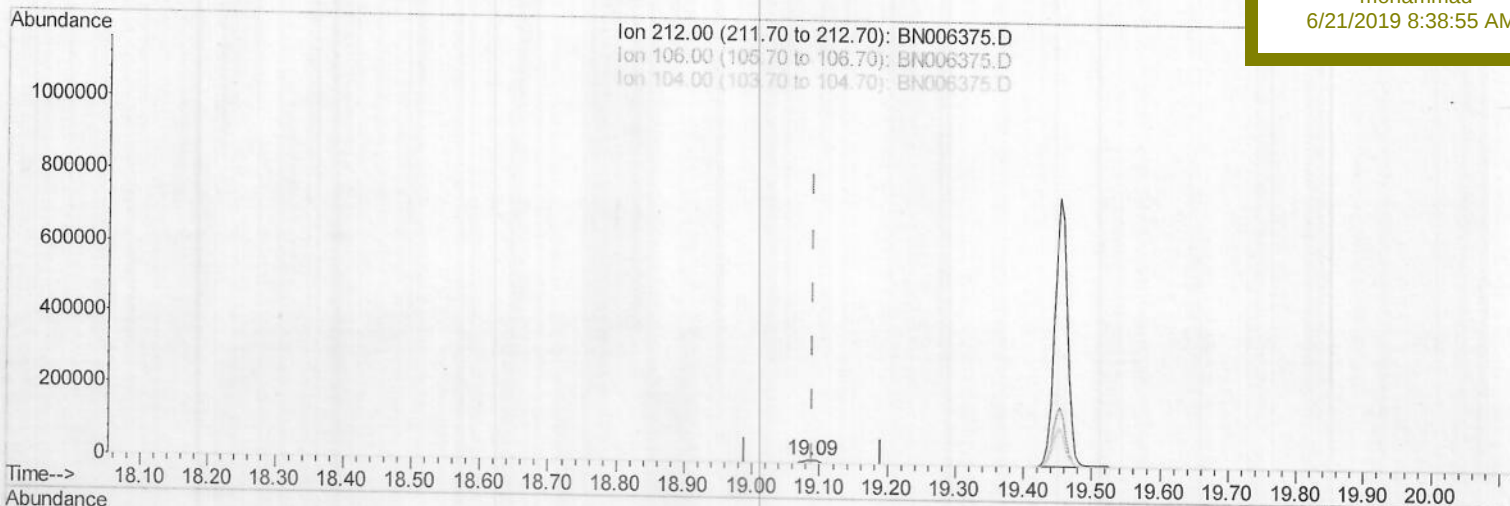

(14) Fluoranthene-d10 (SURR)

19.086min (-0.005) 0.26ng/ul m

response 11794

Ion Exp% Act%

212.00 100 100

106.00 18.10 0.00#

104.00 9.90 0.00#

0.00 0.00 0.00

JU 06/25/19

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061819\
 Data File : BN006375.D
 Acq On : 18 Jun 2019 13:30
 Operator : JU/SJ
 Sample : K3335-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jun 18 16:32:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 18 15:57:40 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 A4220

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:38:55 AM

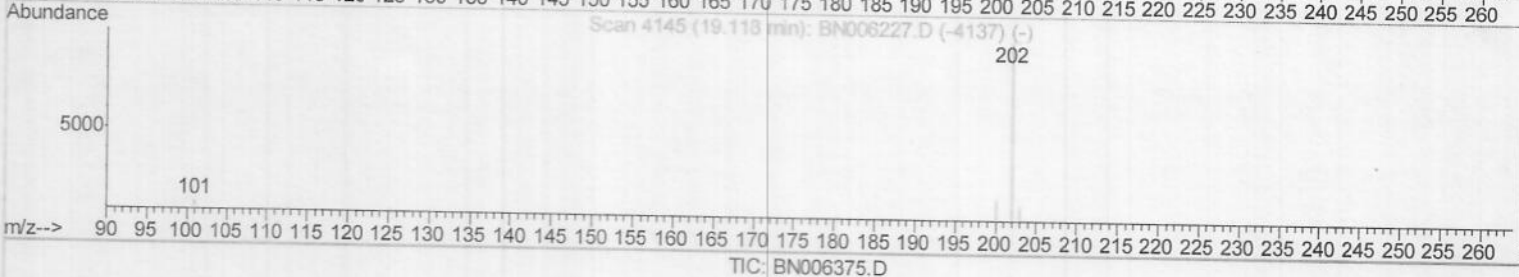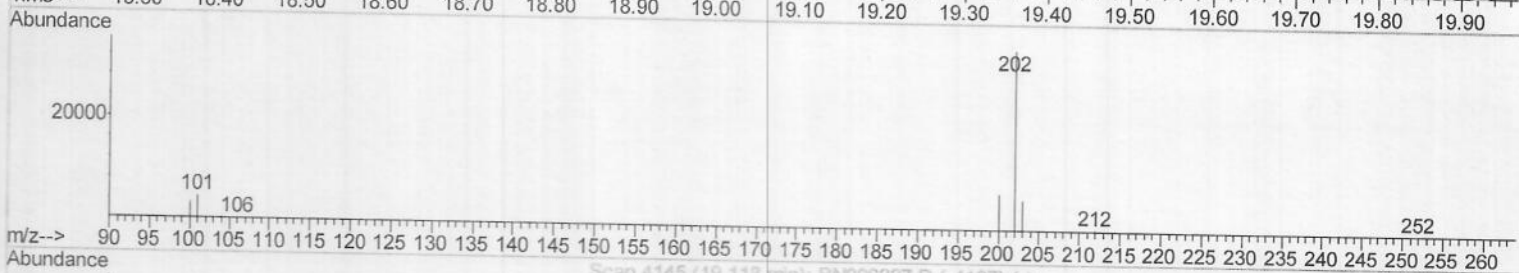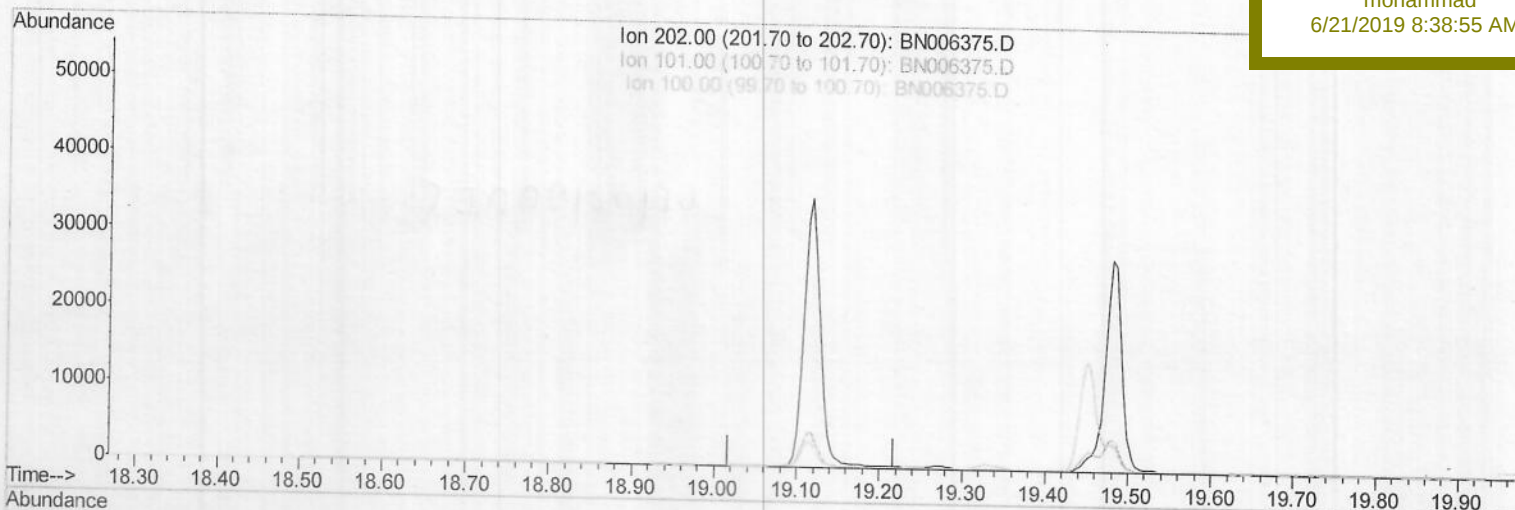

TIC: BN006375.D

(15) Fluoranthene (C)

19.118min (-19.118) 0.00ng/ul

response 0

Ion	Exp%	Act%
202.00	100	0.00
101.00	12.10	0.00
100.00	8.70	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061819\

Data File : BN006375.D

Acq On : 18 Jun 2019 13:30

Operator : JU/SJ

Sample : K3335-06

Misc :

ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jun 18 16:32:40 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Jun 18 15:57:40 2019

Response via : Initial Calibration

Instrument :




BNA_N

ClientSampleId :

A4220

Manual Integrations
APPROVED

mohammad
6/21/2019 8:38:55 AM

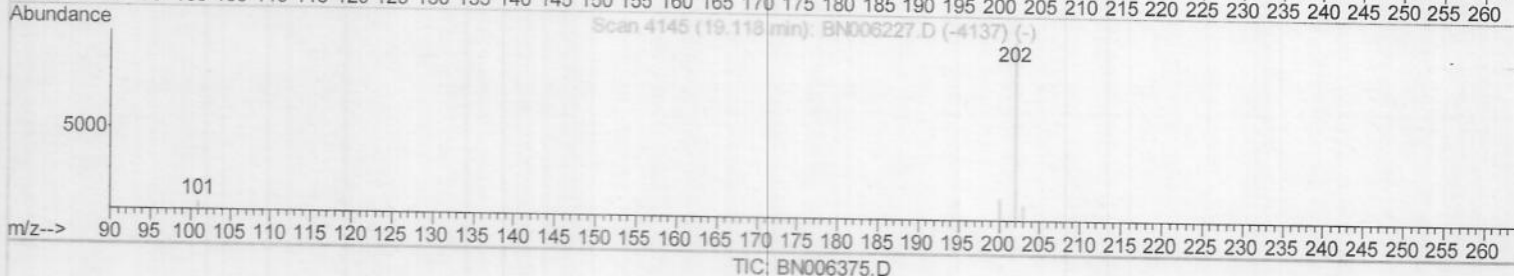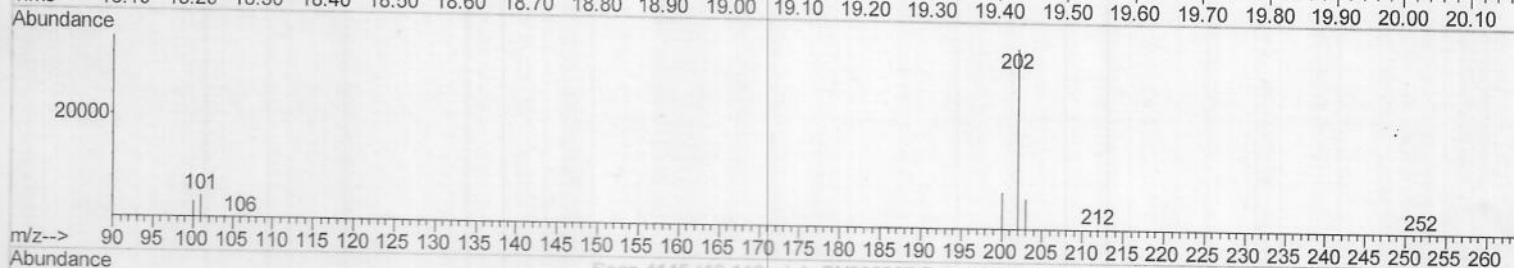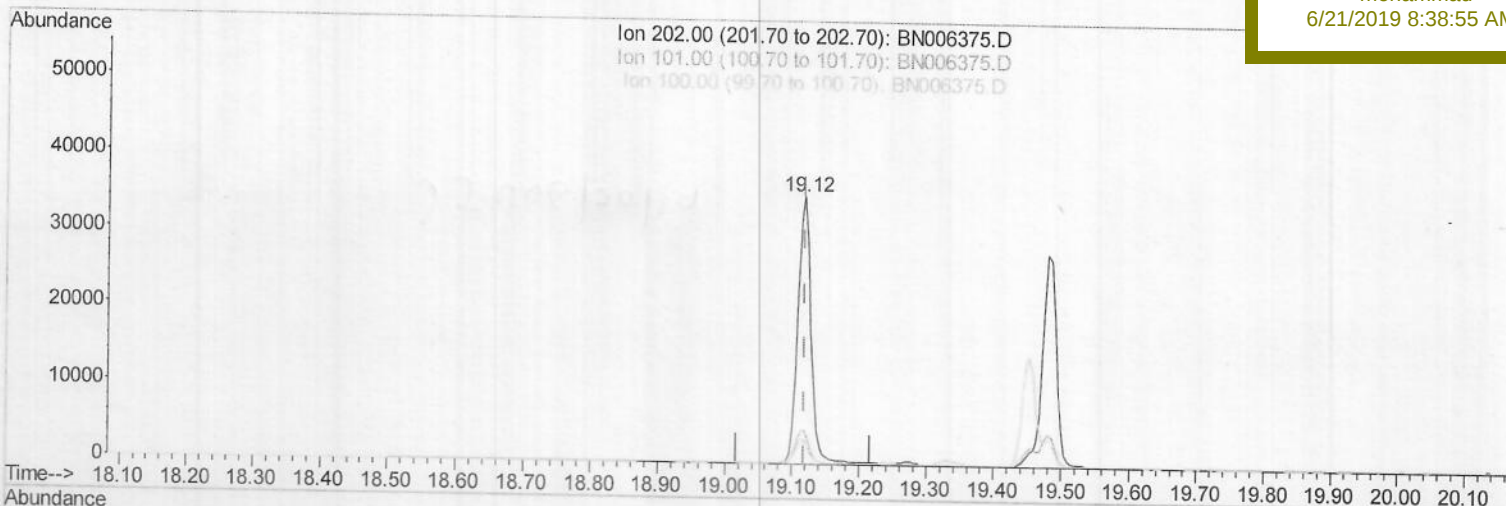

TIC: BN006375.D

(15) Fluoranthene (C)

19.118min (+0.000) 0.81ng/ul m

response 48409

Ion	Exp%	Act%
202.00	100	100
101.00	12.10	12.76
100.00	8.70	9.25
0.00	0.00	0.00

> JU 06/25/19

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061819\

Data File : BN006375.D

Acq On : 18 Jun 2019 13:30

Operator : JU/SJ

Sample : K3335-06

Misc :

ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jun 18 16:32:40 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Jun 18 15:57:40 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A4220

Manual Integrations

APPROVED

mohammad

6/21/2019 8:38:55 AM

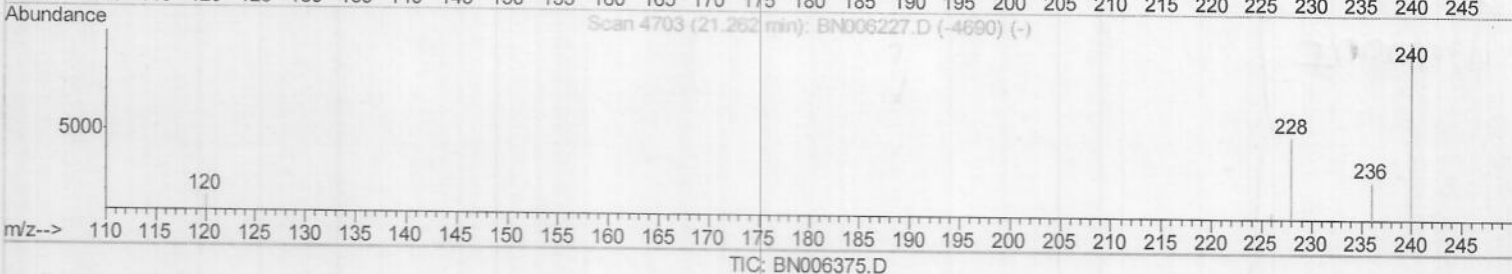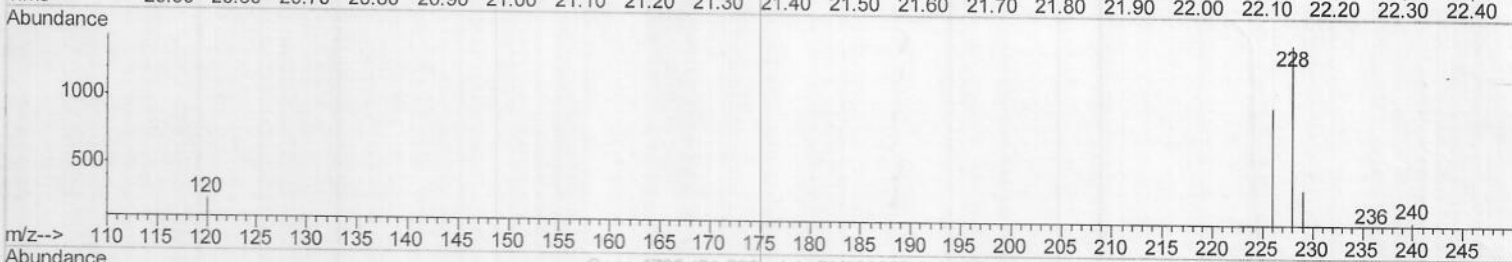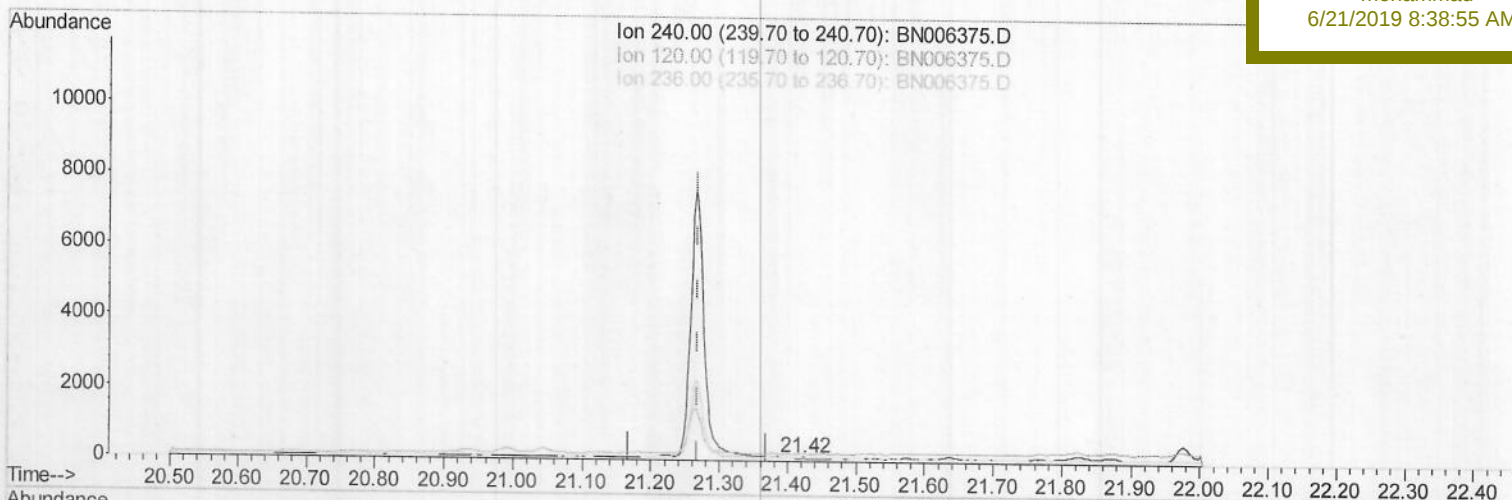

(16) Chrysene-d12 (I)

21.423min (+0.155) 0.40ng/ul

response 53

Ion	Exp%	Act%
240.00	100	100
120.00	20.10	186.18#
236.00	30.10	75.61#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061819\

Data File : BN006375.D

Acq On : 18 Jun 2019 13:30

Operator : JU/SJ

Sample : K3335-06

Misc :

ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jun 18 16:32:40 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Jun 18 15:57:40 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A4220

Manual Integrations

APPROVED

mohammad

6/21/2019 8:38:55 AM

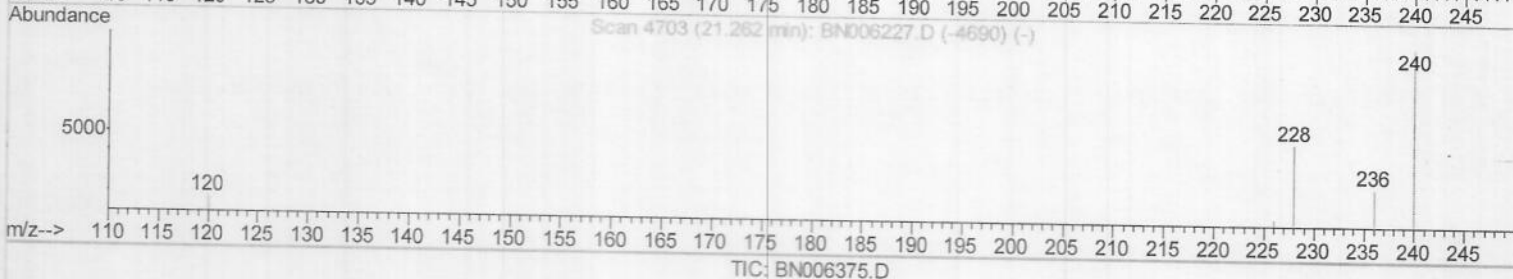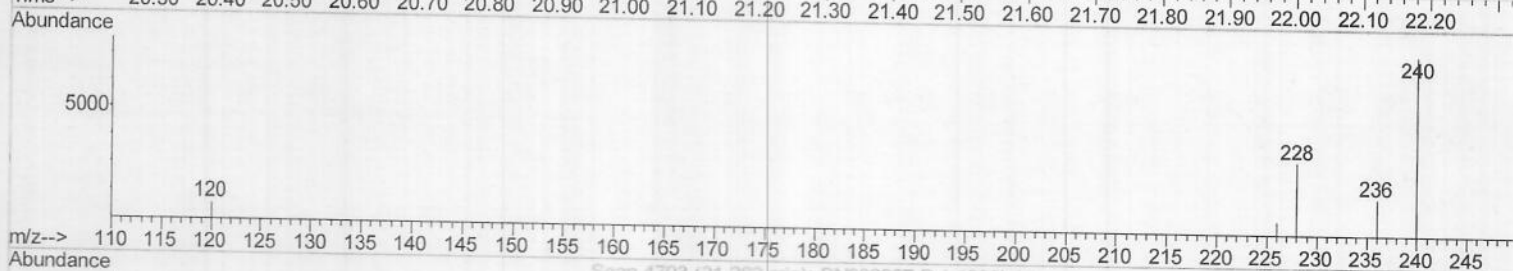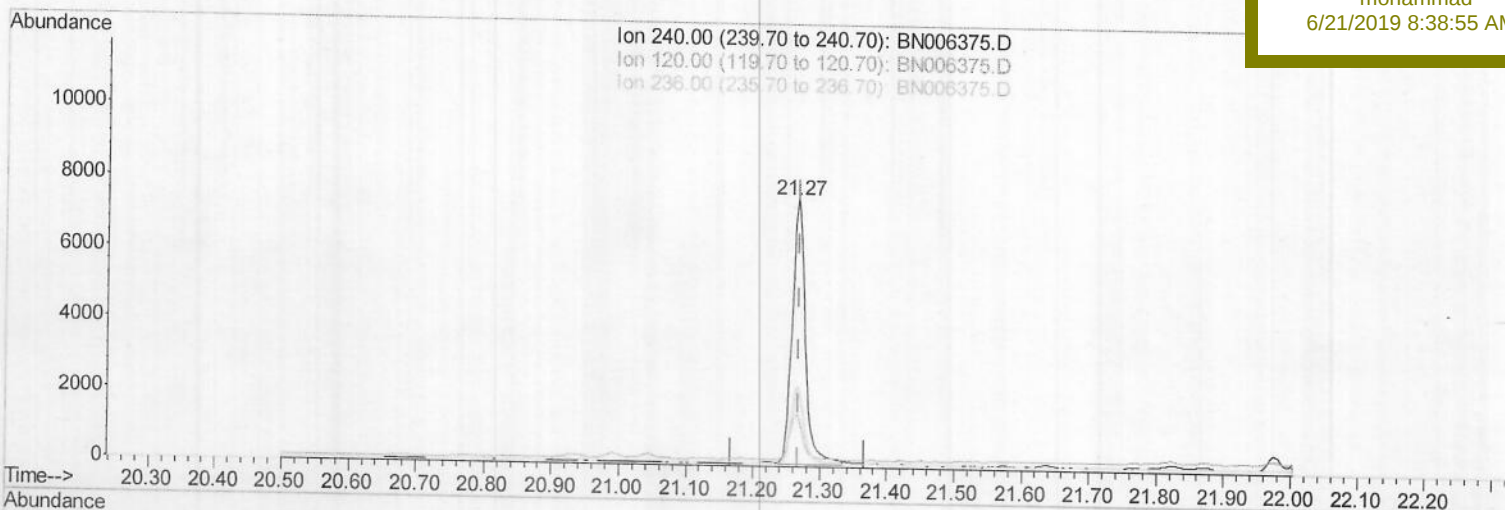

(16) Chrysene-d12 (I)

21.265min (-0.003) 0.40ng/ul m

response 10260

Ion	Exp%	Act%
240.00	100	100
120.00	20.10	19.69
236.00	30.10	29.81
0.00	0.00	0.00

JU 06/25/19

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061819\

Data File : BN006375.D

Acq On : 18 Jun 2019 13:30

Operator : JU/SJ

Sample : K3335-06

Misc :

ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jun 18 16:39:35 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Jun 18 15:57:40 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A4220

Manual Integrations

APPROVED

mohammad

6/21/2019 8:38:55 AM

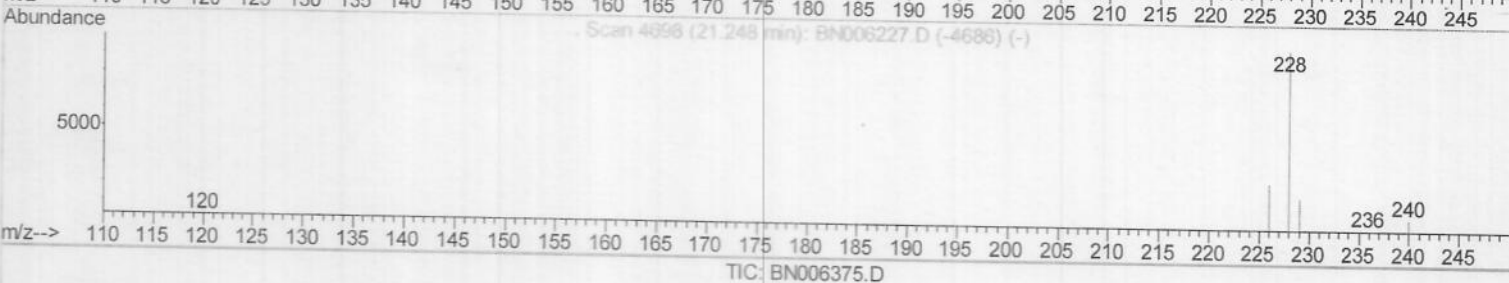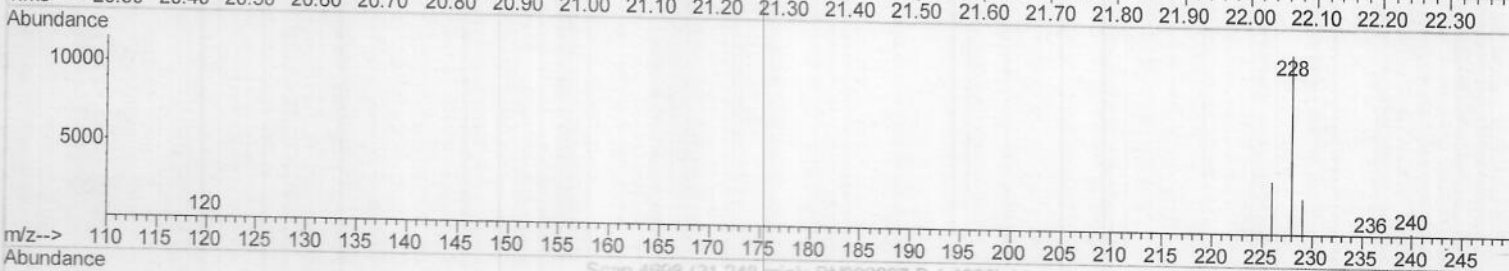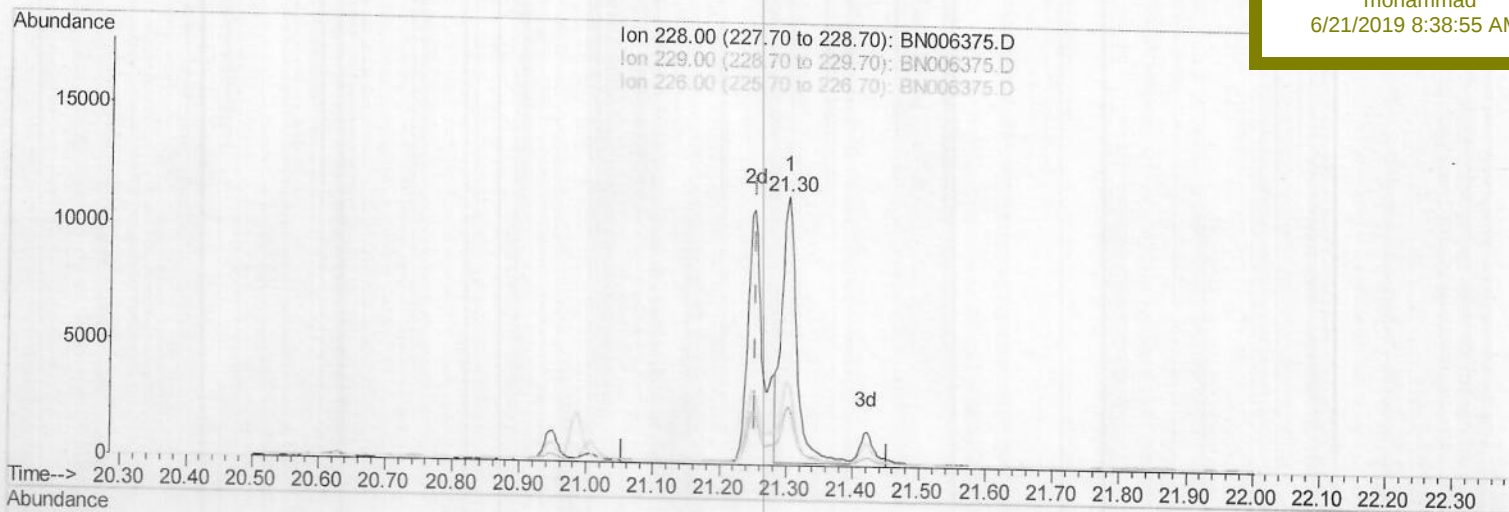

(18) Benzo(a)anthracene

21.303min (+0.050) 0.40ng/ul

response 18131

Ion	Exp%	Act%
228.00	100	100
229.00	20.60	21.75
226.00	28.50	31.07
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061819\
 Data File : BN006375.D
 Acq On : 18 Jun 2019 13:30
 Operator : JU/SJ
 Sample : K3335-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jun 18 16:39:35 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 18 15:57:40 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 A4220

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:38:55 AM

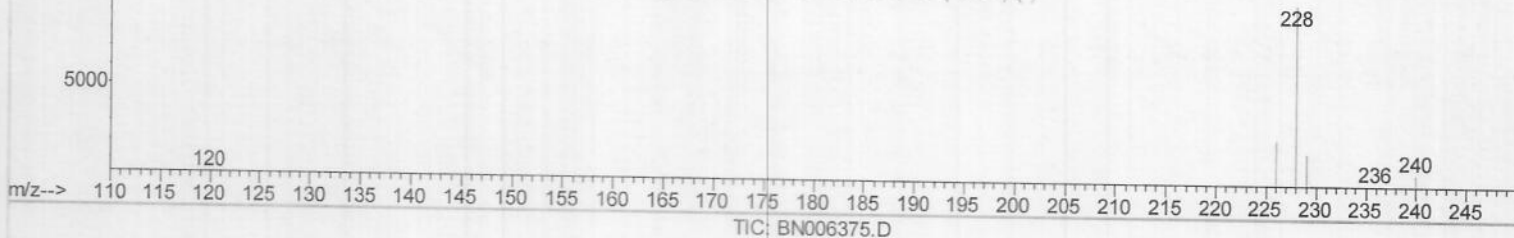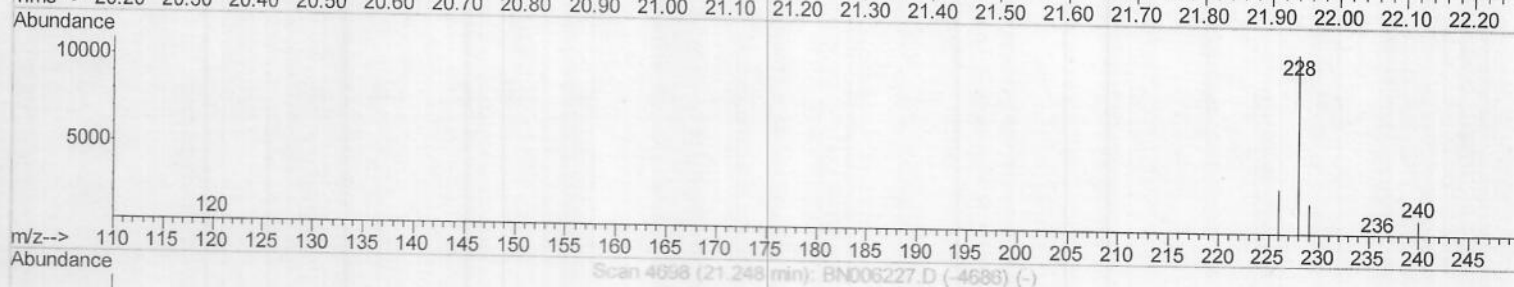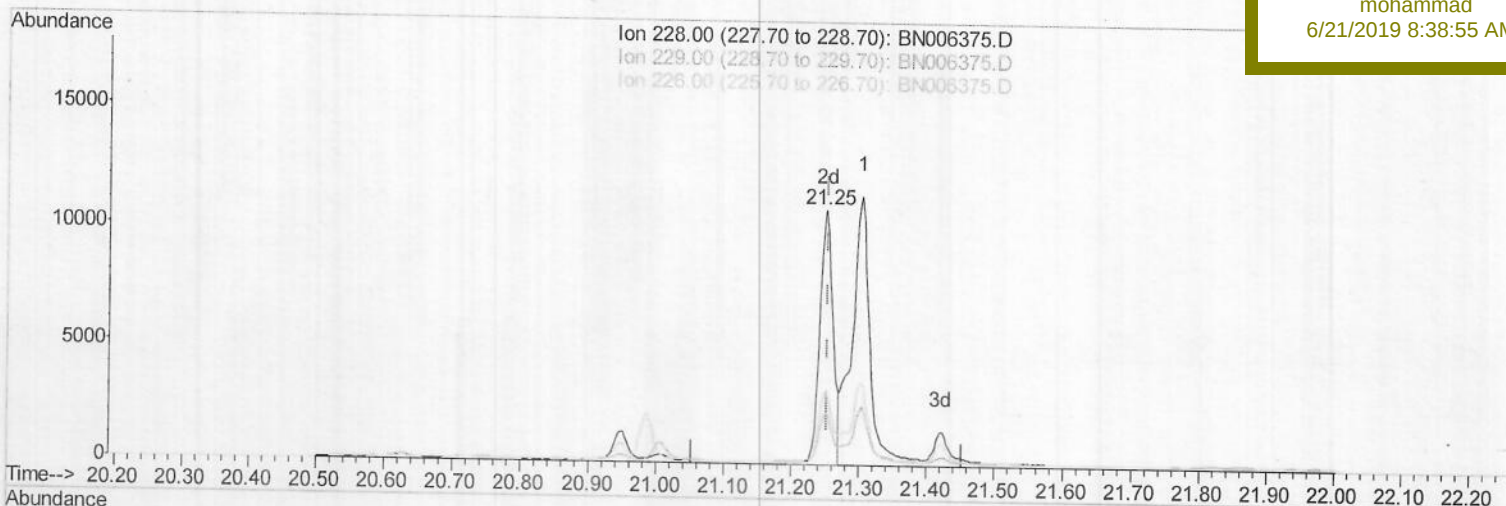

(18) Benzo(a)anthracene

21.251min (-0.003) 0.33ng/ul m

> JU 06/25/19

response 14807

Ion	Exp%	Act%
228.00	100	100
229.00	20.60	20.43
226.00	28.50	28.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061819\

Data File : BN006375.D

Acq On : 18 Jun 2019 13:30

Operator : JU/SJ

Sample : K3335-06

Misc :

ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jun 18 16:39:35 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Jun 18 15:57:40 2019




Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A4220

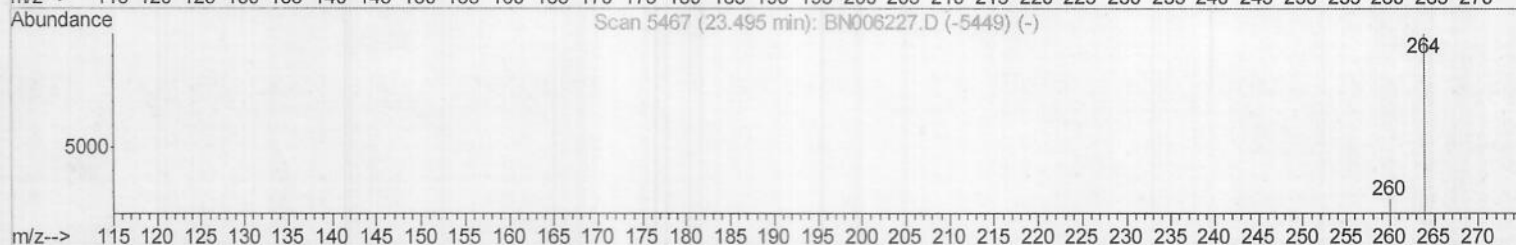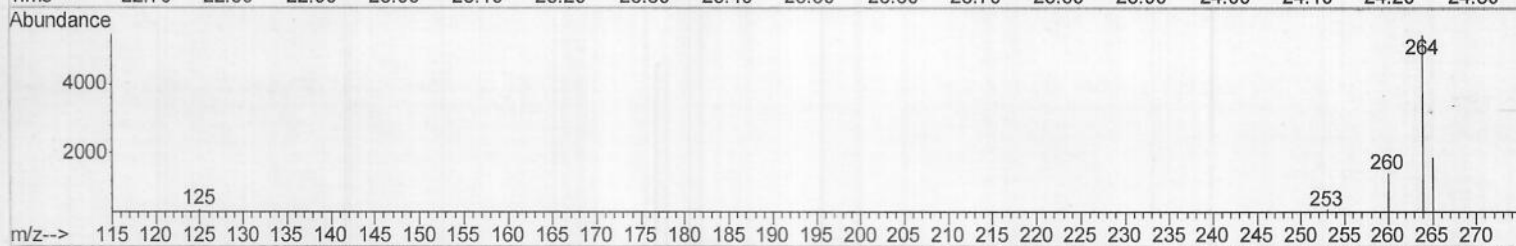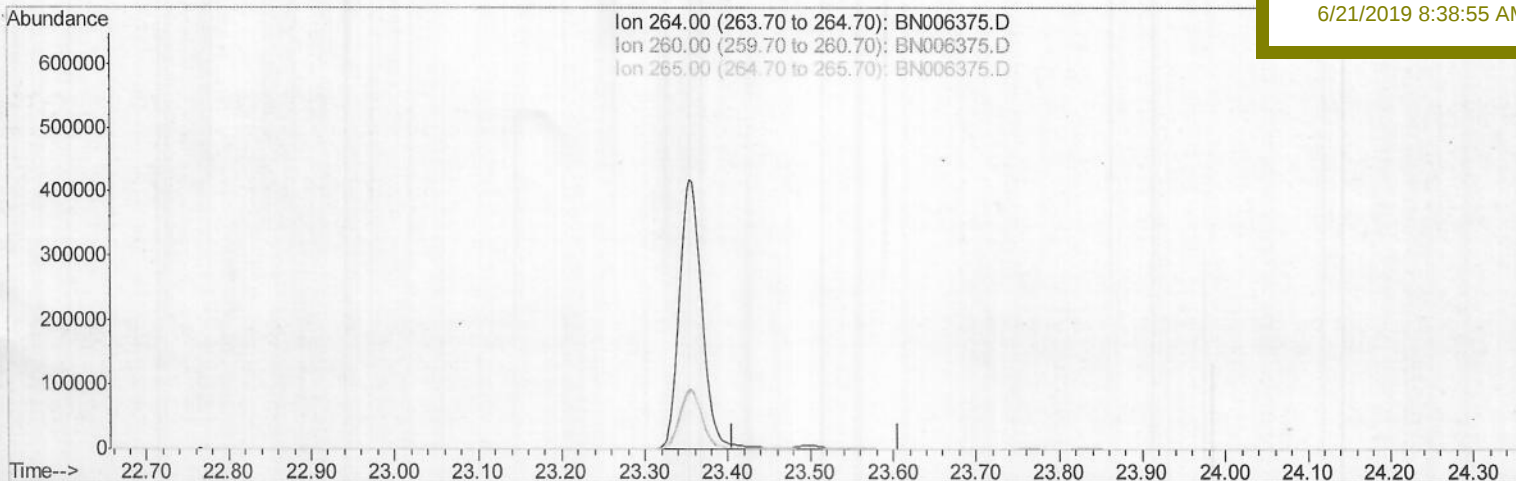Manual Integrations
APPROVEDmohammad
6/21/2019 8:38:55 AM

TIC: BN006375.D

(20) Perylene-d12 (I)

23.506min (-23.506) 0.00ng/ul

response 0

Ion	Exp%	Act%
264.00	100	0.00
260.00	29.20	0.00#
265.00	44.70	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061819\

Data File : BN006375.D

Acq On : 18 Jun 2019 13:30

Operator : JU/SJ

Sample : K3335-06

Misc :

ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jun 18 16:39:35 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Jun 18 15:57:40 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A4220

Manual Integrations

APPROVED

mohammad

6/21/2019 8:38:55 AM

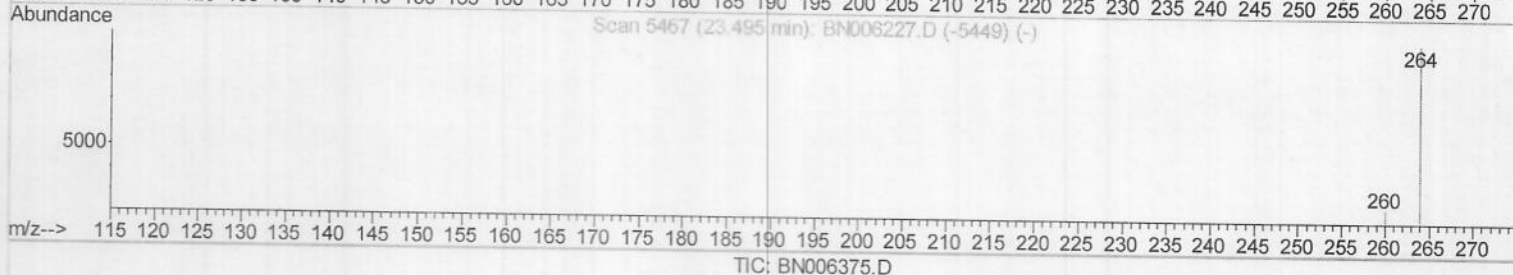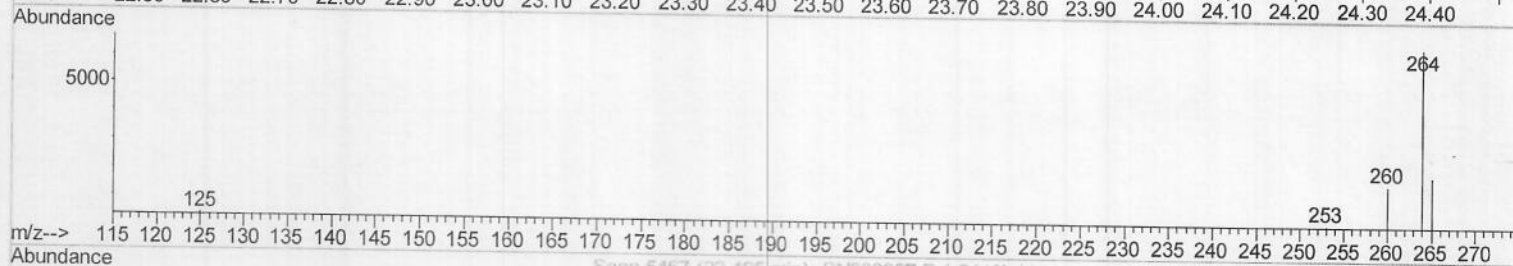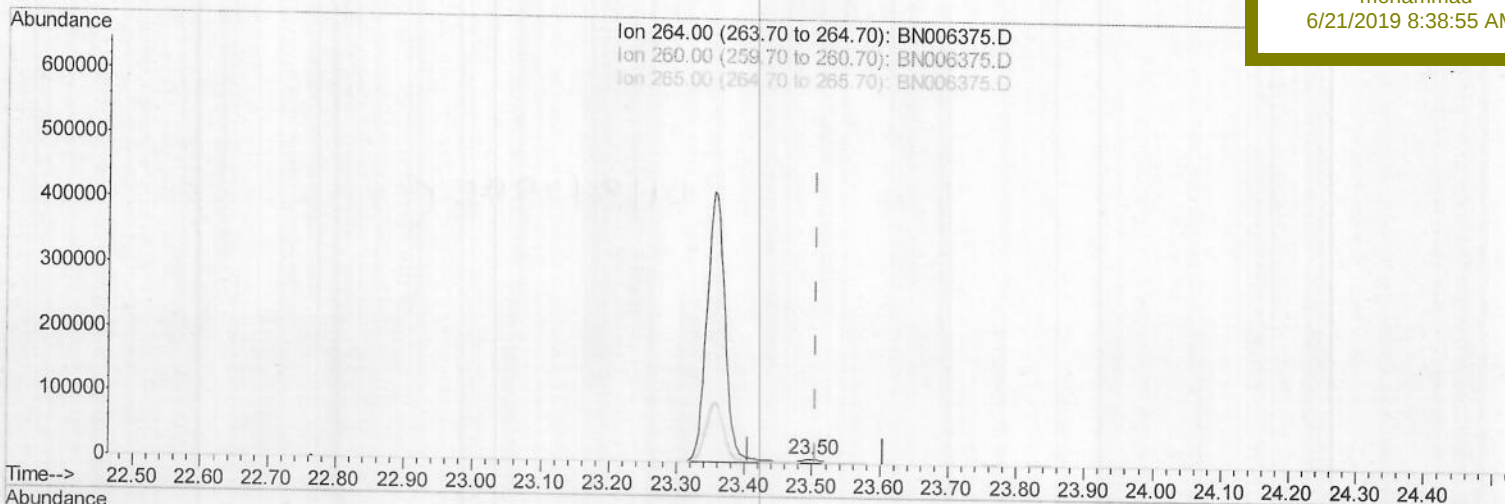

(20) Perylene-d12 (I)

23.498min (-0.008) 0.40ng/ul m

response 8809

Ion	Exp%	Act%
264.00	100	100
260.00	29.20	26.69
265.00	44.70	32.04#
0.00	0.00	0.00

JU 06/25/19

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061819\

Data File : BN006375.D

Acq On : 18 Jun 2019 13:30

Operator : JU/SJ

Sample : K3335-06

Misc :

ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jun 18 16:40:37 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Jun 18 15:57:40 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A4220

Manual Integrations

APPROVED

mohammad

6/21/2019 8:38:55 AM

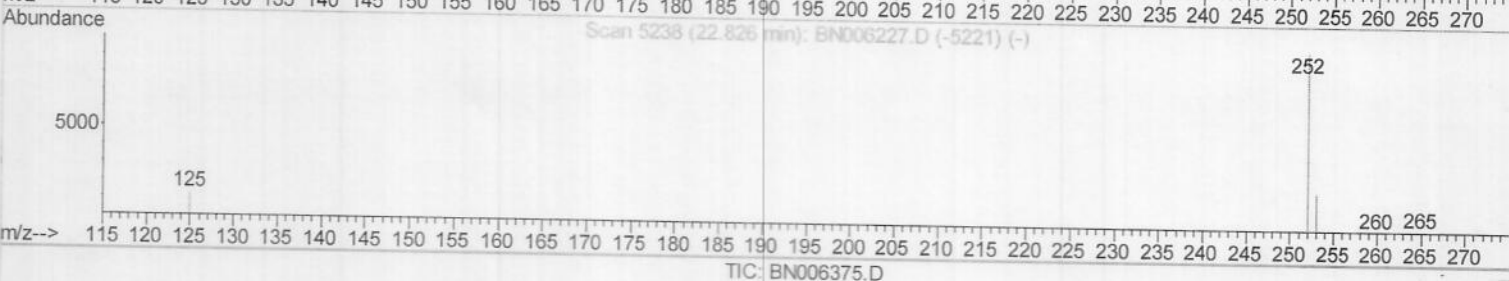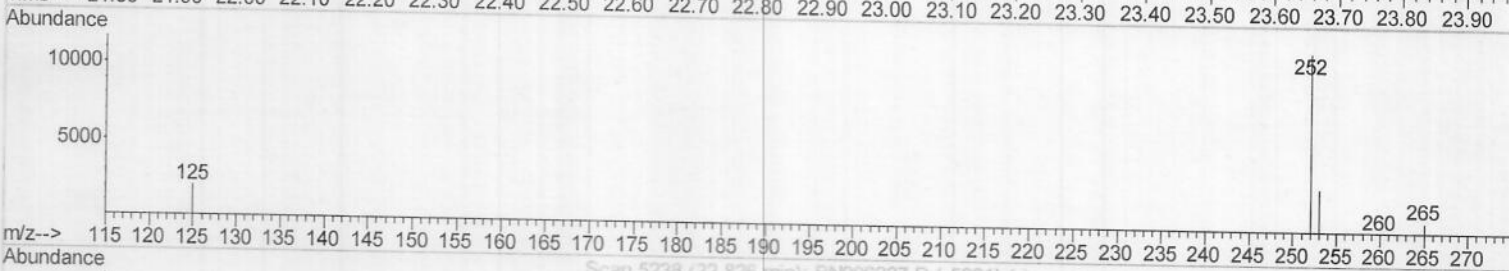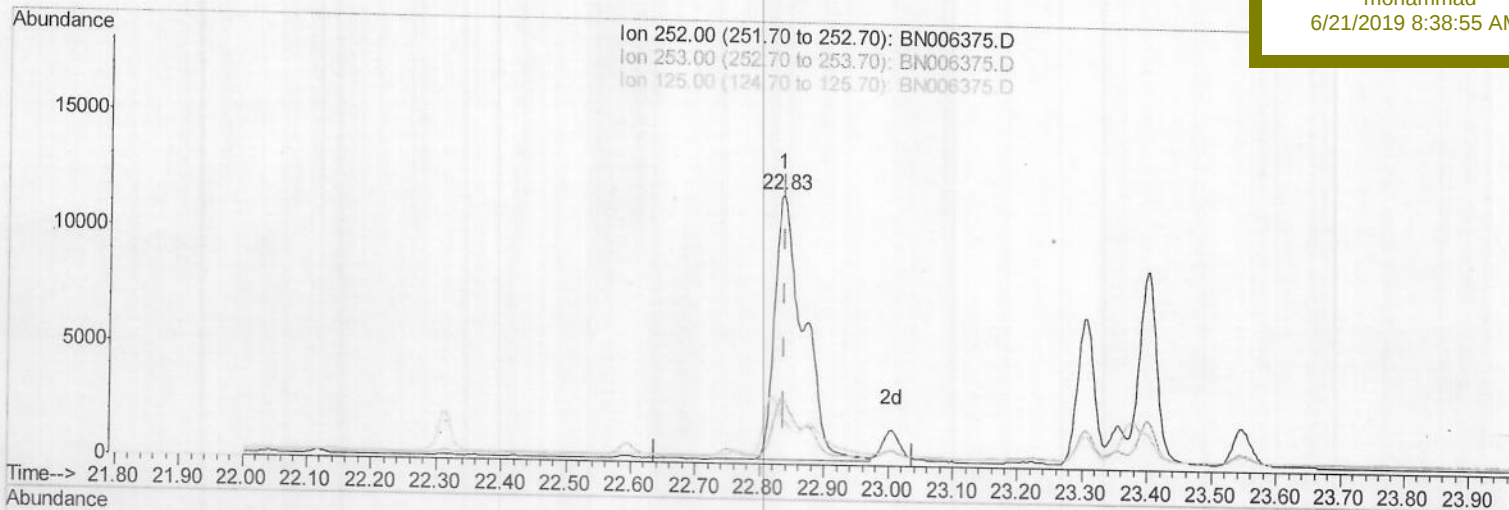

(21) Benzo(b)fluoranthene

22.835min (-0.003) 0.98ng/ul

response 36168

Ion Exp% Act%

252.00 100 100

253.00 25.70 24.75

125.00 20.50 17.55

0.00 0.00 0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061819\
Data File : BN006375.D
Acq On : 18 Jun 2019 13:30
Operator : JU/SJ
Sample : K3335-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jun 18 16:40:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 15:57:40 2019
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
A4220

Manual Integrations
APPROVED

mohammad
6/21/2019 8:38:55 AM

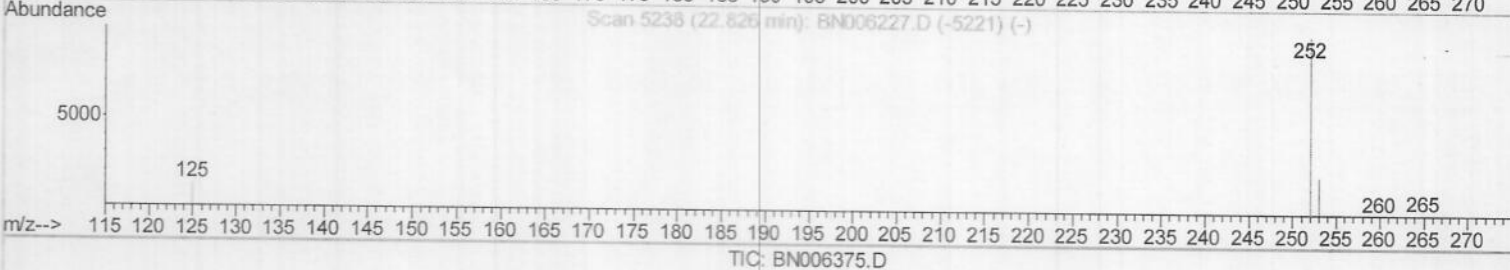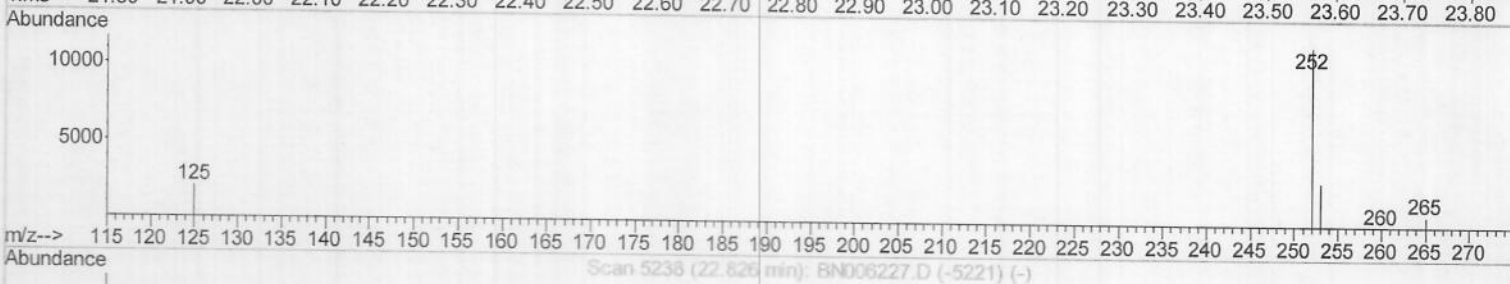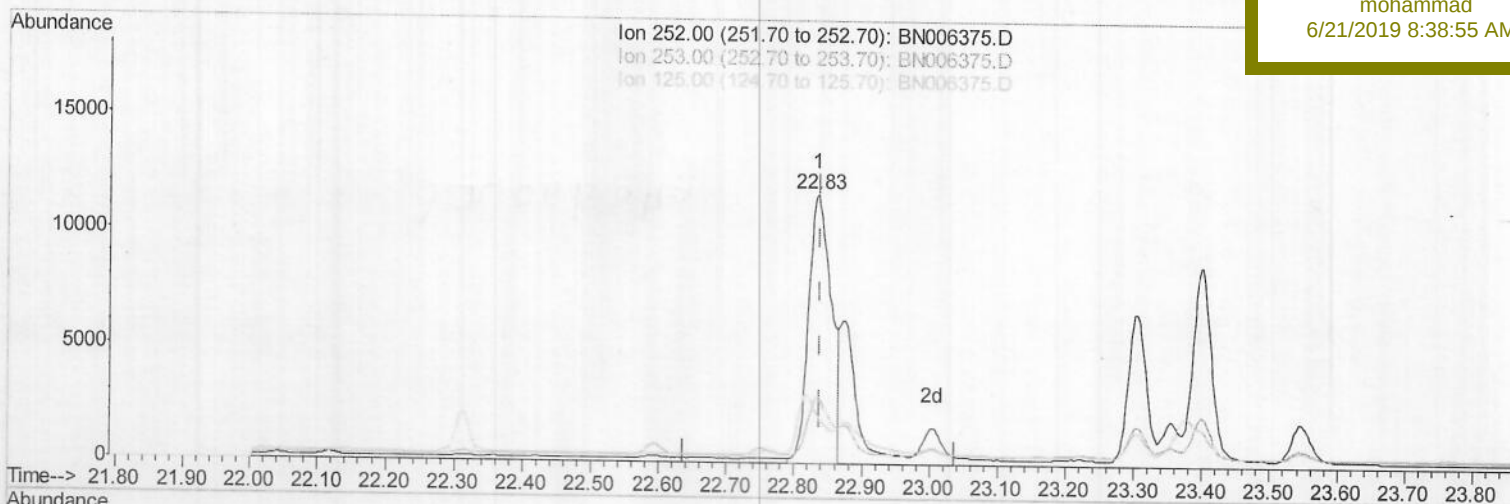

(21) Benzo(b)fluoranthene

22.835min (-0.003) 0.73ng/ul m

response 26731

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	24.75
125.00	20.50	17.55
0.00	0.00	0.00

> JU 06/25/19

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061819\

Data File : BN006375.D

Acq On : 18 Jun 2019 13:30

Operator : JU/SJ

Sample : K3335-06

Misc :

ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jun 18 16:40:37 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Jun 18 15:57:40 2019




Response via : Initial Calibration

Instrument :

BNA_N

Client Sampled :

A4220

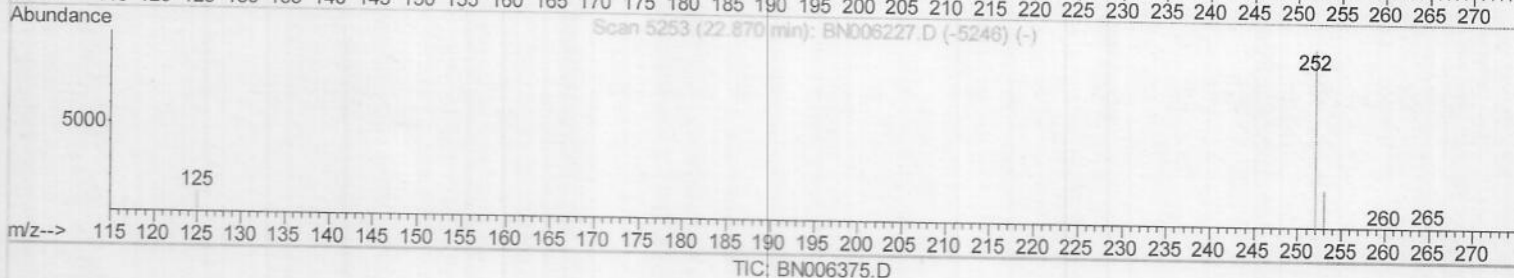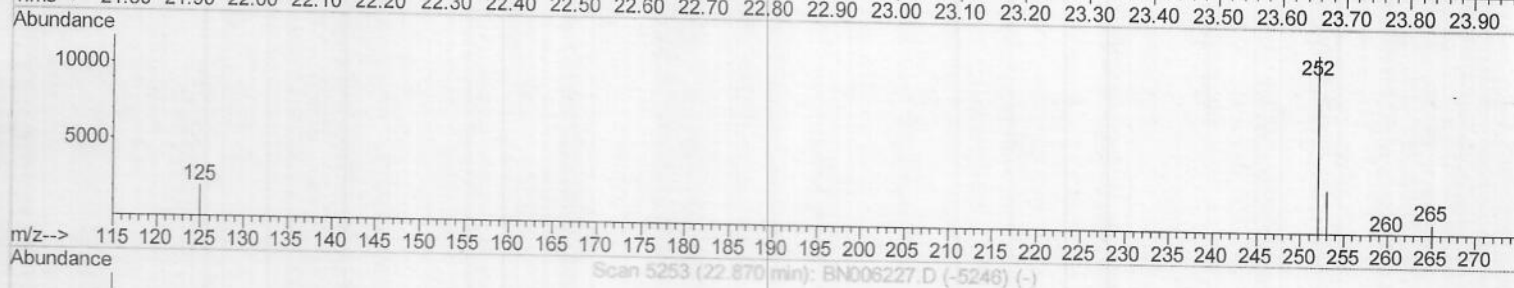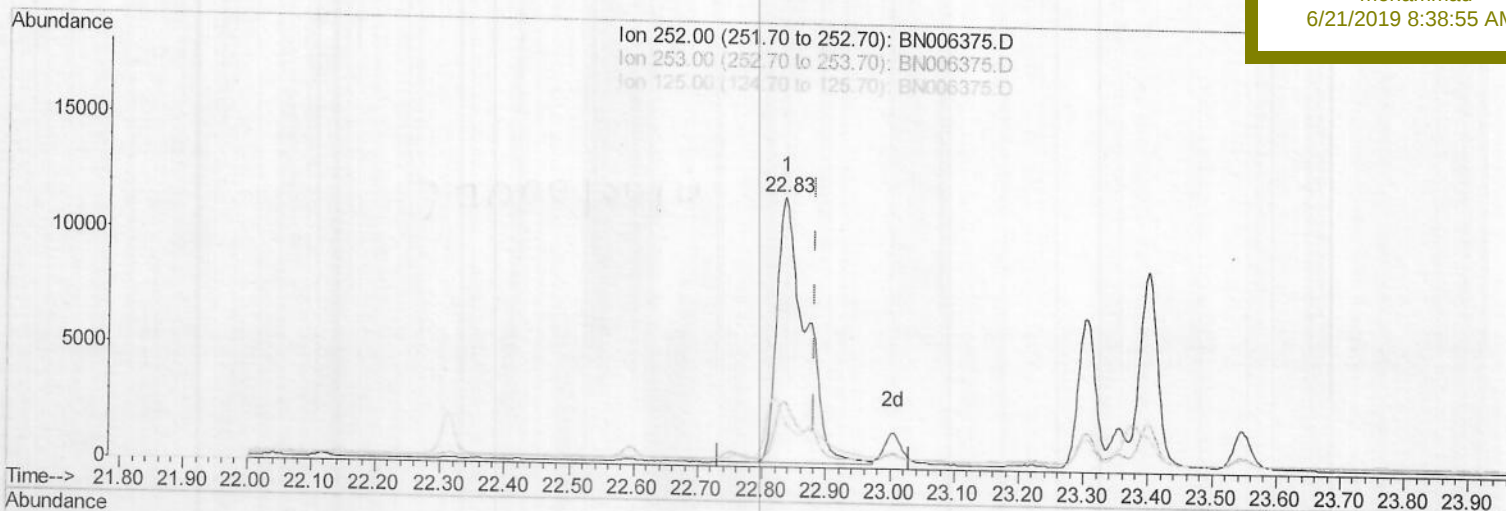Manual Integrations
APPROVEDmohammad
6/21/2019 8:38:55 AM

(22) Benzo(k)fluoranthene

22.835min (-0.047) 1.01ng/ul

response 36191

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	24.75
125.00	17.90	17.55
0.00	0.00	0.00

Quantitation Report. (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061819\

Data File : BN006375.D

Acq On : 18 Jun 2019 13:30

Operator : JU/SJ

Sample : K3335-06

Misc :

ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jun 18 16:40:37 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Jun 18 15:57:40 2019

Response via : Initial Calibration

Instrument :

BNA_N

Client Sampled :




A4220

Manual Integrations

APPROVED

mohammad

6/21/2019 8:38:55 AM

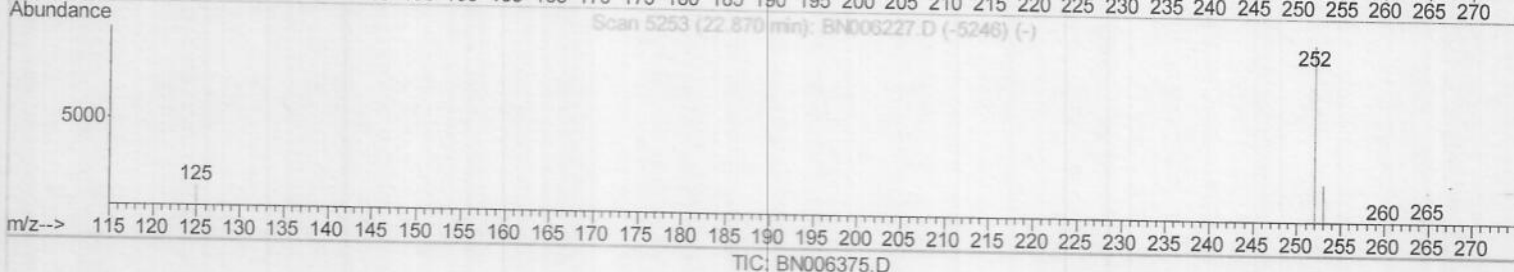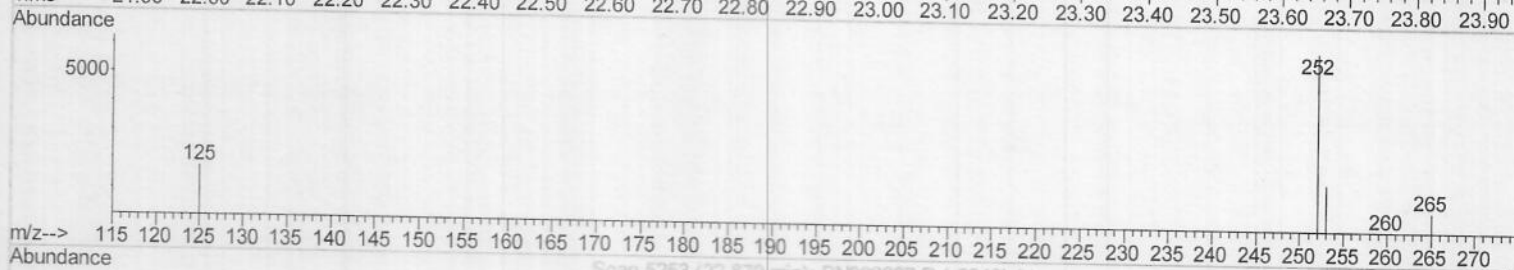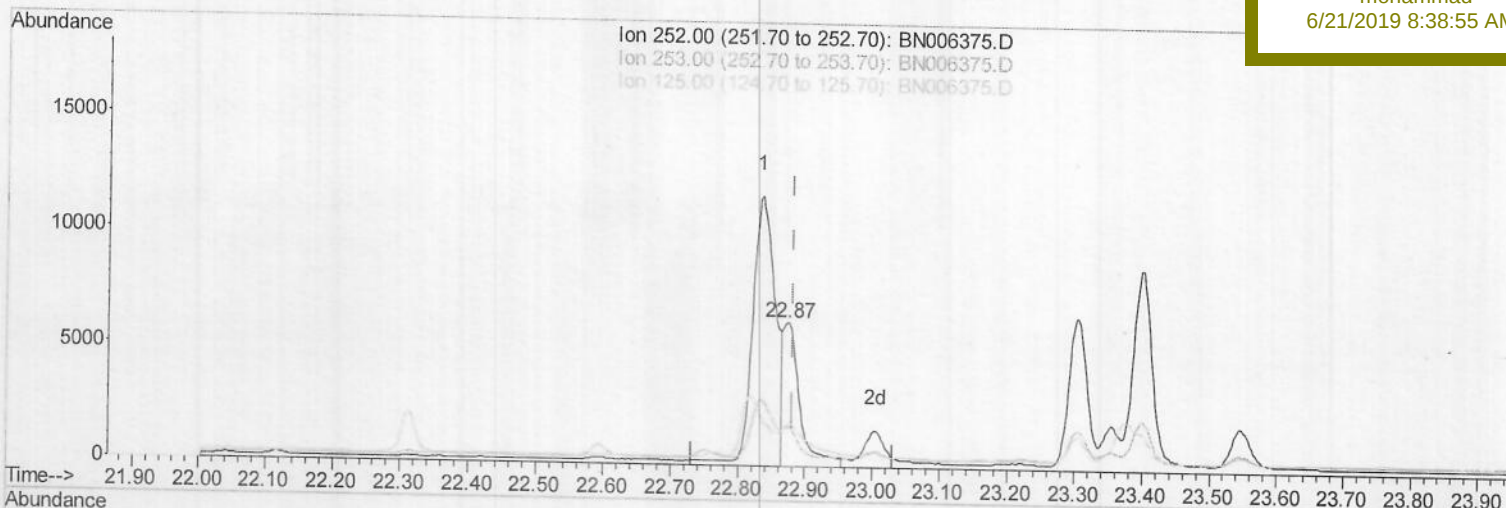

(22) Benzo(k)fluoranthene

22.873min (-0.009) 0.31ng/ul m

response 11150

Ion Exp% Act%

252.00 100 100

253.00 25.40 27.10

125.00 17.90 28.05#

0.00 0.00 0.00

7 JU 06/25/19

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061819\
 Data File : BN006375.D
 Acq On : 18 Jun 2019 13:30
 Operator : JU/SJ
 Sample : K3335-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jun 18 16:41:23 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 18 15:57:40 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 A4220

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:38:55 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	4287	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	17242	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.29	164	9104	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	16934m	0.40	ng/ul	0.00
16) Chrysene-d12	21.27	240	10260m	0.40	ng/ul	0.00
20) Perylene-d12	23.50	264	8809m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	6084	0.23	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	11794m	0.26	ng/ul	0.00
Target Compounds						
7) Acenaphthylene	14.01	152	1069	0.021	ng/ul#	82
12) Phenanthrene	17.09	178	17860	0.329	ng/ul	99
13) Anthracene	17.18	178	2724m	0.052	ng/ul	
15) Fluoranthene	19.12	202	48409m	0.806	ng/ul	
17) Pyrene	19.48	202	39807	0.737	ng/ul	98
18) Benzo(a)anthracene	21.25	228	14807m	0.326	ng/ul	
19) Chrysene	21.30	228	17126	0.402	ng/ul	99
21) Benzo(b)fluoranthene	22.83	252	26731m	0.728	ng/ul	
22) Benzo(k)fluoranthene	22.87	252	11150m	0.312	ng/ul	
23) Benzo(a)pyrene	23.40	252	16243	0.475	ng/ul#	92
24) Indeno(1,2,3-cd)pyrene	25.74	276	11443	0.309	ng/ul#	86
25) Dibenzo(a,h)anthracene	25.74	278	2631	0.089	ng/ul#	84
26) Benzo(g,h,i)perylene	26.42	276	9252	0.298	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU
 06/25/19