


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
Data File : BN006382.D
Acq On : 18 Jun 2019 18:25
Operator : JU/SJ
Sample : K3335-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Jun 19 01:39:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
A41T9

Manual Integrations
APPROVED

mohammad
6/21/2019 8:39:13 AM

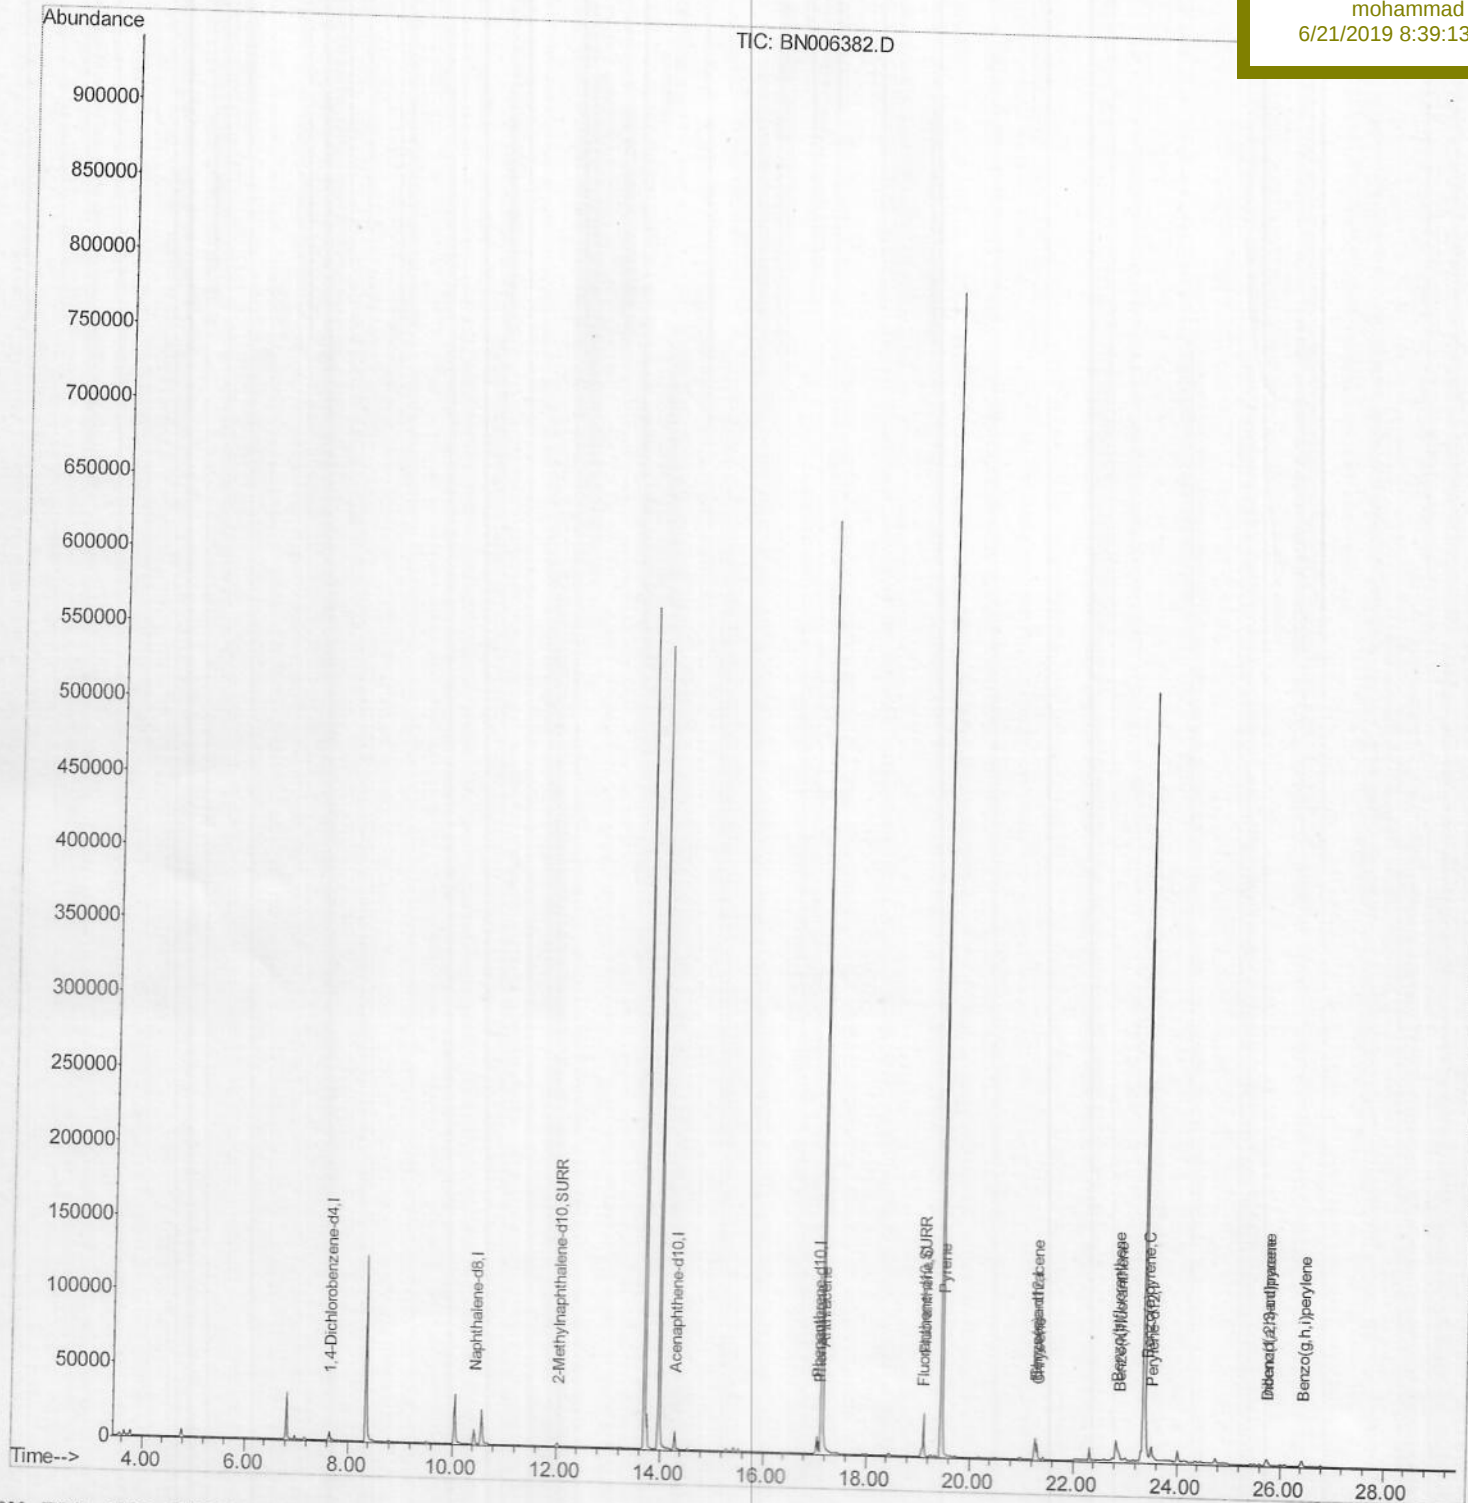

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\

Data File : BN006382.D

Acq On : 18 Jun 2019 18:25

Operator : JU/SJ

Sample : K3335-03

Misc :

ALS Vial : 14 Sample Multiplier: 1

Quant Time: Jun 19 01:28:49 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :




BNA_N

ClientSampleId :

A41T9

Manual Integrations
APPROVED

mohammad
6/21/2019 8:39:13 AM

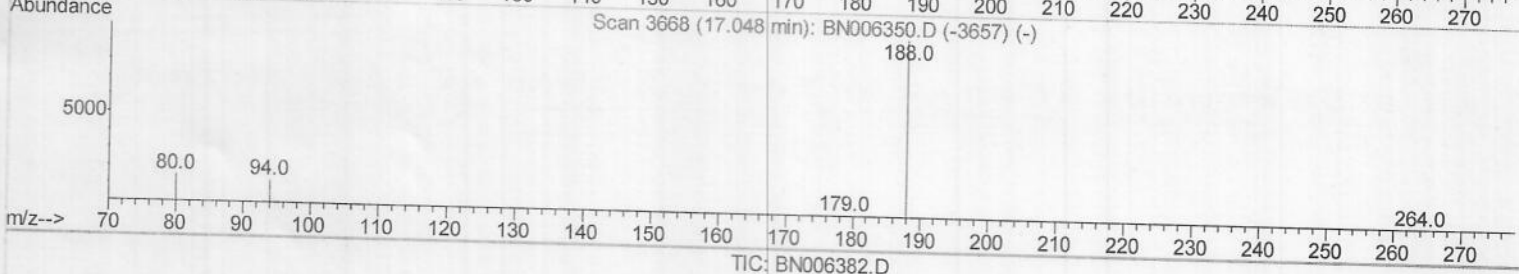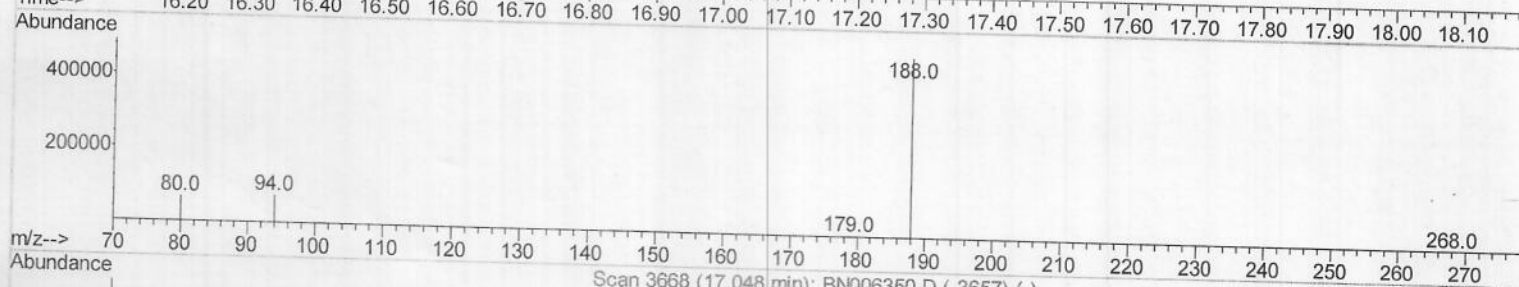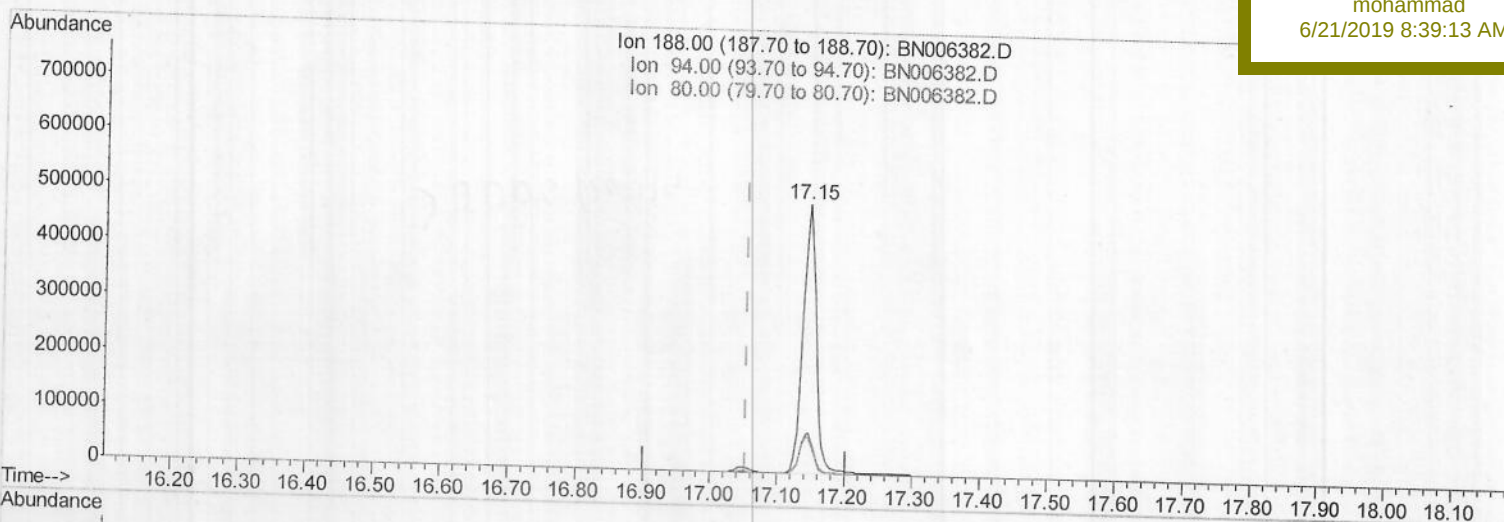

(10) Phenanthrene-d10 (I)

17.145min (+0.093) 0.40ng/ul

response 667519

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	14.82
80.00	13.60	13.53
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006382.D
 Acq On : 18 Jun 2019 18:25
 Operator : JU/SJ
 Sample : K3335-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :

BNA_N

ClientSampleId :

A41T9

Manual Integrations

APPROVED

mohammad

6/21/2019 8:39:13 AM



Quant Time: Jun 19 01:28:49 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

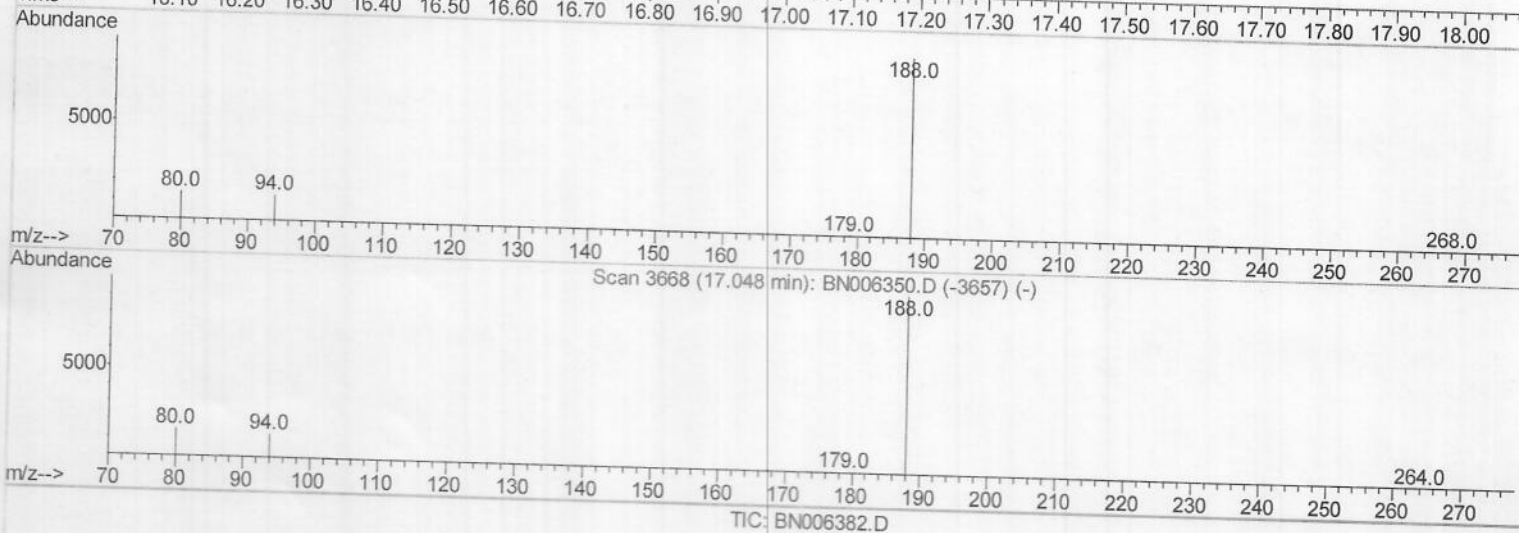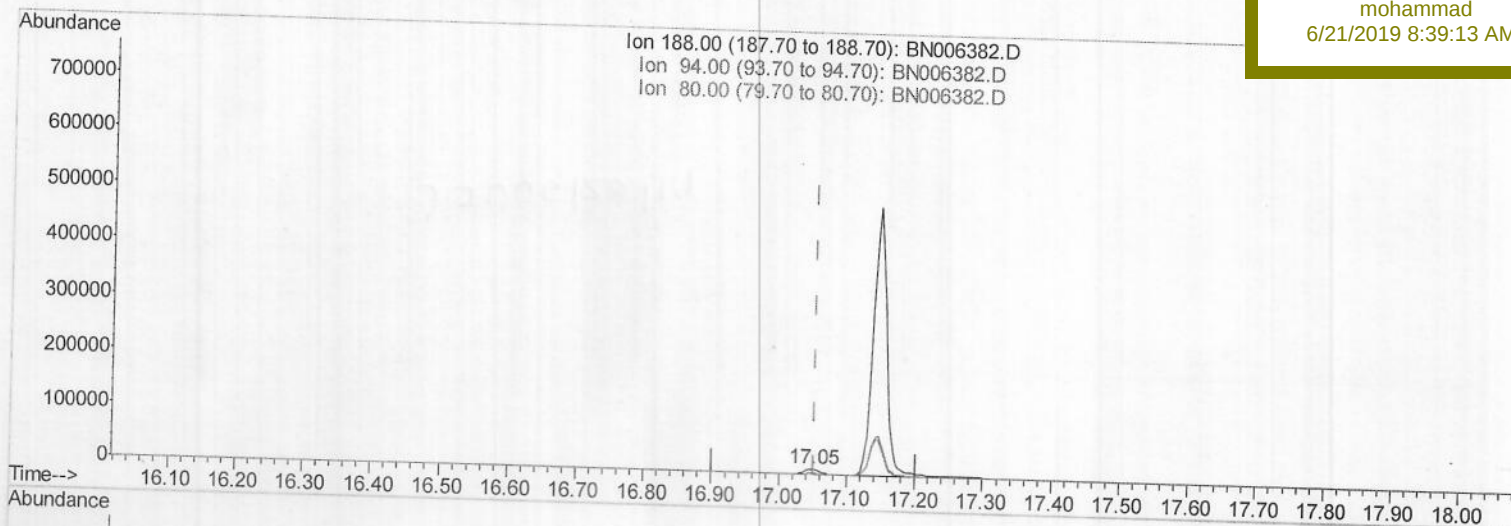

(10) Phenanthrene-d10 (I)

17.048min (-0.004) 0.40ng/ul m

> JU 06/25/19

response 13652

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	14.23
80.00	13.60	15.32
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006382.D
 Acq On : 18 Jun 2019 18:25
 Operator : JU/SJ
 Sample : K3335-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Jun 19 01:35:55 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 A41T9

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:39:13 AM

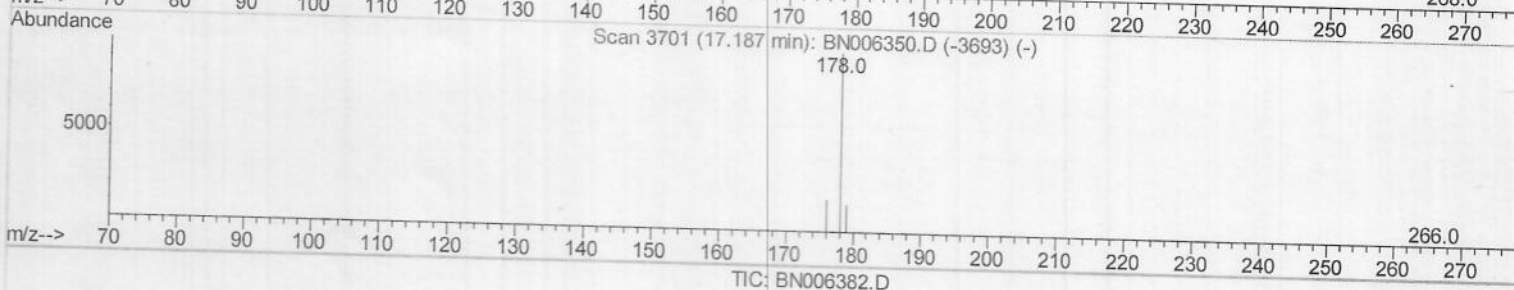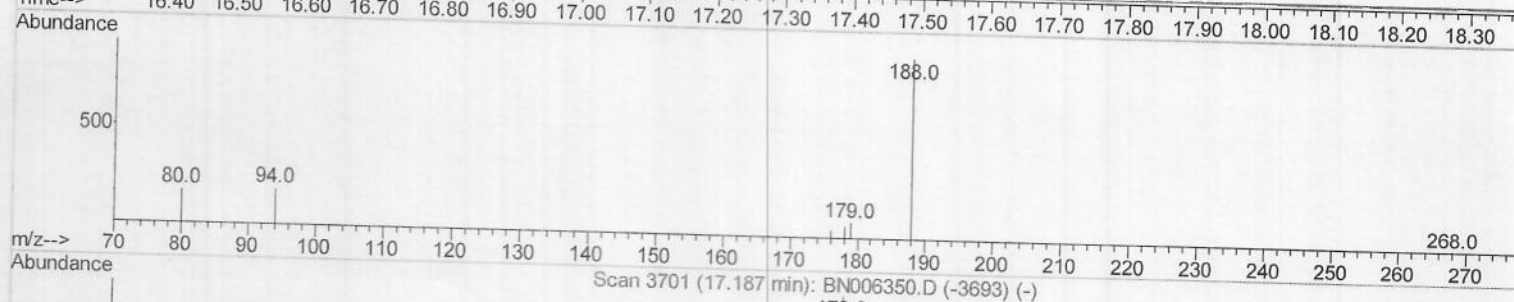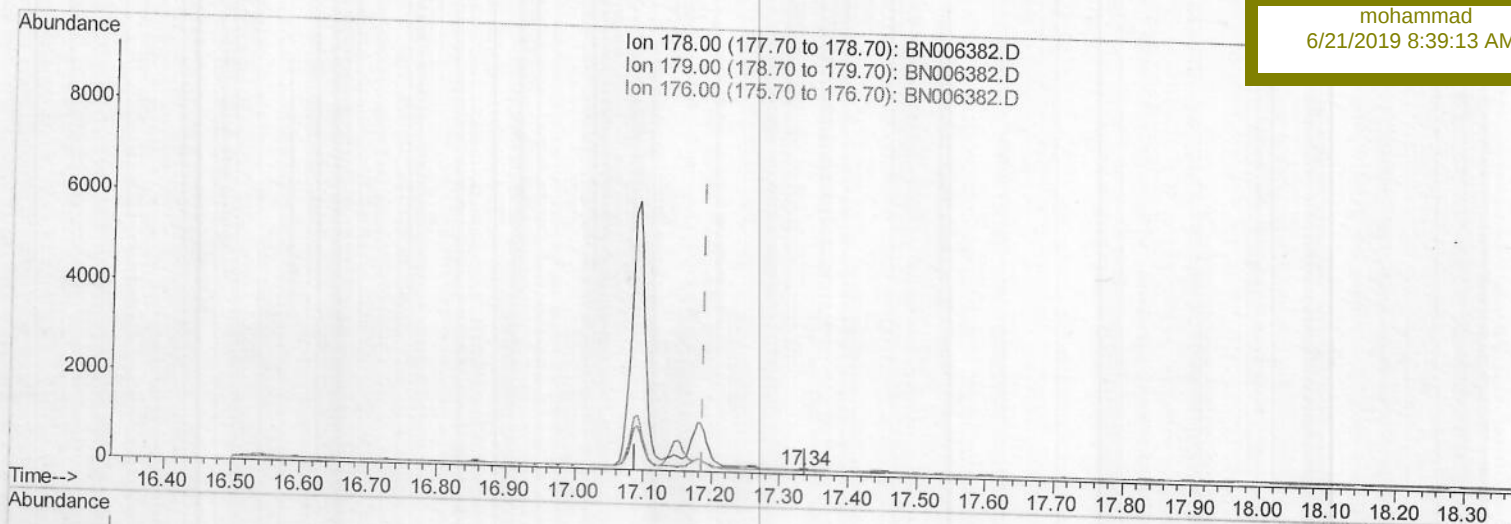

(13) Anthracene

17.335min (+0.148) 0.00ng/ul

response 37

Ion	Exp%	Act%
178.00	100	100
179.00	15.30	115.74#
176.00	18.90	76.85#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
Data File : BN006382.D

Acq On : 18 Jun 2019 18:25

Operator : JU/SJ

Sample : K3335-03

Misc :

ALS Vial : 14 Sample Multiplier: 1

Quant Time: Jun 19 01:35:55 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A41T9

Manual Integrations

APPROVED

mohammad

6/21/2019 8:39:13 AM

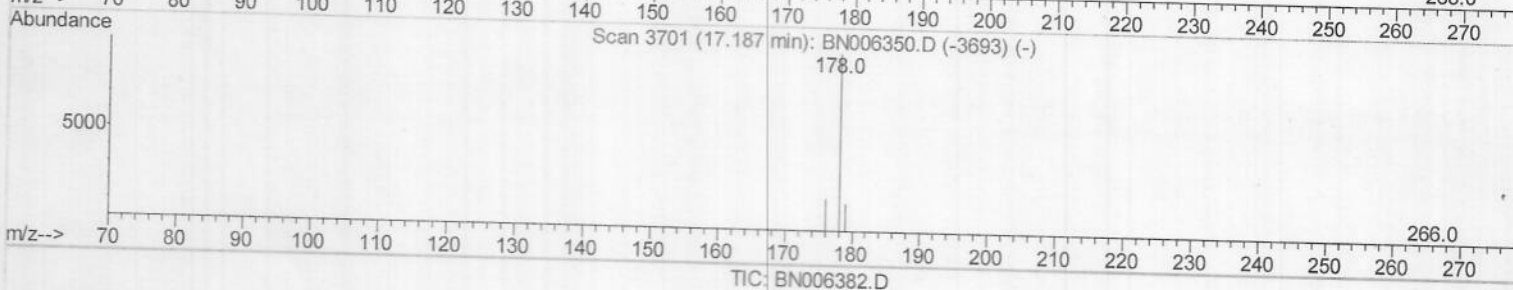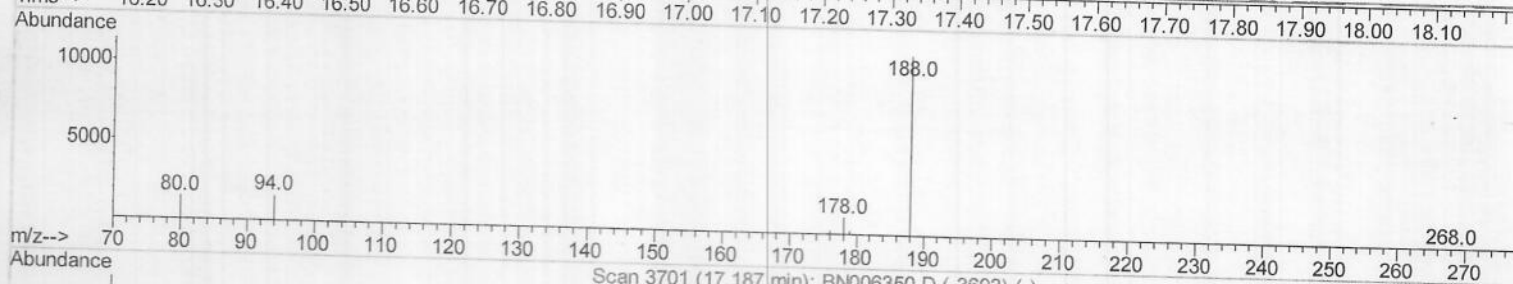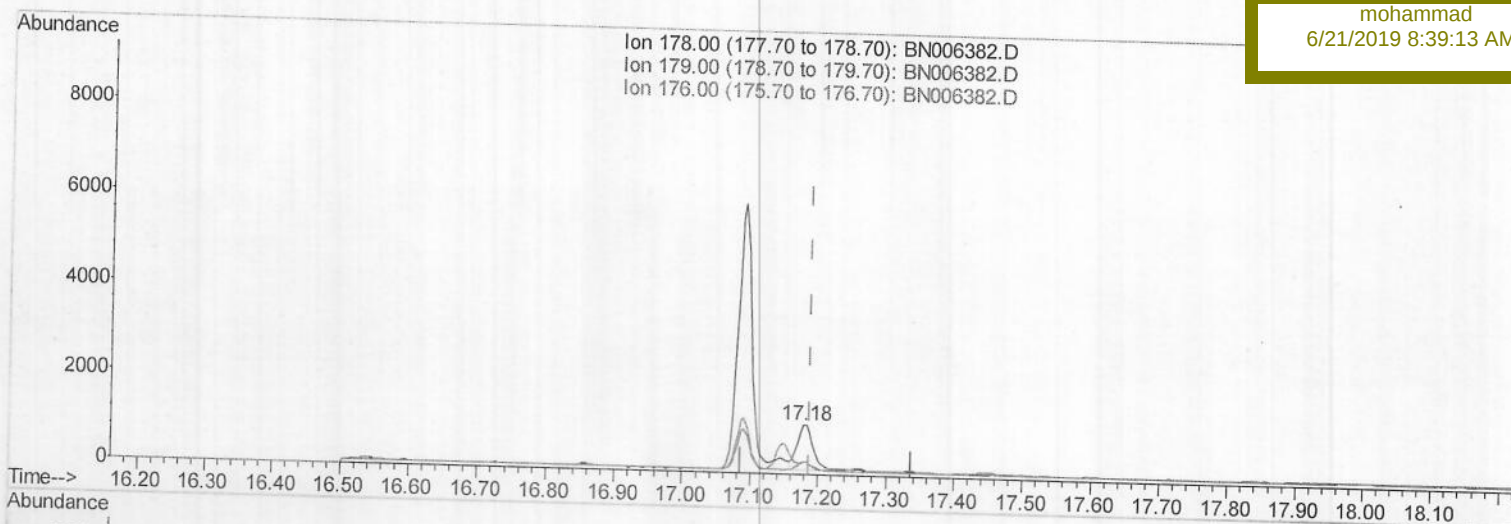

(13) Anthracene

17.179min (-0.008) 0.04ng/ul m > JU 06/25/19

response 1567

Ion	Exp%	Act%
178.00	100	100
179.00	15.30	23.91#
176.00	18.90	25.45#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006382.D
 Acq On : 18 Jun 2019 18:25
 Operator : JU/SJ
 Sample : K3335-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A41T9

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:39:13 AM

Quant Time: Jun 19 01:35:55 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

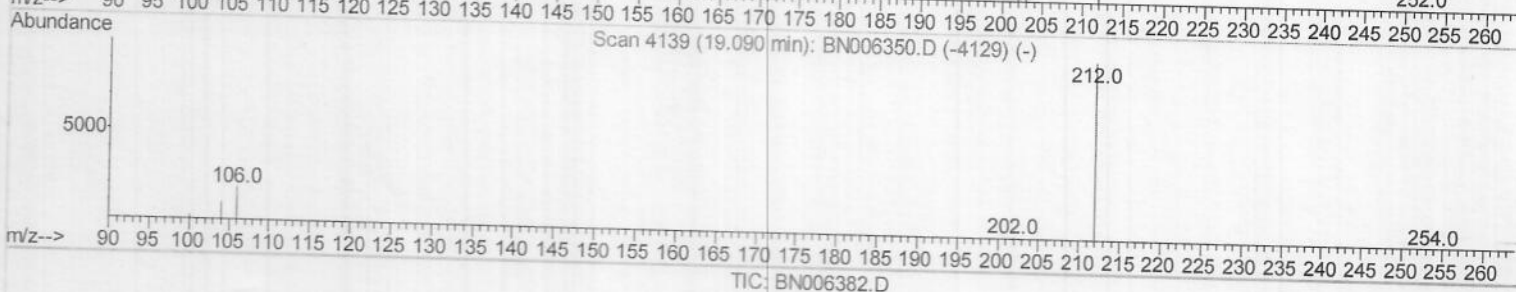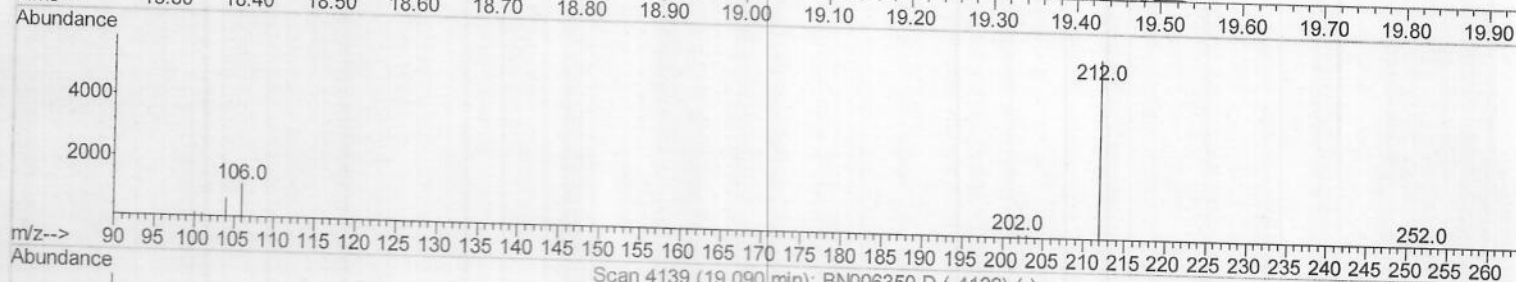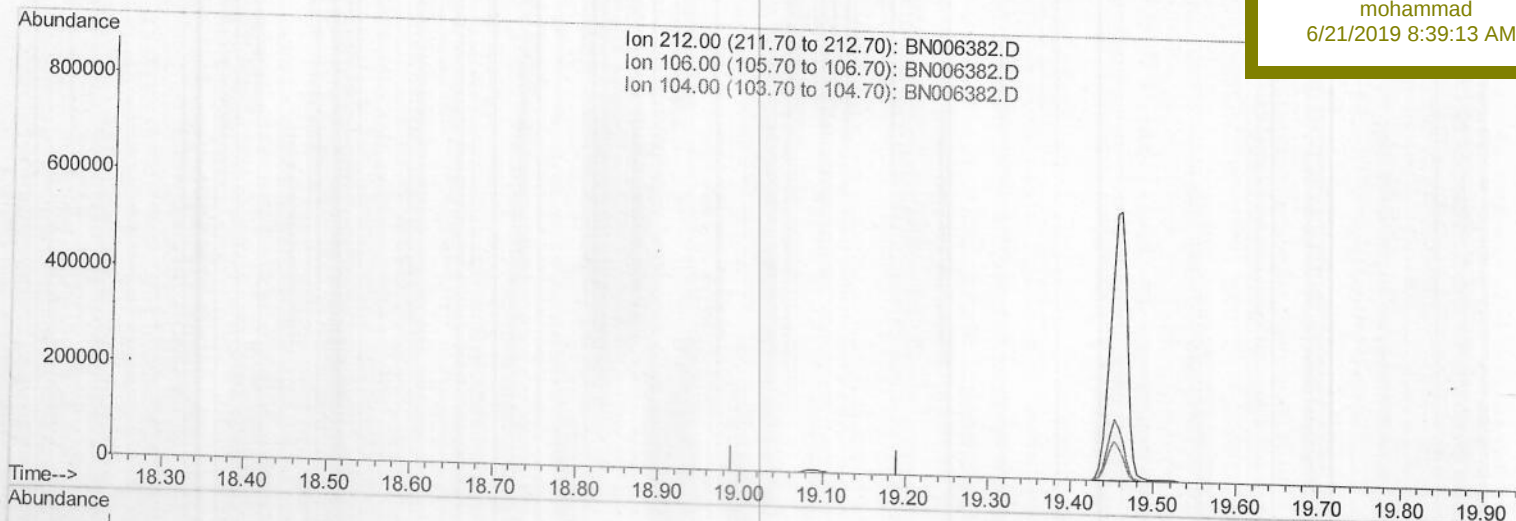

(14) Fluoranthene-d10 (SURR)

19.090min (-19.090) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061819\
 Data File : BN006382.D
 Acq On : 18 Jun 2019 18:25
 Operator : JU/SJ
 Sample : K3335-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A41T9

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:39:13 AM

Quant Time: Jun 19 01:39:42 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

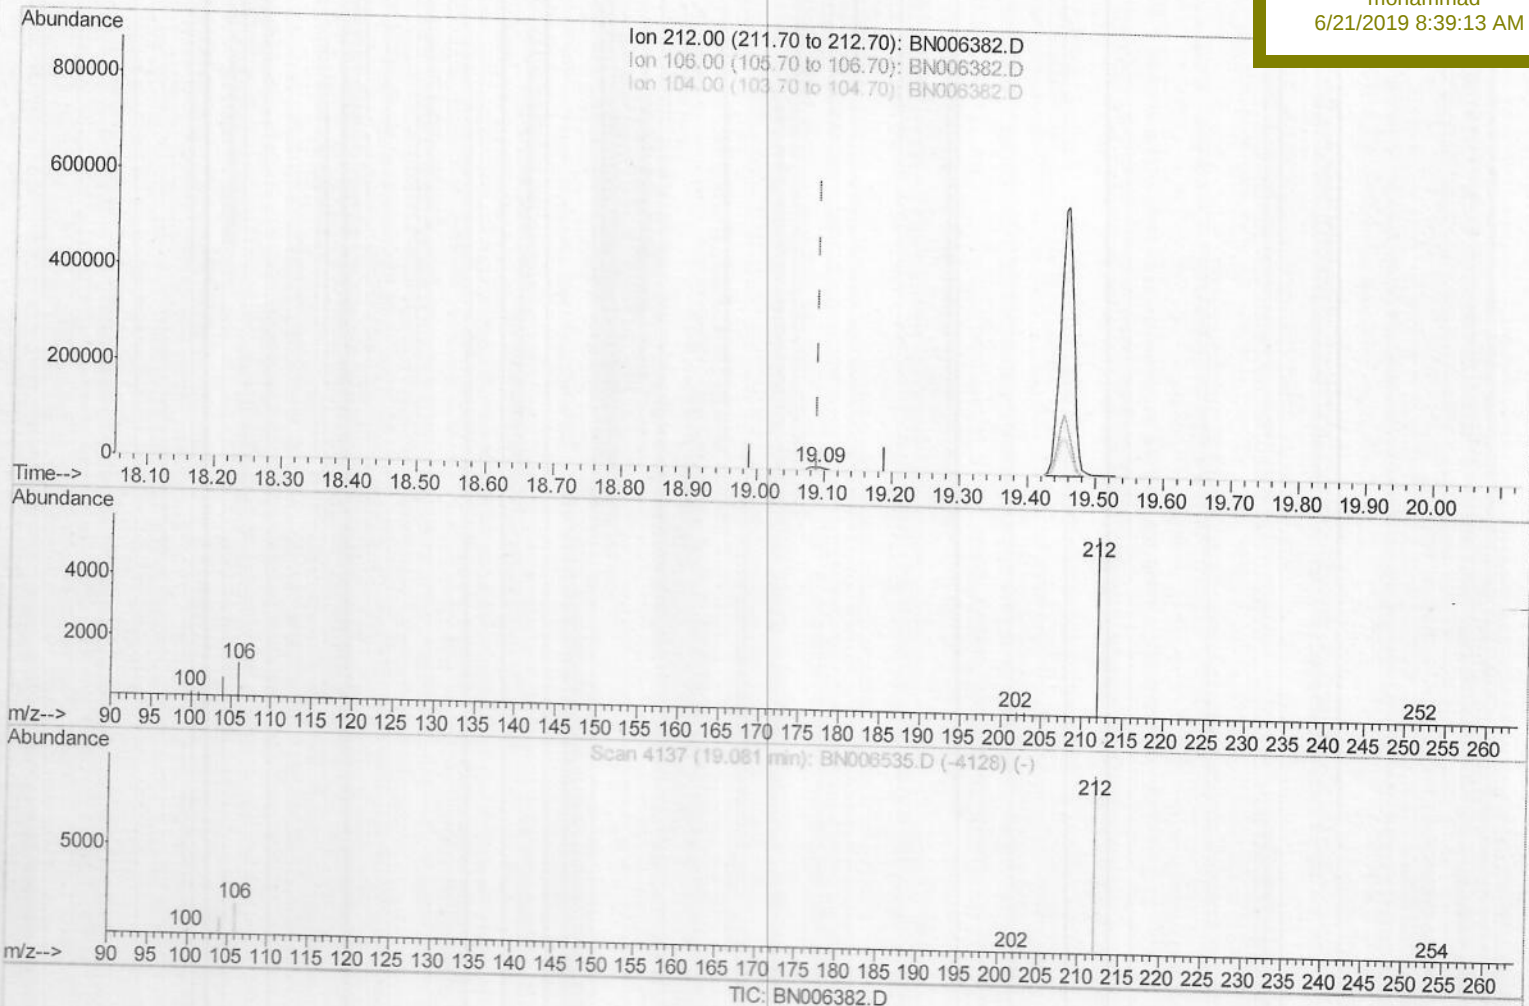

(14) Fluoranthene-d10 (SURR)

19.090min (-0.000) 0.23ng/ul m

response 8311

Ion	Exp%	Act%
212.00	100	100
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00

JU06/25/19

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006382.D
 Acq On : 18 Jun 2019 18:25
 Operator : JU/SJ
 Sample : K3335-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :

BNA_N

ClientSampleId :

A41T9




Manual Integrations

APPROVED

mohammad

6/21/2019 8:39:13 AM

Quant Time: Jun 19 01:35:55 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

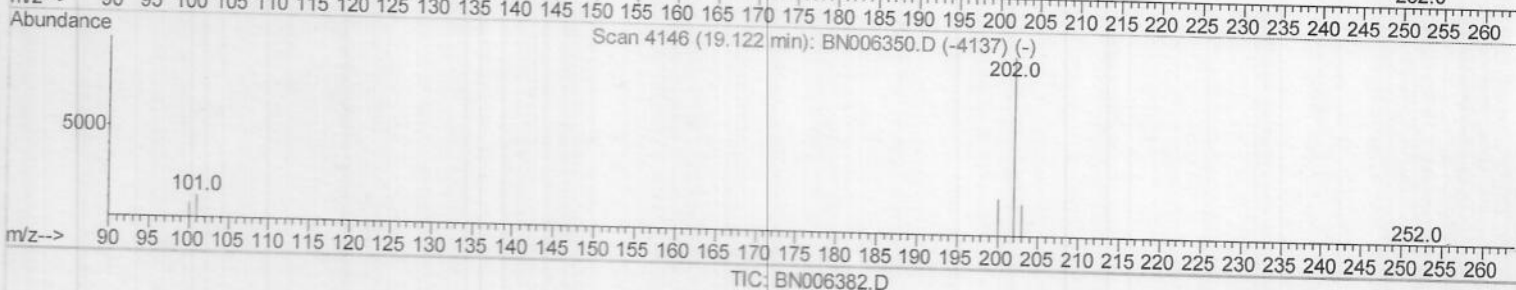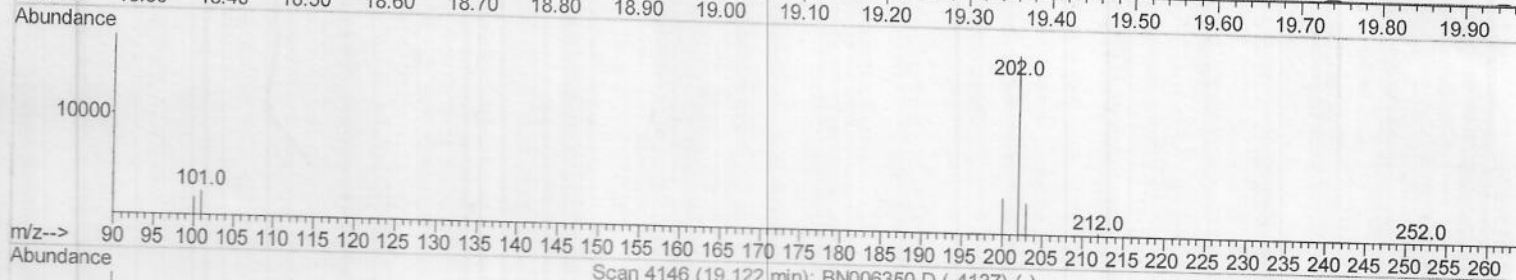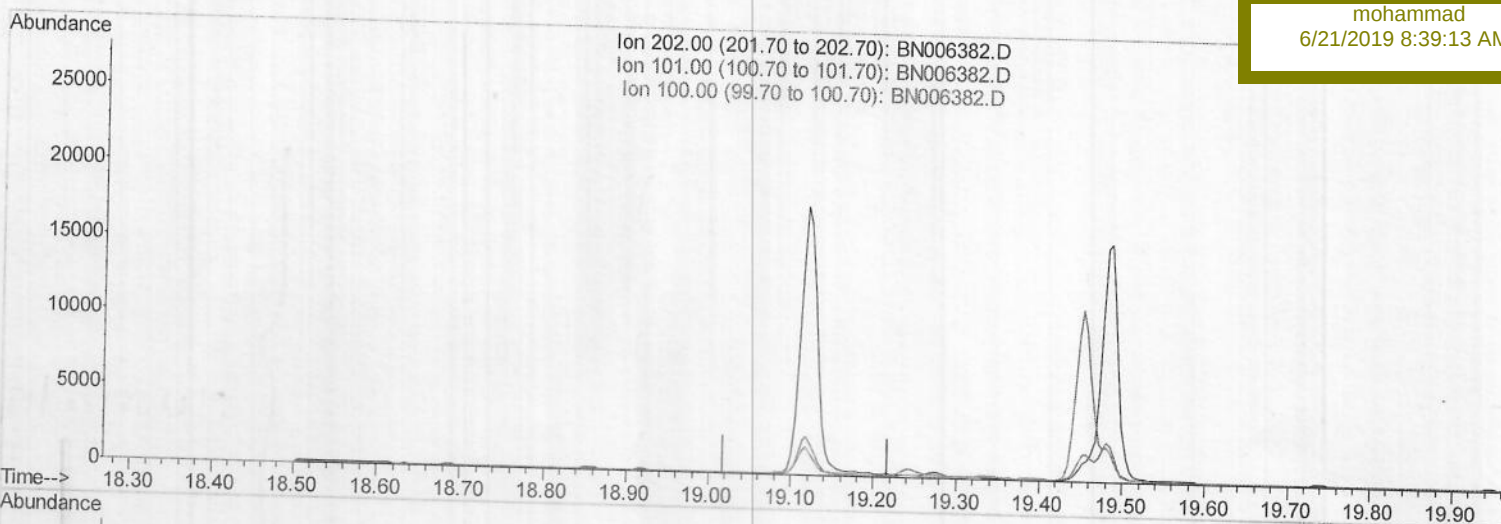

(15) Fluoranthene (C)

19.118min (-19.118) 0.00ng/ul

response 0

Ion	Exp%	Act%
202.00	100	0.00
101.00	12.10	0.00
100.00	8.70	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006382.D
 Acq On : 18 Jun 2019 18:25
 Operator : JU/SJ
 Sample : K3335-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Jun 19 01:35:55 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 A41T9

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:39:13 AM

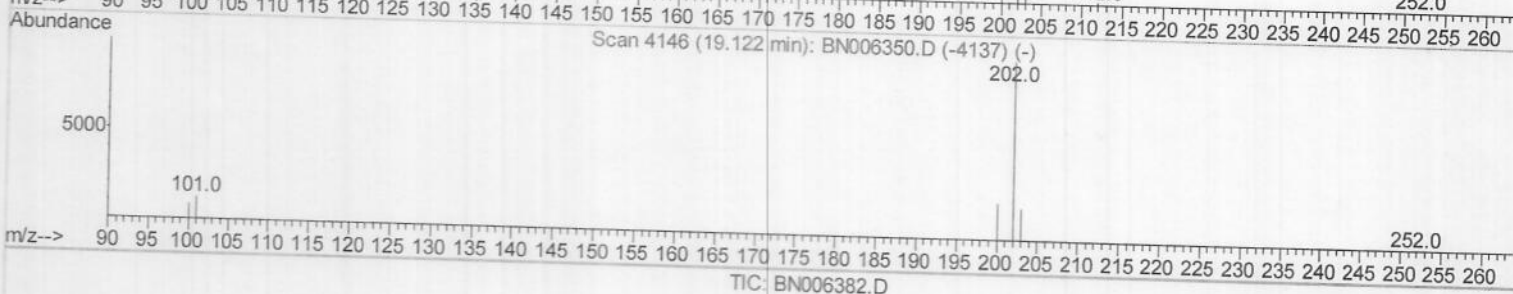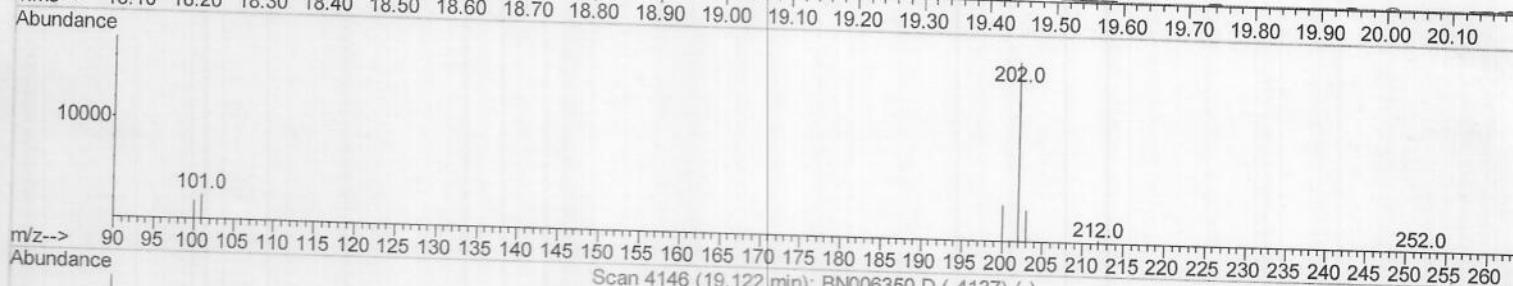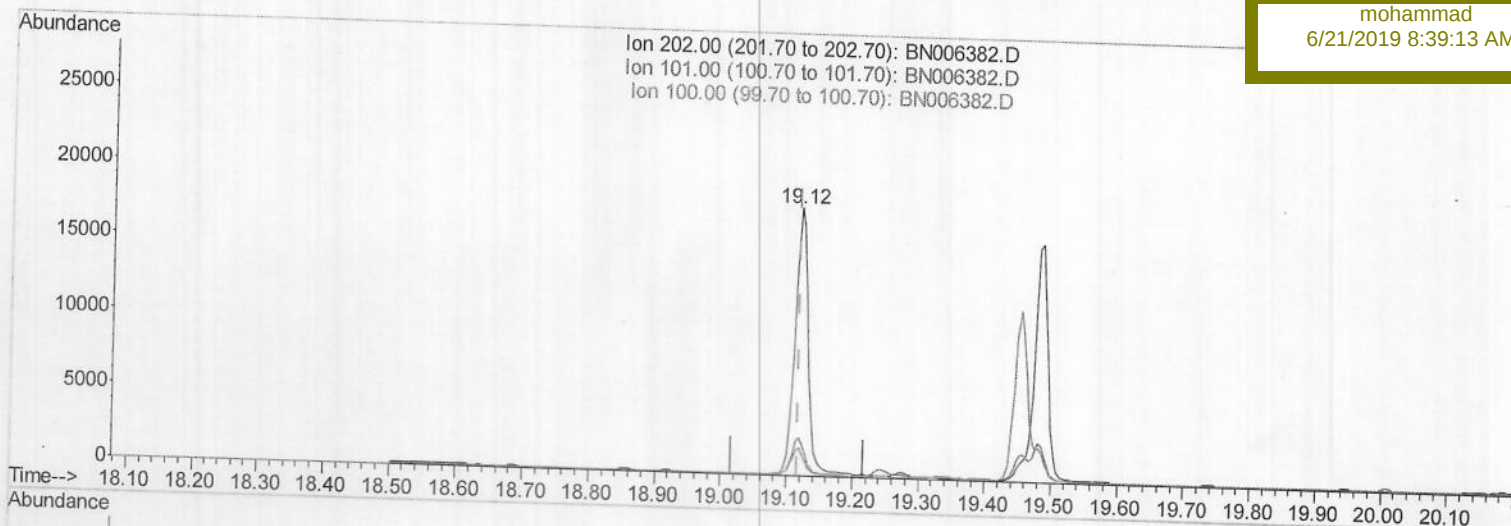

(15) Fluoranthene (C)

19.118min (-0.000) 0.51ng/ul m

response 24677

Ion	Exp%	Act%
202.00	100	100
101.00	12.10	14.01
100.00	8.70	10.28
0.00	0.00	0.00

> JU 06/25/19

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
Data File : BN006382.D

Acq On : 18 Jun 2019 18:25

Operator : JU/SJ

Sample : K3335-03

Misc :

ALS Vial : 14 Sample Multiplier: 1

Quant Time: Jun 19 01:35:55 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A41T9

Manual Integrations

APPROVED

mohammad

6/21/2019 8:39:13 AM

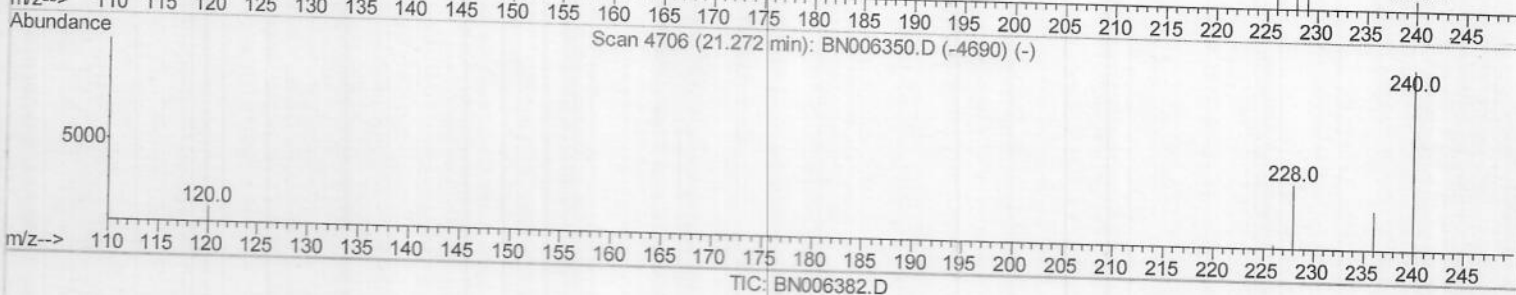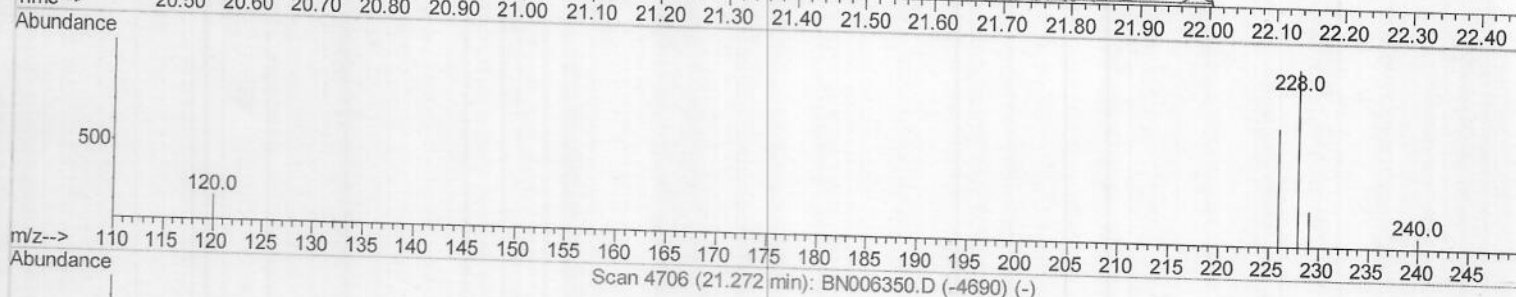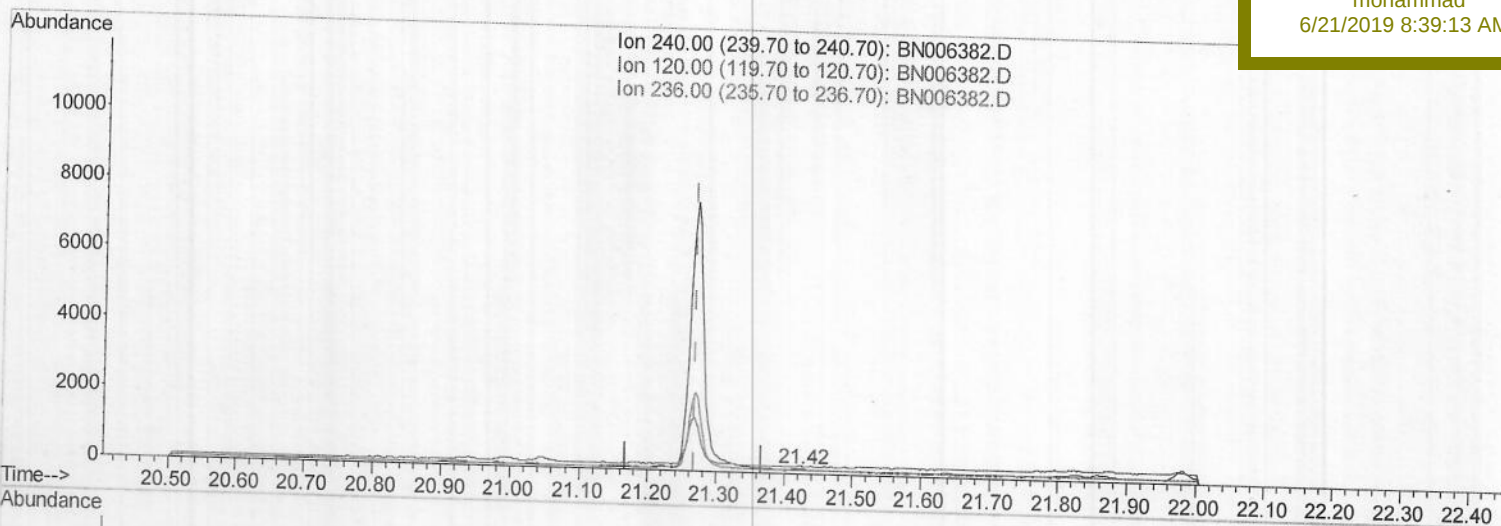

(16) Chrysene-d12 (I)

21.425min (+0.157) 0.40ng/ul

response 76

Ion	Exp%	Act%
240.00	100	100
120.00	20.10	145.22#
236.00	30.10	65.61#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006382.D
 Acq On : 18 Jun 2019 18:25
 Operator : JU/SJ
 Sample : K3335-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :

BNA_N

ClientSampleId :

A41T9




Manual Integrations

APPROVED

mohammad

6/21/2019 8:39:13 AM

Quant Time: Jun 19 01:35:55 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

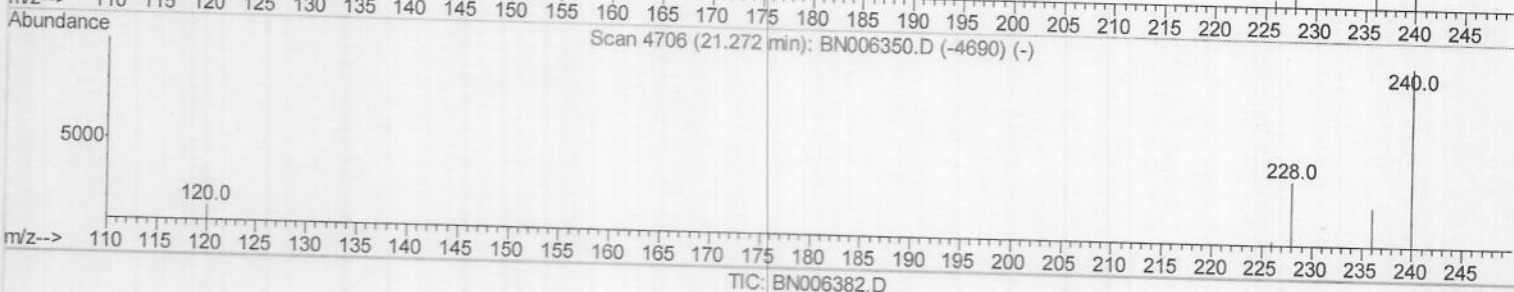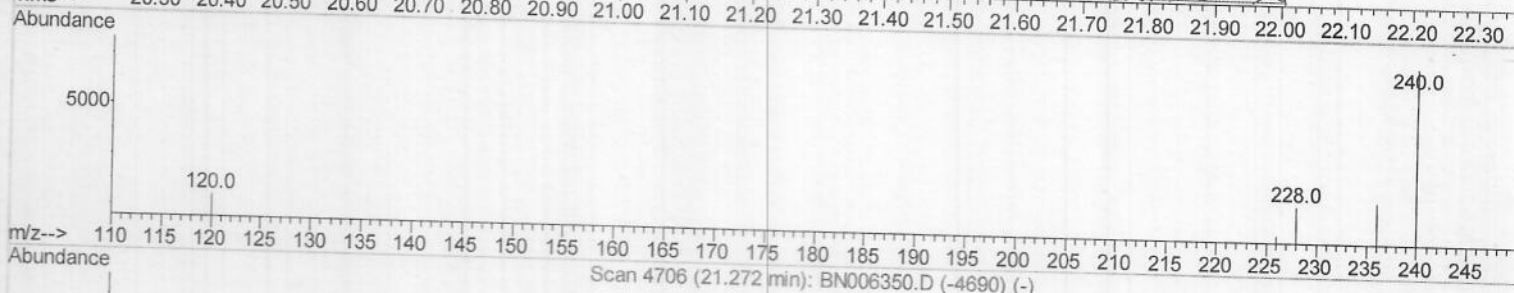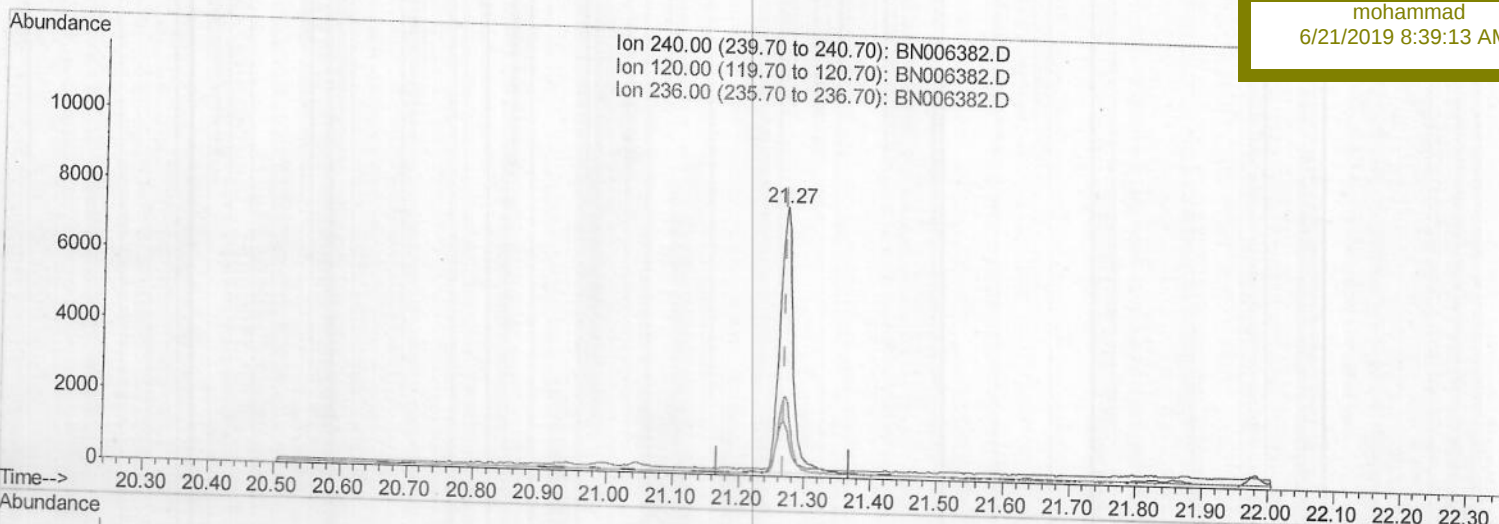

(16) Chrysene-d12 (I)

21.270min (+0.002) 0.40ng/ul m > JU 06/25/19

response 10606

Ion	Exp%	Act%
240.00	100	100
120.00	20.10	18.84
236.00	30.10	29.03
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006382.D
 Acq On : 18 Jun 2019 18:25
 Operator : JU/SJ
 Sample : K3335-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Jun 19 01:37:36 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 OLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 A41T9

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:39:13 AM

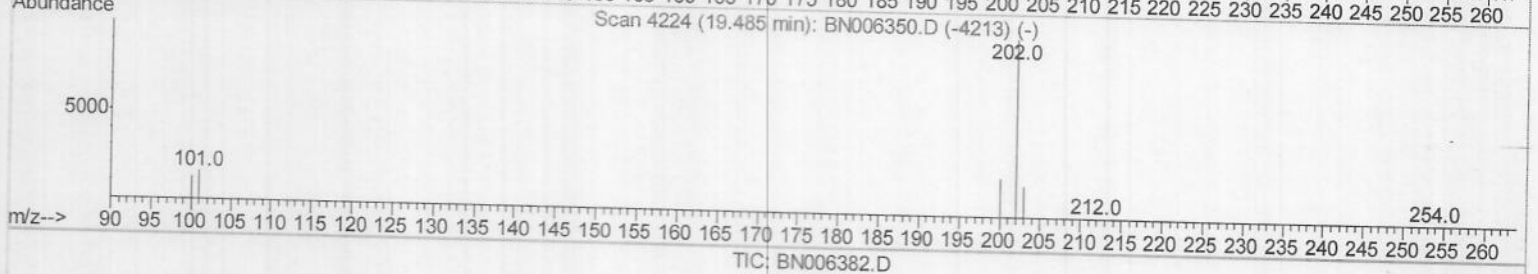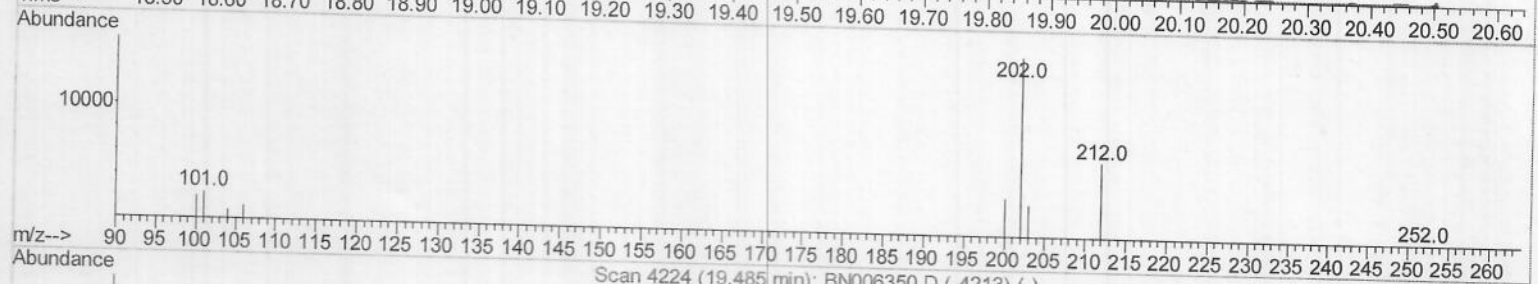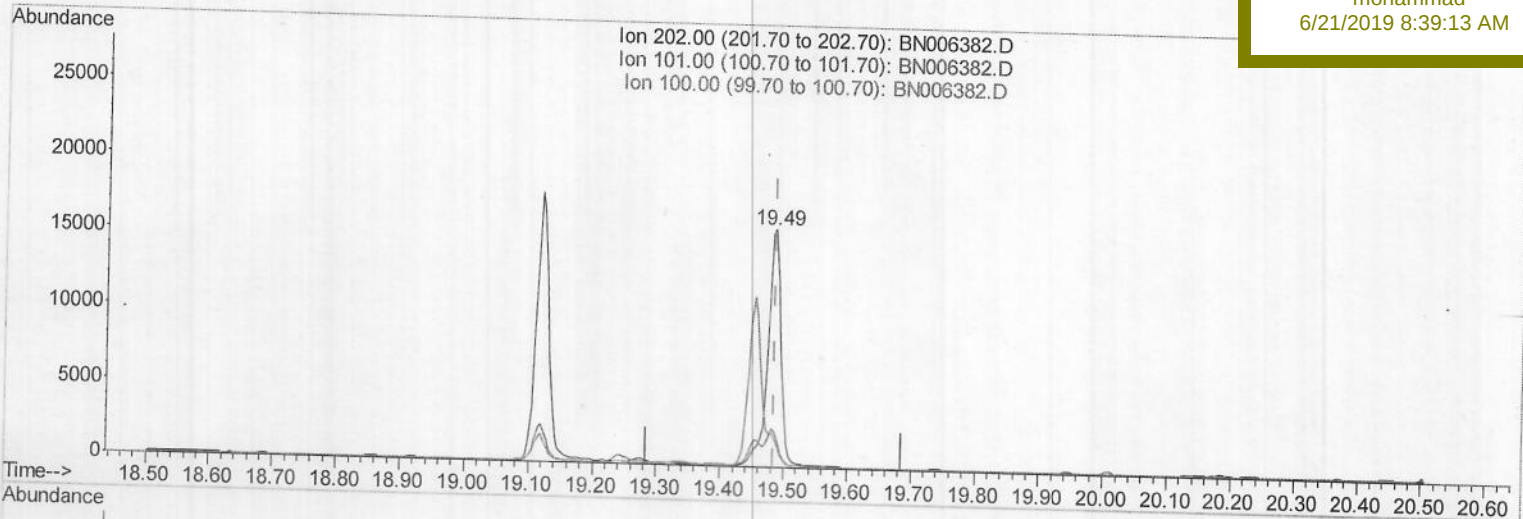

TIC: BN006382.D

(17) Pyrene

19.485min (-0.000) 0.41ng/ul

response 22915

Ion	Exp%	Act%
202.00	100	100
101.00	15.20	15.03
100.00	12.20	12.35
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
Data File : BN006382.D

Acq On : 18 Jun 2019 18:25

Operator : JU/SJ

Sample : K3335-03

Misc :

ALS Vial : 14 Sample Multiplier: 1

Quant Time: Jun 19 01:37:36 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N




ClientSampleId :

A41T9

Manual Integrations
APPROVED

mohammad

6/21/2019 8:39:13 AM

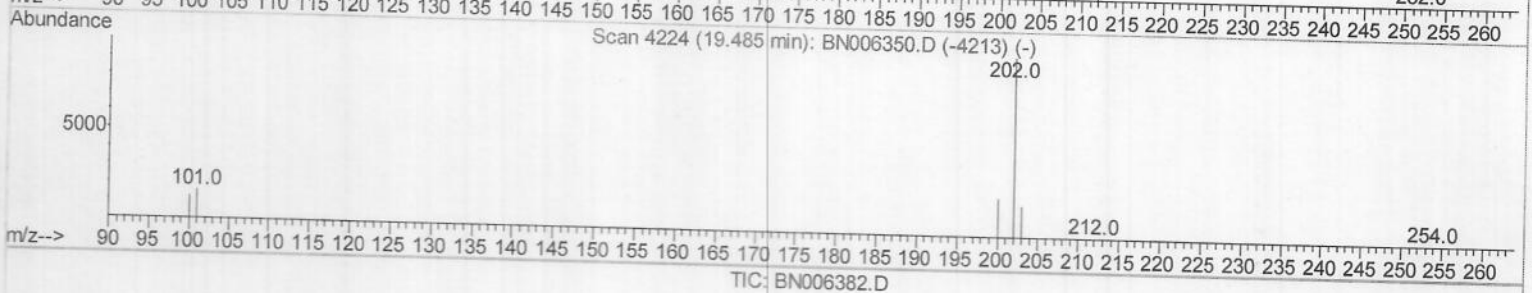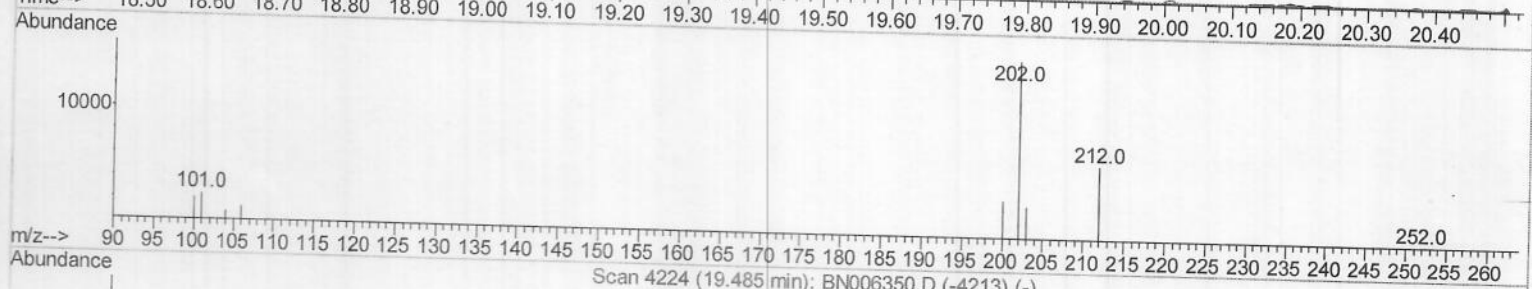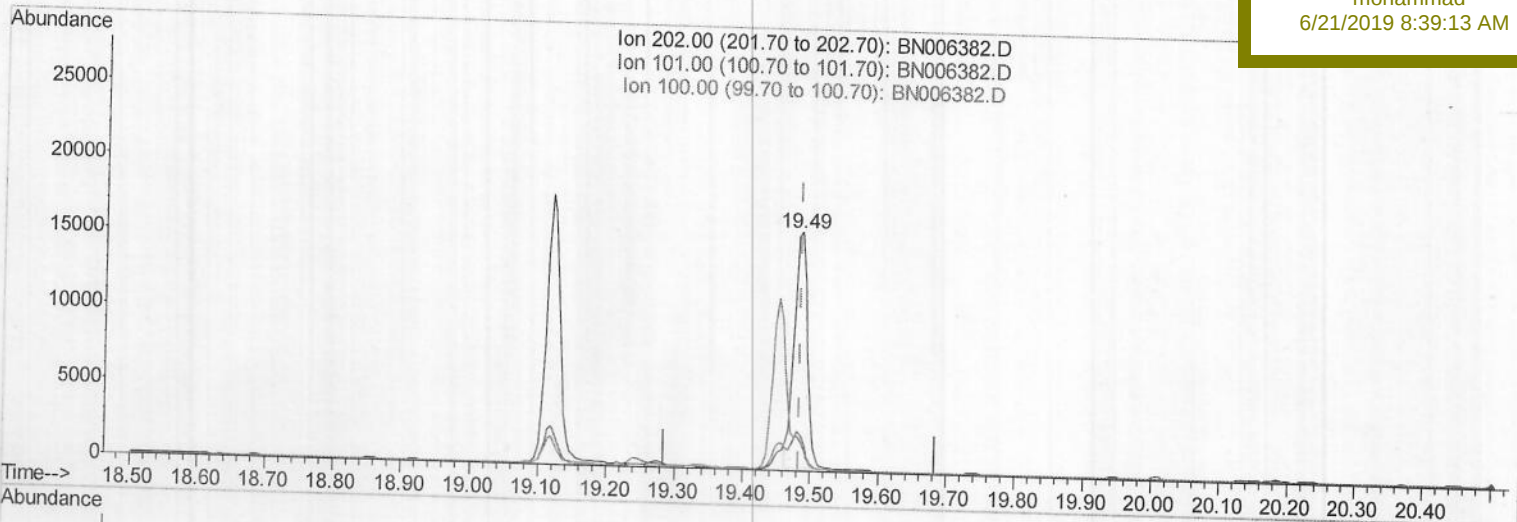

(17) Pyrene

19.485min (-0.000) 0.38ng/ul m

> JU 06/25/19

response 20997

Ion	Exp%	Act%
202.00	100	100
101.00	15.20	15.03
100.00	12.20	12.35
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006382.D
 Acq On : 18 Jun 2019 18:25
 Operator : JU/SJ
 Sample : K3335-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Jun 19 01:37:36 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 A41T9

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:39:13 AM

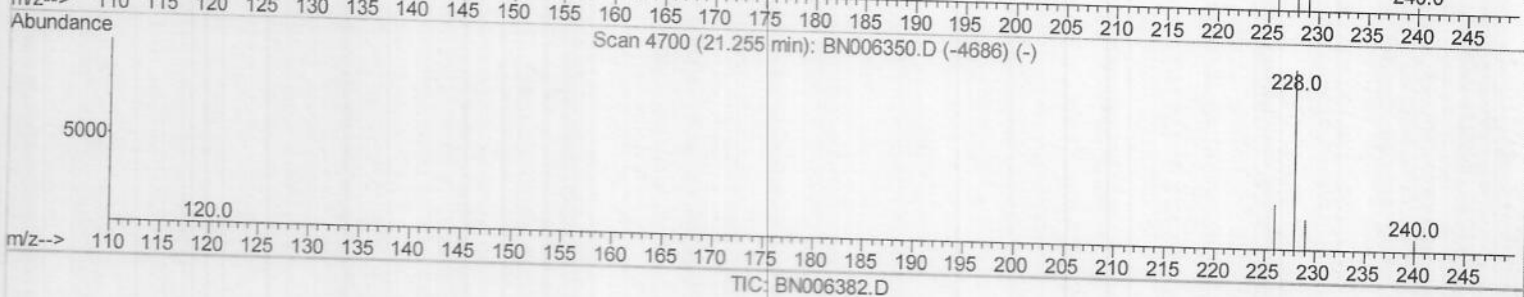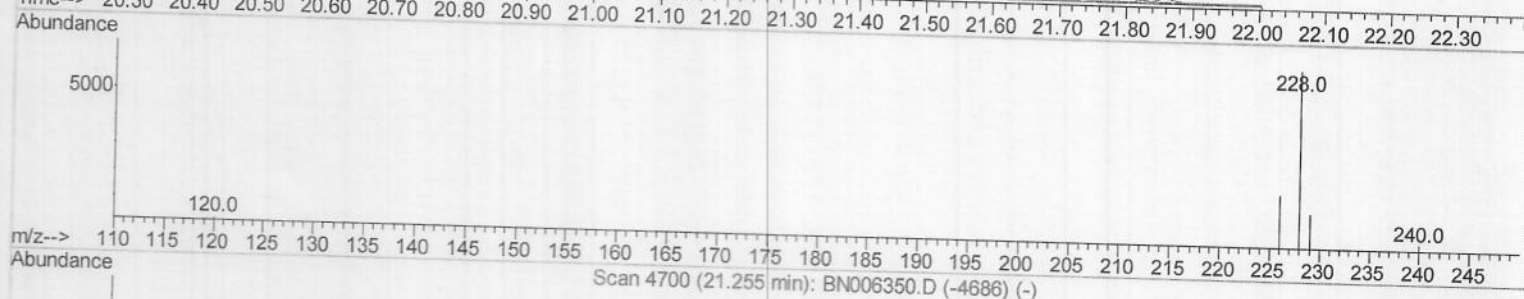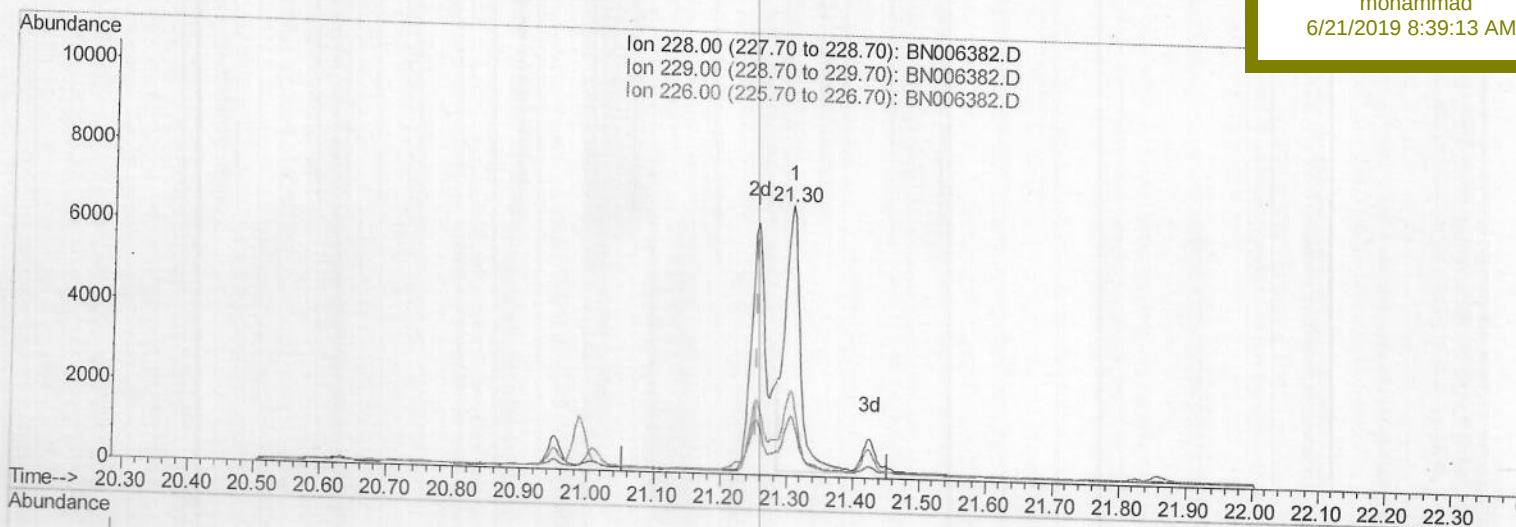

(18) Benzo(a)anthracene
 21.305min (+0.051) 0.23ng/ul
 response 10988

Ion	Exp%	Act%
228.00	100	100
229.00	20.60	22.10
226.00	28.50	31.91
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006382.D
 Acq On : 18 Jun 2019 18:25
 Operator : JU/SJ
 Sample : K3335-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Jun 19 01:37:36 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 A41T9

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:39:13 AM

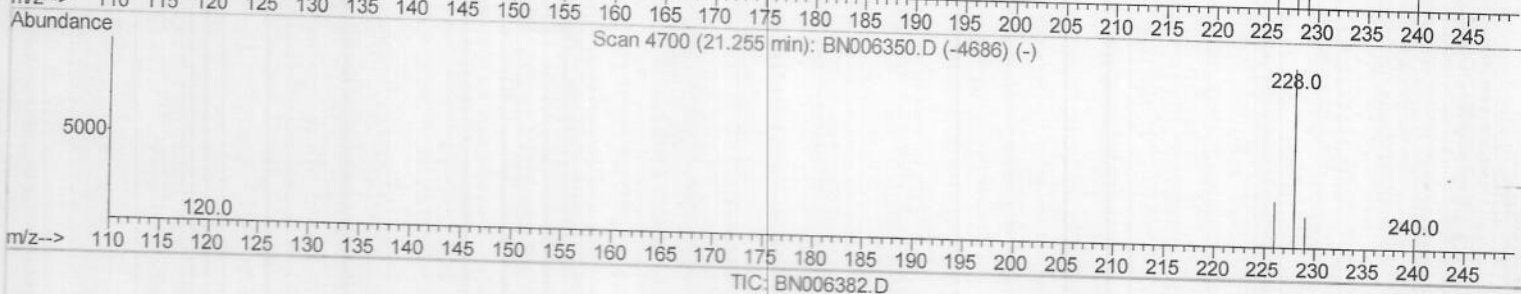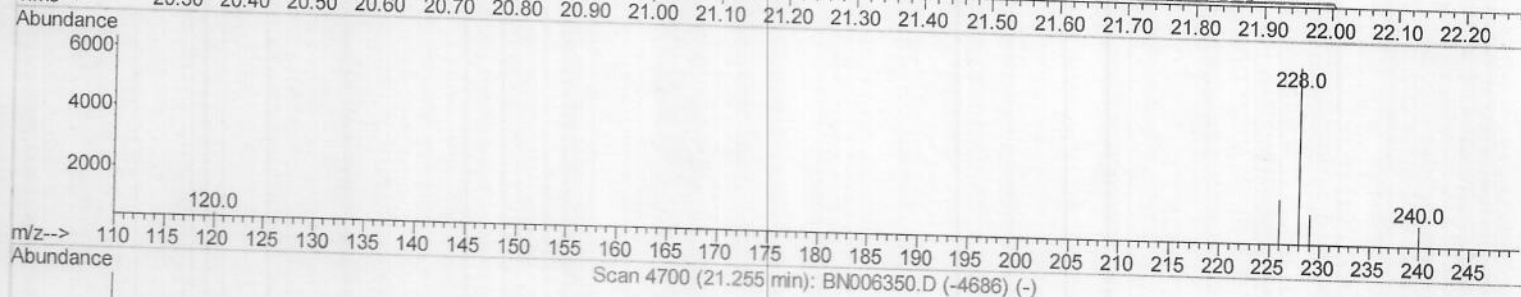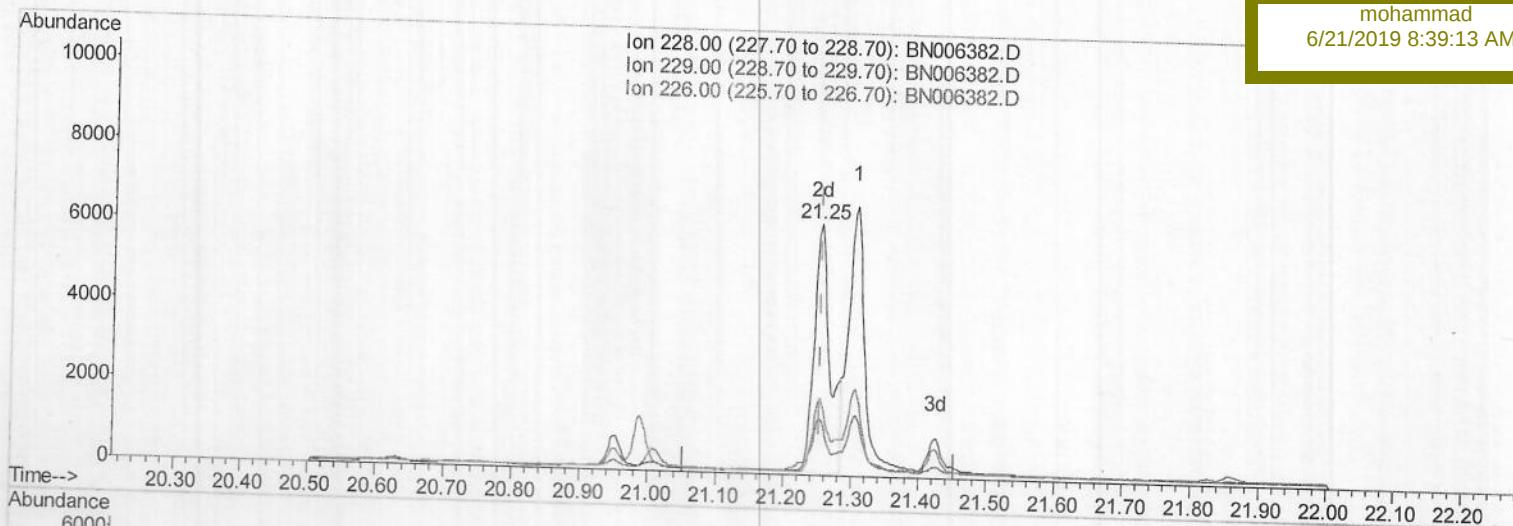

(18) Benzo(a)anthracene

21.252min (-0.001) 0.22ng/ul m > JU 06/25/19

response 10138

Ion	Exp%	Act%
228.00	100	100
229.00	20.60	21.82
226.00	28.50	30.11
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006382.D
 Acq On : 18 Jun 2019 18:25
 Operator : JU/SJ
 Sample : K3335-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A41T9

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:39:13 AM

Quant Time: Jun 19 01:37:36 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

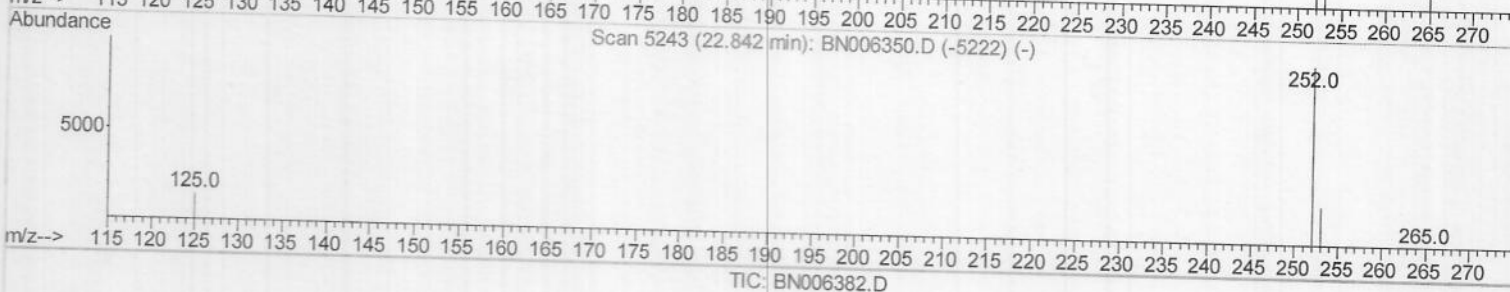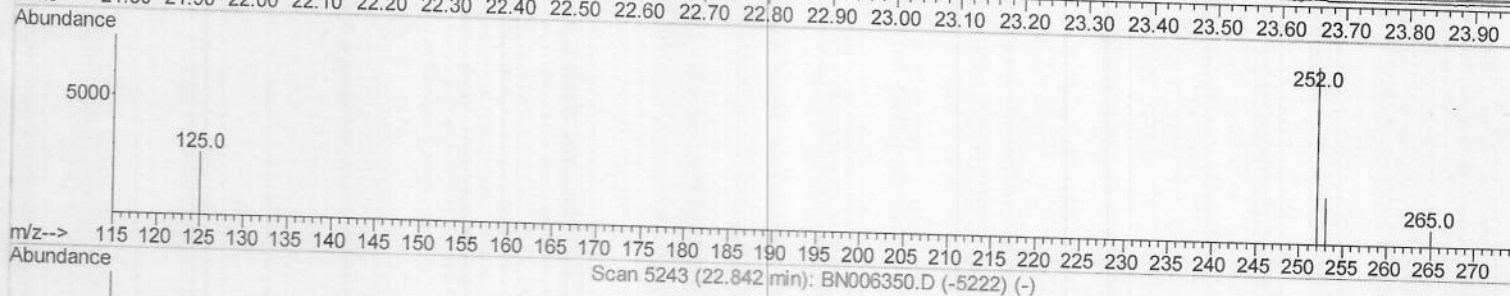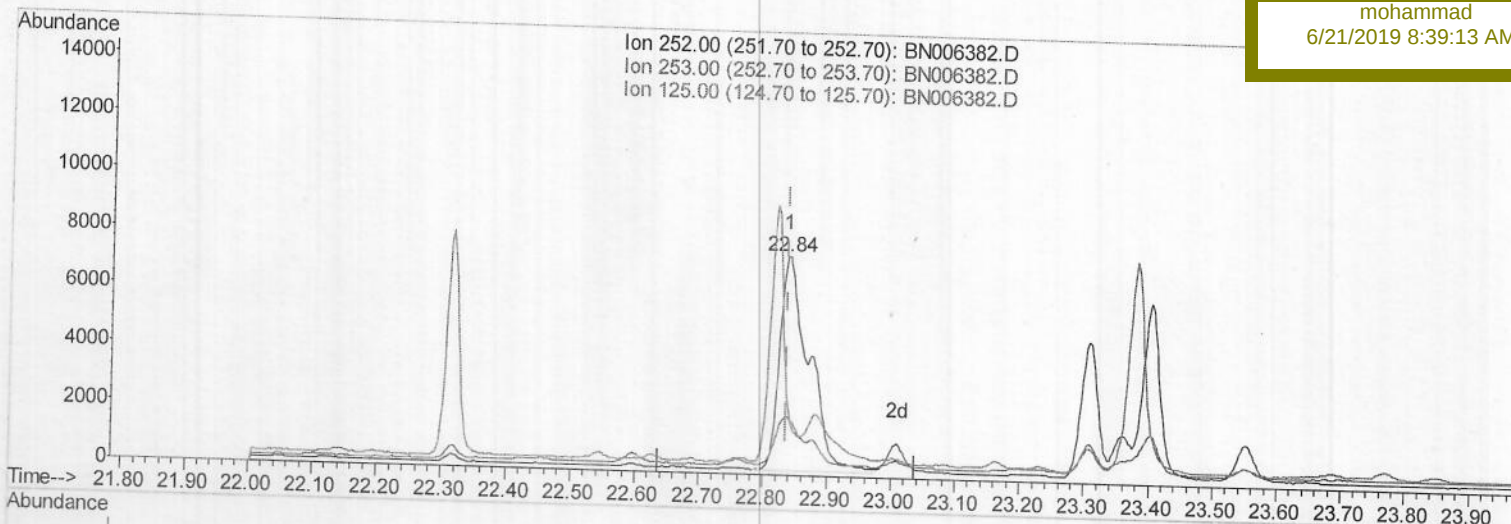

(21) Benzo(b)fluoranthene
 22.836min (-0.001) 0.33ng/ul
 response 23194

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	26.84
125.00	20.50	35.39
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006382.D
 Acq On : 18 Jun 2019 18:25
 Operator : JU/SJ
 Sample : K3335-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A41T9

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:39:13 AM

Quant Time: Jun 19 01:37:36 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

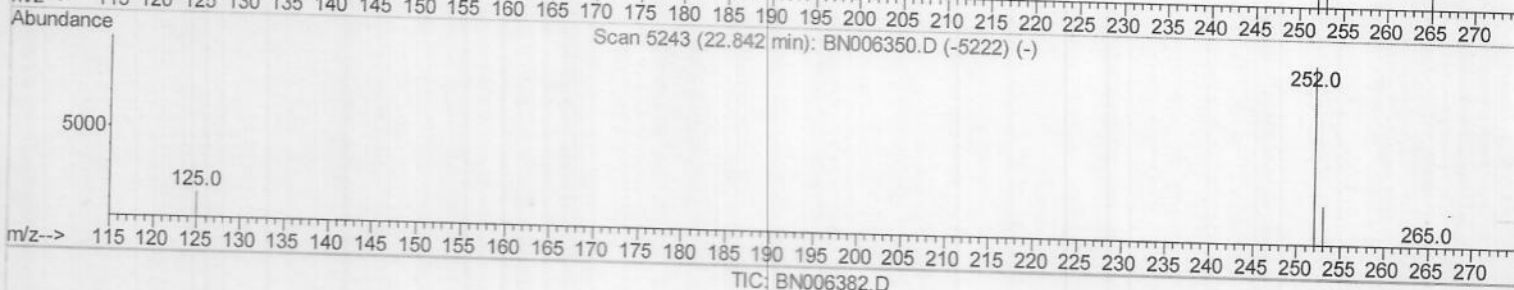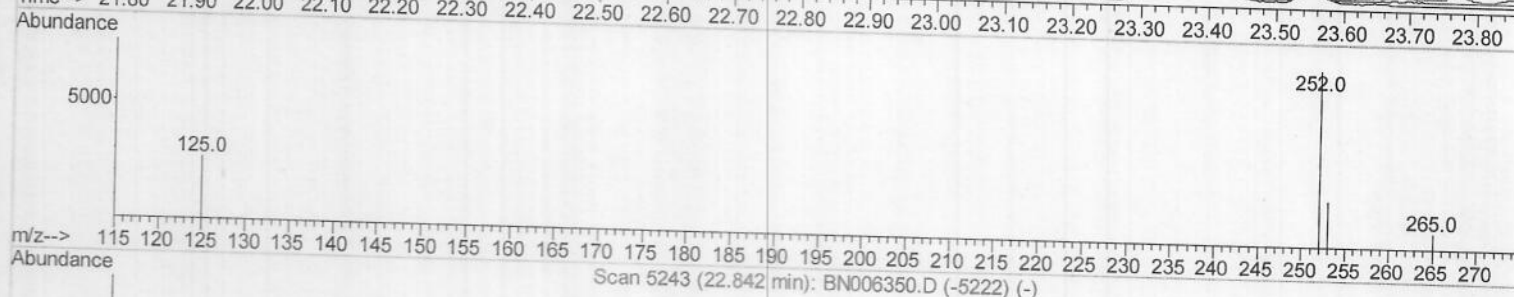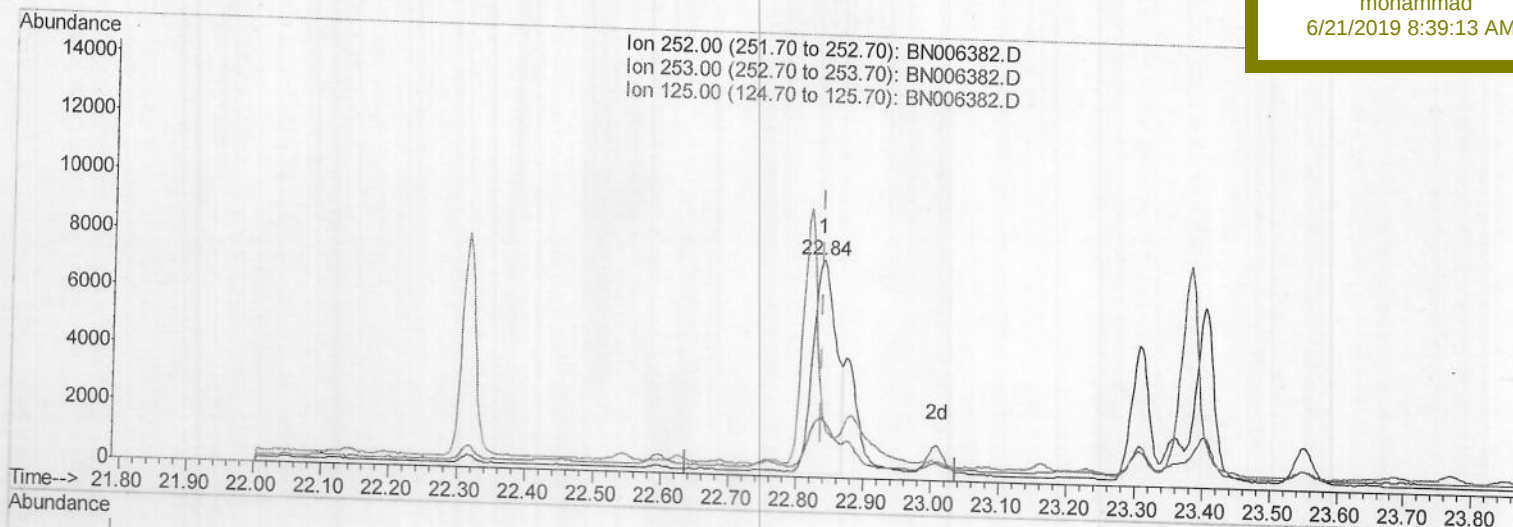

(21) Benzo(b)fluoranthene

22.836min (-0.001) 0.24ng/ul m -> JU 06/25/19

response 17201

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	26.84
125.00	20.50	35.39
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006382.D
 Acq On : 18 Jun 2019 18:25
 Operator : JU/SJ
 Sample : K3335-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A41T9

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:39:13 AM

Quant Time: Jun 19 01:37:36 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

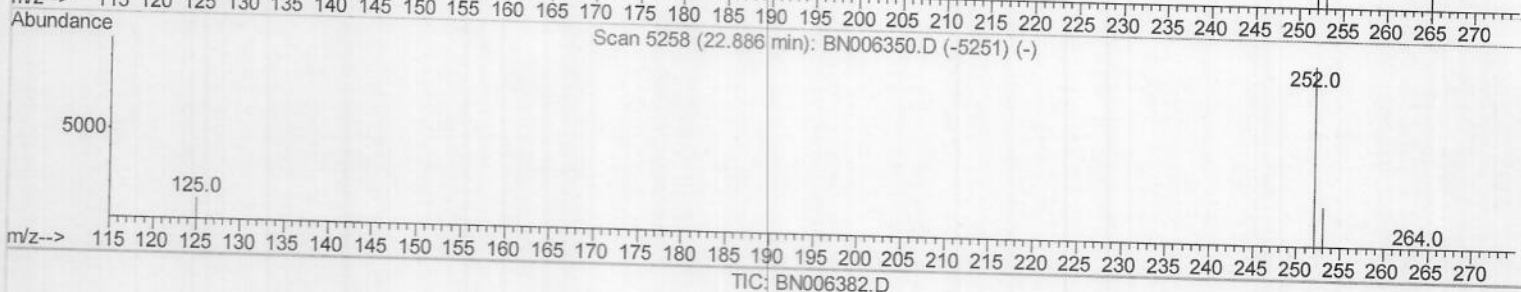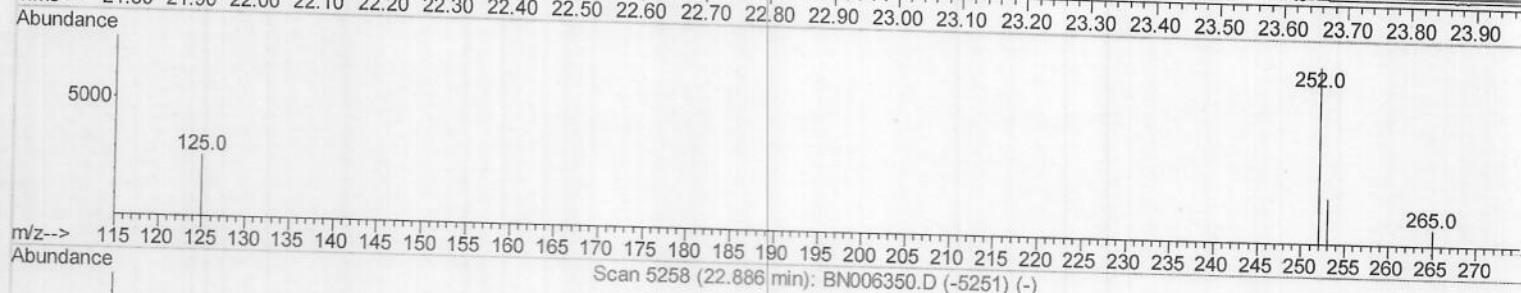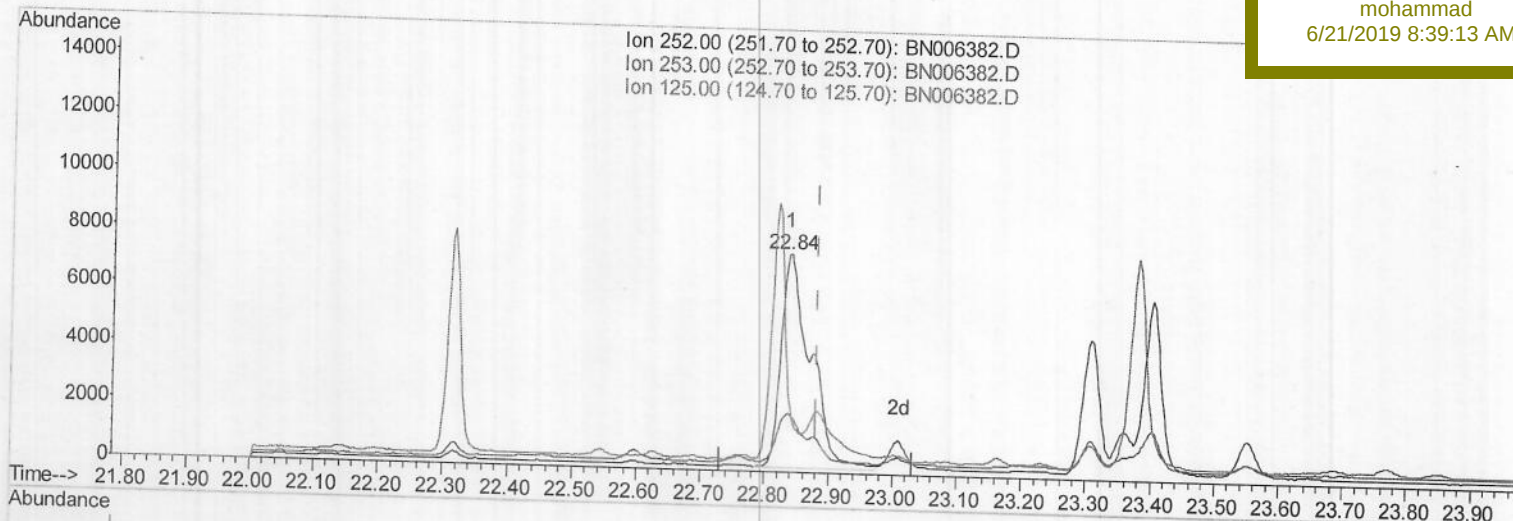

(22) Benzo(k)fluoranthene
 22.836min (-0.045) 0.34ng/ul
 response 23194

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	26.84
125.00	17.90	35.39#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006382.D
 Acq On : 18 Jun 2019 18:25
 Operator : JU/SJ
 Sample : K3335-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 A41T9

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:39:13 AM

Quant Time: Jun 19 01:37:36 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

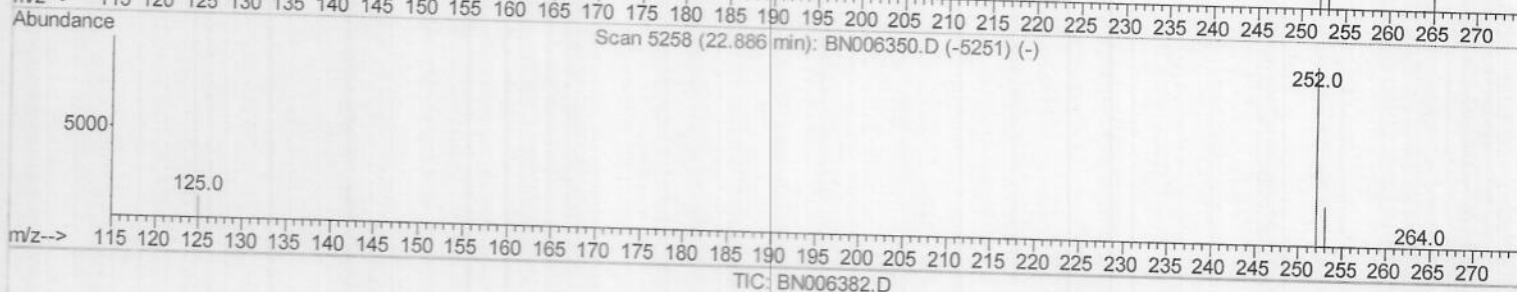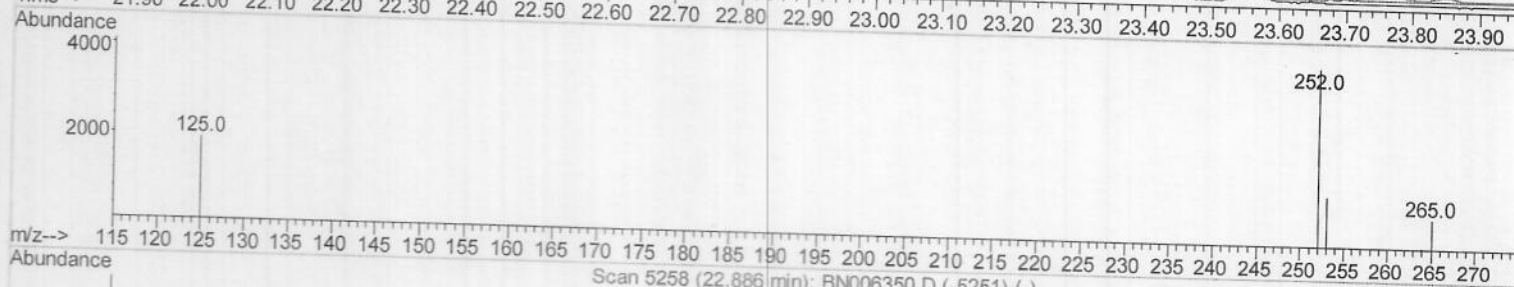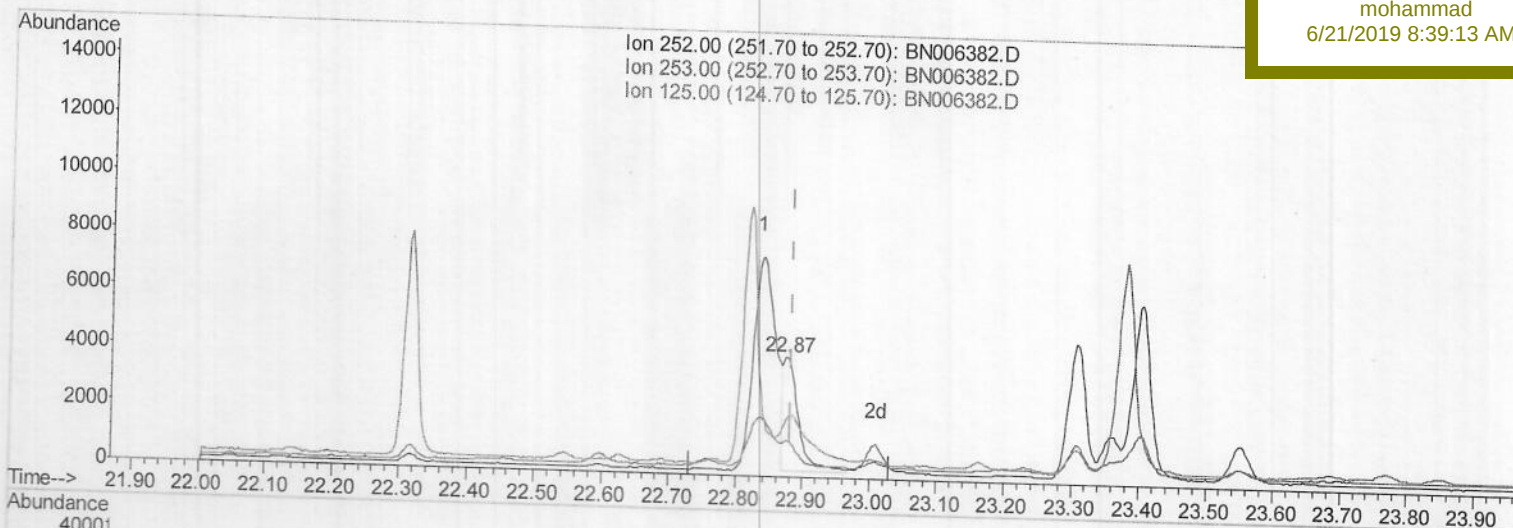

(22) Benzo(k)fluoranthene

22.874min (-0.007) 0.09ng/ul m & JU 06/25/19

response 6062

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	29.53
125.00	17.90	46.76#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006382.D
 Acq On : 18 Jun 2019 18:25
 Operator : JU/SJ
 Sample : K3335-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 Client Sample Id :
 A41T9

Quant Time: Jun 19 01:39:42 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:39:13 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	3699	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	13888	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.29	164	7112	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	13652m	0.40	ng/ul	0.00
16) Chrysene-d12	21.27	240	10606m	0.40	ng/ul	0.00
20) Perylene-d12	23.50	264	16932	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	3944	0.19	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	8311m	0.23	ng/ul	0.00
Target Compounds						
12) Phenanthrene	17.09	178	8202	0.187	ng/ul	97
13) Anthracene	17.18	178	1567m	0.037	ng/ul	
15) Fluoranthene	19.12	202	24677m	0.510	ng/ul	98
17) Pyrene	19.49	202	20997m	0.376	ng/ul	
18) Benzo(a)anthracene	21.25	228	10138m	0.216	ng/ul	97
19) Chrysene	21.30	228	10435	0.237	ng/ul	
21) Benzo(b)fluoranthene	22.84	252	17201m	0.244	ng/ul	86
22) Benzo(k)fluoranthene	22.87	252	6062m	0.088	ng/ul	
23) Benzo(a)pyrene	23.40	252	10976	0.167	ng/ul	64
24) Indeno(1,2,3-cd)pyrene	25.74	276	7762	0.109	ng/ul#	
25) Dibenzo(a,h)anthracene	25.74	278	1703	0.030	ng/ul#	99
26) Benzo(g,h,i)perylene	26.42	276	7816	0.131	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU
 06/25/19