

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\

Data File : BN006383.D

Acq On : 18 Jun 2019 18:59

Operator : JU/SJ

Sample : K3335-09

Misc :

ALS Vial : 15 Sample Multiplier: 1

Quant Time: Jun 19 01:51:16 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019


Response via : Initial Calibration

Instrument :

BNA_N

Client Sampled :

A4236

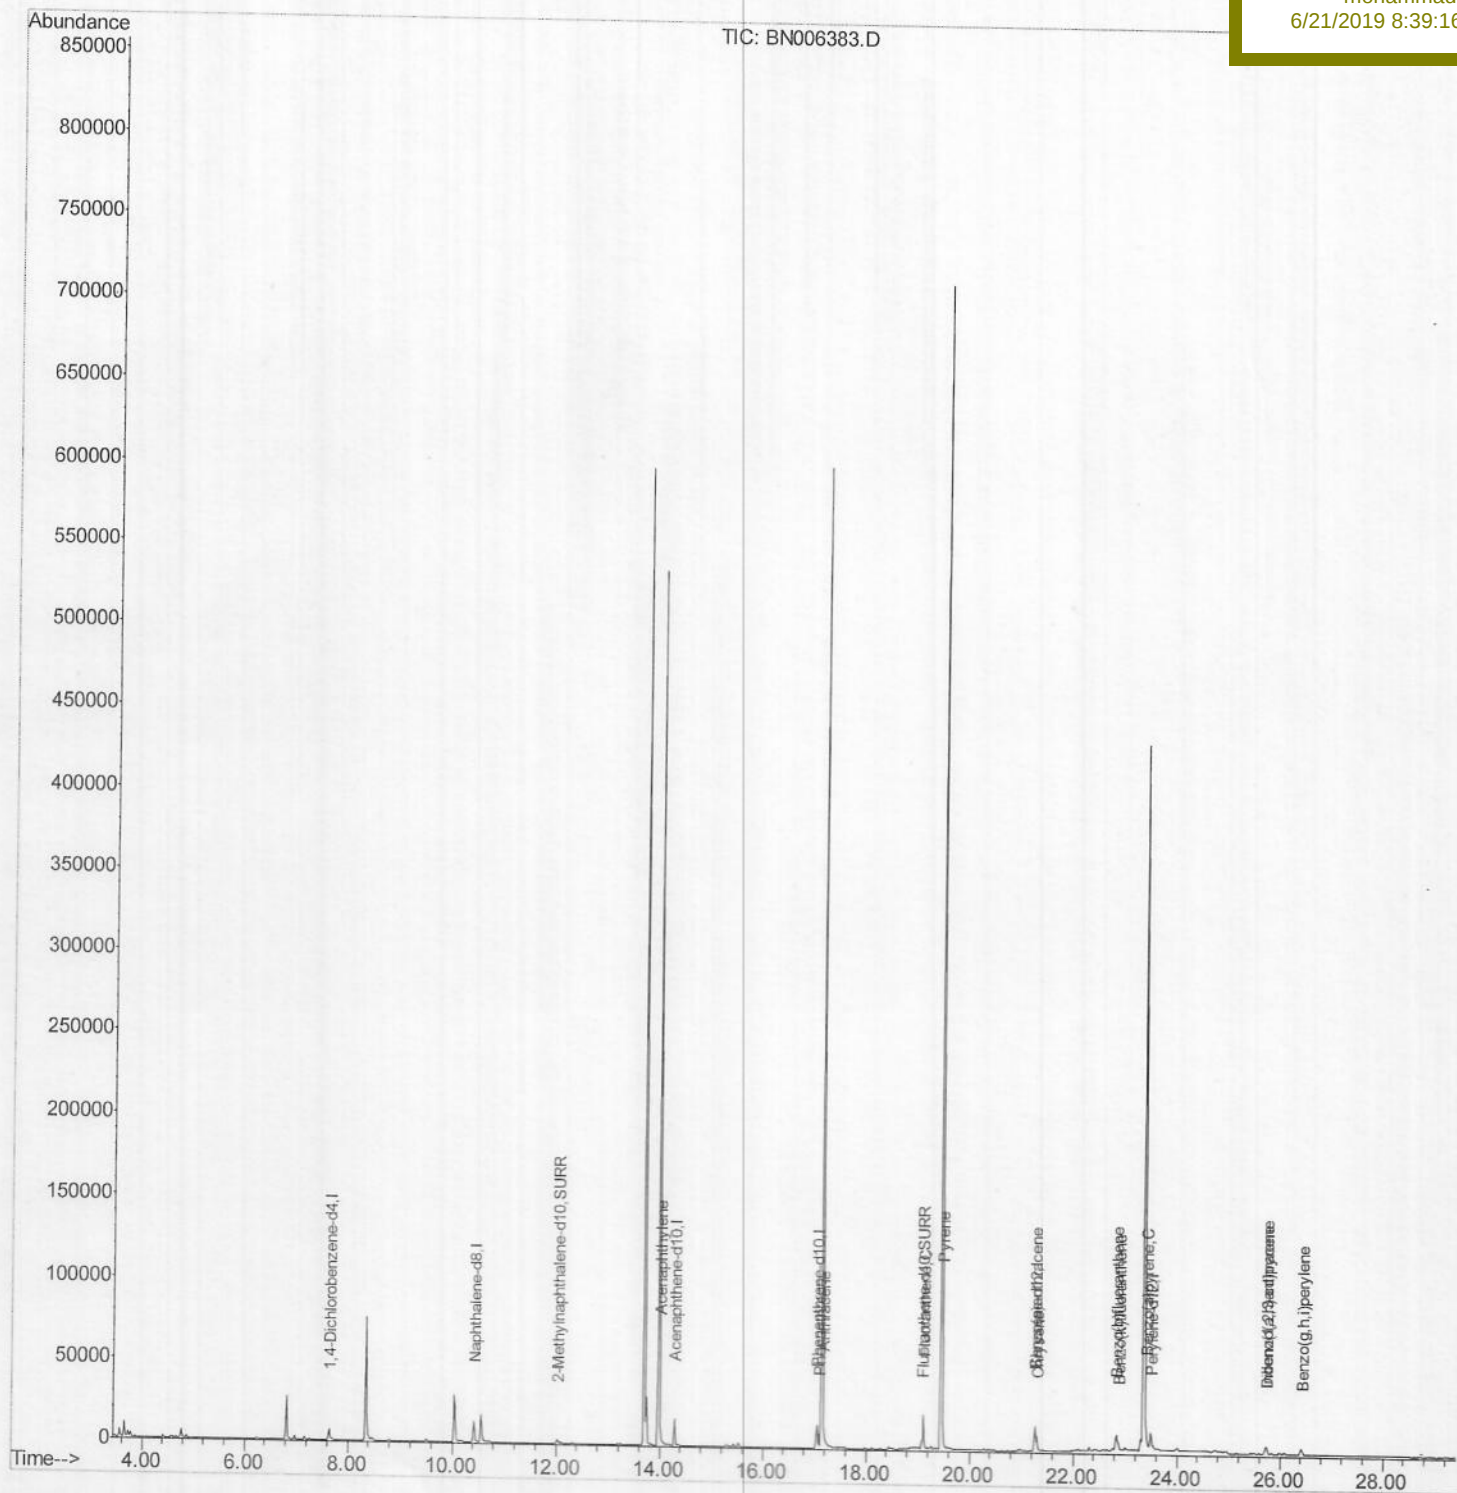Manual Integrations
APPROVEDmohammad
6/21/2019 8:39:16 AM

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\

Data File : BN006383.D

Acq On : 18 Jun 2019 18:59

Operator : JU/SJ

Sample : K3335-09

Misc :

ALS Vial : 15 Sample Multiplier: 1

Quant Time: Jun 19 01:28:54 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019




Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A4236

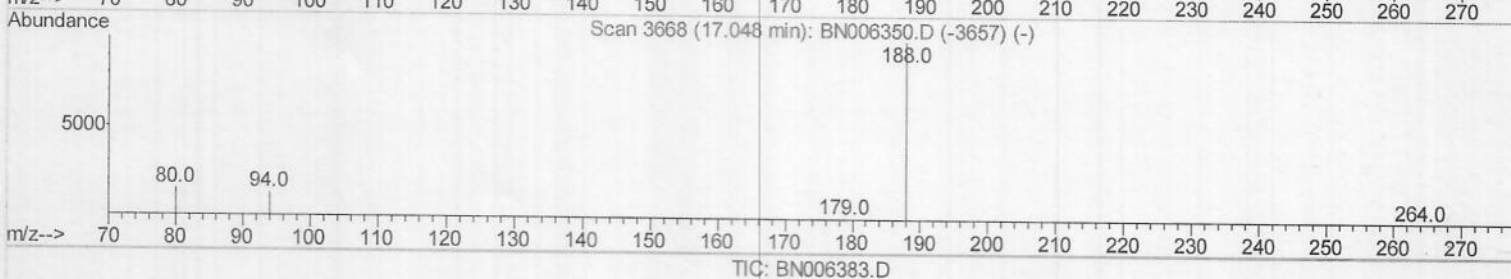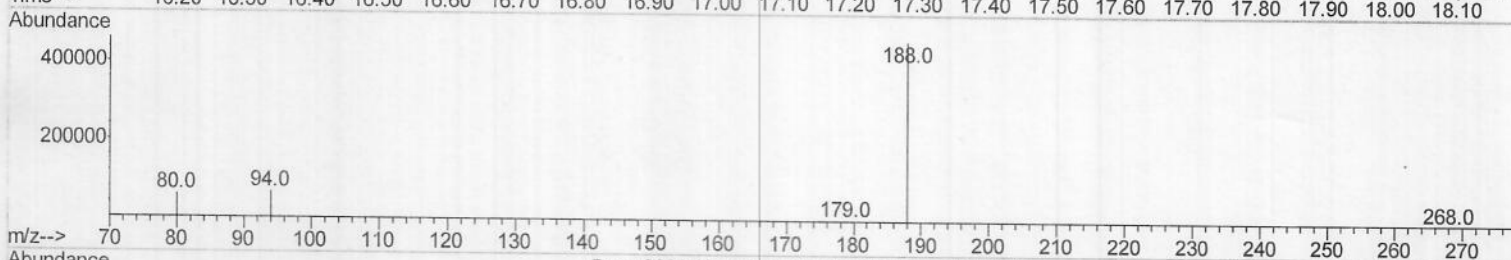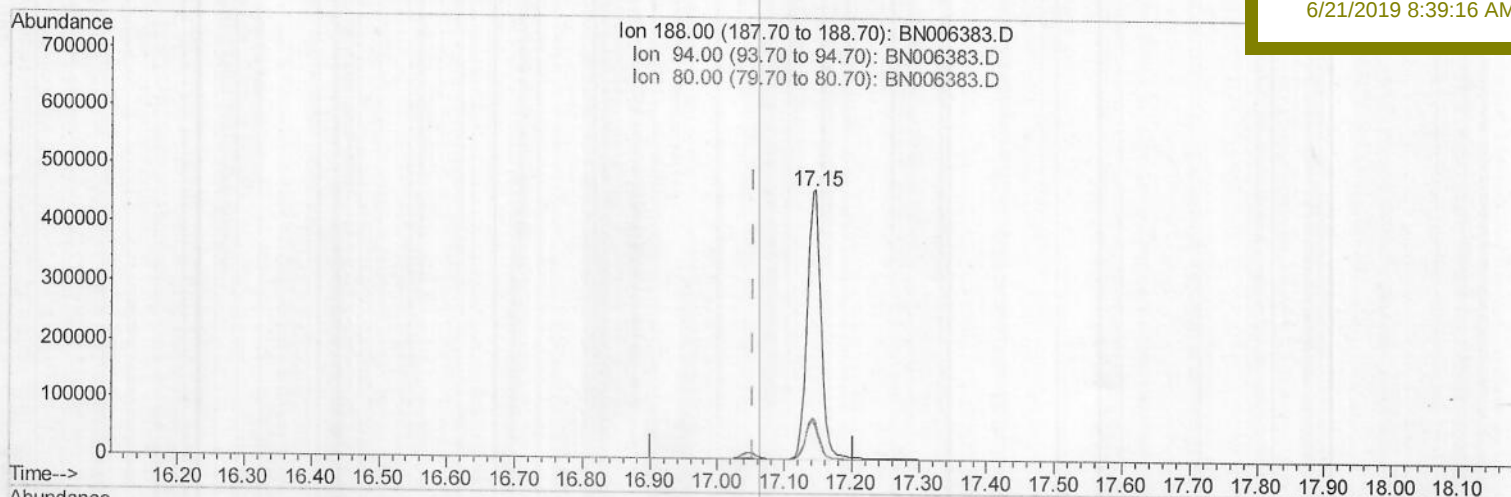Manual Integrations
APPROVEDmohammad
6/21/2019 8:39:16 AM

(10) Phenanthrene-d10 (I)

17.145min (+0.093) 0.40ng/ul

response 657255

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	14.36
80.00	13.60	12.95
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
Data File : BN006383.D
Acq On : 18 Jun 2019 18:59
Operator : JU/SJ
Sample : K3335-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Jun 19 01:28:54 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
A4236

Manual Integrations
APPROVED

mohammad
6/21/2019 8:39:16 AM

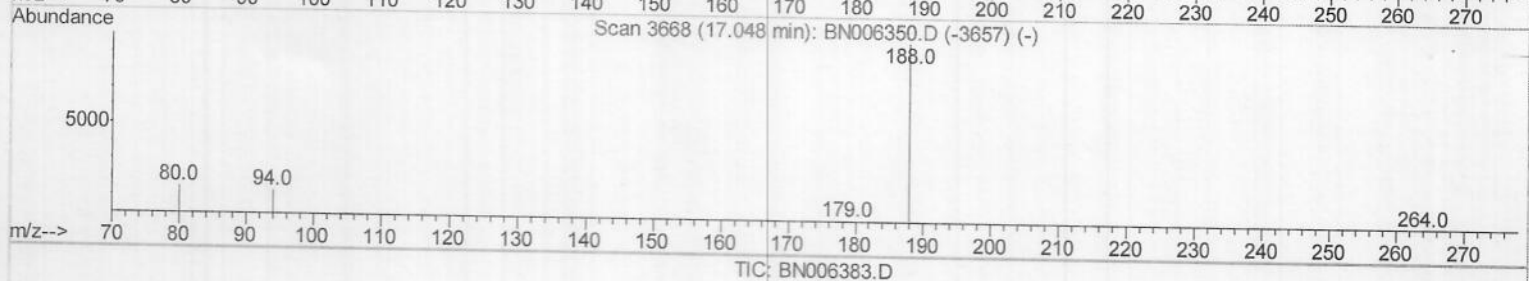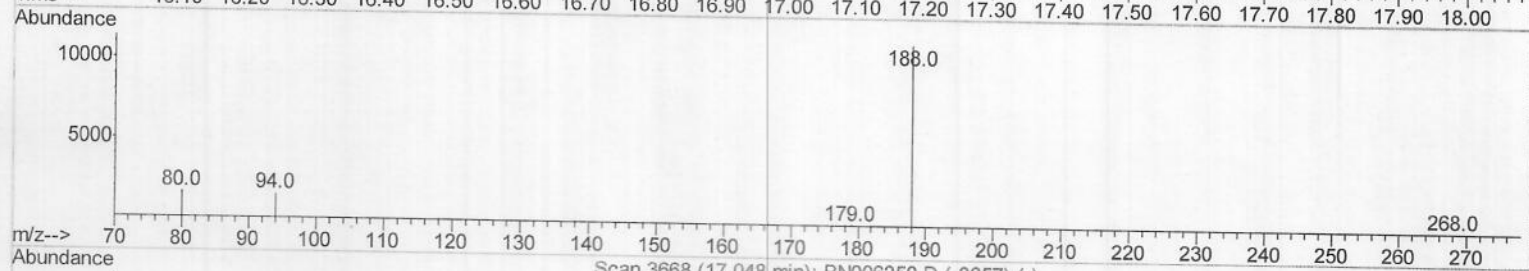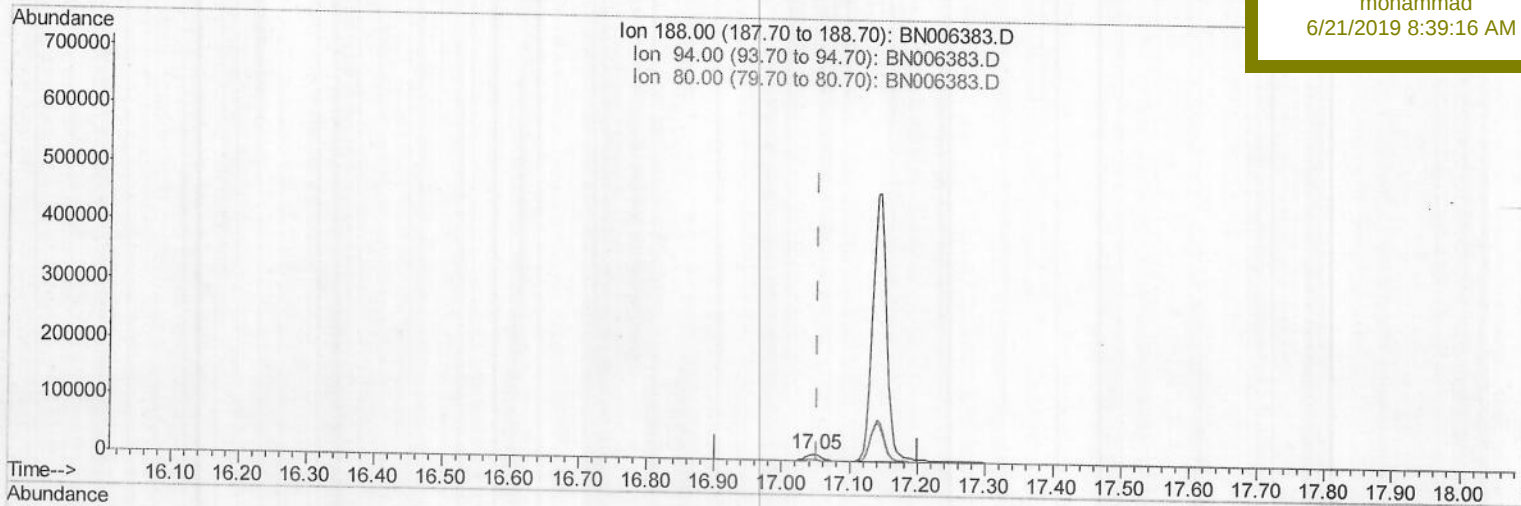

(10) Phenanthrene-d10 (I)

17.048min (-0.004) 0.40ng/ul m > JU 06/25/19

response 16698

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	13.51
80.00	13.60	14.73
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\

Data File : BN006383.D

Acq On : 18 Jun 2019 18:59

Operator : JU/SJ

Sample : K3335-09

Misc :

ALS Vial : 15 Sample Multiplier: 1

Quant Time: Jun 19 01:41:39 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A4236

Manual Integrations

APPROVED

mohammad

6/21/2019 8:39:16 AM

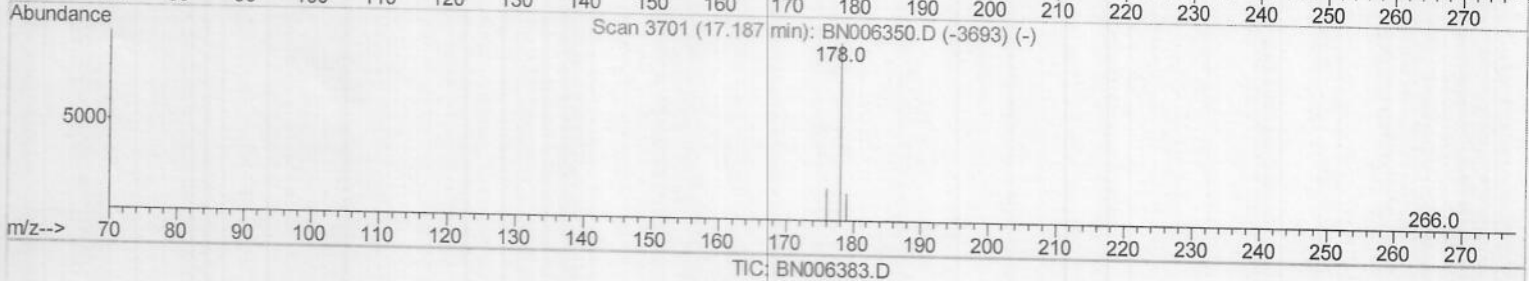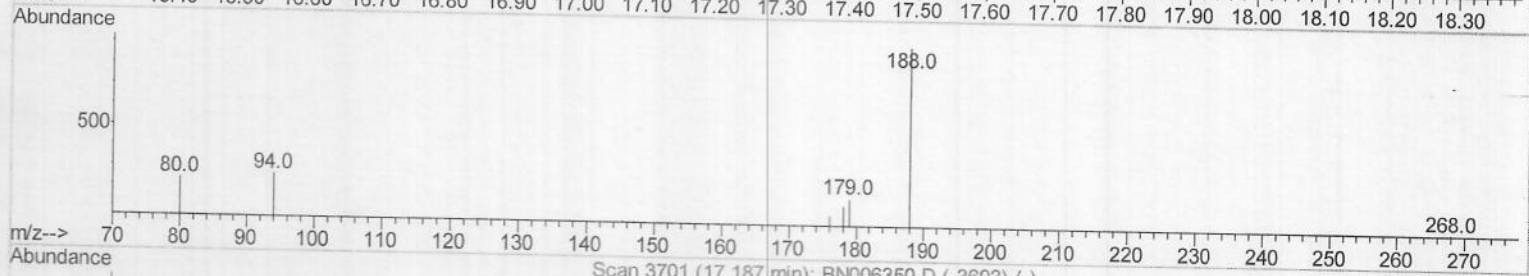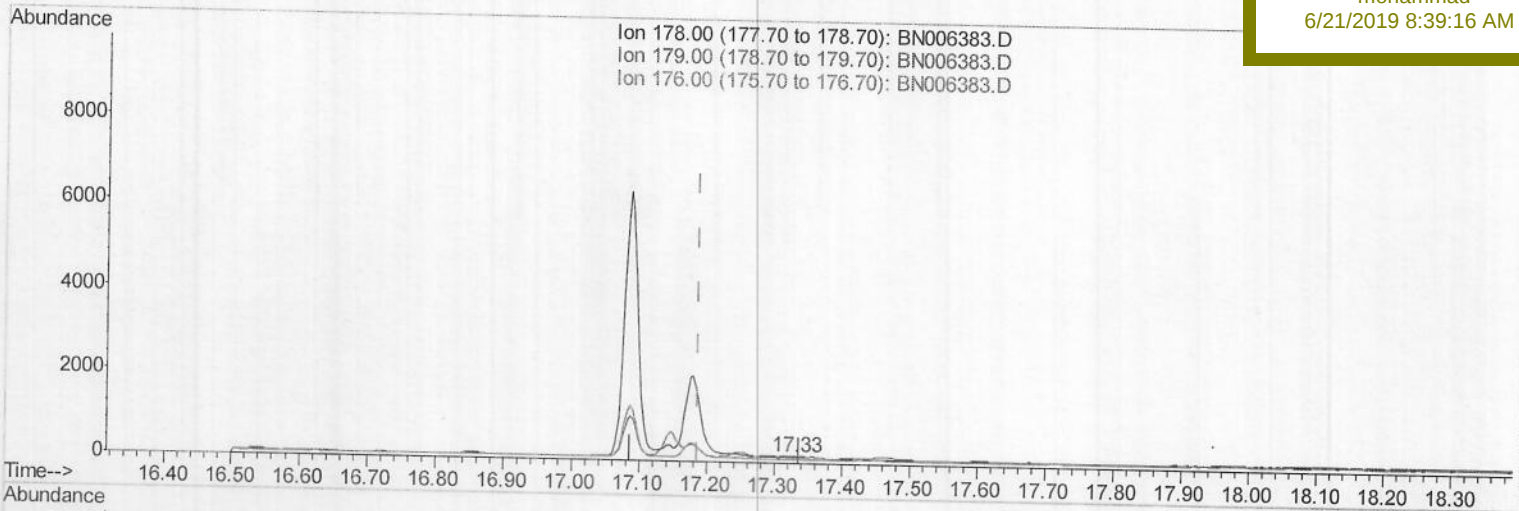

(13) Anthracene

17.331min (+0.144) 0.00ng/ul

response 90

Ion	Exp%	Act%
178.00	100	100
179.00	15.30	124.83#
176.00	18.90	65.77#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006383.D
 Acq On : 18 Jun 2019 18:59
 Operator : JU/SJ
 Sample : K3335-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Quant Time: Jun 19 01:41:39 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 A4236

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:39:16 AM

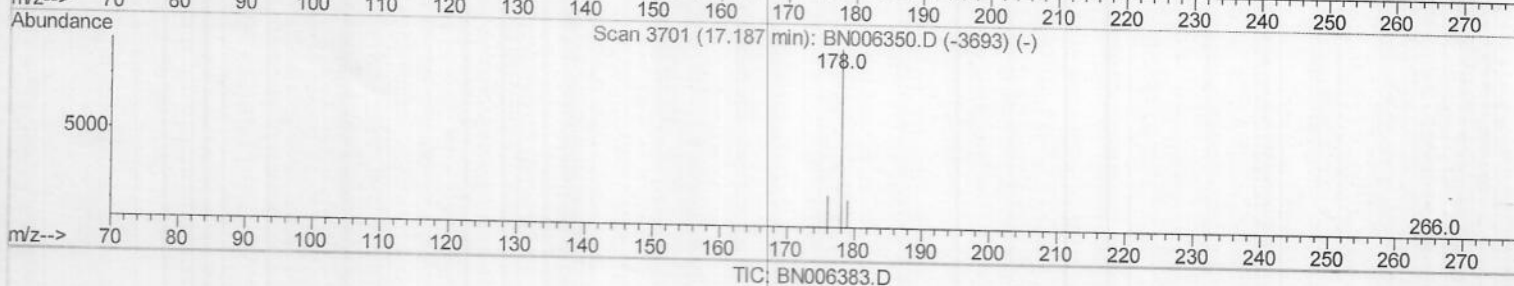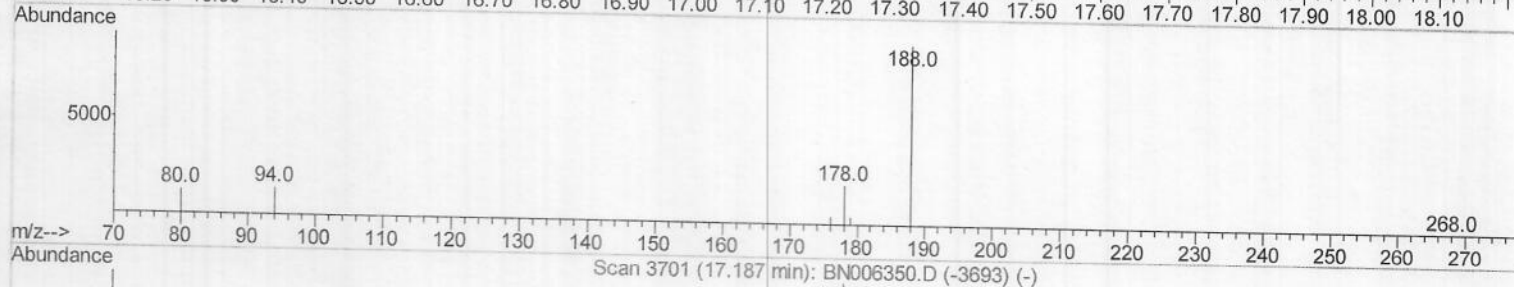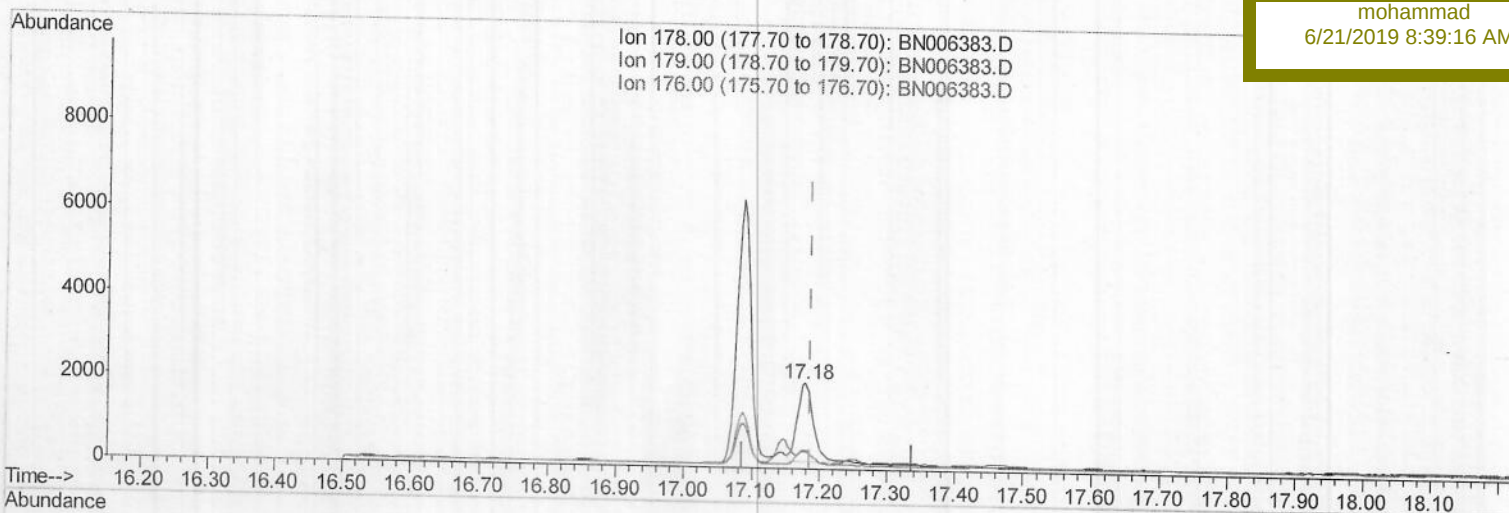

(13) Anthracene

17.179min (-0.008) 0.06ng/ul m

> JU 06/25/19

response 2910

Ion	Exp%	Act%
178.00	100	100
179.00	15.30	19.87#
176.00	18.90	21.71
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\

Data File : BN006383.D

Acq On : 18 Jun 2019 18:59

Operator : JU/SJ

Sample : K3335-09

Misc :

ALS Vial : 15 Sample Multiplier: 1

Quant Time: Jun 19 01:41:39 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A4236

Manual Integrations

APPROVED

mohammad

6/21/2019 8:39:16 AM

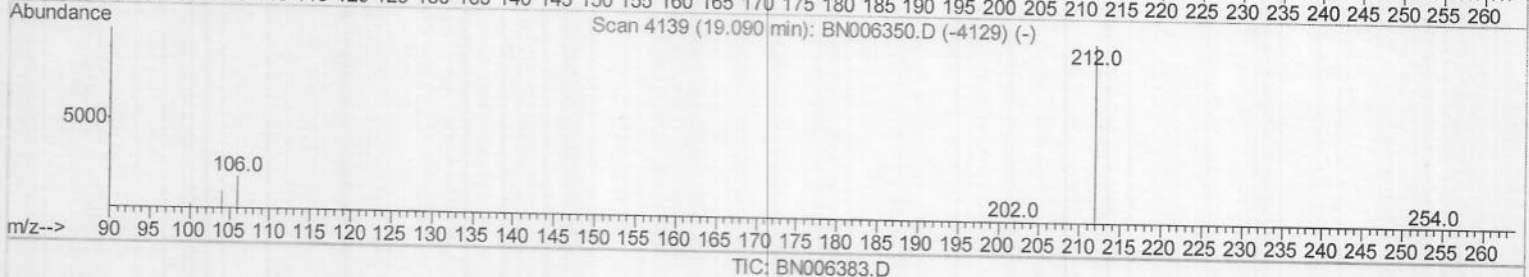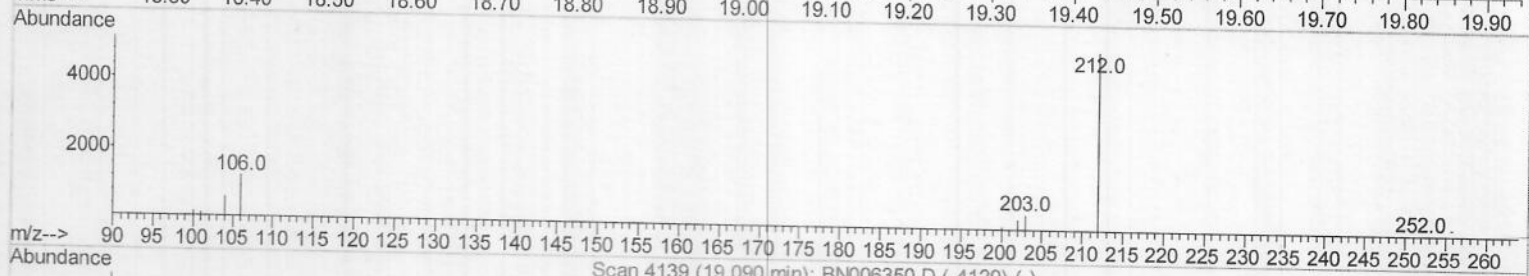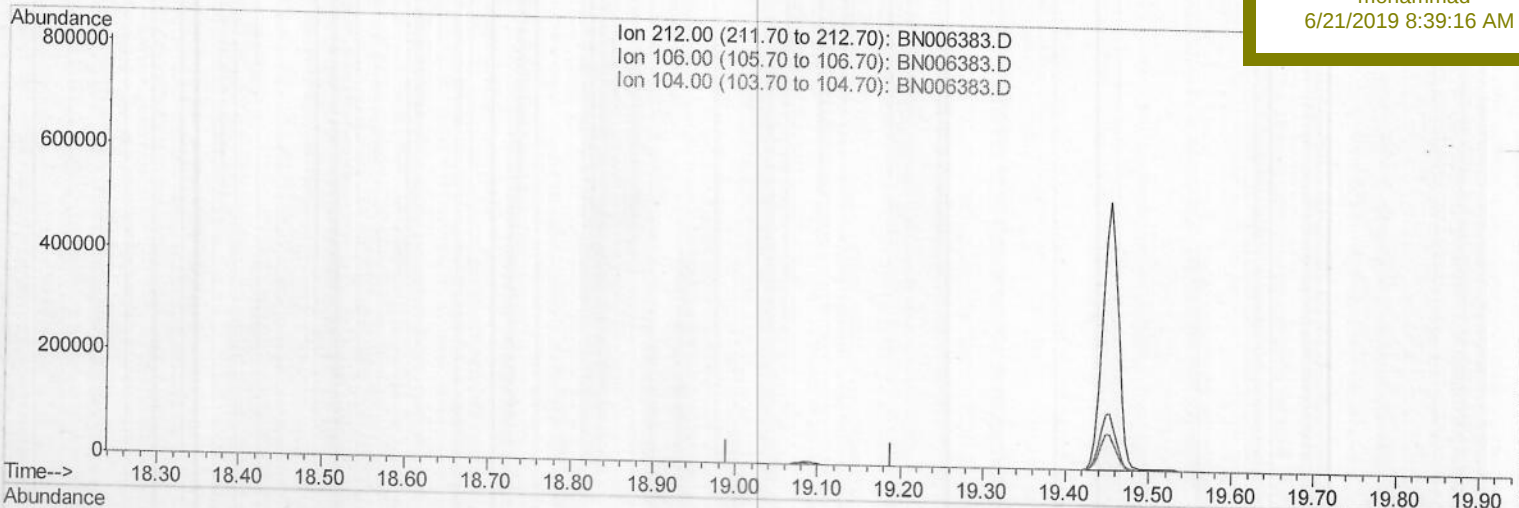

(14) Fluoranthene-d10 (SURR)

19.090min (-19.090) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\

Data File : BN006383.D

Acq On : 18 Jun 2019 18:59

Operator : JU/SJ

Sample : K3335-09

Misc :

ALS Vial : 15 Sample Multiplier: 1

Quant Time: Jun 19 01:41:39 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A4236

Manual Integrations

APPROVED

mohammad

6/21/2019 8:39:16 AM

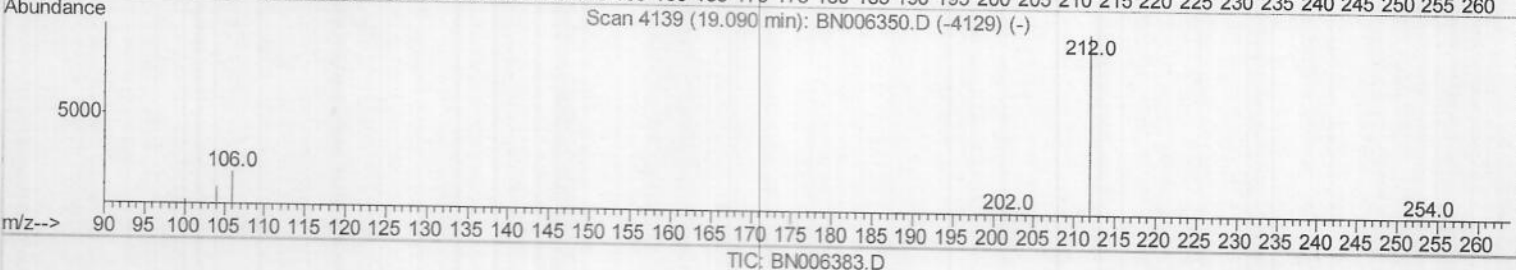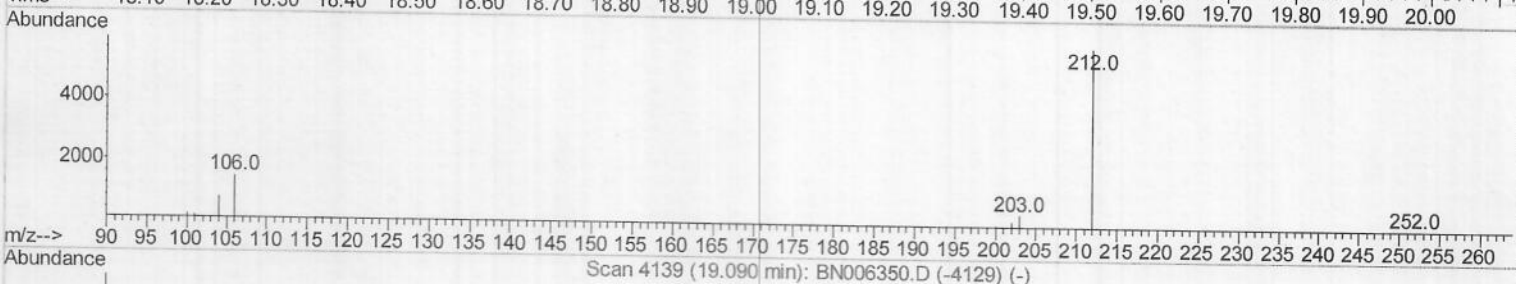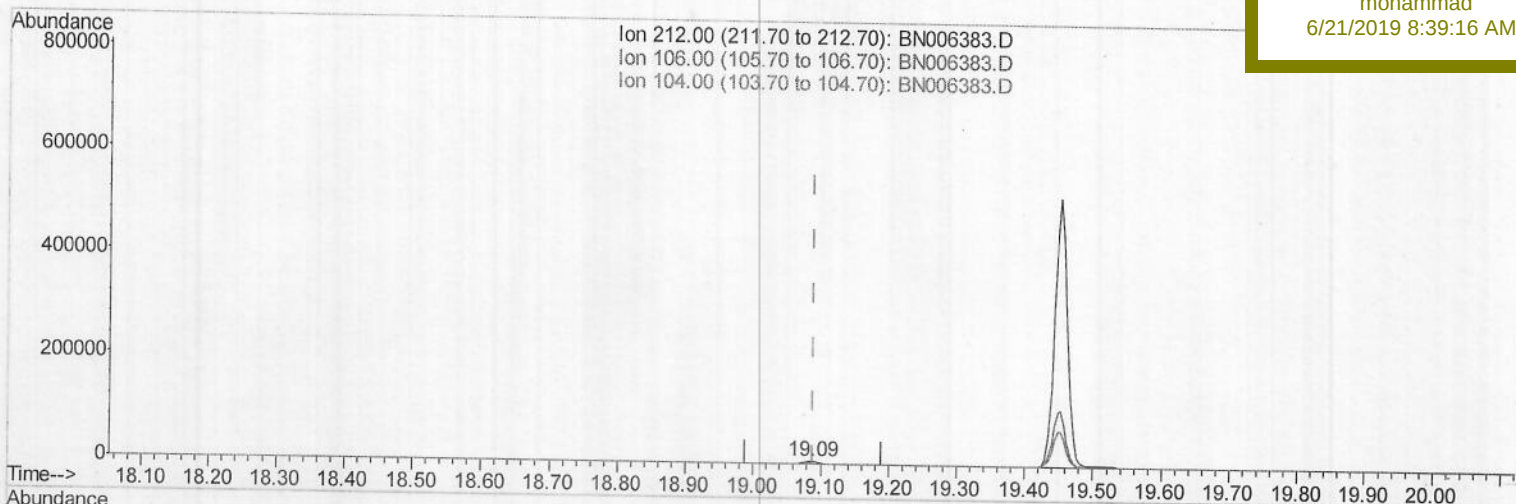

(14) Fluoranthene-d10 (SURR)

19.086min (-0.005) 0.18ng/ul m

> JU 06/25/19

response 7927

Ion	Exp%	Act%
212.00	100	100
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006383.D
 Acq On : 18 Jun 2019 18:59
 Operator : JU/SJ
 Sample : K3335-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Quant Time: Jun 19 01:41:39 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 A4236

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:39:16 AM

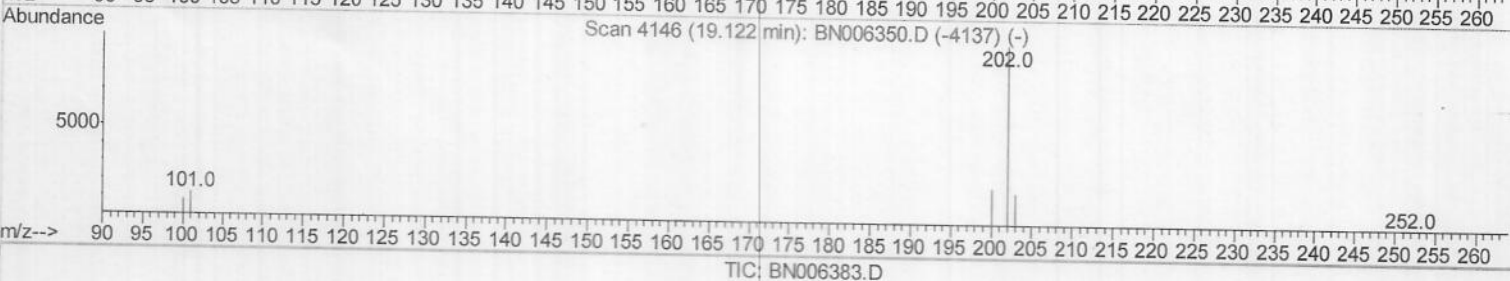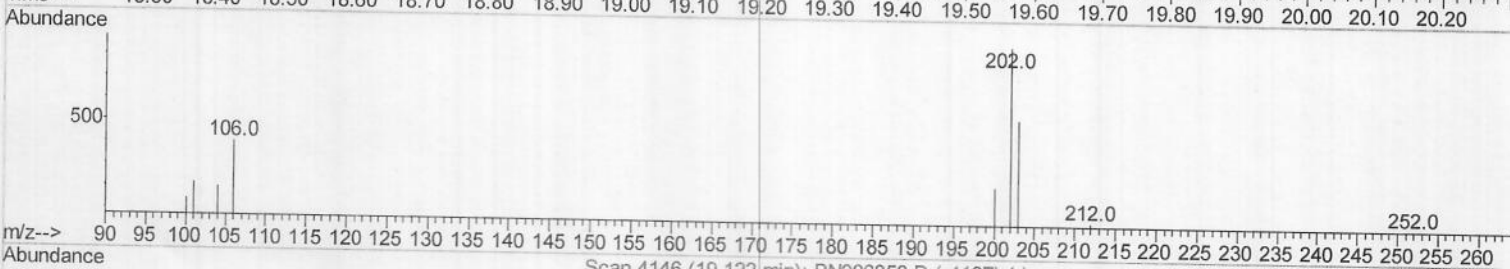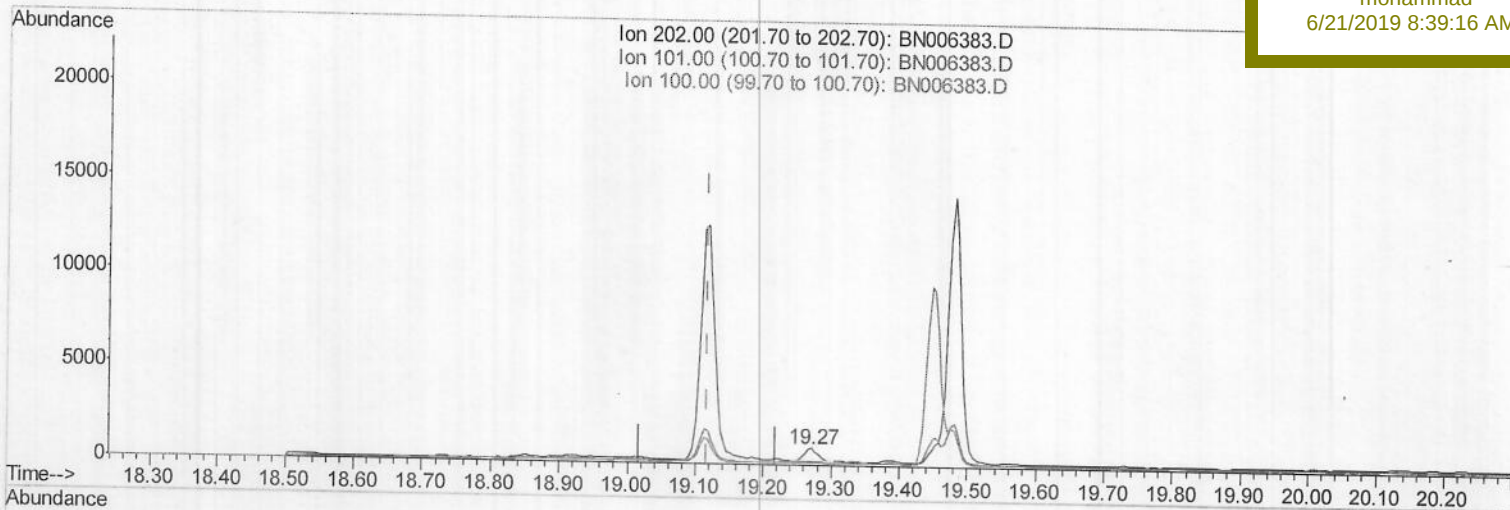

TIC: BN006383.D

(15) Fluoranthene (C)
 19.271min (+0.153) 0.01ng/ul
 response 854

Ion	Exp%	Act%
202.00	100	100
101.00	12.10	24.63
100.00	8.70	16.50
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\

Data File : BN006383.D

Acq On : 18 Jun 2019 18:59

Operator : JU/SJ

Sample : K3335-09

Misc :

ALS Vial : 15 Sample Multiplier: 1

Quant Time: Jun 19 01:41:39 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :




BNA_N

ClientSampleId :

A4236

Manual Integrations
APPROVED

mohammad
6/21/2019 8:39:16 AM

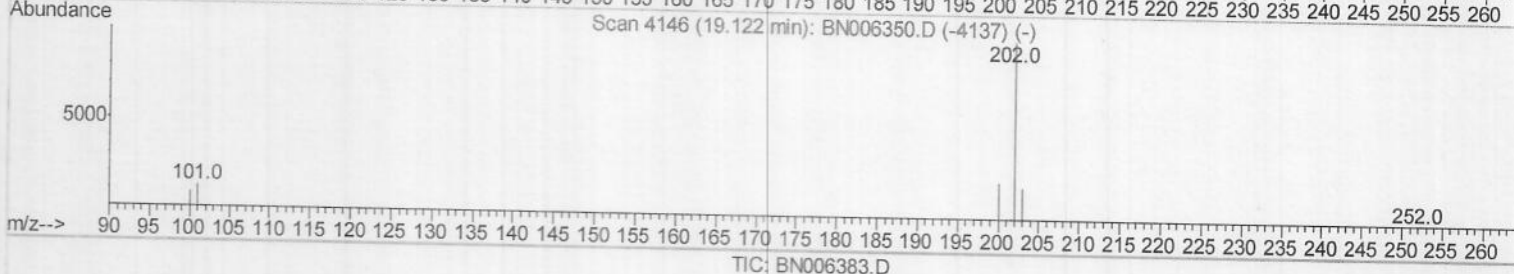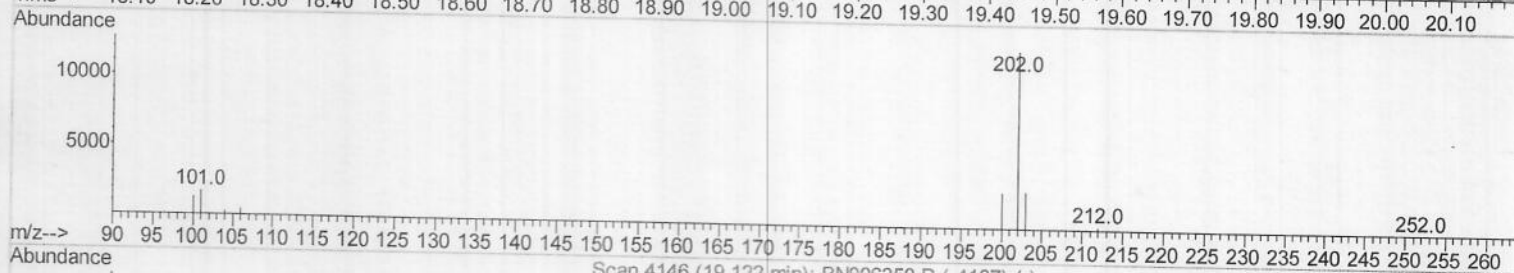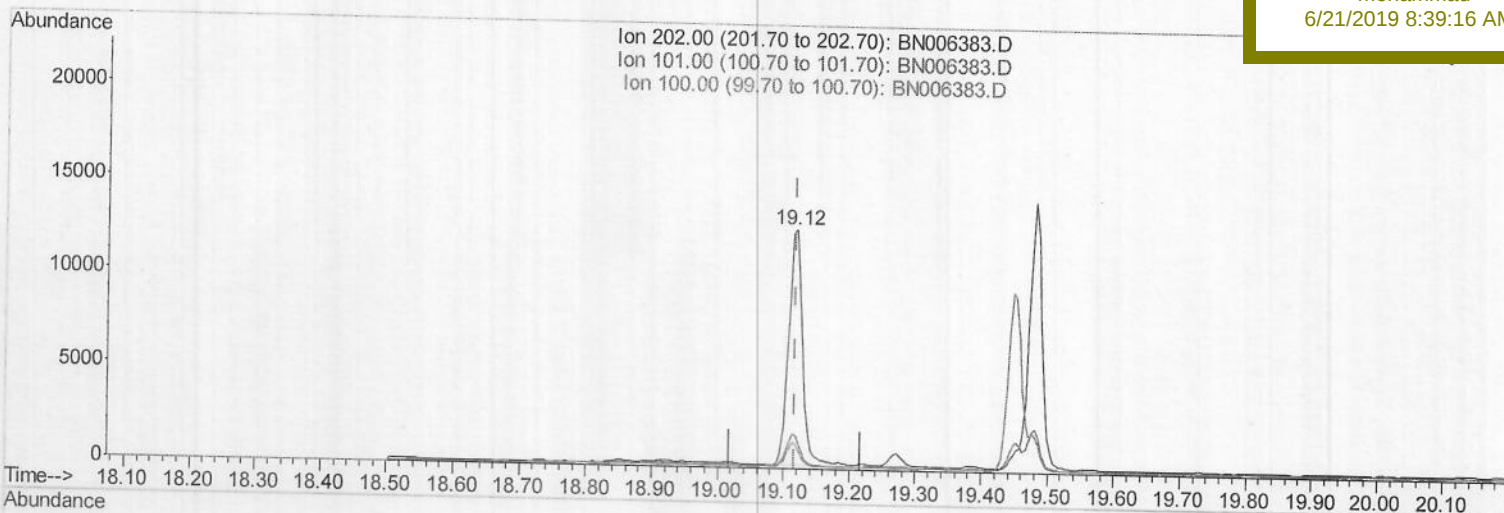

(15) Fluoranthene (C)

19.118min (+0.000) 0.31ng/ul m

response 18375

Ion Exp% Act%

202.00 100 100

101.00 12.10 13.47

100.00 8.70 9.97

0.00 0.00 0.00

> JU 06/25/19

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006383.D
 Acq On : 18 Jun 2019 18:59
 Operator : JU/SJ
 Sample : K3335-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Quant Time: Jun 19 01:41:39 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 A4236

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:39:16 AM

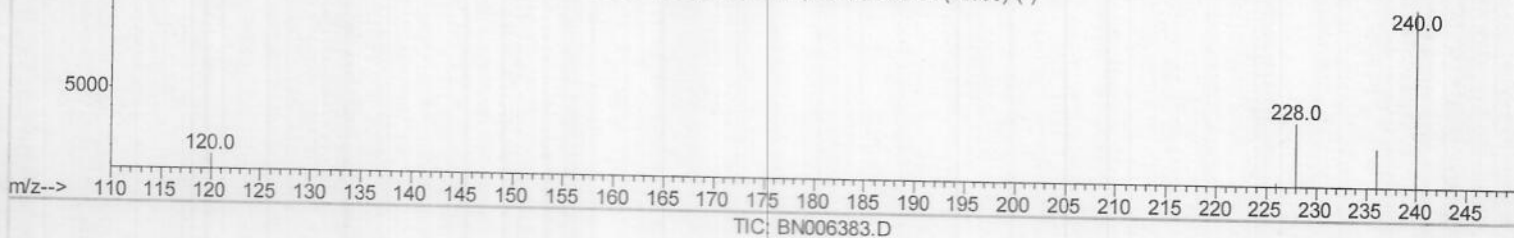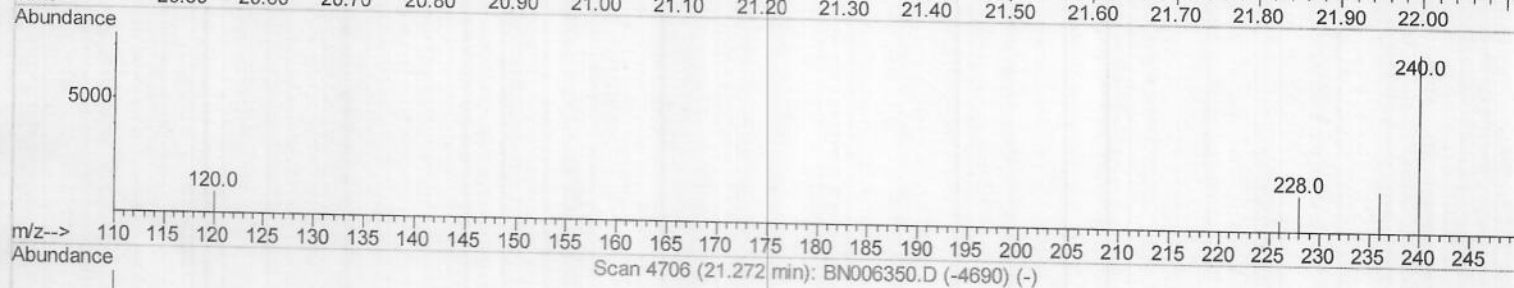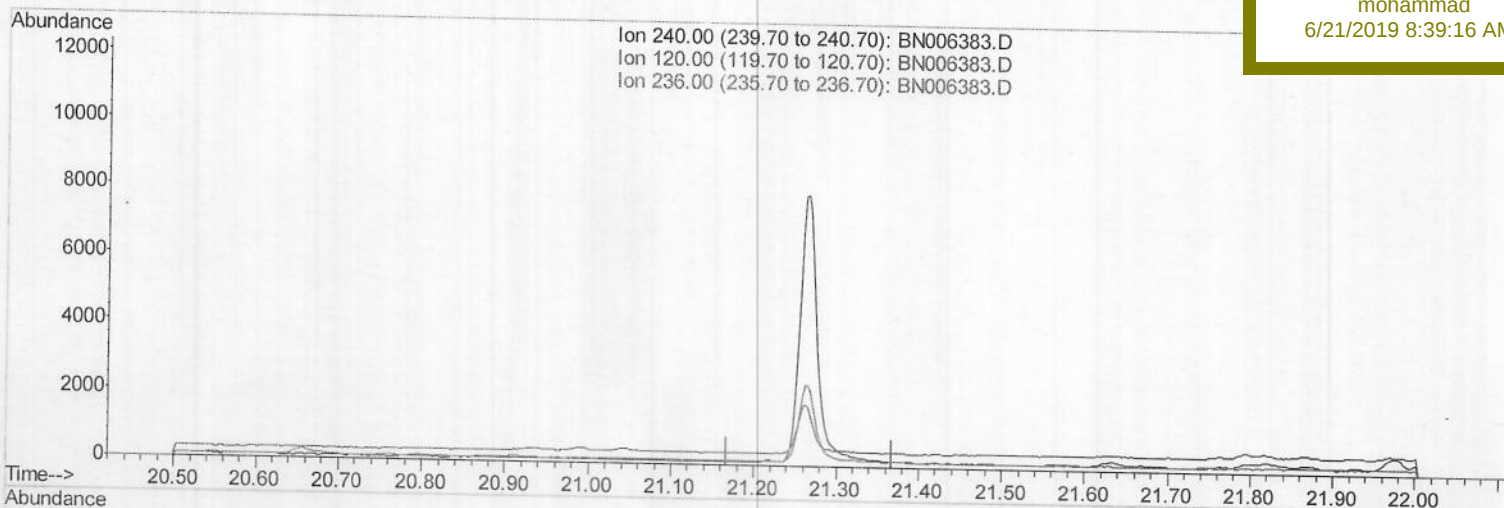

(16) Chrysene-d12 (I)

21.268min (-21.268) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	20.10	0.00#
236.00	30.10	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006383.D
 Acq On : 18 Jun 2019 18:59
 Operator : JU/SJ
 Sample : K3335-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Quant Time: Jun 19 01:41:39 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 A4236

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:39:16 AM

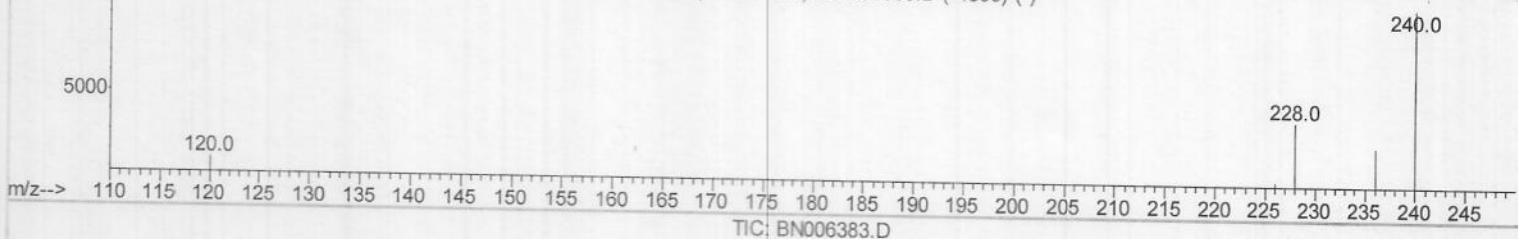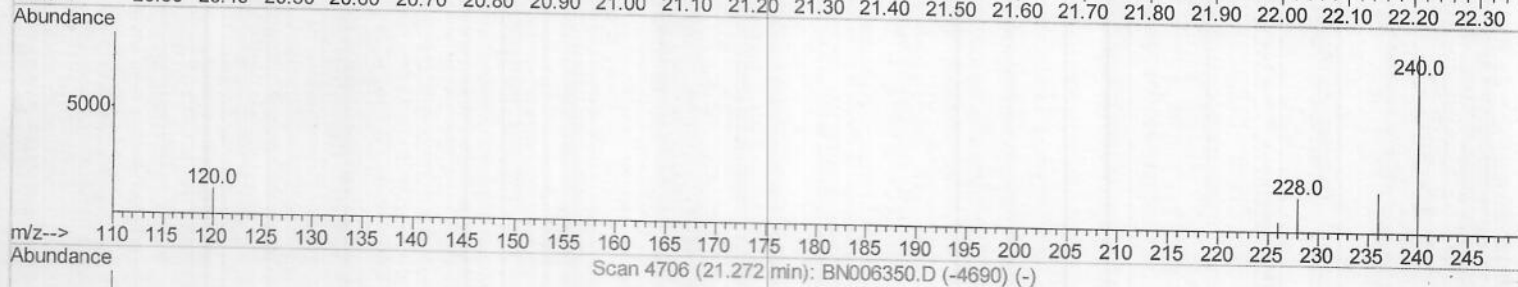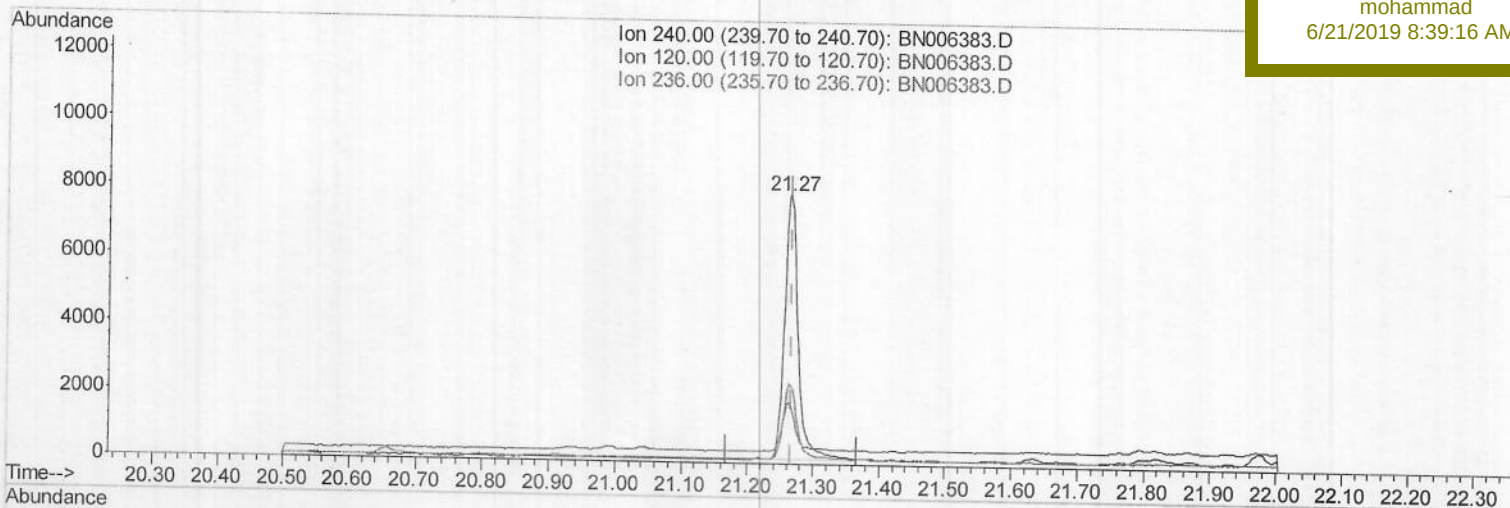

(16) Chrysene-d12 (I)

21.265min (-0.003) 0.40ng/ul m > JU 06/25/19

response 11362

Ion	Exp%	Act%
240.00	100	100
120.00	20.10	22.04
236.00	30.10	29.57
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\

Data File : BN006383.D

Acq On : 18 Jun 2019 18:59

Operator : JU/SJ

Sample : K3335-09

Misc :

ALS Vial : 15 Sample Multiplier: 1

Quant Time: Jun 19 01:49:25 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :




BNA_N

ClientSampleId :

A4236

Manual Integrations
APPROVED

mohammad
6/21/2019 8:39:16 AM

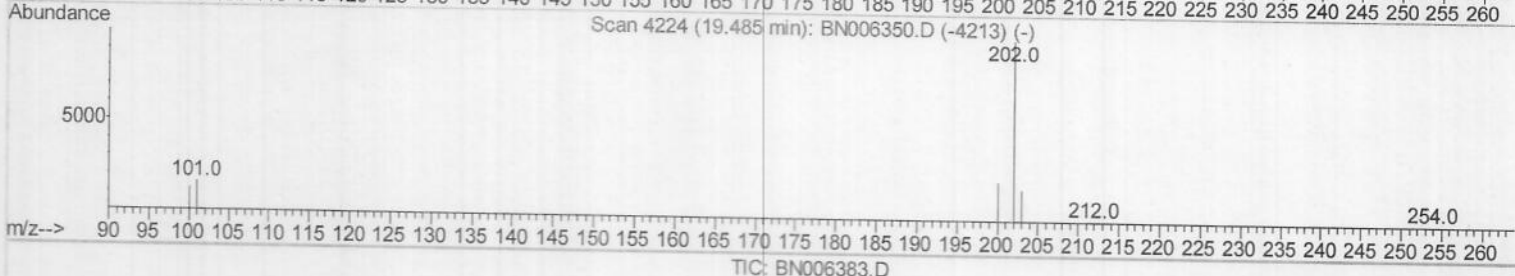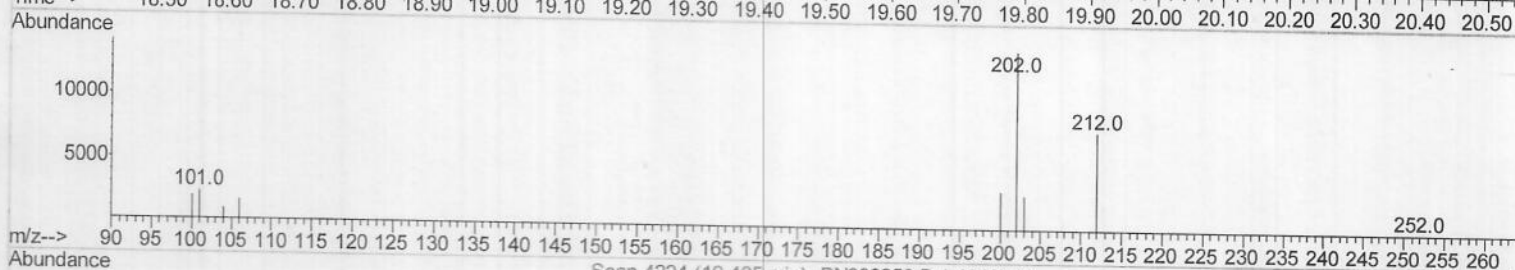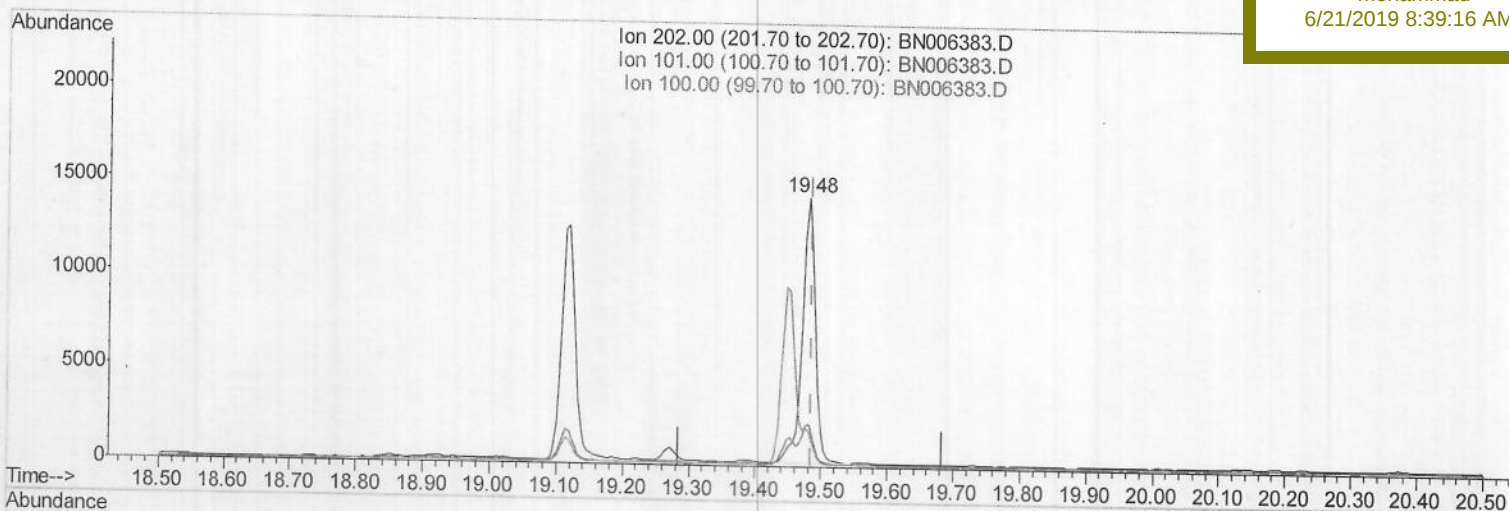

(17) Pyrene

19.481min (-0.005) 0.33ng/ul

response 19552

Ion	Exp%	Act%
202.00	100	100
101.00	15.20	15.88
100.00	12.20	13.38
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006383.D
 Acq On : 18 Jun 2019 18:59
 Operator : JU/SJ
 Sample : K3335-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Quant Time: Jun 19 01:49:25 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 A4236

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:39:16 AM

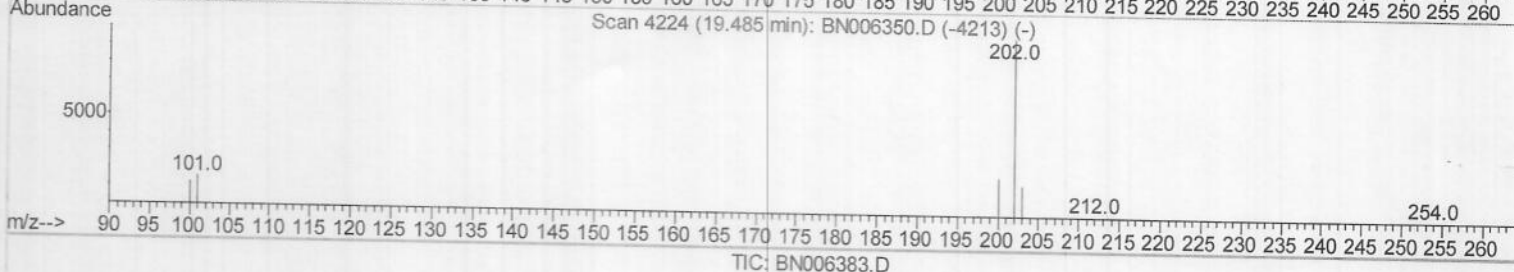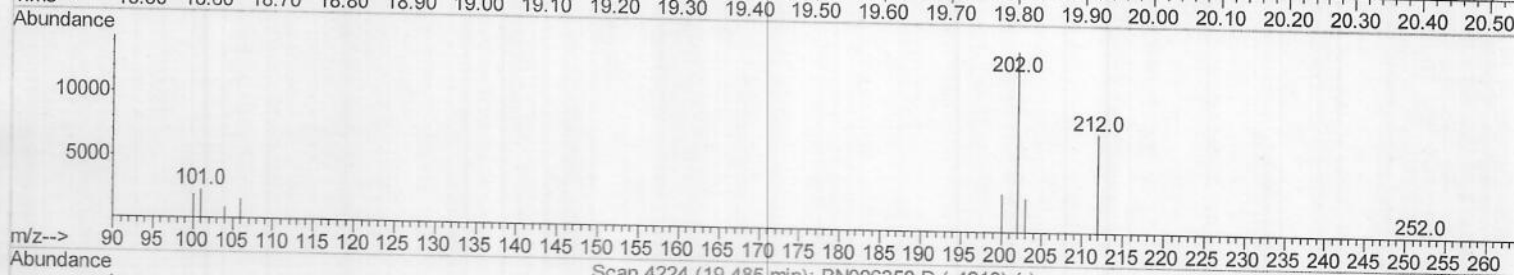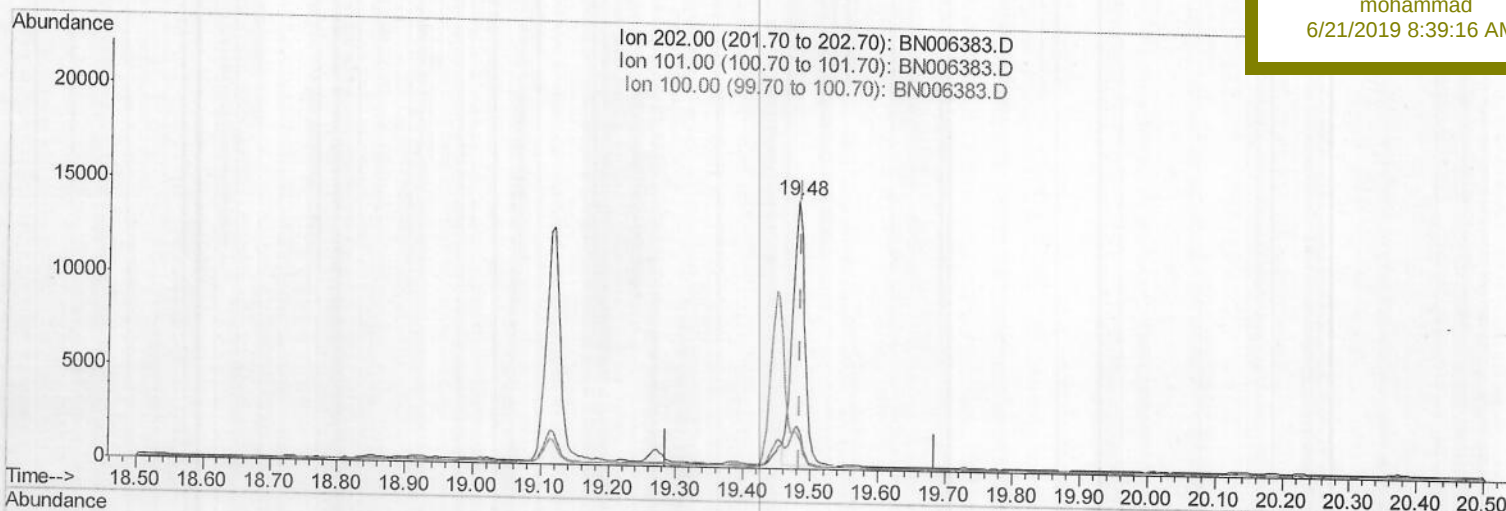

(17) Pyrene

19.481min (-0.005) 0.31ng/ul m

response 18439

Ion	Exp%	Act%
202.00	100	100
101.00	15.20	15.88
100.00	12.20	13.38
0.00	0.00	0.00

> JU 06/25/19

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006383.D
 Acq On : 18 Jun 2019 18:59
 Operator : JU/SJ
 Sample : K3335-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampled :
 A4236

Quant Time: Jun 19 01:49:25 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
 6/21/2019 8:39:16 AM

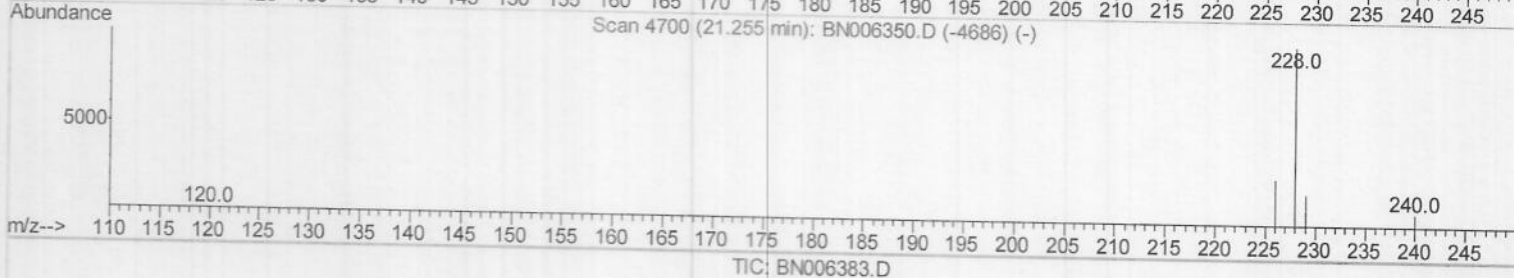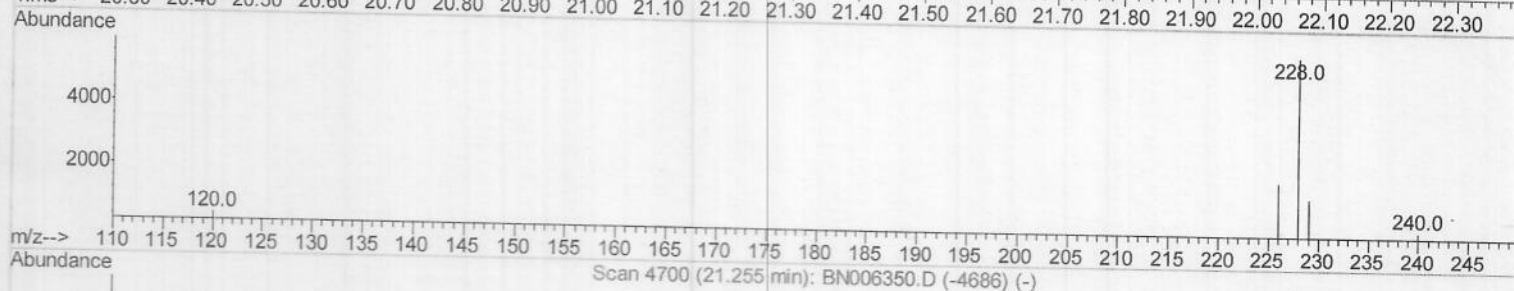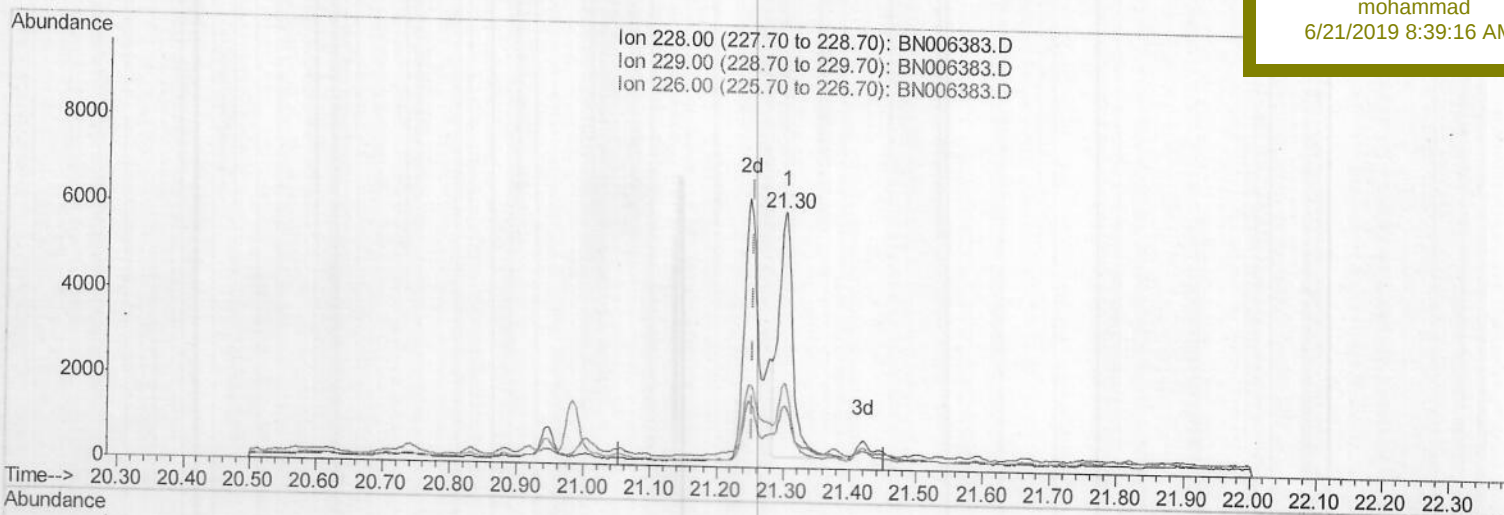

(18) Benzo(a)anthracene
 21.303min (+0.050) 0.18ng/ul
 response 8814

Ion	Exp%	Act%
228.00	100	100
229.00	20.60	24.42
226.00	28.50	32.70
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006383.D
 Acq On : 18 Jun 2019 18:59
 Operator : JU/SJ
 Sample : K3335-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Quant Time: Jun 19 01:49:25 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 A4236

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:39:16 AM

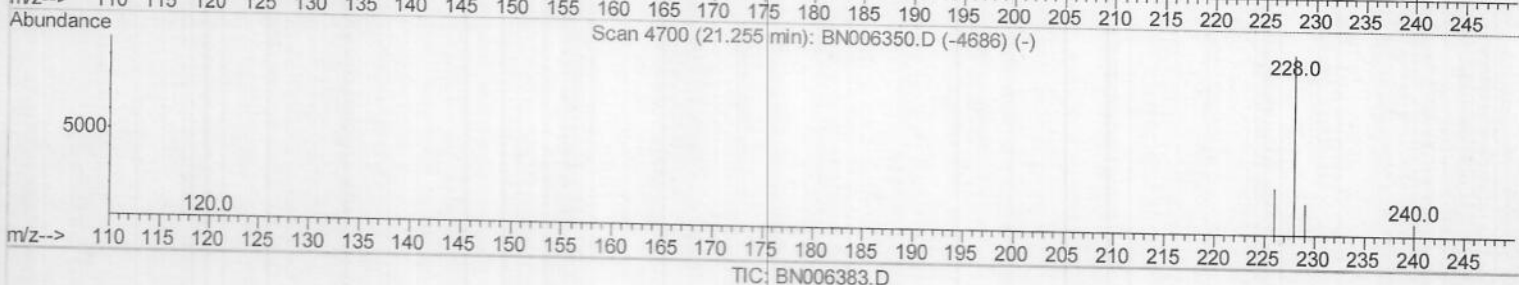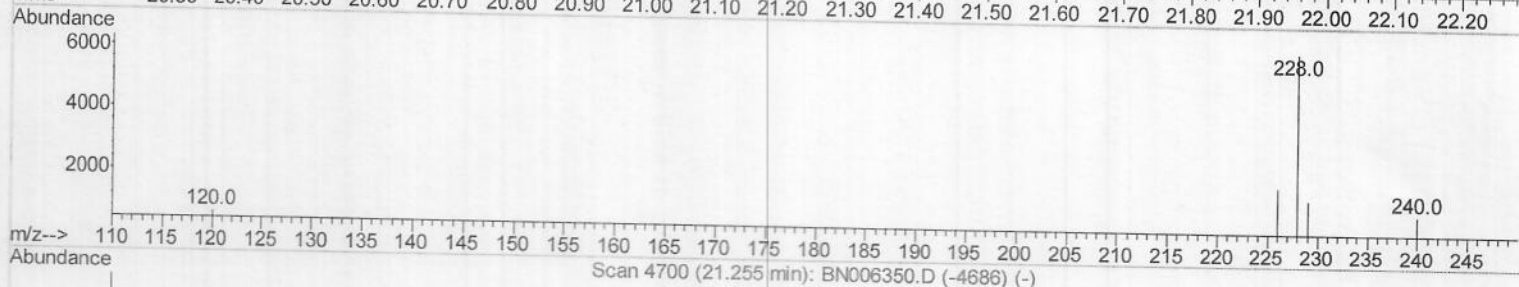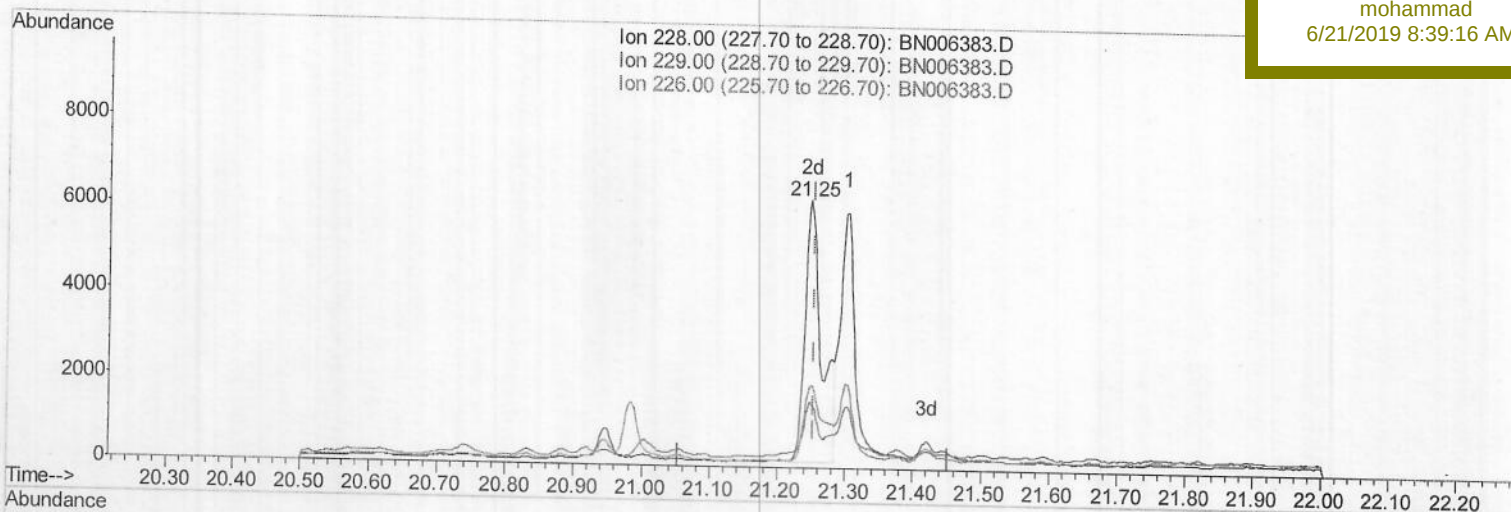

(18) Benzo(a)anthracene

21.248min (-0.006) 0.21ng/ul m > JU 06/25/19

response 10480

Ion	Exp%	Act%
228.00	100	100
229.00	20.60	24.90#
226.00	28.50	31.15
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006383.D
 Acq On : 18 Jun 2019 18:59
 Operator : JU/SJ
 Sample : K3335-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Quant Time: Jun 19 01:49:25 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 A4236

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:39:16 AM

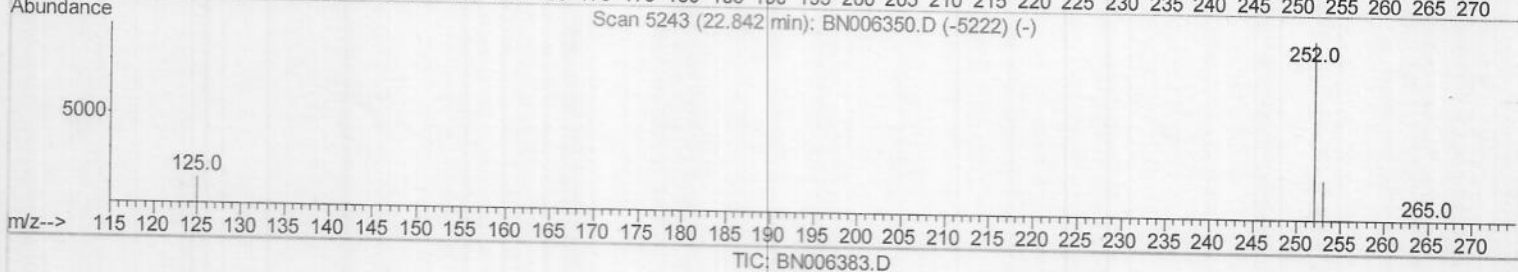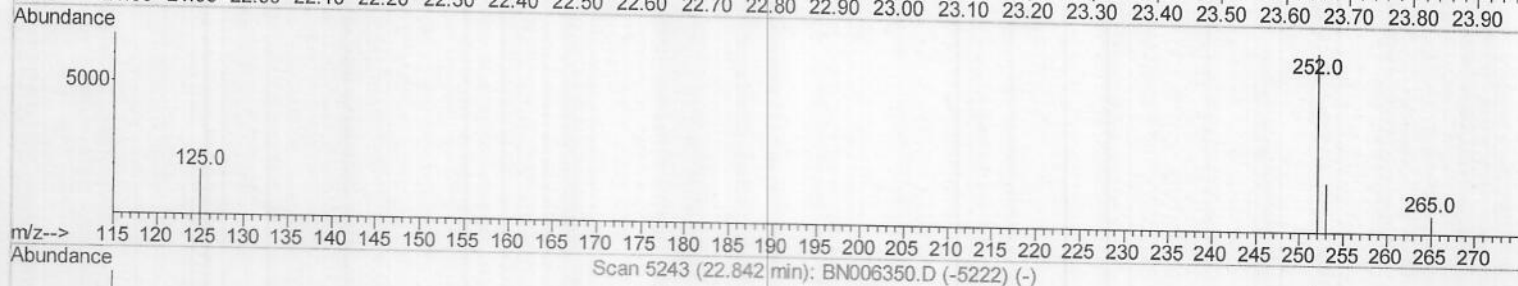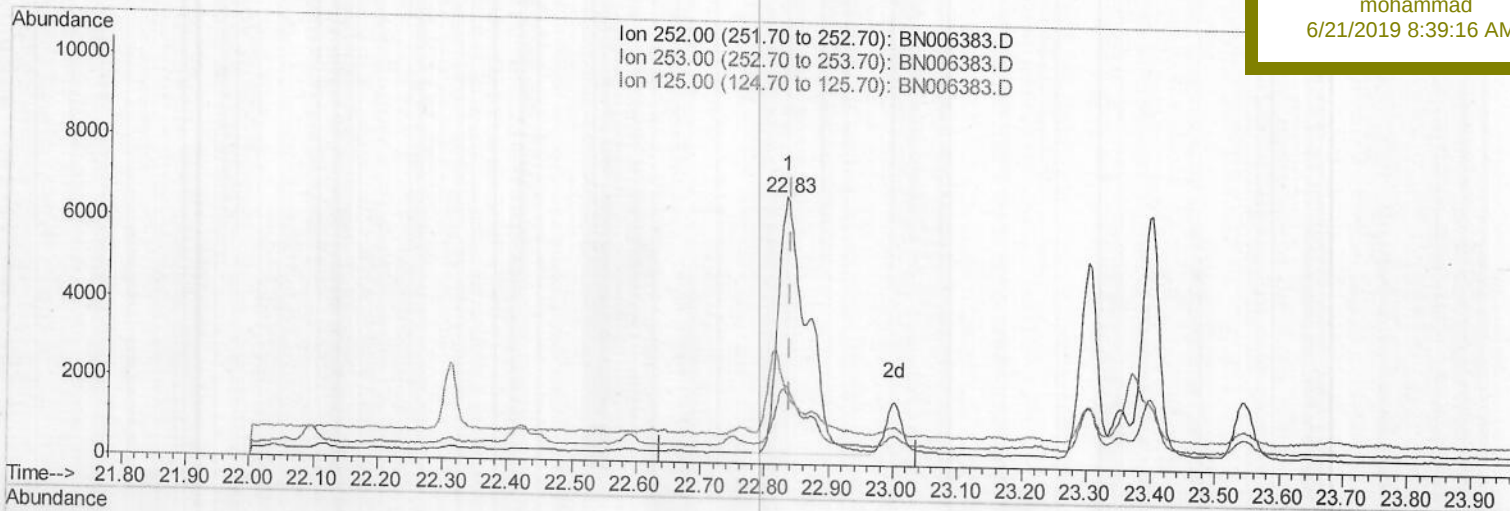

(21) Benzo(b)fluoranthene
 22.832min (-0.006) 0.28ng/ul
 response 20318

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	29.61
125.00	20.50	26.83
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\

Data File : BN006383.D

Acq On : 18 Jun 2019 18:59

Operator : JU/SJ

Sample : K3335-09

Misc :

ALS Vial : 15 Sample Multiplier: 1

Quant Time: Jun 19 01:49:25 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019




Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A4236

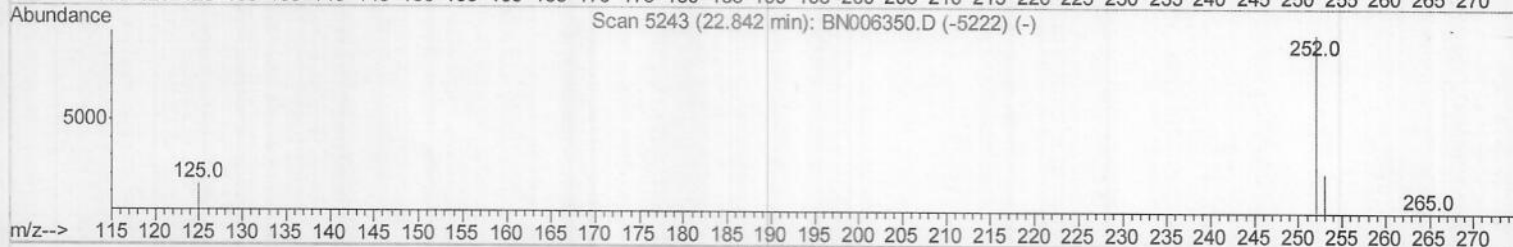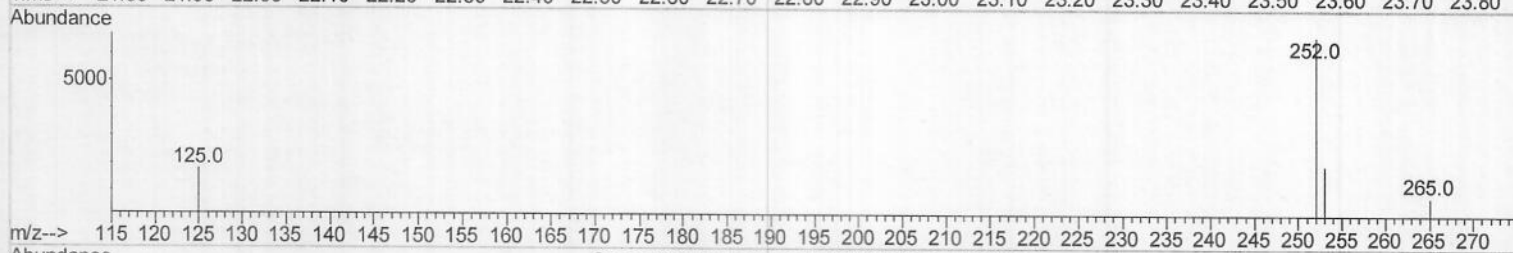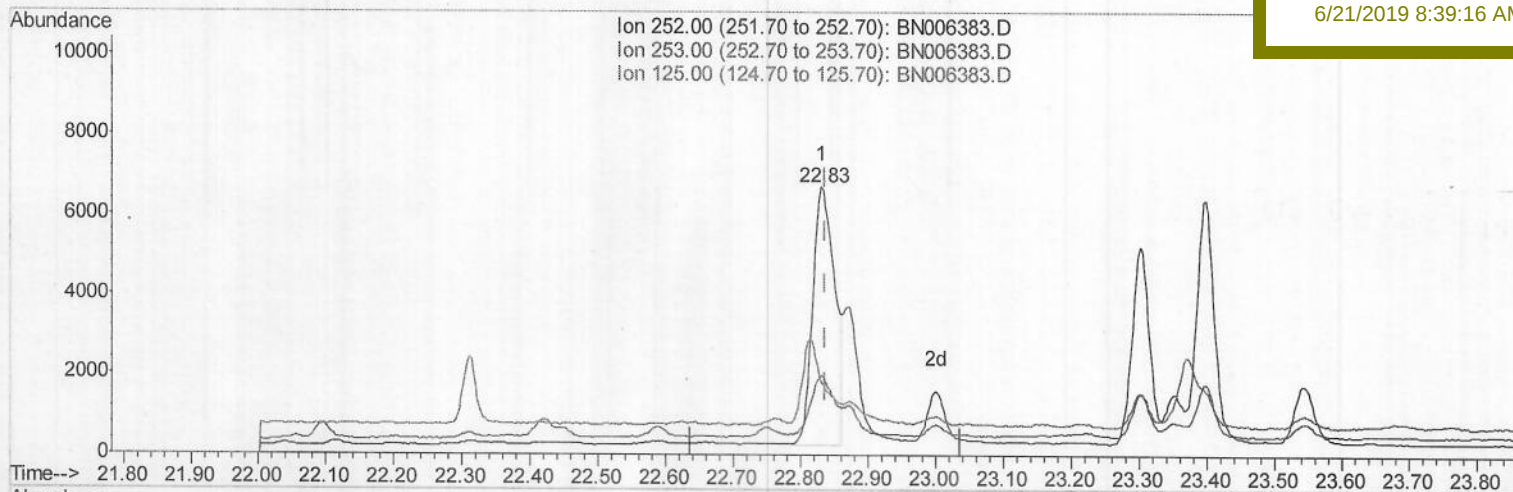Manual Integrations
APPROVEDmohammad
6/21/2019 8:39:16 AM

TIC: BN006383.D

(21) Benzo(b)fluoranthene

22.832min (-0.006) 0.20ng/ul m

response 14562

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	29.61
125.00	20.50	26.83
0.00	0.00	0.00

JU
06/25/19

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\

Data File : BN006383.D

Acq On : 18 Jun 2019 18:59

Operator : JU/SJ

Sample : K3335-09

Misc :

ALS Vial : 15 Sample Multiplier: 1

Quant Time: Jun 19 01:49:25 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019




Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A4236

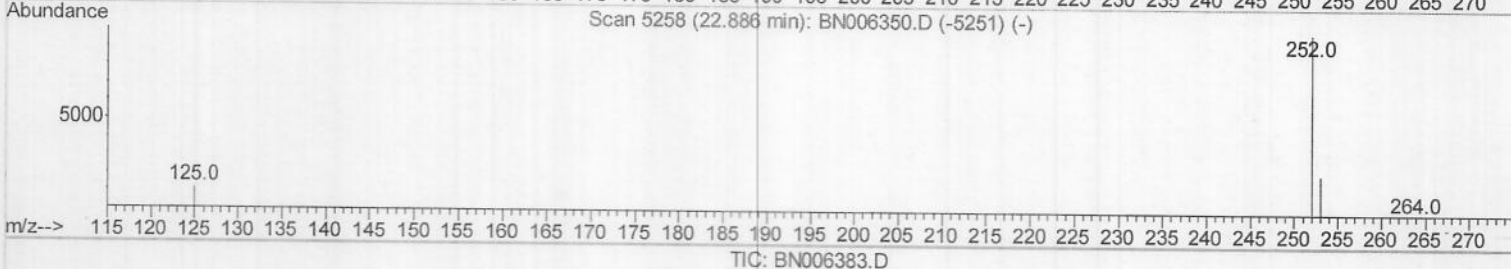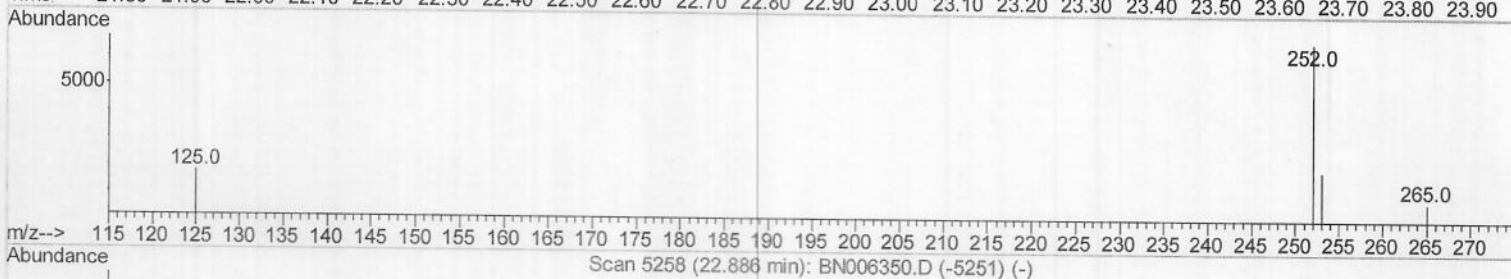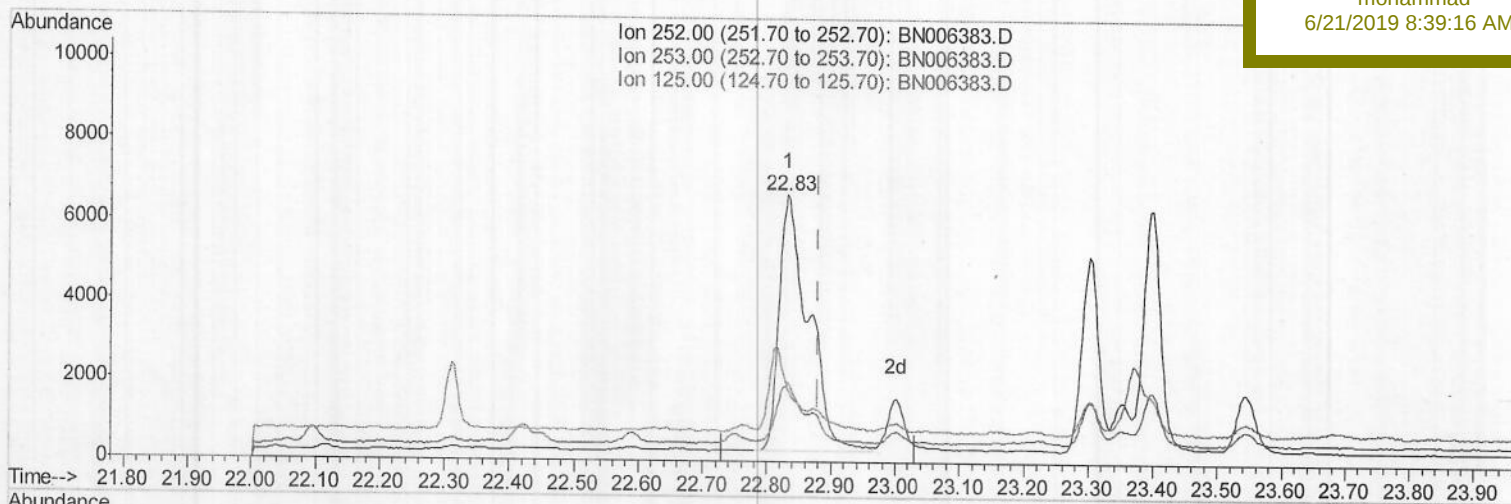Manual Integrations
APPROVEDmohammad
6/21/2019 8:39:16 AM

(22) Benzo(k)fluoranthene

22.832min (-0.050) 0.29ng/ul

response 20318

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	29.61
125.00	17.90	26.83#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006383.D
 Acq On : 18 Jun 2019 18:59
 Operator : JU/SJ
 Sample : K3335-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Quant Time: Jun 19 01:49:25 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 A4236

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:39:16 AM

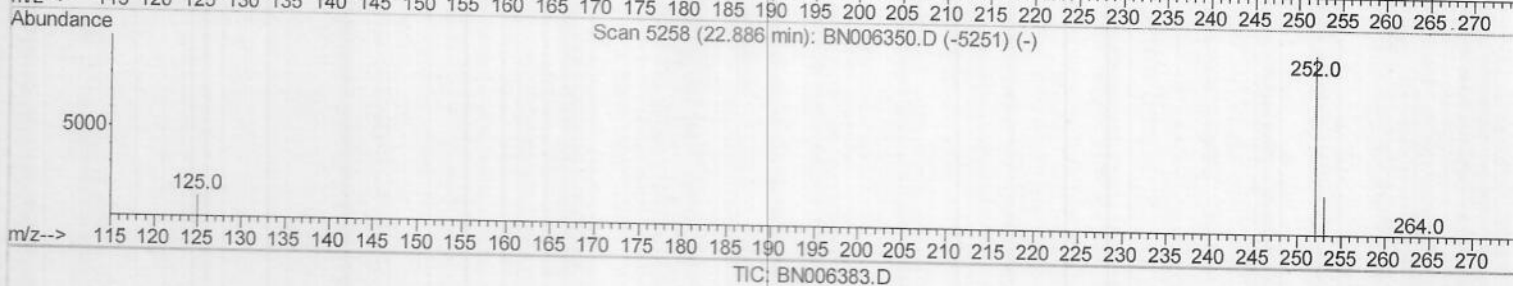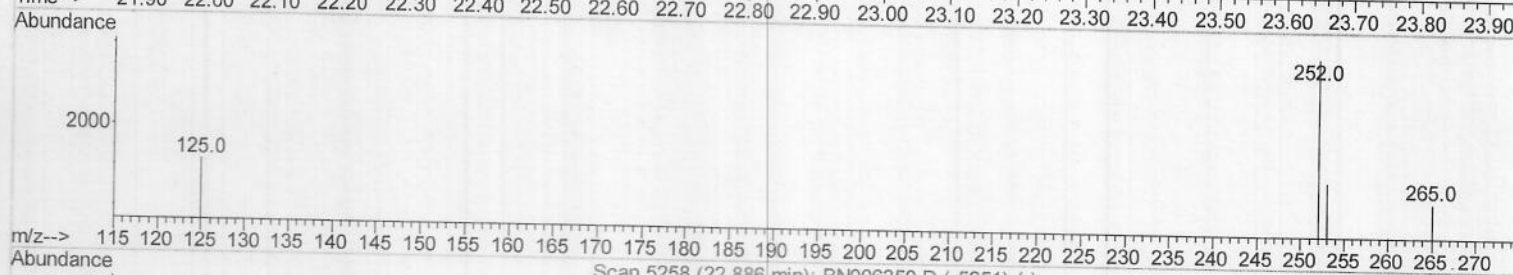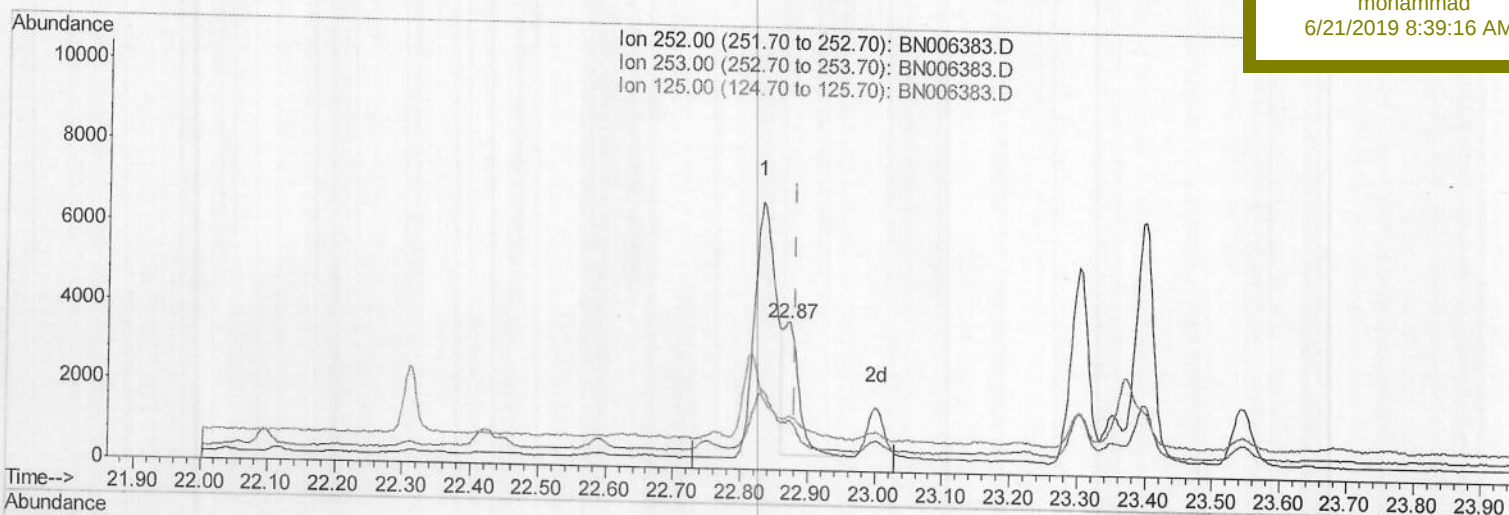

(22) Benzo(k)fluoranthene

22.873min (-0.009) 0.07ng/ul m > JU 06/25/19

response 5200

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	33.38#
125.00	17.90	36.62#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006383.D
 Acq On : 18 Jun 2019 18:59
 Operator : JU/SJ
 Sample : K3335-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 Client Sample Id :
 A4236

Quant Time: Jun 19 01:51:16 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:39:16 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	4588	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	17985	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.29	164	9099	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	16698m	0.40	ng/ul	0.00
16) Chrysene-d12	21.27	240	11362m	0.40	ng/ul	0.00
20) Perylene-d12	23.50	264	17252	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	3940	0.14	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	7927m	0.18	ng/ul	0.00
Target Compounds						
7) Acenaphthylene	14.01	152	2641	0.052	ng/ul#	93
12) Phenanthrene	17.09	178	8856	0.165	ng/ul	98
13) Anthracene	17.18	178	2910m	0.057	ng/ul	
15) Fluoranthene	19.12	202	18375m	0.310	ng/ul	
17) Pyrene	19.48	202	18439m	0.308	ng/ul	
18) Benzo(a)anthracene	21.25	228	10480m	0.209	ng/ul	
19) Chrysene	21.30	228	9207	0.195	ng/ul	95
21) Benzo(b)fluoranthene	22.83	252	14562m	0.202	ng/ul	
22) Benzo(k)fluoranthene	22.87	252	5200m	0.074	ng/ul	
23) Benzo(a)pyrene	23.40	252	10980	0.164	ng/ul	98
24) Indeno(1,2,3-cd)pyrene	25.73	276	8149	0.112	ng/ul#	88
25) Dibenzo(a,h)anthracene	25.74	278	2213	0.038	ng/ul#	56
26) Benzo(a,h,i)perylene	26.42	276	8146	0.134	ng/ul	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU
 06/25/19