


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006387.D
 Acq On : 18 Jun 2019 21:17
 Operator : JU/SJ
 Sample : K3335-19
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4238

Quant Time: Jun 19 02:14:23 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:39:31 AM

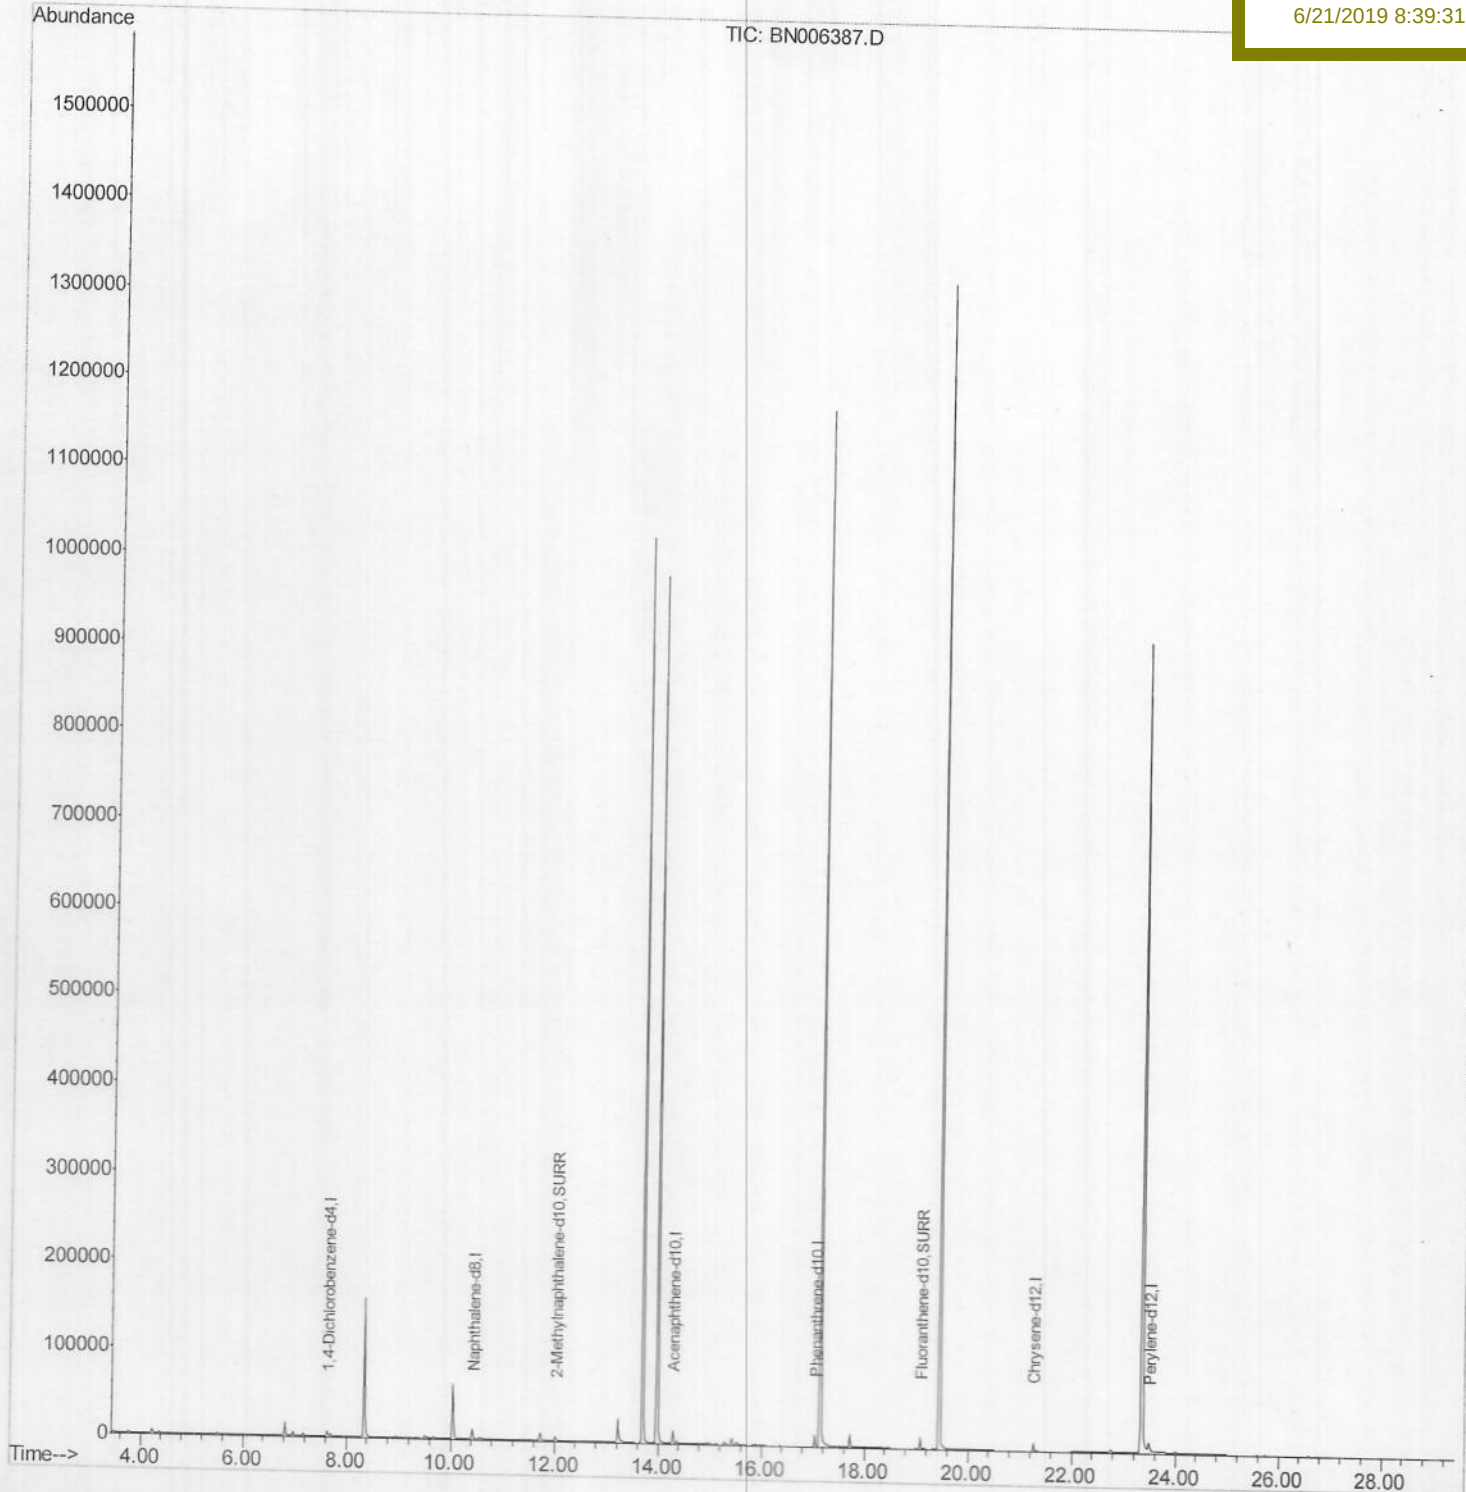

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\

Data File : BN006387.D

Acq On : 18 Jun 2019 21:17

Operator : JU/SJ

Sample : K3335-19

Misc :

ALS Vial : 19 Sample Multiplier: 1

Quant Time: Jun 19 01:29:10 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A4238

Manual Integrations

APPROVED

mohammad

6/21/2019 8:39:31 AM

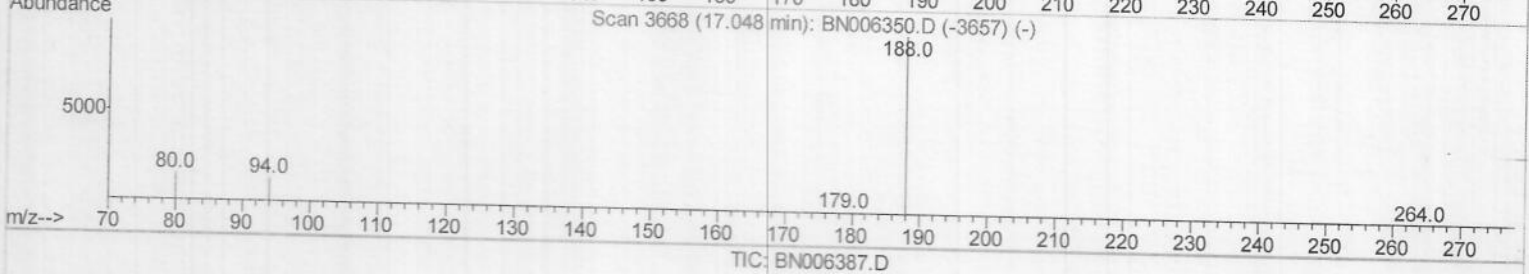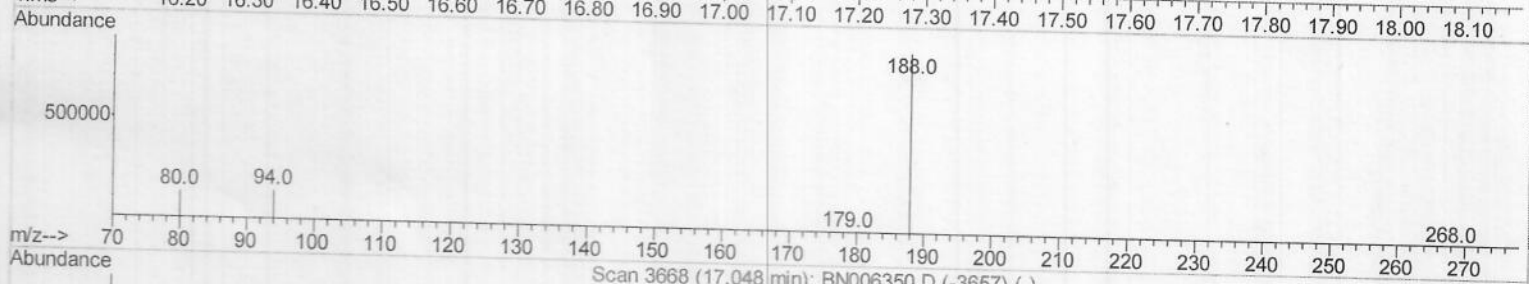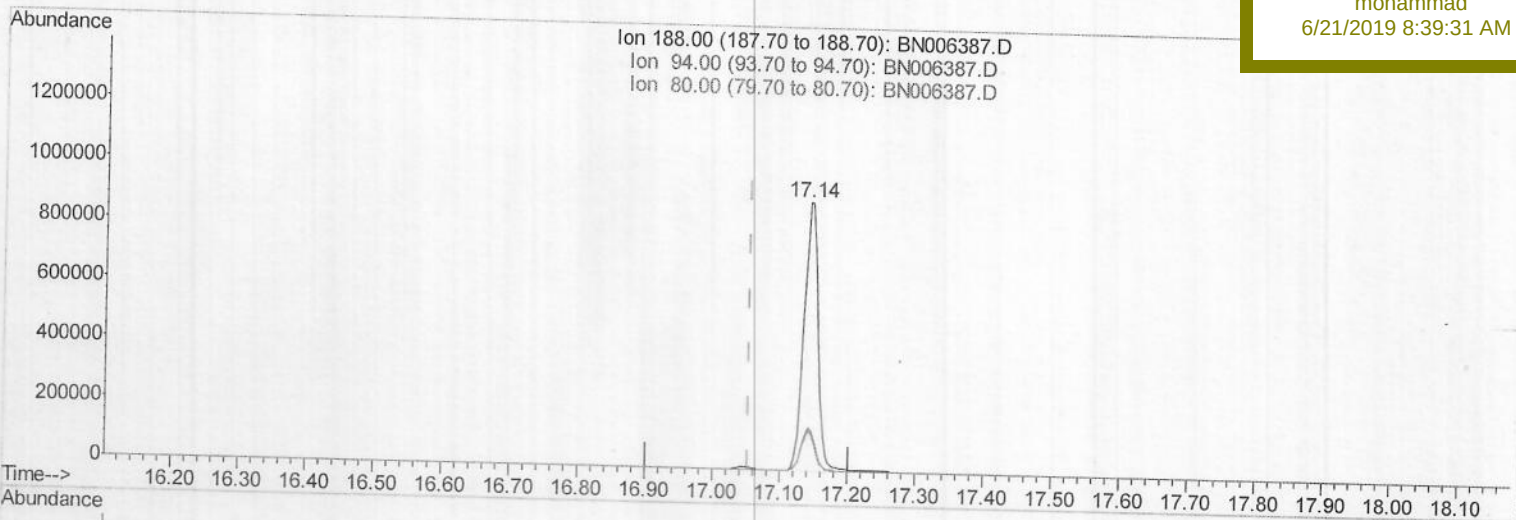

(10) Phenanthrene-d10 (I)

17.141min (+0.089) 0.40ng/ul

response 1284711

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	15.93#
80.00	13.60	14.69
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
Data File : BN006387.D

Acq On : 18 Jun 2019 21:17

Operator : JU/SJ

Sample : K3335-19

Misc :

ALS Vial : 19 Sample Multiplier: 1

Quant Time: Jun 19 01:29:10 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N



ClientSampleId :

A4238

Manual Integrations
APPROVED

mohammad

6/21/2019 8:39:31 AM

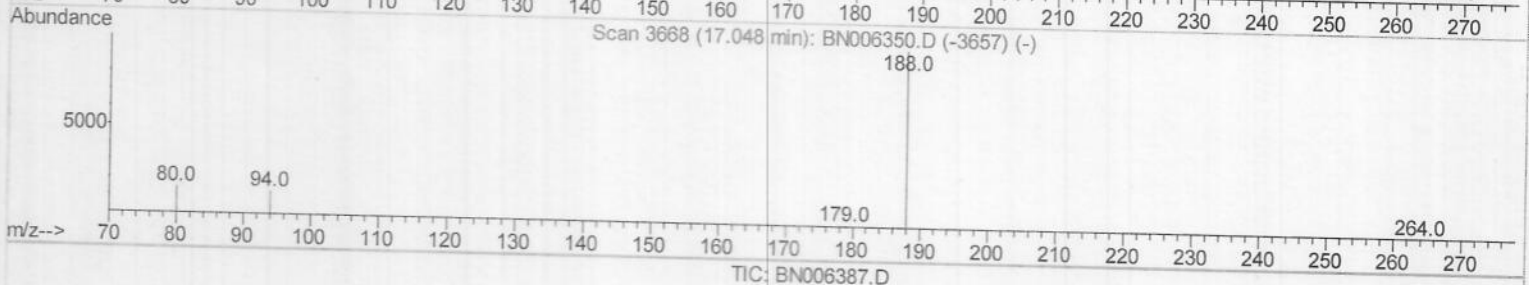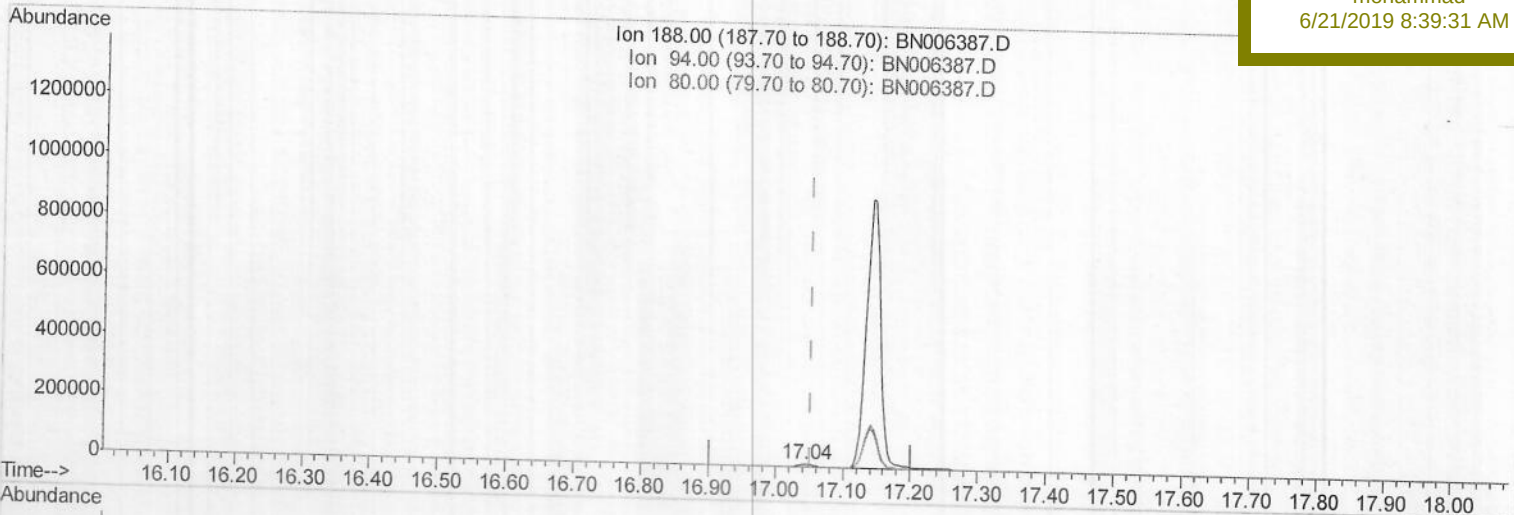

(10) Phenanthrene-d10 (I)

17.044min (-0.008) 0.40ng/ul m

~ JU 06/25/19

response 14606

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	14.07
80.00	13.60	15.39
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006387.D
 Acq On : 18 Jun 2019 21:17
 Operator : JU/SJ
 Sample : K3335-19
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4238

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:39:31 AM

Quant Time: Jun 19 02:12:17 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

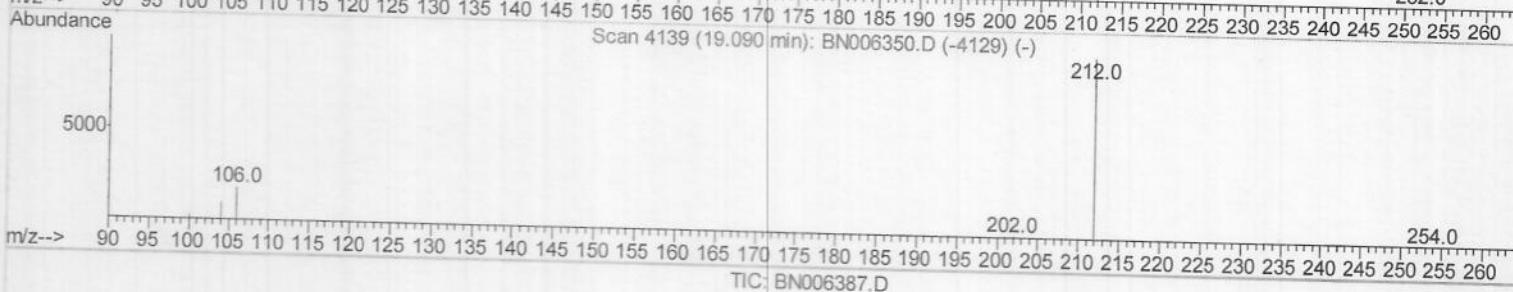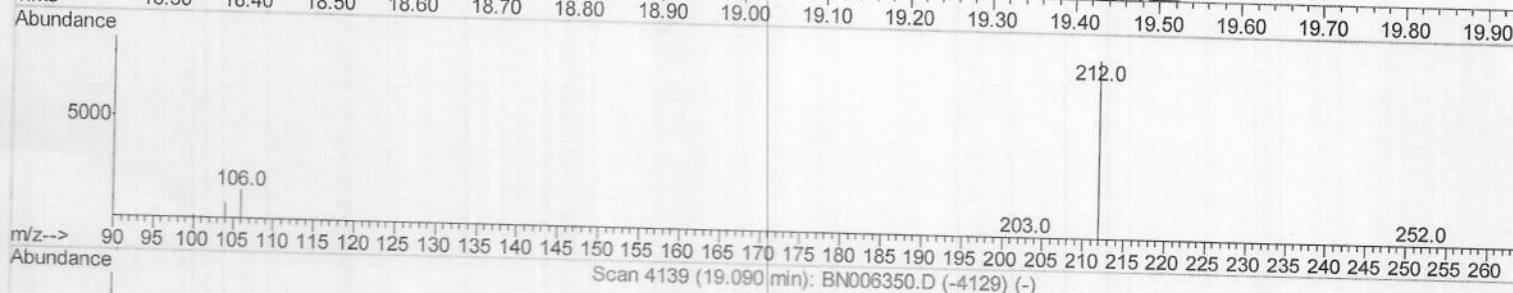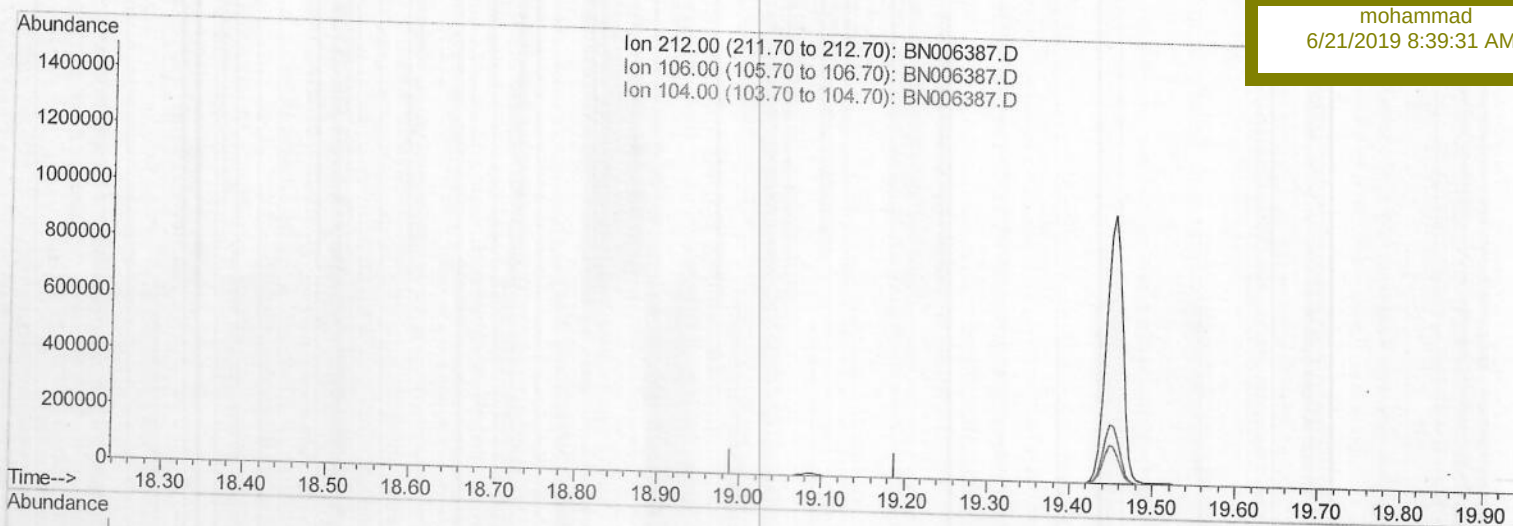

(14) Fluoranthene-d10 (SURR)

19.090min (-19.090) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006387.D

Acq On : 18 Jun 2019 21:17

Operator : JU/SJ

Sample : K3335-19

Misc :

ALS Vial : 19 Sample Multiplier: 1

Quant Time: Jun 19 02:12:17 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A4238

Manual Integrations

APPROVED

mohammad

6/21/2019 8:39:31 AM

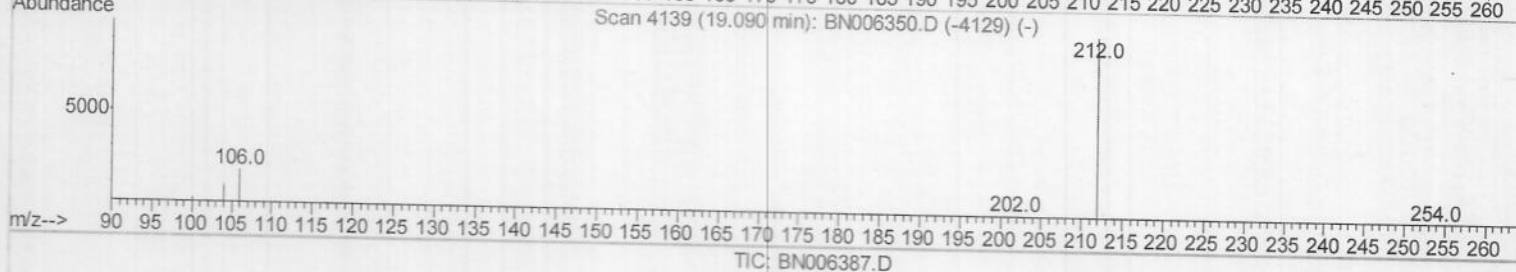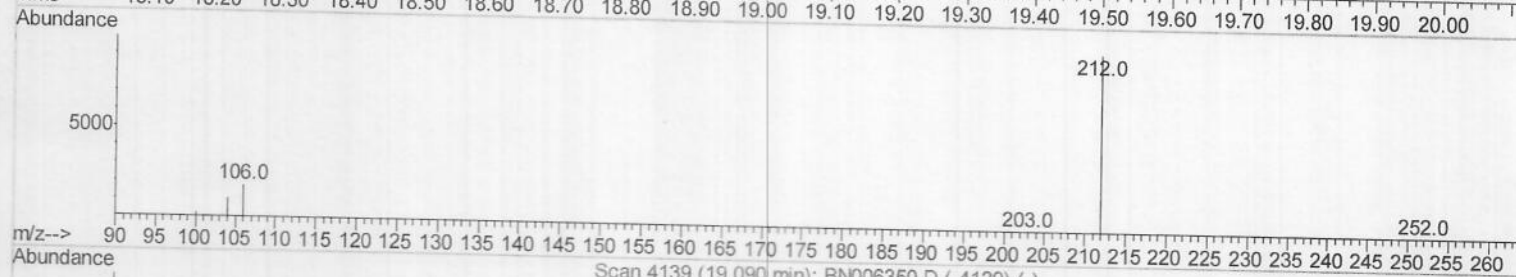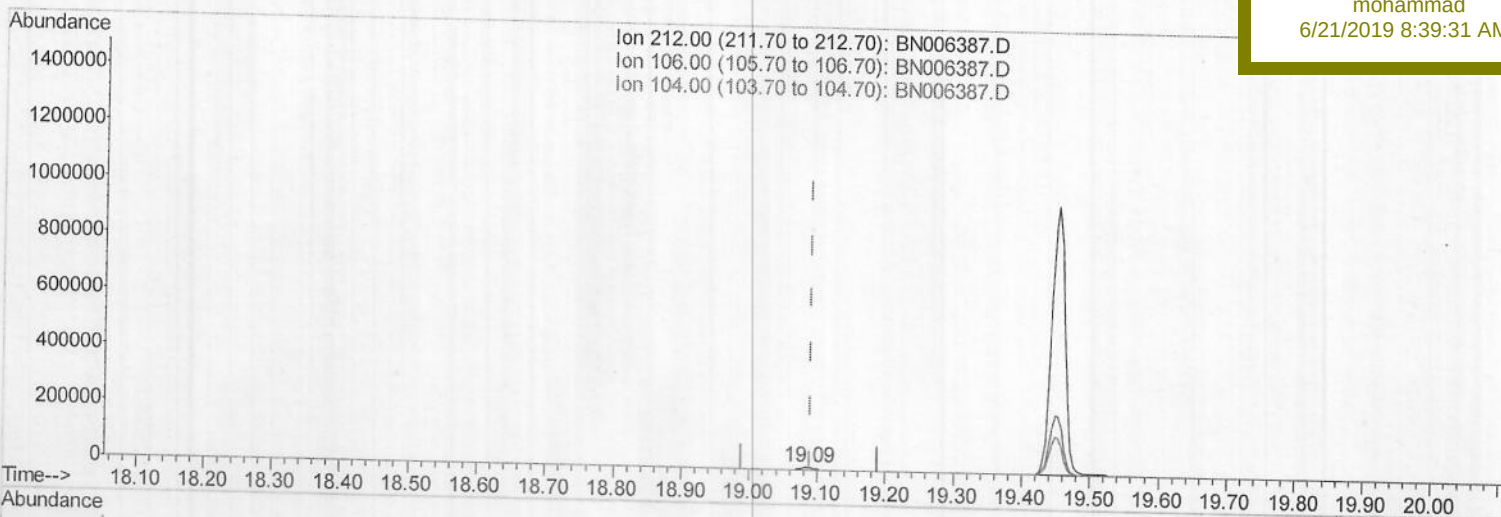

(14) Fluoranthene-d10 (SURR)

19.086min (-0.005) 0.35ng/ul m > JU 06/25/19

response 13734

Ion	Exp%	Act%
212.00	100	100
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006387.D

Acq On : 18 Jun 2019 21:17

Operator : JU/SJ

Sample : K3335-19

Misc :

ALS Vial : 19 Sample Multiplier: 1

Quant Time: Jun 19 02:12:17 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

OLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A4238

Manual Integrations

APPROVED

mohammad

6/21/2019 8:39:31 AM

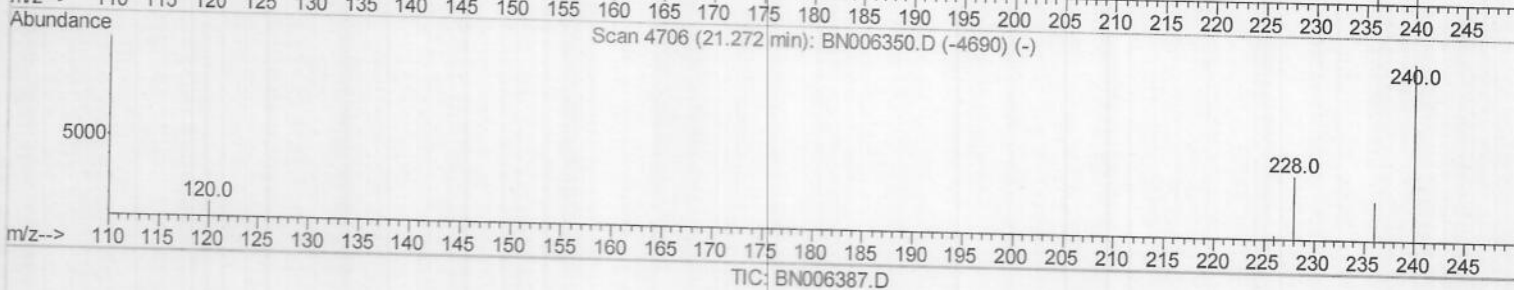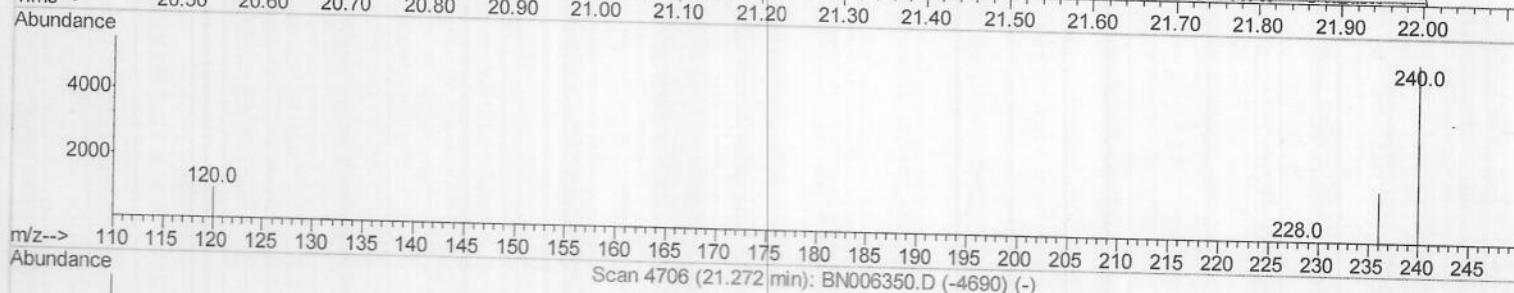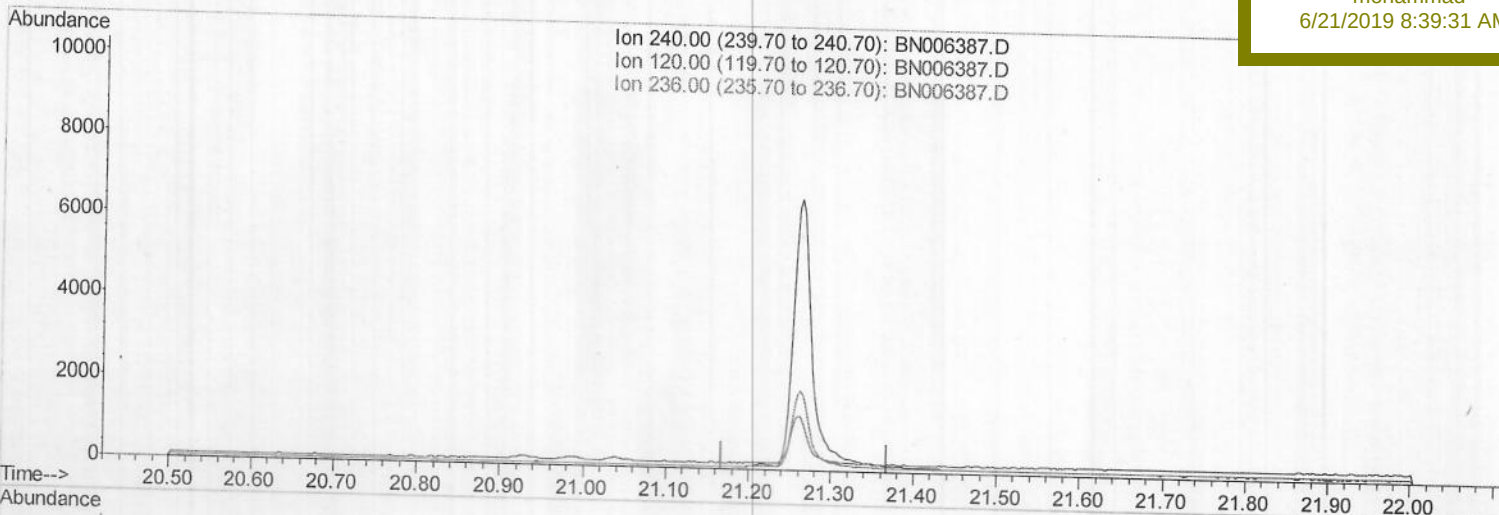

(16) Chrysene-d12 (I)

21.268min (-21.268) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	20.10	0.00#
236.00	30.10	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006387.D
 Acq On : 18 Jun 2019 21:17
 Operator : JU/SJ
 Sample : K3335-19
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4238

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:39:31 AM

Quant Time: Jun 19 02:12:17 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

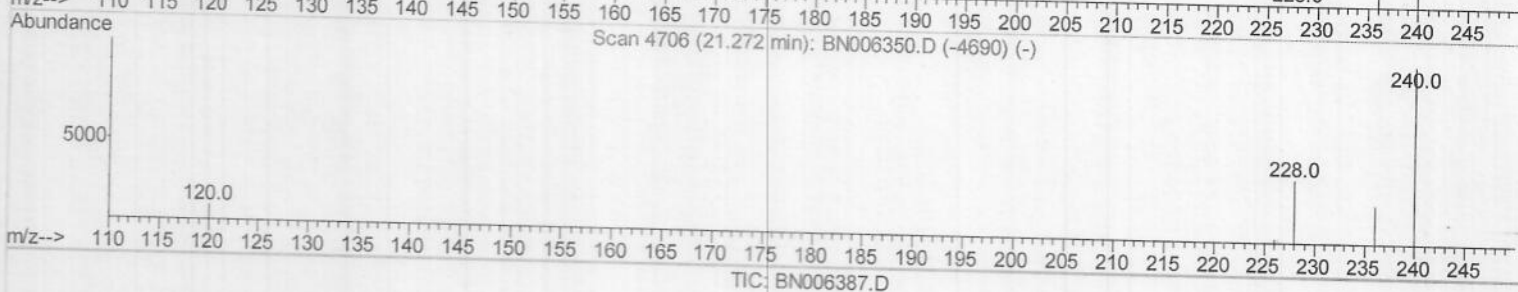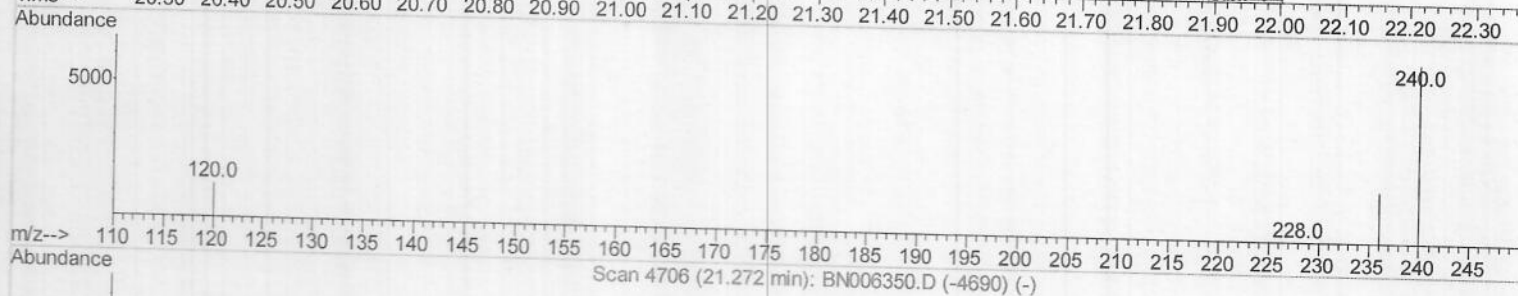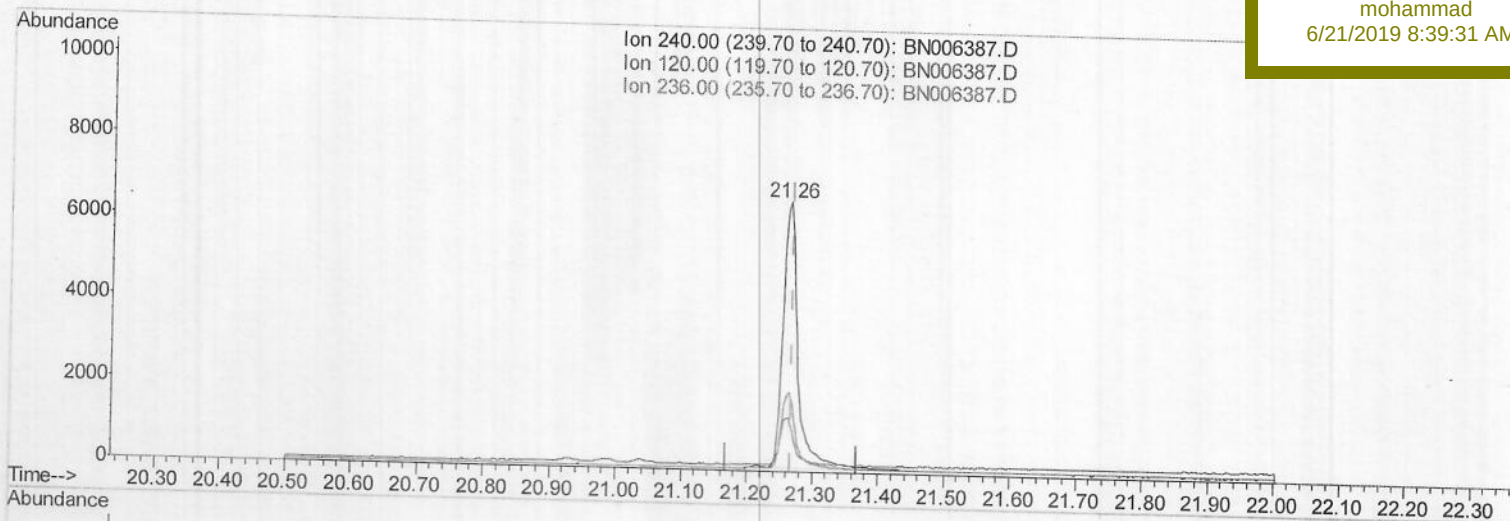

(16) Chrysene-d12 (I)

21.262min (-0.006) 0.40ng/ul m & JU 06/25/19

response 10274

Ion	Exp%	Act%
240.00	100	100
120.00	20.10	19.89
236.00	30.10	29.71
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
Data File : BN006387.D

Acq On : 18 Jun 2019 21:17

Operator : JU/SJ

Sample : K3335-19

Misc :

ALS Vial : 19 Sample Multiplier: 1

Quant Time: Jun 19 02:13:22 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A4238

Manual Integrations

APPROVED

mohammad

6/21/2019 8:39:31 AM

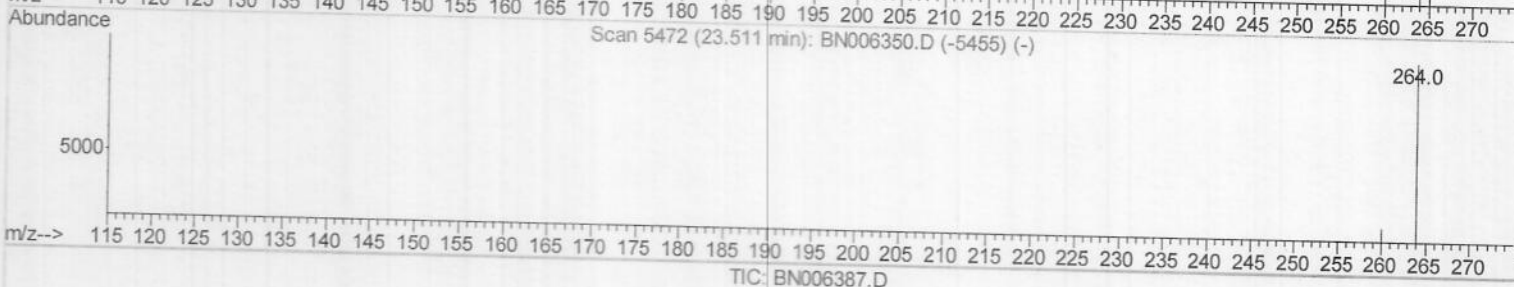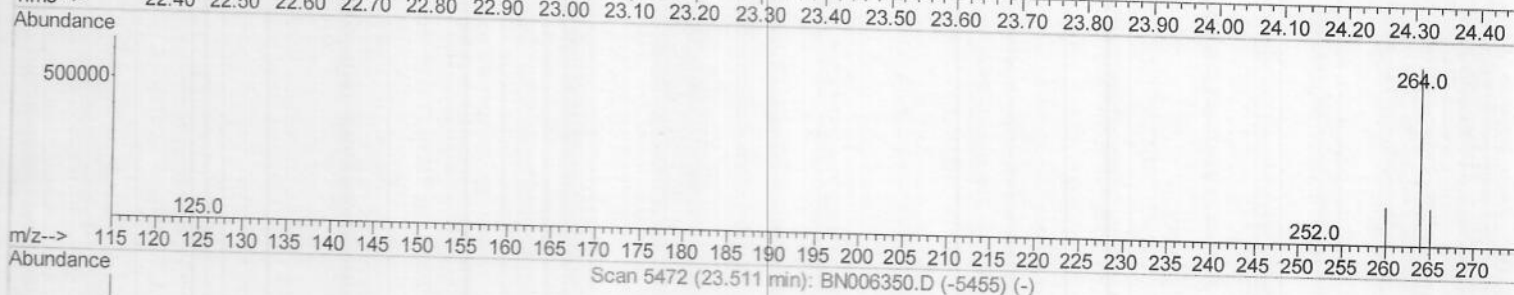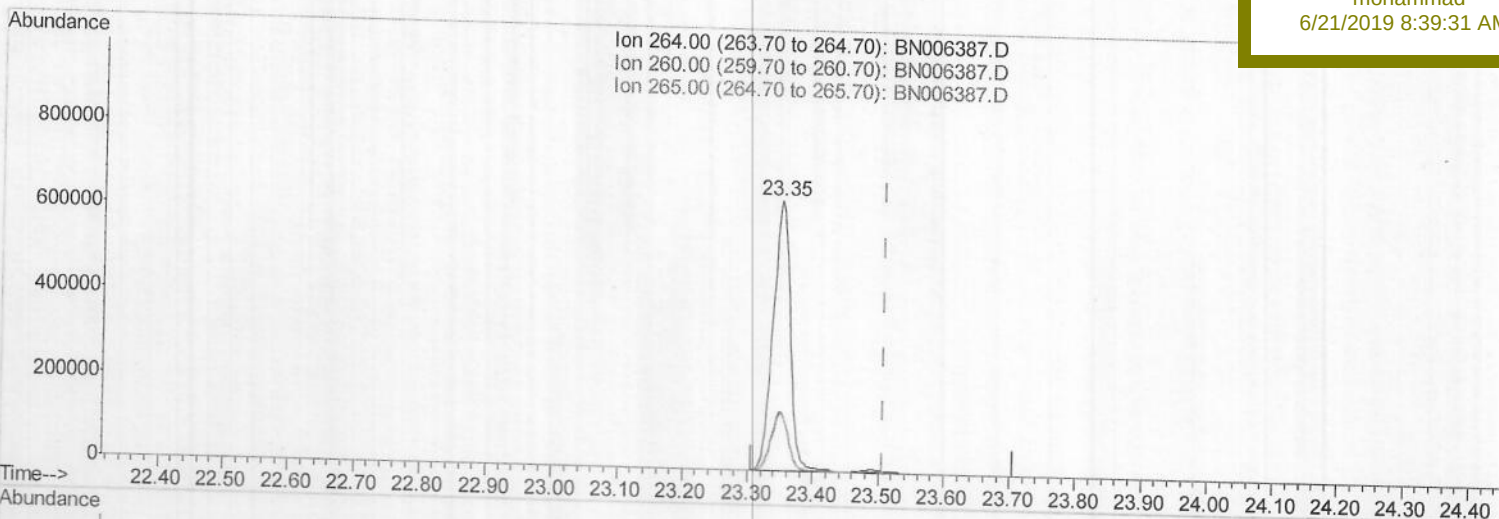

(20) Perylene-d12 (I)

23.349min (-0.158) 0.40ng/ul

response 1153659

Ion Exp% Act%

264.00 100 100

260.00 29.20 22.11#

265.00 44.70 21.51#

0.00 0.00 0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
Data File : BN006387.D

Acq On : 18 Jun 2019 21:17

Operator : JU/SJ

Sample : K3335-19

Misc :

ALS Vial : 19 Sample Multiplier: 1

Quant Time: Jun 19 02:13:22 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A4238

Manual Integrations

APPROVED

mohammad

6/21/2019 8:39:31 AM

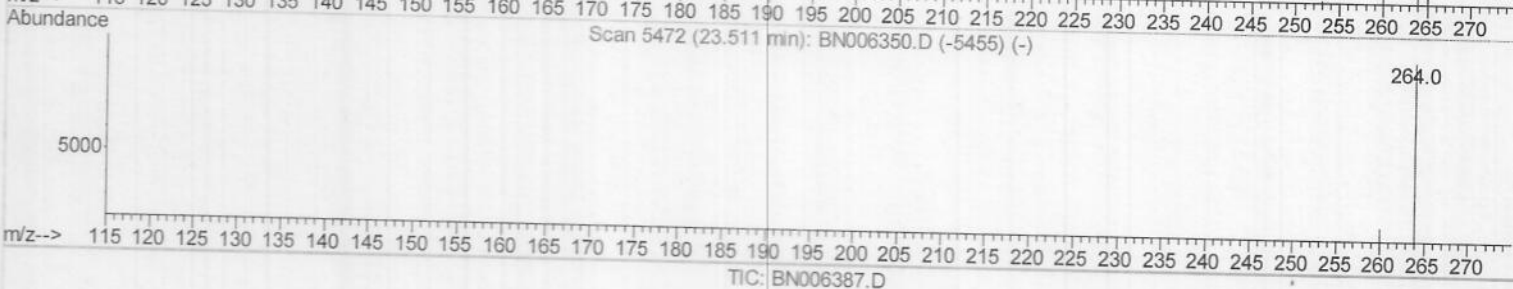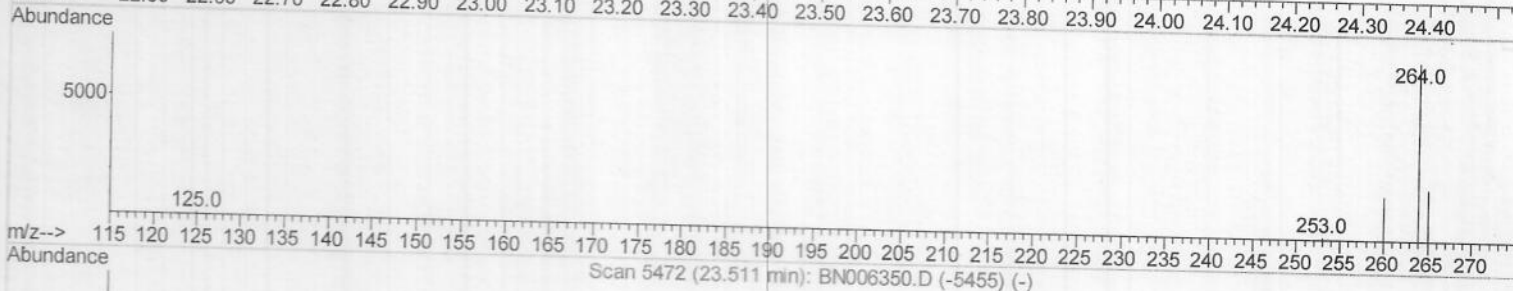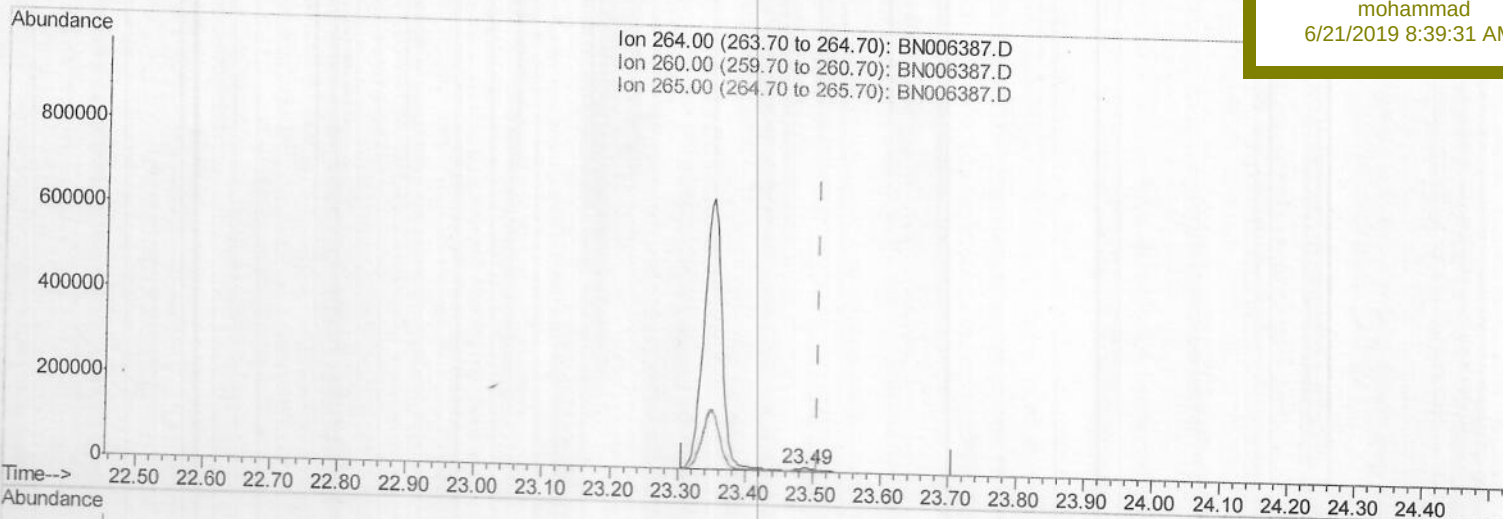

(20) Perylene-d12 (I)

23.490min (-0.017) 0.40ng/ul m

response 9670

Ion	Exp%	Act%
264.00	100	100
260.00	29.20	26.63
265.00	44.70	30.68#
0.00	0.00	0.00

JU 06/25/19

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006387.D
 Acq On : 18 Jun 2019 21:17
 Operator : JU/SJ
 Sample : K3335-19
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4238

Quant Time: Jun 19 02:14:23 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:39:31 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	3933	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	14887	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.29	164	8431	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.04	188	14606m	0.40	ng/ul	0.00
16) Chrysene-d12	21.26	240	10274m	0.40	ng/ul	0.00
20) Perylene-d12	23.49	264	9670m	0.40	ng/ul	-0.02
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	7689	0.34	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	13734m	0.35	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU
 06/25/19