

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006372.D
 Acq On : 18 Jun 2019 10:54
 Operator : JU/SJ
 Sample : K3335-16MSD
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A41Z6MSD

Quant Time: Jun 18 16:06:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 18 15:57:40 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	3360	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	12702	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.29	164	6247	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	10826	0.40	ng/ul	0.00
16) Chrysene-d12	21.27	240	8058	0.40	ng/ul	0.00
20) Perylene-d12	23.51	264	8962	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.03	152	2196	0.11	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	4361	0.15	ng/ul	0.00
Target Compounds				Ovalue		
8) Acenaphthene	14.35	153	3627	0.151	ng/ul	98
17) Pyrene	19.49	202	7618	0.179	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
Data File : BN006372.D
Acq On : 18 Jun 2019 10:54
Operator : JU/SJ
Sample : K3335-16MSD
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41Z6MSD

Quant Time: Jun 18 16:06:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 15:57:40 2019
Response via : Initial Calibration

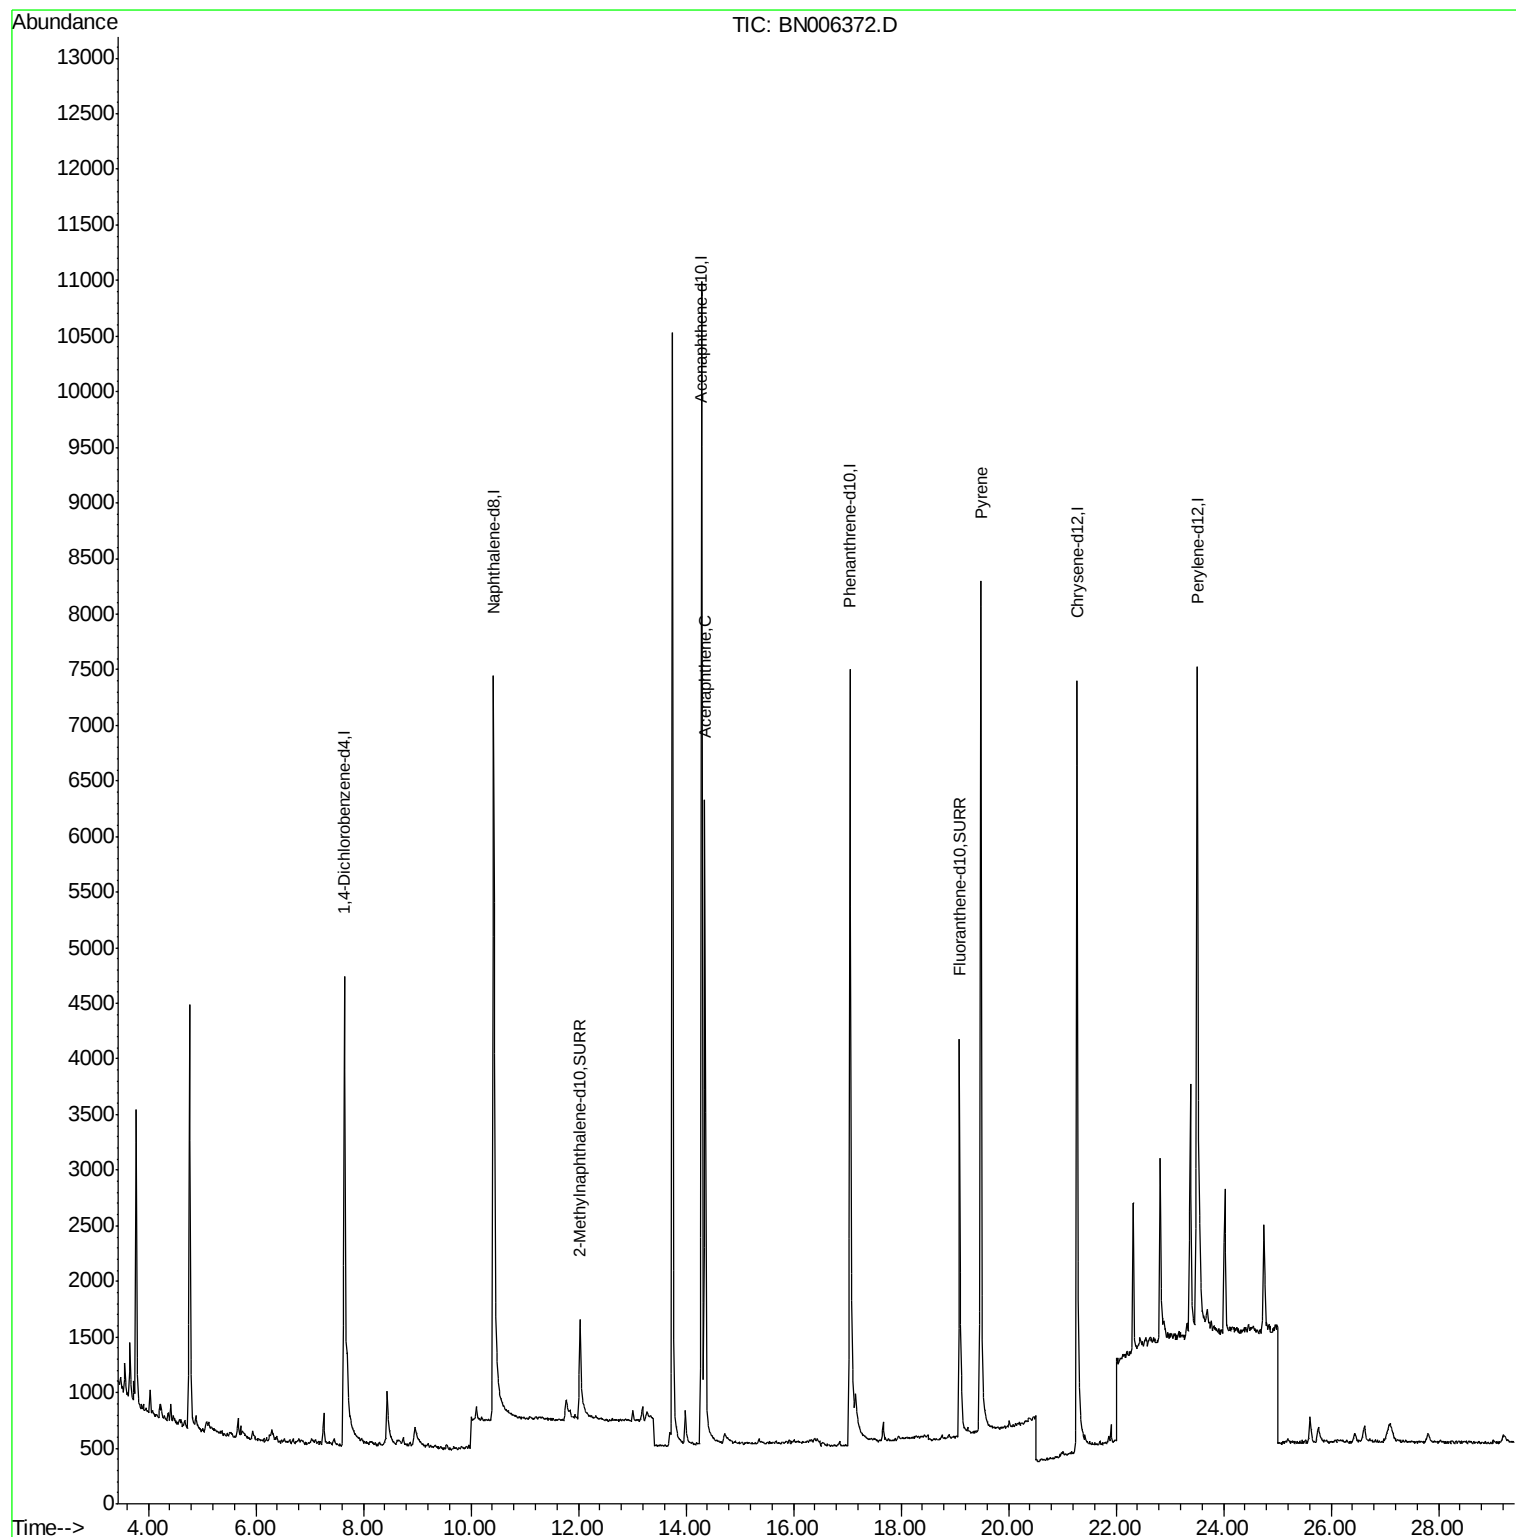

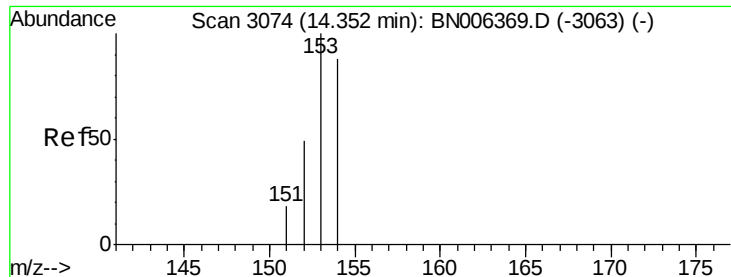

#8

Acenaphthene

Concen: 0.151 ng/ul

RT: 14.35 min Scan# 3074

Delta R.T. -0.00 min

Lab File: BN006372.D

Acq: 18 Jun 2019 10:54

Instrument :

BNA_N

ClientSampleId :

A41Z6MSD


Tot Ion:153 Resp: 3627

Ion Ratio Lower Upper

153 100

152 50.5 39.1 58.7




154 87.4 71.1 106.7

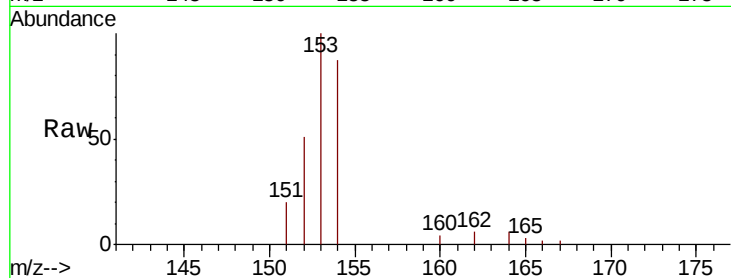

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

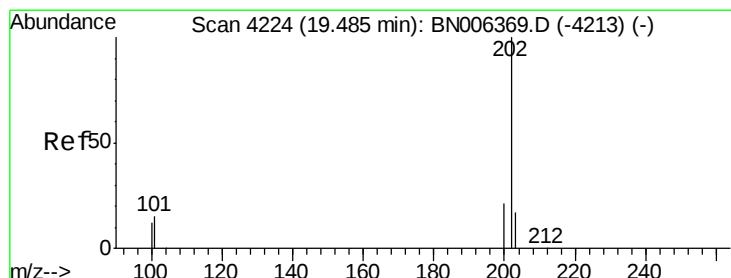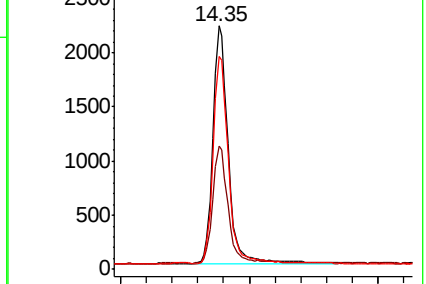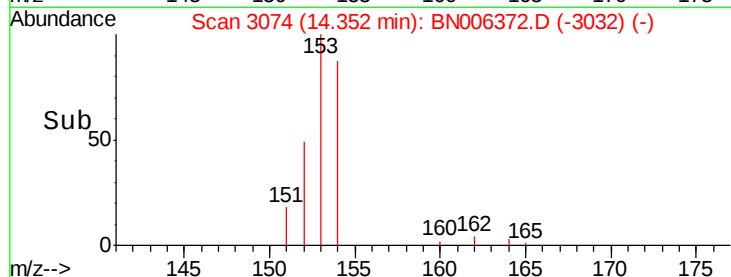

#17

Pyrene

Concen: 0.179 ng/ul

RT: 19.49 min Scan# 4225

Delta R.T. 0.00 min

Lab File: BN006372.D

Acq: 18 Jun 2019 10:54


Tgt Ion:202 Resp: 7618

Ion Ratio Lower Upper

202 100

101 15.0 12.2 18.2

100 11.8 9.8 14.6

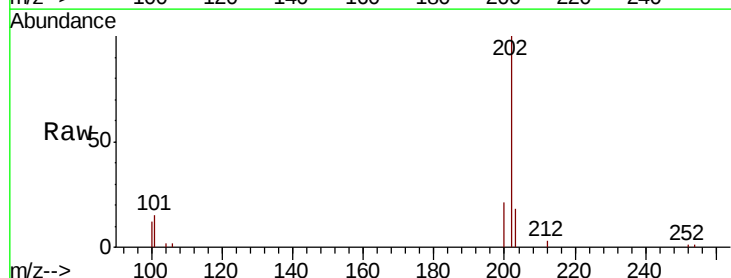

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

