

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
 Data File : BN006380.D
 Acq On : 18 Jun 2019 16:23
 Operator : JU/SJ
 Sample : K3335-15MS
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A41Z6MS

Quant Time: Jun 18 17:07:57 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 18 15:57:40 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	3687	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	14172	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.29	164	7025	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	12074	0.40	ng/ul	0.00
16) Chrysene-d12	21.27	240	8903	0.40	ng/ul	0.00
20) Perylene-d12	23.50	264	9999	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	5655	0.26	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	10017	0.31	ng/ul	0.00
Target Compounds				Ovalue		
8) Acenaphthene	14.35	153	4113	0.152	ng/ul	99
11) Pentachlorophenol	16.72	266	953	0.311	ng/ul	95
17) Pyrene	19.49	202	8252	0.176	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061819\
Data File : BN006380.D
Acq On : 18 Jun 2019 16:23
Operator : JU/SJ
Sample : K3335-15MS
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41Z6MS

Quant Time: Jun 18 17:07:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 15:57:40 2019
Response via : Initial Calibration

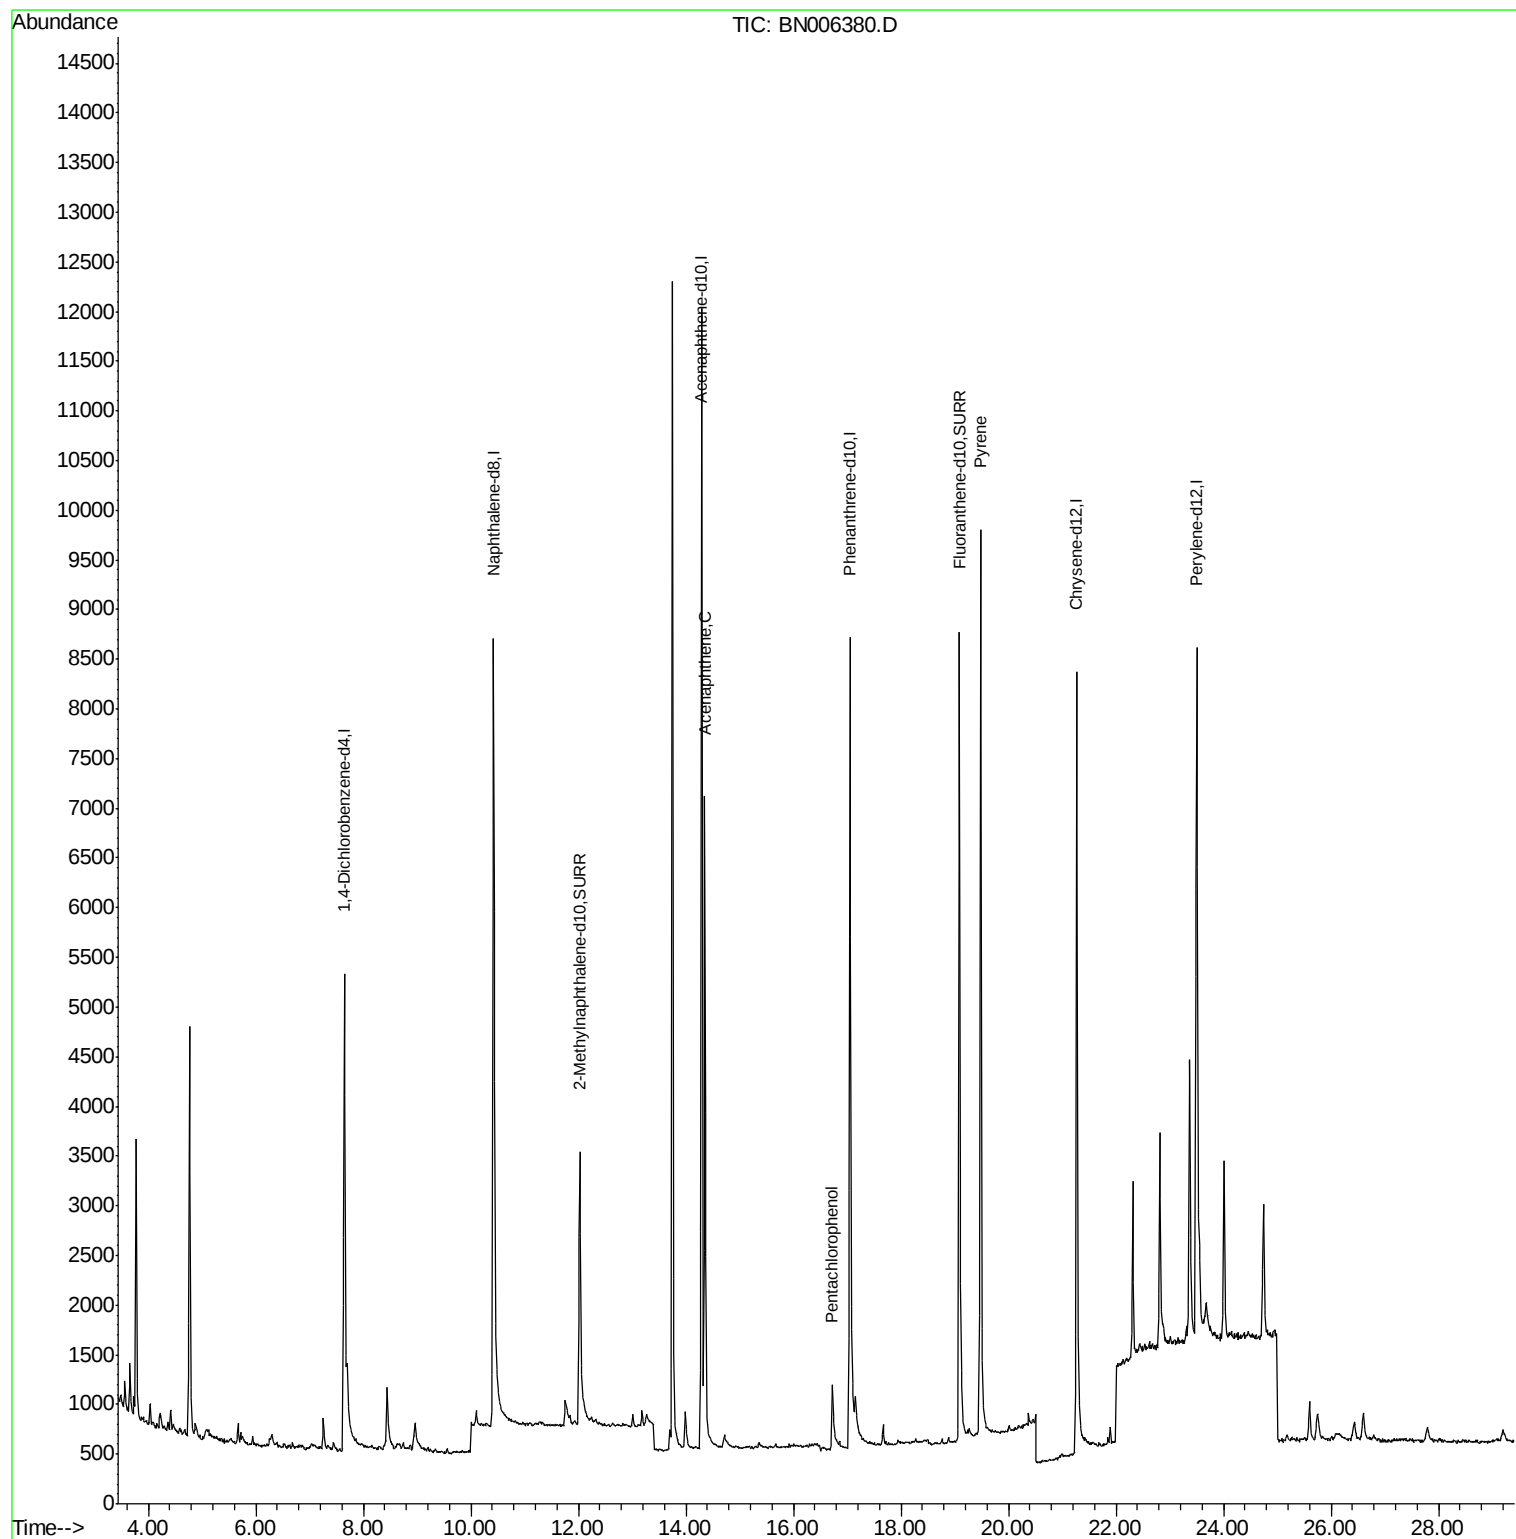

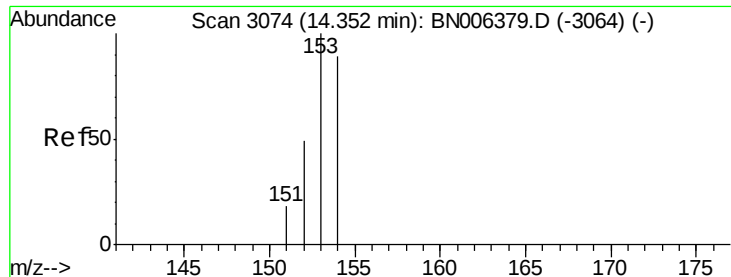

#8

Acenaphthene

Concen: 0.152 ng/ul

RT: 14.35 min Scan# 3074

Delta R.T. -0.00 min

Lab File: BN006380.D

Acq: 18 Jun 2019 16:23

Instrument :

BNA_N

ClientSampleId :

A41Z6MS


Tot Ion:153 Resp: 4113

Ion Ratio Lower Upper

153 100

152 50.2 39.1 58.7




154 89.8 71.1 106.7

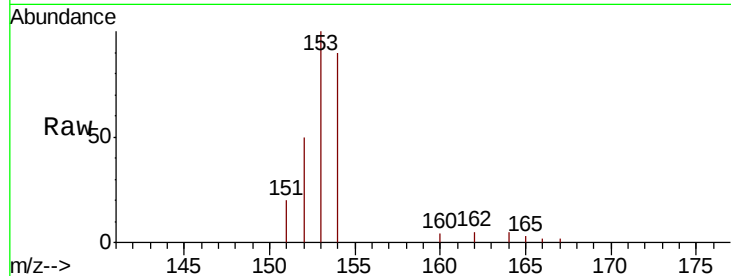

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

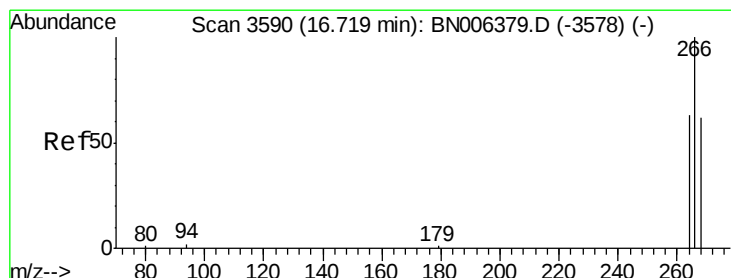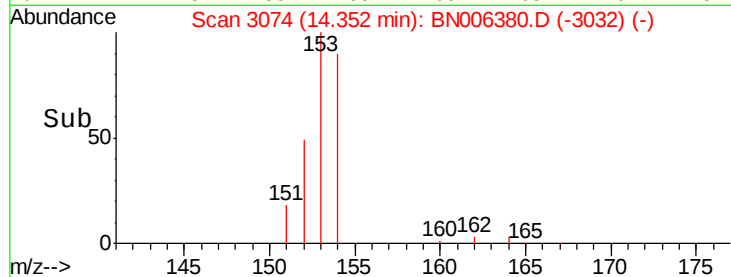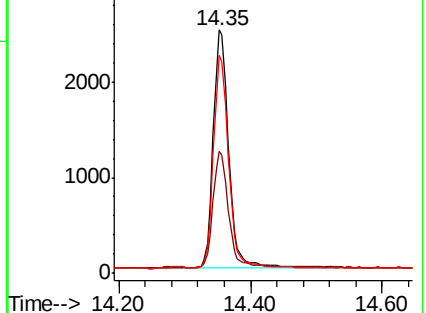

#11

Pentachlorophenol

Concen: 0.311 ng/ul

RT: 16.72 min Scan# 3590

Delta R.T. 0.00 min

Lab File: BN006380.D

Acq: 18 Jun 2019 16:23


Tgt Ion:266 Resp: 953

Ion Ratio Lower Upper

266 100

264 61.5 50.3 75.5



268 57.4 51.3 76.9

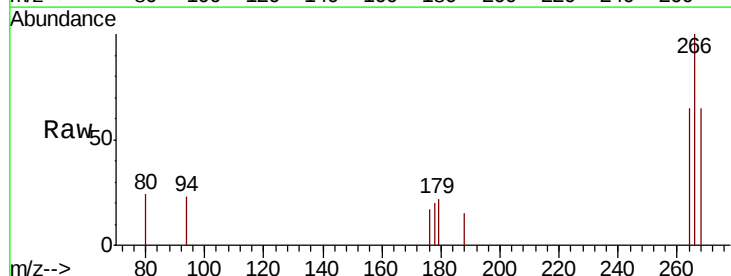


Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

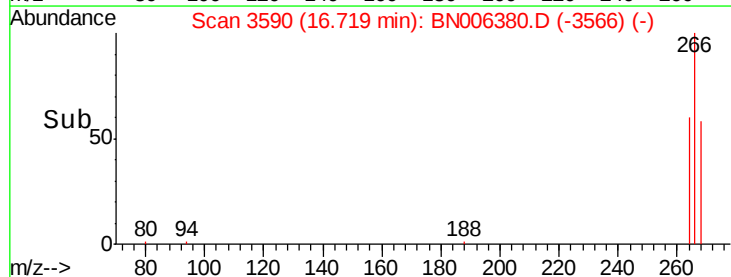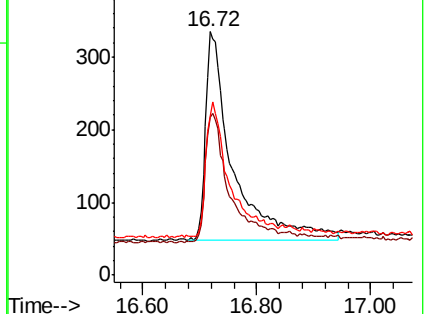

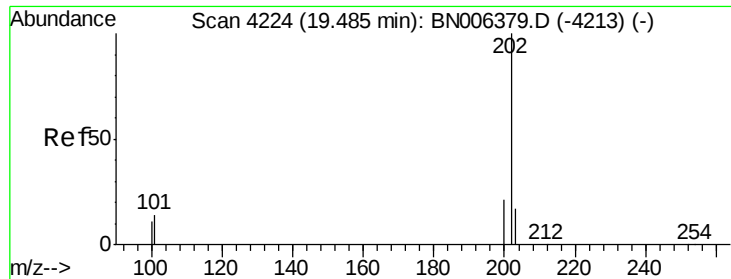

#17
 Pvrene
 Concen: 0.176 ng/ul
 RT: 19.49 min Scan# 4224
 Delta R.T. 0.00 min
 Lab File: BN006380.D
 Acq: 18 Jun 2019 16:23

Instrument :
 BNA_N
 ClientSampleId :
 A41Z6MS

Tot Ion	Ratio	Lower	Upper
202	100		
101	15.2	12.2	18.2
100	12.0	9.8	14.6

