




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061825\
Data File : BN037307.D
Acq On : 18 Jun 2025 10:07
Operator : RC/JU
Sample : PB168466BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK466

Manual IntegrationsAPPROVED

Quant Time: Jun 18 12:50:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN061725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 17 15:03:28 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 06/18/2025
Supervised By :Jagrut Upadhyay 06/18/2025

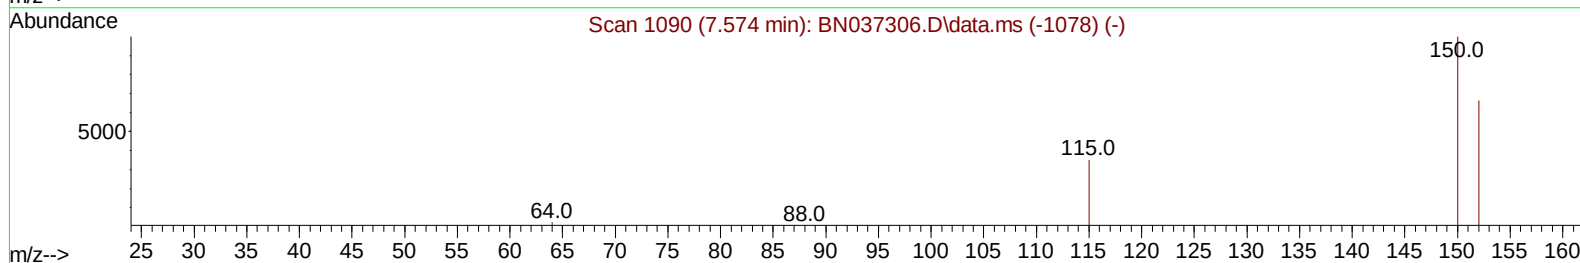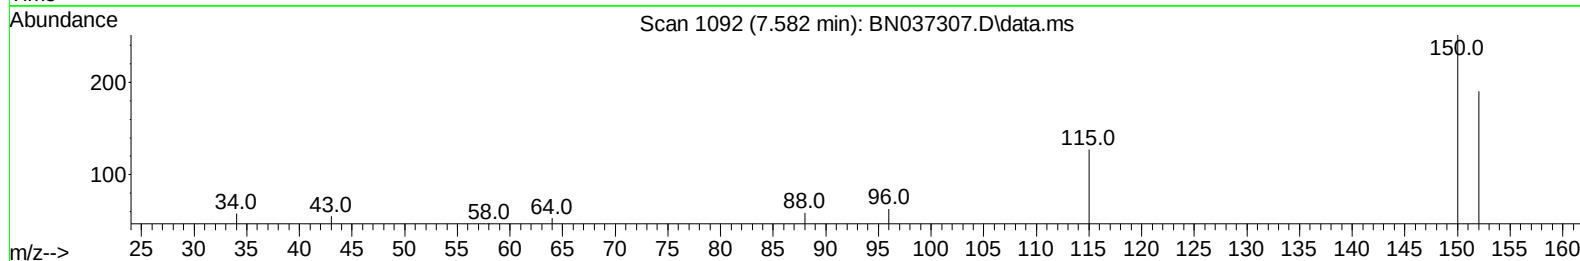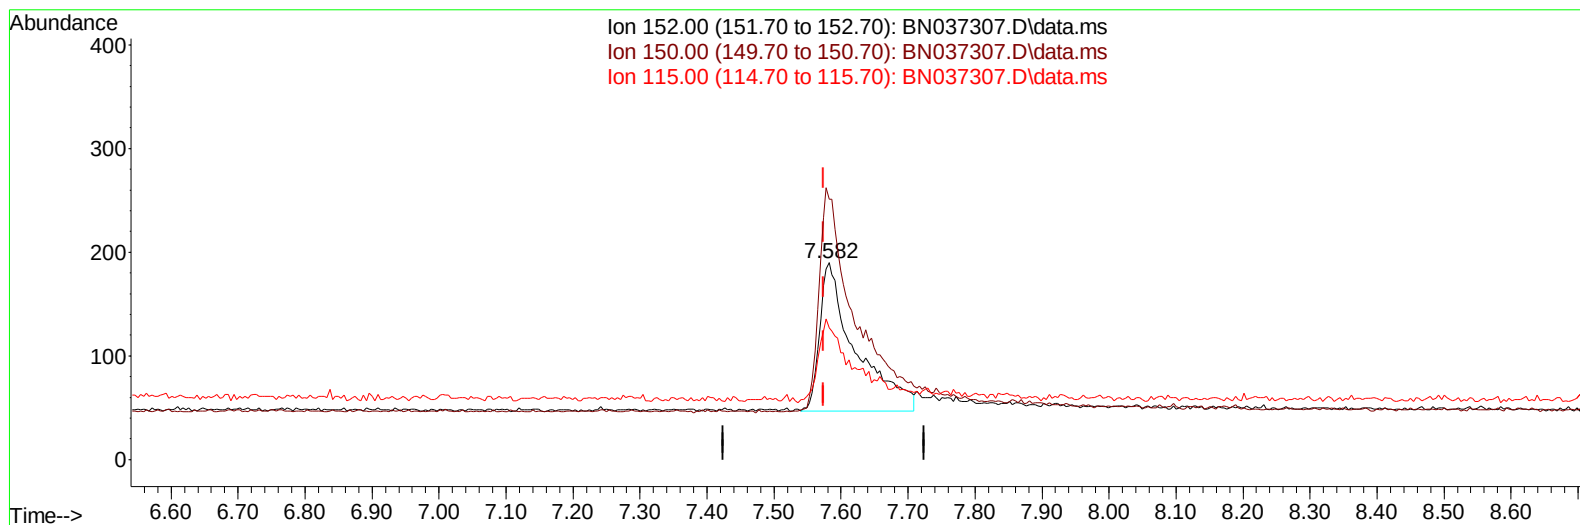

TIC: BN037307.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.582min (+ 0.008) 0.40 ng/u1

response 529

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	140.10	132.11
115.00	59.10	66.84
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061825\
Data File : BN037307.D
Acq On : 18 Jun 2025 10:07
Operator : RC/JU
Sample : PB168466BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK466

Manual IntegrationsAPPROVED

Quant Time: Jun 18 12:50:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN061725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 17 15:03:28 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 06/18/2025
Supervised By :Jagrut Upadhyay 06/18/2025

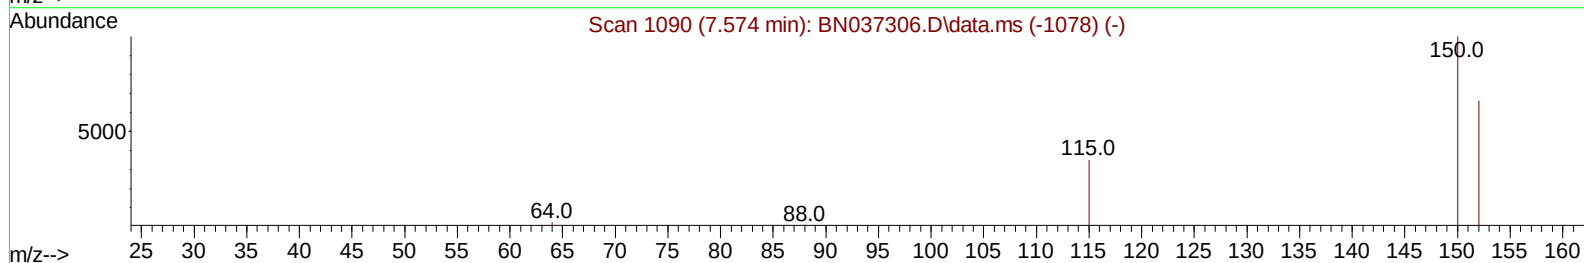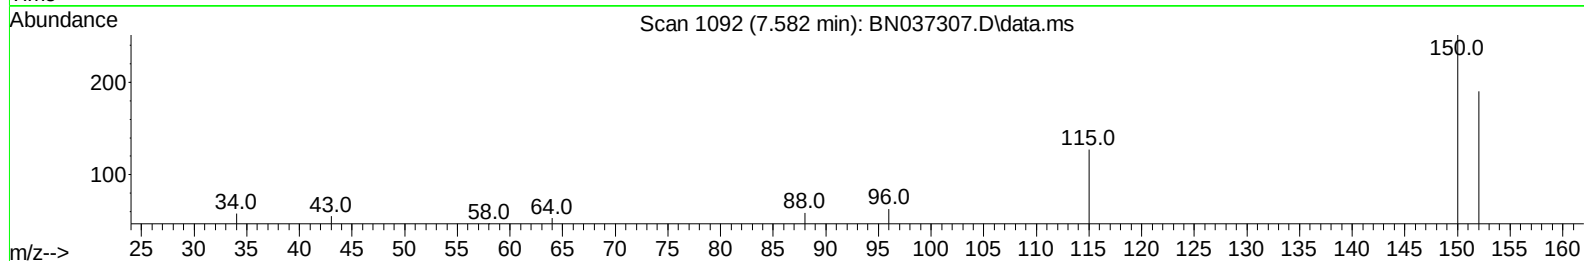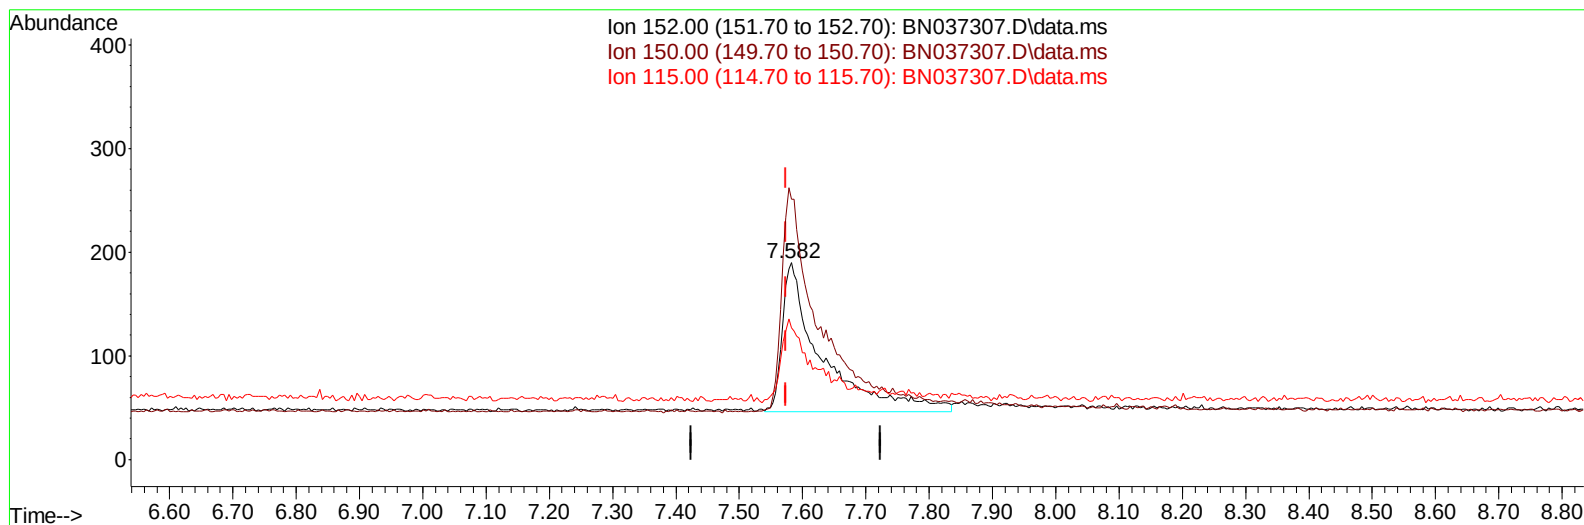

TIC: BN037307.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.582min (+ 0.008) 0.40 ng/ul m

response 628

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	140.10	132.11
115.00	59.10	66.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061825\
 Data File : BN037307.D
 Acq On : 18 Jun 2025 10:07
 Operator : RC/JU
 Sample : PB168466BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK466

Manual IntegrationsAPPROVED

Reviewed By :Rahul Chavli 06/18/2025
 Supervised By :Jagrut Upadhyay 06/18/2025

Quant Time: Jun 18 12:50:48 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN061725.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 17 15:03:28 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.582	152	628m	0.400	ng/ul	0.00
4) Naphthalene-d8	10.371	136	1160	0.400	ng/ul #	0.02
9) Acenaphthene-d10	14.230	164	962	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.995	188	1700	0.400	ng/ul #	0.02
17) Chrysene-d12	21.182	240	2068	0.400	ng/ul #	0.00
23) Perylene-d12	23.366	264	2336	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.068	96	540	0.927	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.982	152	837	0.433	ng/ul	0.03
18) Fluoranthene-d10	19.022	212	2501	0.379	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061825\
Data File : BN037307.D
Acq On : 18 Jun 2025 10:07
Operator : RC/JU
Sample : PB168466BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK466

Manual IntegrationsAPPROVED

Quant Time: Jun 18 12:50:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN061725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 17 15:03:28 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 06/18/2025
Supervised By :Jagrut Upadhyay 06/18/2025

