




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061825\
Data File : BN037310.D
Acq On : 18 Jun 2025 11:56
Operator : RC/JU
Sample : PB168470BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK470

Manual IntegrationsAPPROVED

Quant Time: Jun 18 13:03:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN061725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 17 15:03:28 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 06/18/2025
Supervised By :Jagrut Upadhyay 06/18/2025

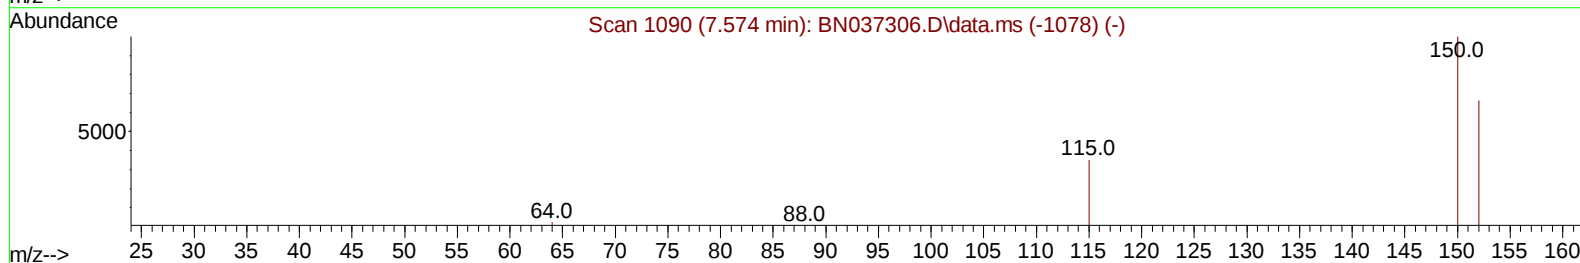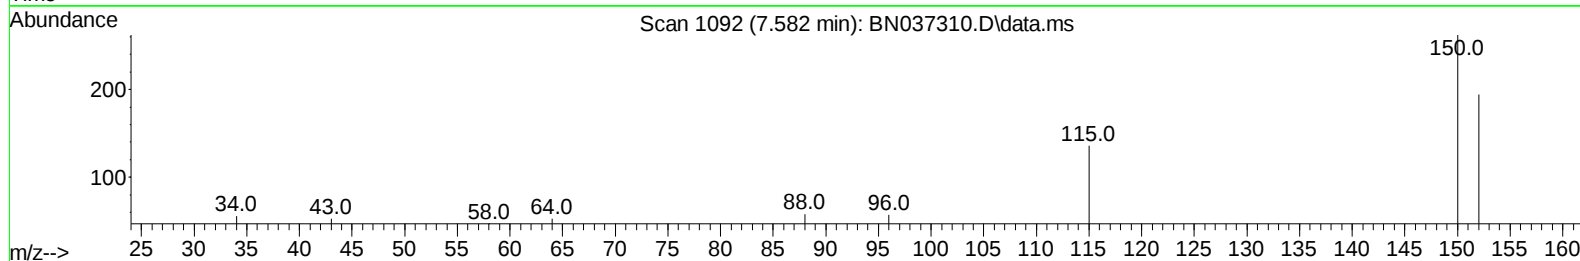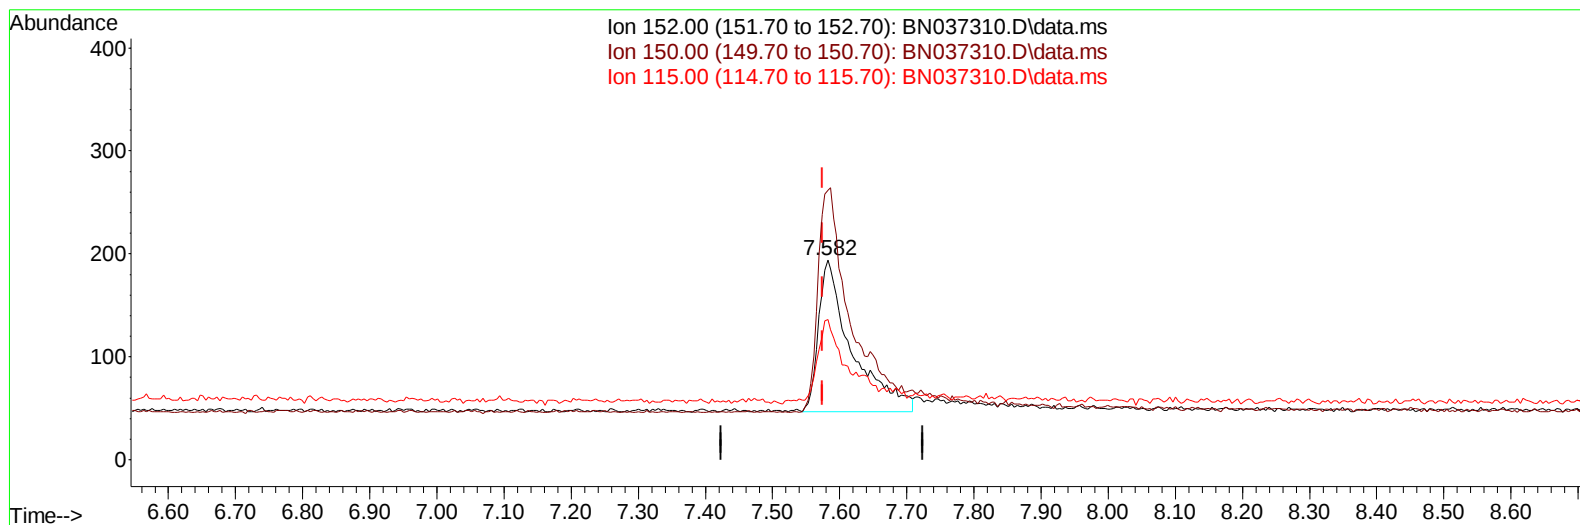

TIC: BN037310.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.582min (+ 0.008) 0.40 ng/u1

response 505

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	140.10	135.05
115.00	59.10	70.10
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061825\
Data File : BN037310.D
Acq On : 18 Jun 2025 11:56
Operator : RC/JU
Sample : PB168470BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK470

Manual IntegrationsAPPROVED

Quant Time: Jun 18 13:03:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN061725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 17 15:03:28 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 06/18/2025
Supervised By :Jagrut Upadhyay 06/18/2025

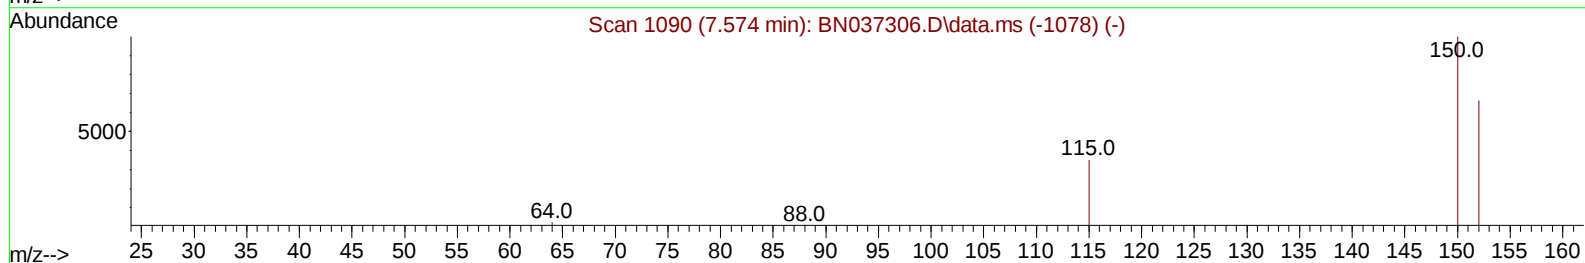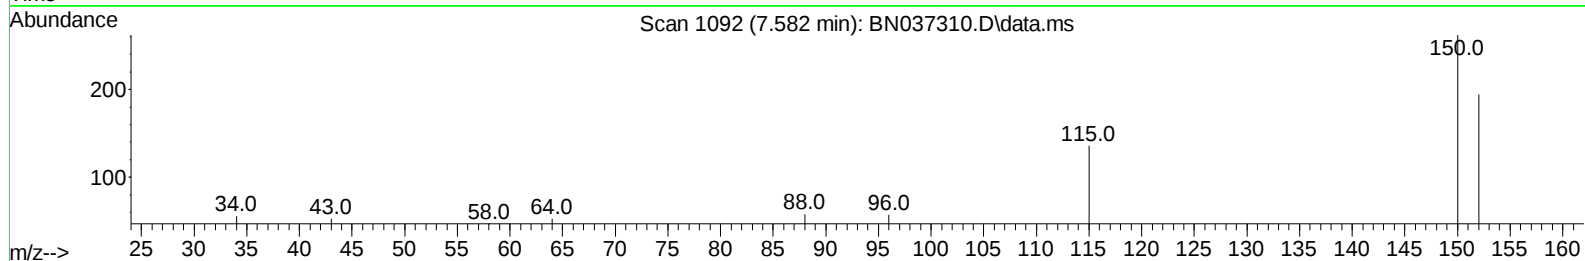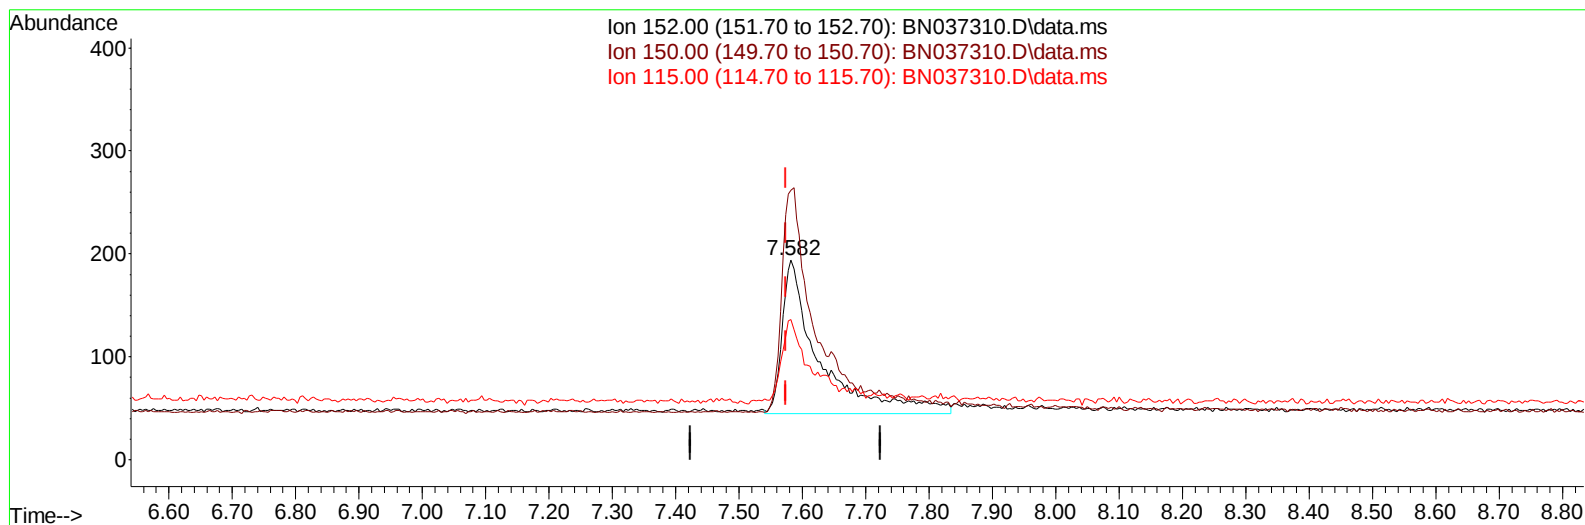

TIC: BN037310.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.582min (+ 0.008) 0.40 ng/ul m

response 610

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	140.10	135.05
115.00	59.10	70.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061825\
 Data File : BN037310.D
 Acq On : 18 Jun 2025 11:56
 Operator : RC/JU
 Sample : PB168470BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK470

Manual IntegrationsAPPROVED

Reviewed By :Rahul Chavli 06/18/2025
 Supervised By :Jagrut Upadhyay 06/18/2025

Quant Time: Jun 18 13:03:31 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN061725.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 17 15:03:28 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.582	152	610m	0.400	ng/ul	0.00
4) Naphthalene-d8	10.360	136	1116	0.400	ng/ul #	0.01
9) Acenaphthene-d10	14.230	164	912	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.995	188	1688	0.400	ng/ul #	0.02
17) Chrysene-d12	21.185	240	2056	0.400	ng/ul #	0.00
23) Perylene-d12	23.365	264	2365	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.068	96	491	0.868	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.982	152	670	0.360	ng/ul	0.03
18) Fluoranthene-d10	19.017	212	2259	0.344	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061825\
Data File : BN037310.D
Acq On : 18 Jun 2025 11:56
Operator : RC/JU
Sample : PB168470BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK470

Manual IntegrationsAPPROVED

Quant Time: Jun 18 13:03:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN061725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 17 15:03:28 2025
Response via : Initial Calibration

Reviewed By :Rahul Chavli 06/18/2025
Supervised By :Jagrut Upadhyay 06/18/2025

