


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061825\
Data File : BN037305.D
Acq On : 18 Jun 2025 08:52
Operator : RC/JU
Sample : DFTPP273
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP273

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN061725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jun 17 15:03:28 2025

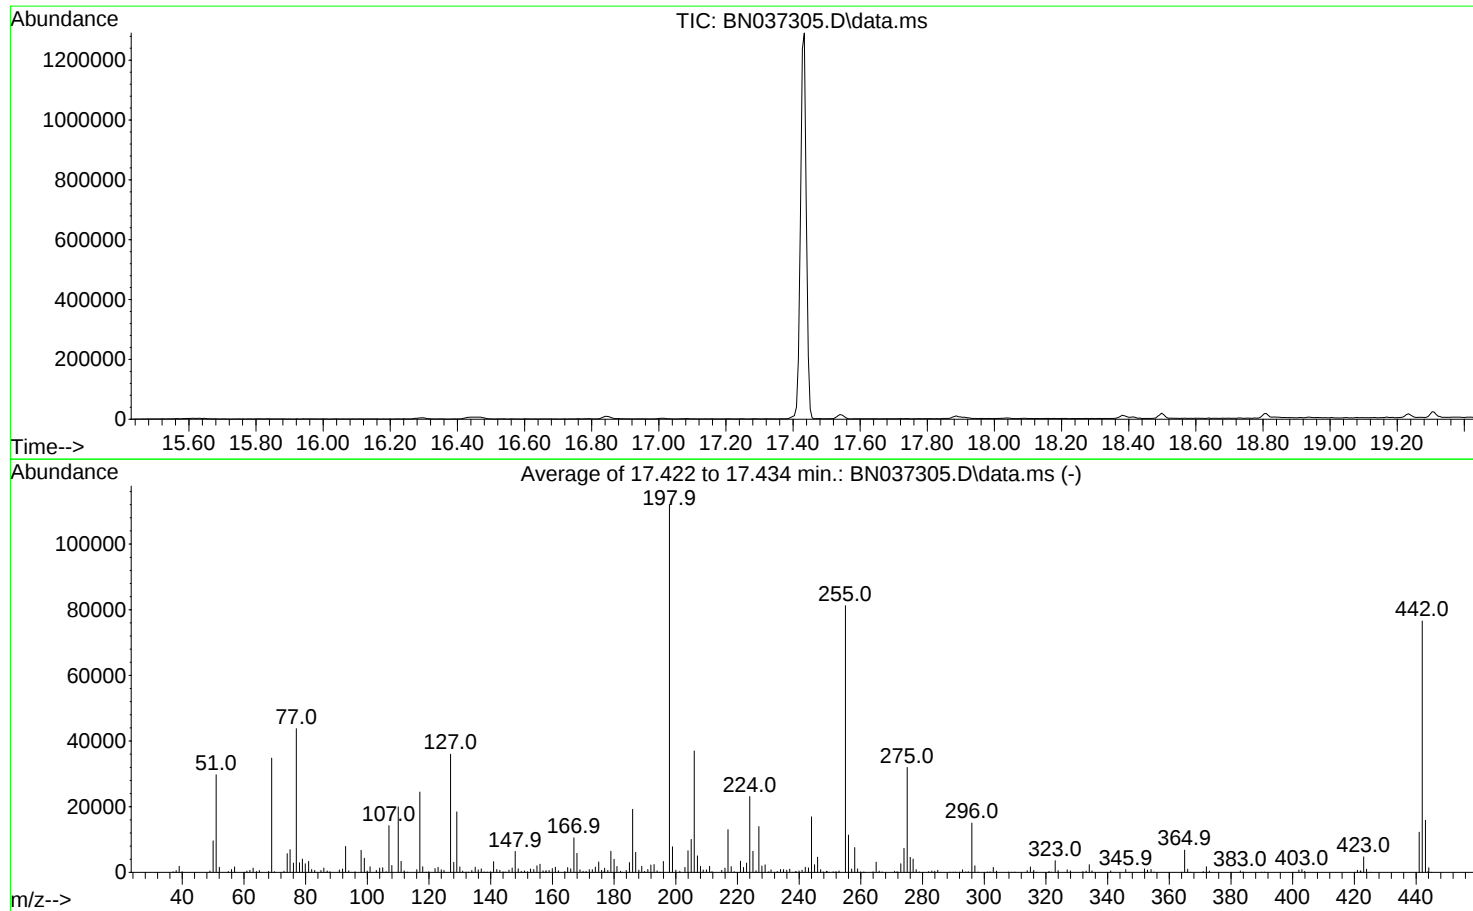

AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.5	29736	PASS
68	69	0.00	2	0.9	302	PASS
69	198	0.00	100	31.1	34816	PASS
70	69	0.00	2	0.5	181	PASS
127	198	10	80	32.1	35960	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	112067	PASS
199	198	5	9	7.0	7816	PASS
275	198	10	60	28.5	31976	PASS
365	198	1	100	6.0	6777	PASS
441	198	0.01	100	10.9	12254	PASS
442	198	50	100	68.3	76589	PASS
443	442	15	24	20.7	15887	PASS